

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN033022\
 Data File : VN071665.D
 Acq On : 30 Mar 2022 17:44
 Operator : JC\MD
 Sample : N2130-04
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 STORAGE-BLANK-SAMPLE-MANAG

Quant Time: Mar 31 01:35:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 30 19:18:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.081	168	648007	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	1086476	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	1073428	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.669	152	383153	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.434	65	370217	50.04	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	100.08%
35) Dibromofluoromethane	8.022	113	311072	48.66	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	97.32%
50) Toluene-d8	10.439	98	1334527	51.03	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	102.06%
62) 4-Bromofluorobenzene	12.727	95	445326	52.65	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	105.30%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN033022\
Data File : VN071665.D
Acq On : 30 Mar 2022 17:44
Operator : JC\MD
Sample : N2130-04
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG

Quant Time: Mar 31 01:35:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 30 19:18:20 2022
Response via : Initial Calibration

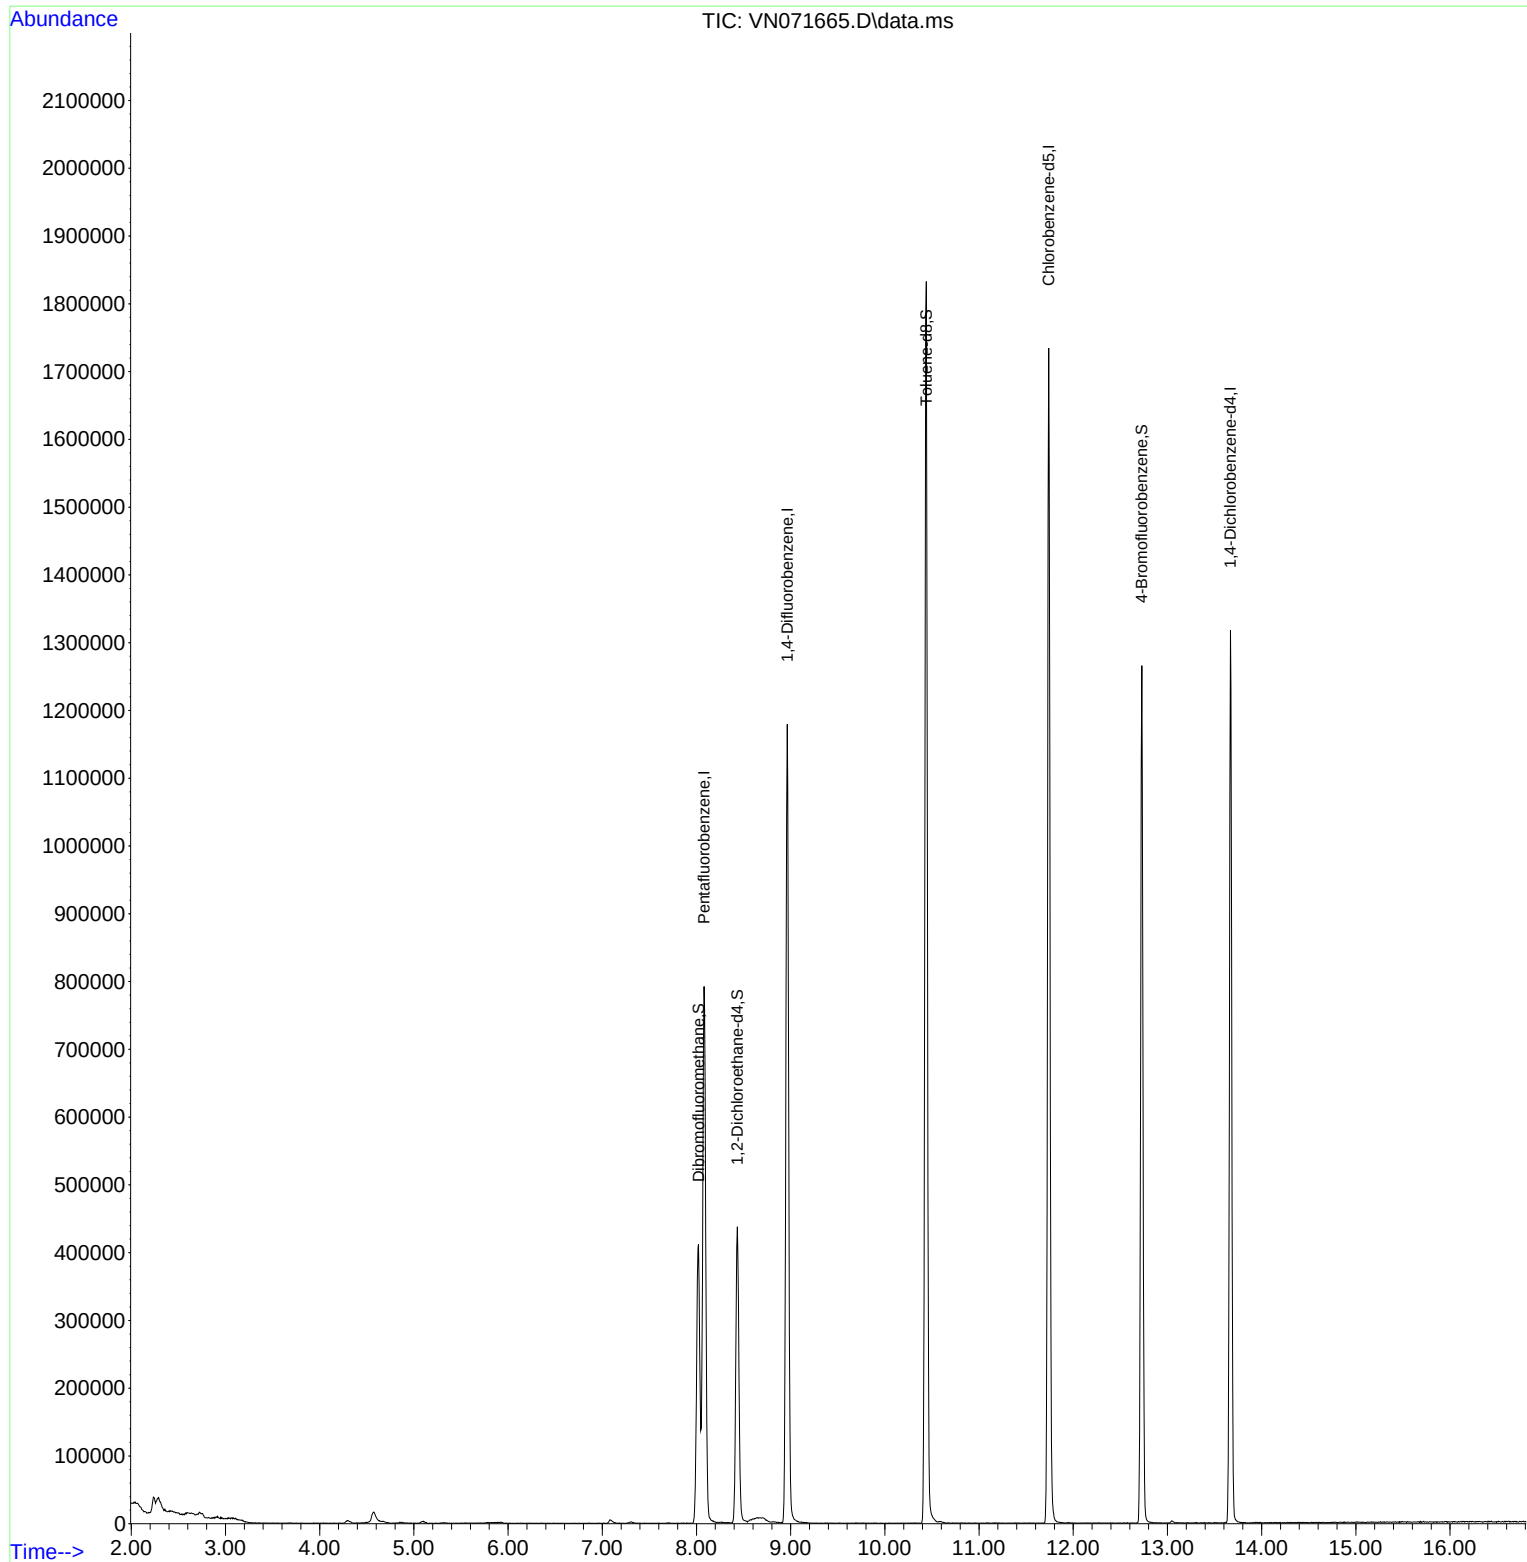

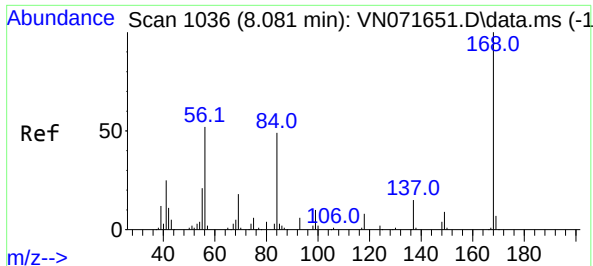

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 8.081 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN071665.D

Acq: 30 Mar 2022 17:44

Instrument :

MSVOA_N

ClientSampleId :





STORAGE-BLANK-SAMPLE-MANAG

Tgt Ion:168 Resp: 648007

Ion Ratio Lower Upper

168 100

99 54.4 42.3 63.5

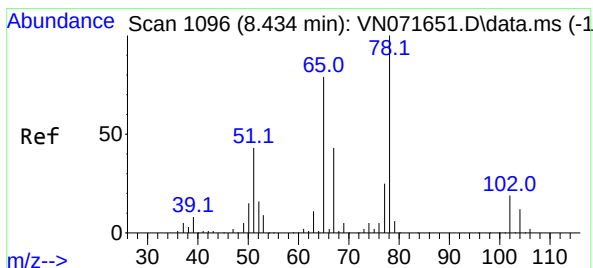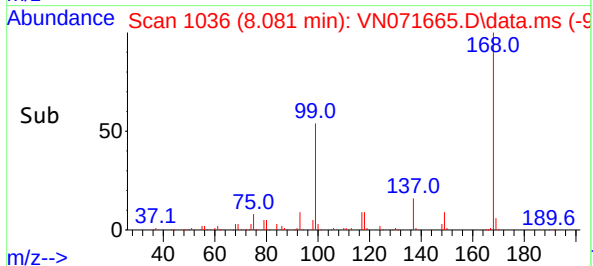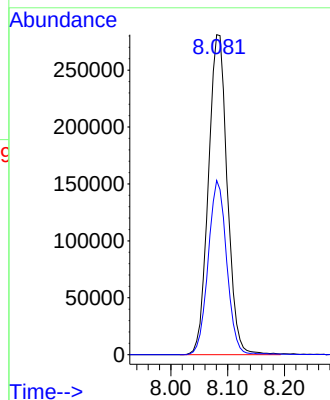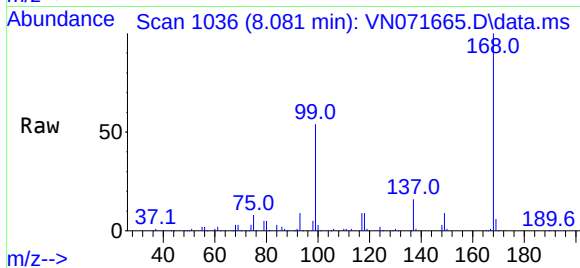

#33

1,2-Dichloroethane-d4

Concen: 50.04 ug/l

RT: 8.434 min Scan# 1096

Delta R.T. -0.000 min

Lab File: VN071665.D




Acq: 30 Mar 2022 17:44


Tgt Ion: 65 Resp: 370217

Ion Ratio Lower Upper

65 100

67 52.1 0.0 104.8


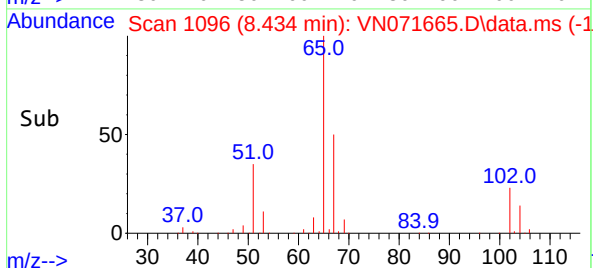
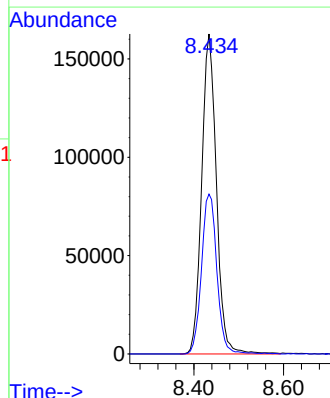
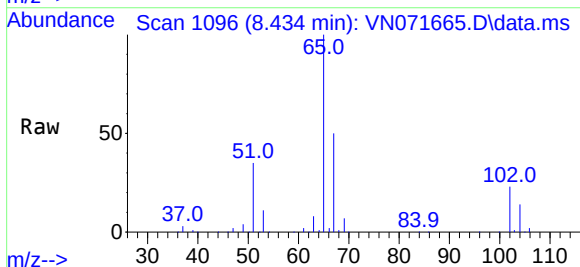


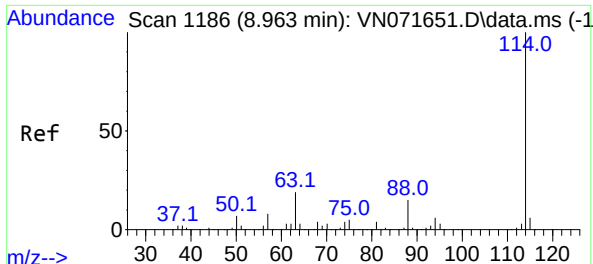

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.963 min Scan# 1186
Delta R.T. -0.000 min
Lab File: VN071665.D
Acq: 30 Mar 2022 17:44




Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG


Tgt Ion:114 Resp: 1086476
Ion Ratio Lower Upper
114 100
63 19.6 0.0 40.0
88 16.5 0.0 32.6

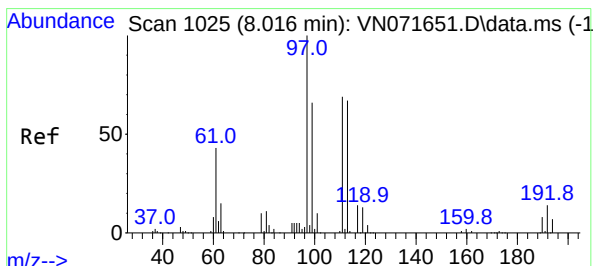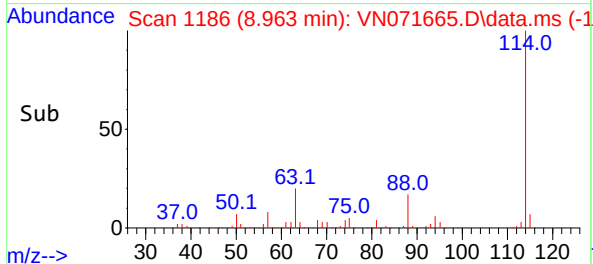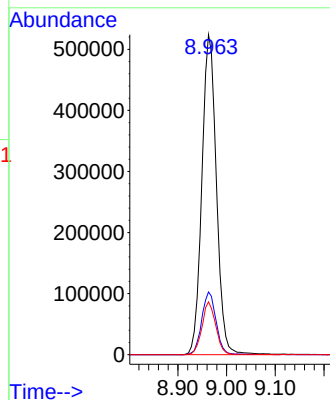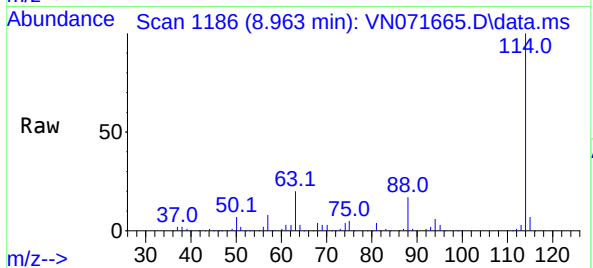

#35
Dibromofluoromethane
Concen: 48.66 ug/l
RT: 8.022 min Scan# 1026
Delta R.T. 0.006 min
Lab File: VN071665.D
Acq: 30 Mar 2022 17:44

Tgt Ion:113 Resp: 311072
Ion Ratio Lower Upper
113 100
111 102.7 81.4 122.0
192 22.0 17.0 25.6


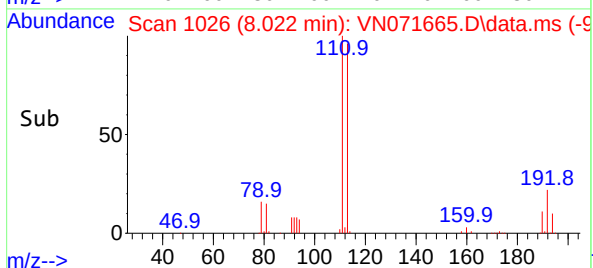
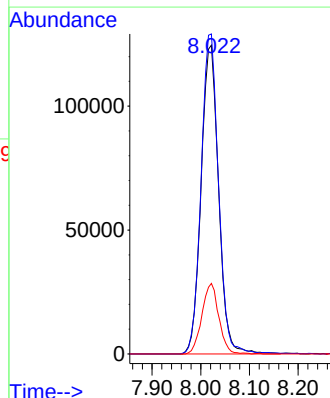
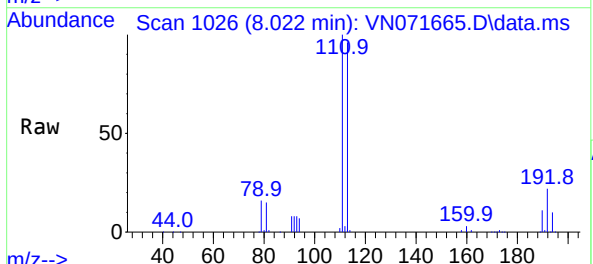


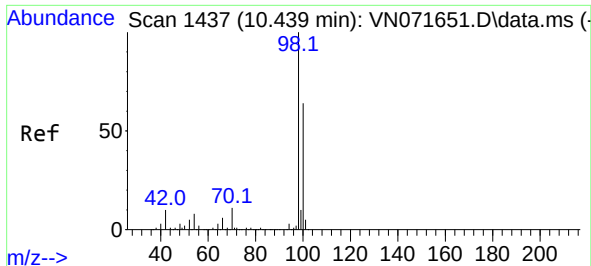

#50
Toluene-d8
Concen: 51.03 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. 0.000 min
Lab File: VN071665.D
Acq: 30 Mar 2022 17:44




Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG


Tgt Ion: 98 Resp: 1334527
Ion Ratio Lower Upper
98 100
100 64.5 52.6 78.8

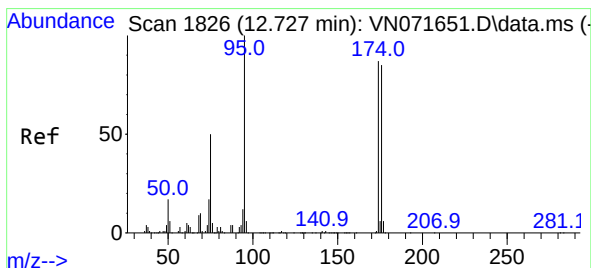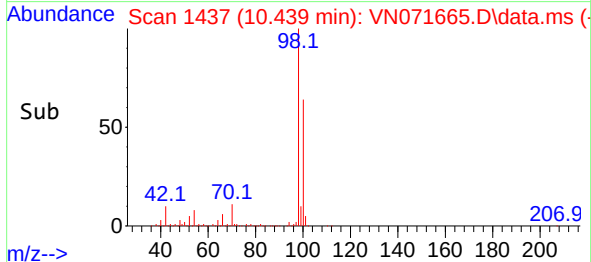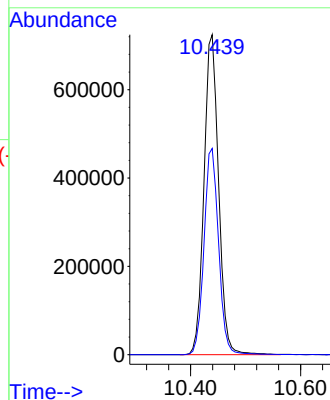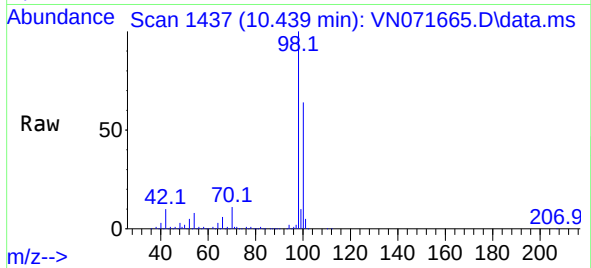

#62
4-Bromofluorobenzene
Concen: 52.65 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN071665.D
Acq: 30 Mar 2022 17:44

Tgt Ion: 95 Resp: 445326
Ion Ratio Lower Upper
95 100
174 84.9 0.0 167.6
176 82.8 0.0 163.4


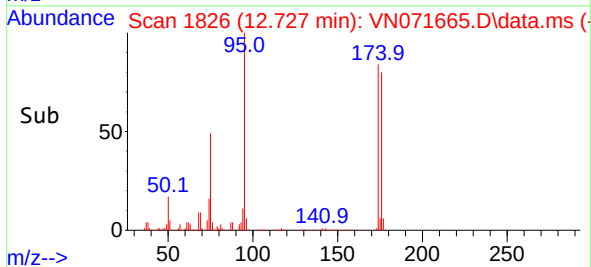
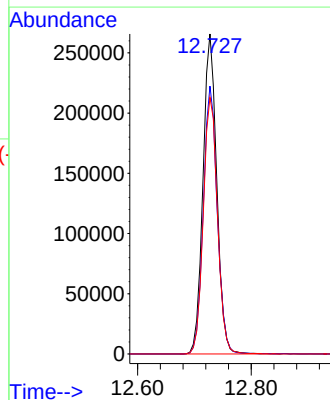
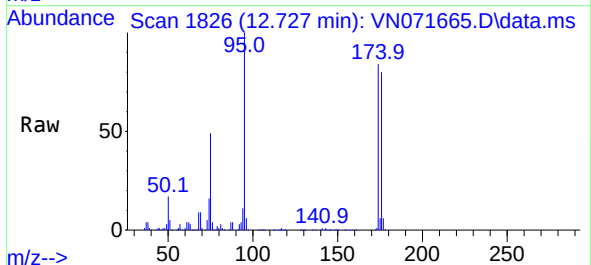


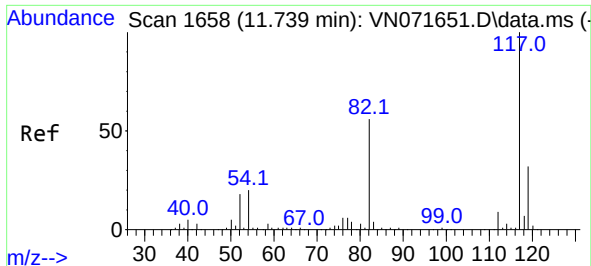

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.739 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN071665.D
Acq: 30 Mar 2022 17:44

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-SAMPLE-MANAG

Tgt Ion:117 Resp: 1073428
Ion Ratio Lower Upper
117 100
82 53.8 44.2 66.2
119 31.8 25.4 38.0

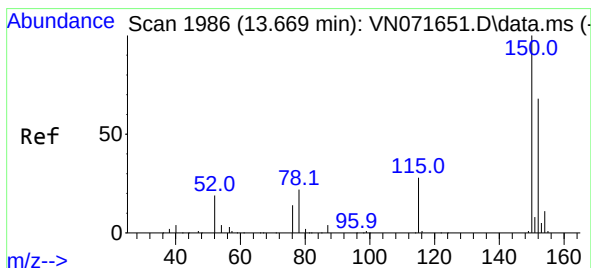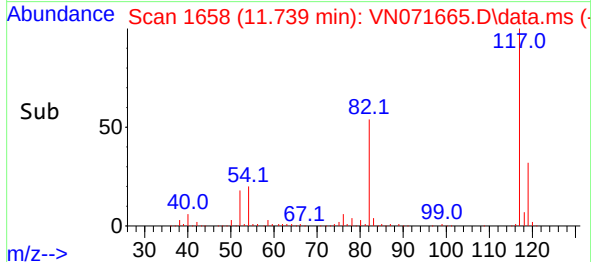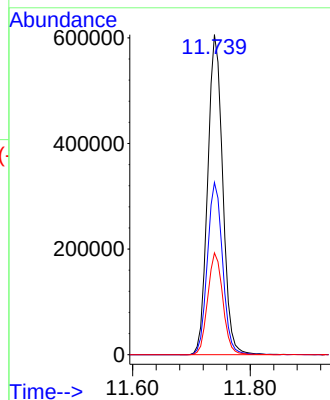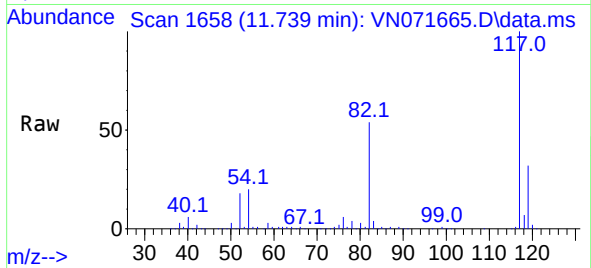

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.669 min Scan# 1986
Delta R.T. -0.001 min
Lab File: VN071665.D
Acq: 30 Mar 2022 17:44

Tgt Ion:152 Resp: 383153
Ion Ratio Lower Upper
152 100
115 56.5 28.9 86.7
150 158.4 0.0 356.2

