

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN033022\
 Data File : VN071687.D
 Acq On : 31 Mar 2022 03:21
 Operator : JC\MD
 Sample : N2075-10
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-178S-20220322

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M

Title : SW846 8260

Signal : TIC: VN071687.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.240	37	43	46	rBV3	29487	63474	1.83%	0.361%
2	5.610	604	616	630	rBV2	15850	56906	1.64%	0.323%
3	8.022	1010	1026	1031	rBV	418217	1037090	29.90%	5.891%
4	8.080	1031	1036	1058	rVB	779420	1776119	51.21%	10.089%
5	8.433	1087	1096	1108	rBV	442637	1008460	29.08%	5.729%
6	8.963	1178	1186	1201	rBV	1202153	2433507	70.17%	13.824%
7	9.216	1220	1229	1242	rVB	27182	56120	1.62%	0.319%
8	10.439	1428	1437	1457	rBV	1903228	3468002	100.00%	19.700%
9	11.739	1650	1658	1678	rBV	1830331	3191065	92.01%	18.127%
10	12.727	1817	1826	1841	rBV	1311781	2215723	63.89%	12.587%
11	13.668	1978	1986	2000	rBV	1356482	2297438	66.25%	13.051%




Sum of corrected areas: 17603904

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN033022\
Data File : VN071687.D
Acq On : 31 Mar 2022 03:21
Operator : JC\MD
Sample : N2075-10
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-178S-20220322

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

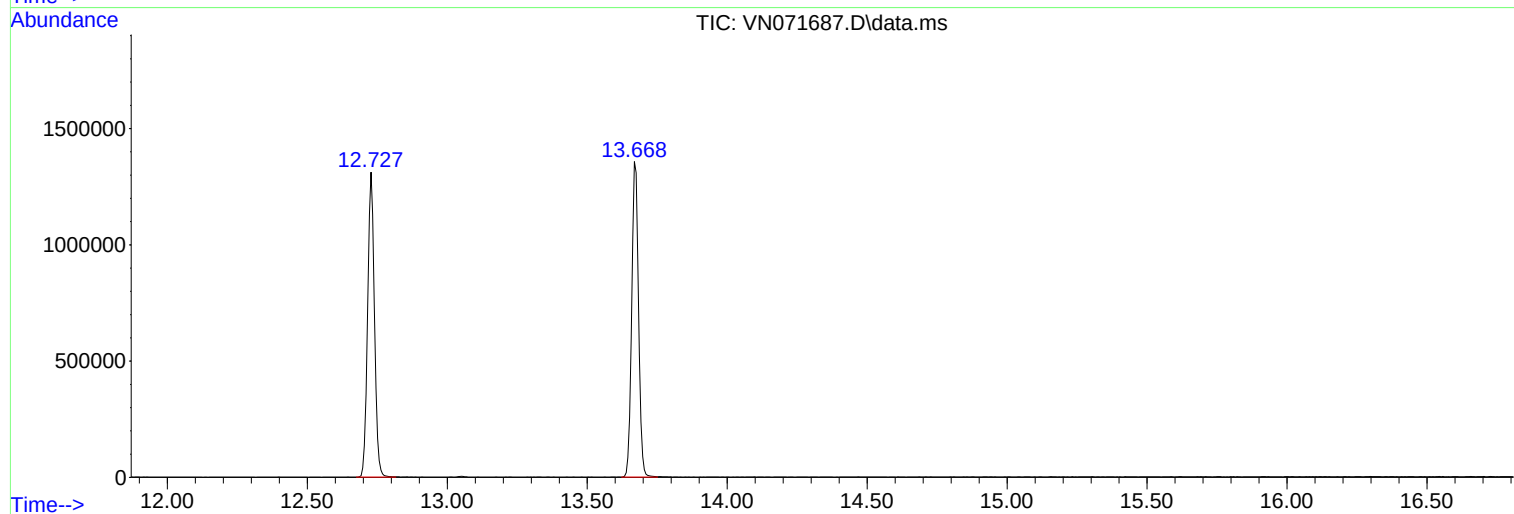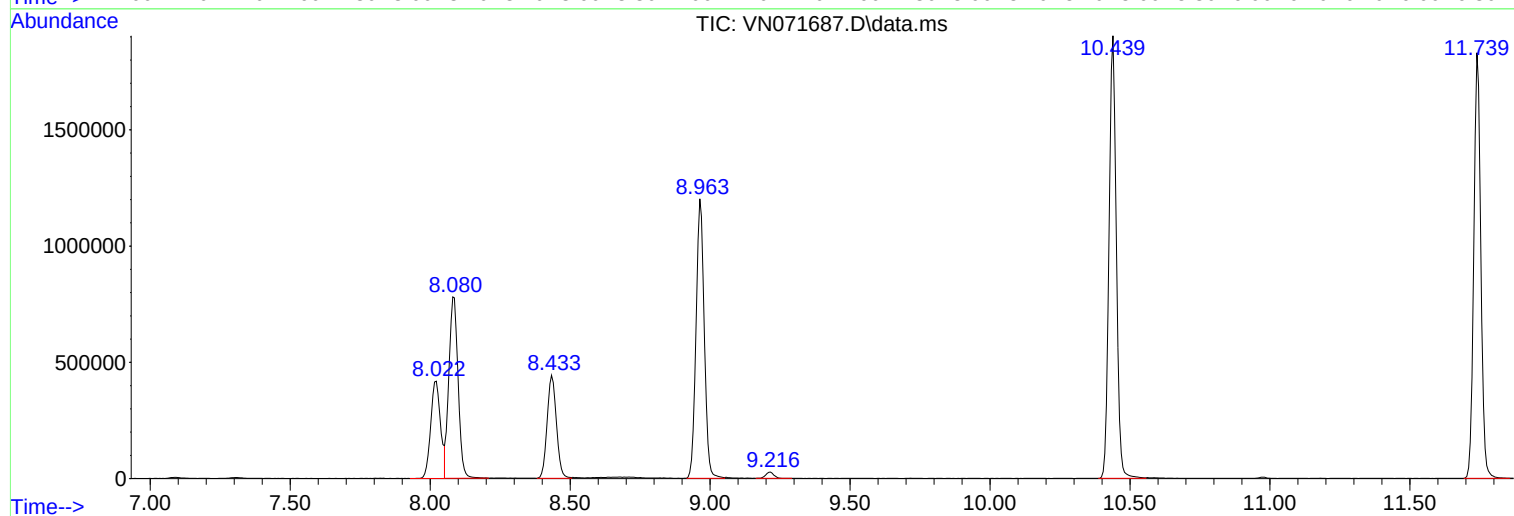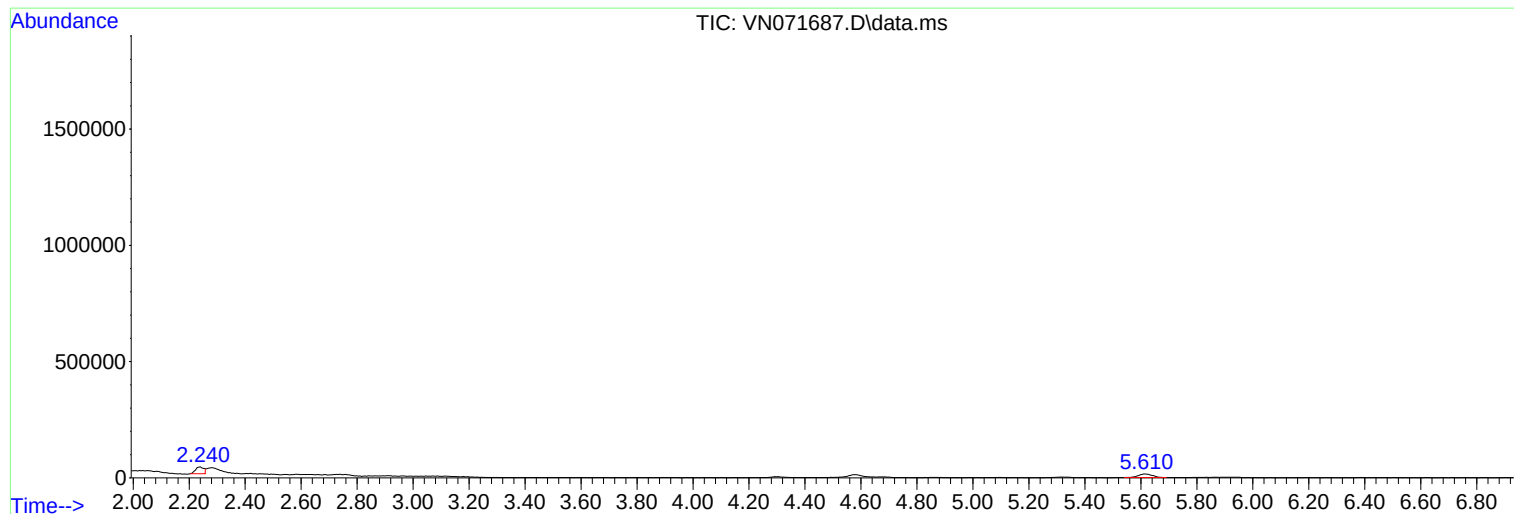

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN033022\
Data File : VN071687.D
Acq On : 31 Mar 2022 03:21
Operator : JC\MD
Sample : N2075-10
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-178S-20220322

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN033022\
Data File : VN071687.D
Acq On : 31 Mar 2022 03:21
Operator : JC\MD
Sample : N2075-10
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-178S-20220322

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc