

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN033022\  
 Data File : VN071688.D  
 Acq On : 31 Mar 2022 03:45  
 Operator : JC\MD  
 Sample : N2075-12  
 Misc : 5.0mL/MSVOA\_N/WATER  
 ALS Vial : 45 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 MW179D-20220322

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N033022W.M

Title : SW846 8260

Signal : TIC: VN071688.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.246       | 36            | 44          | 45           | rBV3     | 37515          | 72763         | 2.08%           | 0.336%        |
| 2         | 4.569       | 430           | 439         | 452          | rBV3     | 11629          | 42448         | 1.21%           | 0.196%        |
| 3         | 7.322       | 895           | 907         | 922          | rBV      | 219568         | 595380        | 17.02%          | 2.745%        |
| 4         | 8.016       | 1014          | 1025        | 1031         | rBV      | 406857         | 1013795       | 28.98%          | 4.675%        |
| 5         | 8.081       | 1031          | 1036        | 1053         | rVB      | 774279         | 1738490       | 49.70%          | 8.016%        |
| 6         | 8.433       | 1085          | 1096        | 1108         | rBV      | 427887         | 983537        | 28.12%          | 4.535%        |
| 7         | 8.963       | 1177          | 1186        | 1206         | rBV      | 1150898        | 2370338       | 67.76%          | 10.930%       |
| 8         | 9.216       | 1219          | 1229        | 1251         | rBV      | 1684690        | 3497998       | 100.00%         | 16.129%       |
| 9         | 10.439      | 1427          | 1437        | 1459         | rBV      | 1833825        | 3373063       | 96.43%          | 15.553%       |
| 10        | 10.974      | 1520          | 1528        | 1539         | rBV      | 326224         | 578959        | 16.55%          | 2.670%        |
| 11        | 11.739      | 1650          | 1658        | 1673         | rBV      | 1764493        | 3072940       | 87.85%          | 14.169%       |
| 12        | 12.727      | 1818          | 1826        | 1840         | rBV      | 1255792        | 2134858       | 61.03%          | 9.844%        |
| 13        | 13.668      | 1978          | 1986        | 2000         | rBV      | 1278449        | 2212481       | 63.25%          | 10.202%       |




Sum of corrected areas: 21687050

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN033022\  
Data File : VN071688.D  
Acq On : 31 Mar 2022 03:45  
Operator : JC\MD  
Sample : N2075-12  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 45 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
MW179D-20220322

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N033022W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

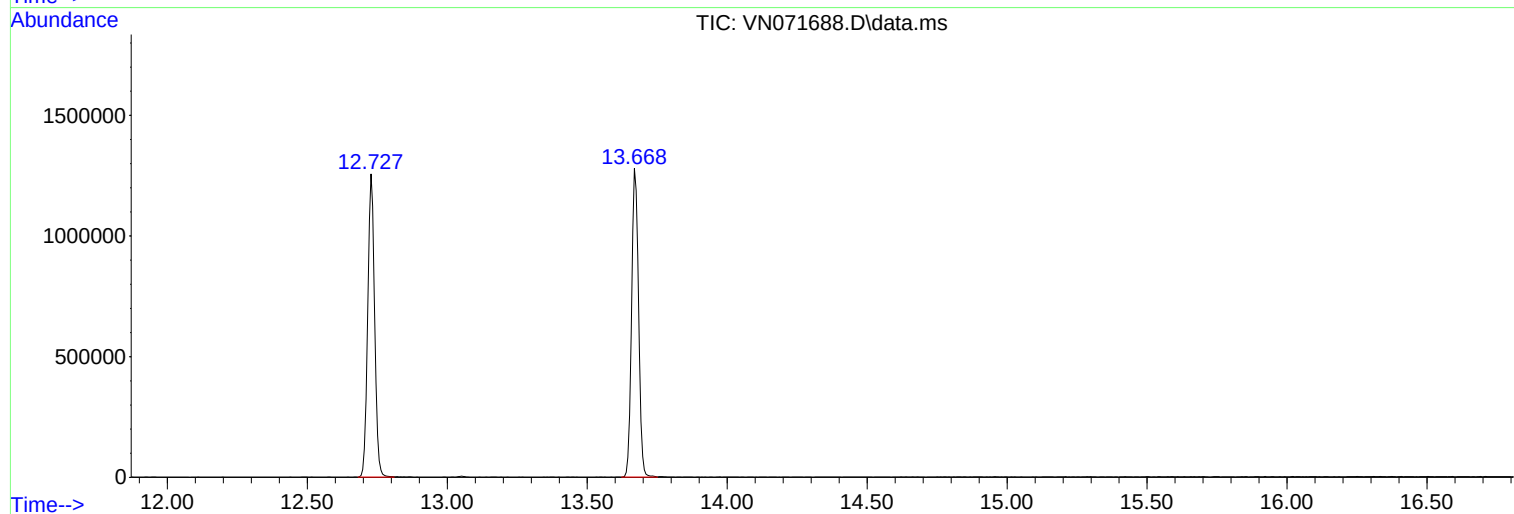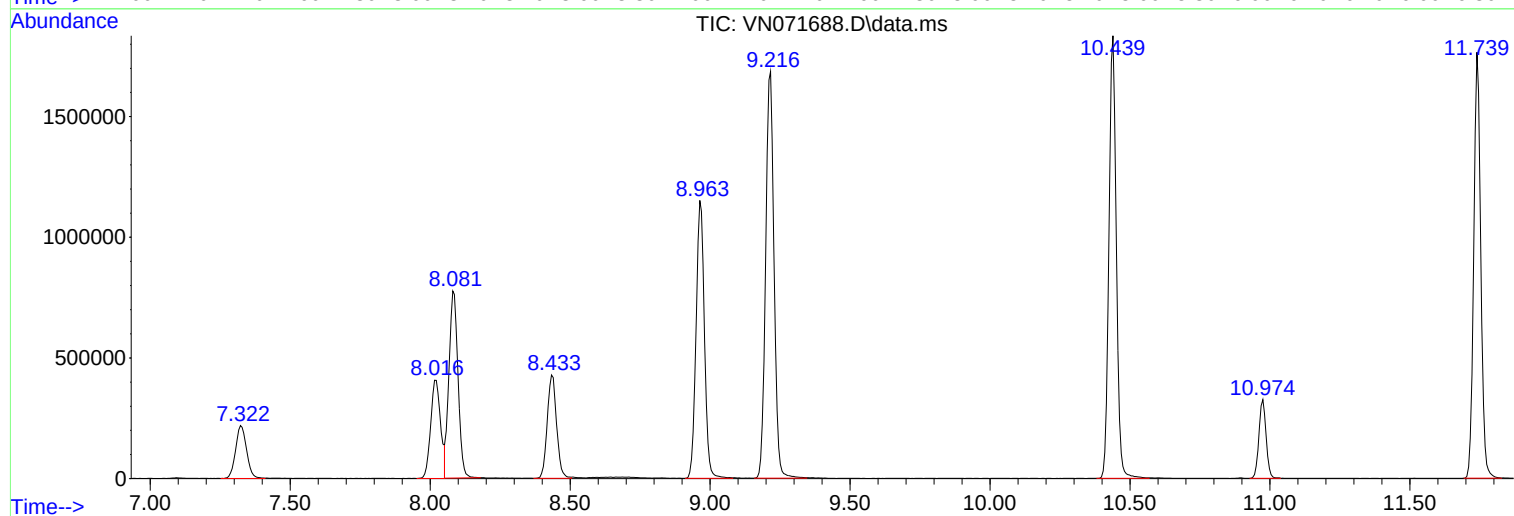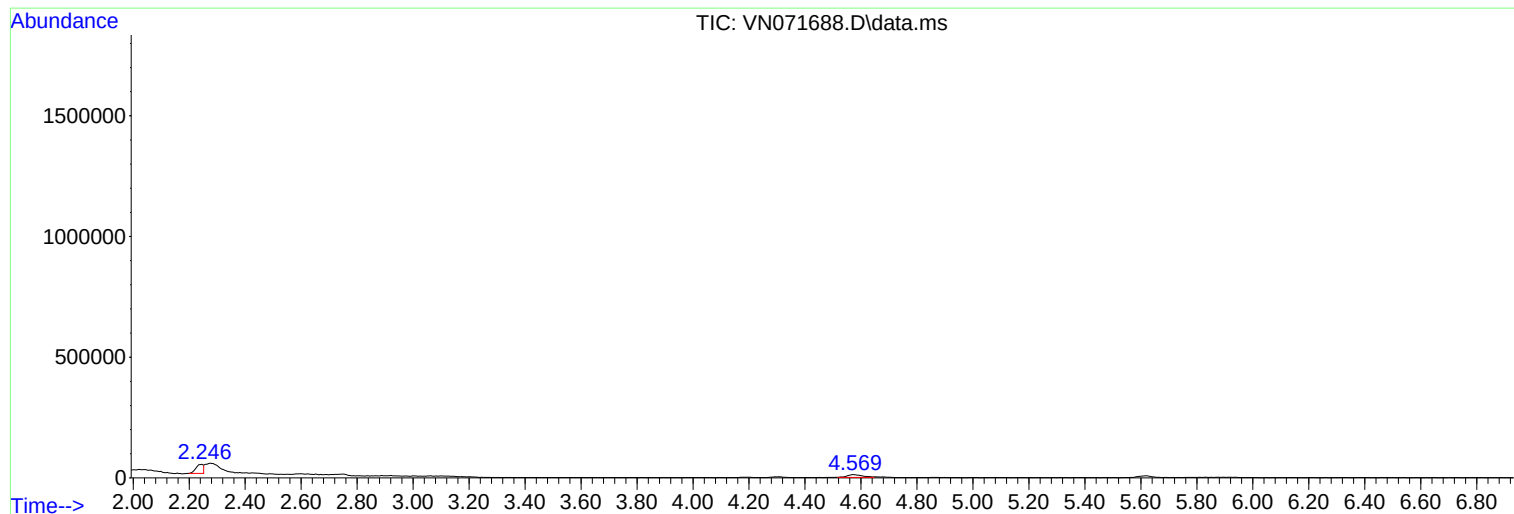

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN033022\  
Data File : VN071688.D  
Acq On : 31 Mar 2022 03:45  
Operator : JC\MD  
Sample : N2075-12  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 45 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
MW179D-20220322

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N033022W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN033022\  
Data File : VN071688.D  
Acq On : 31 Mar 2022 03:45  
Operator : JC\MD  
Sample : N2075-12  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 45 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
MW179D-20220322

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N033022W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |