

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN033121\
 Data File : VN066441.D
 Acq On : 31 Mar 2021 14:11
 Operator : JC/MD
 Sample : M1838-02
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PHC-BEAPT-001

Quant Time: Apr 01 01:37:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N032521W.M
 Quant Title : SW846 8260
 QLast Update : Fri Mar 26 16:26:01 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.585	168	443884	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.515	114	673440	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.347	117	613971	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.289	152	217559	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.947	65	288626	48.91	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	97.82%		
35) Dibromofluoromethane	7.507	113	219807	49.24	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	98.48%		
50) Toluene-d8	10.028	98	898753	53.08	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	106.16%		
62) 4-Bromofluorobenzene	12.345	95	252069	42.86	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	85.72%		
Target Compounds						Qvalue
3) Chloromethane	2.017	50	5616	Below Cal	#	85
5) Bromomethane	2.524	94	1565	0.36	ug/l	93
11) Tert butyl alcohol	4.731	59	184	0.20	ug/l #	85
13) Acrolein	3.532	56	4879	Below Cal		94
16) Acetone	3.739	43	131030	41.10	ug/l	97
17) Carbon Disulfide	3.967	76	9381	0.62	ug/l #	85
18) Methyl Acetate	4.237	43	135415	16.26	ug/l	99
20) Methylene Chloride	4.452	84	38342	5.65	ug/l	97
25) 2-Butanone	6.756	43	17858	5.12	ug/l	97
29) Tetrahydrofuran	7.129	42	1046	0.46	ug/l #	80
31) Cyclohexane	7.577	56	9482	1.16	ug/l #	22
36) 1,1-Dichloropropene	7.582	75	32853	5.19	ug/l #	48
37) Ethyl Acetate	6.756	43	17858	2.56	ug/l #	69
38) Carbon Tetrachloride	7.587	117	40624	6.39	ug/l #	17
43) Isopropyl Acetate	8.091	43	32240	2.71	ug/l	98
45) 1,2-Dichloropropane	9.202	63	1487	0.29	ug/l #	43
48) Methyl methacrylate	9.119	41	7068	1.25	ug/l #	30
49) 1,4-Dioxane	9.124	88	25	0.35	ug/l #	1
51) 4-Methyl-2-Pentanone	9.923	43	11140	1.60	ug/l	98
52) Toluene	10.092	92	3430	0.29	ug/l	97
54) cis-1,3-Dichloropropene	9.843	75	46066	5.73	ug/l #	61
57) 1,3-Dichloropropane	10.706	76	19217	2.46	ug/l #	42
59) 2-Hexanone	10.706	43	272307	55.88	ug/l #	53
68) m/p-Xylenes	11.562	106	5404	0.64	ug/l	95
71) Bromoform	12.348	173	2519	0.64	ug/l #	1
74) N-amyl acetate	12.002	43	259	3.23	ug/l #	54
76) 1,2,3-Trichloropropane	12.342	75	128163	26.85	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.342	75	128163	80.74	ug/l #	12
84) 1,2,4-Trimethylbenzene	12.986	105	5369	0.42	ug/l	99
95) Naphthalene	15.081	128	8815	1.75	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN033121\
Data File : VN066441.D
Acq On : 31 Mar 2021 14:11
Operator : JC/MD
Sample : M1838-02
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PHC-BEAPT-001

Quant Time: Apr 01 01:37:13 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N032521W.M
Quant Title : SW846 8260
QLast Update : Fri Mar 26 16:26:01 2021
Response via : Initial Calibration




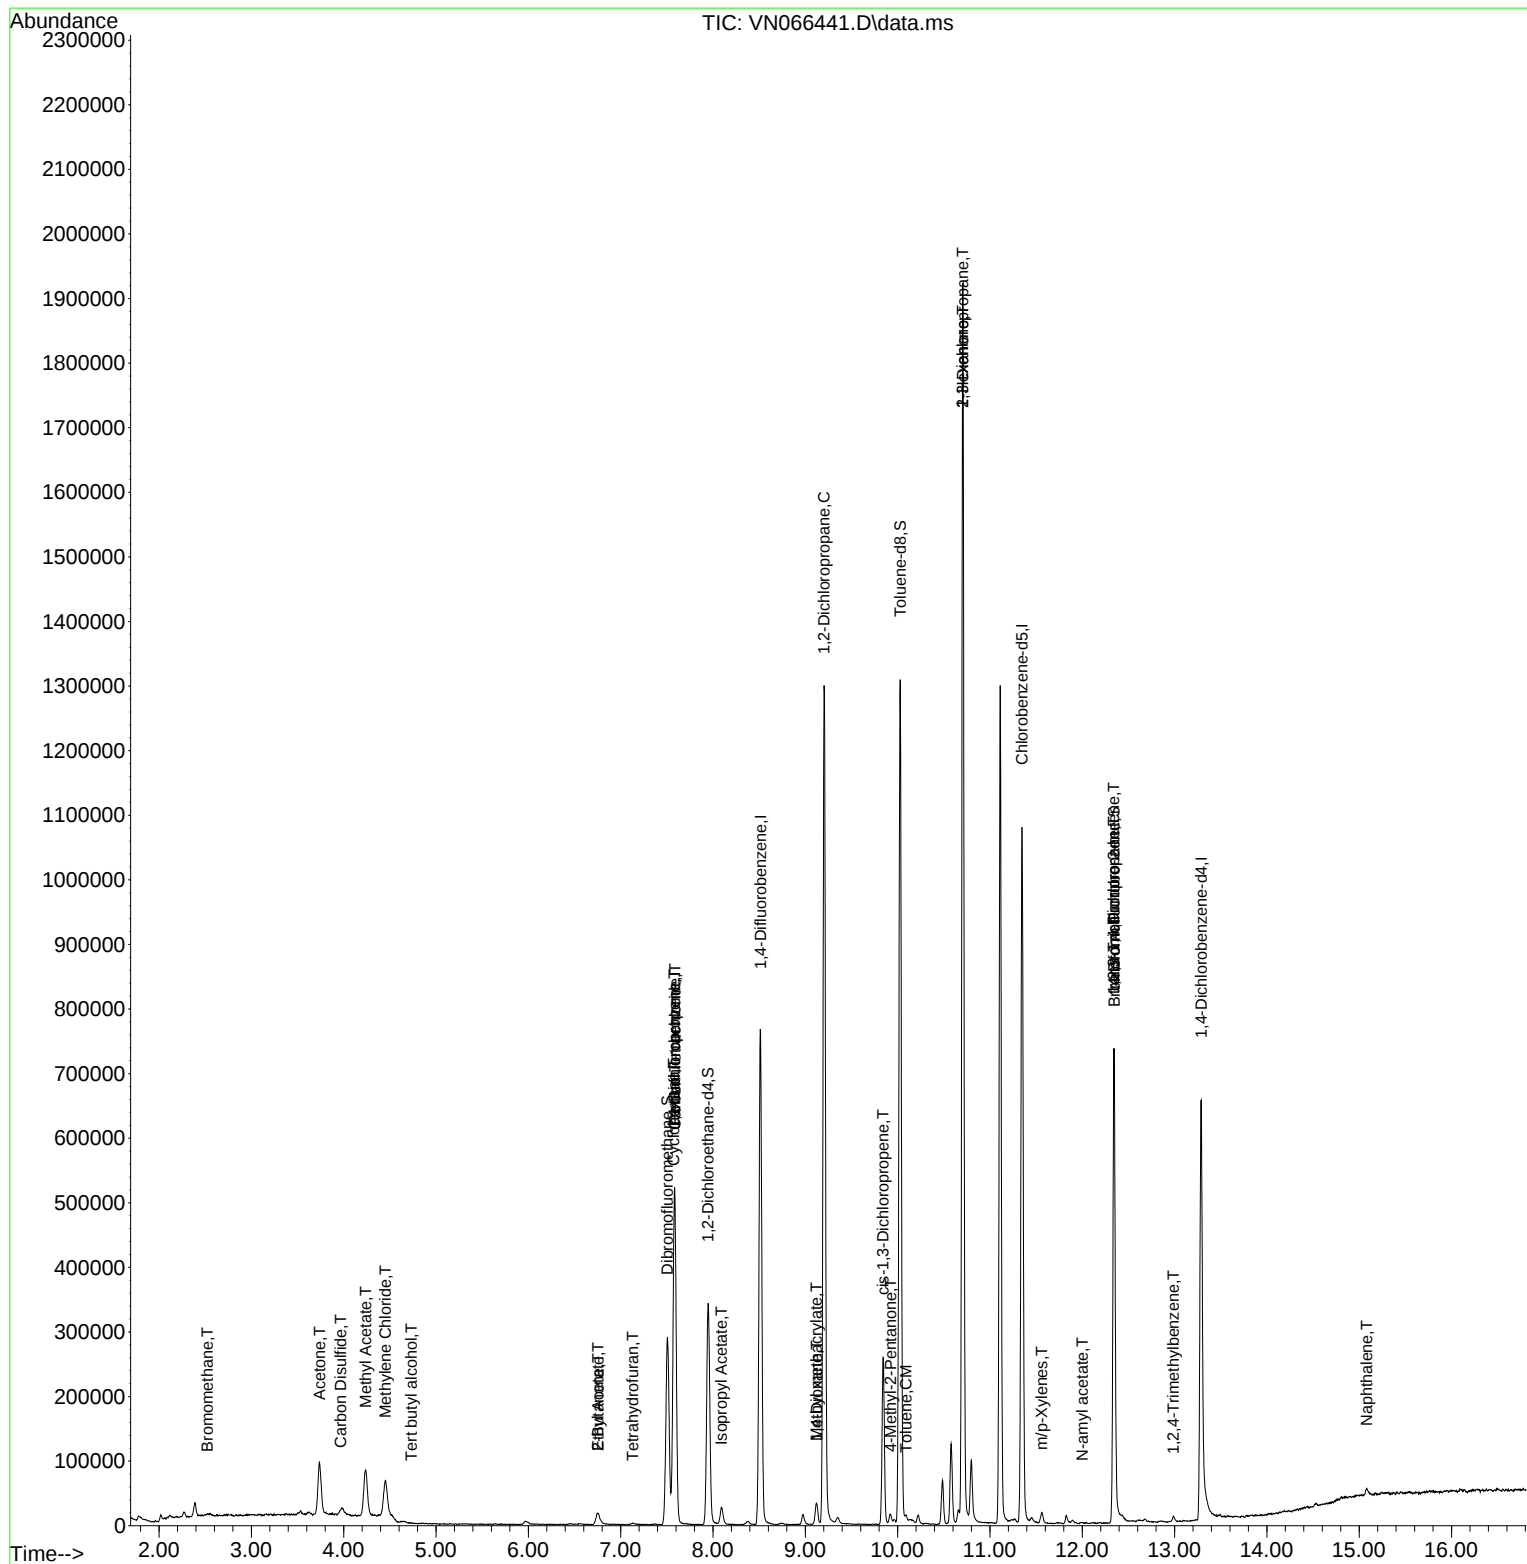




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.585 min Scan# 2198
Delta R.T. -0.000 min
Lab File: VN066441.D
Acq: 31 Mar 2021 14:11




Instrument :
MSVOA_N
ClientSampleId :
PHC-BEAPT-001


Tgt Ion:168 Resp: 443884
Ion Ratio Lower Upper
168 100
99 52.2 41.1 61.7

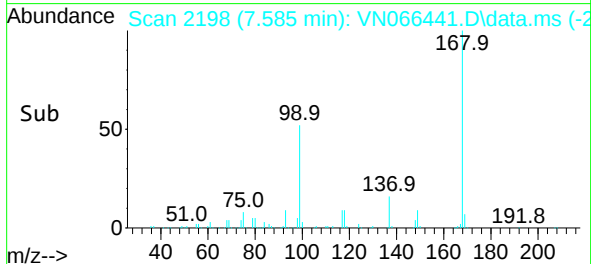

#5
Bromomethane
Concen: 0.36 ug/l
RT: 2.524 min Scan# 311
Delta R.T. 0.019 min
Lab File: VN066441.D
Acq: 31 Mar 2021 14:11

Tgt Ion: 94 Resp: 1565
Ion Ratio Lower Upper
94 100
96 88.1 75.8 113.6

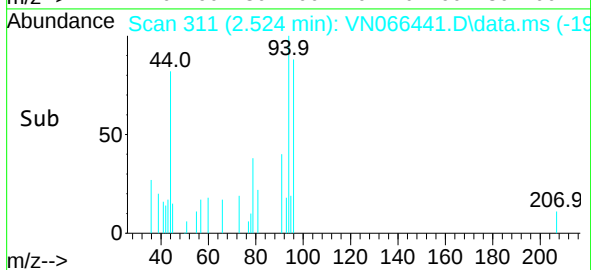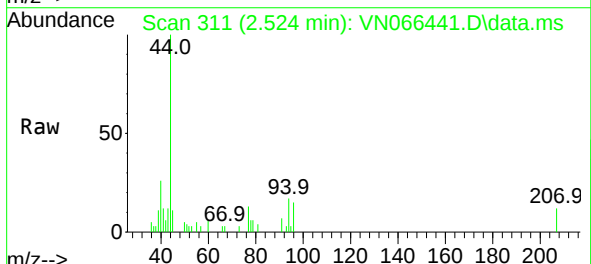




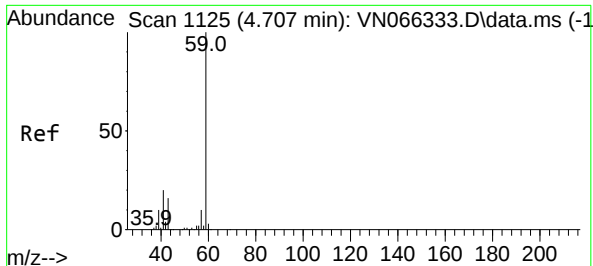


#11

Tert butyl alcohol
Concen: 0.20 ug/l
RT: 4.731 min Scan# 1134
Delta R.T. 0.024 min
Lab File: VN066441.D
Acq: 31 Mar 2021 14:11

Instrument :
MSVOA_N
ClientSampleId :
PHC-BEAPT-001




Tgt Ion: 59 Resp: 184
Ion Ratio Lower Upper
59 100
57 0.0 4.1 6.1#

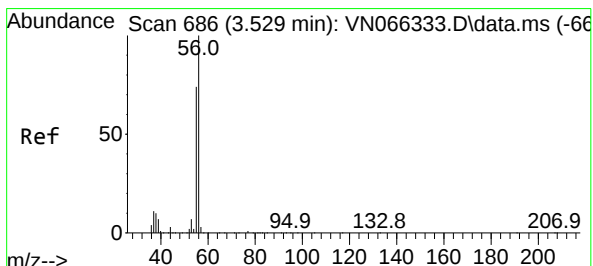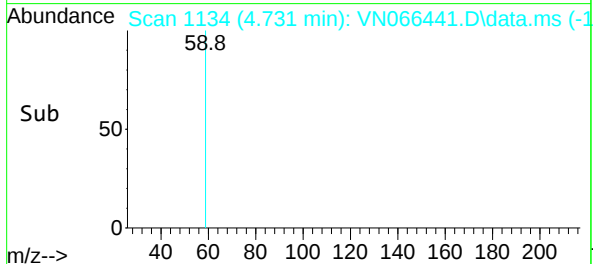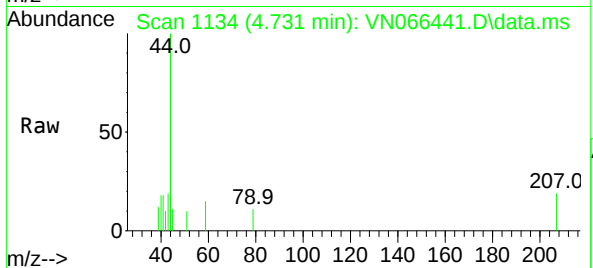


#13

Acrolein
Concen: Below Cal
RT: 3.532 min Scan# 687
Delta R.T. 0.003 min
Lab File: VN066441.D
Acq: 31 Mar 2021 14:11

Tgt Ion: 56 Resp: 4879
Ion Ratio Lower Upper
56 100
55 67.6 57.9 86.9


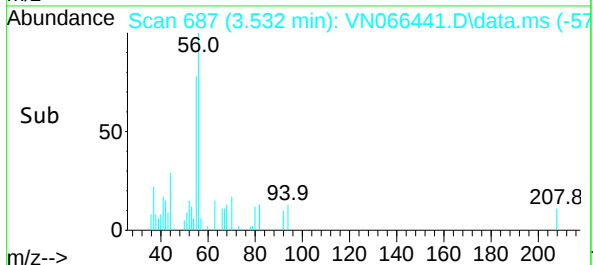

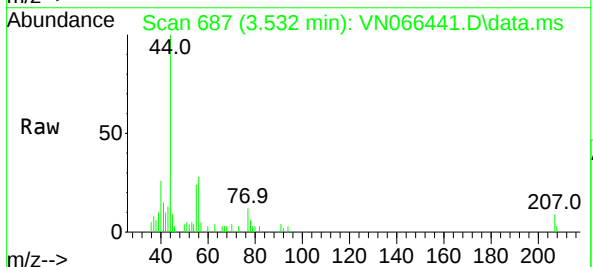




#16
Acetone
Concen: 41.10 ug/l
RT: 3.739 min Scan# 764
Delta R.T. 0.003 min
Lab File: VN066441.D
Acq: 31 Mar 2021 14:11




Instrument :
MSVOA_N
ClientSampleId :
PHC-BEAPT-001


Tgt Ion: 43 Resp: 131030
Ion Ratio Lower Upper
43 100
58 31.4 23.8 35.8

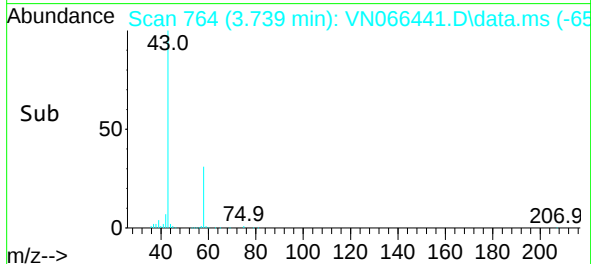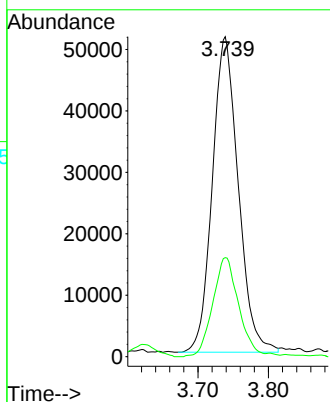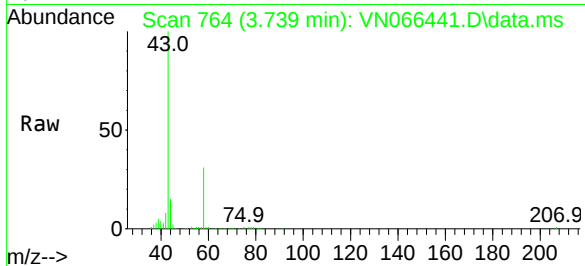

#17
Carbon Disulfide
Concen: 0.62 ug/l
RT: 3.967 min Scan# 849
Delta R.T. 0.003 min
Lab File: VN066441.D
Acq: 31 Mar 2021 14:11

Tgt Ion: 76 Resp: 9381
Ion Ratio Lower Upper
76 100
78 3.8 7.4 11.0#

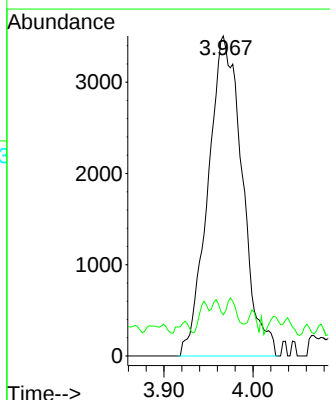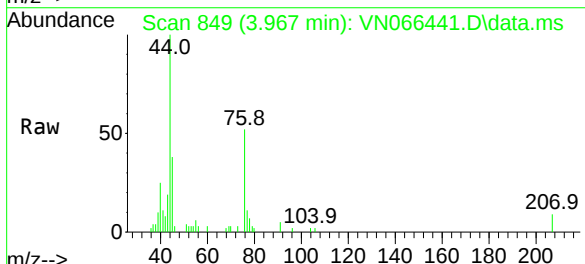



#18

Methyl Acetate

Concen: 16.26 ug/l

RT: 4.237 min Scan# 950

Delta R.T. 0.003 min

Lab File: VN066441.D





Acq: 31 Mar 2021 14:11

Tgt Ion: 43 Resp: 135415

Ion Ratio Lower Upper

43 100

74 21.3 17.6 26.4

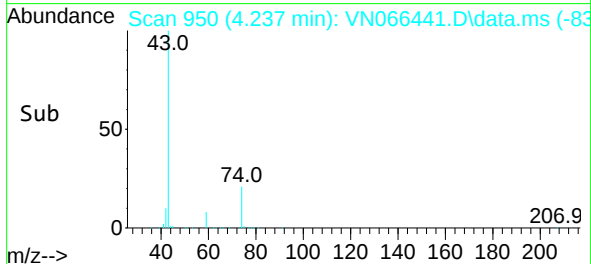

#20

Methylene Chloride

Concen: 5.65 ug/l

RT: 4.452 min Scan# 1030

Delta R.T. 0.000 min

Lab File: VN066441.D

Acq: 31 Mar 2021 14:11

Tgt Ion: 84 Resp: 38342




Ion Ratio Lower Upper


84 100

49 129.9 105.0 157.6

51 39.8 31.6 47.4

86 58.7 53.0 79.6

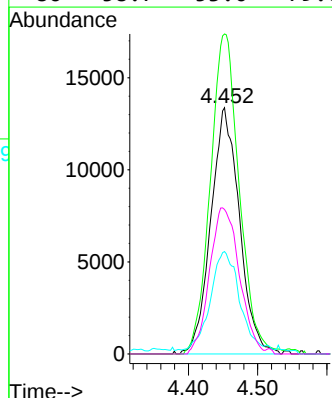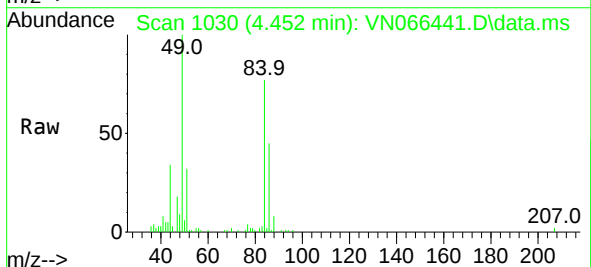

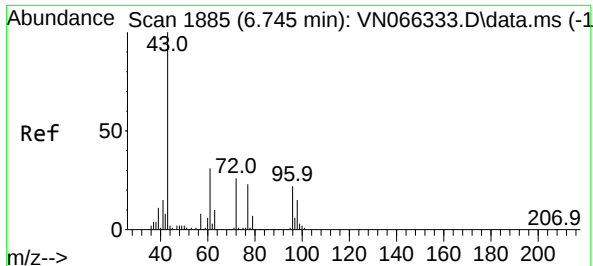

#25

2-Butanone

Concen: 5.12 ug/l

RT: 6.756 min Scan# 1889

Delta R.T. 0.011 min





Lab File: VN066441.D

Acq: 31 Mar 2021 14:11

Tgt Ion: 43 Resp: 17858

Ion Ratio Lower Upper

43	100		
72	27.4	20.7	31.1

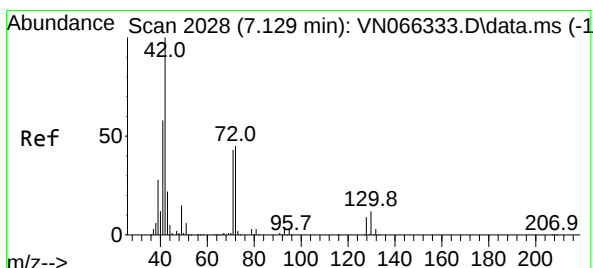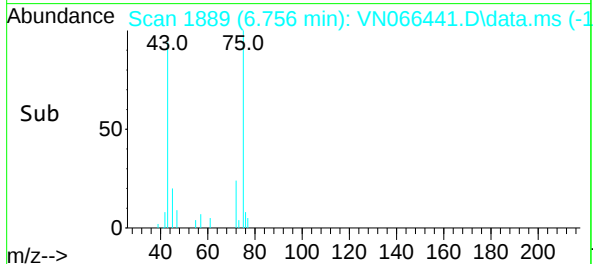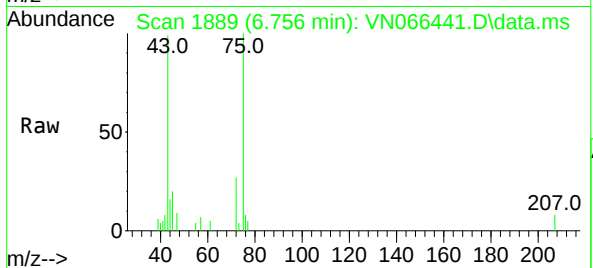

#29

Tetrahydrofuran

Concen: 0.46 ug/l

RT: 7.129 min Scan# 2028

Delta R.T. 0.000 min




Lab File: VN066441.D


Acq: 31 Mar 2021 14:11

Tgt Ion: 42 Resp: 1046

Ion Ratio Lower Upper

42	100		
72	29.2	35.2	52.8#
71	30.5	33.1	49.7#


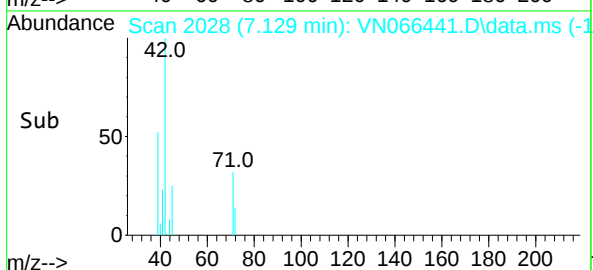

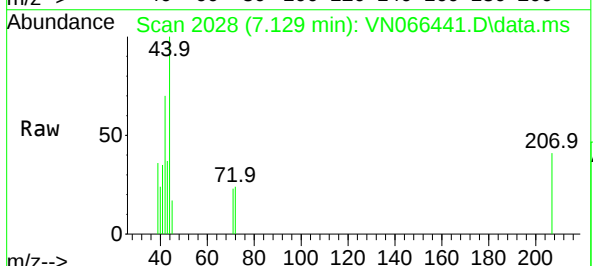




#31
Cyclohexane
Concen: 1.16 ug/l
RT: 7.577 min Scan# 2195
Delta R.T. 0.008 min
Lab File: VN066441.D
Acq: 31 Mar 2021 14:11




Instrument :
MSVOA_N
ClientSampleId :
PHC-BEAPT-001


Tgt Ion: 56 Resp: 9482
Ion Ratio Lower Upper
56 100
69 139.8 26.6 40.0#
84 118.6 68.7 103.1#

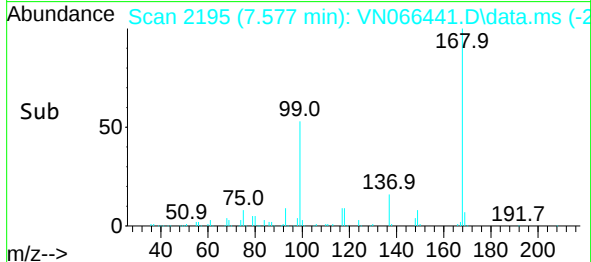

#33
1,2-Dichloroethane-d4
Concen: 48.91 ug/l
RT: 7.947 min Scan# 2333
Delta R.T. -0.002 min
Lab File: VN066441.D
Acq: 31 Mar 2021 14:11

Tgt Ion: 65 Resp: 288626
Ion Ratio Lower Upper
65 100
67 53.3 0.0 105.2


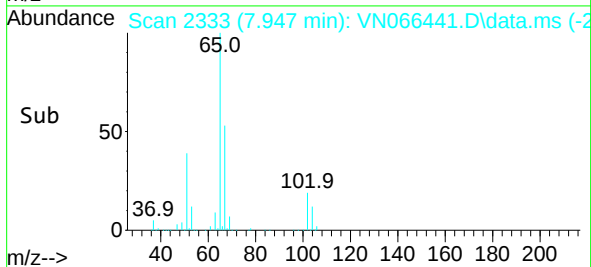

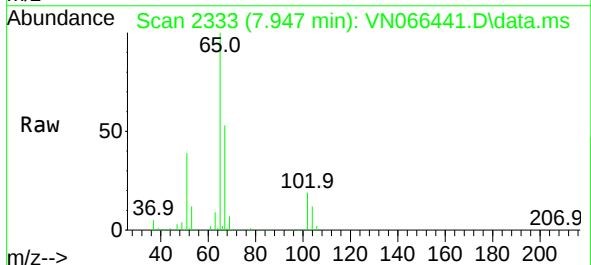




#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.515 min Scan# 2545
Delta R.T. 0.000 min
Lab File: VN066441.D
Acq: 31 Mar 2021 14:11




Instrument :
MSVOA_N
ClientSampleId :
PHC-BEAPT-001


Tgt Ion:114 Resp: 673440
Ion Ratio Lower Upper
114 100
63 21.2 0.0 42.0
88 15.5 0.0 31.0

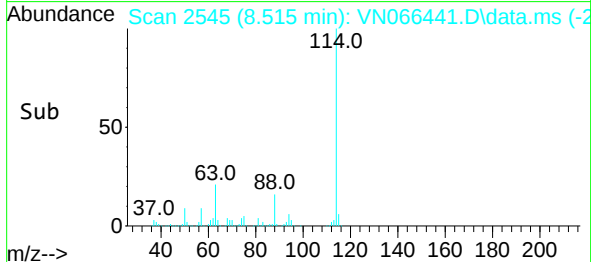

#35
Dibromofluoromethane
Concen: 49.24 ug/l
RT: 7.507 min Scan# 2169
Delta R.T. -0.000 min
Lab File: VN066441.D
Acq: 31 Mar 2021 14:11

Tgt Ion:113 Resp: 219807
Ion Ratio Lower Upper
113 100
111 102.9 81.8 122.8
192 20.9 17.1 25.7


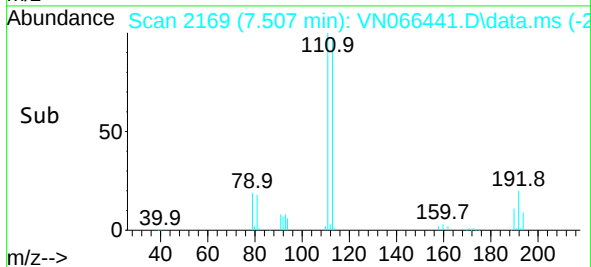

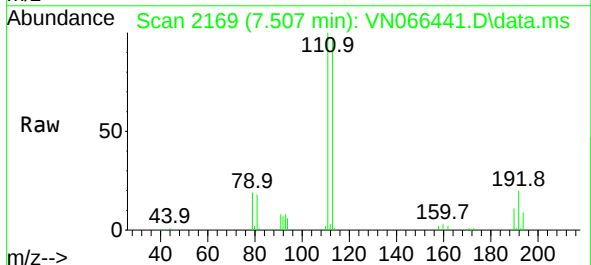


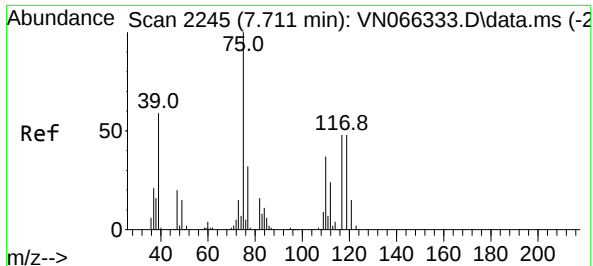

#36
1,1-Dichloropropene
Concen: 5.19 ug/l
RT: 7.582 min Scan# 2197
Delta R.T. -0.129 min
Lab File: VN066441.D
Acq: 31 Mar 2021 14:11




Instrument :
MSVOA_N
ClientSampleId :
PHC-BEAPT-001


Tgt Ion: 75 Resp: 32853
Ion Ratio Lower Upper
75 100
110 7.4 18.1 54.3#
77 0.0 25.0 37.4#

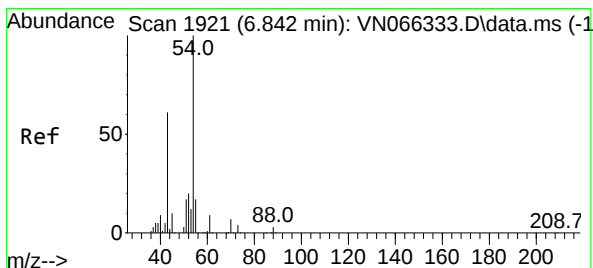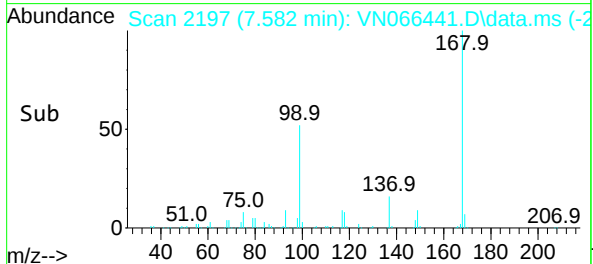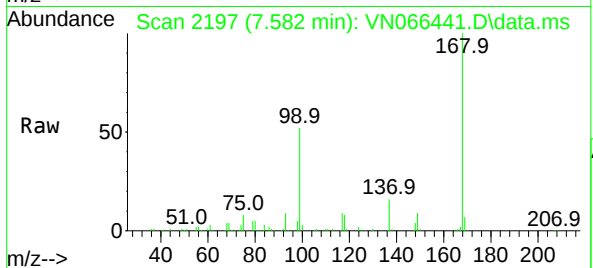

#37
Ethyl Acetate
Concen: 2.56 ug/l
RT: 6.756 min Scan# 1889
Delta R.T. -0.086 min
Lab File: VN066441.D
Acq: 31 Mar 2021 14:11


Tgt Ion: 43 Resp: 17858
Ion Ratio Lower Upper
43 100
61 0.5 11.1 16.7#
70 0.0 8.0 12.0#

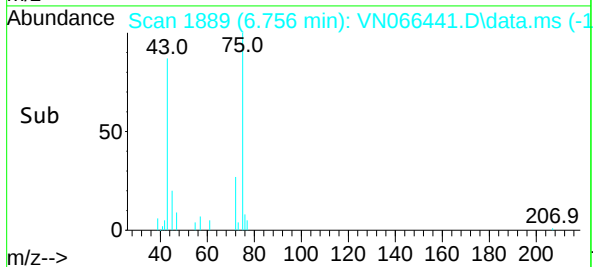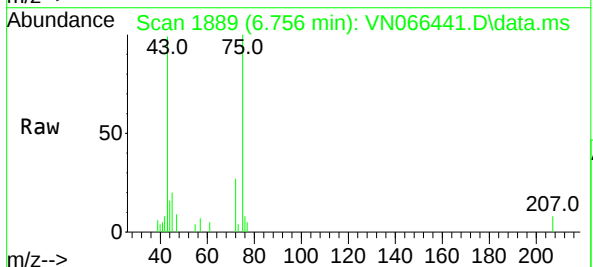






#38
Carbon Tetrachloride
Concen: 6.39 ug/l
RT: 7.587 min Scan# 2199
Delta R.T. -0.105 min
Lab File: VN066441.D
Acq: 31 Mar 2021 14:11


Instrument :
MSVOA_N
ClientSampleId :
PHC-BEAPT-001





Tgt Ion:117 Resp: 40624
Ion Ratio Lower Upper
117 100
119 6.6 77.2 115.8#
121 0.0 24.2 36.4#




#43
Isopropyl Acetate
Concen: 2.71 ug/l
RT: 8.091 min Scan# 2387
Delta R.T. -0.003 min
Lab File: VN066441.D
Acq: 31 Mar 2021 14:11



Tgt Ion: 43 Resp: 32240
Ion Ratio Lower Upper
43 100
61 19.1 15.5 23.3
87 11.9 10.5 15.7

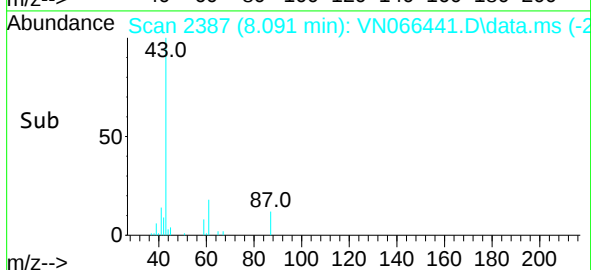







#45

1,2-Dichloropropane
Concen: 0.29 ug/l
RT: 9.202 min Scan# 2801
Delta R.T. 0.153 min
Lab File: VN066441.D
Acq: 31 Mar 2021 14:11

Instrument :
MSVOA_N
ClientSampleId :
PHC-BEAPT-001




Tgt Ion: 63 Resp: 1487
Ion Ratio Lower Upper
63 100
65 0.0 25.5 38.3#

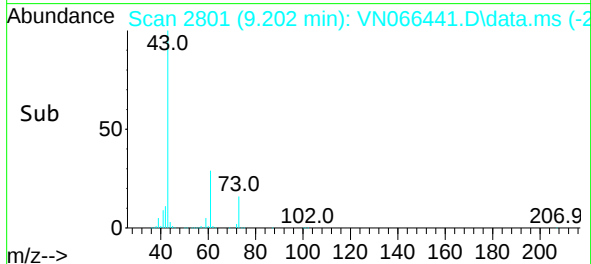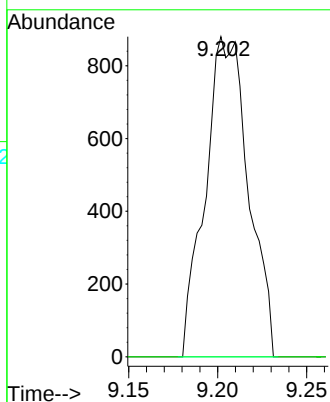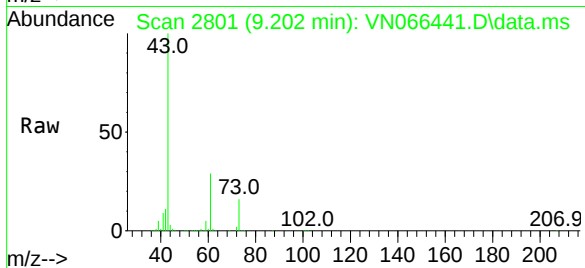


#48

Methyl methacrylate
Concen: 1.25 ug/l
RT: 9.119 min Scan# 2770
Delta R.T. -0.016 min
Lab File: VN066441.D
Acq: 31 Mar 2021 14:11

Tgt Ion: 41 Resp: 7068
Ion Ratio Lower Upper
41 100
69 0.0 66.2 99.4#
39 31.3 51.5 77.3#

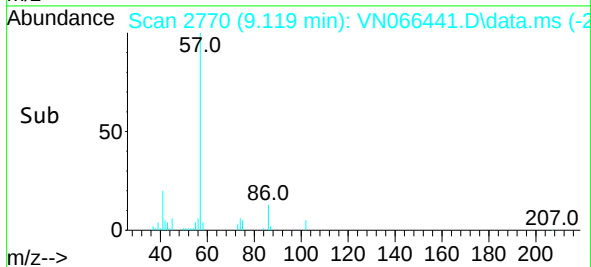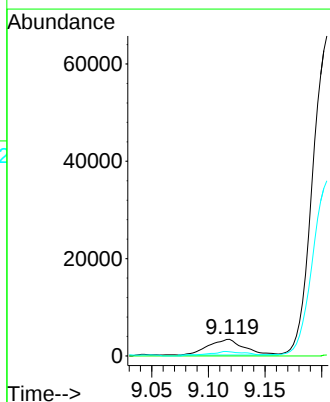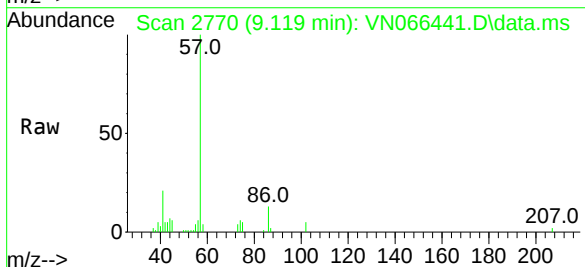



#49

1,4-Dioxane

Concen: 0.35 ug/l

RT: 9.124 min Scan# 2772

Delta R.T. -0.013 min

Lab File: VN066441.D


Acq: 31 Mar 2021 14:11

Instrument :




MSVOA_N

ClientSampleId :

PHC-BEAPT-001



Tgt Ion:	88	Resp:	25
Ion Ratio	Lower	Upper	
88	100		
43	0.0	28.2	42.4#
58	3300.0	56.6	84.8#



#50

Toluene-d8

Concen: 53.08 ug/l




RT: 10.028 min Scan# 3109


Delta R.T. -0.000 min

Lab File: VN066441.D

Acq: 31 Mar 2021 14:11

Tgt Ion:	98	Resp:	898753
Ion Ratio	Lower	Upper	
98	100		
100	63.0	50.5	75.7


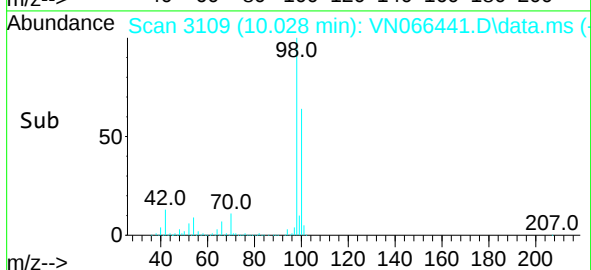






#51
4-Methyl-2-Pentanone
Concen: 1.60 ug/l
RT: 9.923 min Scan# 3070
Delta R.T. 0.000 min
Lab File: VN066441.D
Acq: 31 Mar 2021 14:11




Instrument :
MSVOA_N
ClientSampleId :
PHC-BEAPT-001


Tgt Ion: 43 Resp: 11140
Ion Ratio Lower Upper
43 100
58 37.5 30.8 46.2

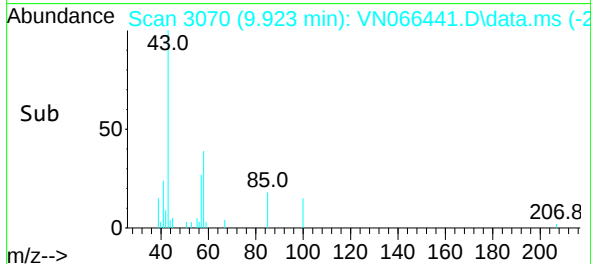

#52
Toluene
Concen: 0.29 ug/l
RT: 10.092 min Scan# 3133
Delta R.T. 0.000 min
Lab File: VN066441.D
Acq: 31 Mar 2021 14:11


Tgt Ion: 92 Resp: 3430
Ion Ratio Lower Upper
92 100
91 169.2 138.8 208.2

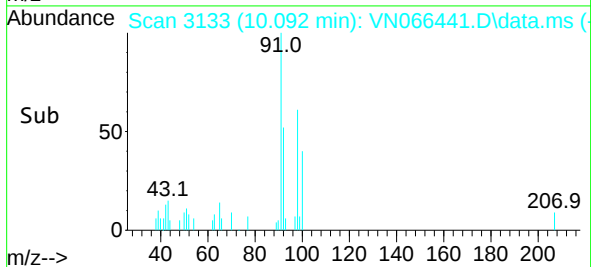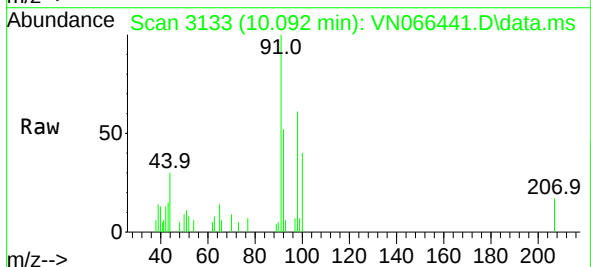






#54
 cis-1,3-Dichloropropene
 Concen: 5.73 ug/l
 RT: 9.843 min Scan# 3040
 Delta R.T. 0.067 min
 Lab File: VN066441.D
 Acq: 31 Mar 2021 14:11

Instrument :
 MSVOA_N
 ClientSampleId :
 PHC-BEAPT-001







Tgt Ion: 75 Resp: 46066
 Ion Ratio Lower Upper
 75 100
 77 0.8 25.4 38.2#
 39 33.7 44.2 66.4#

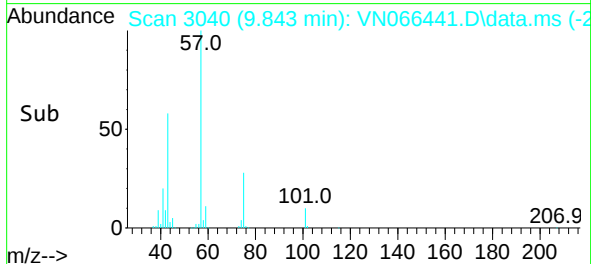

#57
 1,3-Dichloropropane
 Concen: 2.46 ug/l
 RT: 10.706 min Scan# 3362
 Delta R.T. 0.059 min
 Lab File: VN066441.D
 Acq: 31 Mar 2021 14:11

Tgt Ion: 76 Resp: 19217
 Ion Ratio Lower Upper
 76 100
 78 0.0 25.9 38.9#


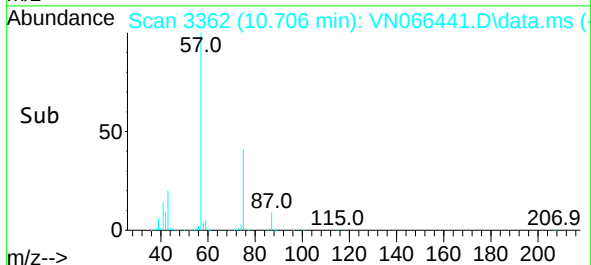

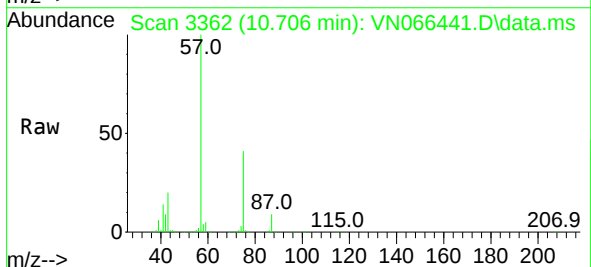


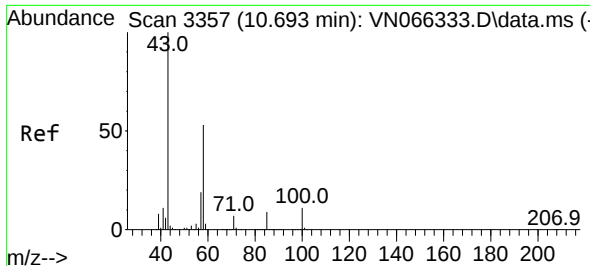

#59
2-Hexanone
Concen: 55.88 ug/l
RT: 10.706 min Scan# 3362
Delta R.T. 0.013 min
Lab File: VN066441.D
Acq: 31 Mar 2021 14:11




Instrument :
MSVOA_N
ClientSampleId :
PHC-BEAPT-001


Tgt Ion: 43 Resp: 272307
Ion Ratio Lower Upper
43 100
58 19.7 26.6 79.8#

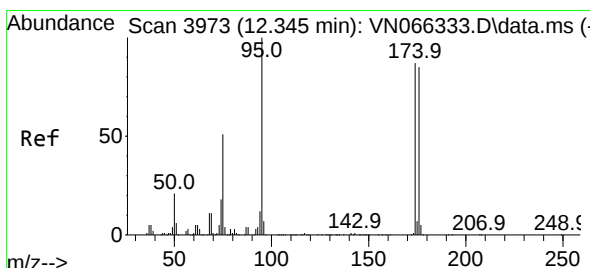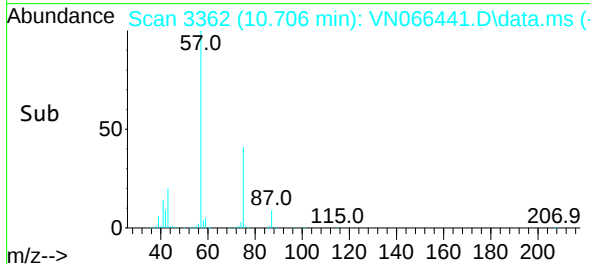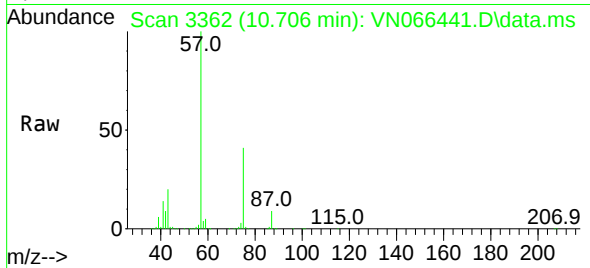

#62
4-Bromofluorobenzene
Concen: 42.86 ug/l
RT: 12.345 min Scan# 3973
Delta R.T. 0.000 min
Lab File: VN066441.D
Acq: 31 Mar 2021 14:11

Tgt Ion: 95 Resp: 252069
Ion Ratio Lower Upper
95 100
174 87.7 0.0 172.2
176 83.3 0.0 167.8


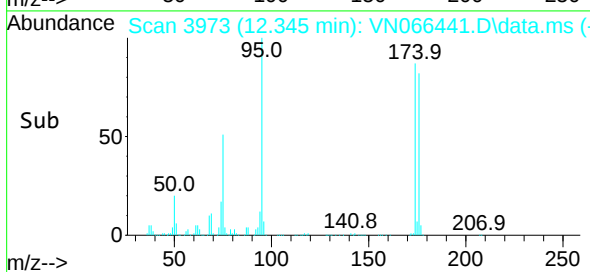

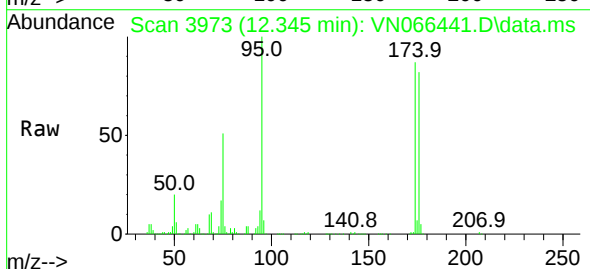


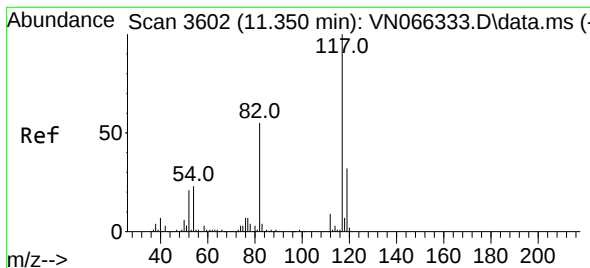

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.347 min Scan# 3601
Delta R.T. -0.003 min
Lab File: VN066441.D
Acq: 31 Mar 2021 14:11




Instrument :
MSVOA_N
ClientSampleId :
PHC-BEAPT-001


Tgt Ion:117 Resp: 613971
Ion Ratio Lower Upper
117 100
82 57.0 44.2 66.4
119 32.3 25.8 38.6

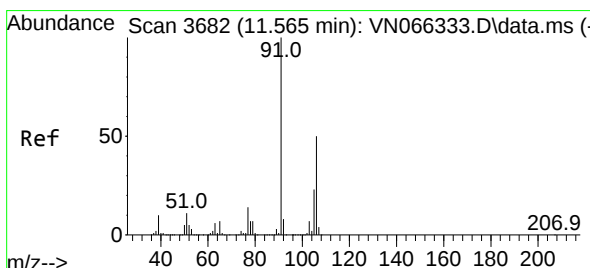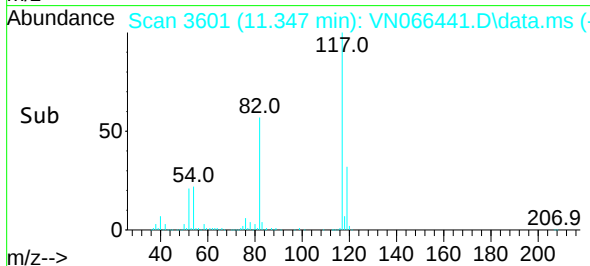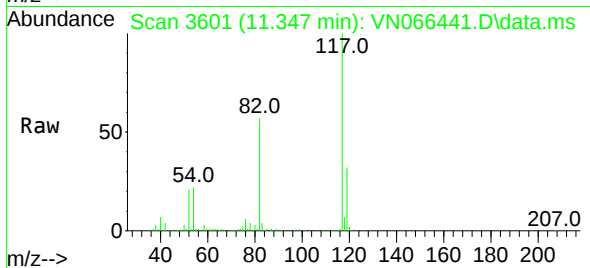

#68
m/p-Xylenes
Concen: 0.64 ug/l
RT: 11.562 min Scan# 3681
Delta R.T. -0.003 min
Lab File: VN066441.D
Acq: 31 Mar 2021 14:11

Tgt Ion:106 Resp: 5404
Ion Ratio Lower Upper
106 100
91 196.2 162.7 244.1


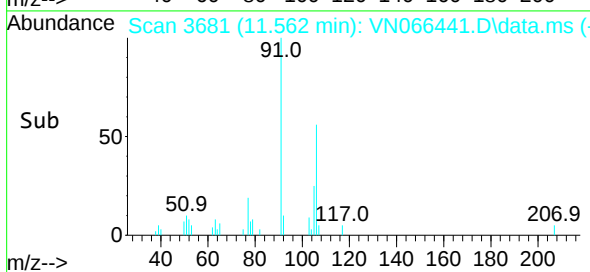

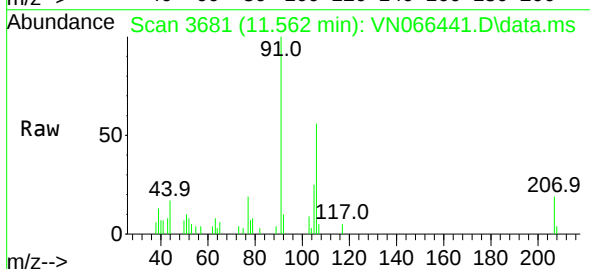


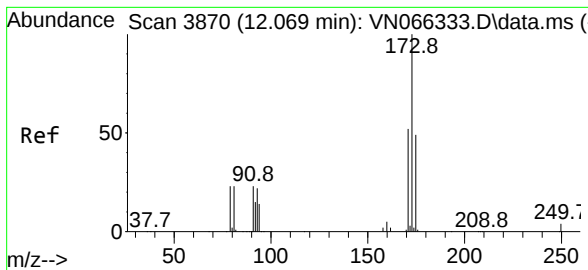

#71
Bromoform
Concen: 0.64 ug/l
RT: 12.348 min Scan# 3974
Delta R.T. 0.279 min
Lab File: VN066441.D
Acq: 31 Mar 2021 14:11




Instrument :
MSVOA_N
ClientSampleId :
PHC-BEAPT-001


Tgt Ion:173 Resp: 2519
Ion Ratio Lower Upper
173 100
175 567.7 24.3 72.8#
254 0.0 0.0 0.0

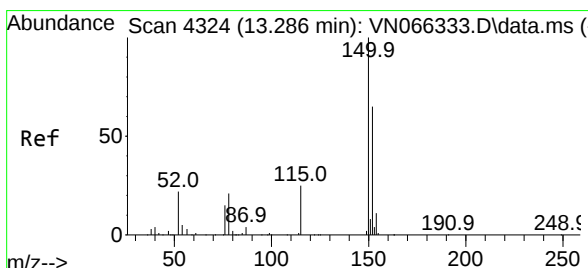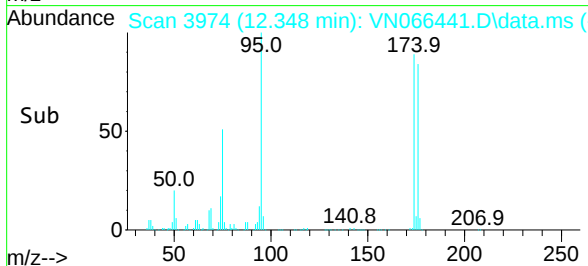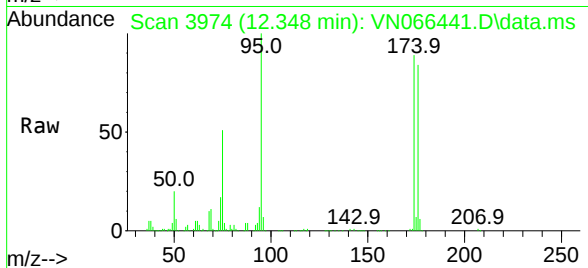

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.289 min Scan# 4325
Delta R.T. 0.003 min
Lab File: VN066441.D
Acq: 31 Mar 2021 14:11

Tgt Ion:152 Resp: 217559
Ion Ratio Lower Upper
152 100
115 55.7 27.8 83.4
150 155.0 0.0 348.4

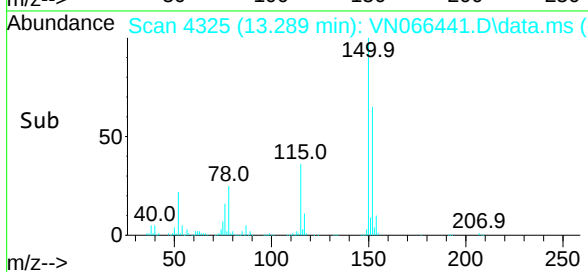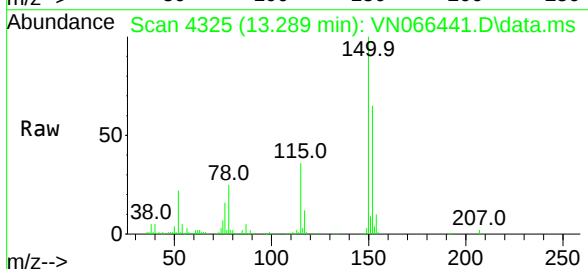







#74
N-amy1 acetate
Concen: 3.23 ug/l
RT: 12.002 min Scan# 3845
Delta R.T. -0.013 min
Lab File: VN066441.D
Acq: 31 Mar 2021 14:11

Instrument :
MSVOA_N
ClientSampleId :
PHC-BEAPT-001

Tgt Ion: 43 Resp: 259




Ion	Ratio	Lower	Upper
43	100		
70	0.0	31.2	46.8#
55	29.7	18.6	28.0#
61	0.0	18.2	27.4#

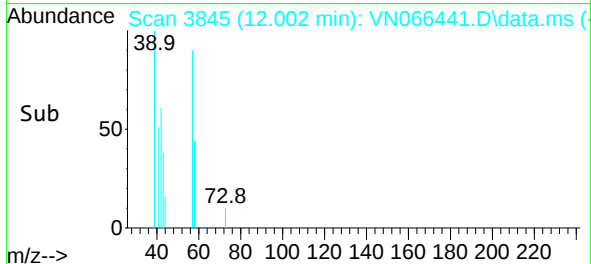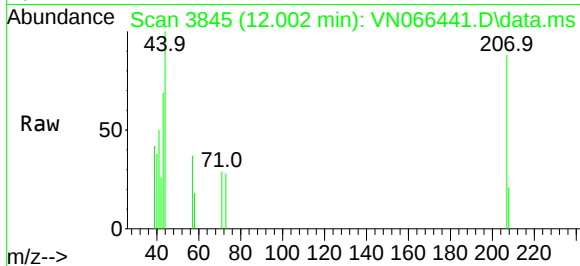


#76
1,2,3-Trichloropropane
Concen: 26.85 ug/l
RT: 12.342 min Scan# 3972
Delta R.T. -0.156 min
Lab File: VN066441.D
Acq: 31 Mar 2021 14:11

Tgt Ion: 75 Resp: 128163

Ion	Ratio	Lower	Upper
75	100		
77	1.4	0.0	0.0#


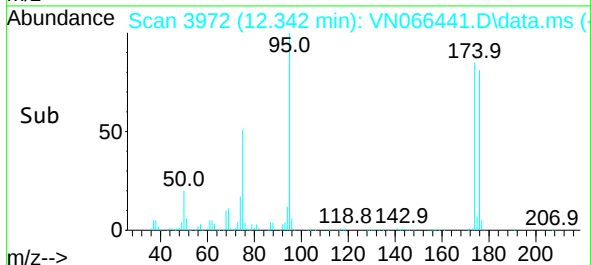

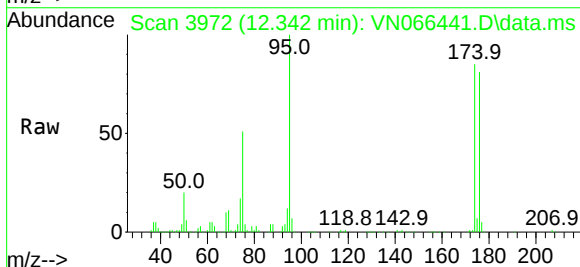




#81
trans-1,4-Dichloro-2-butene
Concen: 80.74 ug/l
RT: 12.342 min Scan# 3972
Delta R.T. 0.099 min
Lab File: VN066441.D
Acq: 31 Mar 2021 14:11




Instrument :
MSVOA_N
ClientSampleId :
PHC-BEAPT-001


Tgt Ion: 75 Resp: 128163
Ion Ratio Lower Upper
75 100
53 0.0 76.1 114.1#
89 0.0 35.7 53.5#

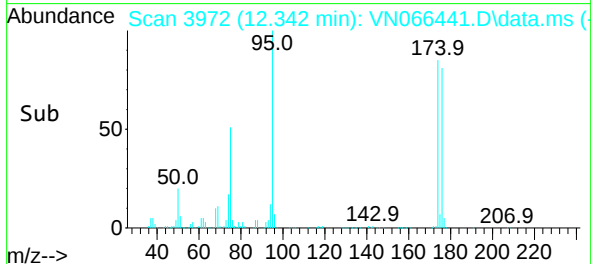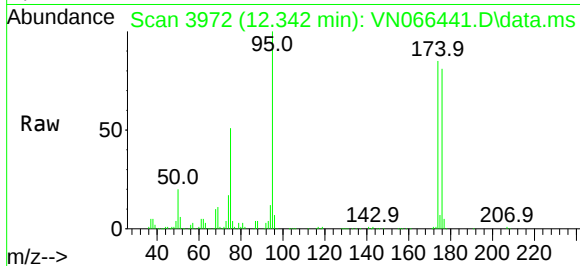

#84
1,2,4-Trimethylbenzene
Concen: 0.42 ug/l
RT: 12.986 min Scan# 4212
Delta R.T. 0.003 min
Lab File: VN066441.D
Acq: 31 Mar 2021 14:11

Tgt Ion:105 Resp: 5369
Ion Ratio Lower Upper
105 100
120 45.2 23.1 69.2

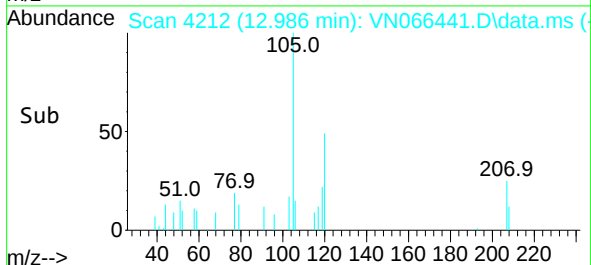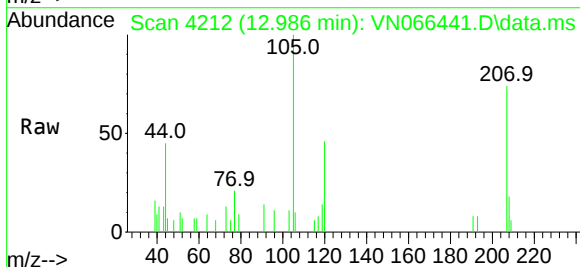

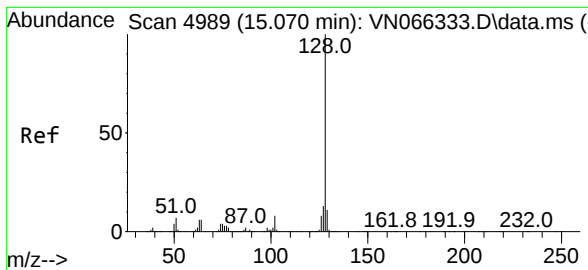

#95
Naphthalene
Concen: 1.75 ug/l
RT: 15.081 min Scan# 4993
Delta R.T. 0.011 min
Lab File: VN066441.D
Acq: 31 Mar 2021 14:11

Instrument :
MSVOA_N
ClientSampleId :
PHC-BEAPT-001

Tgt Ion:	128	Resp:	8815
Ion	Ratio	Lower	Upper
128	100		
127	13.6	10.5	15.7
129	10.2	8.5	12.7

