

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN033122\
 Data File : VN071709.D
 Acq On : 31 Mar 2022 17:13
 Operator : JC\MD
 Sample : N2075-01DL 4X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 RE104D2-20220321DL

Quant Time: Apr 01 01:38:12 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 31 01:57:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.086	168	595819	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	996613	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.745	117	986746	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.674	152	340087	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.433	65	338362	49.745	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	99.480%
35) Dibromofluoromethane	8.022	113	285473	48.678	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	97.360%
50) Toluene-d8	10.439	98	1249742	52.094	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	104.180%
62) 4-Bromofluorobenzene	12.727	95	395033	50.914	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	101.820%


Target Compounds				Qvalue		
3) Chloromethane	2.304	50	2153	0.359	ug/l #	87
6) Chloroethane	2.981	64	1060	0.224	ug/l #	42
10) Methyl Iodide	4.434	142	2018	0.279	ug/l #	89
13) Acrolein	4.045	56	735	0.546	ug/l #	63
15) Acrylonitrile	5.569	53	1137	0.354	ug/l #	80
16) Acetone	4.298	43	3482	1.198	ug/l #	78
17) Carbon Disulfide	4.539	76	2329	0.206	ug/l #	75
18) Methyl Acetate	4.869	43	4031	Below Cal		92
25) 2-Butanone	7.345	43	1341	0.320	ug/l	94
27) cis-1,2-Dichloroethene	7.333	96	29699	4.486	ug/l	89
29) Tetrahydrofuran	7.680	42	762	0.281	ug/l #	35
30) Chloroform	7.810	83	2623	0.244	ug/l #	83
31) Cyclohexane	8.080	56	10286	1.112	ug/l #	3
36) 1,1-Dichloropropene	8.080	75	41686	5.090	ug/l #	48
38) Carbon Tetrachloride	8.080	117	54492	6.789	ug/l #	18
42) 1,2-Dichloroethane	8.533	62	2651	0.296	ug/l #	74
43) Isopropyl Acetate	8.639	43	17383	1.166	ug/l #	53
44) Trichloroethene	9.216	130	235119	35.277	ug/l	96
49) 1,4-Dioxane	9.574	88	178	Below Cal	#	22
51) 4-Methyl-2-Pentanone	10.333	43	3014	0.352	ug/l #	81
59) 2-Hexanone	11.086	43	5790	0.959	ug/l	97
74) N-amyl acetate	12.386	43	2839	0.346	ug/l	93
76) 1,2,3-Trichloropropane	12.727	75	193037	24.502	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.727	75	193037	75.931	ug/l #	10
87) 1,3-Dichlorobenzene	13.609	146	2461	0.215	ug/l	91
88) 1,4-Dichlorobenzene	13.609	146	2461	0.220	ug/l	89
89) n-Butylbenzene	13.945	91	4617	0.290	ug/l	95
91) 1,2-Dichlorobenzene	13.980	146	3029	0.270	ug/l	88
92) 1,2-Dibromo-3-Chloropr...	14.604	75	557	0.376	ug/l	77
93) 1,2,4-Trichlorobenzene	15.262	180	3215	2.655	ug/l	92
95) Naphthalene	15.503	128	10545	4.432	ug/l	98
96) 1,2,3-Trichlorobenzene	15.692	180	3877	3.118	ug/l	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN033122\
Data File : VN071709.D
Acq On : 31 Mar 2022 17:13
Operator : JC\MD
Sample : N2075-01DL 4X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
RE104D2-20220321DL

Quant Time: Apr 01 01:38:12 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
Quant Title : SW846 8260
QLast Update : Thu Mar 31 01:57:54 2022
Response via : Initial Calibration




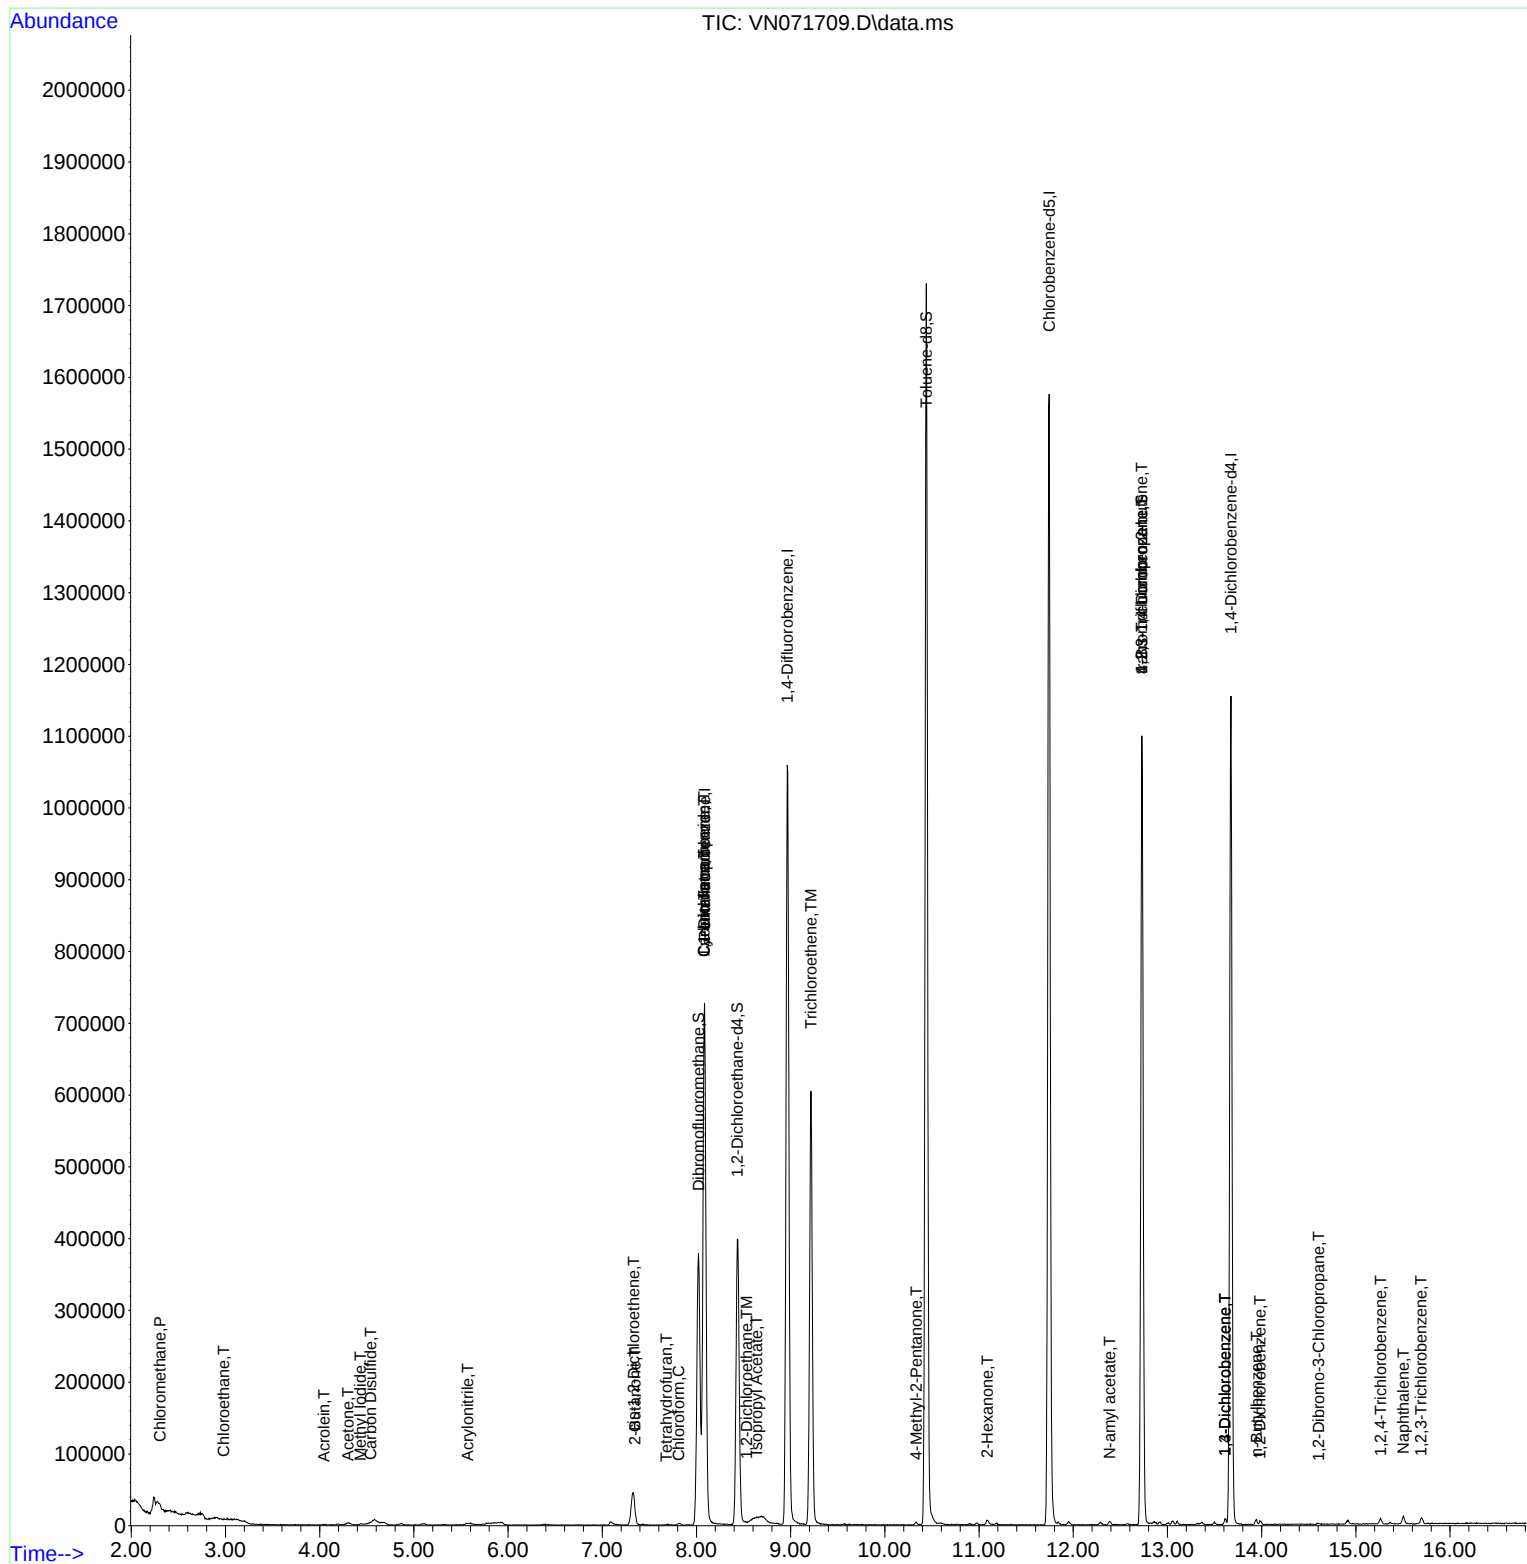




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.086 min Scan# 10
Delta R.T. 0.005 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13




Instrument :
MSVOA_N
ClientSampleId :
RE104D2-20220321DL


Tgt Ion:168 Resp: 595819
Ion Ratio Lower Upper
168 100
99 52.9 42.3 63.5

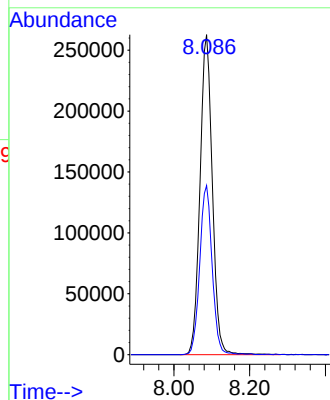

#3
Chloromethane
Concen: 0.359 ug/l
RT: 2.304 min Scan# 54
Delta R.T. 0.005 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13

Tgt Ion: 50 Resp: 2153
Ion Ratio Lower Upper
50 100
52 25.1 25.7 38.5#


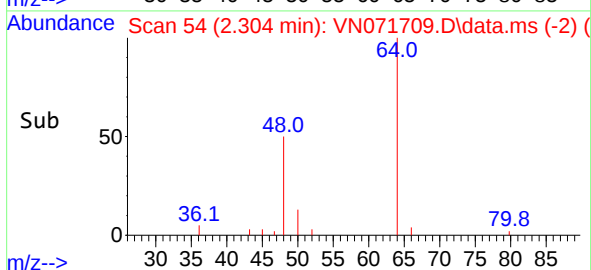
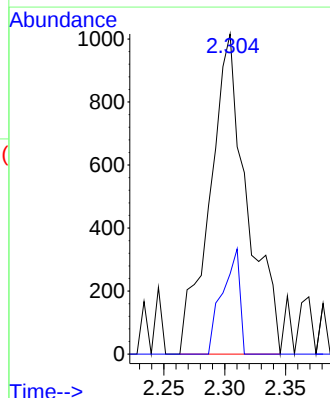



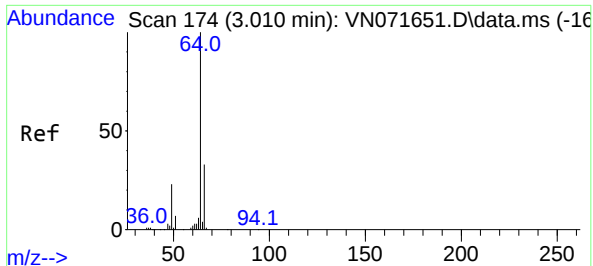

#6
Chloroethane
Concen: 0.224 ug/l
RT: 2.981 min Scan# 11
Delta R.T. -0.029 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13




Instrument :
MSVOA_N
ClientSampleId :
RE104D2-20220321DL


Tgt Ion: 64 Resp: 1060
Ion Ratio Lower Upper
64 100
66 0.0 26.2 39.4#

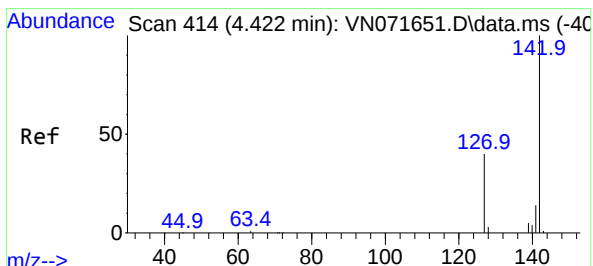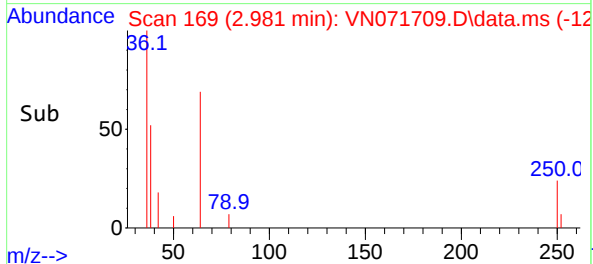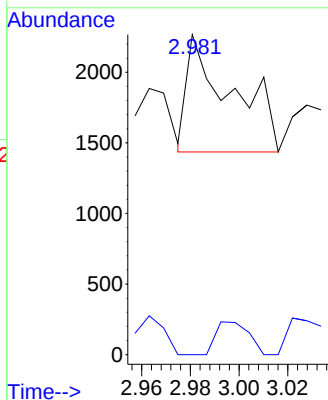

#10
Methyl Iodide
Concen: 0.279 ug/l
RT: 4.434 min Scan# 416
Delta R.T. 0.012 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13

Tgt Ion: 142 Resp: 2018
Ion Ratio Lower Upper
142 100
127 36.2 31.3 46.9
141 2.8 11.2 16.8#


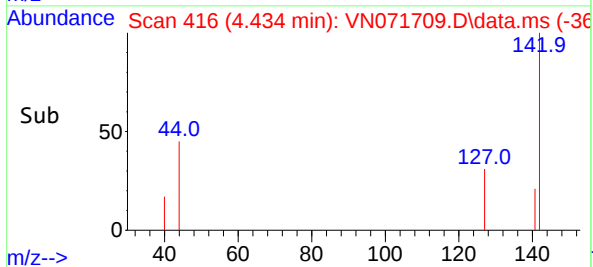
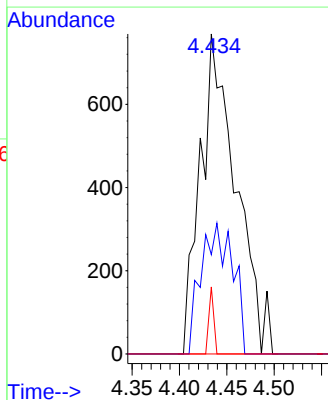
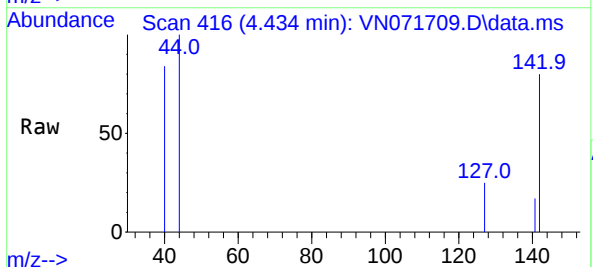




#13
Acrolein
Concen: 0.546 ug/l
RT: 4.045 min Scan# 31
Delta R.T. 0.005 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13




Instrument :
MSVOA_N
ClientSampleId :
RE104D2-20220321DL


Tgt Ion: 56 Resp: 735
Ion Ratio Lower Upper
56 100
55 98.2 54.8 82.2#



#15
Acrylonitrile
Concen: 0.354 ug/l
RT: 5.569 min Scan# 609
Delta R.T. 0.023 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13

Tgt Ion: 53 Resp: 1137
Ion Ratio Lower Upper
53 100
52 64.9 66.4 99.6#
51 24.1 28.5 42.7#


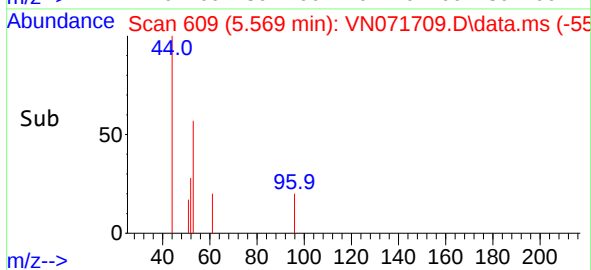






#16
Acetone
Concen: 1.198 ug/l
RT: 4.298 min Scan# 393
Delta R.T. 0.023 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13




Instrument :
MSVOA_N
ClientSampleId :
RE104D2-20220321DL


Tgt Ion: 43 Resp: 3482
Ion Ratio Lower Upper
43 100
58 20.1 26.0 39.0#

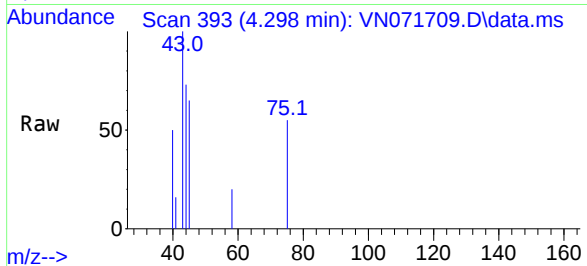

#17
Carbon Disulfide
Concen: 0.206 ug/l
RT: 4.539 min Scan# 434
Delta R.T. 0.005 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13

Tgt Ion: 76 Resp: 2329
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#


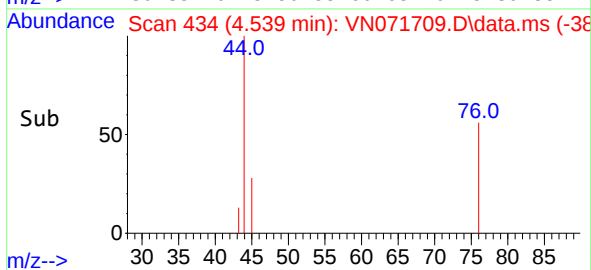

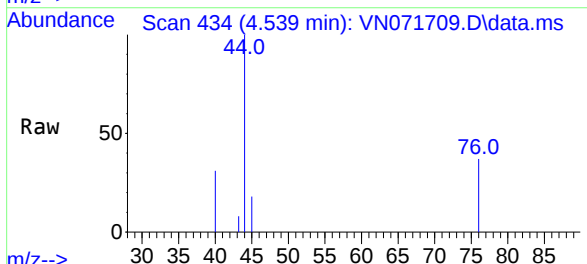




#18
Methyl Acetate
Concen: Below Cal
RT: 4.869 min Scan# 491
Delta R.T. 0.023 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13




Instrument :
MSVOA_N
ClientSampleId :
RE104D2-20220321DL


Tgt Ion: 43 Resp: 4031
Ion Ratio Lower Upper
43 100
74 22.8 21.6 32.4



#25
2-Butanone
Concen: 0.320 ug/l
RT: 7.345 min Scan# 911
Delta R.T. 0.017 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13

Tgt Ion: 43 Resp: 1341
Ion Ratio Lower Upper
43 100
72 32.9 23.7 35.5









#27
cis-1,2-Dichloroethene
Concen: 4.486 ug/l
RT: 7.333 min Scan# 907
Delta R.T. 0.011 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13




Instrument :
MSVOA_N
ClientSampleId :
RE104D2-20220321DL


Tgt Ion: 96 Resp: 29699
Ion Ratio Lower Upper
96 100
61 122.2 0.0 280.6
98 62.4 0.0 128.4

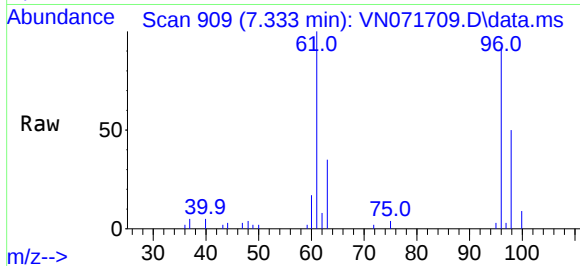

#29
Tetrahydrofuran
Concen: 0.281 ug/l
RT: 7.680 min Scan# 968
Delta R.T. 0.005 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13

Tgt Ion: 42 Resp: 762
Ion Ratio Lower Upper
42 100
72 7.7 39.7 59.5#
71 0.0 36.6 55.0#

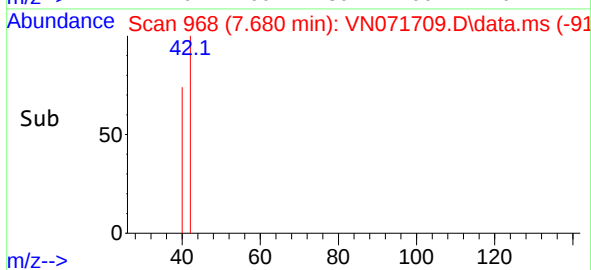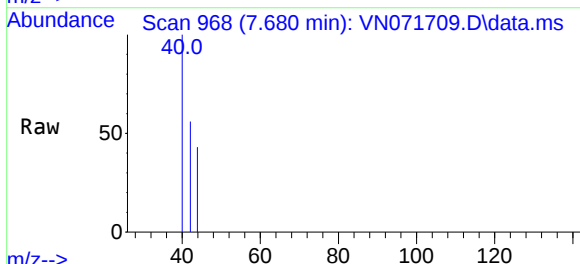



#30

Chloroform

Concen: 0.244 ug/l

RT: 7.810 min Scan# 990

Delta R.T. -0.000 min

Lab File: VN071709.D

Acq: 31 Mar 2022 17:13

Instrument :

MSVOA_N

ClientSampleId :





RE104D2-20220321DL

Tgt Ion: 83 Resp: 2623

Ion Ratio Lower Upper

83 100

85 51.2 51.8 77.8#

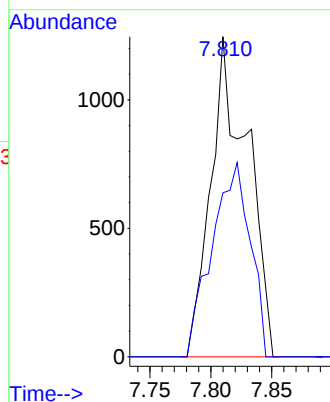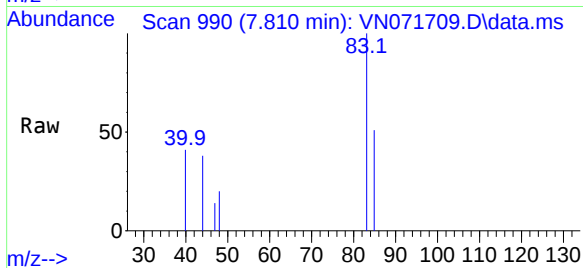

#31

Cyclohexane

Concen: 1.112 ug/l

RT: 8.080 min Scan# 1036

Delta R.T. -0.012 min

Lab File: VN071709.D

Acq: 31 Mar 2022 17:13




Tgt Ion: 56 Resp: 10286


Ion Ratio Lower Upper

56 100

69 185.1 27.8 41.8#

84 133.9 76.9 115.3#


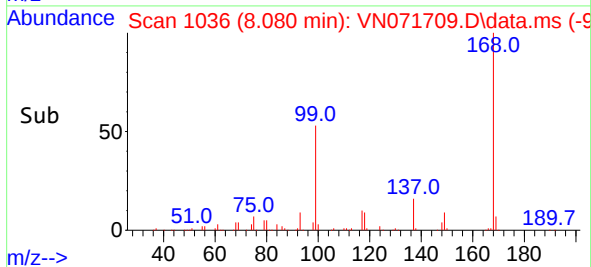
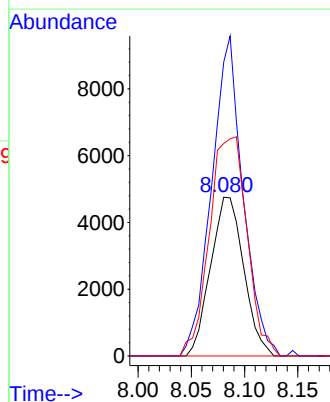
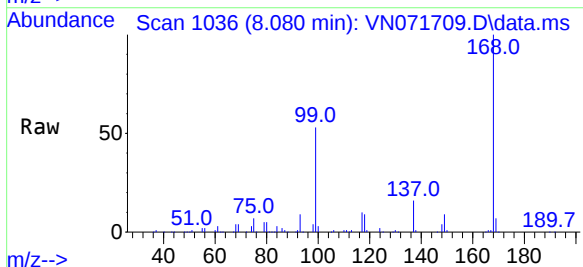


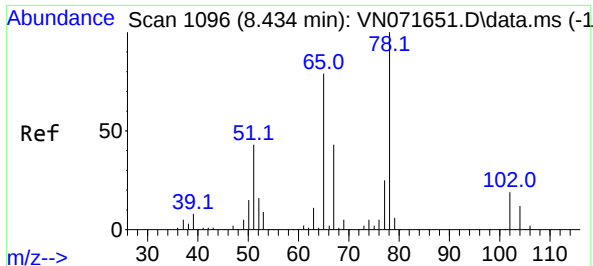

#33
1,2-Dichloroethane-d4
Concen: 49.745 ug/l
RT: 8.433 min Scan# 1096
Delta R.T. -0.001 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13




Instrument :
MSVOA_N
ClientSampleId :
RE104D2-20220321DL


Tgt Ion: 65 Resp: 338362
Ion Ratio Lower Upper
65 100
67 52.8 0.0 104.8

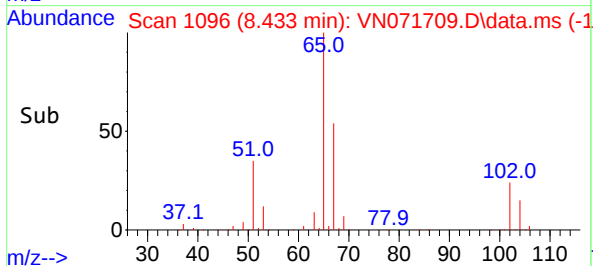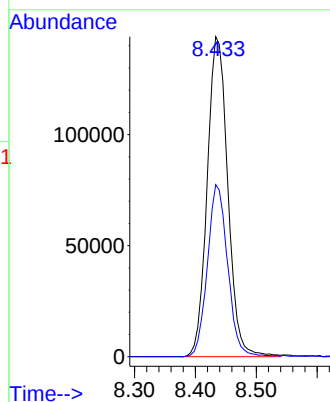

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.963 min Scan# 1186
Delta R.T. -0.000 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13


Tgt Ion:114 Resp: 996613
Ion Ratio Lower Upper
114 100
63 19.1 0.0 40.0
88 15.6 0.0 32.6

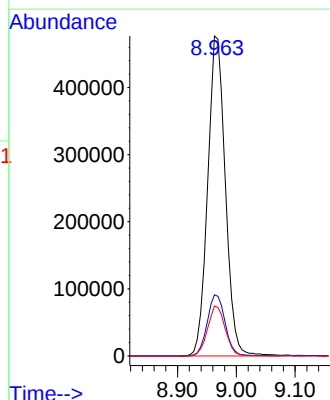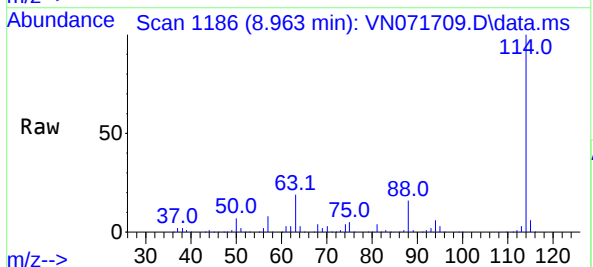



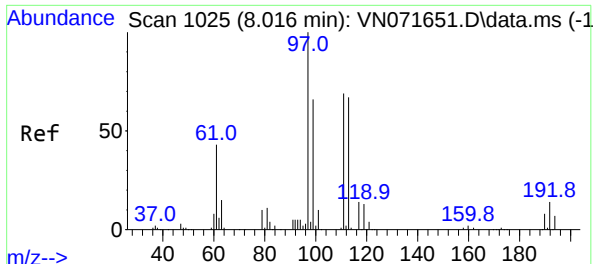


#35
Dibromofluoromethane
Concen: 48.678 ug/l
RT: 8.022 min Scan# 1026
Delta R.T. 0.006 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13

Instrument :
MSVOA_N
ClientSampleId :
RE104D2-20220321DL







Tgt Ion:113 Resp: 285473
Ion Ratio Lower Upper
113 100
111 101.3 81.4 122.0
192 21.4 17.0 25.6

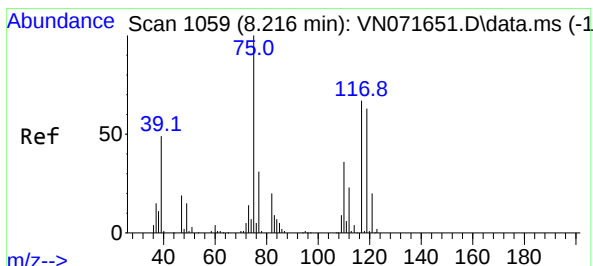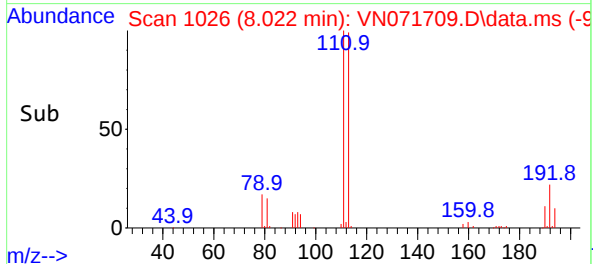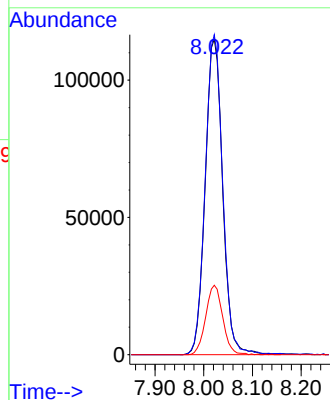

#36
1,1-Dichloropropene
Concen: 5.090 ug/l
RT: 8.080 min Scan# 1036
Delta R.T. -0.136 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13

Tgt Ion: 75 Resp: 41686
Ion Ratio Lower Upper
75 100
110 8.4 18.3 54.8#
77 0.0 25.1 37.7#


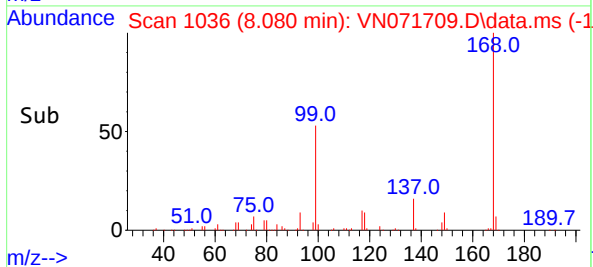
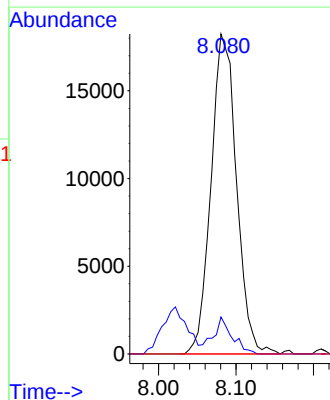
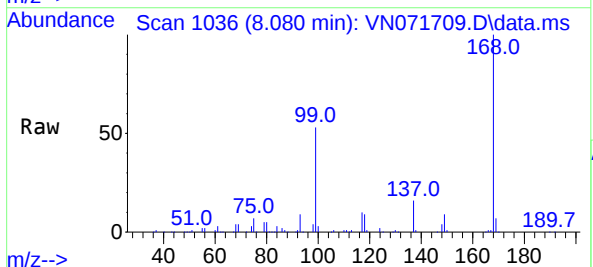


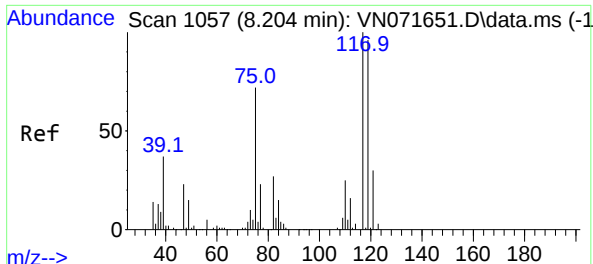

#38
Carbon Tetrachloride
Concen: 6.789 ug/l
RT: 8.080 min Scan# 110
Delta R.T. -0.124 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13




Instrument :
MSVOA_N
ClientSampleId :
RE104D2-20220321DL


Tgt Ion:117 Resp: 54492
Ion Ratio Lower Upper
117 100
119 6.8 75.8 113.8#
121 0.0 24.6 37.0#

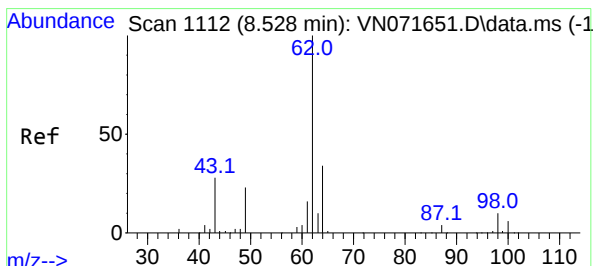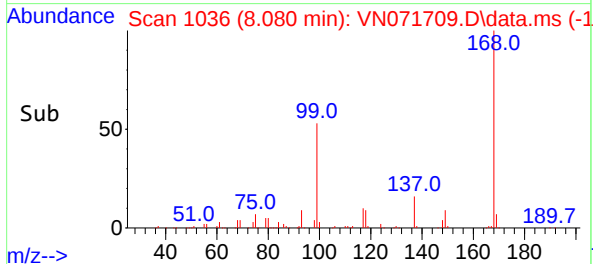

#42
1,2-Dichloroethane
Concen: 0.296 ug/l
RT: 8.533 min Scan# 1113
Delta R.T. 0.005 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13

Tgt Ion: 62 Resp: 2651
Ion Ratio Lower Upper
62 100
98 0.0 0.0 19.4


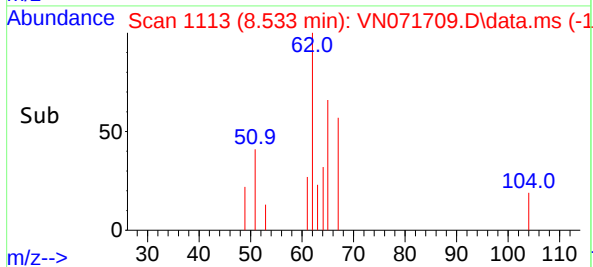

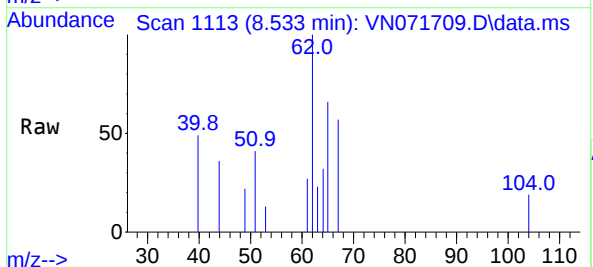


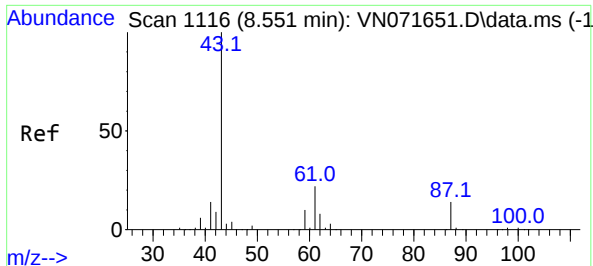

#43
Isopropyl Acetate
Concen: 1.166 ug/l
RT: 8.639 min Scan# 1116
Delta R.T. 0.088 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13




Instrument :
MSVOA_N
ClientSampleId :
RE104D2-20220321DL


Tgt Ion: 43 Resp: 17383
Ion Ratio Lower Upper
43 100
61 0.0 21.9 32.9#
87 0.0 12.0 18.0#

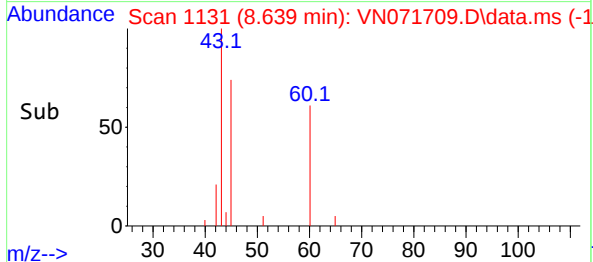

#44
Trichloroethene
Concen: 35.277 ug/l
RT: 9.216 min Scan# 1229
Delta R.T. 0.006 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13

Tgt Ion:130 Resp: 235119
Ion Ratio Lower Upper
130 100
95 89.8 0.0 186.8


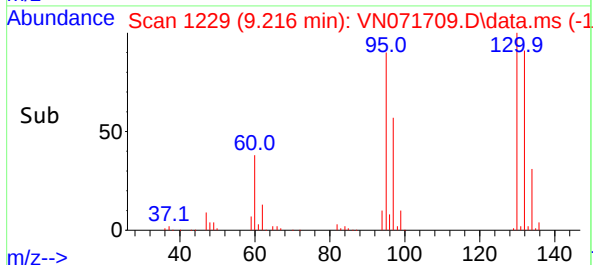
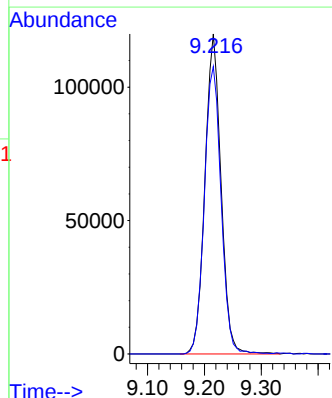
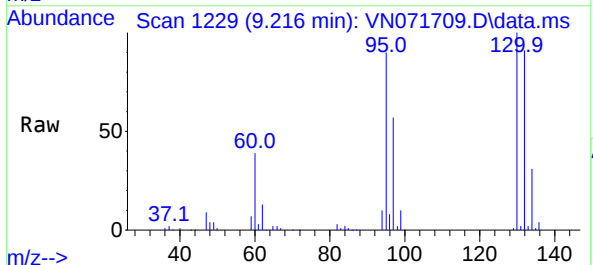


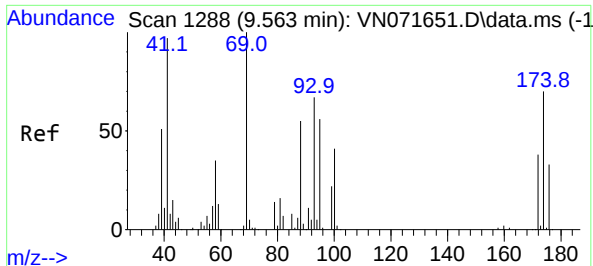

#49
1,4-Dioxane
Concen: Below Cal
RT: 9.574 min Scan# 11
Delta R.T. 0.011 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13




Instrument :
MSVOA_N
ClientSampleId :
RE104D2-20220321DL


Tgt Ion: 88 Resp: 178
Ion Ratio Lower Upper
88 100
43 128.7 20.2 30.4#
58 43.3 54.2 81.4#

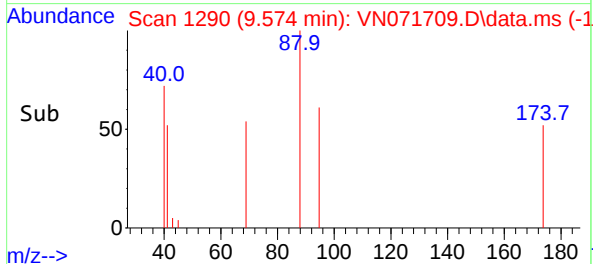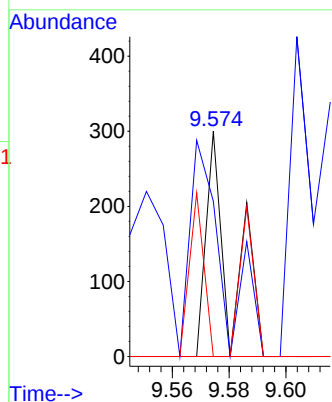

#50
Toluene-d8
Concen: 52.094 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. 0.000 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13

Tgt Ion: 98 Resp: 1249742
Ion Ratio Lower Upper
98 100
100 64.5 52.6 78.8

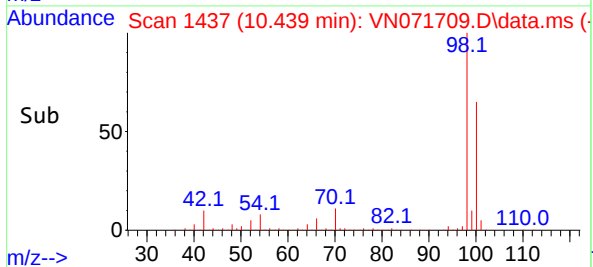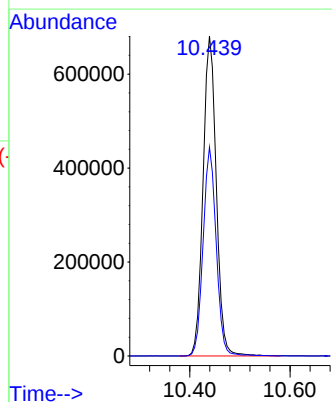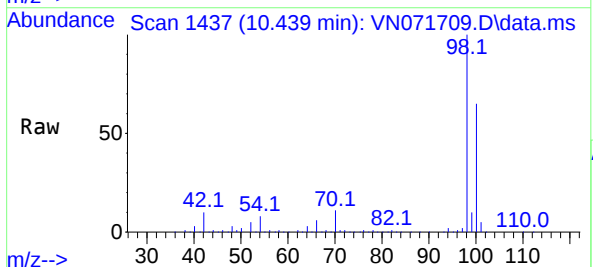



#51

4-Methyl-2-Pentanone

Concen: 0.352 ug/l

RT: 10.333 min Scan# 1419

Delta R.T. 0.011 min

Lab File: VN071709.D

Acq: 31 Mar 2022 17:13

Instrument :

MSVOA_N

ClientSampleId :





RE104D2-20220321DL

Tgt Ion: 43 Resp: 3014

Ion Ratio Lower Upper

43 100

58 30.4 34.1 51.1#

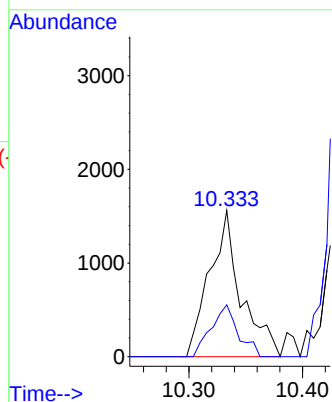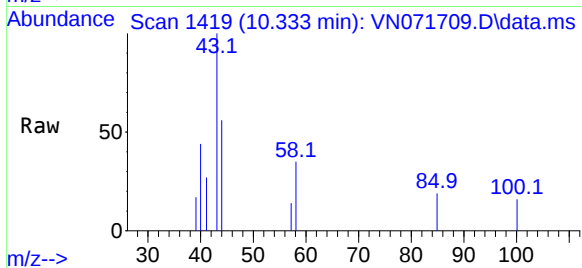

#59

2-Hexanone

Concen: 0.959 ug/l

RT: 11.086 min Scan# 1547

Delta R.T. 0.005 min

Lab File: VN071709.D




Acq: 31 Mar 2022 17:13


Tgt Ion: 43 Resp: 5790

Ion Ratio Lower Upper

43 100

58 57.3 29.7 89.1


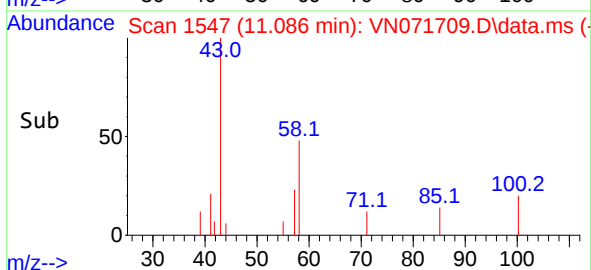

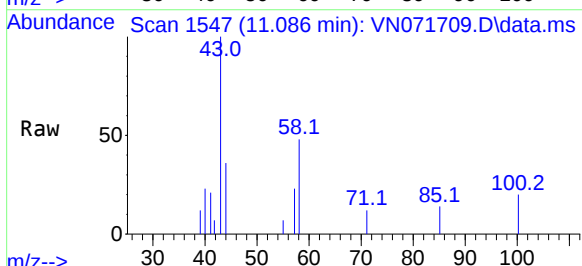


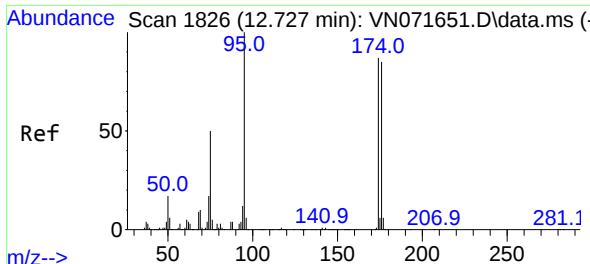

#62
4-Bromofluorobenzene
Concen: 50.914 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13




Instrument :
MSVOA_N
ClientSampleId :
RE104D2-20220321DL


Tgt Ion: 95 Resp: 395033
Ion Ratio Lower Upper
95 100
174 84.7 0.0 167.6
176 81.8 0.0 163.4

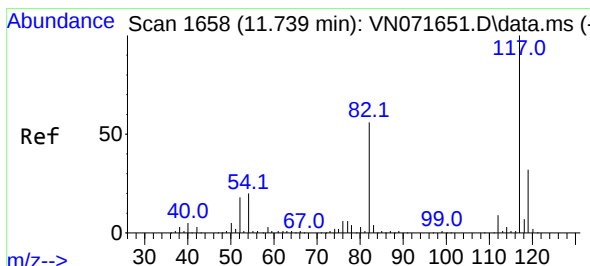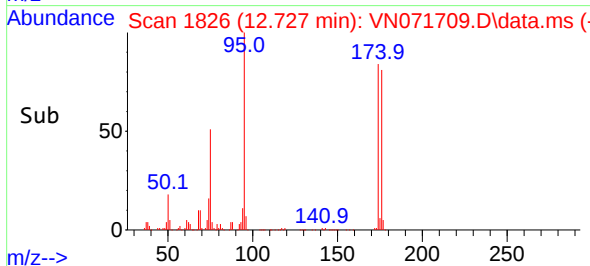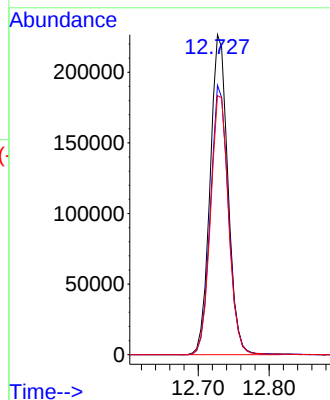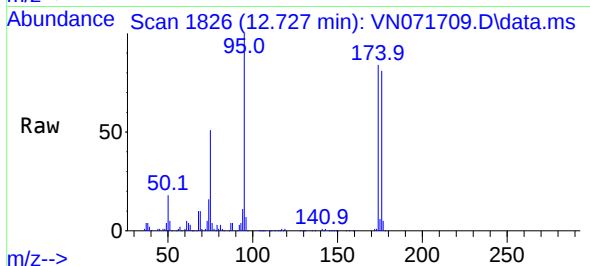

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.745 min Scan# 1659
Delta R.T. 0.006 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13

Tgt Ion: 117 Resp: 986746
Ion Ratio Lower Upper
117 100
82 54.0 44.2 66.2
119 32.3 25.4 38.0


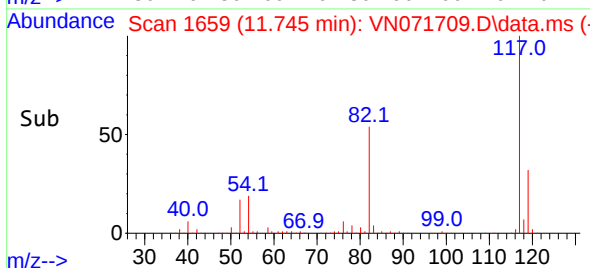
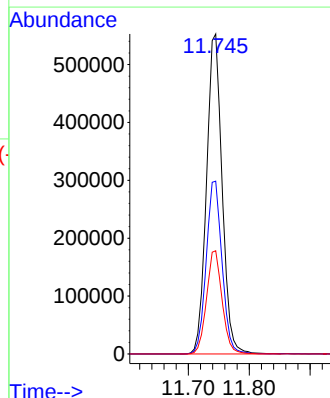
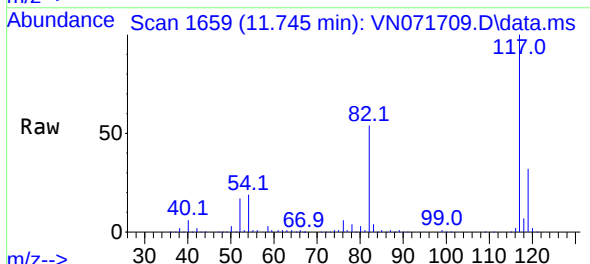




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.674 min Scan# 1986
Delta R.T. 0.005 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13




Instrument :
MSVOA_N
ClientSampleId :
RE104D2-20220321DL


Tgt Ion:152 Resp: 340087
Ion Ratio Lower Upper
152 100
115 56.6 28.9 86.7
150 157.9 0.0 356.2

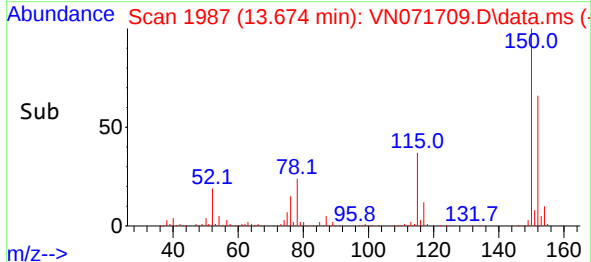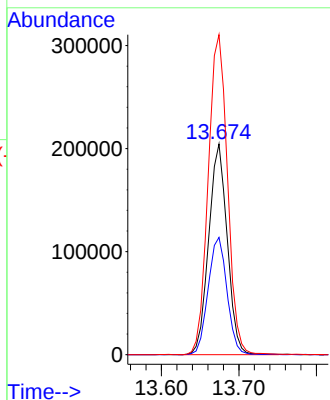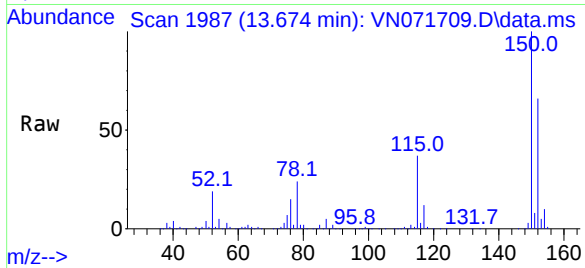

#74
N-ethyl acetate
Concen: 0.346 ug/l
RT: 12.386 min Scan# 1768
Delta R.T. 0.006 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13

Tgt Ion: 43 Resp: 2839
Ion Ratio Lower Upper
43 100
70 40.3 39.0 58.4
55 25.5 21.1 31.7
61 24.6 21.1 31.7


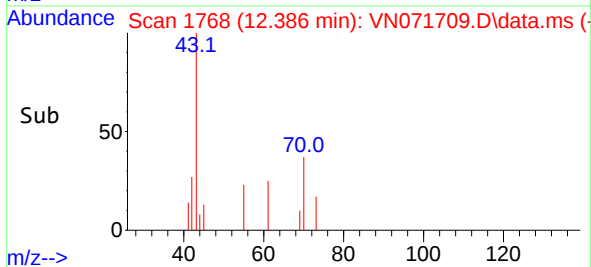
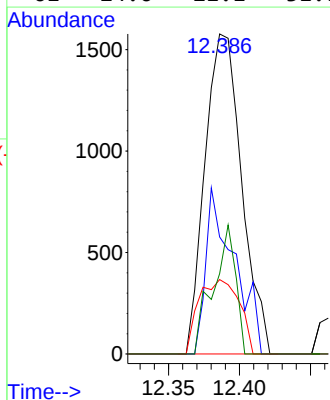
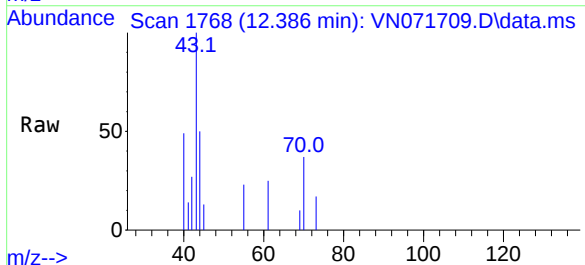




#76
1,2,3-Trichloropropane
Concen: 24.502 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. -0.147 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13




Instrument :
MSVOA_N
ClientSampleId :
RE104D2-20220321DL


Tgt Ion: 75 Resp: 193037
Ion Ratio Lower Upper
75 100
77 1.3 98.5 295.5#

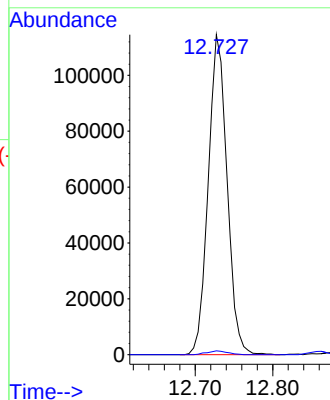

#81
trans-1,4-Dichloro-2-butene
Concen: 75.931 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.105 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13

Tgt Ion: 75 Resp: 193037
Ion Ratio Lower Upper
75 100
53 0.0 78.0 117.0#
89 0.0 37.2 55.8#

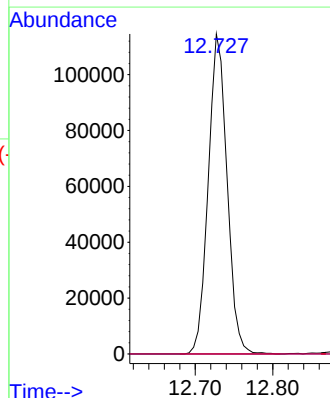



#87

1,3-Dichlorobenzene

Concen: 0.215 ug/l

RT: 13.609 min Scan# 1976

Delta R.T. -0.001 min

Lab File: VN071709.D

Acq: 31 Mar 2022 17:13

Instrument :

MSVOA_N

ClientSampleId :

RE104D2-20220321DL





Tgt Ion:146 Resp: 2461

Ion Ratio Lower Upper

146 100

111 48.1 20.0 60.0

148 69.2 32.0 96.0

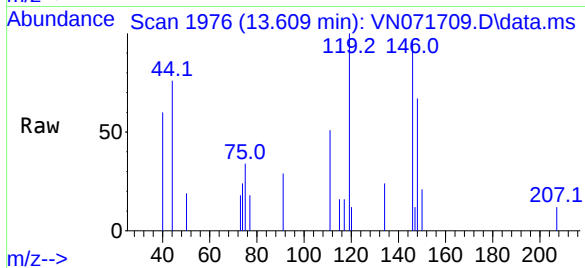

#88

1,4-Dichlorobenzene

Concen: 0.220 ug/l

RT: 13.609 min Scan# 1976

Delta R.T. -0.077 min

Lab File: VN071709.D

Acq: 31 Mar 2022 17:13




Tgt Ion:146 Resp: 2461


Ion Ratio Lower Upper

146 100

111 48.1 19.1 57.1

148 69.2 31.4 94.3




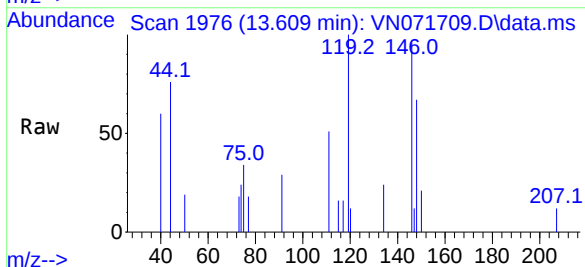


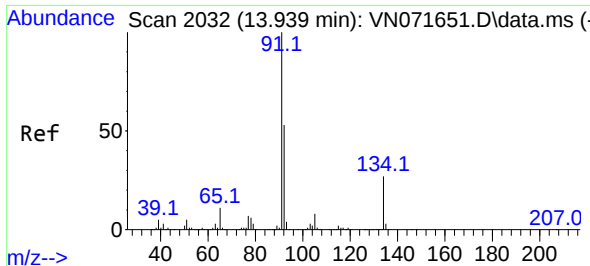

#89
n-Butylbenzene
Concen: 0.290 ug/l
RT: 13.945 min Scan# 2033
Delta R.T. 0.006 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13




Instrument :
MSVOA_N
ClientSampleId :
RE104D2-20220321DL


Tgt Ion: 91	Resp:	4617
Ion Ratio	Lower	Upper
91	100	
92	49.0	26.9 80.7
134	26.9	13.6 40.8

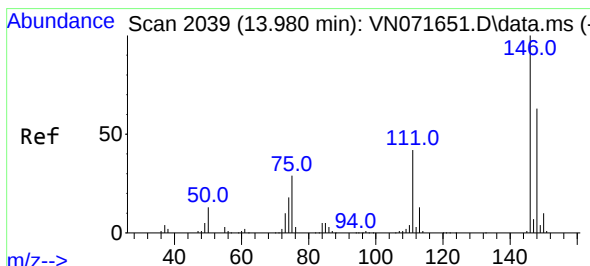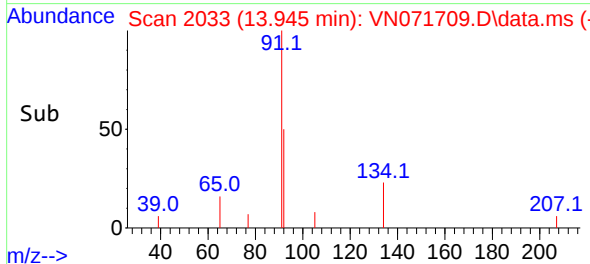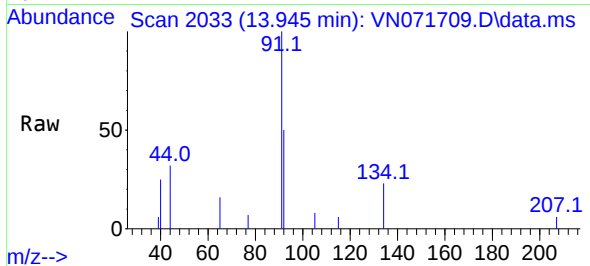

#91
1,2-Dichlorobenzene
Concen: 0.270 ug/l
RT: 13.980 min Scan# 2039
Delta R.T. 0.000 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13

Tgt Ion: 146	Resp:	3029
Ion Ratio	Lower	Upper
146	100	
111	31.5	20.9 62.8
148	56.7	32.1 96.3

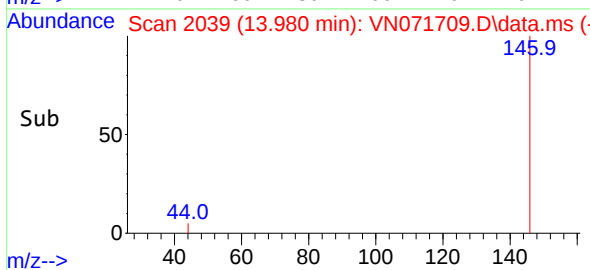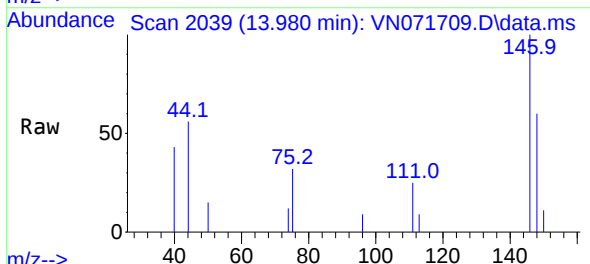



#92

1,2-Dibromo-3-Chloropropane

Concen: 0.376 ug/l

RT: 14.604 min Scan# 2144

Delta R.T. 0.006 min

Lab File: VN071709.D

Acq: 31 Mar 2022 17:13

Instrument :

MSVOA_N

ClientSampleId :

RE104D2-20220321DL





Tgt Ion: 75 Resp: 557

Ion Ratio Lower Upper

75 100

155 84.9 44.9 134.5

157 78.5 59.0 176.8

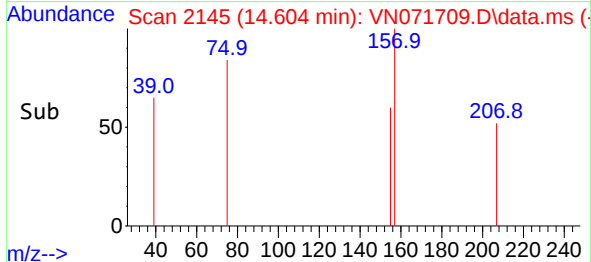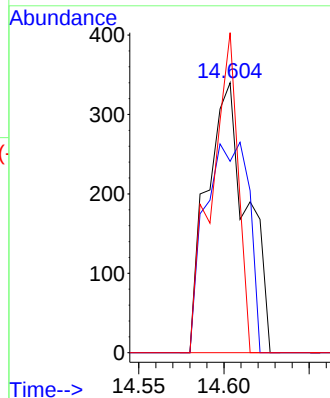

#93

1,2,4-Trichlorobenzene

Concen: 2.655 ug/l

RT: 15.262 min Scan# 2257

Delta R.T. 0.005 min

Lab File: VN071709.D

Acq: 31 Mar 2022 17:13




Tgt Ion:180 Resp: 3215


Ion Ratio Lower Upper

180 100

182 101.6 47.5 142.5

145 34.4 14.5 43.5


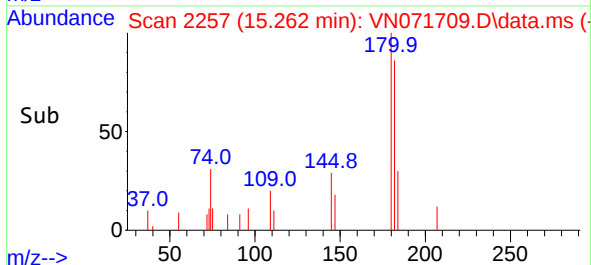
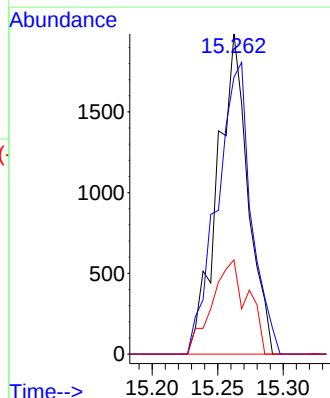
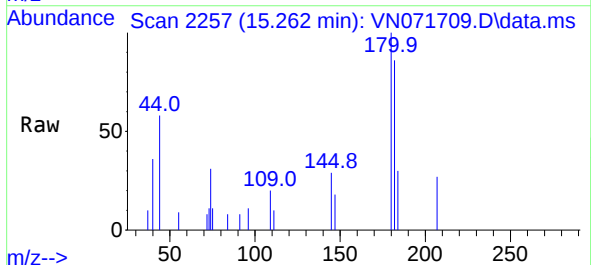


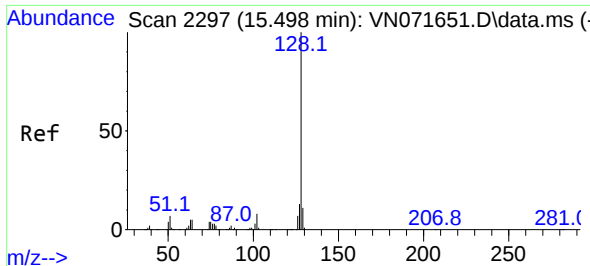

#95
Naphthalene
Concen: 4.432 ug/l
RT: 15.503 min Scan# 21
Delta R.T. 0.005 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13

Instrument :
MSVOA_N
ClientSampleId :
RE104D2-20220321DL

Tgt Ion:	128	Resp:	10545
Ion Ratio	Lower	Upper	
128	100		
127	12.6	10.3	15.5
129	11.8	8.6	13.0

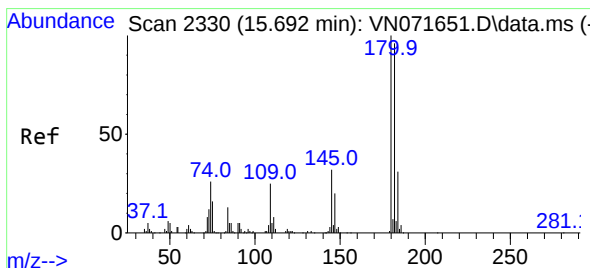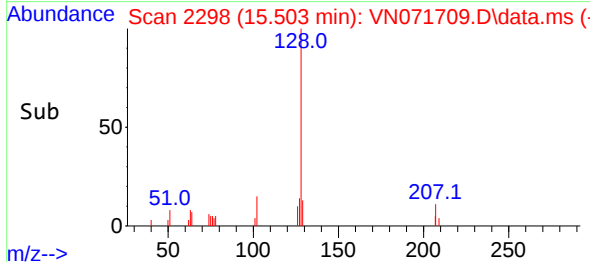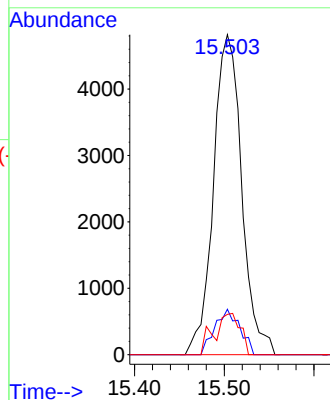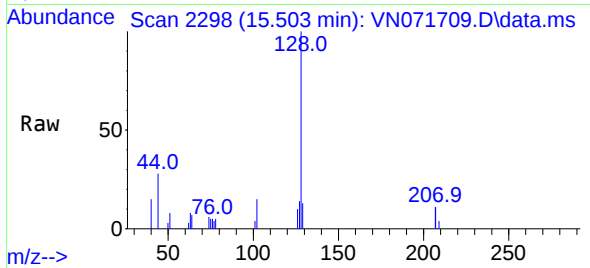

#96
1,2,3-Trichlorobenzene
Concen: 3.118 ug/l
RT: 15.692 min Scan# 2330
Delta R.T. -0.000 min
Lab File: VN071709.D
Acq: 31 Mar 2022 17:13

Tgt Ion:	180	Resp:	3877
Ion Ratio	Lower	Upper	
180	100		
182	98.1	47.8	143.3
145	25.8	15.5	46.5

