
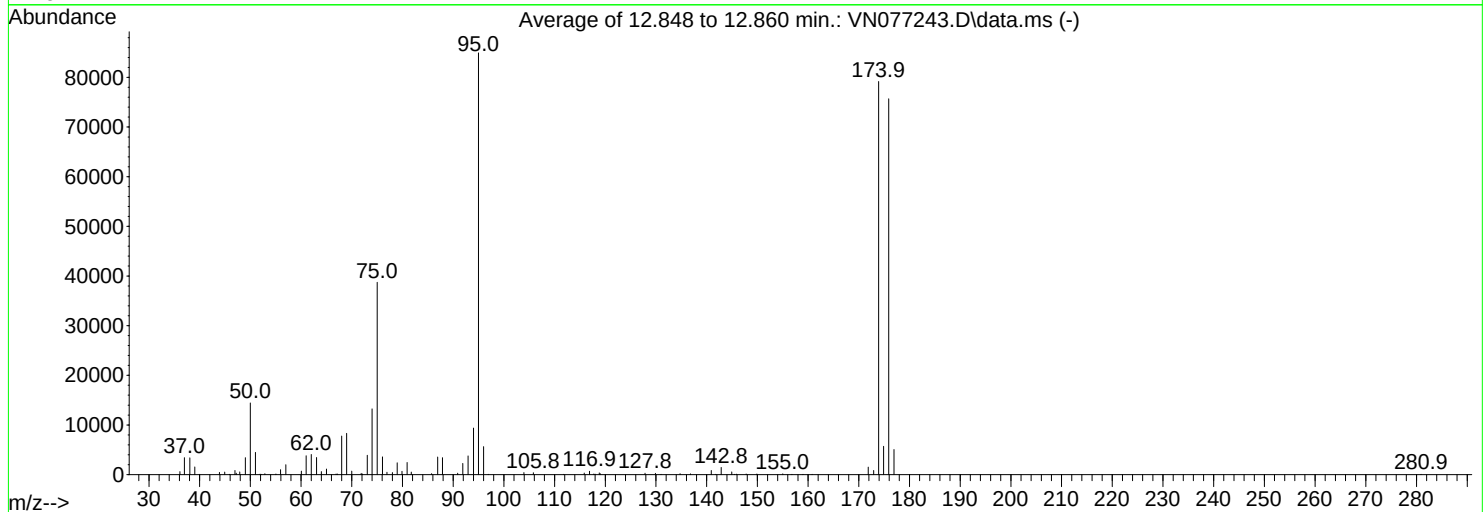


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN033123\
Data File : VN077243.D
Acq On : 31 Mar 2023 08:31
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033123W.M
Title : SW846 8260
Last Update : Sat Apr 01 00:11:10 2023

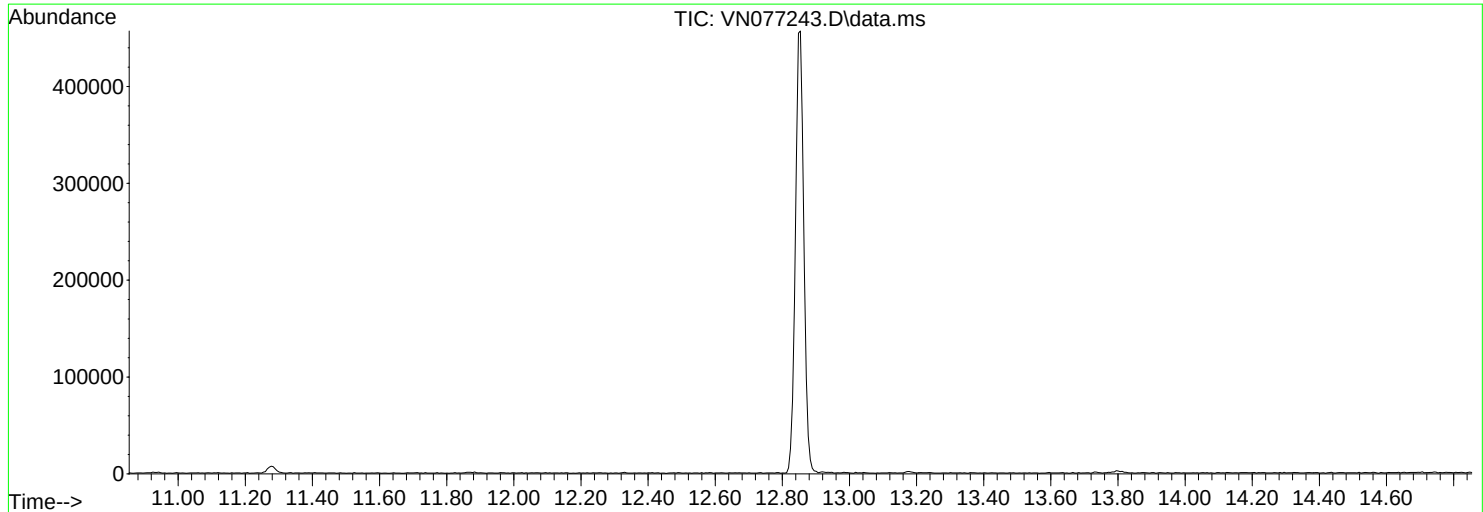

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1846

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.0	14445	PASS
75	95	30	60	45.6	38723	PASS
95	95	100	100	100.0	84939	PASS
96	95	5	9	6.6	5636	PASS
173	174	0.00	2	1.1	836	PASS
174	95	50	100	93.2	79157	PASS
175	174	5	9	7.2	5715	PASS
176	174	95	101	95.6	75699	PASS
177	176	5	9	6.7	5054	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.10	629	49.00	3411	62.00	4071	73.05	388
37.00	3423	50.00	14445	63.05	3464	74.00	1325
38.05	3377	51.00	4471	64.00	628	75.00	3872
39.05	1537	51.90	87	65.00	1123	76.05	357
39.95	57	52.10	57	66.90	131	76.95	476
43.90	467	52.85	200	67.15	130	78.00	430
44.95	515	55.05	140	68.00	7760	78.95	2397
45.90	77	55.95	990	69.00	8315	79.90	670
46.95	832	57.00	2003	70.00	703	80.90	2447
47.20	292	60.05	710	71.85	258	81.75	520
47.90	558	61.00	3795	72.10	135	85.75	183

Average of 12.848 to 12.860 min.: VN077243.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
86.95	3548	111.80	53	136.80	152	159.00	71
87.90	3407	115.85	321	140.90	851	160.80	62
90.90	288	116.90	678	141.80	65	171.85	1518
91.90	2270	117.75	147	142.85	1446	172.95	836
92.95	3769	118.00	102	144.95	554	173.90	79157
94.00	9393	118.80	360	145.50	60	174.90	5715
95.00	84939	119.00	188	145.90	107	175.90	75699
96.00	5636	127.85	282	147.80	145	176.95	5054
96.90	81	129.90	269	149.90	137	280.90	76
103.95	415	131.00	53	155.00	157		
105.80	373	134.75	192	156.80	78		

Instrument :

MSVOA_N

ClientSampleId :

BFB