


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN033125\
Data File : VN086167.D
Acq On : 31 Mar 2025 12:40
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031825W.M
Title : SW846 8260
Last Update : Wed Mar 19 03:20:56 2025

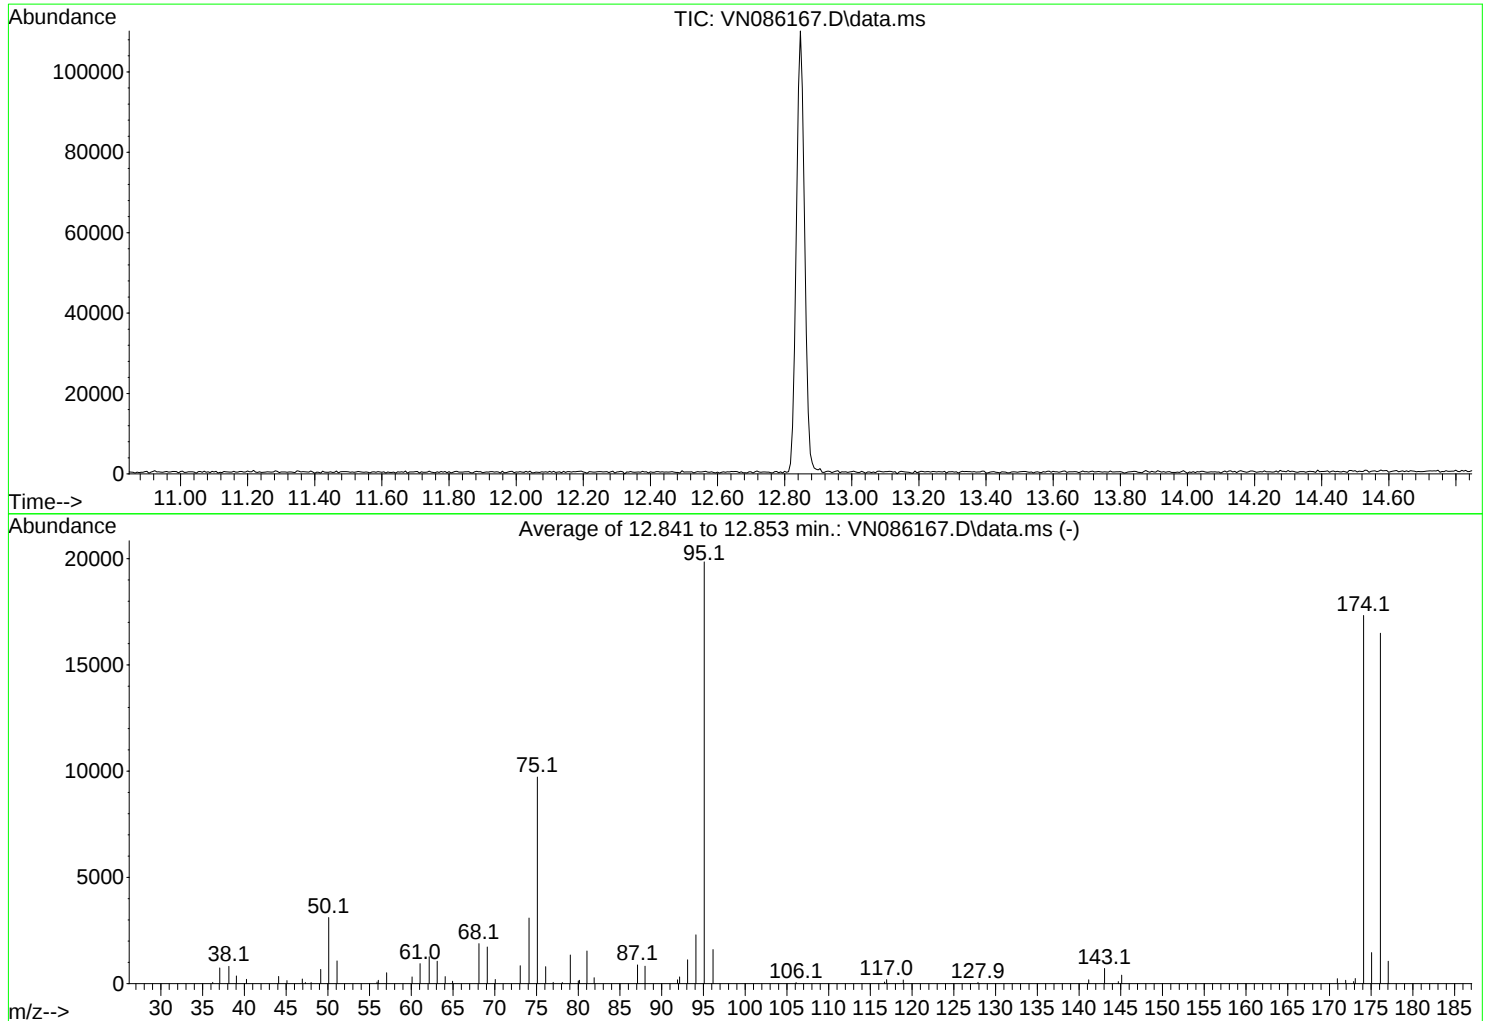

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.7	3110	PASS
75	95	30	60	49.0	9720	PASS
95	95	100	100	100.0	19851	PASS
96	95	5	9	8.1	1605	PASS
173	174	0.00	2	1.4	241	PASS
174	95	50	100	87.3	17328	PASS
175	174	5	9	8.4	1462	PASS
176	174	95	101	95.2	16489	PASS
177	176	5	9	6.4	1052	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.20	61	50.10	3110	68.10	1880	80.15	15
37.05	739	51.10	1069	69.10	1725	81.05	154
38.15	814	55.90	73	70.05	193	81.90	28
39.05	364	56.05	155	73.05	845	87.10	88
40.25	207	57.05	515	74.10	3087	88.00	819
44.10	338	60.10	318	75.10	9720	91.90	178
45.10	140	61.05	940	76.10	795	92.15	318
46.95	218	62.15	1263	77.00	63	93.10	1121
47.30	55	63.10	1053	78.10	52	94.10	2298
48.00	56	64.05	328	79.05	1351	95.10	19851
49.15	671	64.95	114	80.00	130	96.15	1605

Average of 12.841 to 12.853 min.: VN086167.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
106.10	51	172.90	98				
116.70	78	173.10	241				
116.95	190	174.10	17328				
118.95	172	175.05	1462				
127.90	60	176.10	16489				
141.15	182	177.05	1052				
143.05	715						
144.70	100						
145.10	398						
170.95	237						
171.95	159						

Instrument :

MSVOA_N

ClientSampleId :

BFB