

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN040119\
 Data File : VN054872.D
 Acq On : 1 Apr 2019 14:11
 Operator : JC/SP
 Sample : K2178-04
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 COMP-16

Quant Time: Apr 02 04:22:09 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N032919W.M
 Quant Title : SW846 8260
 QLast Update : Sat Mar 30 00:48:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	534688	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	857742	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	717517	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	236875	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.03	65	348909	48.41	ug/l	0.00
Spiked Amount			Recovery	=	96.82%	
35) Dibromofluoromethane	7.59	113	267742	46.82	ug/l	0.00
Spiked Amount			Recovery	=	93.64%	
50) Toluene-d8	10.09	98	1026970	48.31	ug/l	0.00
Spiked Amount			Recovery	=	96.62%	
62) 4-Bromofluorobenzene	12.40	95	305473	43.20	ug/l	0.00
Spiked Amount			Recovery	=	86.40%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
5) Bromomethane	2.58	94	293	Below Cal	#	68
13) Acrolein	3.61	56	153	0.456	ug/l #	63
14) Allyl chloride	4.54	41	510747	49.336	ug/l #	21
16) Acetone	3.82	43	67514	39.280	ug/l #	82
18) Methyl Acetate	4.54	43	56621	11.948	ug/l #	81
20) Methylene Chloride	4.54	84	11214700	1849.733	ug/l #	81
25) 2-Butanone	6.86	43	2502	0.985	ug/l #	46
29) Tetrahydrofuran	7.24	42	517	0.293	ug/l #	52
30) Chloroform	7.37	83	5591	0.537	ug/l #	79
31) Cyclohexane	7.66	56	11751	Below Cal	#	16
36) 1,1-Dichloropropene	7.67	75	40241	5.035	ug/l #	48
38) Carbon Tetrachloride	7.66	117	50491	6.504	ug/l #	16
48) Methyl methacrylate	9.18	41	7471	1.447	ug/l #	21
51) 4-Methyl-2-Pentanone	9.99	43	3166	0.591	ug/l	100
59) 2-Hexanone	10.72	43	17863	5.211	ug/l #	23
68) m/p-Xylenes	11.62	106	2684	0.286	ug/l	100
75) 1,1,2,2-Tetrachloroethane	12.40	83	221	Below Cal	#	1
76) 1,2,3-Trichloropropane	12.40	75	160712	39.055	ug/l #	100
80) 1,3,5-Trimethylbenzene	12.73	105	4404	0.277	ug/l	97
81) trans-1,4-Dichloro-2-buten	12.40	75	160712	151.912	ug/l #	11
83) tert-Butylbenzene	12.99	119	223	Below Cal	#	42
84) 1,2,4-Trimethylbenzene	13.04	105	7348	0.485	ug/l	95
94) Hexachlorobutadiene	15.00	225	121	Below Cal	#	19
95) Naphthalene	15.13	128	6621	0.776	ug/l #	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN040119\
Data File : VN054872.D
Acq On : 1 Apr 2019 14:11
Operator : JC/SP
Sample : K2178-04
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
COMP-16

Quant Time: Apr 02 04:22:09 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N032919W.M
Quant Title : SW846 8260
QLast Update : Sat Mar 30 00:48:18 2019
Response via : Initial Calibration

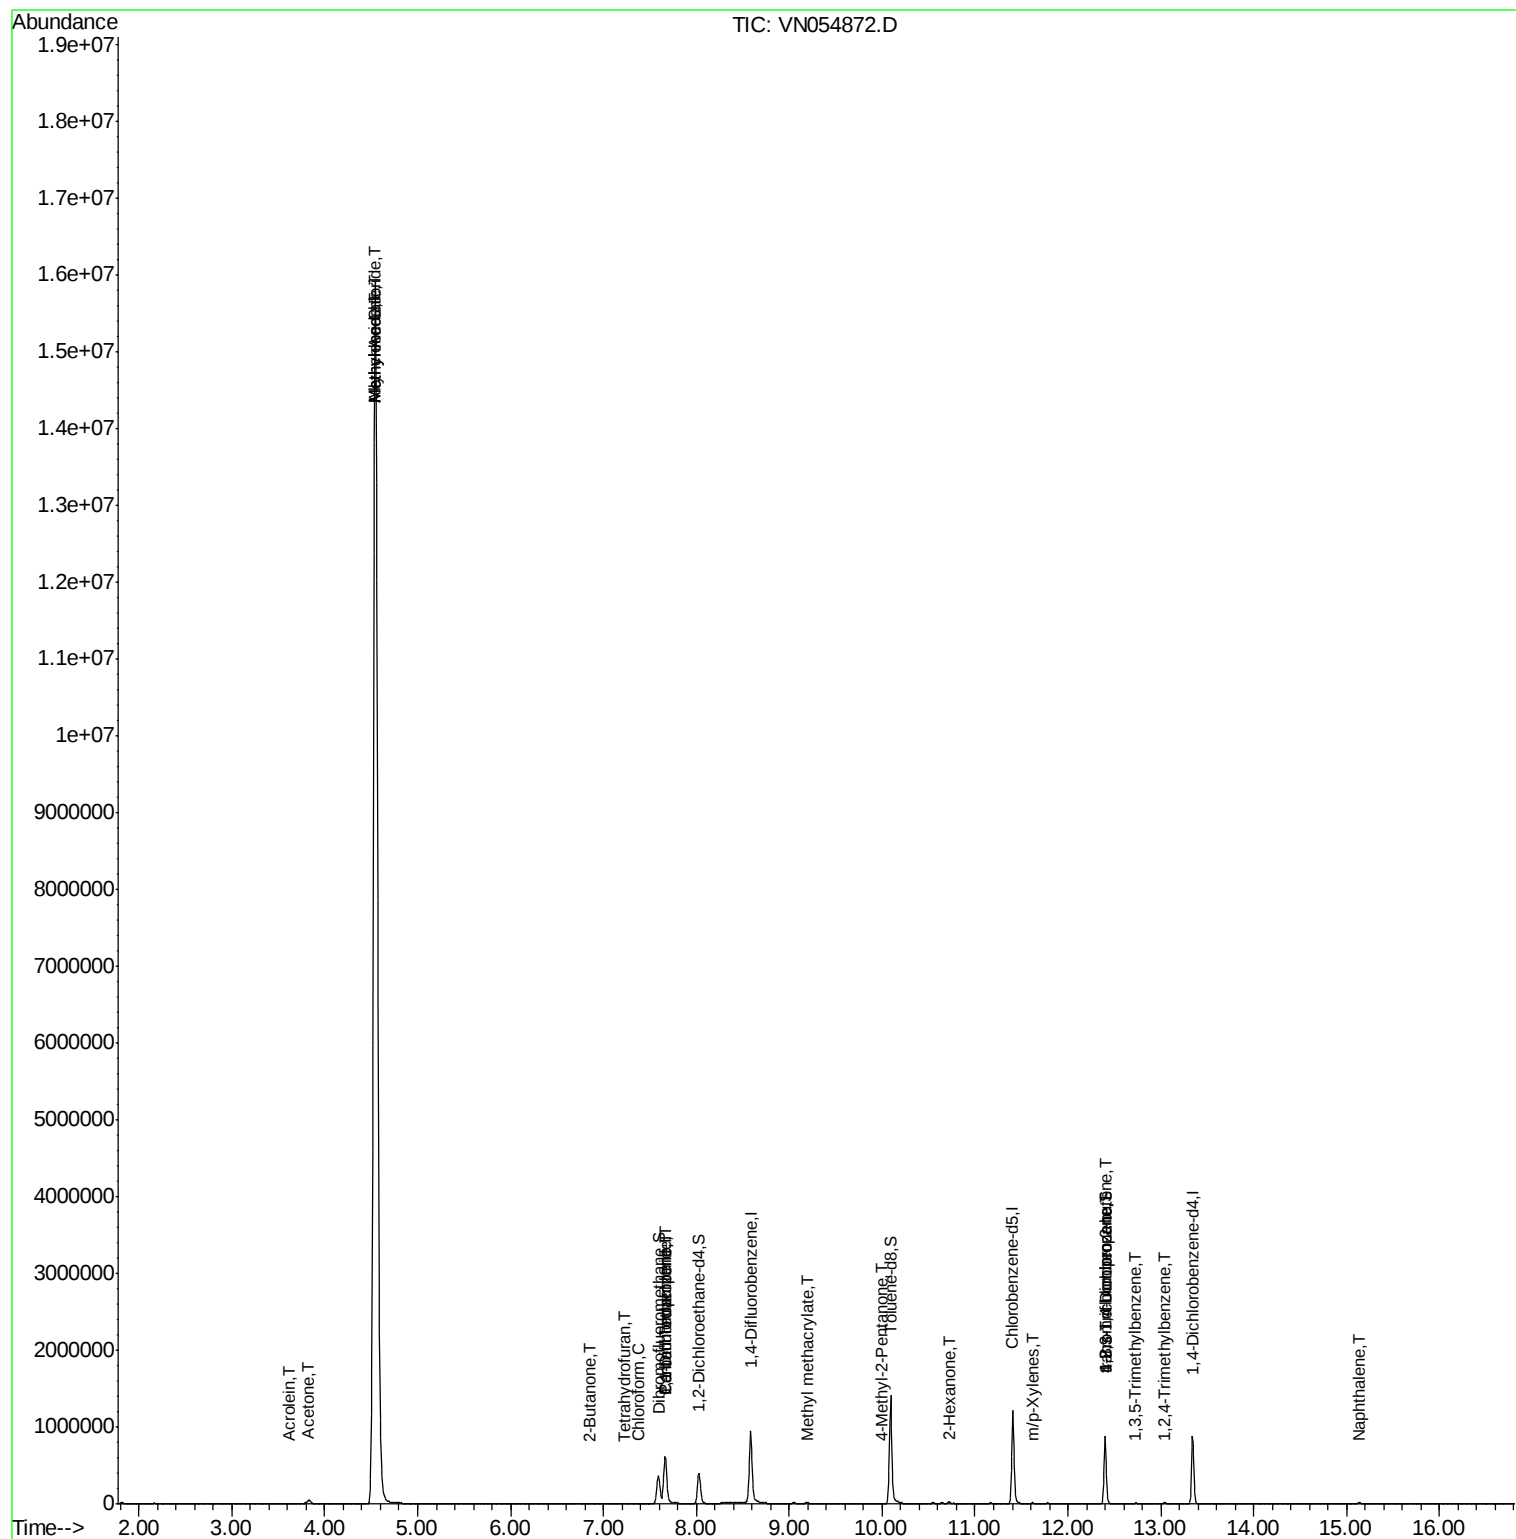

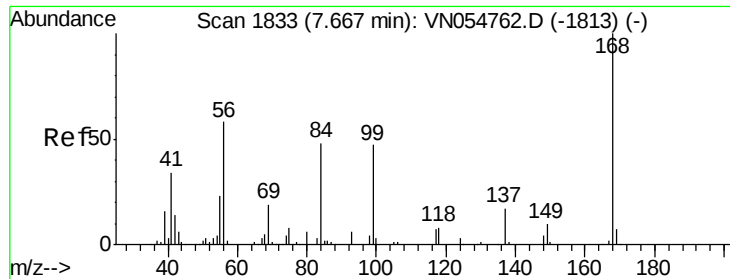

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. -0.00 min

Lab File: VN054872.D

Acq: 1 Apr 2019 14:11

Instrument :

MSVOA_N

ClientSampleId :


COMP-16

Tot Ion:168 Resp: 534688

Ion Ratio Lower Upper

168 100

99 56.3 37.1 55.7#



Abundance Ion 167.90 (167.60 to 168.60): VN054872.D (-1740) (-)

Ion 98.90 (98.60 to 99.60): VN054872.D (-1740) (-)

7.67

200000



150000

100000

50000

0

Time-->



#5

Bromomethane

Concen: Below Cal

RT: 2.58 min Scan# 250

Delta R.T. 0.00 min

Lab File: VN054872.D


Acq: 1 Apr 2019 14:11

Tgt Ion: 94 Resp: 293

Ion Ratio Lower Upper

94 100

96 65.1 77.0 115.4#



Abundance Ion 93.90 (93.60 to 94.60): VN054872.D (-156) (-)

Ion 95.90 (95.60 to 96.60): VN054872.D (-156) (-)

2.58

250

200


150


100

50

0

Time-->



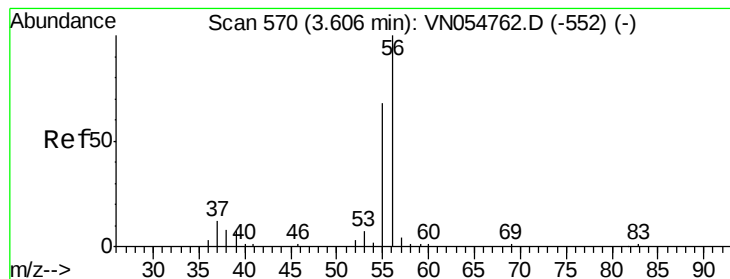

#13

Acrolein

Concen: 0.456 ug/l

RT: 3.61 min Scan# 570

Delta R.T. -0.00 min

Lab File: VN054872.D

Acq: 1 Apr 2019 14:11

Instrument :

MSVOA_N

ClientSampleId :





COMP-16

Tot Ion: 56 Resp: 153

Ion Ratio Lower Upper

56 100

55 101.3 56.7 85.1#

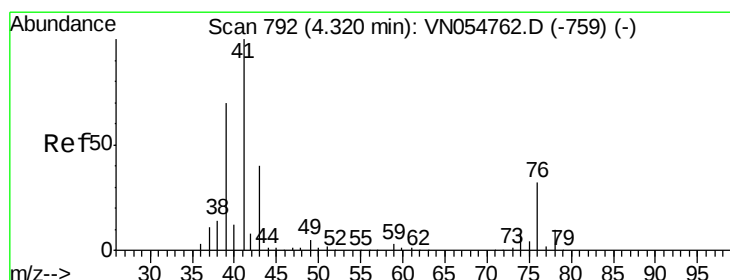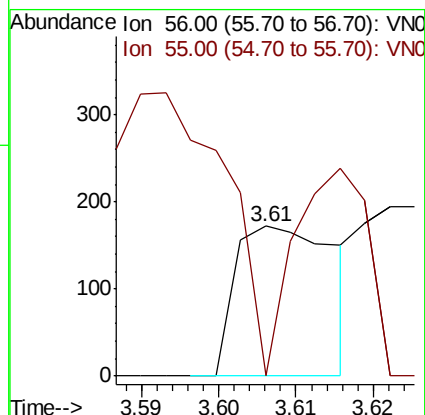

#14

Allyl chloride

Concen: 49.336 ug/l

RT: 4.54 min Scan# 862

Delta R.T. 0.22 min

Lab File: VN054872.D

Acq: 1 Apr 2019 14:11




Tgt Ion: 41 Resp: 510747


Ion Ratio Lower Upper

41 100

39 0.1 58.2 87.4#

76 0.0 31.7 47.5#

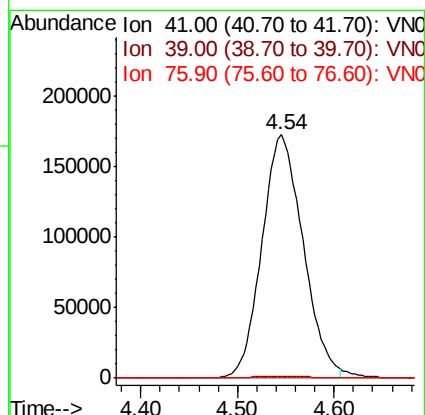

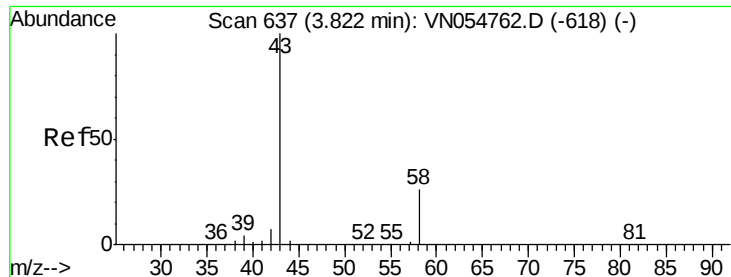

#16

Acetone

Concen: 39.280 ug/l

RT: 3.82 min Scan# 638

Delta R.T. 0.00 min

Lab File: VN054872.D

Acq: 1 Apr 2019 14:11

Instrument :

MSVOA_N

ClientSampleId :





COMP-16

Tot Ion: 43 Resp: 67514

Ion Ratio Lower Upper

43 100

58 26.7 29.9 44.9#

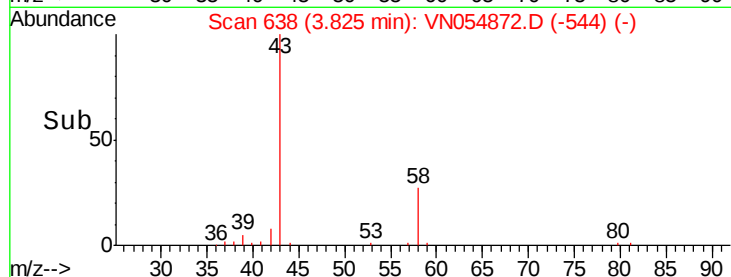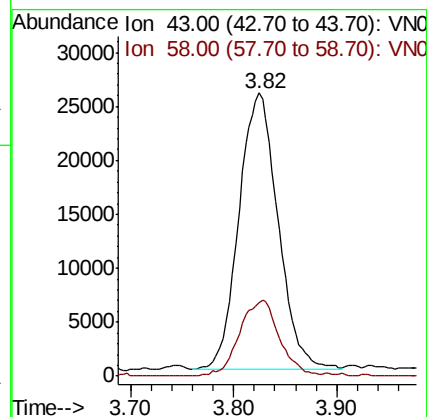

#18

Methyl Acetate

Concen: 11.948 ug/l

RT: 4.54 min Scan# 862

Delta R.T. 0.21 min

Lab File: VN054872.D




Acq: 1 Apr 2019 14:11


Tgt Ion: 43 Resp: 56621

Ion Ratio Lower Upper

43 100

74 16.3 20.8 31.2#

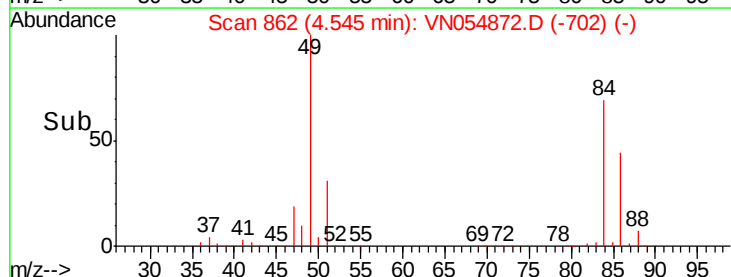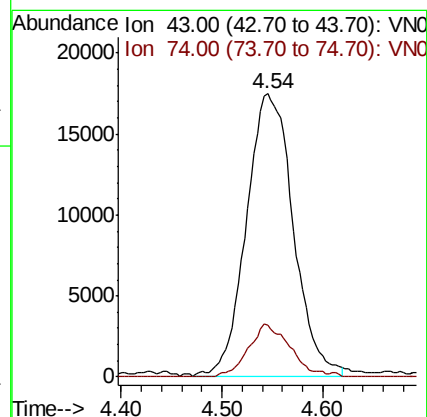



#20

Methylene Chloride

Concen: 1849.733 ug/l

RT: 4.54 min Scan# 862

Delta R.T. -0.00 min

Lab File: VN054872.D

Acq: 1 Apr 2019 14:11

Instrument :

MSVOA_N

ClientSampleId :

COMP-16

Tot Ion: 84 Resp:11214700



Ion Ratio Lower Upper

84 100

49 145.1 89.7 134.5#

51 44.3 28.2 42.4#

86 64.0 50.8 76.2





Abundance Ion 83.90 (83.60 to 84.60): VNO

Ion 48.90 (48.60 to 49.60): VNO

Ion 50.90 (50.60 to 51.60): VNO

Ion 85.90 (85.60 to 86.60): VNO

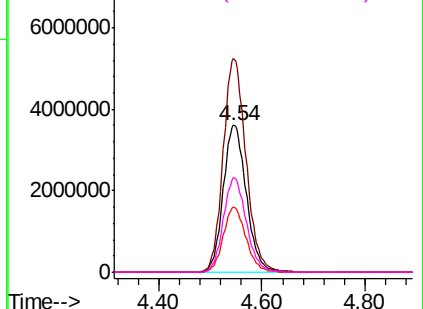

#25

2-Butanone

Concen: 0.985 ug/l

RT: 6.86 min Scan# 1581

Delta R.T. 0.01 min

Lab File: VN054872.D



Acq: 1 Apr 2019 14:11

Tgt Ion: 43 Resp: 2502

Ion Ratio Lower Upper


43 100


72 0.0 23.0 34.6#



Abundance Ion 43.00 (42.70 to 43.70): VNO

Ion 72.00 (71.70 to 72.70): VNO

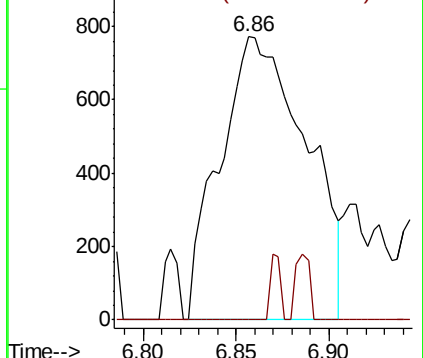



#29

Tetrahydrofuran

Concen: 0.293 ug/l

RT: 7.24 min Scan# 1700

Delta R.T. 0.02 min

Lab File: VN054872.D

Acq: 1 Apr 2019 14:11

Instrument :

MSVOA_N

ClientSampled :

COMP-16


Tot Ion: 42 Resp: 517

Ion Ratio Lower Upper

42 100

72 15.9 37.8 56.6#

71 13.0 36.2 54.2#



Abundance Ion 42.00 (41.70 to 42.70): VN0

Ion 72.00 (71.70 to 72.70): VN0

Ion 71.00 (70.70 to 71.70): VN0

600

500

400

300



200

100

0

7.18 7.20 7.22 7.24 7.26

Time-->



#30

Chloroform

Concen: 0.537 ug/l

RT: 7.37 min Scan# 1740

Delta R.T. -0.01 min

Lab File: VN054872.D


Acq: 1 Apr 2019 14:11

Tgt Ion: 83 Resp: 5591

Ion Ratio Lower Upper

83 100

85 48.3 52.2 78.4#



Abundance Ion 82.90 (82.60 to 83.60): VN0

Ion 84.90 (84.60 to 85.60): VN0

2500

2000

1500


1000


500

0

7.30 7.35 7.40 7.45

Time-->




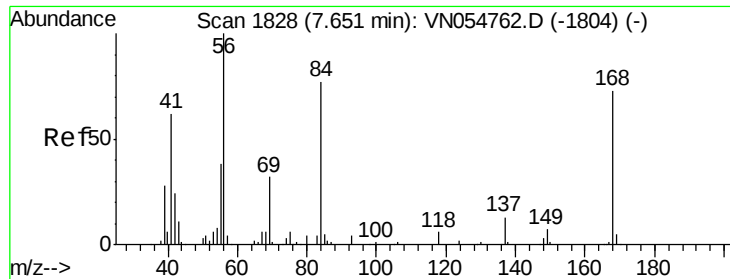




#31
Cyclohexane
Concen: Below Cal
RT: 7.66 min Scan# 1832
Delta R.T. 0.01 min
Lab File: VN054872.D
Acq: 1 Apr 2019 14:11

Instrument :
MSVOA_N
ClientSampled :
COMP-16

Tot Ion: 56 Resp: 11751
Ion Ratio Lower Upper
56 100
69 172.3 27.8 41.6#
84 118.5 74.6 111.8#




Abundance Ion 56.00 (55.70 to 56.70): VNC
Ion 69.00 (68.70 to 69.70): VNC
Ion 84.00 (83.70 to 84.70): VNC

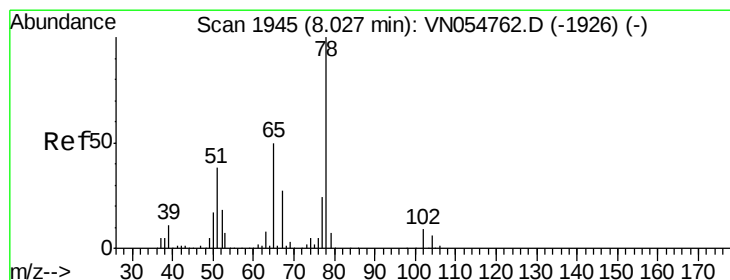
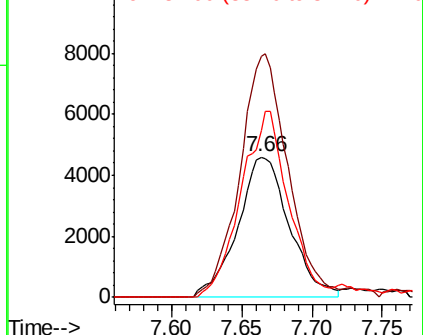



#33
1,2-Dichloroethane-d4
Concen: 48.408 ug/l
RT: 8.03 min Scan# 1945
Delta R.T. -0.00 min
Lab File: VN054872.D
Acq: 1 Apr 2019 14:11

Tgt Ion: 65 Resp: 348909
Ion Ratio Lower Upper
65 100
67 51.9 0.0 104.6

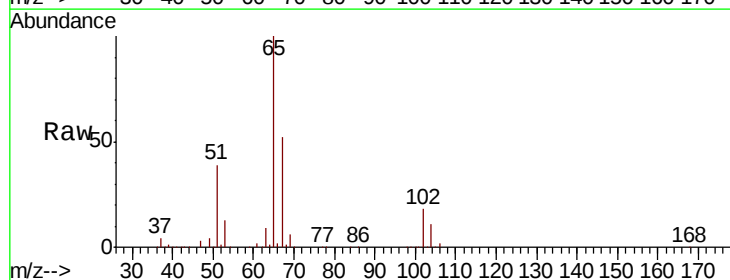

Abundance Ion 64.90 (64.60 to 65.60): VNC
Ion 66.90 (66.60 to 67.60): VNC

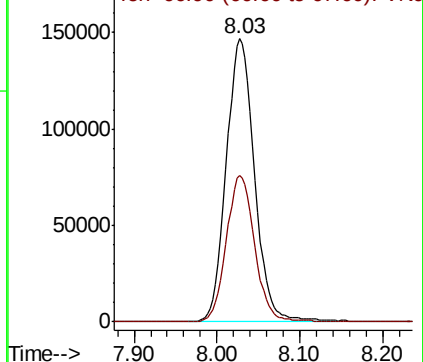

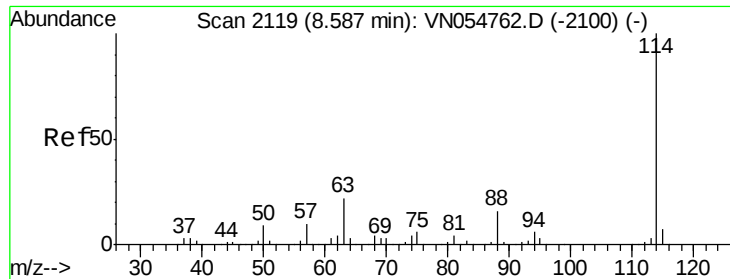

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.59 min Scan# 2119

Delta R.T. -0.00 min

Lab File: VN054872.D

Acq: 1 Apr 2019 14:11

Instrument :

MSVOA_N

ClientSampled :

COMP-16


Tot Ion:114 Resp: 857742

Ion Ratio Lower Upper

114 100

63 21.9 0.0 35.2




88 15.8 0.0 30.2

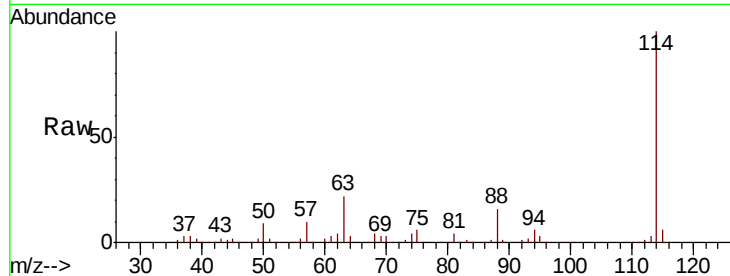

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN

Ion 87.90 (87.60 to 88.60): VN

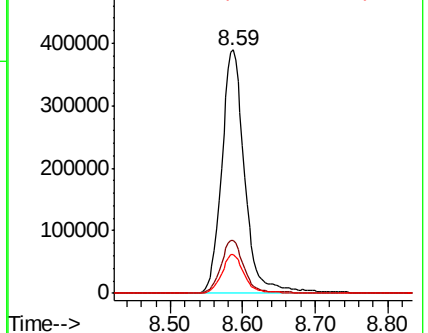

#35

Dibromofluoromethane

Concen: 46.820 ug/l

RT: 7.59 min Scan# 1810

Delta R.T. 0.00 min

Lab File: VN054872.D

Acq: 1 Apr 2019 14:11


Tgt Ion:113 Resp: 267742

Ion Ratio Lower Upper

113 100

111 102.3 82.2 123.4



192 21.4 19.2 28.8




Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V




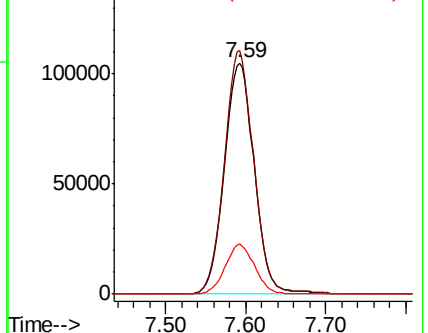


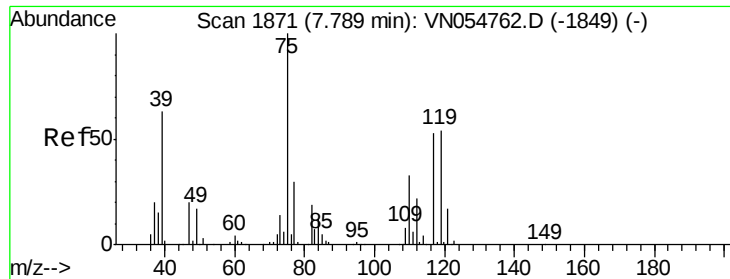

#36
 1,1-Dichloropropene
 Concen: 5.035 ug/l
 RT: 7.67 min Scan# 1833
 Delta R.T. -0.12 min
 Lab File: VN054872.D
 Acq: 1 Apr 2019 14:11




Instrument :
 MSVOA_N
 ClientSampleId :
 COMP-16


Tot Ion: 75 Resp: 40241
 Ion Ratio Lower Upper
 75 100
 110 9.3 19.1 57.5#
 77 0.0 25.0 37.4#

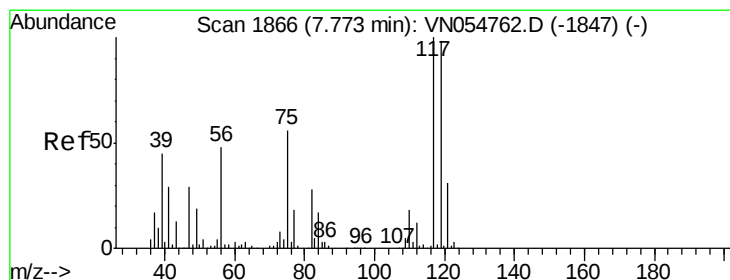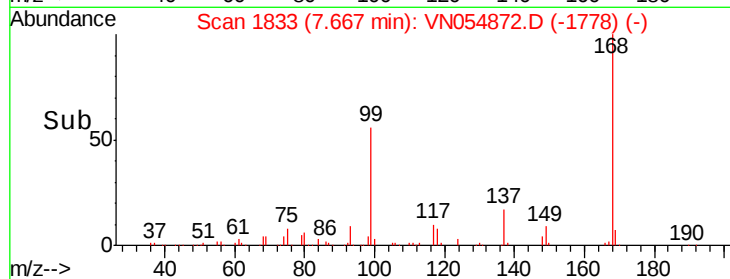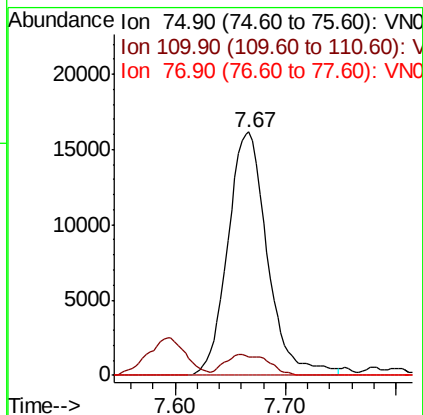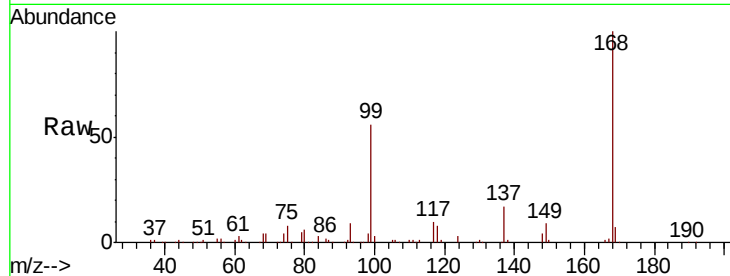

#38
 Carbon Tetrachloride
 Concen: 6.504 ug/l
 RT: 7.66 min Scan# 1832
 Delta R.T. -0.11 min
 Lab File: VN054872.D
 Acq: 1 Apr 2019 14:11

Tgt Ion: 117 Resp: 50491
 Ion Ratio Lower Upper
 117 100
 119 5.0 76.3 114.5#
 121 0.0 24.6 36.8#


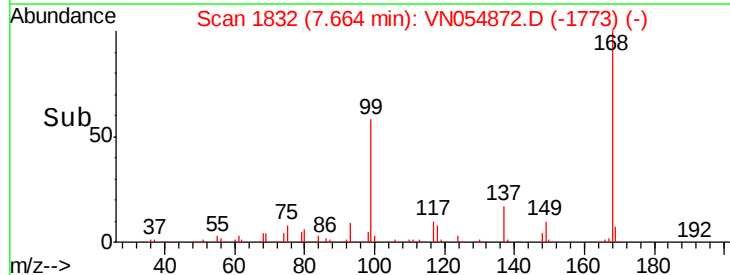
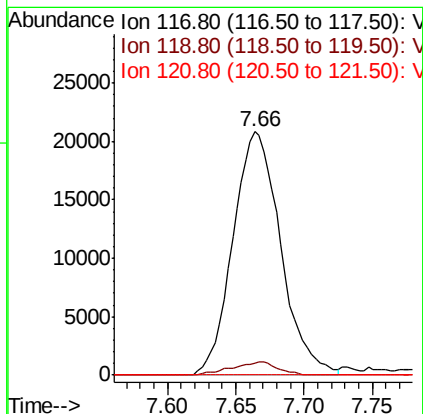



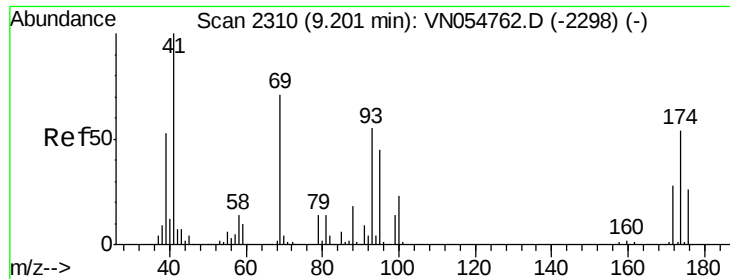

#48
Methvl methacrylate
Concen: 1.447 ug/l
RT: 9.18 min Scan# 2305
Delta R.T. -0.02 min
Lab File: VN054872.D
Acq: 1 Apr 2019 14:11




Instrument :
MSVOA_N
ClientSampleId :
COMP-16


Tot Ion: 41 Resp: 7471
Ion Ratio Lower Upper
41 100
69 0.0 72.6 108.8#
39 18.4 47.5 71.3#

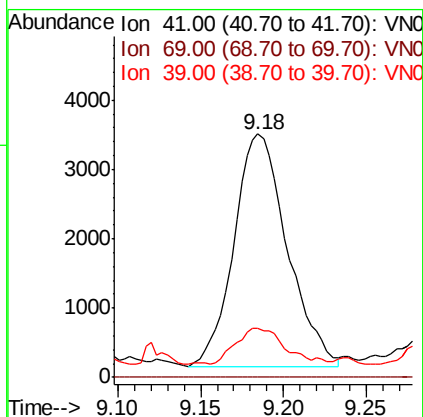

#50
Toluene-d8
Concen: 48.305 ug/l
RT: 10.09 min Scan# 2587
Delta R.T. -0.00 min
Lab File: VN054872.D
Acq: 1 Apr 2019 14:11

Tgt Ion: 98 Resp: 1026970
Ion Ratio Lower Upper
98 100
100 63.6 51.2 76.8

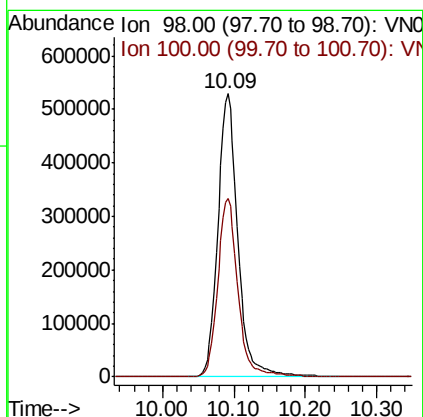

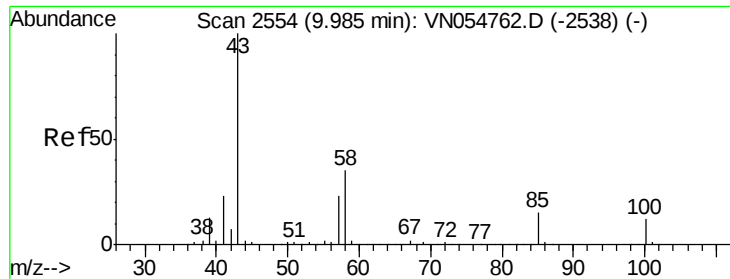

#51

4-Methyl-2-Pentanone

Concen: 0.591 ug/l

RT: 9.99 min Scan# 2555

Delta R.T. 0.00 min

Lab File: VN054872.D

Acq: 1 Apr 2019 14:11

Instrument :

MSVOA_N

ClientSampled :


COMP-16

Tot Ion: 43 Resp: 3166

Ion Ratio Lower Upper




43 100

58 39.9 31.8 47.6

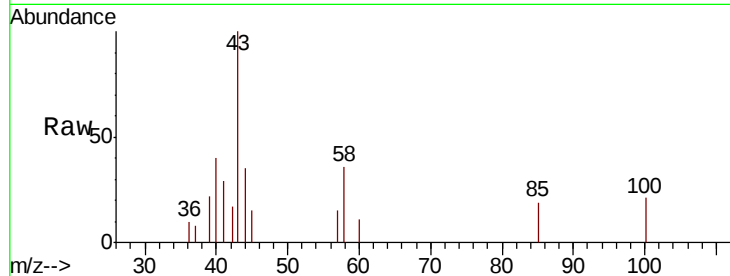

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0

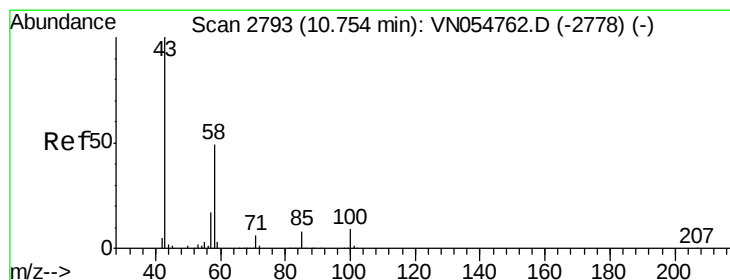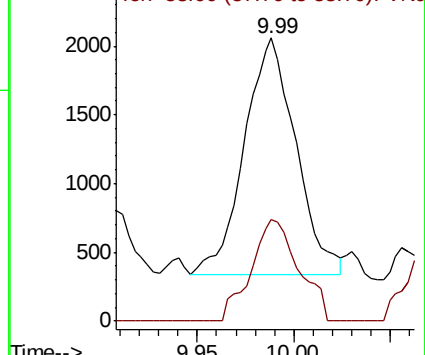

#59

2-Hexanone

Concen: 5.211 ug/l

RT: 10.72 min Scan# 2783

Delta R.T. -0.03 min

Lab File: VN054872.D


Acq: 1 Apr 2019 14:11

Tgt Ion: 43 Resp: 17863

Ion Ratio Lower Upper



43 100


58 0.0 28.0 83.9#



Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0

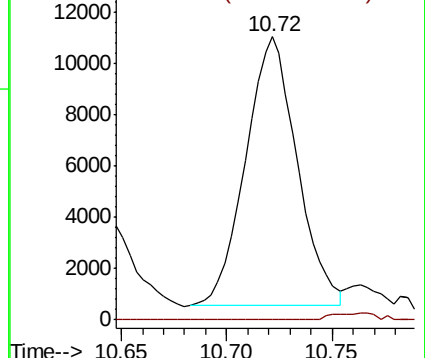

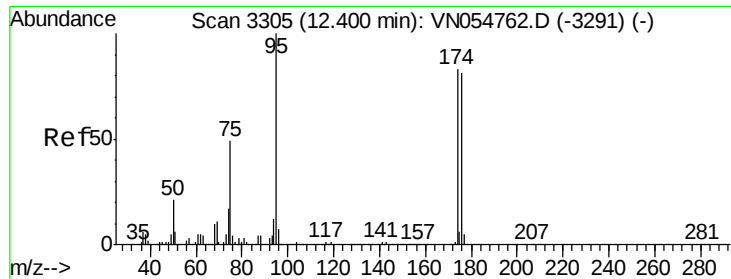

#62

4-Bromofluorobenzene

Concen: 43.203 ug/l

RT: 12.40 min Scan# 3305

Delta R.T. -0.00 min

Lab File: VN054872.D

Acq: 1 Apr 2019 14:11

Instrument :

MSVOA_N

ClientSampleId :

COMP-16


Tot Ion: 95 Resp: 305473

Ion Ratio Lower Upper

95 100

174 83.8 0.0 191.0




176 80.1 0.0 187.4

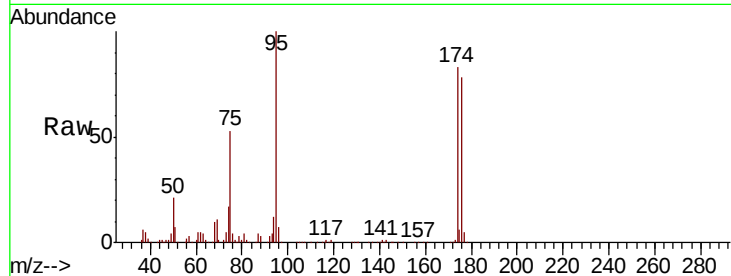

Abundance Ion 94.90 (94.60 to 95.60): VN0

Ion 173.80 (173.50 to 174.50): VN0

Ion 175.80 (175.50 to 176.50): VN0

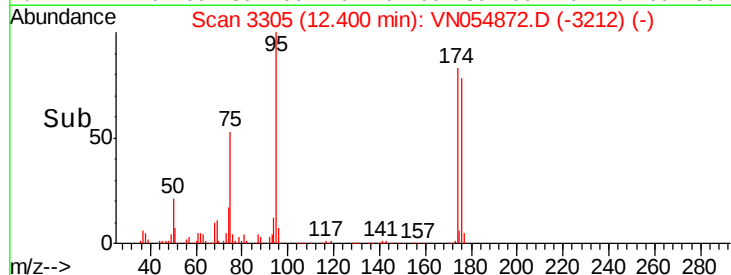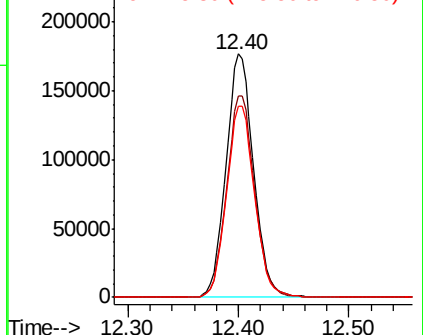

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.41 min Scan# 2996

Delta R.T. -0.00 min

Lab File: VN054872.D

Acq: 1 Apr 2019 14:11


Tgt Ion: 117 Resp: 717517

Ion Ratio Lower Upper

117 100

82 56.1 40.0 60.0



119 32.5 25.8 38.6




Abundance Ion 116.90 (116.60 to 117.60): VN0

Ion 82.00 (81.70 to 82.70): VN0

Ion 118.90 (118.60 to 119.60): VN0

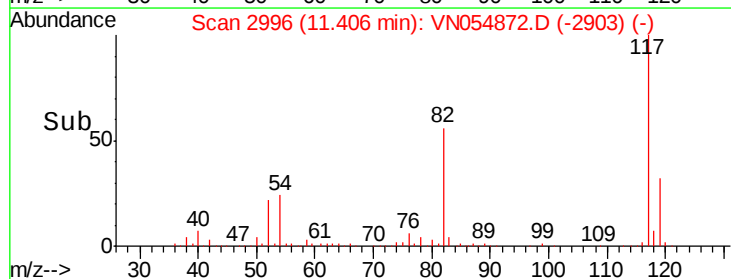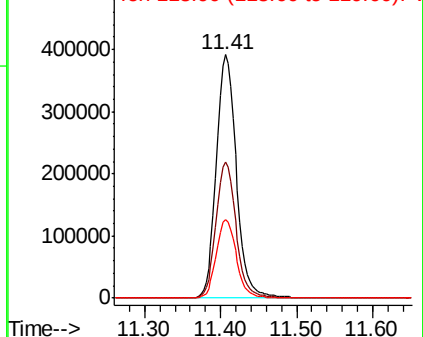

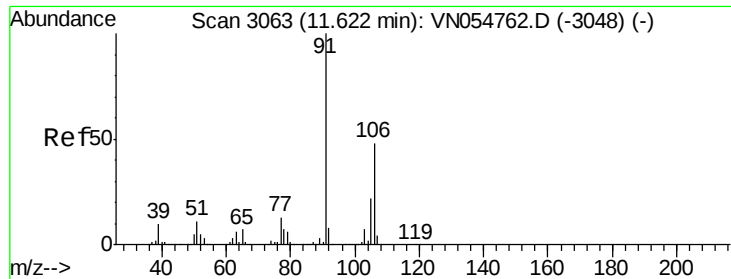

#68

m/p-Xvlenes

Concen: 0.286 ug/l

RT: 11.62 min Scan# 3062

Delta R.T. -0.00 min

Lab File: VN054872.D

Acq: 1 Apr 2019 14:11

Instrument :

MSVOA_N

ClientSampleId :


COMP-16

Tot Ion:106 Resp: 2684

Ion Ratio Lower Upper




106 100

91 199.9 159.4 239.2

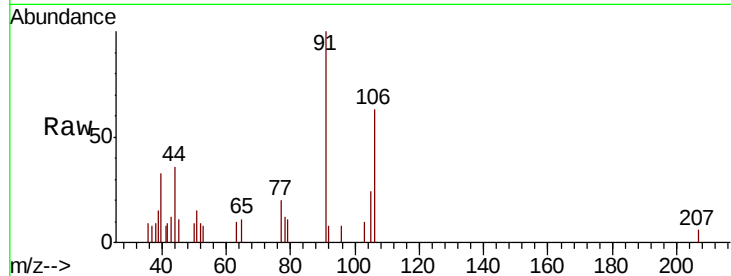

Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VN

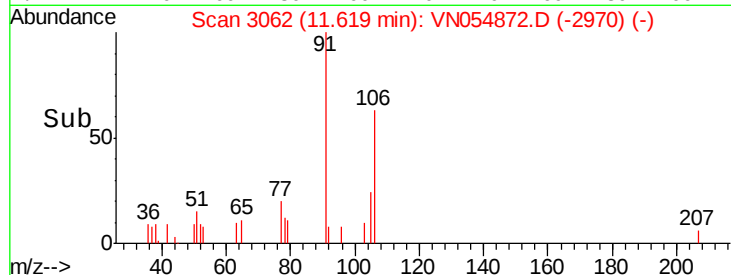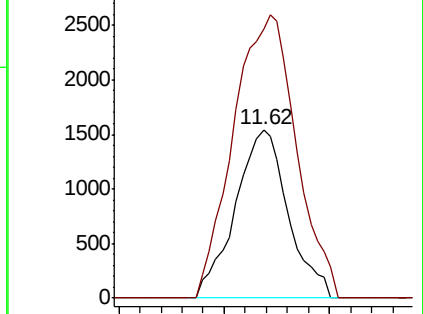

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.34 min Scan# 3598

Delta R.T. -0.00 min

Lab File: VN054872.D

Acq: 1 Apr 2019 14:11


Tgt Ion:152 Resp: 236875

Ion Ratio Lower Upper

152 100

115 57.8 27.2 81.6



150 157.4 0.0 349.2




Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

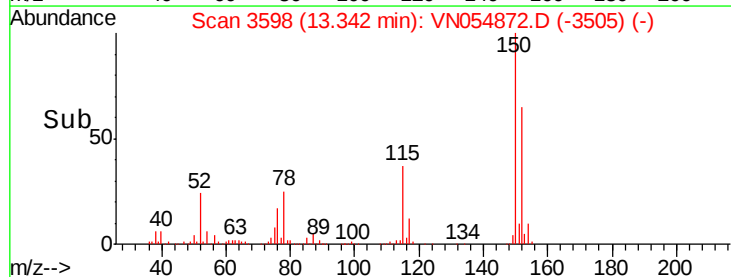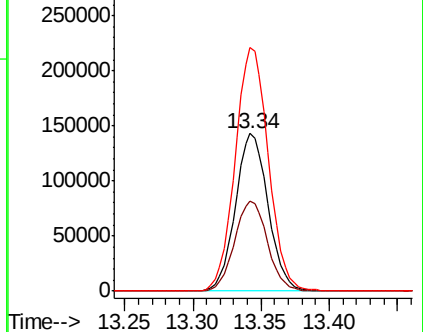



#75

1,1,2,2-Tetrachloroethane

Concen: Below Cal

RT: 12.40 min Scan# 3305

Delta R.T. -0.10 min

Lab File: VN054872.D

Acq: 1 Apr 2019 14:11

Instrument :

MSVOA_N

ClientSampleId :

COMP-16


Tot Ion: 83 Resp: 221

Ion Ratio Lower Upper

83 100

131 207.7 5.8 17.4#




85 0.0 32.2 96.6#



Abundance Ion 82.90 (82.60 to 83.60): VN0

Ion 130.80 (130.50 to 131.50): VN0

Ion 84.90 (84.60 to 85.60): VN0

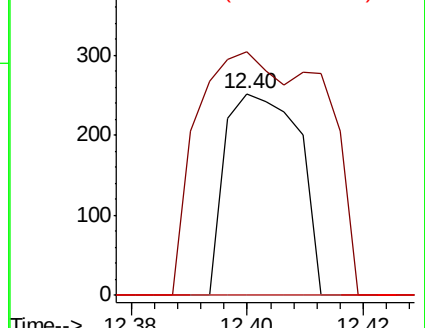

#76

1,2,3-Trichloropropane

Concen: 39.055 ug/l

RT: 12.40 min Scan# 3305

Delta R.T. -0.15 min

Lab File: VN054872.D


Acq: 1 Apr 2019 14:11

Tgt Ion: 75 Resp: 160712

Ion Ratio Lower Upper



75 100


77 1.1 0.0 0.0#



Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 77.00 (76.70 to 77.70): VN0




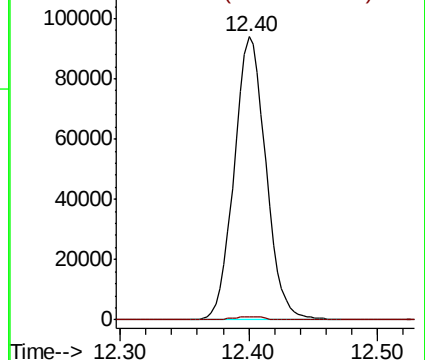


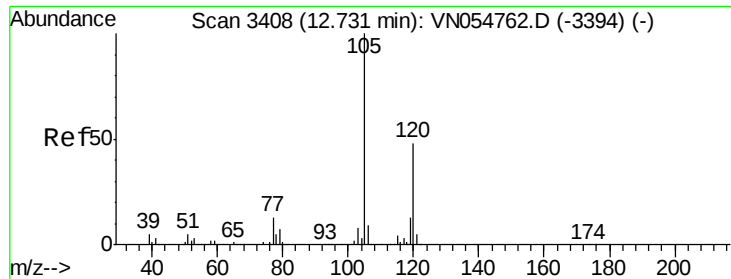

#80
 1,3,5-Trimethylbenzene
 Concen: 0.277 ug/l
 RT: 12.73 min Scan# 3408
 Delta R.T. -0.00 min
 Lab File: VN054872.D
 Acq: 1 Apr 2019 14:11




Instrument :
 MSVOA_N
 ClientSampleId :
 COMP-16


Tot Ion:105 Resp: 4404
 Ion Ratio Lower Upper
 105 100
 120 47.8 25.0 75.0

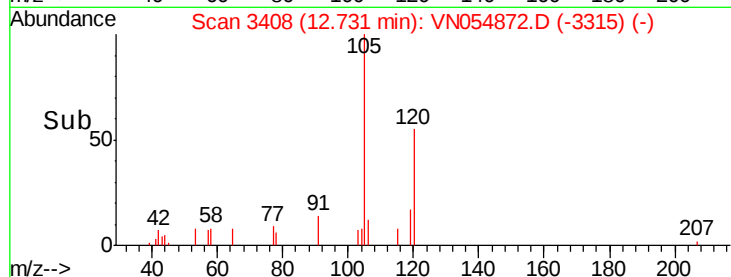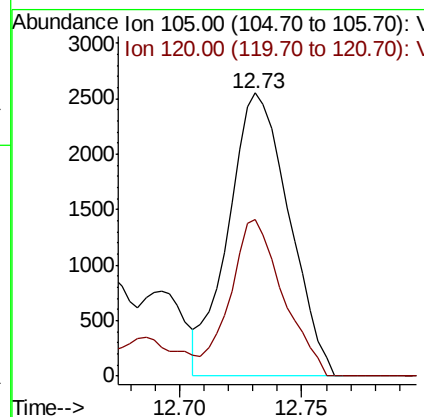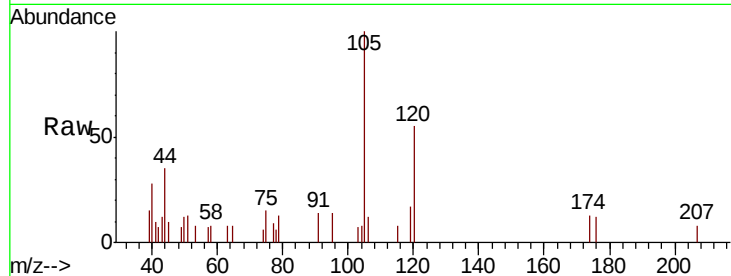

#81
 trans-1,4-Dichloro-2-butene
 Concen: 151.912 ug/l
 RT: 12.40 min Scan# 3305
 Delta R.T. 0.10 min
 Lab File: VN054872.D
 Acq: 1 Apr 2019 14:11

Tgt Ion: 75 Resp: 160712
 Ion Ratio Lower Upper
 75 100
 53 0.0 76.2 114.2#
 89 0.0 39.2 58.8#


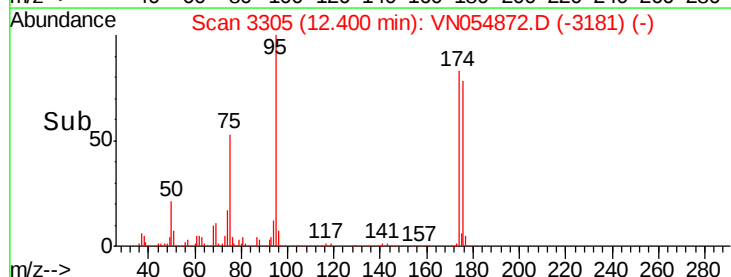
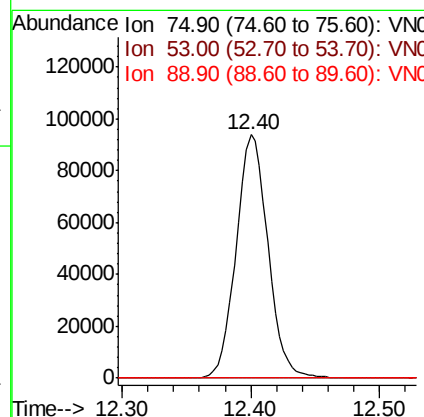



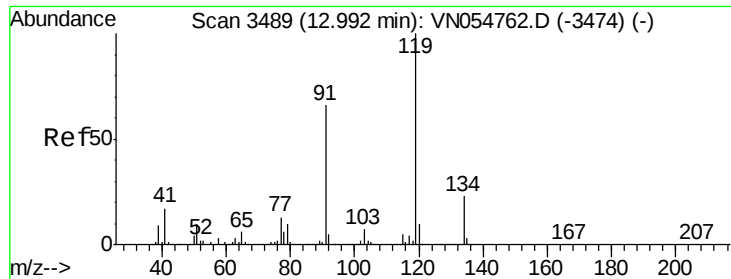

#83
 tert-Butylbenzene
 Concen: Below Cal
 RT: 12.99 min Scan# 3489
 Delta R.T. 0.00 min
 Lab File: VN054872.D
 Acq: 1 Apr 2019 14:11




Instrument :
 MSVOA_N
 ClientSampleId :
 COMP-16


Tot Ion:119 Resp: 223
 Ion Ratio Lower Upper
 119 100
 91 15.2 30.9 92.8#
 134 0.0 13.2 39.6#

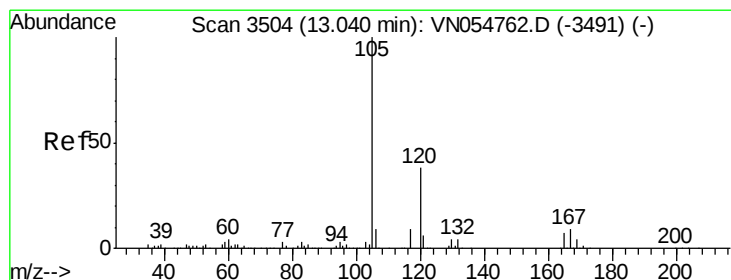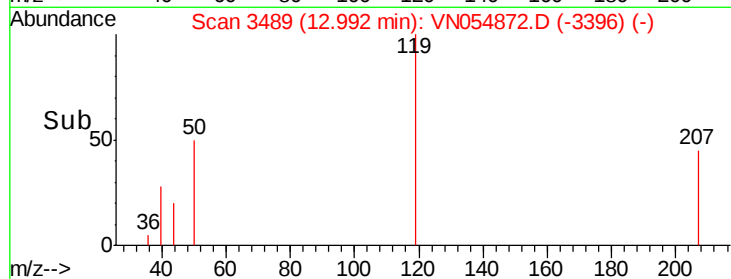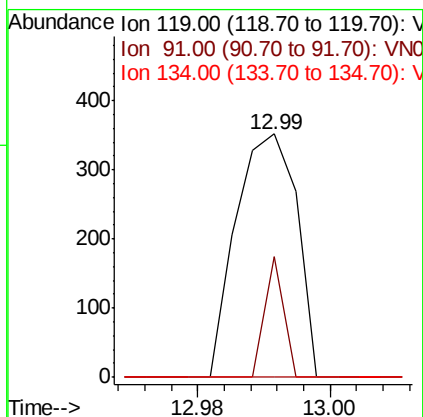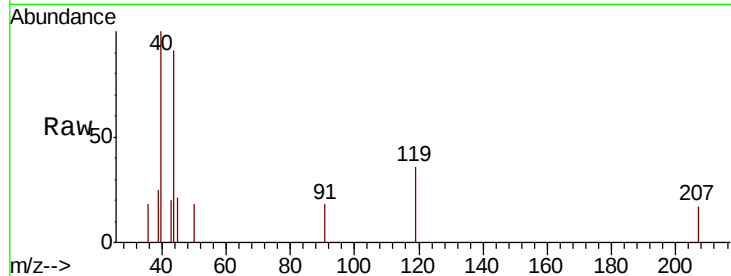

#84
 1,2,4-Trimethylbenzene
 Concen: 0.485 ug/l
 RT: 13.04 min Scan# 3505
 Delta R.T. 0.00 min
 Lab File: VN054872.D
 Acq: 1 Apr 2019 14:11

Tgt Ion:105 Resp: 7348
 Ion Ratio Lower Upper
 105 100
 120 43.8 23.4 70.3

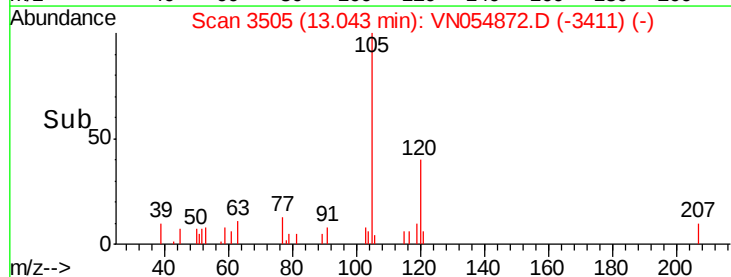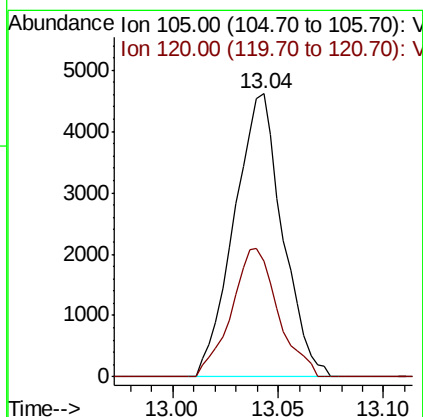



#94

Hexachlorobutadiene

Concen: Below Cal

RT: 15.00 min Scan# 4115

Delta R.T. -0.00 min

Lab File: VN054872.D

Acq: 1 Apr 2019 14:11

Instrument :

MSVOA_N

ClientSampleId :

COMP-16


Tot Ion:225 Resp: 121

Ion Ratio Lower Upper

225 100

223 0.0 31.1 93.5#



227 0.0 31.9 95.9#




Abundance Ion 224.70 (224.40 to 225.40): V

Ion 222.70 (222.40 to 223.40): V

Ion 226.70 (226.40 to 227.40): V

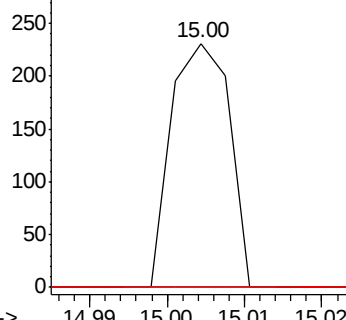

Time-->



#95

Naphthalene

Concen: 0.776 ug/l

RT: 15.13 min Scan# 4155

Delta R.T. -0.00 min

Lab File: VN054872.D

Acq: 1 Apr 2019 14:11


Tgt Ion:128 Resp: 6621

Ion Ratio Lower Upper

128 100

127 13.5 10.1 15.1

129 6.8 8.7 13.1#



Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

