


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN040120\
 Data File : VN060803.D
 Acq On : 1 Apr 2020 9:57
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N031820W.M
 Title : SW846 8260
 Last Update : Wed Mar 18 08:49:09 2020

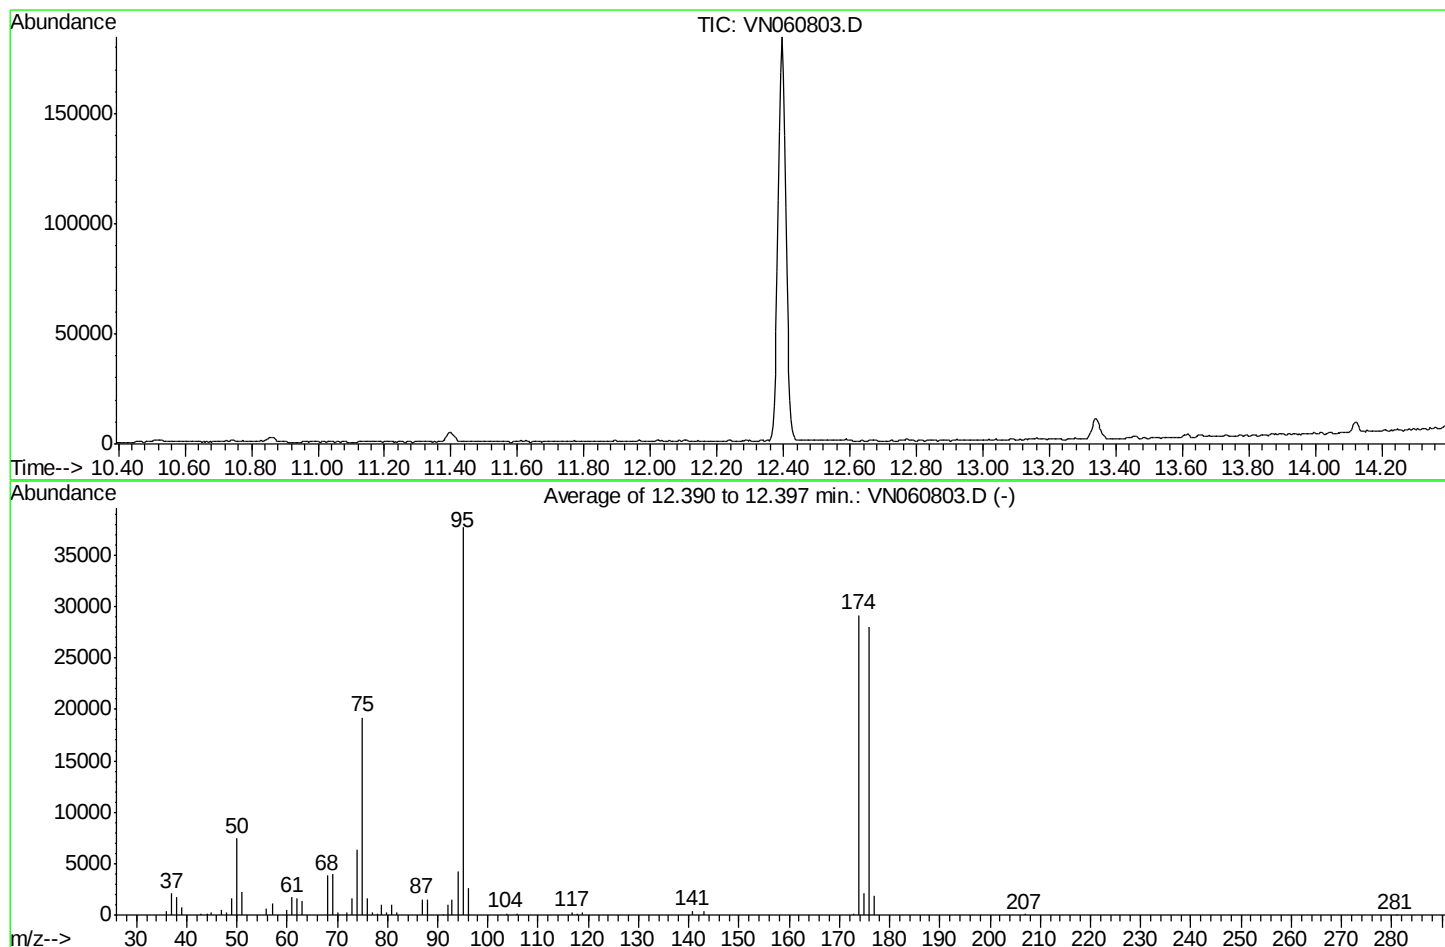

AutoFind: Scans 3302, 3303, 3304; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	7427	PASS
75	95	30	60	50.9	19192	PASS
95	95	100	100	100.0	37704	PASS
96	95	5	9	6.9	2601	PASS
173	174	0.00	2	0.3	102	PASS
174	95	50	100	77.4	29173	PASS
175	174	5	9	7.2	2099	PASS
176	174	95	101	96.1	28042	PASS
177	176	5	9	6.8	1914	PASS