
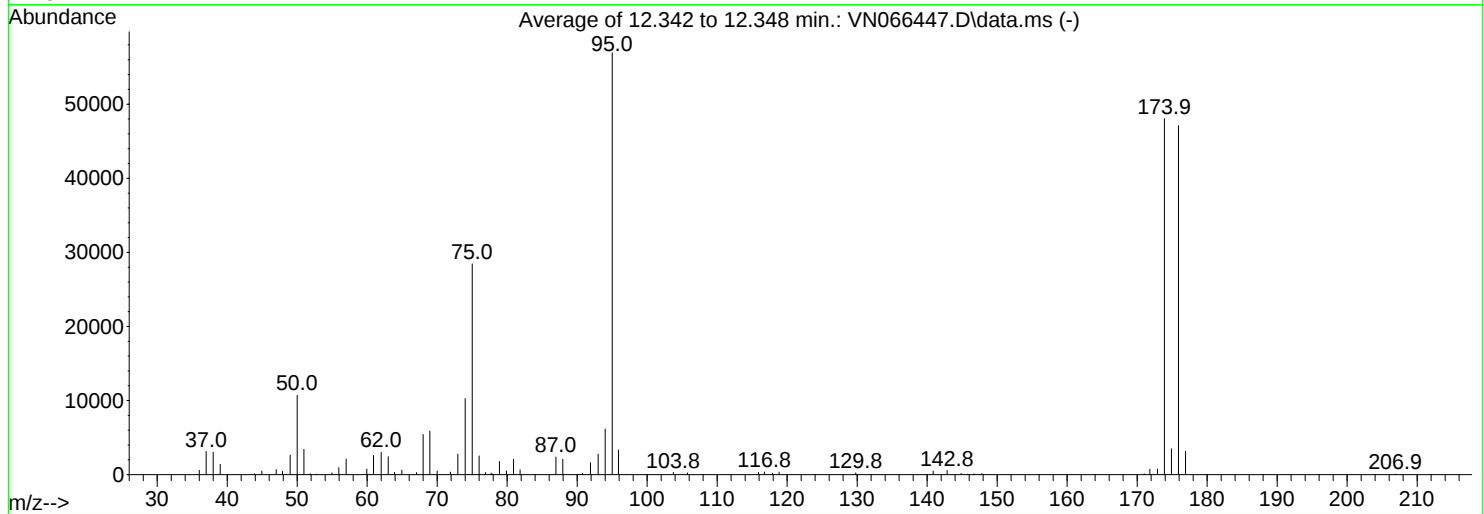


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN040121\
Data File : VN066447.D
Acq On : 1 Apr 2021 10:08
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N032521W.M
Title : SW846 8260
Last Update : Thu Apr 01 14:08:22 2021

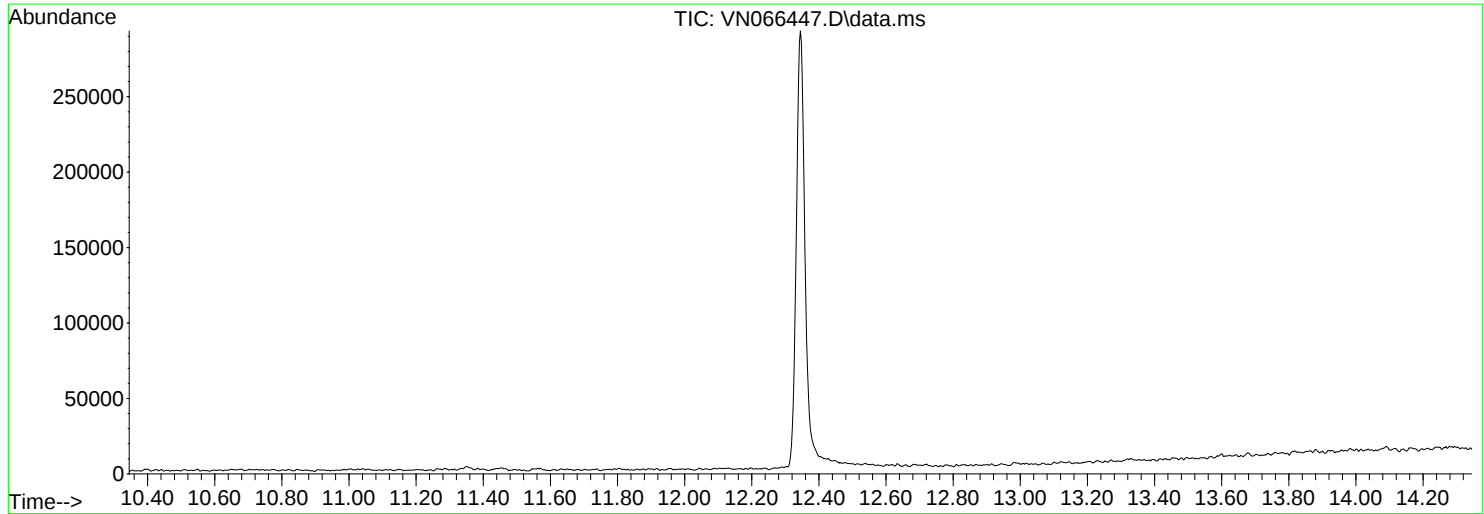

AutoFind: Scans 3972, 3973, 3974; Background Corrected with Scan 3956

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	10714	PASS
75	95	30	60	50.0	28451	PASS
95	95	100	100	100.0	56933	PASS
96	95	5	9	5.8	3323	PASS
173	174	0.00	2	1.6	766	PASS
174	95	50	100	84.4	48061	PASS
175	174	5	9	7.3	3502	PASS
176	174	95	101	98.0	47109	PASS
177	176	5	9	6.7	3158	PASS