

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN040122\
 Data File : VN071763.D
 Acq On : 01 Apr 2022 19:20
 Operator : JC\MD
 Sample : N2090-14
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-58

Quant Time: Apr 02 00:57:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 31 01:57:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.087	168	604005	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.969	114	1025368	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	1047651	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.674	152	380336	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.434	65	348045	50.475	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 100.940%	
35) Dibromofluoromethane	8.022	113	291914	48.381	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 96.760%	
50) Toluene-d8	10.439	98	1298450	52.606	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 105.220%	
62) 4-Bromofluorobenzene	12.727	95	434347	54.411	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 108.820%	


Target Compounds				Qvalue		
3) Chloromethane	2.299	50	2406	0.395	ug/l	96
5) Bromomethane	2.869	94	1038	0.239	ug/l #	73
6) Chloroethane	2.763	64	1609	0.335	ug/l #	54
11) Tert butyl alcohol	5.375	59	6679	5.969	ug/l #	72
16) Acetone	4.293	43	12966	4.400	ug/l	94
18) Methyl Acetate	4.875	43	2891	Below Cal	#	76
19) Methyl tert-butyl Ether	5.610	73	35987	1.943	ug/l #	64
20) Methylene Chloride	5.093	84	1393	0.224	ug/l #	71
25) 2-Butanone	7.351	43	2751	0.648	ug/l	93
31) Cyclohexane	8.087	56	20755	2.213	ug/l #	52
36) 1,1-Dichloropropene	8.087	75	42157	5.003	ug/l #	48
37) Ethyl Acetate	7.351	43	2751	0.298	ug/l #	67
38) Carbon Tetrachloride	8.087	117	55685	6.743	ug/l #	16
39) Methylcyclohexane	9.463	83	12679	1.264	ug/l #	81
43) Isopropyl Acetate	8.651	43	17688	1.153	ug/l #	53
48) Methyl methacrylate	9.645	41	1367	0.215	ug/l #	34
55) 1,1,2-Trichloroethane	10.881	97	3425	0.495	ug/l #	20
58) 2-Chloroethyl Vinyl ether	9.957	63	70	16.988	ug/l #	44
68) m/p-Xylenes	11.945	106	5982	0.438	ug/l	92
73) Isopropylbenzene	12.575	105	34561	1.078	ug/l	98
76) 1,2,3-Trichloropropane	12.727	75	211558	24.011	ug/l #	1
78) n-propylbenzene	12.916	91	24510	0.727	ug/l	97
79) 2-Chlorotoluene	12.916	91	24510	1.134	ug/l #	40
81) trans-1,4-Dichloro-2-b...	12.727	75	211558	74.410	ug/l #	10
85) sec-Butylbenzene	13.498	105	15014	0.499	ug/l #	62
86) p-Isopropyltoluene	13.769	119	12936	0.539	ug/l	92
89) n-Butylbenzene	13.922	91	8336	0.468	ug/l #	26
90) Hexachloroethane	14.210	117	6170	1.405	ug/l #	9
92) 1,2-Dibromo-3-Chloropr...	14.539	75	716	0.432	ug/l #	1
93) 1,2,4-Trichlorobenzene	15.257	180	143	2.108	ug/l #	1
95) Naphthalene	15.504	128	1675	3.892	ug/l #	69
96) 1,2,3-Trichlorobenzene	15.698	180	103	2.431	ug/l #	33


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN040122\
Data File : VN071763.D
Acq On : 01 Apr 2022 19:20
Operator : JC\MD
Sample : N2090-14
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-58

Quant Time: Apr 02 00:57:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
Quant Title : SW846 8260
QLast Update : Thu Mar 31 01:57:54 2022
Response via : Initial Calibration




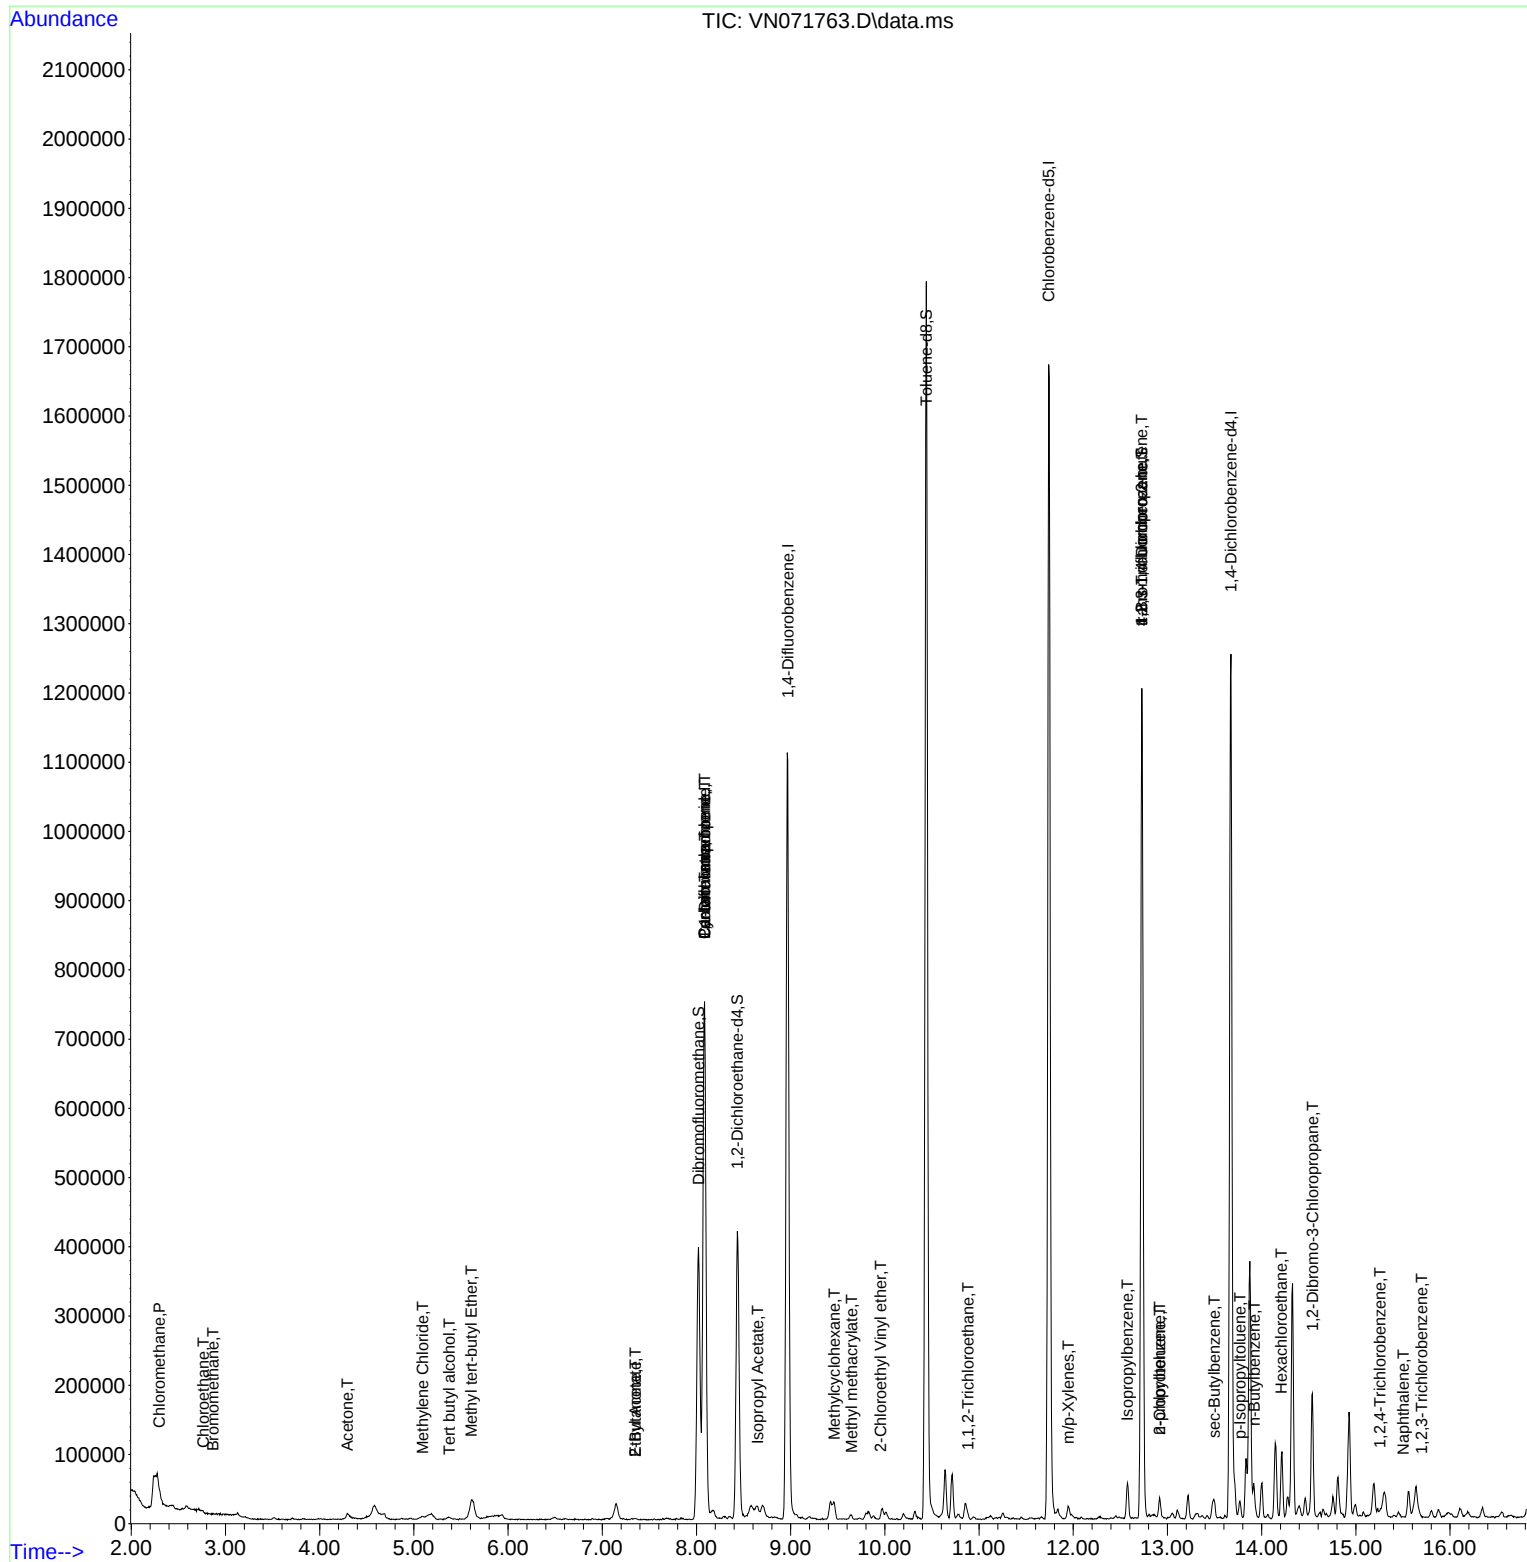




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.087 min Scan# 1
Delta R.T. 0.006 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20




Instrument :
MSVOA_N
ClientSampleId :
MW-58


Tgt Ion:168 Resp: 604005
Ion Ratio Lower Upper
168 100
99 53.3 42.3 63.5



#3
Chloromethane
Concen: 0.395 ug/l
RT: 2.299 min Scan# 53
Delta R.T. -0.000 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20

Tgt Ion: 50 Resp: 2406
Ion Ratio Lower Upper
50 100
52 29.8 25.7 38.5


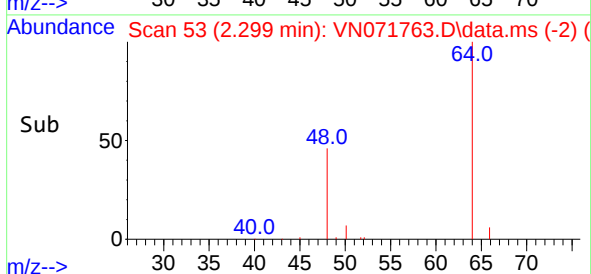






#5
Bromomethane
Concen: 0.239 ug/l
RT: 2.869 min Scan# 11
Delta R.T. 0.023 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20




Instrument :
MSVOA_N
ClientSampleId :
MW-58


Tgt Ion: 94 Resp: 1038
Ion Ratio Lower Upper
94 100
96 69.2 76.0 114.0#



#6
Chloroethane
Concen: 0.335 ug/l
RT: 2.763 min Scan# 132
Delta R.T. -0.247 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20

Tgt Ion: 64 Resp: 1609
Ion Ratio Lower Upper
64 100
66 7.1 26.2 39.4#


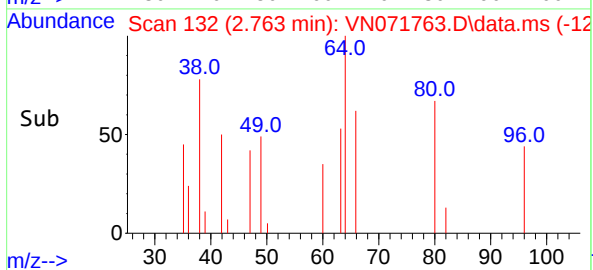






#11
Tert butyl alcohol
Concen: 5.969 ug/l
RT: 5.375 min Scan# 51
Delta R.T. 0.018 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20




Instrument :
MSVOA_N
ClientSampleId :
MW-58


Tgt Ion: 59 Resp: 6679
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#



#16
Acetone
Concen: 4.400 ug/l
RT: 4.293 min Scan# 392
Delta R.T. 0.018 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20

Tgt Ion: 43 Resp: 12966
Ion Ratio Lower Upper
43 100
58 36.0 26.0 39.0



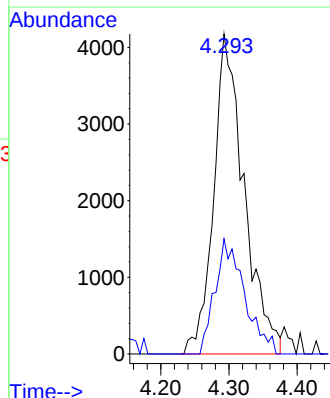





#18
Methyl Acetate
Concen: Below Cal
RT: 4.875 min Scan# 491
Delta R.T. 0.029 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20




Instrument :
MSVOA_N
ClientSampleId :
MW-58


Tgt Ion: 43 Resp: 2891
Ion Ratio Lower Upper
43 100
74 14.3 21.6 32.4#



#19
Methyl tert-butyl Ether
Concen: 1.943 ug/l
RT: 5.610 min Scan# 616
Delta R.T. 0.000 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20

Tgt Ion: 73 Resp: 35987
Ion Ratio Lower Upper
73 100
57 39.3 17.6 26.4#


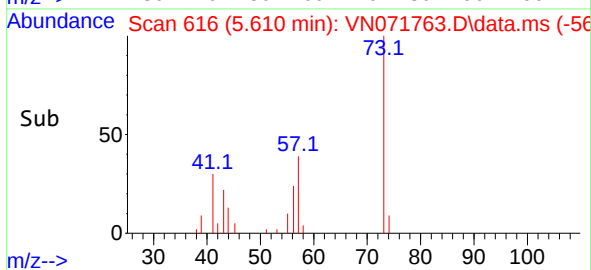






#20
Methylene Chloride
Concen: 0.224 ug/l
RT: 5.093 min Scan# 51
Delta R.T. -0.000 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20




Instrument :
MSVOA_N
ClientSampleId :
MW-58


Tgt Ion: 84	Resp: 1393
Ion Ratio	Lower Upper
84 100	
49 68.0	88.3 132.5#
51 37.4	28.2 42.2
86 45.6	50.6 76.0#

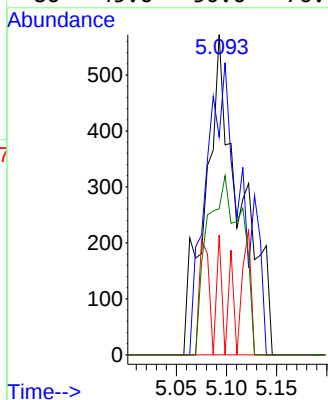

#25
2-Butanone
Concen: 0.648 ug/l
RT: 7.351 min Scan# 912
Delta R.T. 0.023 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20

Tgt Ion: 43	Resp:	2751	
Ion	Ratio	Lower	Upper
43	100		
72	33.2	23.7	35.5

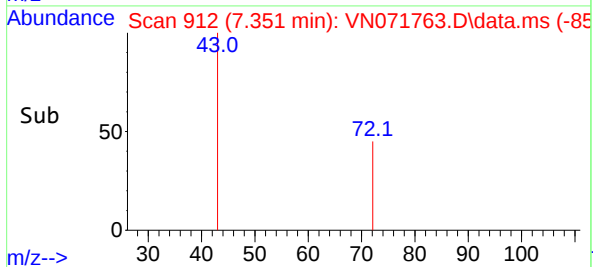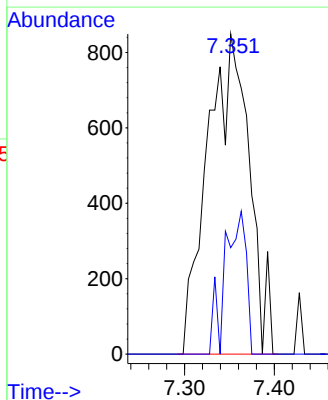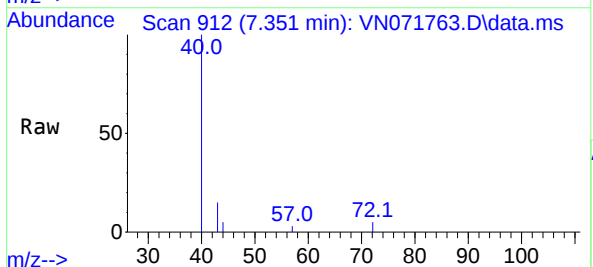



#31

Cyclohexane

Concen: 2.213 ug/l

RT: 8.087 min Scan# 1037

Delta R.T. -0.005 min

Lab File: VN071763.D

Acq: 01 Apr 2022 19:20

Instrument :

MSVOA_N

ClientSampleId :

MW-58





Tgt Ion: 56 Resp: 20755

Ion Ratio Lower Upper

56 100

69 102.3 27.8 41.8#

84 119.4 76.9 115.3#



#33

1,2-Dichloroethane-d4

Concen: 50.475 ug/l

RT: 8.434 min Scan# 1096

Delta R.T. -0.000 min

Lab File: VN071763.D




Acq: 01 Apr 2022 19:20


Tgt Ion: 65 Resp: 348045

Ion Ratio Lower Upper

65 100

67 52.2 0.0 104.8


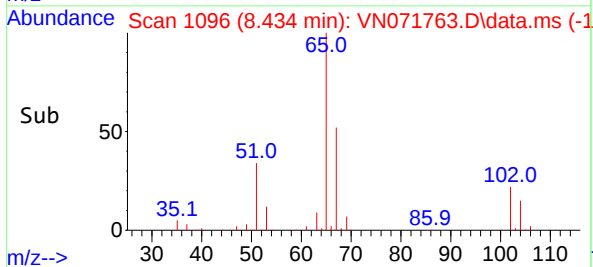

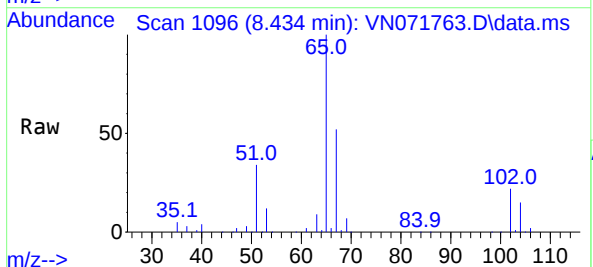




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.969 min Scan# 1186
Delta R.T. 0.006 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20




Instrument :
MSVOA_N
ClientSampleId :
MW-58


Tgt Ion:114 Resp: 1025368
Ion Ratio Lower Upper
114 100
63 18.7 0.0 40.0
88 15.9 0.0 32.6

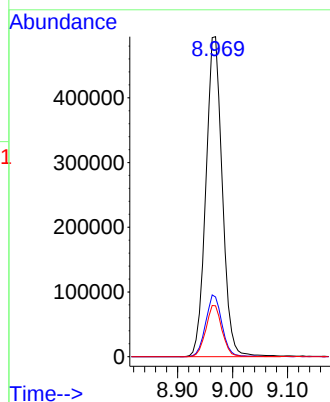

#35
Dibromofluoromethane
Concen: 48.381 ug/l
RT: 8.022 min Scan# 1026
Delta R.T. 0.006 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20

Tgt Ion:113 Resp: 291914
Ion Ratio Lower Upper
113 100
111 102.6 81.4 122.0
192 22.2 17.0 25.6


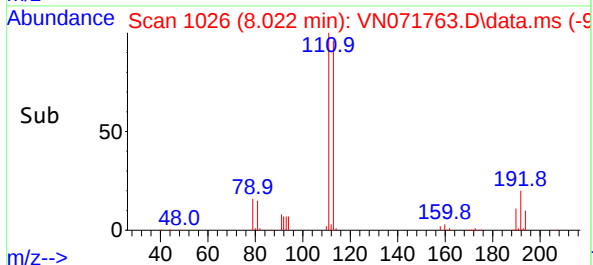

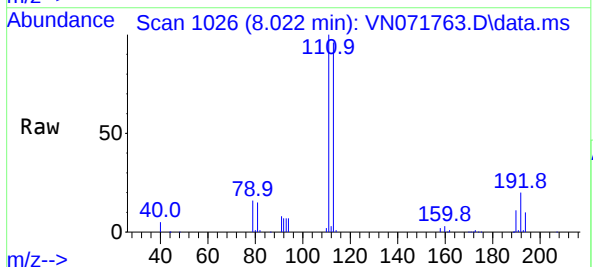




#36
1,1-Dichloropropene
Concen: 5.003 ug/l
RT: 8.087 min Scan# 1059
Delta R.T. -0.129 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20




Instrument :
MSVOA_N
ClientSampleId :
MW-58


Tgt Ion: 75 Resp: 42157
Ion Ratio Lower Upper
75 100
110 8.3 18.3 54.8#
77 0.3 25.1 37.7#



#37
Ethyl Acetate
Concen: 0.298 ug/l
RT: 7.351 min Scan# 912
Delta R.T. -0.053 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20

Tgt Ion: 43 Resp: 2751
Ion Ratio Lower Upper
43 100
61 0.0 11.8 17.6#
70 0.0 9.3 13.9#


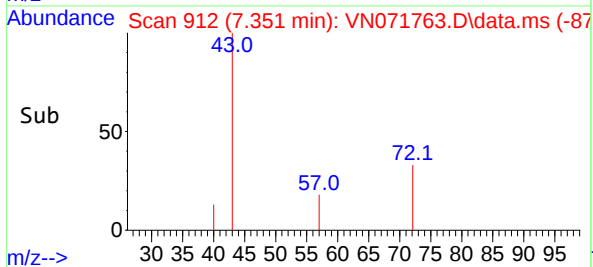

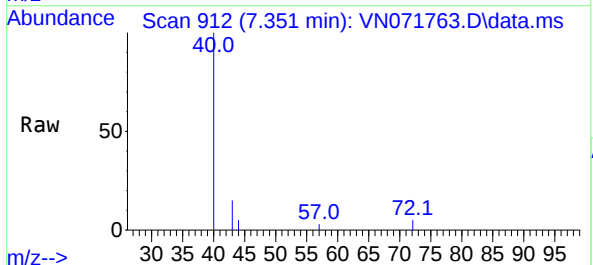




#38
Carbon Tetrachloride
Concen: 6.743 ug/l
RT: 8.087 min Scan# 117
Delta R.T. -0.117 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20




Instrument :
MSVOA_N
ClientSampleId :
MW-58


Tgt Ion:117 Resp: 55685
Ion Ratio Lower Upper
117 100
119 4.7 75.8 113.8#
121 0.0 24.6 37.0#

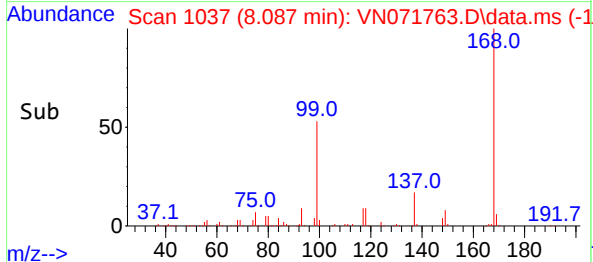

#39
Methylcyclohexane
Concen: 1.264 ug/l
RT: 9.463 min Scan# 1271
Delta R.T. 0.012 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20

Tgt Ion: 83 Resp: 12679
Ion Ratio Lower Upper
83 100
55 55.9 57.8 86.8#
98 37.6 39.4 59.2#


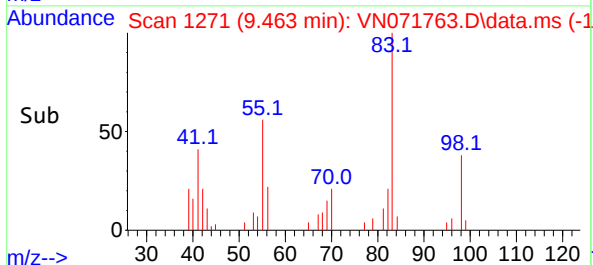
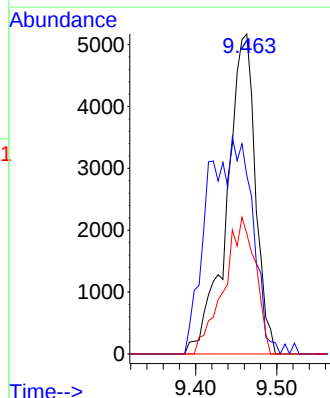
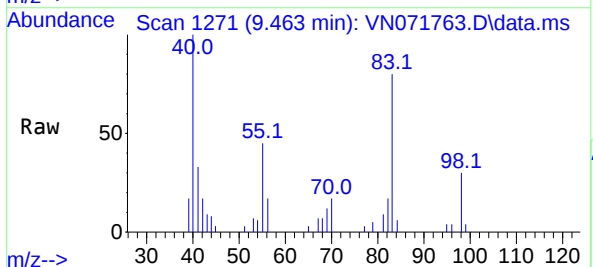




#43
Isopropyl Acetate
Concen: 1.153 ug/l
RT: 8.651 min Scan# 1116
Delta R.T. 0.100 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20




Instrument :
MSVOA_N
ClientSampleId :
MW-58


Tgt Ion: 43 Resp: 17688
Ion Ratio Lower Upper
43 100
61 0.0 21.9 32.9#
87 0.0 12.0 18.0#



#48
Methyl methacrylate
Concen: 0.215 ug/l
RT: 9.645 min Scan# 1302
Delta R.T. 0.094 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20

Tgt Ion: 41 Resp: 1367
Ion Ratio Lower Upper
41 100
69 180.4 74.7 112.1#
39 38.3 45.6 68.4#



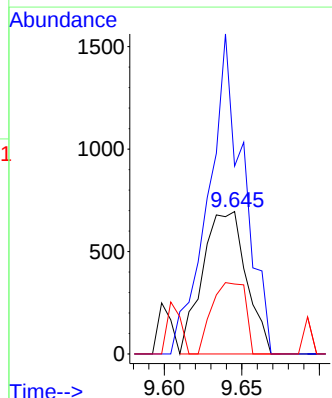





#50
Toluene-d8
Concen: 52.606 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. 0.000 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20




Instrument :
MSVOA_N
ClientSampleId :
MW-58


Tgt Ion: 98 Resp: 1298450
Ion Ratio Lower Upper
98 100
100 64.7 52.6 78.8

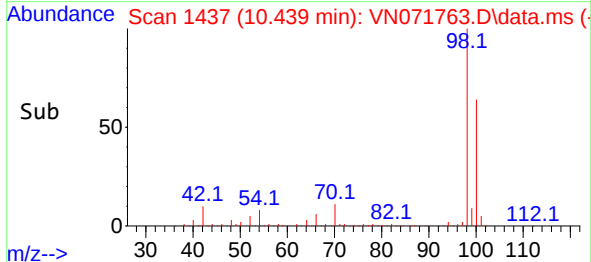

#55
1,1,2-Trichloroethane
Concen: 0.495 ug/l
RT: 10.881 min Scan# 1512
Delta R.T. -0.011 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20

Tgt Ion: 97 Resp: 3425
Ion Ratio Lower Upper
97 100
83 9.2 66.2 99.4#
85 0.0 43.9 65.9#
99 0.0 50.6 76.0#


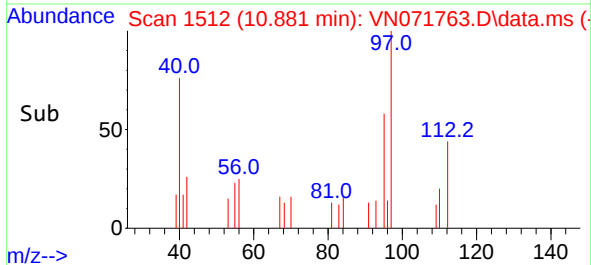

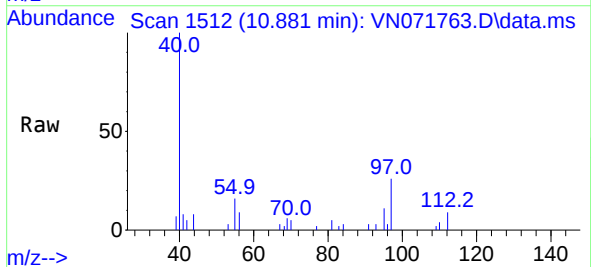




#58
2-Chloroethyl Vinyl ether
Concen: 16.988 ug/l
RT: 9.957 min Scan# 11
Delta R.T. -0.077 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20




Instrument :
MSVOA_N
ClientSampleId :
MW-58


Tgt Ion: 63 Resp: 70
Ion Ratio Lower Upper
63 100
106 0.0 24.6 36.8#

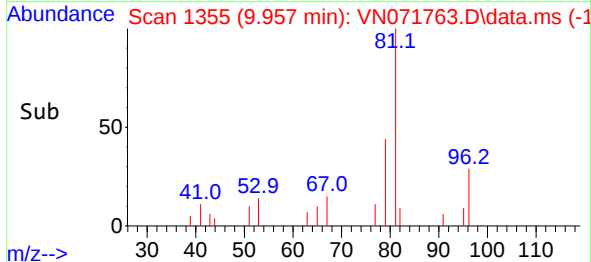

#62
4-Bromofluorobenzene
Concen: 54.411 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20

Tgt Ion: 95 Resp: 434347
Ion Ratio Lower Upper
95 100
174 84.9 0.0 167.6
176 81.3 0.0 163.4


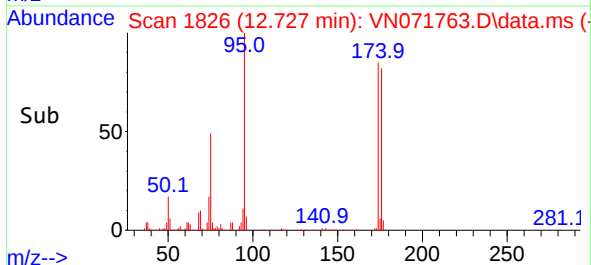
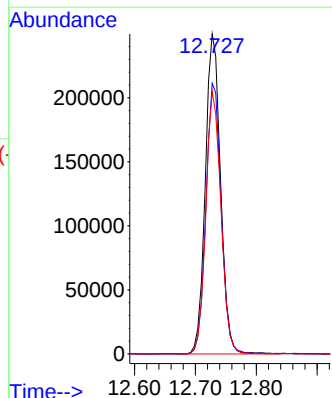
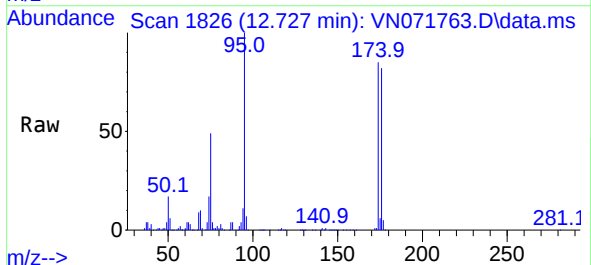




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 1658
Delta R.T. 0.000 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20




Instrument :
MSVOA_N
ClientSampleId :
MW-58


Tgt Ion:117 Resp: 1047651
Ion Ratio Lower Upper
117 100
82 53.9 44.2 66.2
119 31.4 25.4 38.0

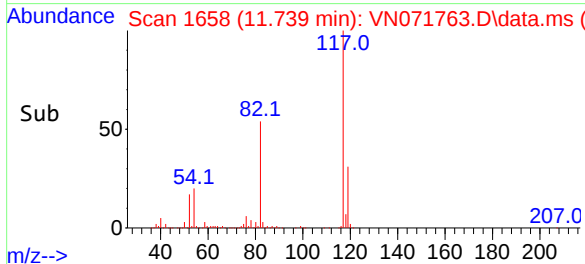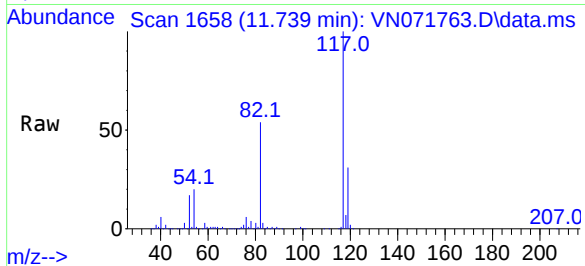

#68
m/p-Xylenes
Concen: 0.438 ug/l
RT: 11.945 min Scan# 1693
Delta R.T. -0.006 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20

Tgt Ion:106 Resp: 5982
Ion Ratio Lower Upper
106 100
91 211.0 158.9 238.3


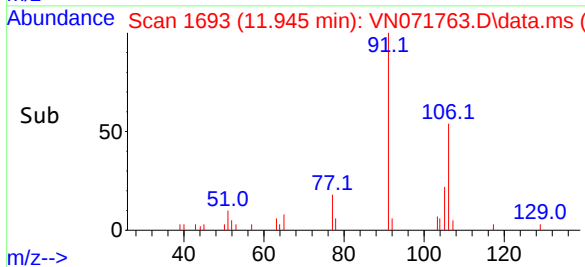

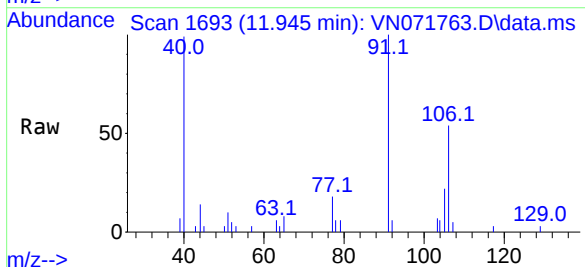




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.674 min Scan# 1986
Delta R.T. 0.005 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20




Instrument :
MSVOA_N
ClientSampleId :
MW-58


Tgt Ion:152 Resp: 380336
Ion Ratio Lower Upper
152 100
115 57.2 28.9 86.7
150 156.9 0.0 356.2

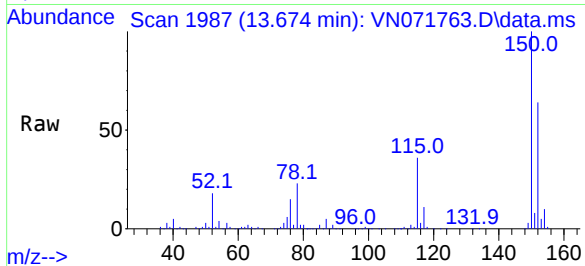

#73
Isopropylbenzene
Concen: 1.078 ug/l
RT: 12.575 min Scan# 1800
Delta R.T. -0.000 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20

Tgt Ion:105 Resp: 34561
Ion Ratio Lower Upper
105 100
120 28.0 13.5 40.4


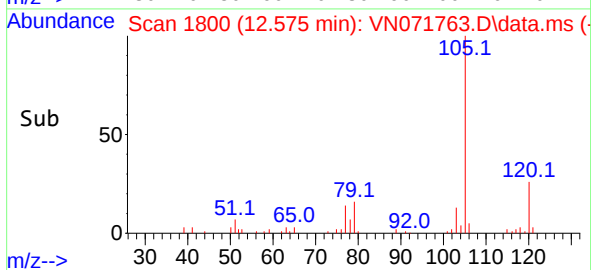

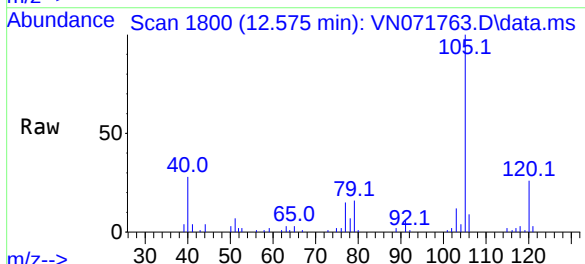




#76
1,2,3-Trichloropropane
Concen: 24.011 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. -0.147 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20




Instrument :
MSVOA_N
ClientSampleId :
MW-58


Tgt Ion: 75 Resp: 211558
Ion Ratio Lower Upper
75 100
77 1.4 98.5 295.5#

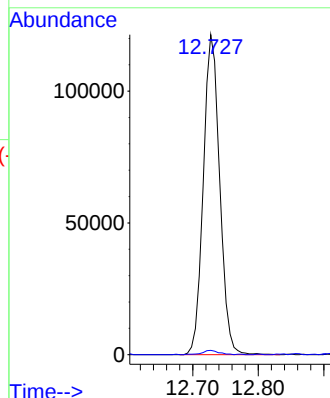

#78
n-propylbenzene
Concen: 0.727 ug/l
RT: 12.916 min Scan# 1858
Delta R.T. -0.000 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20

Tgt Ion: 91 Resp: 24510
Ion Ratio Lower Upper
91 100
120 22.1 11.9 35.5



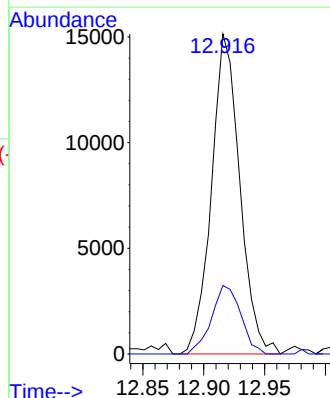



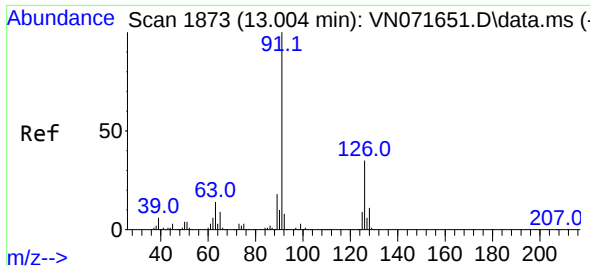

#79
2-Chlorotoluene
Concen: 1.134 ug/l
RT: 12.916 min Scan# 1858
Delta R.T. -0.088 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20




Instrument :
MSVOA_N
ClientSampleId :
MW-58


Tgt Ion: 91 Resp: 24510
Ion Ratio Lower Upper
91 100
126 0.0 17.3 51.9#

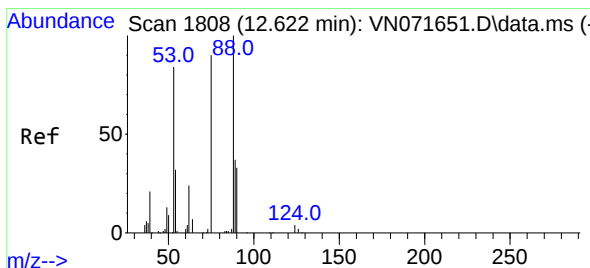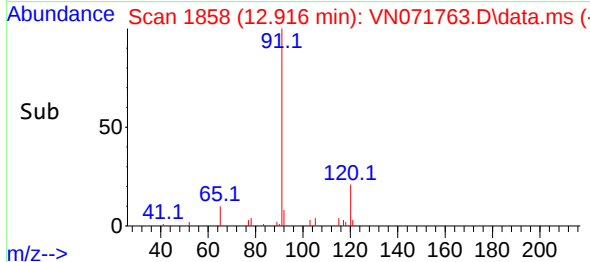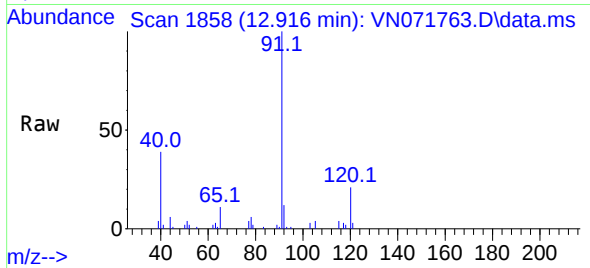

#81
trans-1,4-Dichloro-2-butene
Concen: 74.410 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.105 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20

Tgt Ion: 75 Resp: 211558
Ion Ratio Lower Upper
75 100
53 0.1 78.0 117.0#
89 0.0 37.2 55.8#


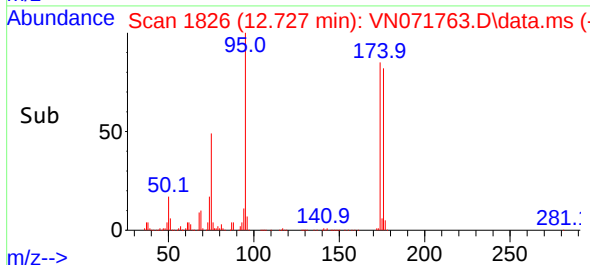
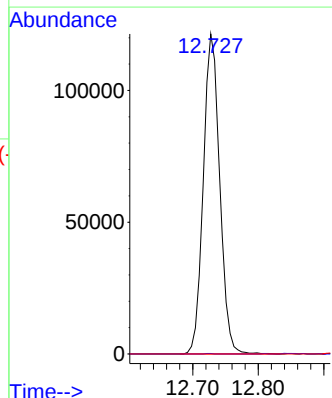
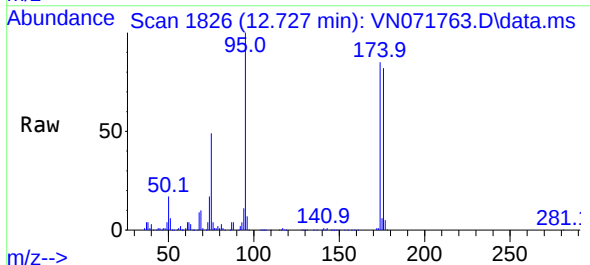




#85
 sec-Butylbenzene
 Concen: 0.499 ug/l
 RT: 13.498 min Scan# 1957
 Delta R.T. 0.000 min
 Lab File: VN071763.D
 Acq: 01 Apr 2022 19:20




Instrument :
 MSVOA_N
 ClientSampleId :
 MW-58


Tgt Ion:105 Resp: 15014
 Ion Ratio Lower Upper
 105 100
 134 38.5 10.4 31.1#

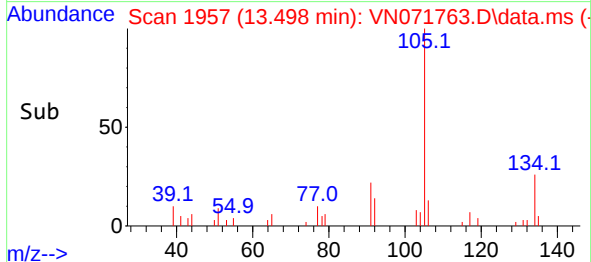

#86
 p-Isopropyltoluene
 Concen: 0.539 ug/l
 RT: 13.769 min Scan# 2003
 Delta R.T. 0.159 min
 Lab File: VN071763.D
 Acq: 01 Apr 2022 19:20

Tgt Ion:119 Resp: 12936
 Ion Ratio Lower Upper
 119 100
 134 28.8 13.3 39.8
 91 28.1 11.3 33.9


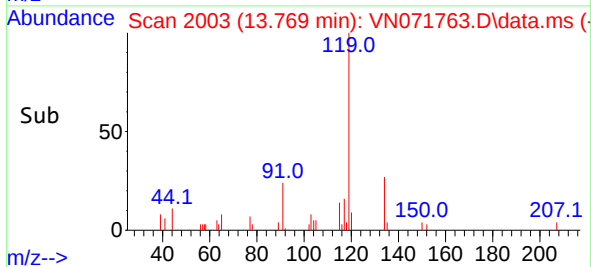

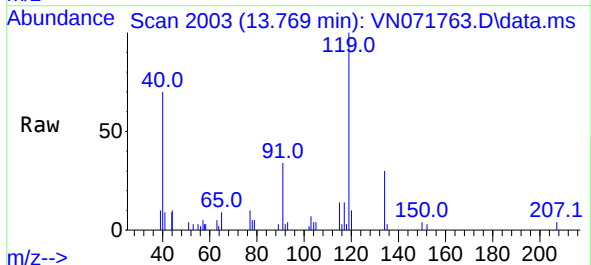




#89
n-Butylbenzene
Concen: 0.468 ug/l
RT: 13.922 min Scan# 2032
Delta R.T. -0.018 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20




Instrument :
MSVOA_N
ClientSampleId :
MW-58


Tgt Ion: 91 Resp: 8336
Ion Ratio Lower Upper
91 100
92 27.2 26.9 80.7
134 103.0 13.6 40.8#



#90
Hexachloroethane
Concen: 1.405 ug/l
RT: 14.210 min Scan# 2078
Delta R.T. 0.006 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20

Tgt Ion: 117 Resp: 6170
Ion Ratio Lower Upper
117 100
201 0.0 40.6 122.0#


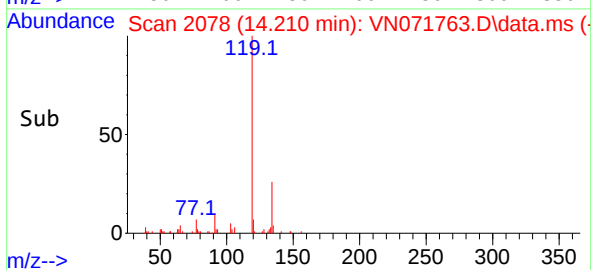






#92
1,2-Dibromo-3-Chloropropane
Concen: 0.432 ug/l
RT: 14.539 min Scan# 2144
Delta R.T. -0.059 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20




Instrument :
MSVOA_N
ClientSampleId :
MW-58


Tgt Ion: 75 Resp: 716
Ion Ratio Lower Upper
75 100
155 0.0 44.9 134.5#
157 0.0 59.0 176.8#



#93
1,2,4-Trichlorobenzene
Concen: 2.108 ug/l
RT: 15.257 min Scan# 2256
Delta R.T. -0.000 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20

Tgt Ion: 180 Resp: 143
Ion Ratio Lower Upper
180 100
182 155.2 47.5 142.5#
145 3432.9 14.5 43.5#


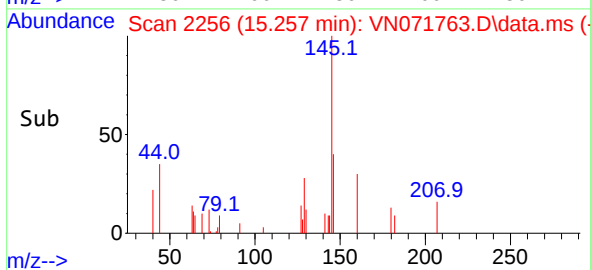






#95
Naphthalene
Concen: 3.892 ug/l
RT: 15.504 min Scan# 21
Delta R.T. 0.006 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20

Instrument :
MSVOA_N
ClientSampleId :
MW-58

Tgt Ion:	128	Resp:	1675
Ion	Ratio	Lower	Upper
128	100		
127	0.0	10.3	15.5#
129	0.0	8.6	13.0#

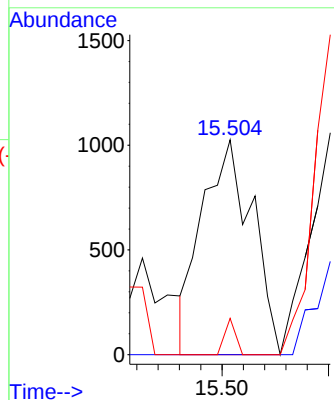

#96
1,2,3-Trichlorobenzene
Concen: 2.431 ug/l
RT: 15.698 min Scan# 2331
Delta R.T. 0.006 min
Lab File: VN071763.D
Acq: 01 Apr 2022 19:20

Tgt Ion:	180	Resp:	103
Ion	Ratio	Lower	Upper
180	100		
182	164.1	47.8	143.3#
145	0.0	15.5	46.5#

