

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN040122\
 Data File : VN071774.D
 Acq On : 02 Apr 2022 00:34
 Operator : JC\MD
 Sample : N2222-01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-8

Quant Time: Apr 02 05:31:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 31 01:57:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.086	168	532231	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	907296	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.745	117	891452	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.674	152	296751	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.433	65	307594	50.624	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 101.240%	
35) Dibromofluoromethane	8.022	113	257040	48.145	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 96.280%	
50) Toluene-d8	10.439	98	1128045	51.650	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 103.300%	
62) 4-Bromofluorobenzene	12.727	95	341343	48.325	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 96.660%	
Target Compounds						
					Qvalue	
3) Chloromethane	2.299	50	2568	0.479	ug/l #	71
5) Bromomethane	2.869	94	891	0.233	ug/l #	70
11) Tert butyl alcohol	5.375	59	956	0.970	ug/l #	72
13) Acrolein	4.057	56	880	0.732	ug/l #	75
15) Acrylonitrile	5.569	53	791	0.276	ug/l #	32
16) Acetone	4.310	43	9525	3.668	ug/l #	68
17) Carbon Disulfide	4.545	76	3507	0.348	ug/l #	81
18) Methyl Acetate	4.851	43	1040	Below Cal	#	61
25) 2-Butanone	7.345	43	1617	0.432	ug/l	92
29) Tetrahydrofuran	7.692	42	16713	6.895	ug/l	97
30) Chloroform	7.816	83	2771	0.288	ug/l	91
31) Cyclohexane	8.081	56	9507	1.151	ug/l #	12
36) 1,1-Dichloropropene	8.081	75	37832	5.074	ug/l #	49
38) Carbon Tetrachloride	8.086	117	48223	6.600	ug/l #	17
41) Methacrylonitrile	7.698	41	10798	2.702	ug/l #	34
49) 1,4-Dioxane	9.575	88	57	Below Cal	#	25
51) 4-Methyl-2-Pentanone	10.333	43	3672	0.471	ug/l #	76
59) 2-Hexanone	11.092	43	5597	1.019	ug/l	93
74) N-amyl acetate	12.392	43	3148	0.439	ug/l #	86
76) 1,2,3-Trichloropropane	12.727	75	169425	24.646	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.727	75	169425	76.376	ug/l #	10
82) 4-Chlorotoluene	13.104	91	3355	0.215	ug/l	89
87) 1,3-Dichlorobenzene	13.610	146	2661	0.266	ug/l	93
88) 1,4-Dichlorobenzene	13.610	146	2661	0.273	ug/l	95
89) n-Butylbenzene	13.939	91	4758	0.343	ug/l	89
91) 1,2-Dichlorobenzene	13.980	146	2939	0.300	ug/l	92
92) 1,2-Dibromo-3-Chloropr...	14.598	75	337	0.260	ug/l #	74
93) 1,2,4-Trichlorobenzene	15.262	180	2785	2.651	ug/l	97
95) Naphthalene	15.504	128	9091	4.424	ug/l #	97
96) 1,2,3-Trichlorobenzene	15.698	180	3619	3.167	ug/l	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN040122\
Data File : VN071774.D
Acq On : 02 Apr 2022 00:34
Operator : JC\MD
Sample : N2222-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-8

Quant Time: Apr 02 05:31:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
Quant Title : SW846 8260
QLast Update : Thu Mar 31 01:57:54 2022
Response via : Initial Calibration



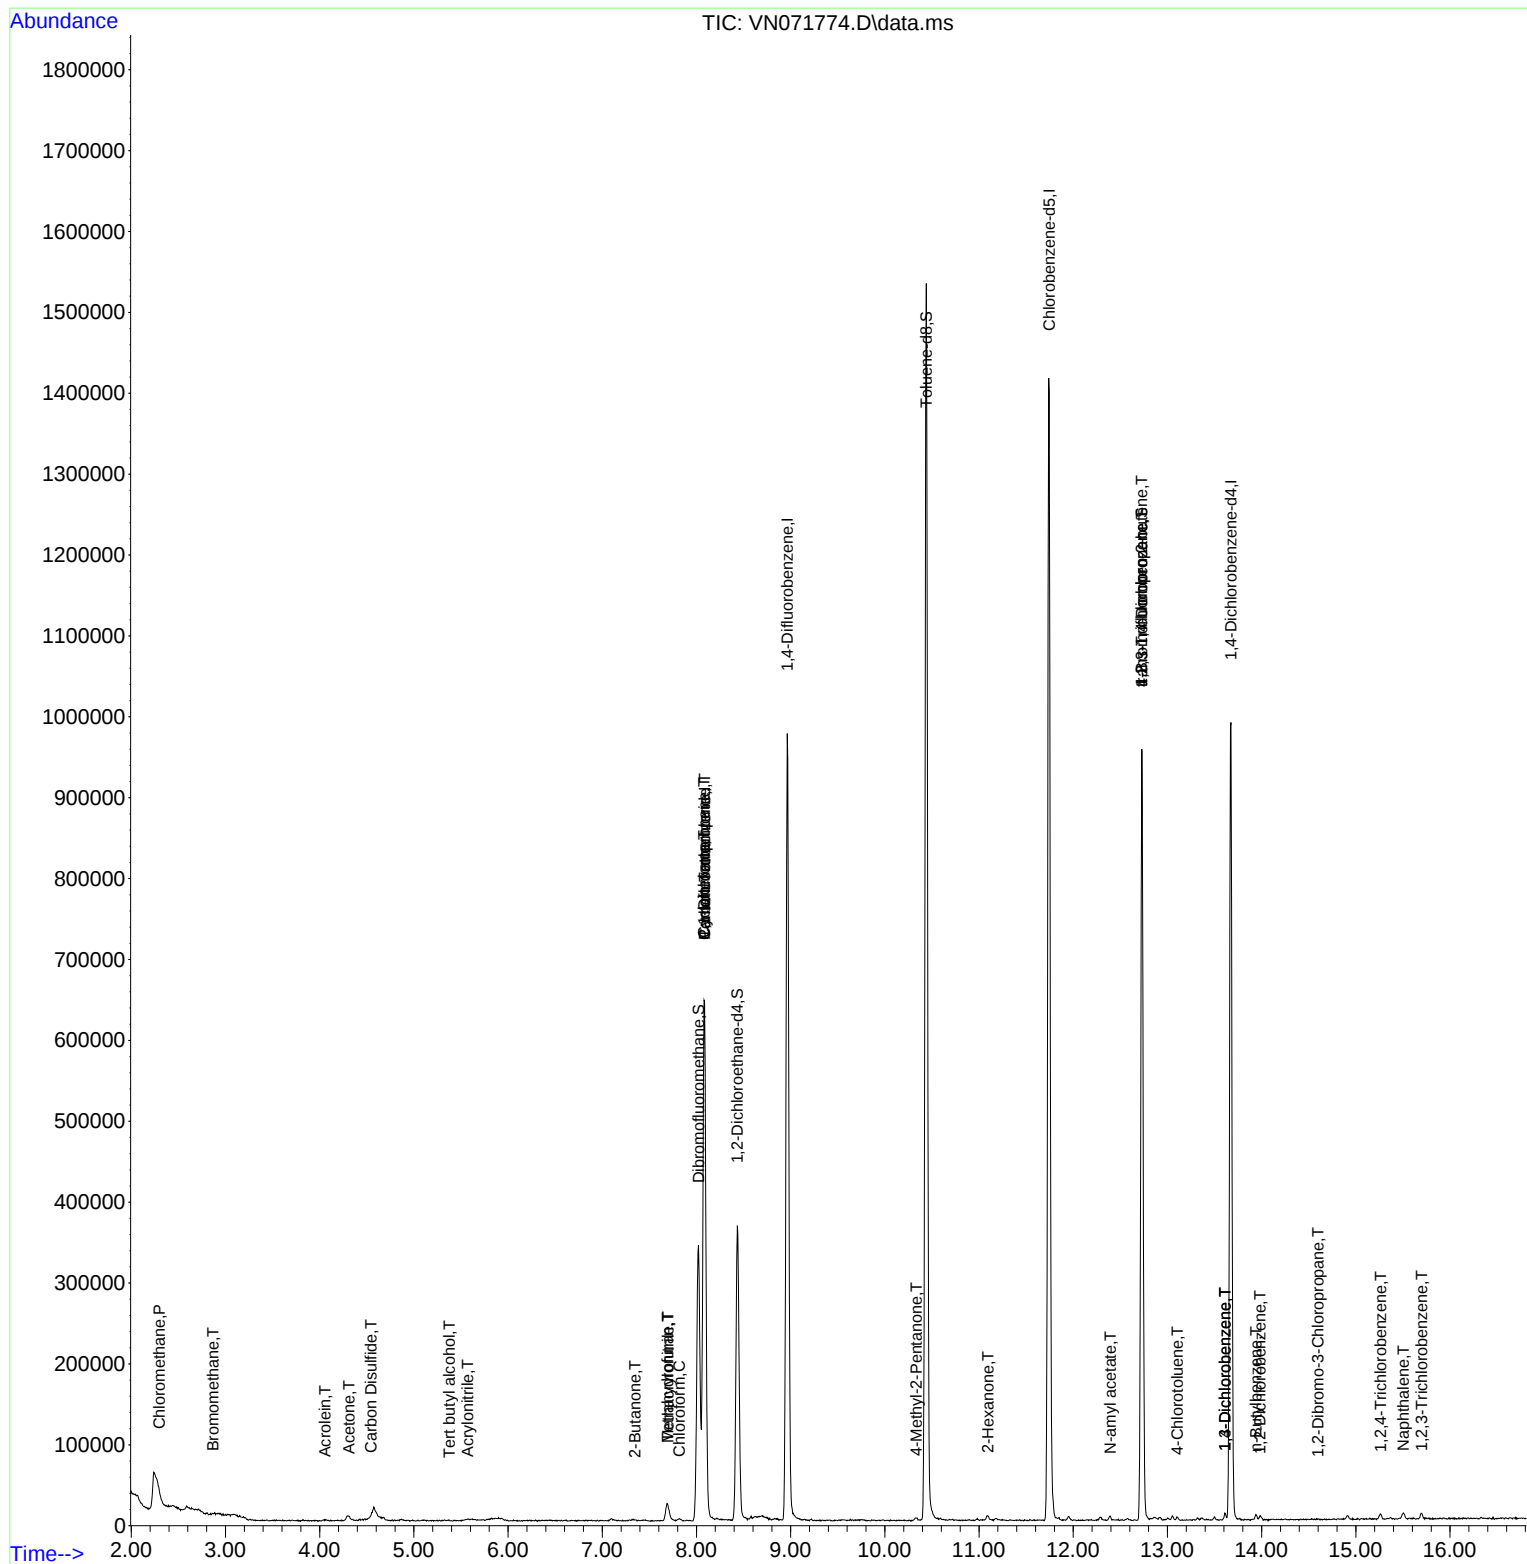




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.086 min Scan# 10
Delta R.T. 0.005 min
Lab File: VN071774.D
Acq: 02 Apr 2022 00:34




Instrument :
MSVOA_N
ClientSampleId :
MW-8


Tgt Ion:168 Resp: 532231
Ion Ratio Lower Upper
168 100
99 53.5 42.3 63.5

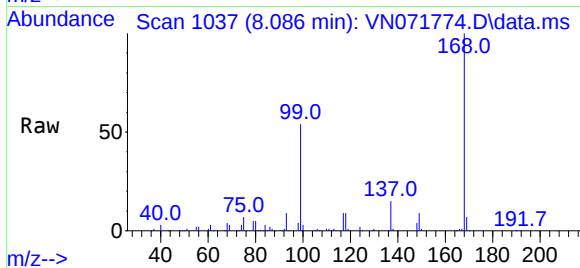

#3
Chloromethane
Concen: 0.479 ug/l
RT: 2.299 min Scan# 53
Delta R.T. -0.000 min
Lab File: VN071774.D
Acq: 02 Apr 2022 00:34

Tgt Ion: 50 Resp: 2568
Ion Ratio Lower Upper
50 100
52 15.8 25.7 38.5#


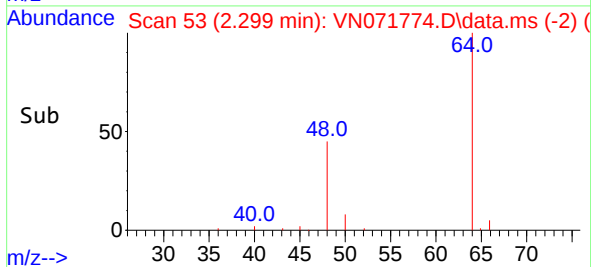

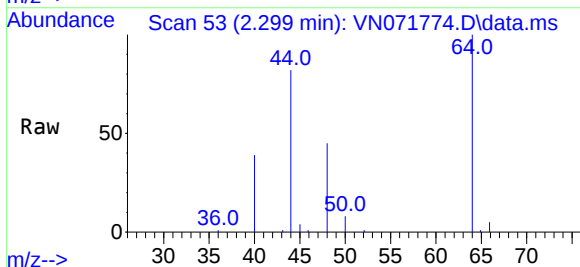


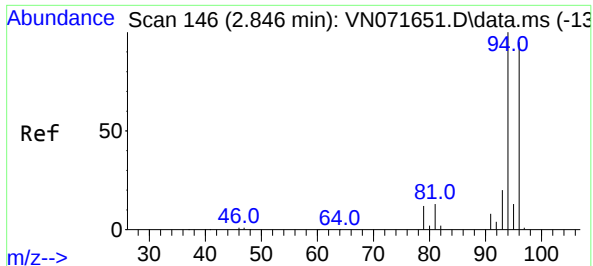

#5
Bromomethane
Concen: 0.233 ug/l
RT: 2.869 min Scan# 11
Delta R.T. 0.023 min
Lab File: VN071774.D
Acq: 02 Apr 2022 00:34




Instrument :
MSVOA_N
ClientSampleId :
MW-8


Tgt Ion: 94 Resp: 891
Ion Ratio Lower Upper
94 100
96 66.3 76.0 114.0#

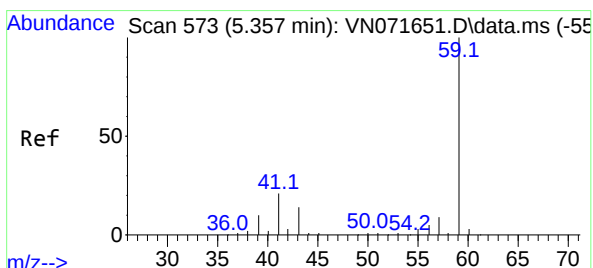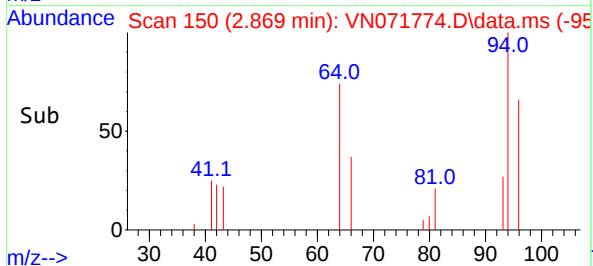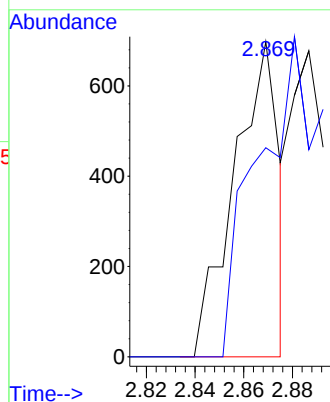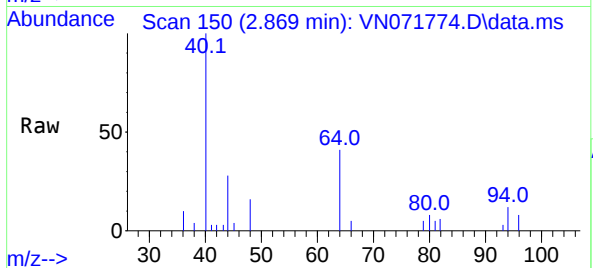

#11
Tert butyl alcohol
Concen: 0.970 ug/l
RT: 5.375 min Scan# 576
Delta R.T. 0.018 min
Lab File: VN071774.D
Acq: 02 Apr 2022 00:34

Tgt Ion: 59 Resp: 956
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#


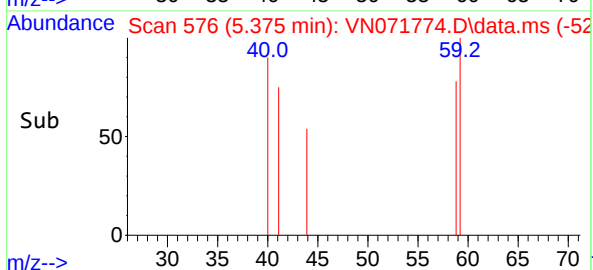

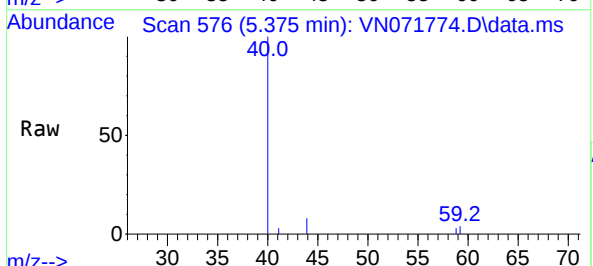




#13
Acrolein
Concen: 0.732 ug/l
RT: 4.057 min Scan# 31
Delta R.T. 0.017 min
Lab File: VN071774.D
Acq: 02 Apr 2022 00:34




Instrument :
MSVOA_N
ClientSampleId :
MW-8


Tgt Ion: 56 Resp: 880
Ion Ratio Lower Upper
56 100
55 89.1 54.8 82.2#

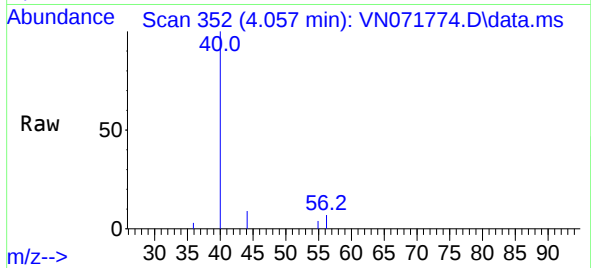

#15
Acrylonitrile
Concen: 0.276 ug/l
RT: 5.569 min Scan# 609
Delta R.T. 0.023 min
Lab File: VN071774.D
Acq: 02 Apr 2022 00:34

Tgt Ion: 53 Resp: 791
Ion Ratio Lower Upper
53 100
52 0.0 66.4 99.6#
51 29.2 28.5 42.7


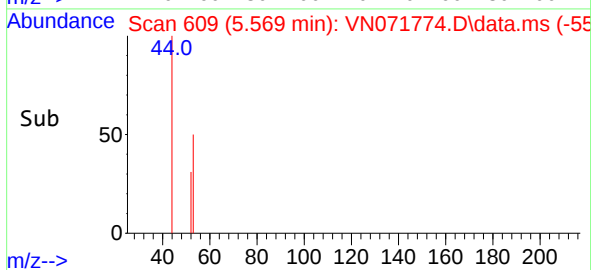

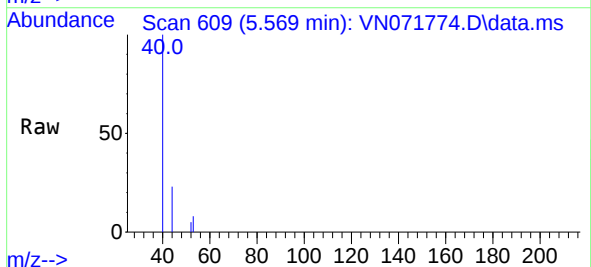




#16
Acetone
Concen: 3.668 ug/l
RT: 4.310 min Scan# 395
Delta R.T. 0.035 min
Lab File: VN071774.D
Acq: 02 Apr 2022 00:34




Instrument :
MSVOA_N
ClientSampleId :
MW-8


Tgt Ion: 43 Resp: 9525
Ion Ratio Lower Upper
43 100
58 14.6 26.0 39.0#



#17
Carbon Disulfide
Concen: 0.348 ug/l
RT: 4.545 min Scan# 435
Delta R.T. 0.011 min
Lab File: VN071774.D
Acq: 02 Apr 2022 00:34

Tgt Ion: 76 Resp: 3507
Ion Ratio Lower Upper
76 100
78 15.7 7.2 10.8#


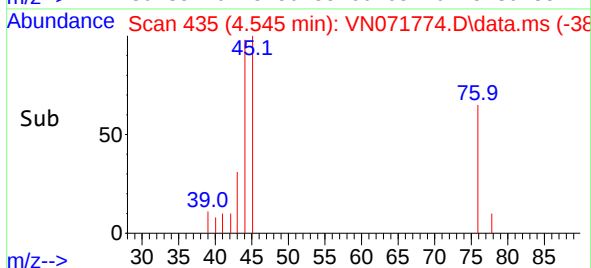
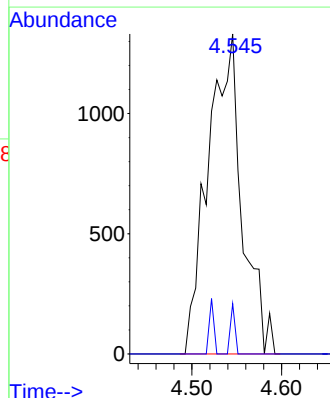





#18
Methyl Acetate
Concen: Below Cal
RT: 4.851 min Scan# 41
Delta R.T. 0.005 min
Lab File: VN071774.D
Acq: 02 Apr 2022 00:34




Instrument :
MSVOA_N
ClientSampleId :
MW-8


Tgt Ion: 43 Resp: 1040
Ion Ratio Lower Upper
43 100
74 7.0 21.6 32.4#



#25
2-Butanone
Concen: 0.432 ug/l
RT: 7.345 min Scan# 911
Delta R.T. 0.017 min
Lab File: VN071774.D
Acq: 02 Apr 2022 00:34

Tgt Ion: 43 Resp: 1617
Ion Ratio Lower Upper
43 100
72 25.4 23.7 35.5

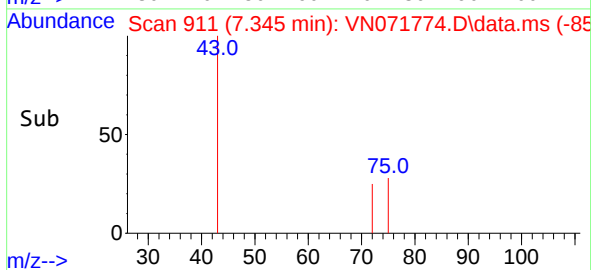



#29

Tetrahydrofuran

Concen: 6.895 ug/l

RT: 7.692 min Scan# 91

Delta R.T. 0.017 min

Lab File: VN071774.D

Acq: 02 Apr 2022 00:34

Instrument :

MSVOA_N

ClientSampleId :

MW-8





Tgt Ion: 42 Resp: 16713

Ion Ratio Lower Upper

42 100

72 50.2 39.7 59.5

71 49.7 36.6 55.0

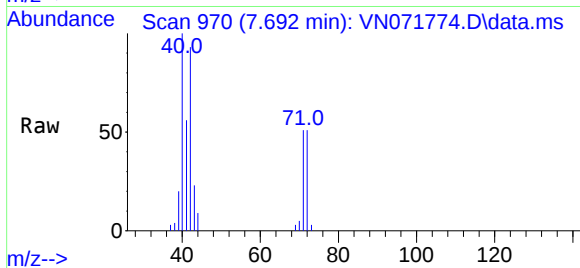

#30

Chloroform

Concen: 0.288 ug/l

RT: 7.816 min Scan# 991

Delta R.T. 0.006 min

Lab File: VN071774.D




Acq: 02 Apr 2022 00:34


Tgt Ion: 83 Resp: 2771

Ion Ratio Lower Upper

83 100

85 72.0 51.8 77.8

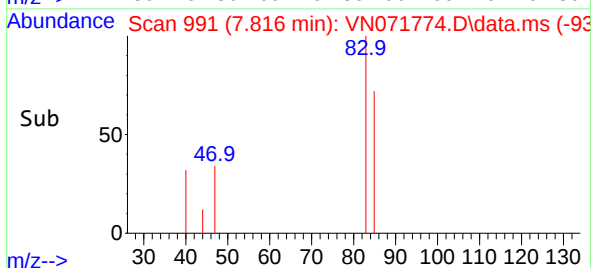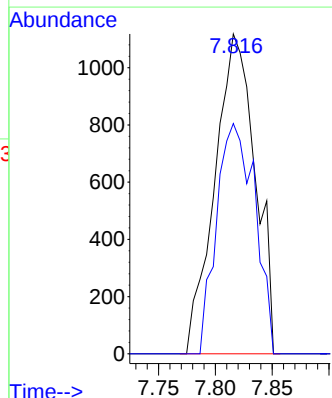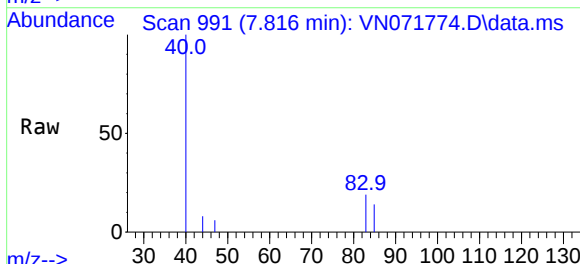

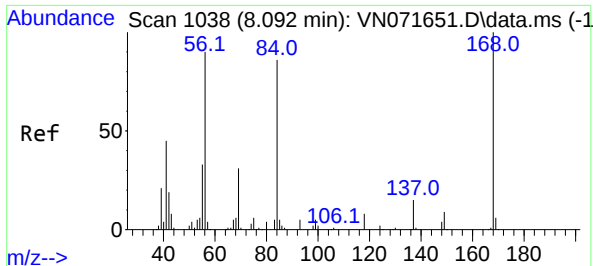

#31

Cyclohexane

Concen: 1.151 ug/l

RT: 8.081 min Scan# 1

Delta R.T. -0.011 min

Lab File: VN071774.D

Acq: 02 Apr 2022 00:34

Instrument :

MSVOA_N

ClientSampleId :

MW-8





Tgt Ion: 56 Resp: 9507

Ion Ratio Lower Upper

56 100

69 148.0 27.8 41.8#

84 143.9 76.9 115.3#

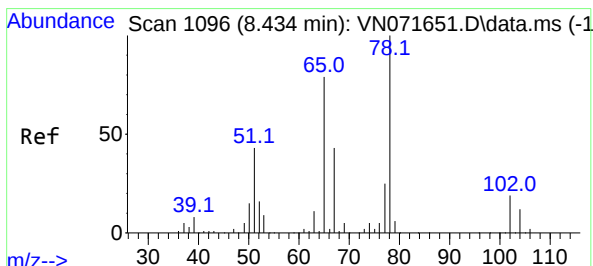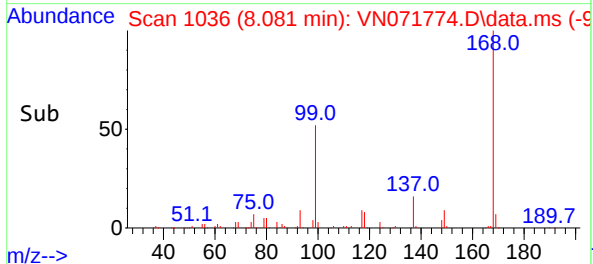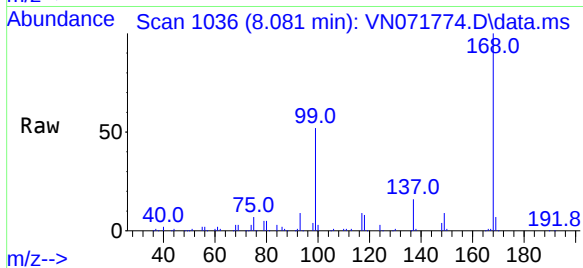

#33

1,2-Dichloroethane-d4

Concen: 50.624 ug/l

RT: 8.433 min Scan# 1096

Delta R.T. -0.001 min

Lab File: VN071774.D




Acq: 02 Apr 2022 00:34


Tgt Ion: 65 Resp: 307594

Ion Ratio Lower Upper

65 100

67 52.3 0.0 104.8


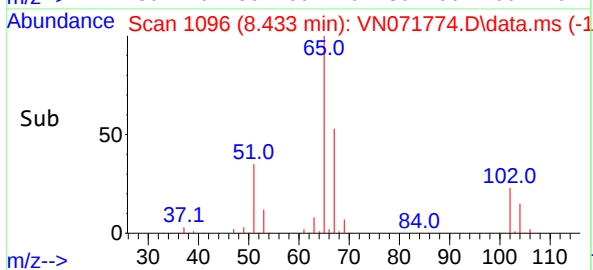

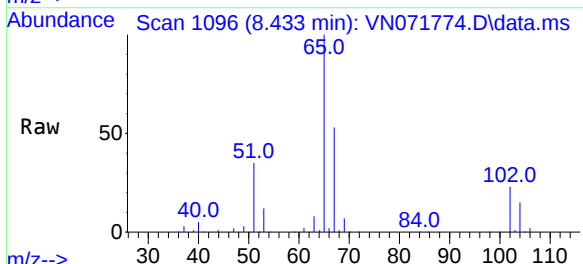


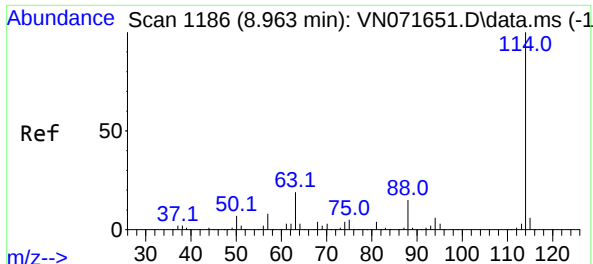

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.963 min Scan# 1186
Delta R.T. -0.000 min
Lab File: VN071774.D
Acq: 02 Apr 2022 00:34




Instrument :
MSVOA_N
ClientSampleId :
MW-8


Tgt Ion:114 Resp: 907296
Ion Ratio Lower Upper
114 100
63 19.1 0.0 40.0
88 15.3 0.0 32.6

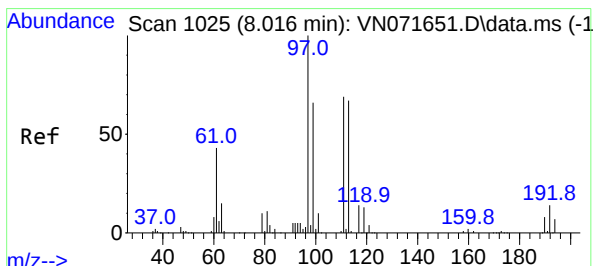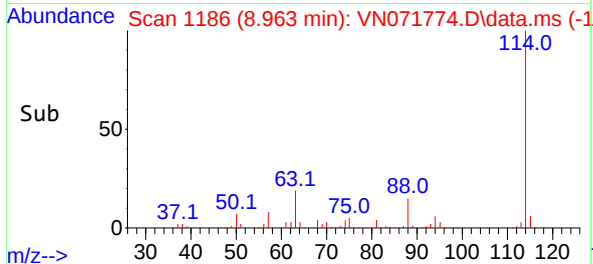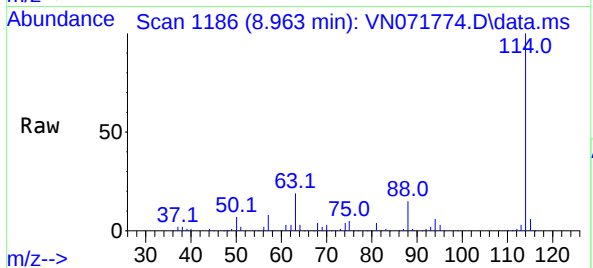

#35
Dibromofluoromethane
Concen: 48.145 ug/l
RT: 8.022 min Scan# 1026
Delta R.T. 0.006 min
Lab File: VN071774.D
Acq: 02 Apr 2022 00:34

Tgt Ion:113 Resp: 257040
Ion Ratio Lower Upper
113 100
111 102.9 81.4 122.0
192 22.1 17.0 25.6


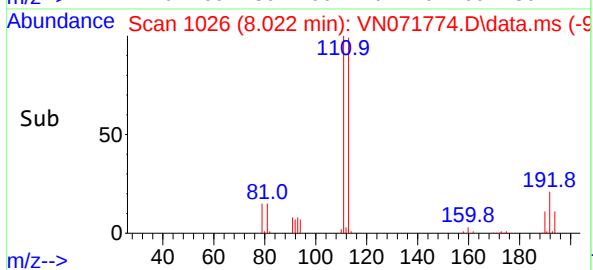

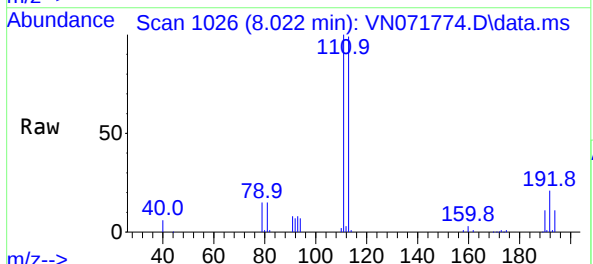


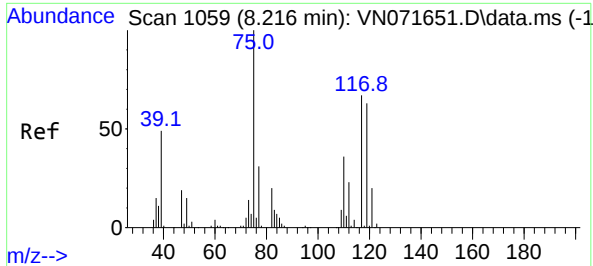

#36
1,1-Dichloropropene
Concen: 5.074 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. -0.135 min
Lab File: VN071774.D
Acq: 02 Apr 2022 00:34




Instrument :
MSVOA_N
ClientSampleId :
MW-8


Tgt Ion: 75 Resp: 37832
Ion Ratio Lower Upper
75 100
110 9.5 18.3 54.8#
77 0.0 25.1 37.7#

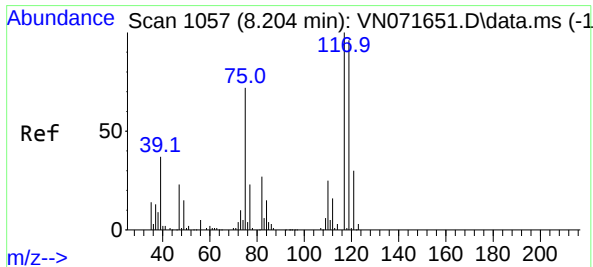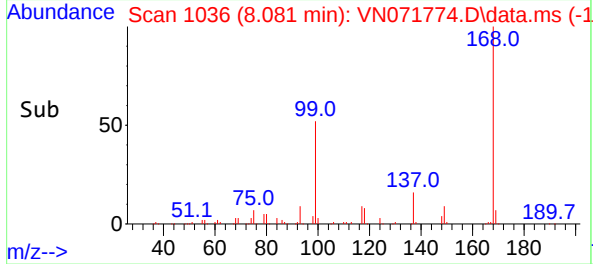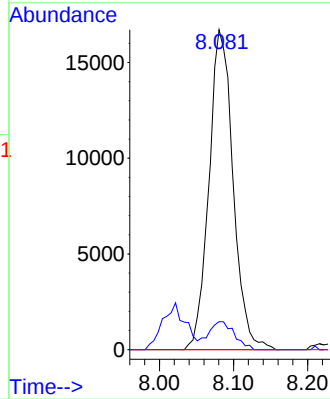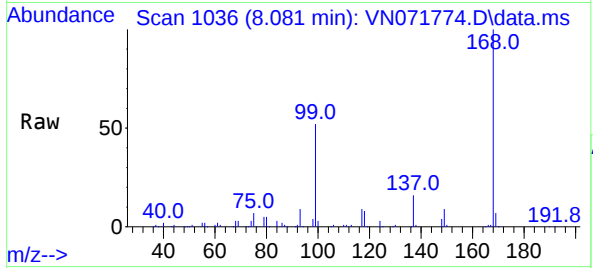

#38
Carbon Tetrachloride
Concen: 6.600 ug/l
RT: 8.086 min Scan# 1037
Delta R.T. -0.118 min
Lab File: VN071774.D
Acq: 02 Apr 2022 00:34

Tgt Ion: 117 Resp: 48223
Ion Ratio Lower Upper
117 100
119 5.9 75.8 113.8#
121 0.0 24.6 37.0#

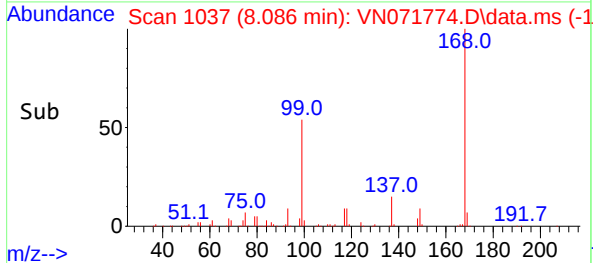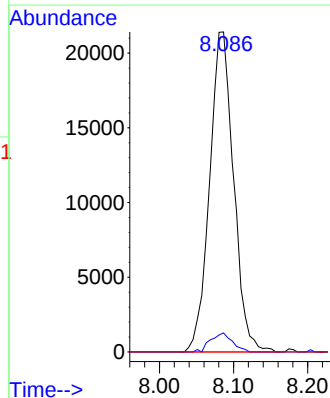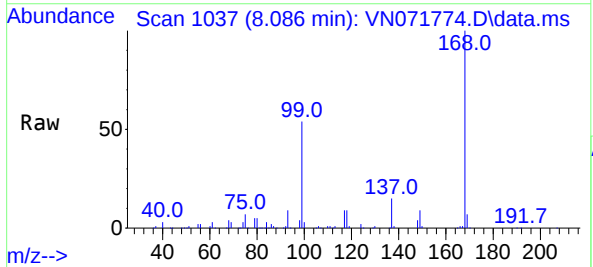







#41
Methacrylonitrile
Concen: 2.702 ug/l
RT: 7.698 min Scan# 91
Delta R.T. 0.070 min
Lab File: VN071774.D
Acq: 02 Apr 2022 00:34

Instrument :
MSVOA_N
ClientSampleId :
MW-8

Tgt Ion: 41 Resp: 10798




Ion	Ratio	Lower	Upper
41	100		
39	41.9	48.6	73.0#
67	0.0	73.4	110.2#
52	0.0	27.7	41.5#

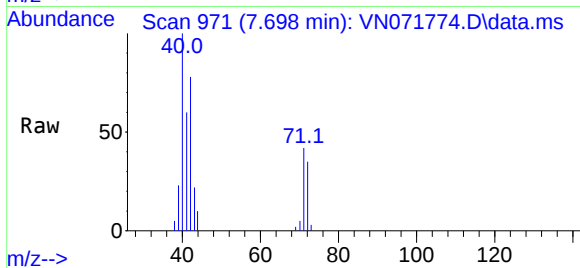


#49
1,4-Dioxane
Concen: Below Cal
RT: 9.575 min Scan# 1290
Delta R.T. 0.012 min
Lab File: VN071774.D
Acq: 02 Apr 2022 00:34

Tgt Ion: 88 Resp: 57

Ion	Ratio	Lower	Upper
88	100		
43	0.0	20.2	30.4#
58	0.0	54.2	81.4#


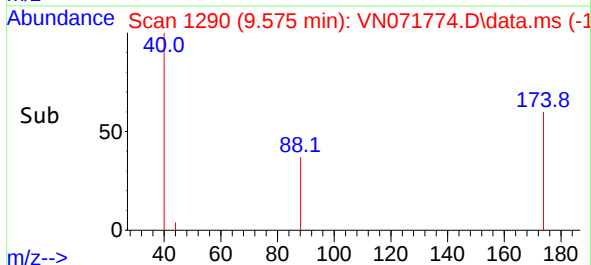
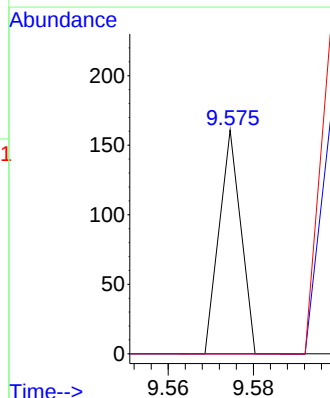
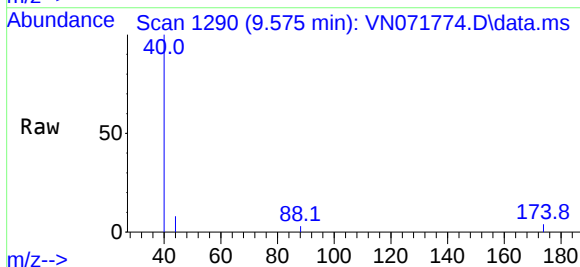




#50
Toluene-d8
Concen: 51.650 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. 0.000 min
Lab File: VN071774.D
Acq: 02 Apr 2022 00:34




Instrument :
MSVOA_N
ClientSampleId :
MW-8


Tgt Ion: 98 Resp: 1128045
Ion Ratio Lower Upper
98 100
100 65.3 52.6 78.8

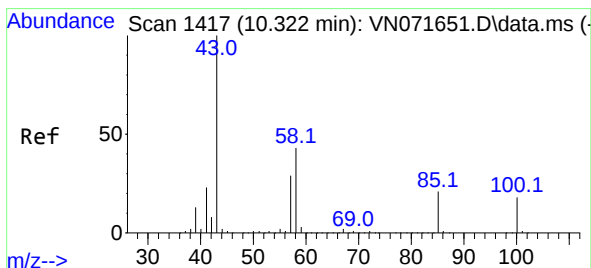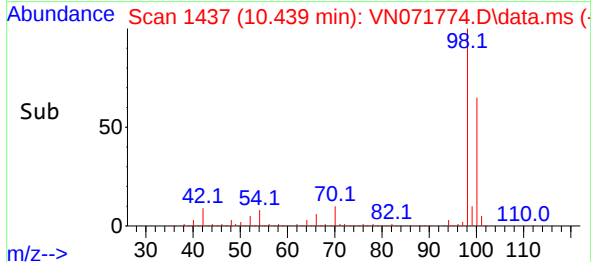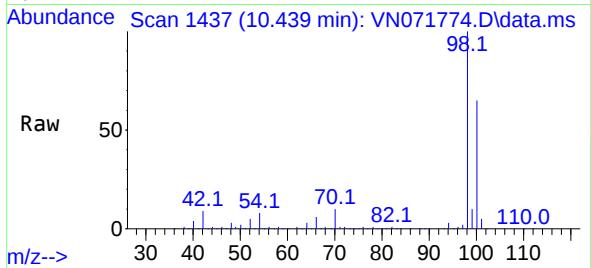

#51
4-Methyl-2-Pentanone
Concen: 0.471 ug/l
RT: 10.333 min Scan# 1419
Delta R.T. 0.011 min
Lab File: VN071774.D
Acq: 02 Apr 2022 00:34

Tgt Ion: 43 Resp: 3672
Ion Ratio Lower Upper
43 100
58 27.5 34.1 51.1#

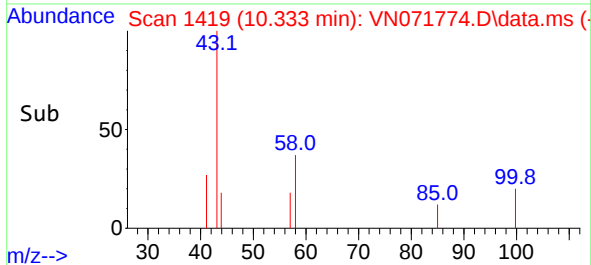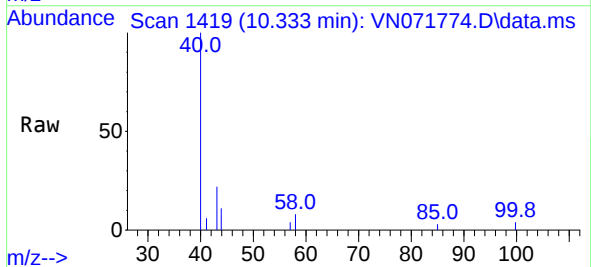



#59

2-Hexanone

Concen: 1.019 ug/l

RT: 11.092 min Scan# 11

Delta R.T. 0.011 min

Lab File: VN071774.D

Acq: 02 Apr 2022 00:34

Instrument :

MSVOA_N

ClientSampleId :





MW-8

Tgt Ion: 43 Resp: 5597

Ion Ratio Lower Upper

43 100

58 54.1 29.7 89.1

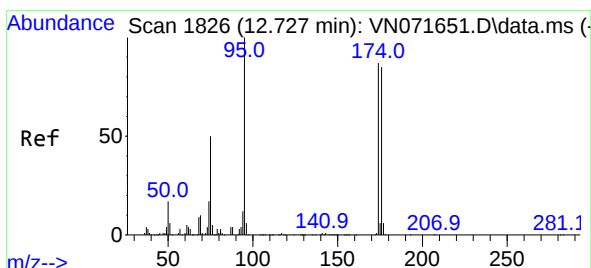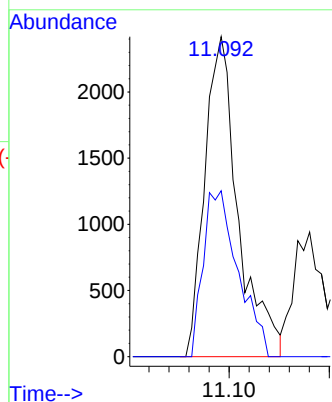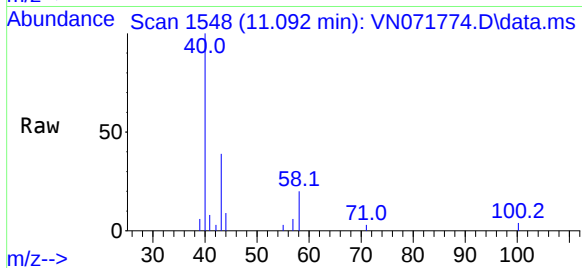

#62

4-Bromofluorobenzene

Concen: 48.325 ug/l

RT: 12.727 min Scan# 1826

Delta R.T. 0.000 min

Lab File: VN071774.D

Acq: 02 Apr 2022 00:34




Tgt Ion: 95 Resp: 341343


Ion Ratio Lower Upper

95 100

174 85.8 0.0 167.6

176 81.9 0.0 163.4


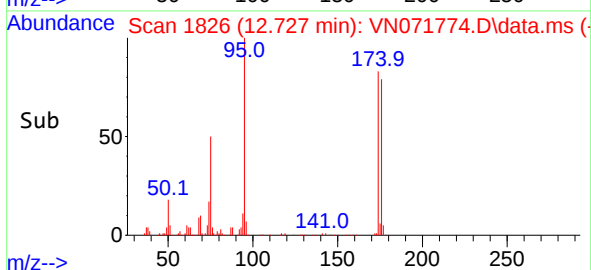

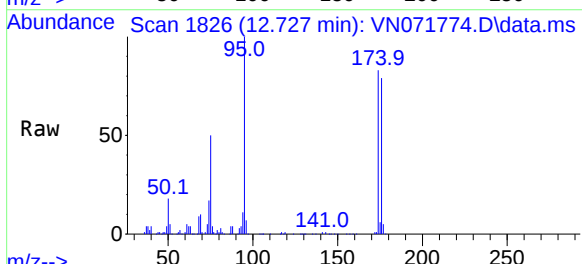




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.745 min Scan# 117
Delta R.T. 0.006 min
Lab File: VN071774.D
Acq: 02 Apr 2022 00:34




Instrument :
MSVOA_N
ClientSampleId :
MW-8


Tgt Ion:117 Resp: 891452
Ion Ratio Lower Upper
117 100
82 53.7 44.2 66.2
119 31.6 25.4 38.0

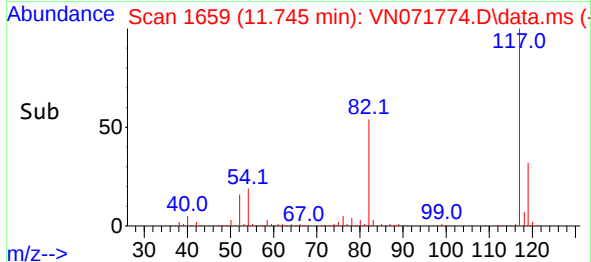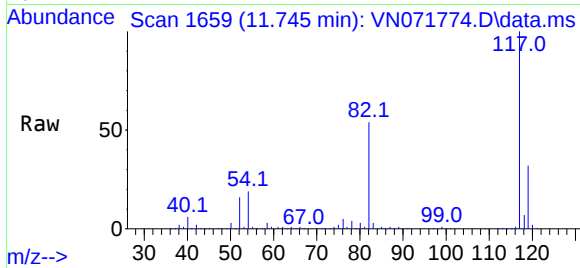

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.674 min Scan# 1987
Delta R.T. 0.005 min
Lab File: VN071774.D
Acq: 02 Apr 2022 00:34

Tgt Ion:152 Resp: 296751
Ion Ratio Lower Upper
152 100
115 57.1 28.9 86.7
150 160.0 0.0 356.2

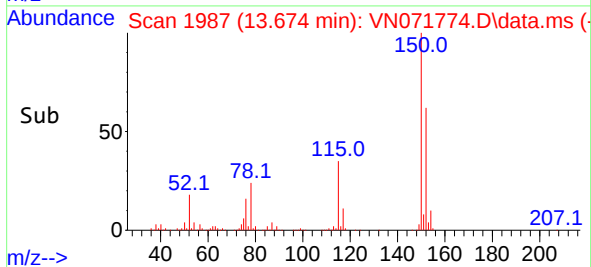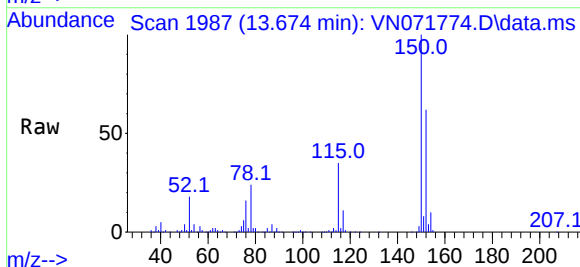







#74
N-amy1 acetate
Concen: 0.439 ug/l
RT: 12.392 min Scan# 11
Delta R.T. 0.012 min
Lab File: VN071774.D
Acq: 02 Apr 2022 00:34

Instrument :
MSVOA_N
ClientSampleId :
MW-8

Tgt Ion: 43 Resp: 3148




Ion	Ratio	Lower	Upper
43	100		
70	37.4	39.0	58.4#
55	24.8	21.1	31.7
61	16.8	21.1	31.7#

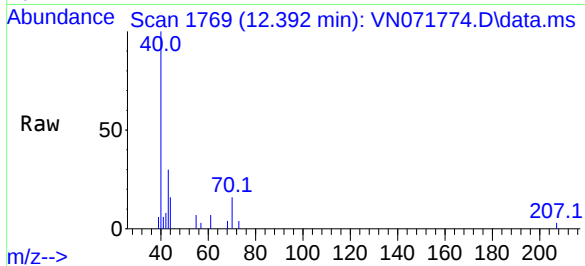


#76
1,2,3-Trichloropropane
Concen: 24.646 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. -0.147 min
Lab File: VN071774.D
Acq: 02 Apr 2022 00:34

Tgt Ion: 75 Resp: 169425

Ion	Ratio	Lower	Upper
75	100		
77	1.1	98.5	295.5#


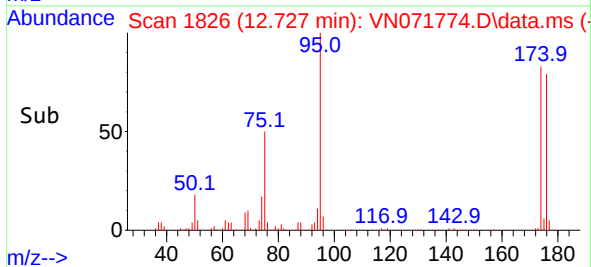

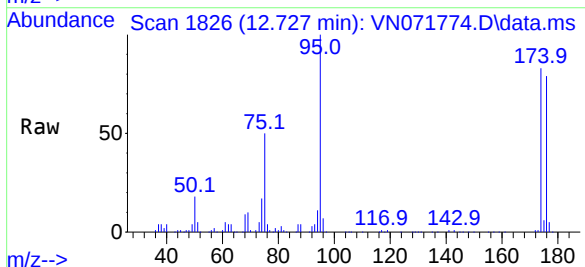




#81
trans-1,4-Dichloro-2-butene
Concen: 76.376 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.105 min
Lab File: VN071774.D
Acq: 02 Apr 2022 00:34




Instrument :
MSVOA_N
ClientSampleId :
MW-8


Tgt Ion: 75 Resp: 169425
Ion Ratio Lower Upper
75 100
53 0.0 78.0 117.0#
89 0.0 37.2 55.8#

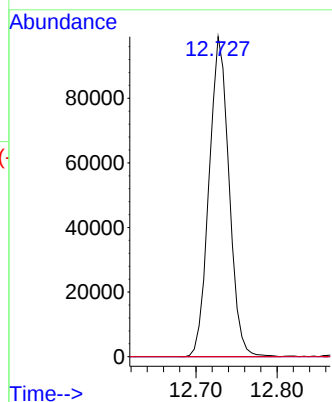

#82
4-Chlorotoluene
Concen: 0.215 ug/l
RT: 13.104 min Scan# 1890
Delta R.T. 0.006 min
Lab File: VN071774.D
Acq: 02 Apr 2022 00:34

Tgt Ion: 91 Resp: 3355
Ion Ratio Lower Upper
91 100
126 28.0 17.2 51.6

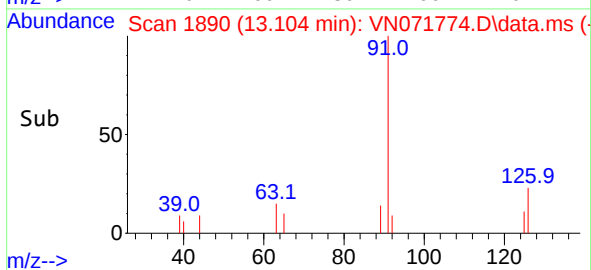



#87

1,3-Dichlorobenzene

Concen: 0.266 ug/l

RT: 13.610 min Scan# 1976

Delta R.T. -0.000 min

Lab File: VN071774.D

Acq: 02 Apr 2022 00:34

Instrument :

MSVOA_N

ClientSampleId :

MW-8





Tgt Ion:146 Resp: 2661

Ion Ratio Lower Upper

146 100

111 35.2 20.0 60.0

148 58.5 32.0 96.0

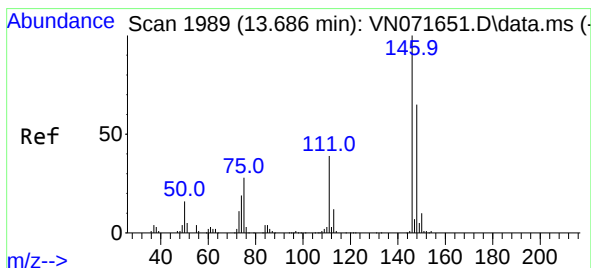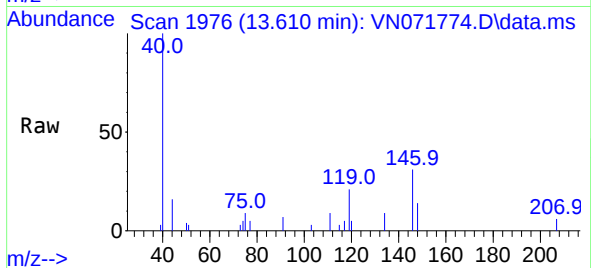

#88

1,4-Dichlorobenzene

Concen: 0.273 ug/l

RT: 13.610 min Scan# 1976

Delta R.T. -0.076 min

Lab File: VN071774.D

Acq: 02 Apr 2022 00:34




Tgt Ion:146 Resp: 2661


Ion Ratio Lower Upper

146 100

111 35.2 19.1 57.1

148 58.5 31.4 94.3


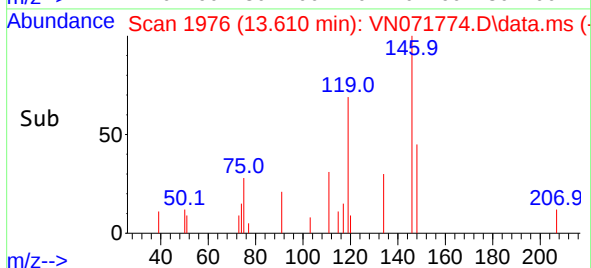

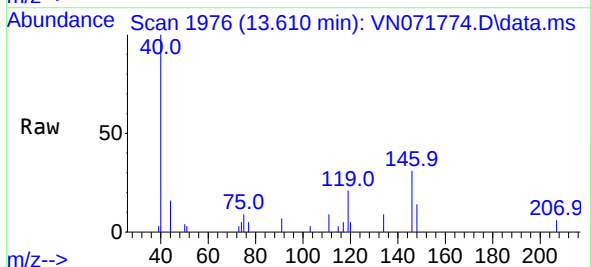




#89
n-Butylbenzene
Concen: 0.343 ug/l
RT: 13.939 min Scan# 2032
Delta R.T. -0.000 min
Lab File: VN071774.D
Acq: 02 Apr 2022 00:34




Instrument :
MSVOA_N
ClientSampleId :
MW-8


Tgt Ion:	91	Resp:	4758
Ion	Ratio	Lower	Upper
91	100		
92	42.9	26.9	80.7
134	25.5	13.6	40.8



#91
1,2-Dichlorobenzene
Concen: 0.300 ug/l
RT: 13.980 min Scan# 2039
Delta R.T. 0.000 min
Lab File: VN071774.D
Acq: 02 Apr 2022 00:34

Tgt Ion:	146	Resp:	2939
Ion	Ratio	Lower	Upper
146	100		
111	37.4	20.9	62.8
148	57.4	32.1	96.3


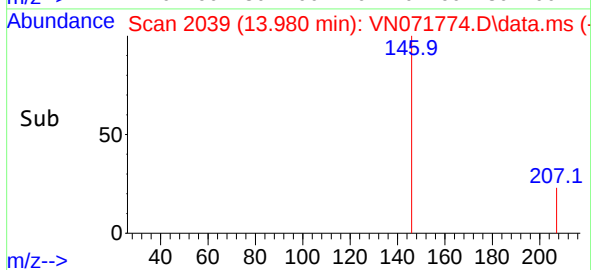




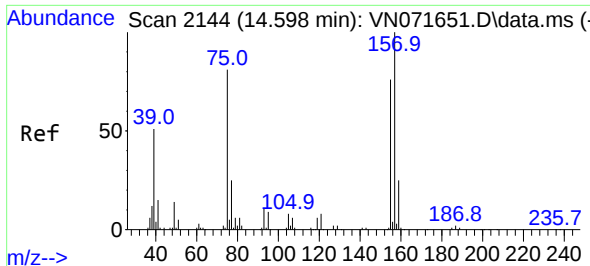

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.260 ug/l
RT: 14.598 min Scan# 2144
Delta R.T. -0.000 min
Lab File: VN071774.D
Acq: 02 Apr 2022 00:34




Instrument :
MSVOA_N
ClientSampleId :
MW-8


Tgt Ion: 75 Resp: 337
Ion Ratio Lower Upper
75 100
155 37.7 44.9 134.5#
157 113.4 59.0 176.8

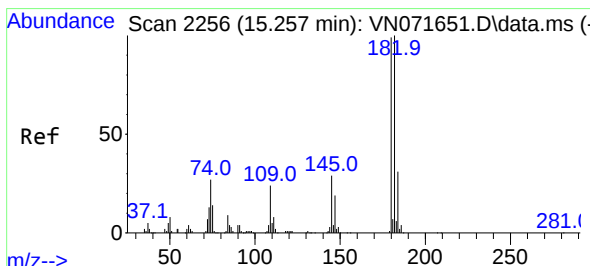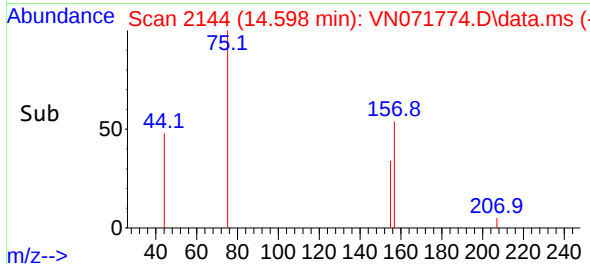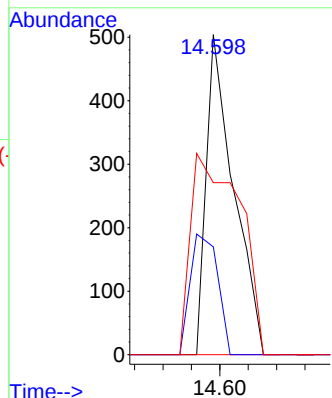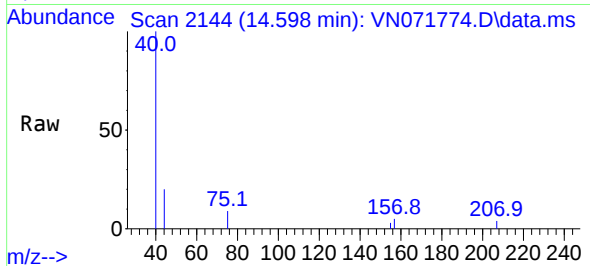

#93
1,2,4-Trichlorobenzene
Concen: 2.651 ug/l
RT: 15.262 min Scan# 2257
Delta R.T. 0.005 min
Lab File: VN071774.D
Acq: 02 Apr 2022 00:34

Tgt Ion: 180 Resp: 2785
Ion Ratio Lower Upper
180 100
182 97.9 47.5 142.5
145 31.0 14.5 43.5


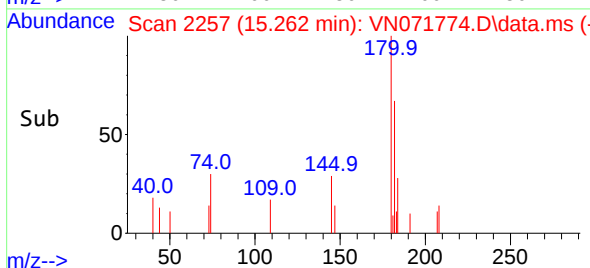
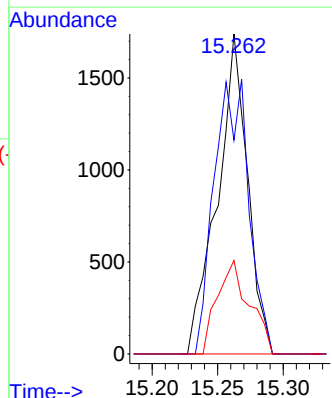
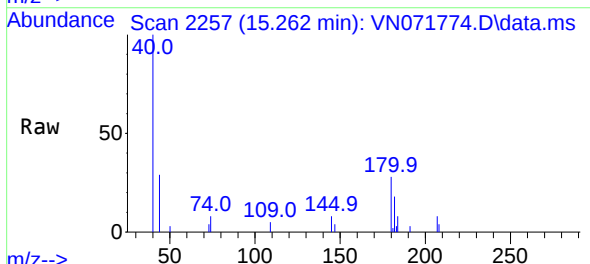


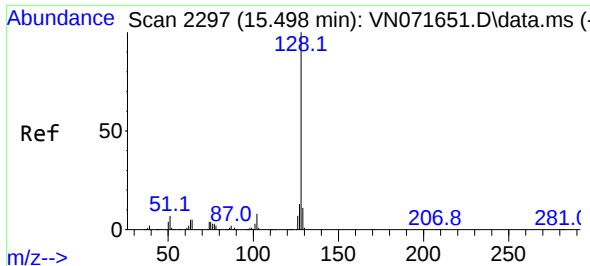

#95
Naphthalene
Concen: 4.424 ug/l
RT: 15.504 min Scan# 21
Delta R.T. 0.006 min
Lab File: VN071774.D
Acq: 02 Apr 2022 00:34

Instrument :
MSVOA_N
ClientSampleId :
MW-8

Tgt Ion:128	Resp:	9091
Ion Ratio	Lower	Upper
128	100	
127	13.4	10.3 15.5
129	8.6	8.6 13.0#

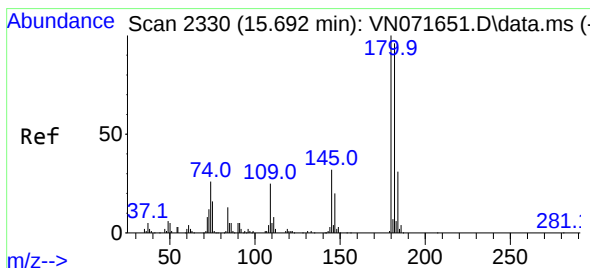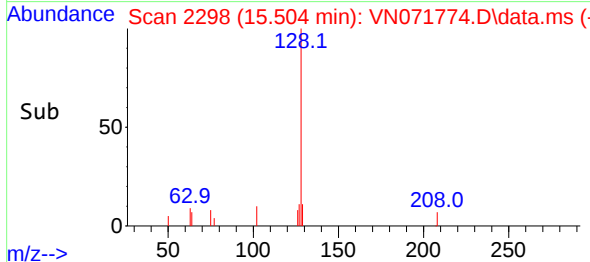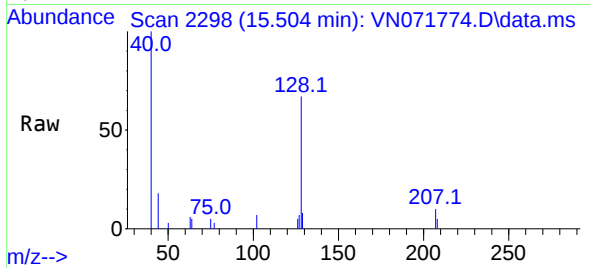

#96
1,2,3-Trichlorobenzene
Concen: 3.167 ug/l
RT: 15.698 min Scan# 2331
Delta R.T. 0.006 min
Lab File: VN071774.D
Acq: 02 Apr 2022 00:34

Tgt Ion:180	Resp:	3619
Ion Ratio	Lower	Upper
180	100	
182	89.2	47.8 143.3
145	27.4	15.5 46.5

