

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN040122\
 Data File : VN071752.D
 Acq On : 01 Apr 2022 14:55
 Operator : JC\MD
 Sample : N2075-10
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-178S-20220322

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M

Title : SW846 8260

Signal : TIC: VN071752.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.240	36	43	44	rBV2	24579	36464	1.11%	0.221%
2	4.575	426	440	453	rBV	26937	97801	2.97%	0.594%
3	5.616	606	617	629	rBV3	16483	55276	1.68%	0.336%
4	8.022	1015	1026	1031	rBV	397169	974120	29.59%	5.916%
5	8.087	1031	1037	1054	rVB	735500	1690888	51.37%	10.270%
6	8.434	1086	1096	1110	rBV	415017	958284	29.11%	5.820%
7	8.969	1176	1187	1207	rBV	1106164	2314630	70.32%	14.058%
8	10.439	1428	1437	1458	rBV	1765867	3291792	100.00%	19.993%
9	11.739	1650	1658	1676	rBV	1679111	2973210	90.32%	18.058%
10	12.727	1818	1826	1837	rBV	1166219	2004575	60.90%	12.175%
11	13.674	1979	1987	1999	rBV	1217349	2067833	62.82%	12.559%




Sum of corrected areas: 16464873

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN040122\
Data File : VN071752.D
Acq On : 01 Apr 2022 14:55
Operator : JC\MD
Sample : N2075-10
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-178S-20220322

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

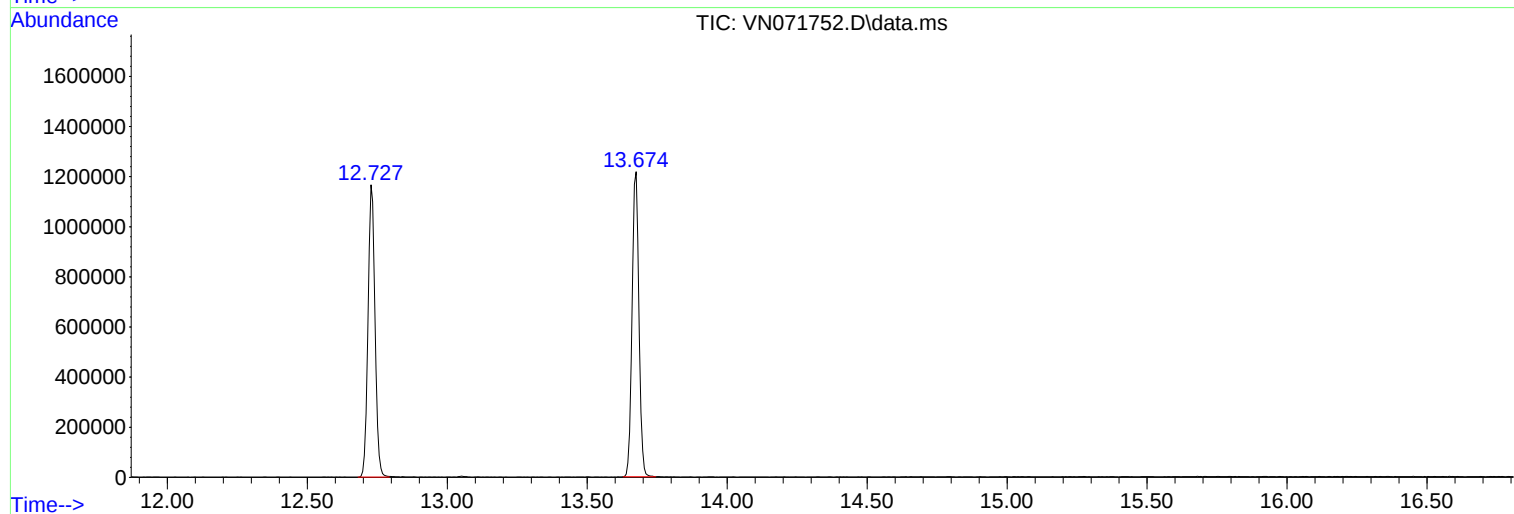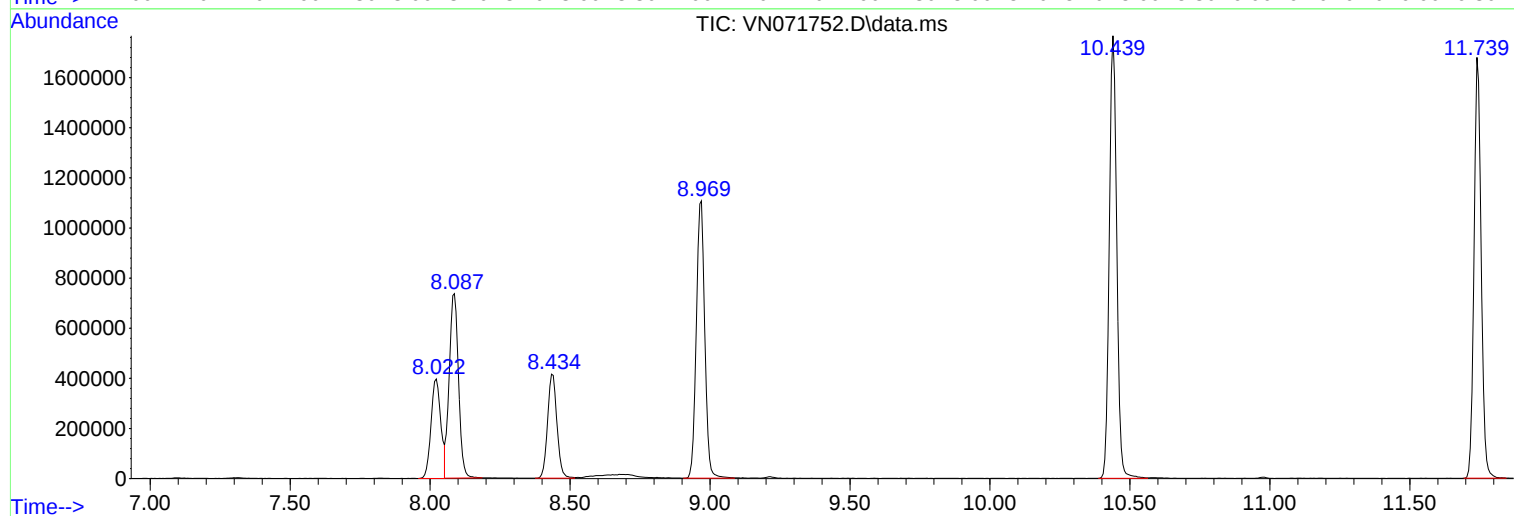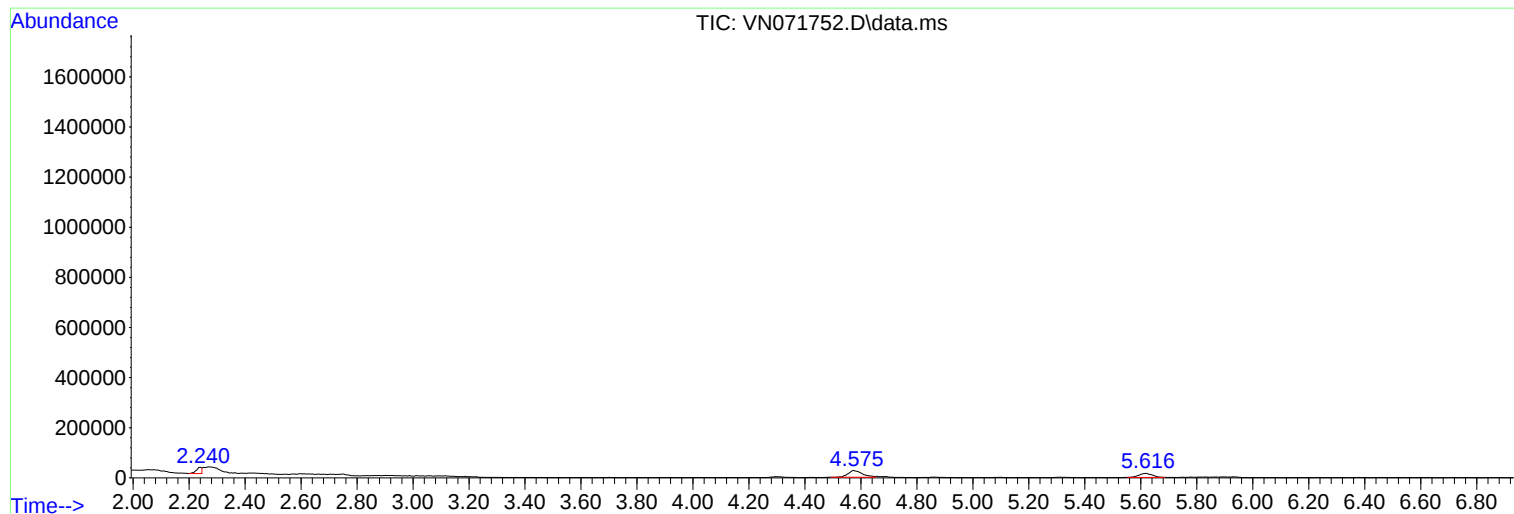

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN040122\
Data File : VN071752.D
Acq On : 01 Apr 2022 14:55
Operator : JC\MD
Sample : N2075-10
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-178S-20220322

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN040122\
Data File : VN071752.D
Acq On : 01 Apr 2022 14:55
Operator : JC\MD
Sample : N2075-10
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-178S-20220322

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc