
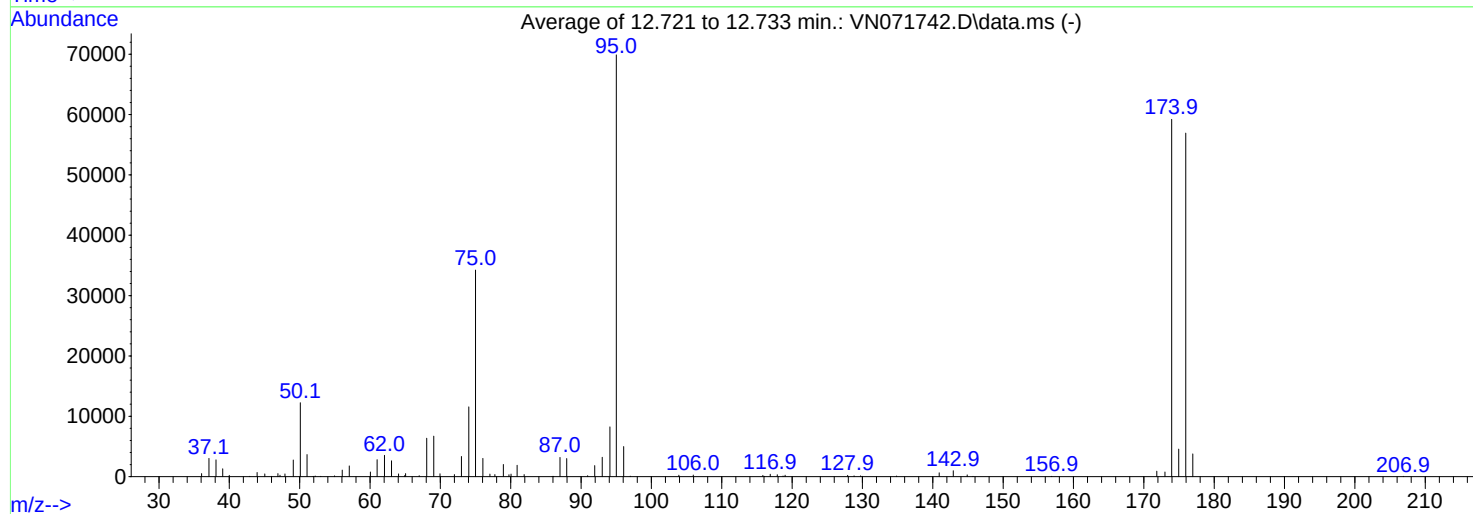


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN040122\
Data File : VN071742.D
Acq On : 01 Apr 2022 09:48
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
Title : SW846 8260
Last Update : Thu Mar 31 01:57:54 2022

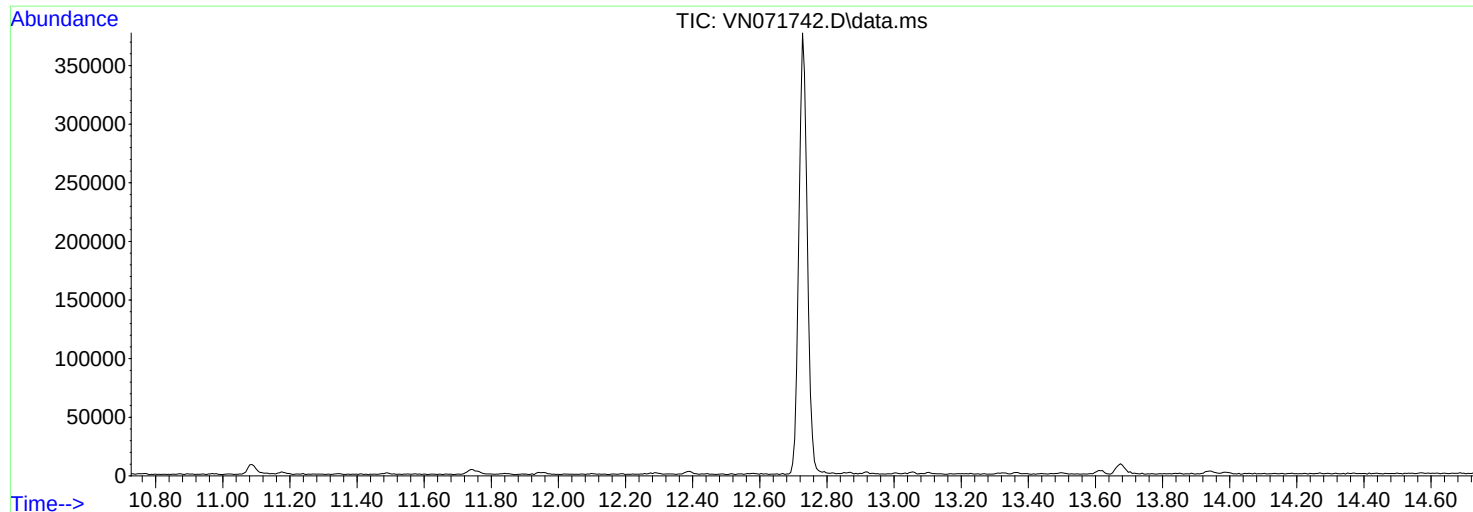

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1817

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	12258	PASS
75	95	30	60	49.0	34235	PASS
95	95	100	100	100.0	69899	PASS
96	95	5	9	7.1	4978	PASS
173	174	0.00	2	1.3	765	PASS
174	95	50	100	84.7	59219	PASS
175	174	5	9	7.7	4556	PASS
176	174	95	101	96.1	56923	PASS
177	176	5	9	6.6	3777	PASS