
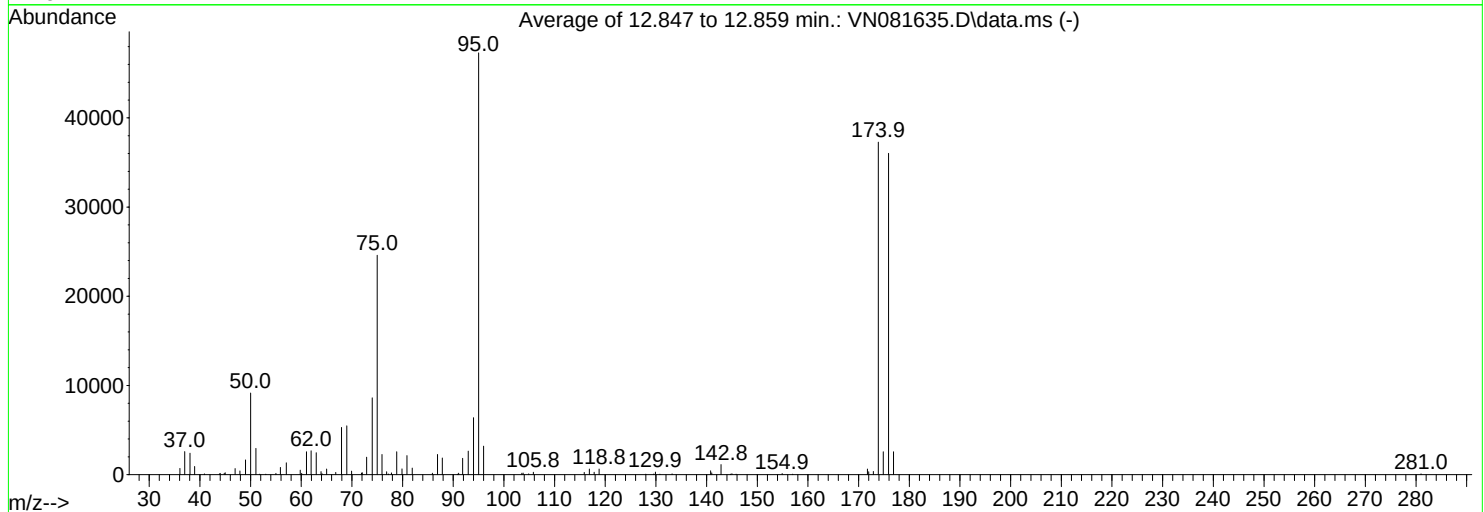


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN040124\
Data File : VN081635.D
Acq On : 01 Apr 2024 08:40
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031824W.M
Title : SW846 8260
Last Update : Tue Mar 19 06:00:00 2024

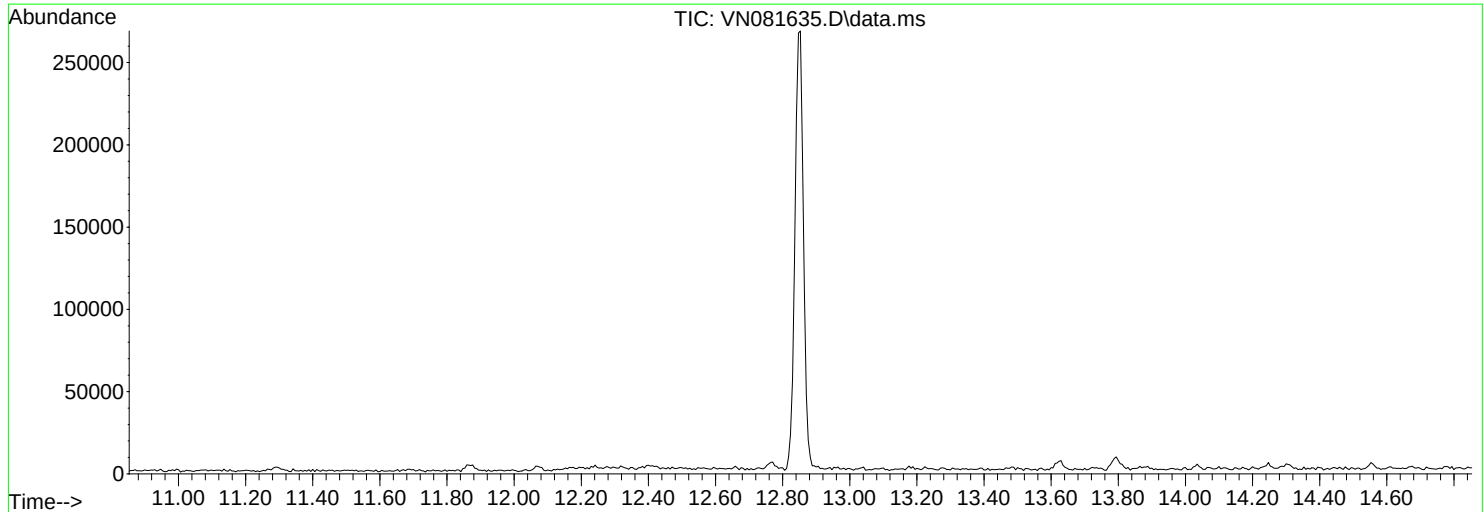

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.4	9155	PASS
75	95	30	60	52.0	24600	PASS
95	95	100	100	100.0	47296	PASS
96	95	5	9	6.8	3194	PASS
173	174	0.00	2	0.9	352	PASS
174	95	50	100	78.8	37277	PASS
175	174	5	9	6.9	2570	PASS
176	174	95	101	96.6	36019	PASS
177	176	5	9	7.1	2570	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	702	49.00	1657	61.95	2680	72.90	1961
37.00	2580	50.00	9155	62.95	2463	74.00	861
38.05	2400	51.05	2943	63.90	338	75.00	2460
38.95	914	51.80	51	64.10	113	75.95	226
40.90	97	53.00	52	65.00	622	76.85	322
43.85	85	55.00	139	66.80	260	77.20	72
44.00	136	55.90	815	67.95	5295	77.80	202
44.80	147	57.05	1329	69.00	5476	78.85	2558
45.00	223	59.80	511	69.95	401	79.90	652
46.95	686	60.10	141	71.90	175	80.85	2137
47.90	419	61.05	2574	72.05	215	81.90	738

Average of 12.847 to 12.859 min.: VN081635.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
85.90	170	103.80	189	133.20	84	172.90	352
86.90	2260	104.90	97	140.80	434	173.90	37277
87.85	1865	105.80	275	141.00	190	174.85	2570
90.80	62	115.85	259	142.85	1132	175.90	36019
91.05	161	116.85	624	144.70	56	176.90	2570
91.85	1825	117.80	262	145.00	100	281.00	91
92.95	2630	118.80	625	145.80	57		
94.00	6394	128.00	56	154.90	126		
95.00	47296	129.60	73	157.00	59		
96.00	3194	129.90	293	171.75	628		
103.55	158	130.80	60	172.00	331		

Instrument :

MSVOA_N

ClientSampleId :

BFB