
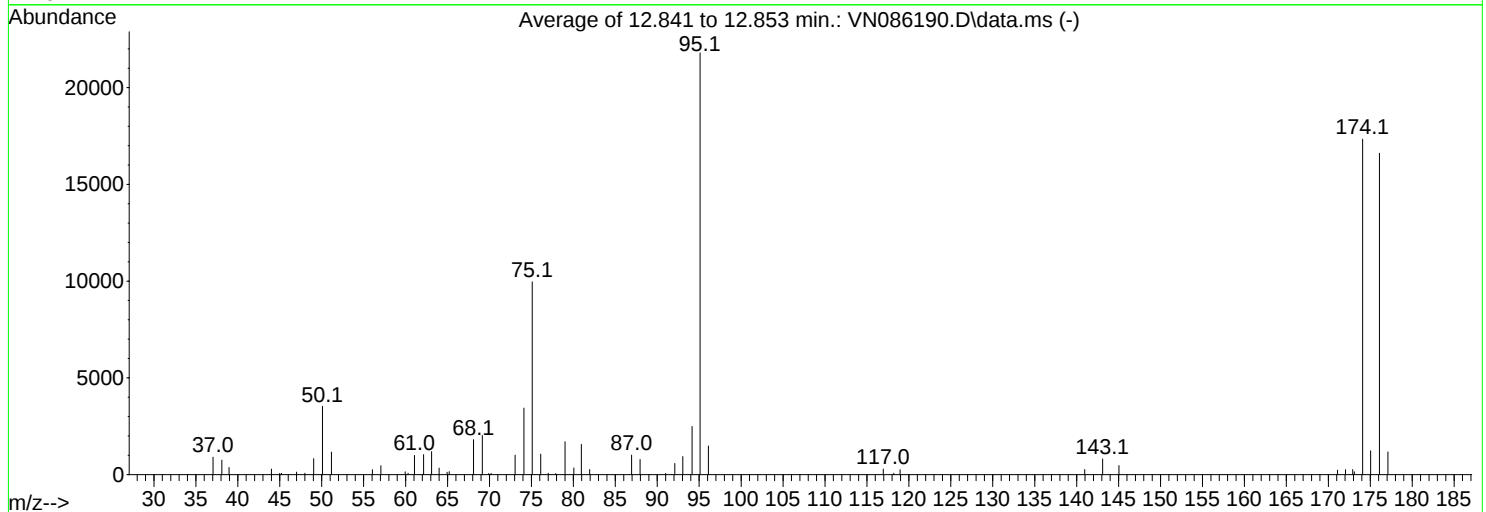


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN040125\  
Data File : VN086190.D  
Acq On : 01 Apr 2025 11:41  
Operator : JC\MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N031825W.M  
Title : SW846 8260  
Last Update : Wed Mar 19 03:20:56 2025

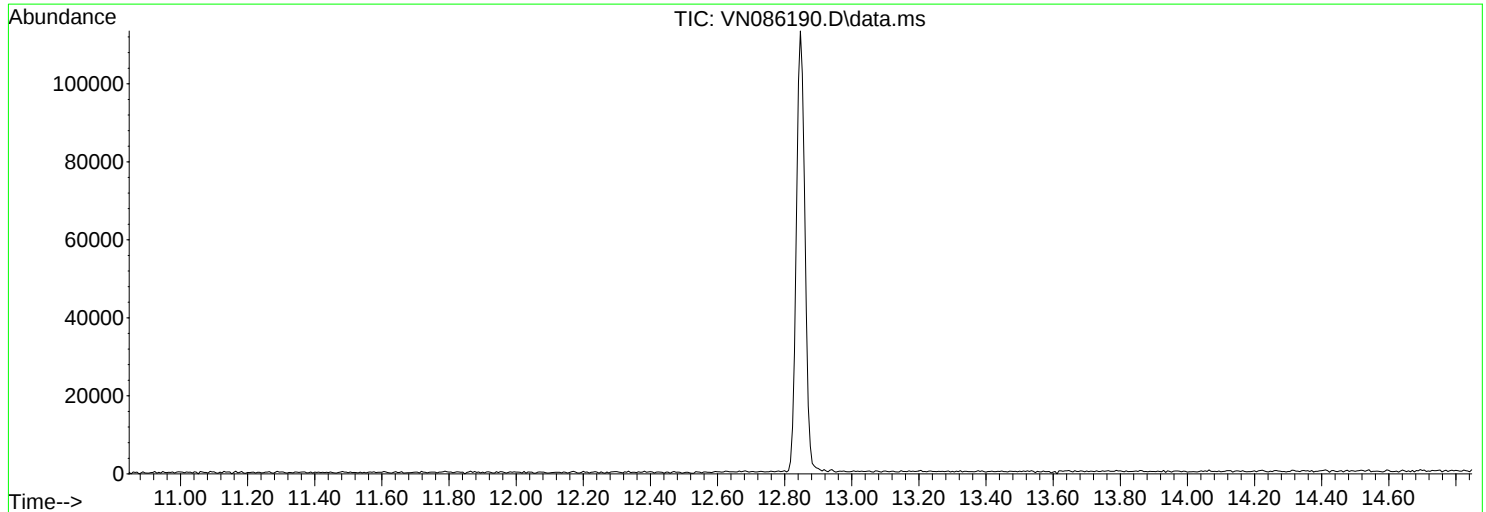

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 16.2         | 3530       | PASS                |
| 75             | 95              | 30              | 60              | 45.7         | 9962       | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 21795      | PASS                |
| 96             | 95              | 5               | 9               | 6.8          | 1483       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.5          | 263        | PASS                |
| 174            | 95              | 50              | 100             | 79.6         | 17338      | PASS                |
| 175            | 174             | 5               | 9               | 7.1          | 1235       | PASS                |
| 176            | 174             | 95              | 101             | 95.8         | 16612      | PASS                |
| 177            | 176             | 5               | 9               | 7.1          | 1174       | PASS                |

BFB

Modified:subtracted

| m/z   | abund. | m/z   | abund. | m/z   | abund. | m/z    | abund. |
|-------|--------|-------|--------|-------|--------|--------|--------|
| 37.05 | 903    | 56.05 | 258    | 69.15 | 2022   | 80.95  | 156    |
| 38.10 | 756    | 57.05 | 463    | 69.90 | 61     | 81.95  | 26     |
| 38.95 | 372    | 59.95 | 147    | 70.20 | 64     | 86.95  | 101    |
| 44.00 | 288    | 60.30 | 76     | 73.05 | 1007   | 87.95  | 78     |
| 45.00 | 64     | 61.05 | 994    | 74.10 | 3443   | 91.00  | 63     |
| 45.20 | 64     | 62.15 | 1036   | 75.10 | 9962   | 92.10  | 577    |
| 47.00 | 134    | 63.10 | 1192   | 76.10 | 1060   | 93.05  | 934    |
| 48.00 | 78     | 64.00 | 338    | 77.00 | 76     | 94.15  | 2485   |
| 49.05 | 831    | 64.95 | 128    | 77.90 | 61     | 95.10  | 21795  |
| 50.10 | 3530   | 65.20 | 161    | 79.00 | 1706   | 96.10  | 1483   |
| 51.15 | 1170   | 68.10 | 1807   | 80.05 | 350    | 116.95 | 287    |

Average of 12.841 to 12.853 min.: VN086190.D\data.ms

BFB

Modified:subtracted

| m/z    | abund. | m/z    | abund. | m/z | abund. | m/z | abund. |
|--------|--------|--------|--------|-----|--------|-----|--------|
| 118.20 | 72     | 176.10 | 16612  |     |        |     |        |
| 118.95 | 255    | 177.10 | 1174   |     |        |     |        |
| 140.95 | 263    |        |        |     |        |     |        |
| 143.10 | 809    |        |        |     |        |     |        |
| 145.05 | 469    |        |        |     |        |     |        |
| 171.10 | 228    |        |        |     |        |     |        |
| 172.05 | 255    |        |        |     |        |     |        |
| 172.90 | 263    |        |        |     |        |     |        |
| 173.10 | 149    |        |        |     |        |     |        |
| 174.10 | 17338  |        |        |     |        |     |        |
| 175.05 | 1235   |        |        |     |        |     |        |

Instrument :

MSVOA\_N

ClientSampleId :

BFB