

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN040219\
 Data File : VN054900.D
 Acq On : 2 Apr 2019 14:31
 Operator : JC/SP
 Sample : PB118500TB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB118500TB

Quant Time: Apr 03 05:55:38 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N032919W.M
 Quant Title : SW846 8260
 QLast Update : Sat Mar 30 00:48:18 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	538990	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	885223	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	776209	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	277048	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	352821	48.56	ug/l	0.00
Spiked Amount 50.000			Recovery	=	97.12%	
35) Dibromofluoromethane	7.59	113	278372	47.17	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.34%	
50) Toluene-d8	10.09	98	1075789	49.03	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.06%	
62) 4-Bromofluorobenzene	12.40	95	336173	46.07	ug/l	0.00
Spiked Amount 50.000			Recovery	=	92.14%	
Target Compounds						
20) Methylene Chloride	4.55	84	9231	1.510	ug/l #	77
43) Isopropyl Acetate	8.17	43	15671	1.594	ug/l #	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN040219\
Data File : VN054900.D
Acq On : 2 Apr 2019 14:31
Operator : JC/SP
Sample : PB118500TB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB118500TB

Quant Time: Apr 03 05:55:38 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N032919W.M
Quant Title : SW846 8260
QLast Update : Sat Mar 30 00:48:18 2019
Response via : Initial Calibration

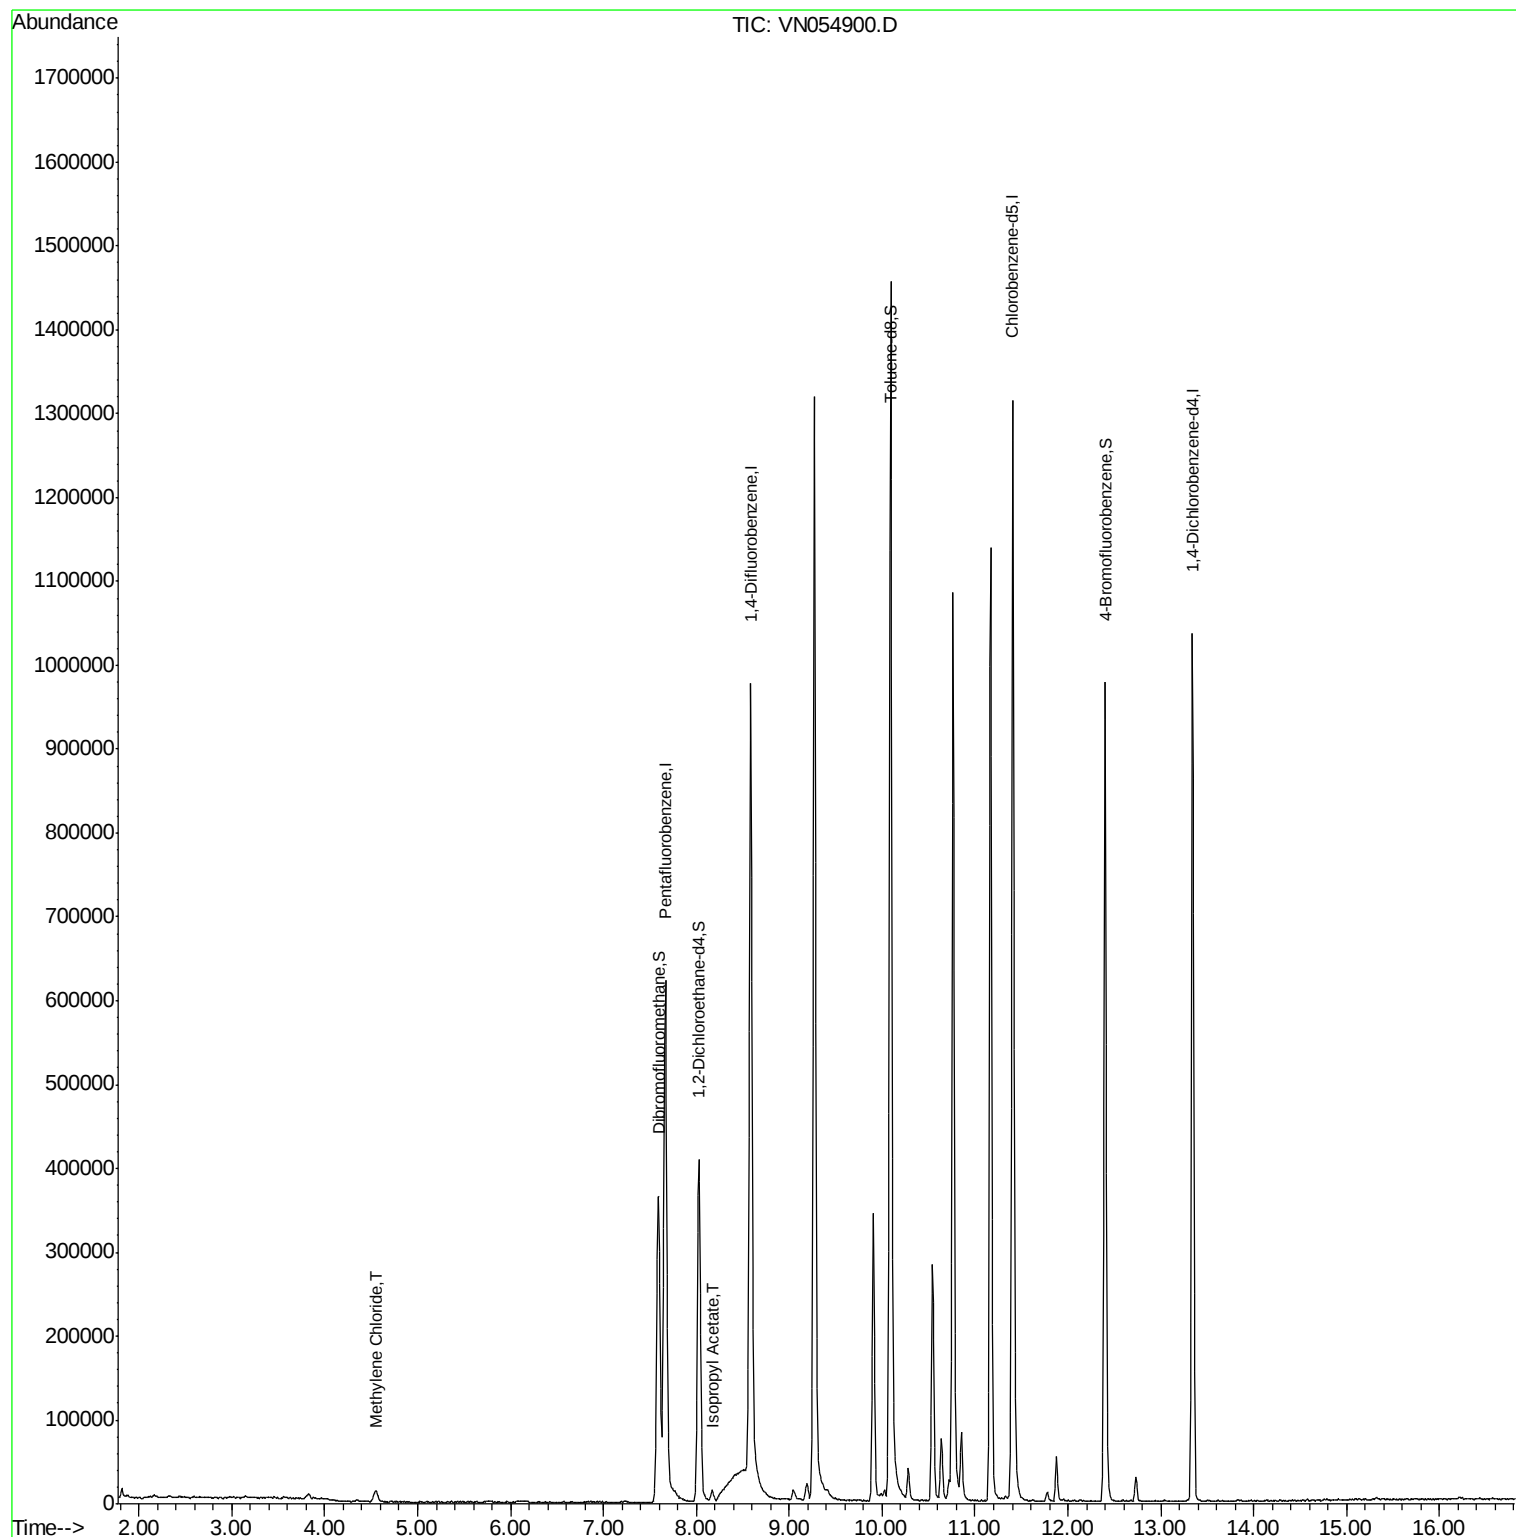



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. -0.00 min

Lab File: VN054900.D

Acq: 2 Apr 2019 14:31

Instrument :

MSVOA_N

ClientSampleId :


PB118500TB

Tot Ion:168 Resp: 538990

Ion Ratio Lower Upper

168 100

99 54.5 37.1 55.7

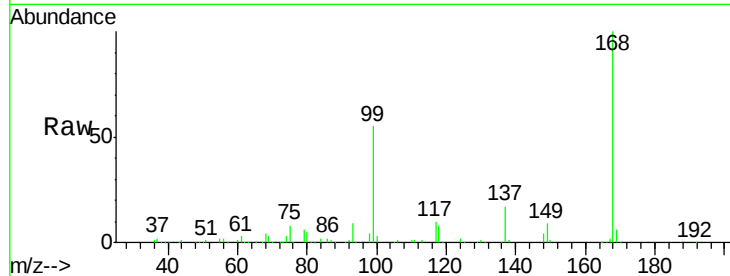

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

7.67

250000

200000



150000

100000

50000

0

Time-->

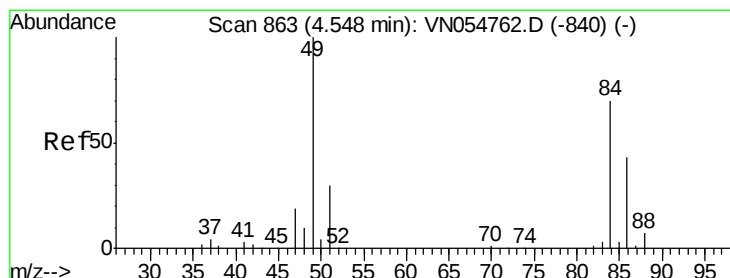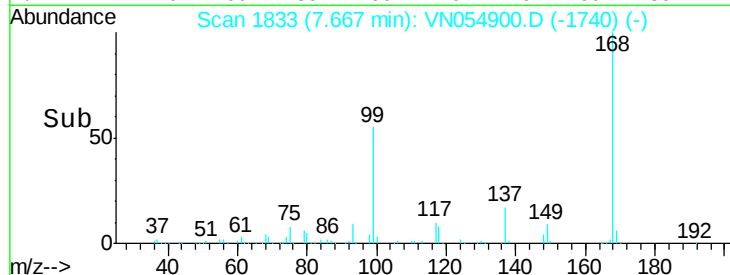

#20

Methylene Chloride

Concen: 1.510 ug/l

RT: 4.55 min Scan# 863

Delta R.T. -0.00 min

Lab File: VN054900.D

Acq: 2 Apr 2019 14:31

Tgt Ion: 84 Resp: 9231


Ion Ratio Lower Upper

84 100

49 143.4 89.7 134.5#

51 45.1 28.2 42.4#

86 74.2 50.8 76.2

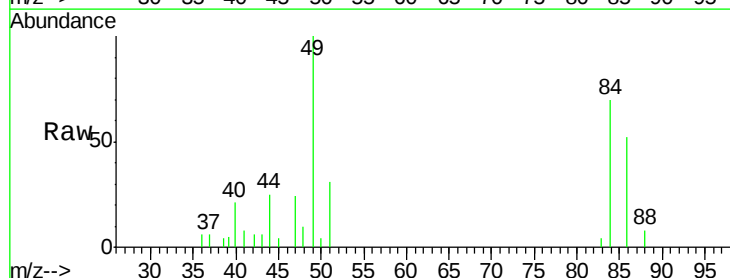

Abundance Ion 83.90 (83.60 to 84.60): VNO

Ion 48.90 (48.60 to 49.60): VNO

Ion 50.90 (50.60 to 51.60): VNO

Ion 85.90 (85.60 to 86.60): VNO

6000

5000

4000


3000


2000

1000

0

Time-->




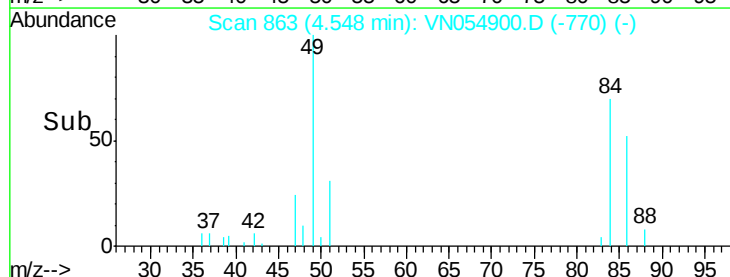


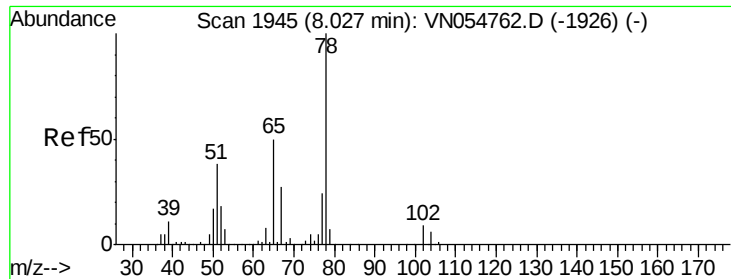

#33
 1,2-Dichloroethane-d4
 Concen: 48.560 ug/l
 RT: 8.03 min Scan# 1946
 Delta R.T. 0.00 min
 Lab File: VN054900.D
 Acq: 2 Apr 2019 14:31




Instrument :
 MSVOA_N
 ClientSampleId :
 PB118500TB


Tot Ion: 65 Resp: 352821
 Ion Ratio Lower Upper
 65 100
 67 52.4 0.0 104.6

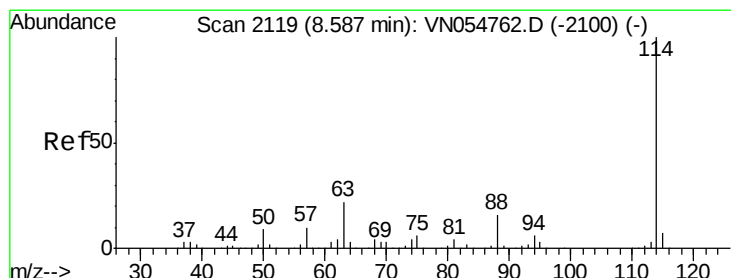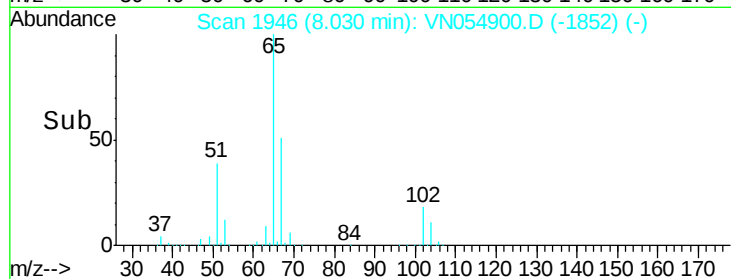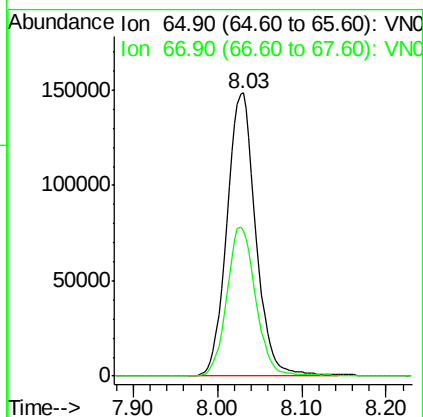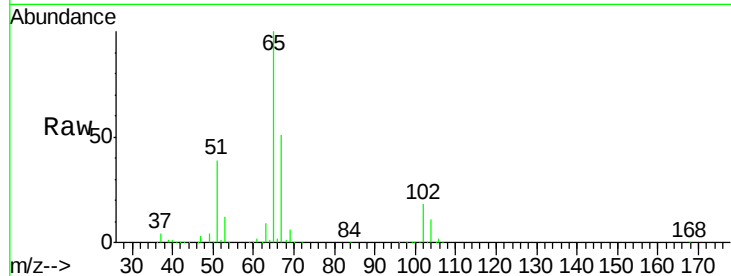

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.59 min Scan# 2119
 Delta R.T. -0.00 min
 Lab File: VN054900.D
 Acq: 2 Apr 2019 14:31

Tgt Ion: 114 Resp: 885223
 Ion Ratio Lower Upper
 114 100
 63 22.2 0.0 35.2
 88 14.6 0.0 30.2

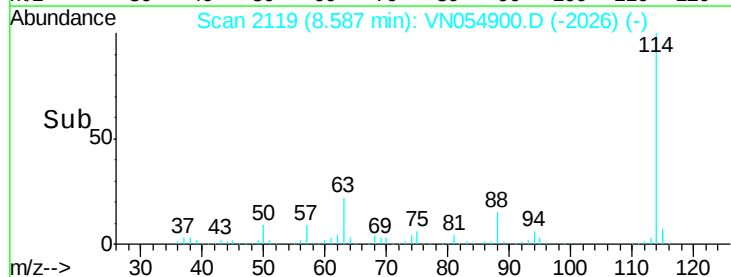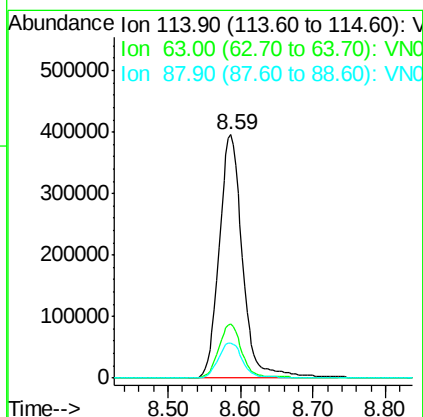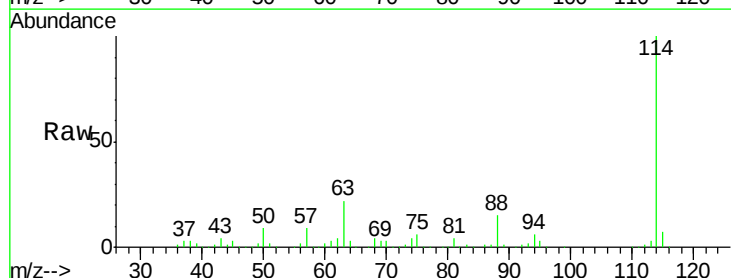

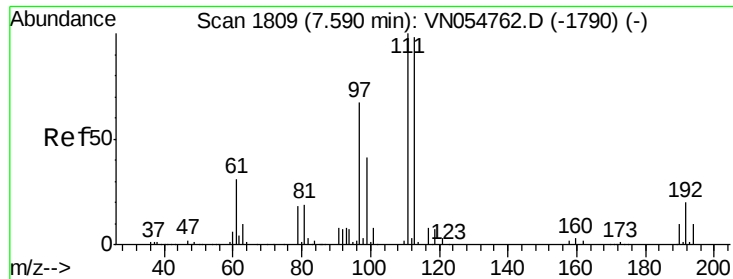

#35

Dibromofluoromethane

Concen: 47.168 ug/l

RT: 7.59 min Scan# 1809

Delta R.T. -0.00 min

Lab File: VN054900.D

Acq: 2 Apr 2019 14:31

Instrument :

MSVOA_N

ClientSampled :

PB118500TB


Tot Ion:113 Resp: 278372

Ion Ratio Lower Upper

113 100

111 103.3 82.2 123.4




192 21.1 19.2 28.8

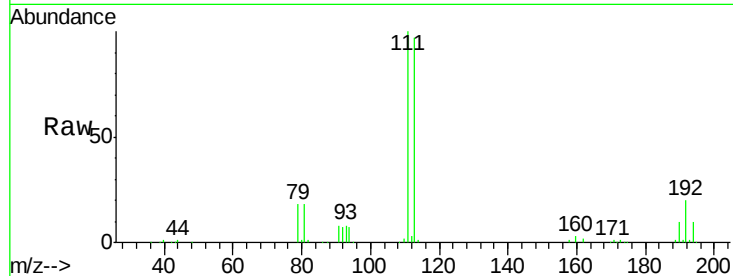

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

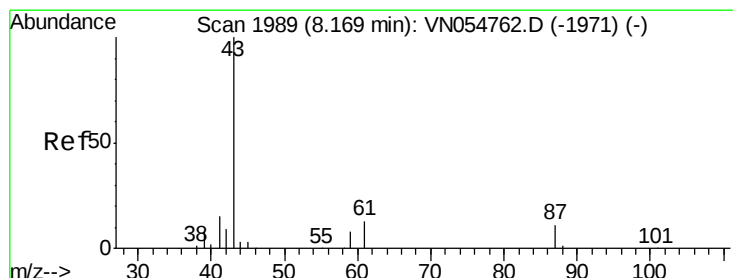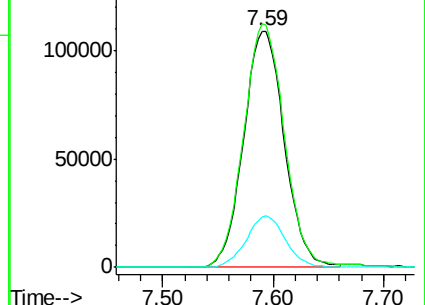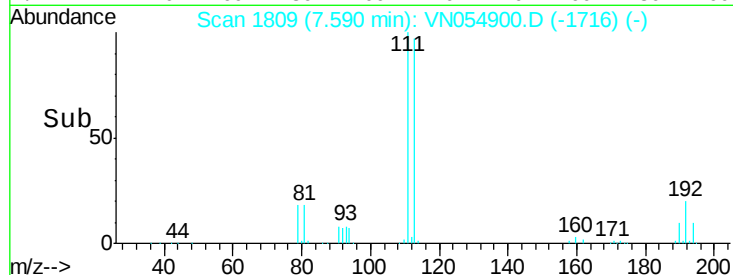

#43

Isopropyl Acetate

Concen: 1.594 ug/l

RT: 8.17 min Scan# 1989

Delta R.T. -0.00 min

Lab File: VN054900.D

Acq: 2 Apr 2019 14:31


Tgt Ion: 43 Resp: 15671

Ion Ratio Lower Upper

43 100

61 16.4 15.8 23.8



87 10.7 12.0 18.0#

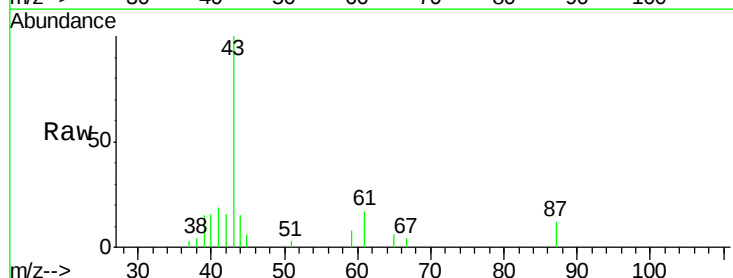


Abundance Ion 43.00 (42.70 to 43.70): VNO

Ion 61.00 (60.70 to 61.70): VNO

Ion 87.00 (86.70 to 87.70): VNO

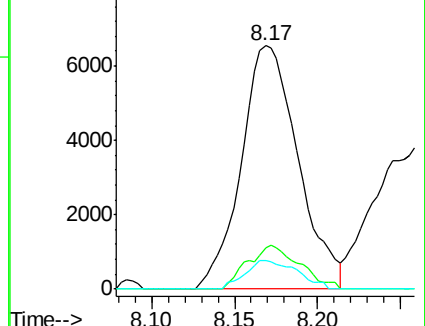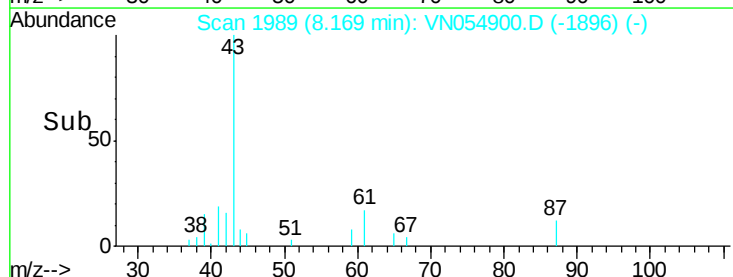

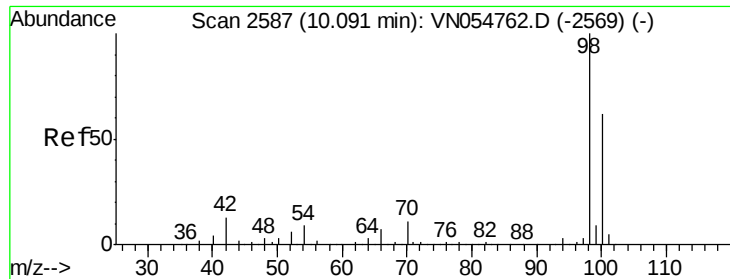

#50

Toluene-d8

Concen: 49.030 ug/l

RT: 10.09 min Scan# 2587

Delta R.T. -0.00 min

Lab File: VN054900.D

Acq: 2 Apr 2019 14:31

Instrument :

MSVOA_N

ClientSampled :


PB118500TB

Tot Ion: 98 Resp: 1075789




Ion Ratio Lower Upper

98 100

100 63.5 51.2 76.8

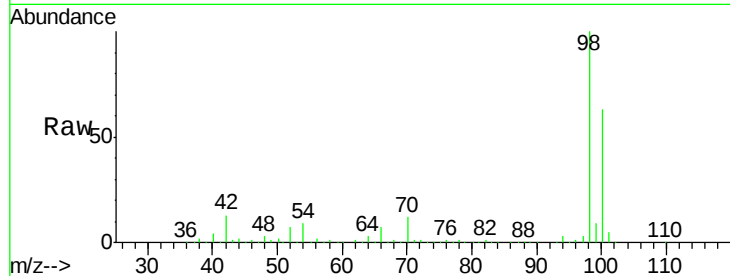

Abundance Ion 98.00 (97.70 to 98.70): VN054762.D (-2569) (-)

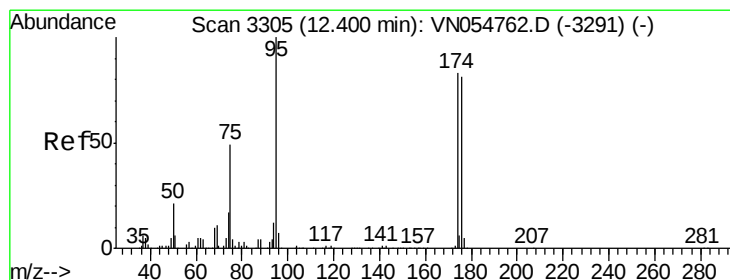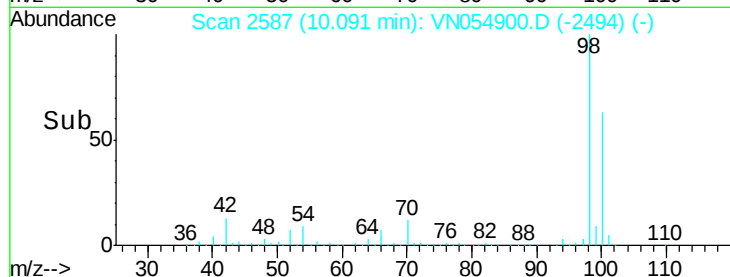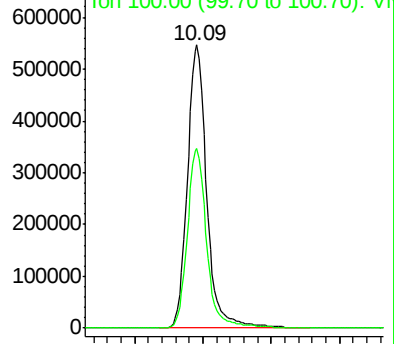

#62

4-Bromofluorobenzene

Concen: 46.069 ug/l

RT: 12.40 min Scan# 3305

Delta R.T. -0.00 min

Lab File: VN054900.D

Acq: 2 Apr 2019 14:31


Tgt Ion: 95 Resp: 336173

Ion Ratio Lower Upper



95 100


174 83.7 0.0 191.0

176 80.4 0.0 187.4

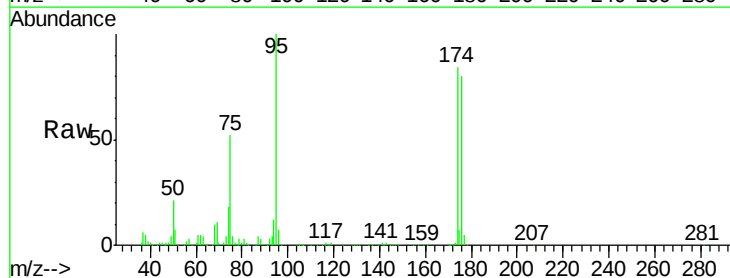

Abundance Ion 94.90 (94.60 to 95.60): VN054762.D (-3291) (-)

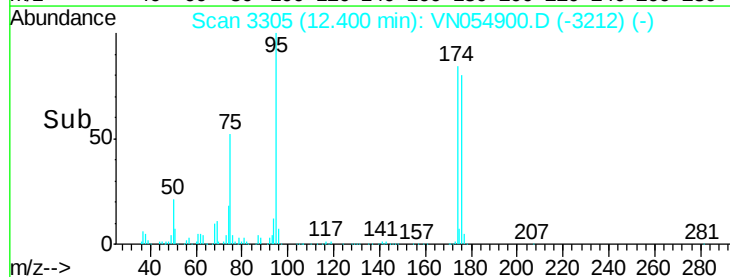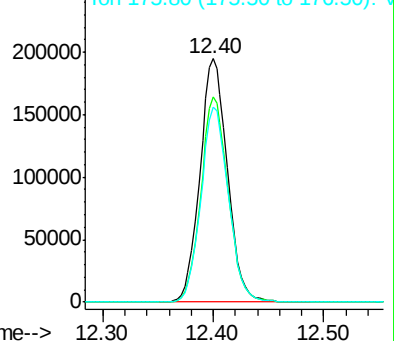


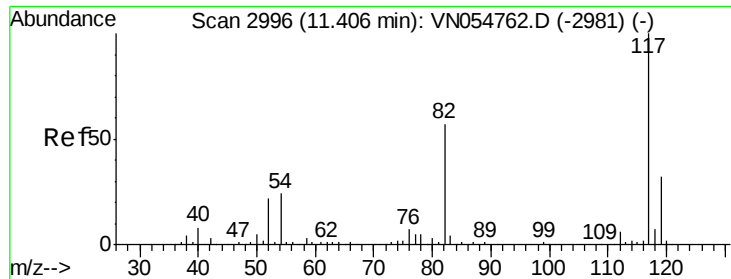




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.41 min Scan# 2996
Delta R.T. -0.00 min
Lab File: VN054900.D
Acq: 2 Apr 2019 14:31

Instrument :
MSVOA_N
ClientSampled :
PB118500TB

Tot Ion:117 Resp: 776209
Ion Ratio Lower Upper
117 100
82 55.4 40.0 60.0
119 32.5 25.8 38.6

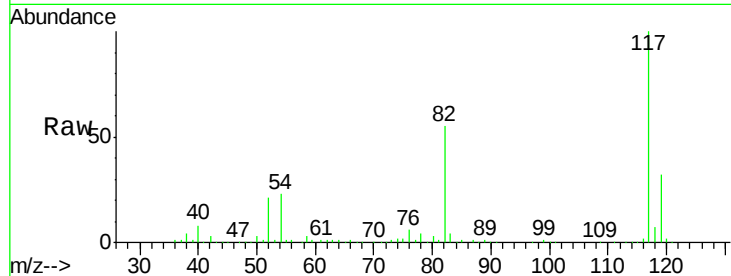


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

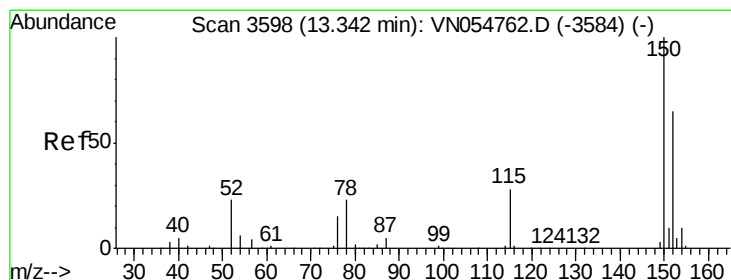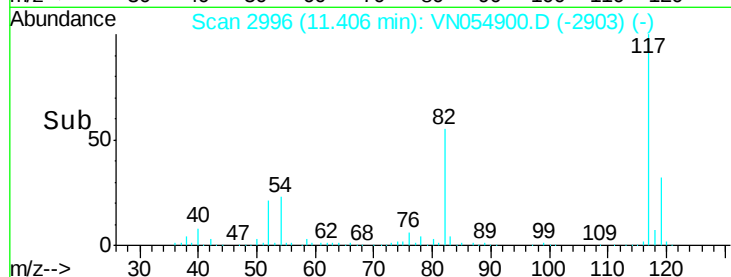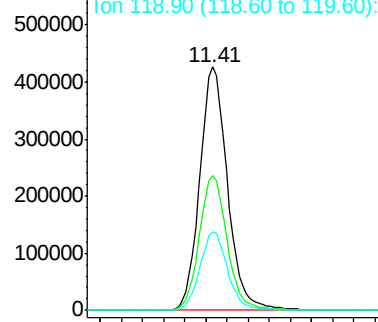

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.34 min Scan# 3598
Delta R.T. -0.00 min
Lab File: VN054900.D
Acq: 2 Apr 2019 14:31

Tgt Ion:152 Resp: 277048
Ion Ratio Lower Upper
152 100
115 57.7 27.2 81.6
150 156.8 0.0 349.2

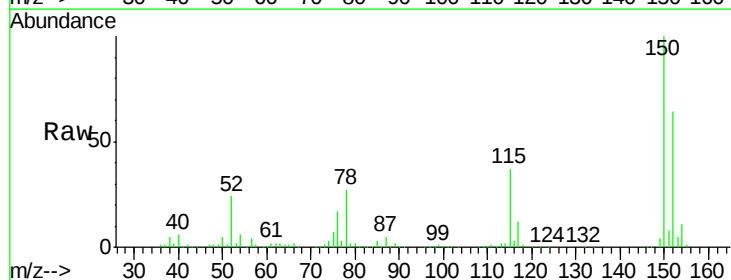

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

