

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN040221\
 Data File : VN066466.D
 Acq On : 2 Apr 2021 14:37
 Operator : JC/MD
 Sample : VN0402MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0402MBL01

Quant Time: Apr 03 03:21:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N032521W.M
 Quant Title : SW846 8260
 QLast Update : Thu Apr 01 14:08:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.579	168	375518	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.510	114	565695	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.347	117	530391	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.286	152	261813	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.941	65	229308	45.94	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	91.88%		
35) Dibromofluoromethane	7.501	113	181676	48.44	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	96.88%		
50) Toluene-d8	10.025	98	707420	49.73	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	99.46%		
62) 4-Bromofluorobenzene	12.345	95	224079	45.35	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	90.70%		
Target Compounds						Qvalue
3) Chloromethane	2.017	50	2219	Below Cal		90
5) Bromomethane	2.524	94	1609	0.44 ug/l		94
11) Tert butyl alcohol	4.667	59	198	0.26 ug/l #		85
13) Acrolein	3.527	56	4600	Below Cal #		43
15) Acrylonitrile	4.868	53	545	0.26 ug/l #		54
16) Acetone	3.741	43	6935	2.57 ug/l		89
17) Carbon Disulfide	3.953	76	3179	0.25 ug/l		96
18) Methyl Acetate	4.224	43	3299	0.47 ug/l #		83
20) Methylene Chloride	4.452	84	1521	Below Cal #		69
25) 2-Butanone	6.742	43	1474	0.50 ug/l #		88
29) Tetrahydrofuran	7.134	42	1413	0.73 ug/l #		47
31) Cyclohexane	7.574	56	7397	1.07 ug/l #		25
36) 1,1-Dichloropropene	7.579	75	27883	5.25 ug/l #		48
38) Carbon Tetrachloride	7.582	117	33402	6.25 ug/l #		15
49) 1,4-Dioxane	9.135	88	373	6.24 ug/l #		67
51) 4-Methyl-2-Pentanone	9.921	43	7364	1.26 ug/l		93
59) 2-Hexanone	10.696	43	8585	2.10 ug/l		97
74) N-amyl acetate	12.031	43	58	3.20 ug/l #		45
76) 1,2,3-Trichloropropane	12.345	75	113136	19.69 ug/l #		100
81) trans-1,4-Dichloro-2-b...	12.345	75	113136	59.22 ug/l #		12
86) p-Isopropyltoluene	13.238	119	3507	0.22 ug/l		96
87) 1,3-Dichlorobenzene	13.227	146	2165	0.26 ug/l #		55
88) 1,4-Dichlorobenzene	13.311	146	2532	0.30 ug/l #		1
89) n-Butylbenzene	13.579	91	5690	0.43 ug/l #		40
91) 1,2-Dichlorobenzene	13.600	146	1807	0.22 ug/l		68
92) 1,2-Dibromo-3-Chloropr...	14.220	75	253	0.21 ug/l #		1
93) 1,2,4-Trichlorobenzene	14.984	180	2280	0.45 ug/l #		1
94) Hexachlorobutadiene	15.102	225	1878	0.68 ug/l		94
95) Naphthalene	15.274	128	37552	3.55 ug/l		97
96) 1,2,3-Trichlorobenzene	15.504	180	4462	0.88 ug/l #		48


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN040221\
Data File : VN066466.D
Acq On : 2 Apr 2021 14:37
Operator : JC/MD
Sample : VN0402MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0402MBL01

Quant Time: Apr 03 03:21:13 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N032521W.M
Quant Title : SW846 8260
QLast Update : Thu Apr 01 14:08:22 2021
Response via : Initial Calibration




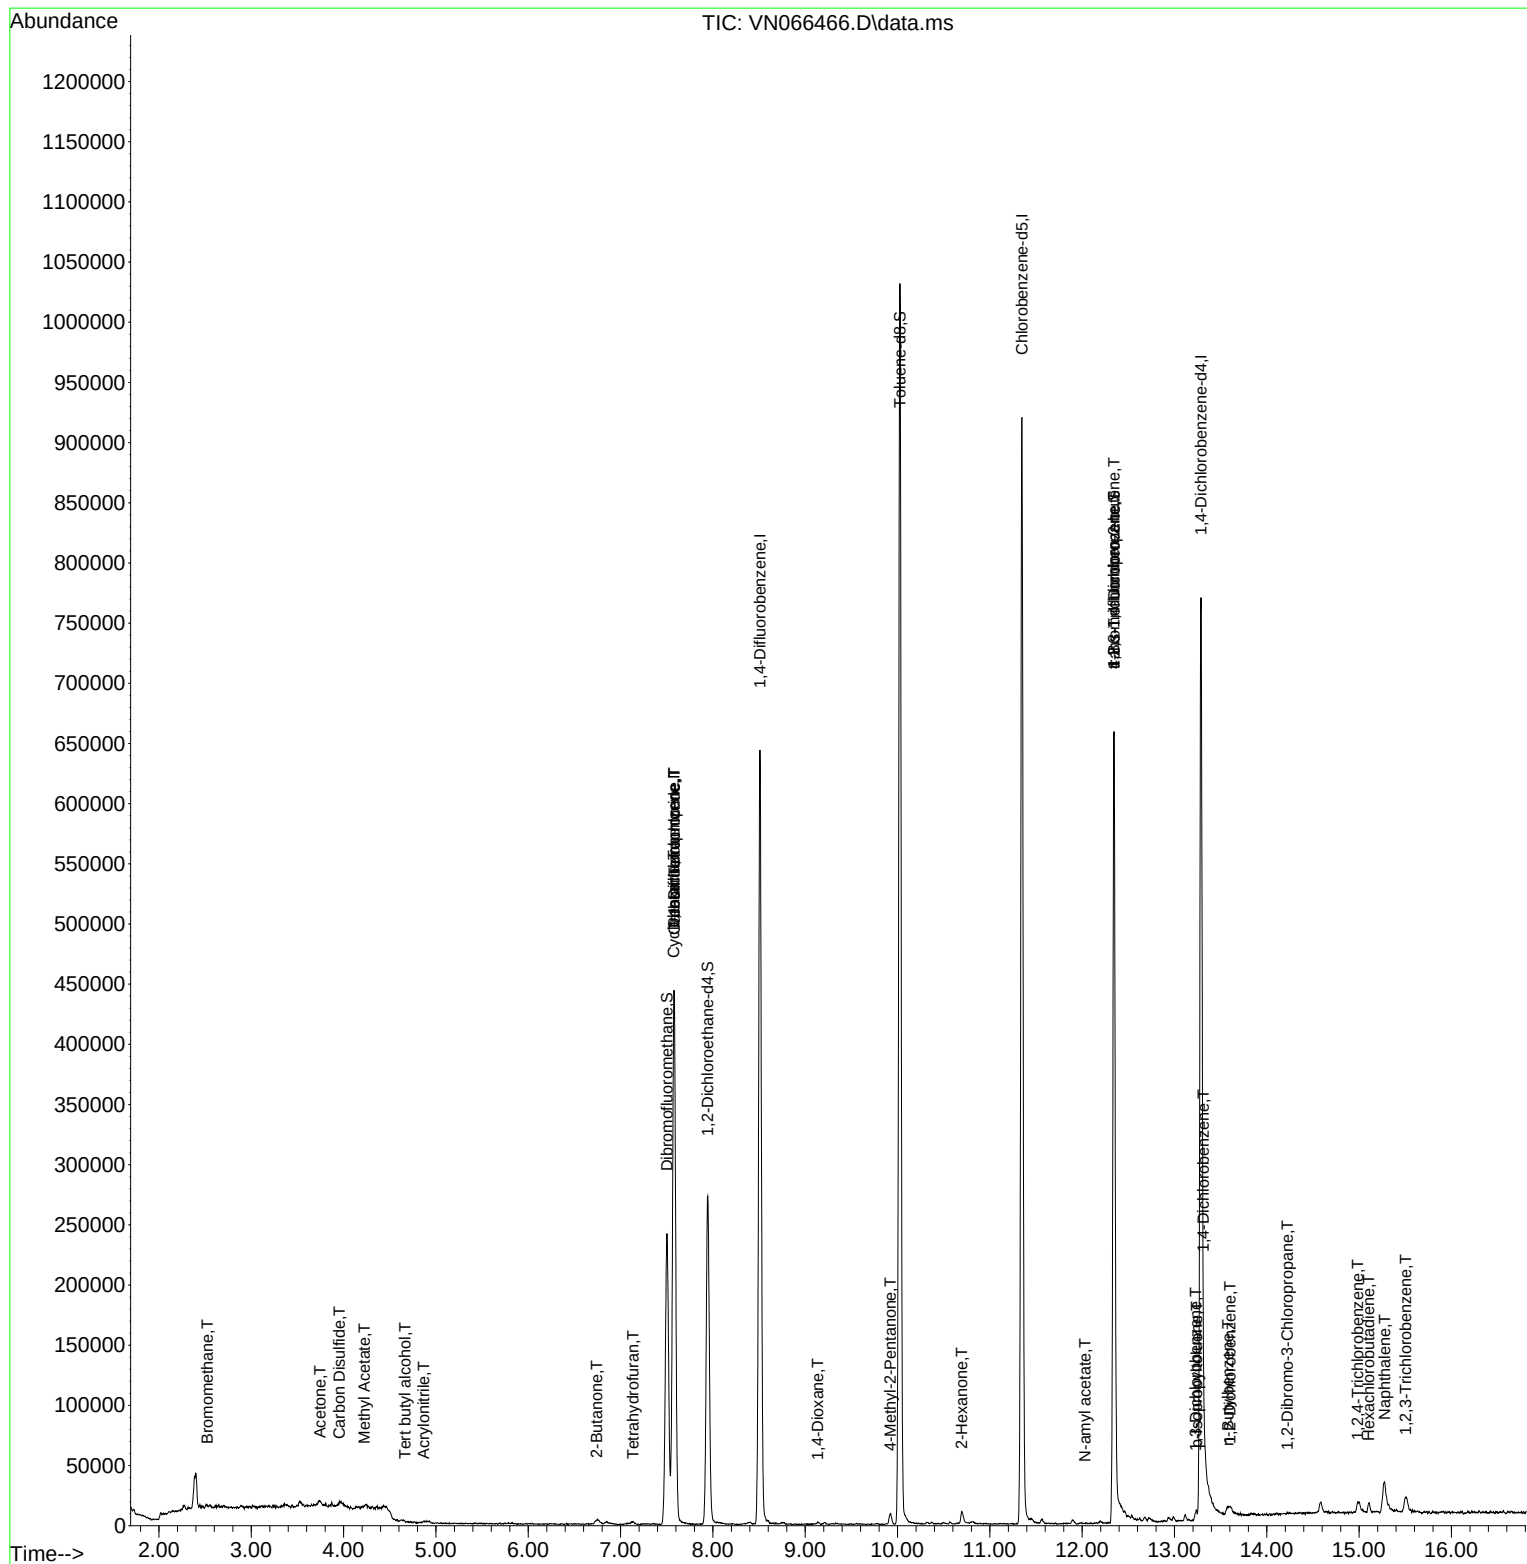




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.579 min Scan# 2196
Delta R.T. 0.000 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37




Instrument :
MSVOA_N
ClientSampleId :
VN0402MBL01


Tgt Ion:168 Resp: 375518
Ion Ratio Lower Upper
168 100
99 51.5 41.1 61.7



#3
Chloromethane
Concen: Below Cal
RT: 2.017 min Scan# 122
Delta R.T. -0.000 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37

Tgt Ion: 50 Resp: 2219
Ion Ratio Lower Upper
50 100
52 27.2 26.2 39.2


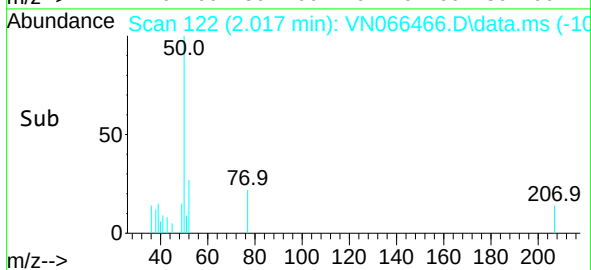






#5
Bromomethane
Concen: 0.44 ug/l
RT: 2.524 min Scan# 311
Delta R.T. 0.011 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37




Instrument :
MSVOA_N
ClientSampled :
VN0402MBL01


Tgt Ion: 94 Resp: 1609
Ion Ratio Lower Upper
94 100
96 89.3 75.8 113.6

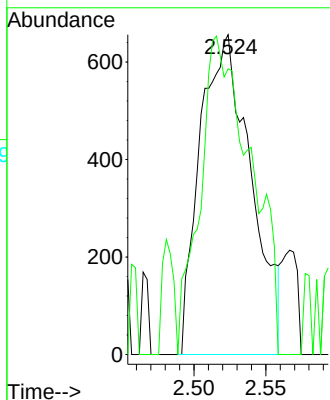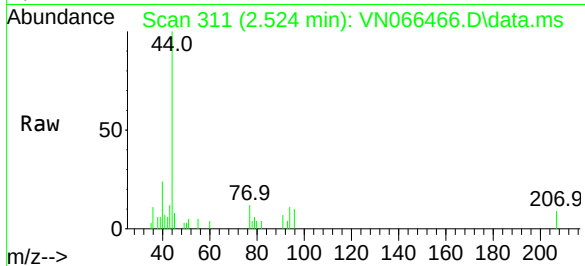

#11
Tert butyl alcohol
Concen: 0.26 ug/l
RT: 4.667 min Scan# 1110
Delta R.T. -0.035 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37

Tgt Ion: 59 Resp: 198
Ion Ratio Lower Upper
59 100
57 0.0 4.1 6.1#


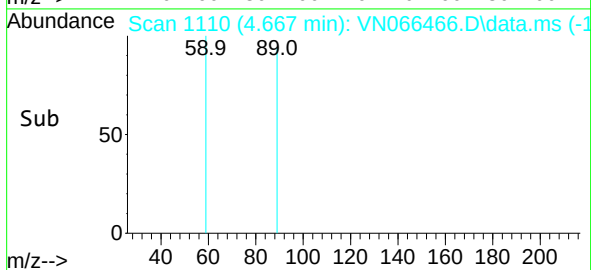
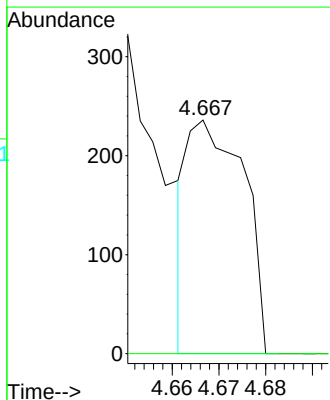
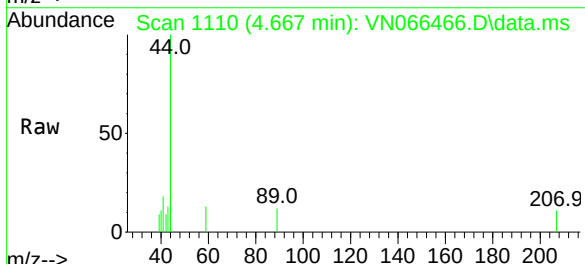




#13
Acrolein
Concen: Below Cal
RT: 3.527 min Scan# 685
Delta R.T. -0.000 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37




Instrument :
MSVOA_N
ClientSampleId :
VN0402MBL01


Tgt Ion: 56 Resp: 4600
Ion Ratio Lower Upper
56 100
55 24.6 57.9 86.9#

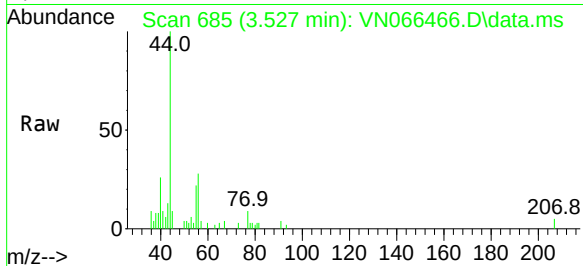

#15
Acrylonitrile
Concen: 0.26 ug/l
RT: 4.868 min Scan# 1185
Delta R.T. -0.008 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37

Tgt Ion: 53 Resp: 545
Ion Ratio Lower Upper
53 100
52 125.7 66.6 99.8#
51 62.4 29.4 44.0#


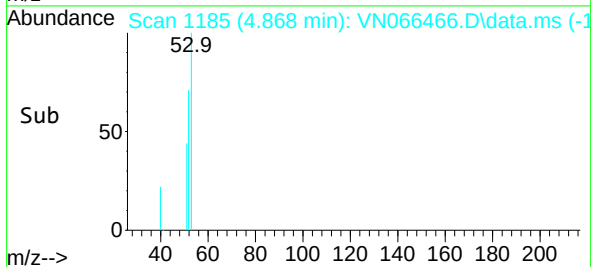

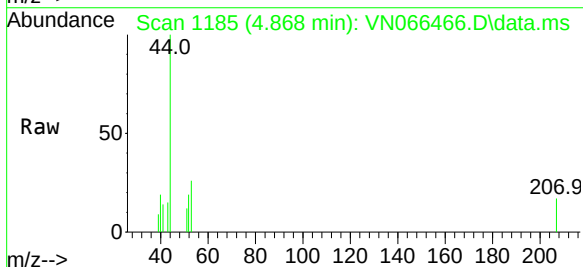




#16
Acetone
Concen: 2.57 ug/l
RT: 3.741 min Scan# 765
Delta R.T. 0.008 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37




Instrument :
MSVOA_N
ClientSampleId :
VN0402MBL01


Tgt Ion: 43 Resp: 6935
Ion Ratio Lower Upper
43 100
58 35.5 23.8 35.8



#17
Carbon Disulfide
Concen: 0.25 ug/l
RT: 3.953 min Scan# 844
Delta R.T. -0.008 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37

Tgt Ion: 76 Resp: 3179
Ion Ratio Lower Upper
76 100
78 7.8 7.4 11.0


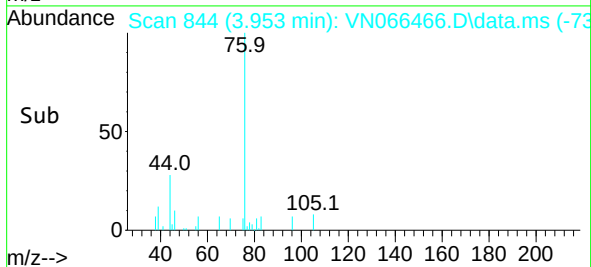

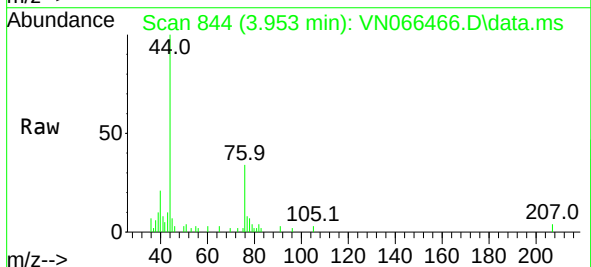




#18
Methyl Acetate
Concen: 0.47 ug/l
RT: 4.224 min Scan# 945
Delta R.T. -0.005 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37




Instrument :
MSVOA_N
ClientSampleId :
VN0402MBL01


Tgt Ion: 43 Resp: 3299
Ion Ratio Lower Upper
43 100
74 14.0 17.6 26.4#



#20
Methylene Chloride
Concen: Below Cal
RT: 4.452 min Scan# 1030
Delta R.T. 0.005 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37


Tgt Ion: 84 Resp: 1521
Ion Ratio Lower Upper
84 100
49 94.8 105.0 157.6#
51 21.9 31.6 47.4#
86 41.2 53.0 79.6#

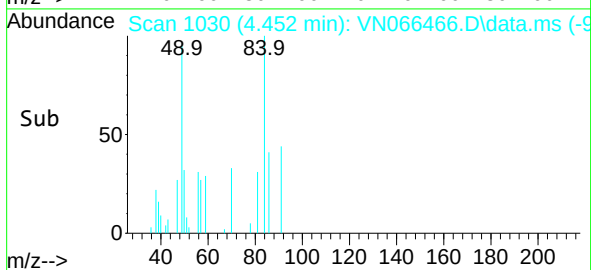



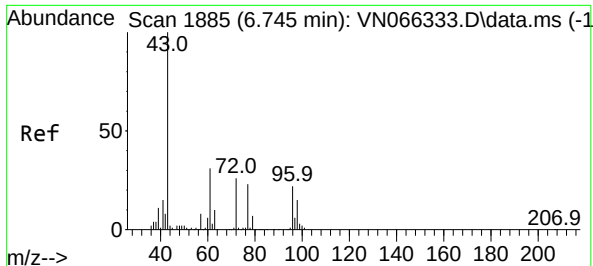


#25
2-Butanone
Concen: 0.50 ug/l
RT: 6.742 min Scan# 1884
Delta R.T. 0.003 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37


Instrument :
MSVOA_N
ClientSampleId :
VN0402MBL01

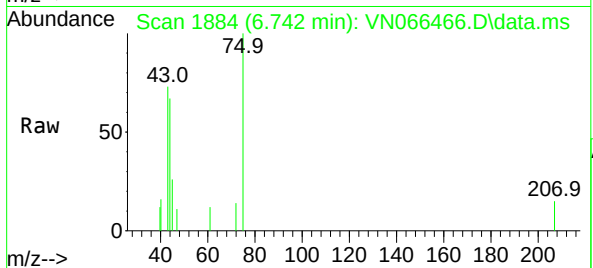



Tgt Ion: 43 Resp: 1474
Ion Ratio Lower Upper
43 100
72 19.8 20.7 31.1#

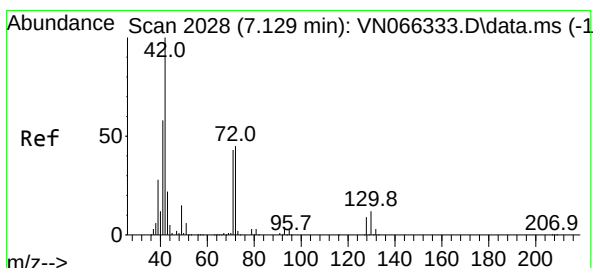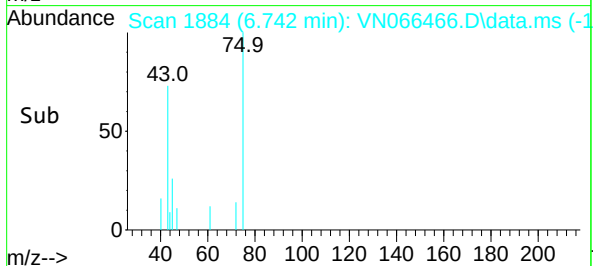


#29
Tetrahydrofuran
Concen: 0.73 ug/l
RT: 7.134 min Scan# 2030
Delta R.T. 0.011 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37

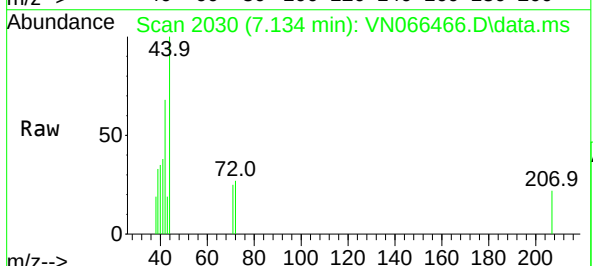


Tgt Ion: 42 Resp: 1413
Ion Ratio Lower Upper
42 100
72 0.0 35.2 52.8#
71 17.8 33.1 49.7#

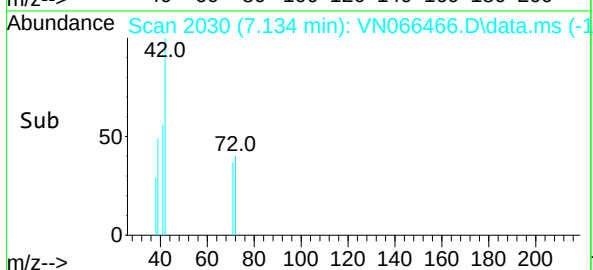






#31
Cyclohexane
Concen: 1.07 ug/l
RT: 7.574 min Scan# 2194
Delta R.T. 0.008 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37


Instrument :
MSVOA_N
ClientSampleId :
VN0402MBL01





Tgt Ion	Ratio	Lower	Upper
56	100		
69	148.8	26.6	40.0#
84	108.6	68.7	103.1#




#33
1,2-Dichloroethane-d4
Concen: 45.94 ug/l
RT: 7.941 min Scan# 2331
Delta R.T. -0.003 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37



Tgt Ion	Ratio	Lower	Upper
65	100		
67	53.2	0.0	105.2




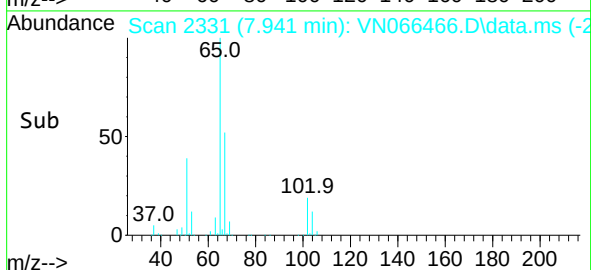




#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.510 min Scan# 2543
Delta R.T. -0.000 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37




Instrument :
MSVOA_N
ClientSampleId :
VN0402MBL01


Tgt Ion:114 Resp: 565695
Ion Ratio Lower Upper
114 100
63 20.0 0.0 42.0
88 14.6 0.0 31.0

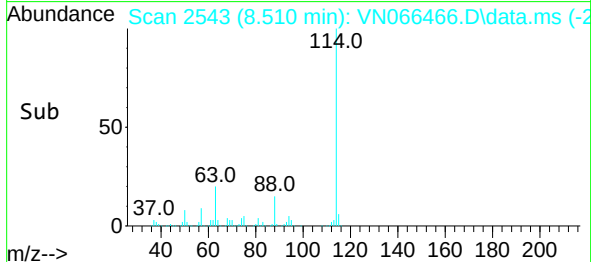

#35
Dibromofluoromethane
Concen: 48.44 ug/l
RT: 7.501 min Scan# 2167
Delta R.T. -0.000 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37

Tgt Ion:113 Resp: 181676
Ion Ratio Lower Upper
113 100
111 103.6 81.8 122.8
192 21.9 17.1 25.7


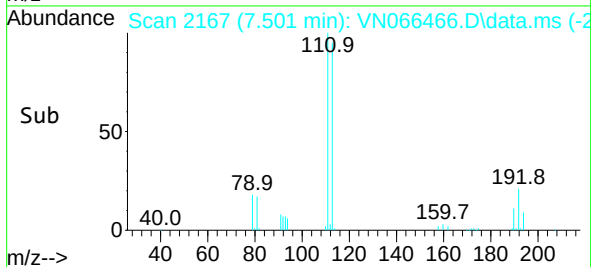

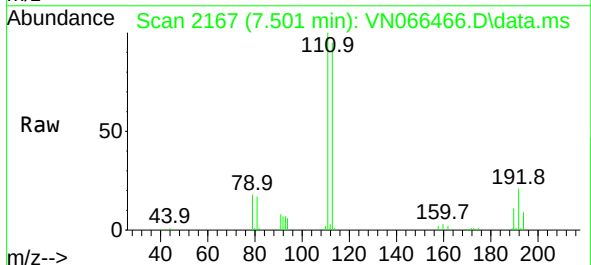




#36
1,1-Dichloropropene
Concen: 5.25 ug/l
RT: 7.579 min Scan# 2196
Delta R.T. -0.126 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37




Instrument :
MSVOA_N
ClientSampleId :
VN0402MBL01


Tgt Ion: 75 Resp: 27883
Ion Ratio Lower Upper
75 100
110 7.6 18.1 54.3#
77 0.1 25.0 37.4#



#38
Carbon Tetrachloride
Concen: 6.25 ug/l
RT: 7.582 min Scan# 2197
Delta R.T. -0.102 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37

Tgt Ion: 117 Resp: 33402
Ion Ratio Lower Upper
117 100
119 4.5 77.2 115.8#
121 0.0 24.2 36.4#


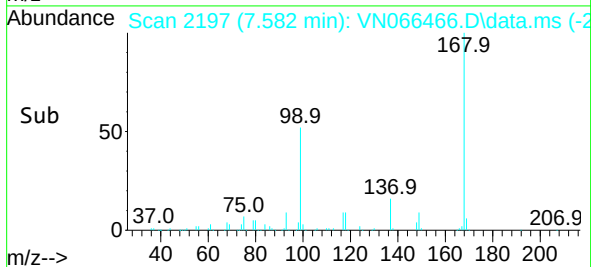

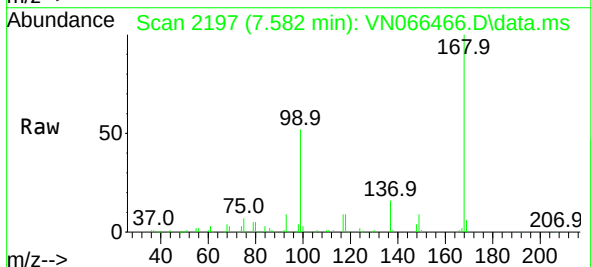




#49
1,4-Dioxane
Concen: 6.24 ug/l
RT: 9.135 min Scan# 2776
Delta R.T. 0.003 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37




Instrument :
MSVOA_N
ClientSampled :
VN0402MBL01


Tgt Ion: 88 Resp: 373
Ion Ratio Lower Upper
88 100
43 60.3 28.2 42.4#
58 47.2 56.6 84.8#



#50
Toluene-d8
Concen: 49.73 ug/l
RT: 10.025 min Scan# 3108
Delta R.T. -0.000 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37

Tgt Ion: 98 Resp: 707420
Ion Ratio Lower Upper
98 100
100 63.2 50.5 75.7


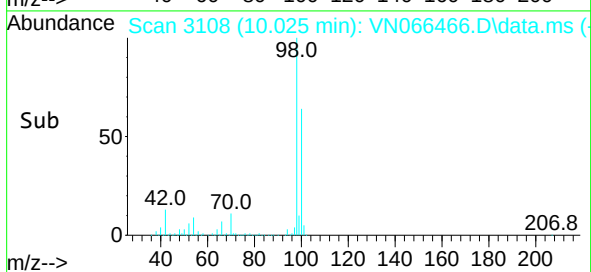






#51
4-Methyl-2-Pentanone
Concen: 1.26 ug/l
RT: 9.921 min Scan# 3069
Delta R.T. 0.003 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37




Instrument :
MSVOA_N
ClientSampleId :
VN0402MBL01


Tgt Ion: 43 Resp: 7364
Ion Ratio Lower Upper
43 100
58 34.1 30.8 46.2



#59
2-Hexanone
Concen: 2.10 ug/l
RT: 10.696 min Scan# 3358
Delta R.T. 0.005 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37

Tgt Ion: 43 Resp: 8585
Ion Ratio Lower Upper
43 100
58 55.2 26.6 79.8


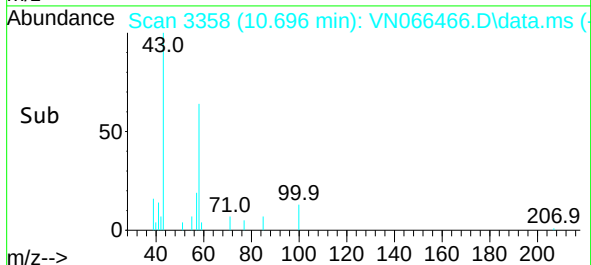

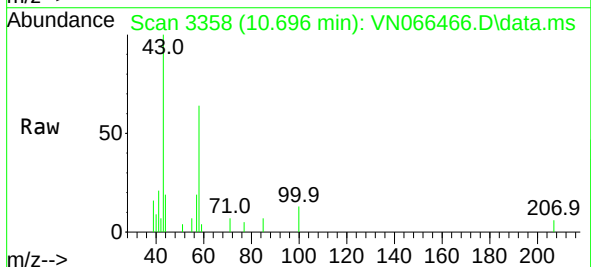


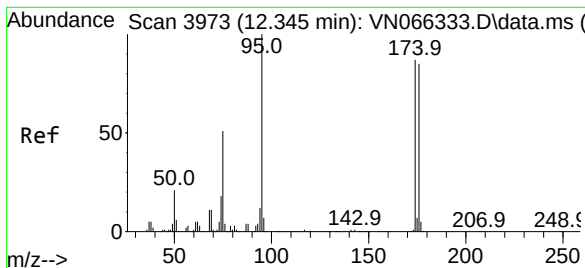

#62
4-Bromofluorobenzene
Concen: 45.35 ug/l
RT: 12.345 min Scan# 3973
Delta R.T. 0.003 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37




Instrument :
MSVOA_N
ClientSampleId :
VN0402MBL01


Tgt Ion: 95 Resp: 224079
Ion Ratio Lower Upper
95 100
174 92.1 0.0 172.2
176 85.8 0.0 167.8

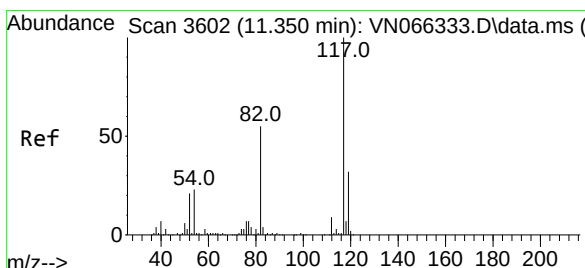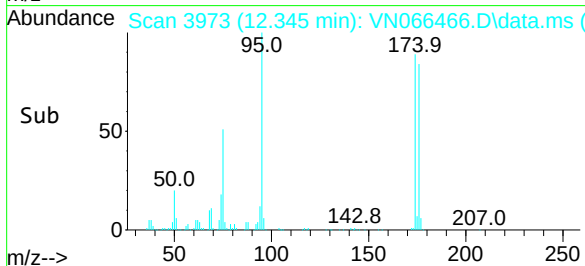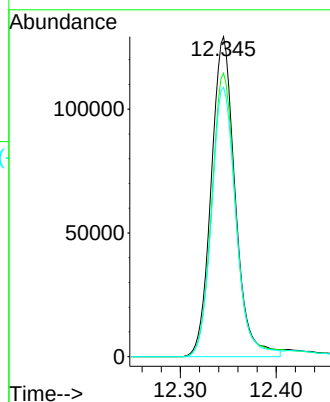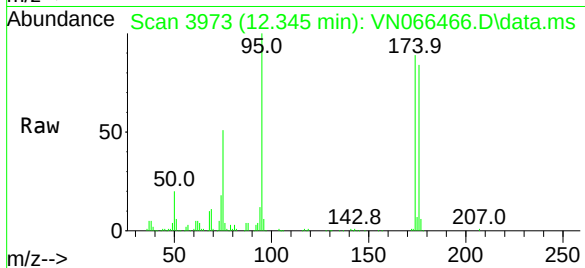

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.347 min Scan# 3601
Delta R.T. -0.000 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37

Tgt Ion: 117 Resp: 530391
Ion Ratio Lower Upper
117 100
82 53.4 44.2 66.4
119 31.3 25.8 38.6


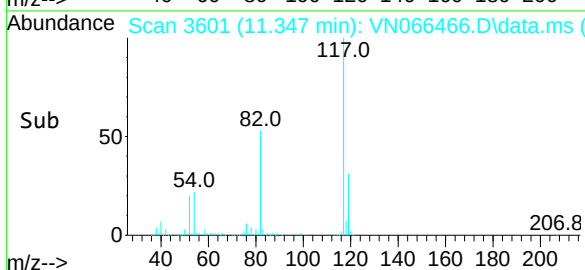
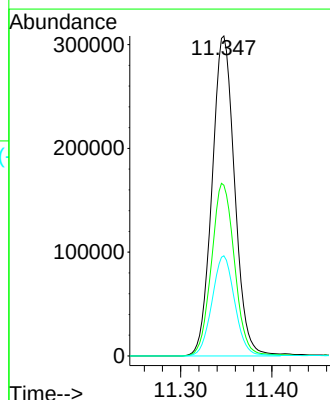
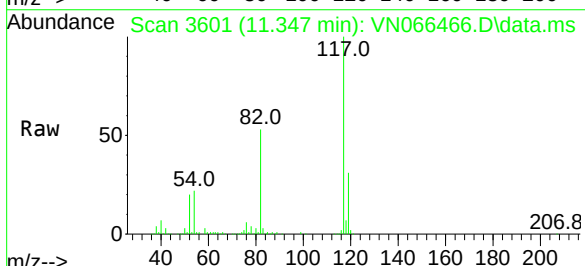


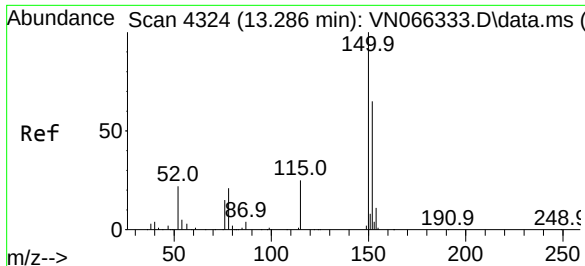

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.286 min Scan# 4324
Delta R.T. 0.003 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37




Instrument :
MSVOA_N
ClientSampleId :
VN0402MBL01


Tgt Ion:152 Resp: 261813
Ion Ratio Lower Upper
152 100
115 54.4 27.8 83.4
150 158.7 0.0 348.4

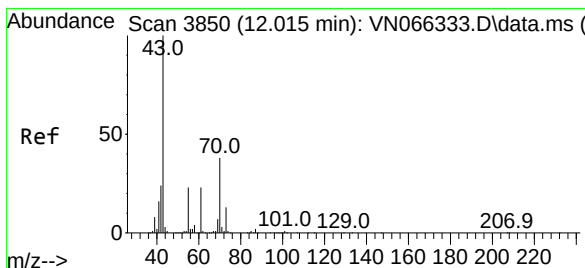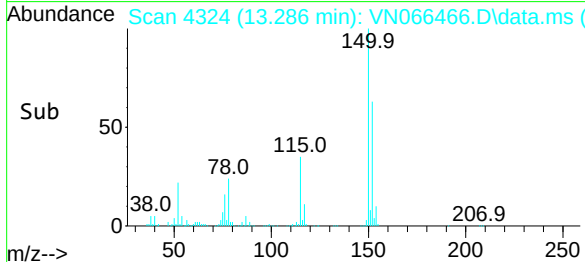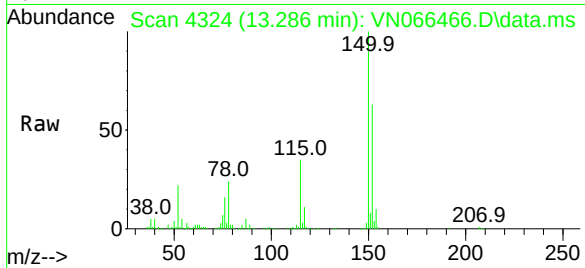

#74
N-ethyl acetate
Concen: 3.20 ug/l
RT: 12.031 min Scan# 3856
Delta R.T. 0.016 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37

Tgt Ion: 43 Resp: 58
Ion Ratio Lower Upper
43 100
70 0.0 31.2 46.8#
55 0.0 18.6 28.0#
61 0.0 18.2 27.4#


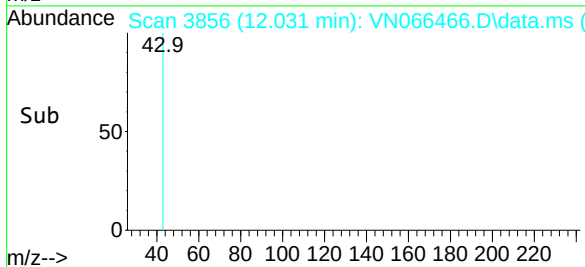

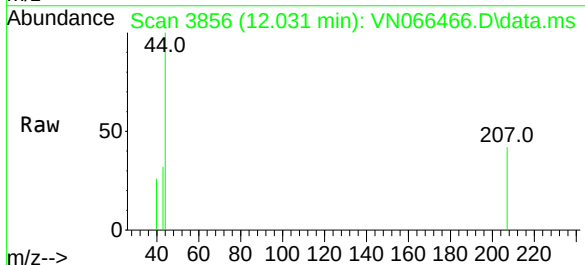


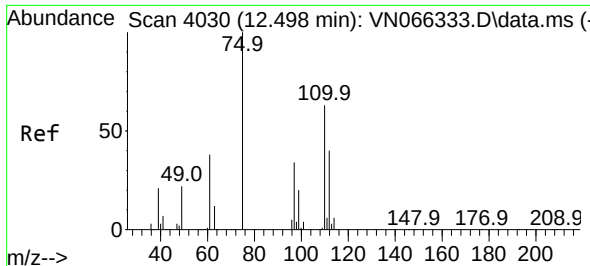

#76
1,2,3-Trichloropropane
Concen: 19.69 ug/l
RT: 12.345 min Scan# 3973
Delta R.T. -0.150 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37




Instrument :
MSVOA_N
ClientSampleId :
VN0402MBL01


Tgt Ion: 75 Resp: 113136
Ion Ratio Lower Upper
75 100
77 1.4 0.0 0.0#

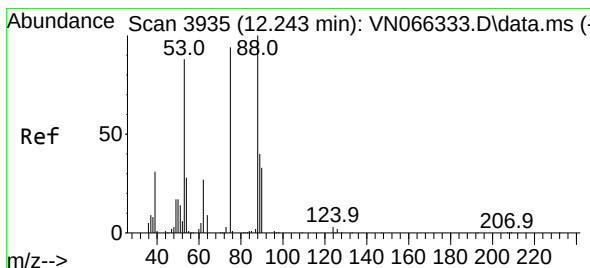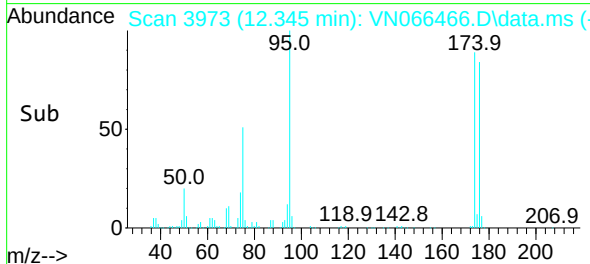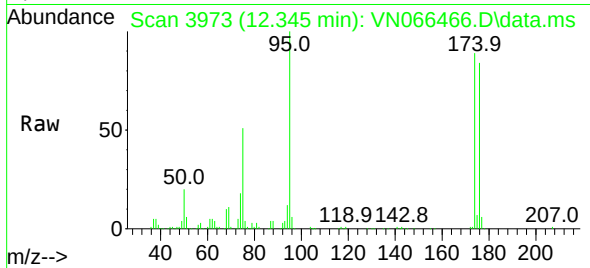

#81
trans-1,4-Dichloro-2-butene
Concen: 59.22 ug/l
RT: 12.345 min Scan# 3973
Delta R.T. 0.102 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37

Tgt Ion: 75 Resp: 113136
Ion Ratio Lower Upper
75 100
53 0.1 76.1 114.1#
89 0.0 35.7 53.5#


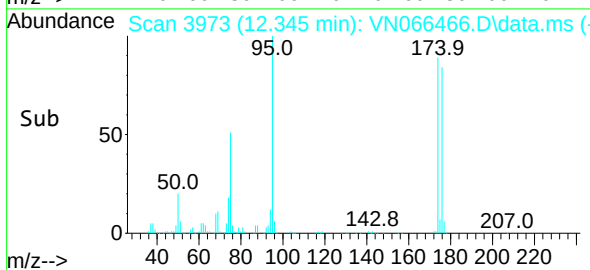

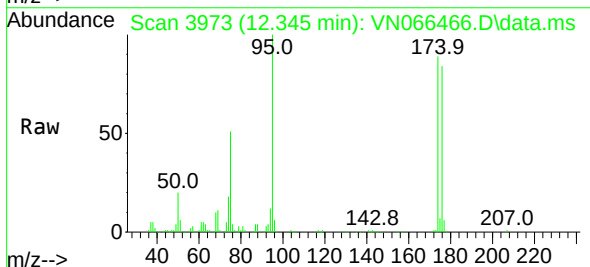


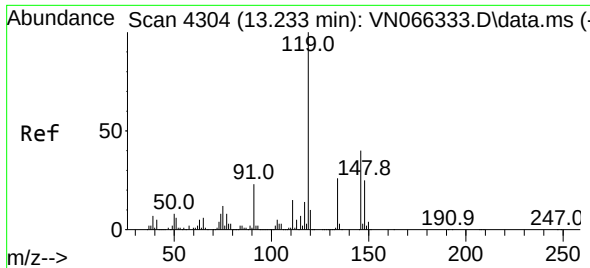

#86
p-Isopropyltoluene
Concen: 0.22 ug/l
RT: 13.238 min Scan# 4306
Delta R.T. 0.005 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37




Instrument :
MSVOA_N
ClientSampleId :
VN0402MBL01


Tgt Ion:119 Resp: 3507
Ion Ratio Lower Upper
119 100
134 26.6 12.9 38.7
91 26.6 11.5 34.5

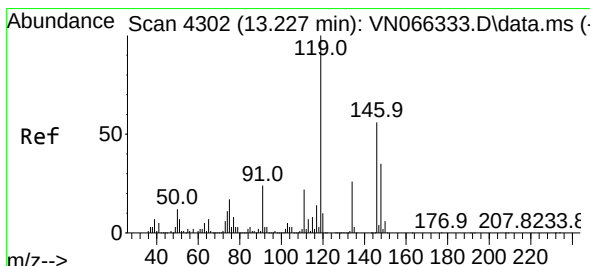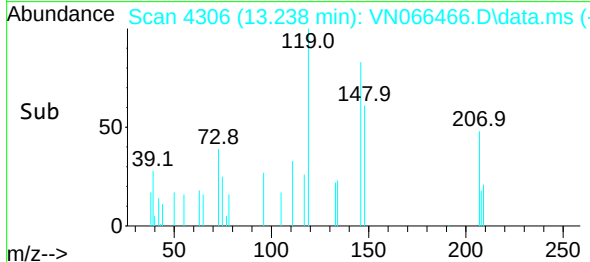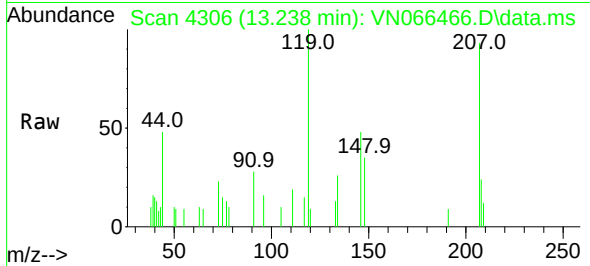

#87
1,3-Dichlorobenzene
Concen: 0.26 ug/l
RT: 13.227 min Scan# 4302
Delta R.T. 0.003 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37

Tgt Ion:146 Resp: 2165
Ion Ratio Lower Upper
146 100
111 18.6 19.4 58.1#
148 23.4 31.8 95.4#


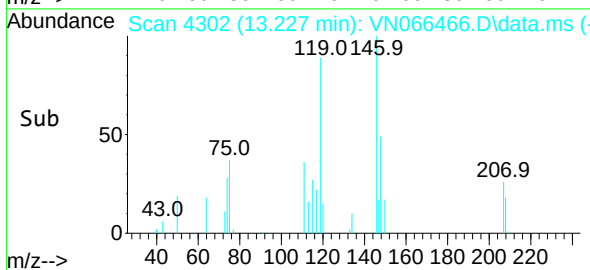

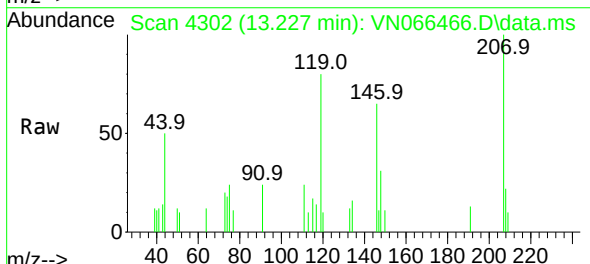


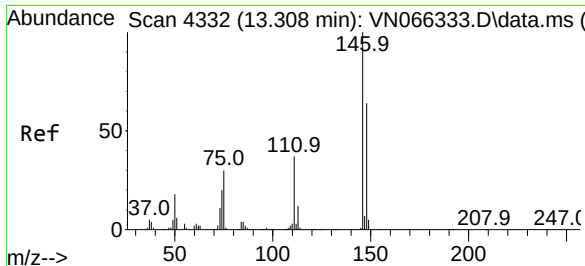

#88
1,4-Dichlorobenzene
Concen: 0.30 ug/l
RT: 13.311 min Scan# 4333
Delta R.T. 0.005 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37




Instrument :
MSVOA_N
ClientSampleId :
VN0402MBL01


Tgt Ion:146 Resp: 2532
Ion Ratio Lower Upper
146 100
111 175.1 18.3 54.9#
148 131.1 31.9 95.9#

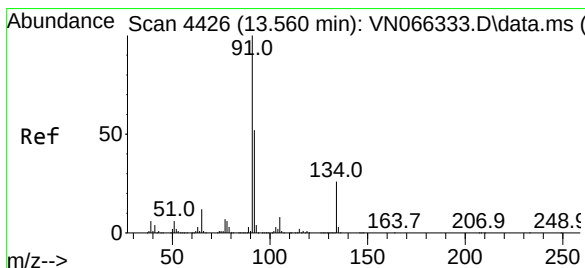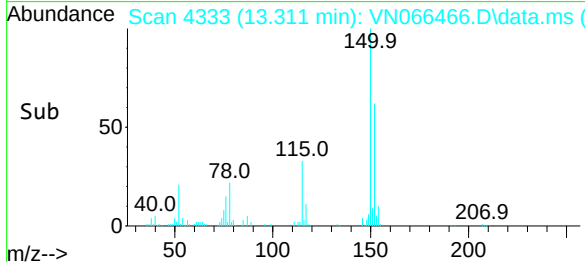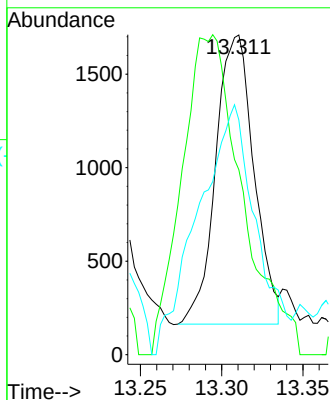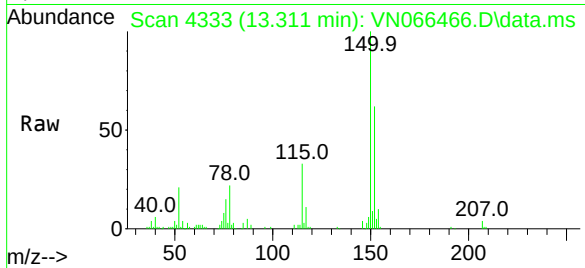

#89
n-Butylbenzene
Concen: 0.43 ug/l
RT: 13.579 min Scan# 4433
Delta R.T. 0.021 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37

Tgt Ion: 91 Resp: 5690
Ion Ratio Lower Upper
91 100
92 0.0 26.1 78.3#
134 10.6 12.8 38.4#


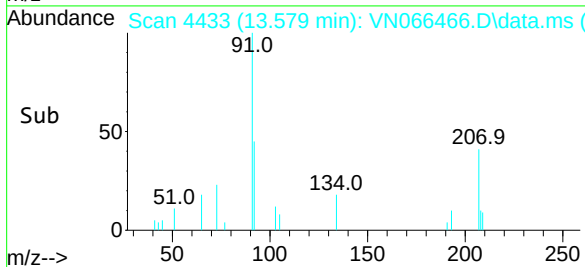
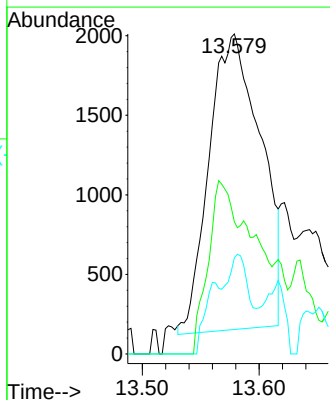
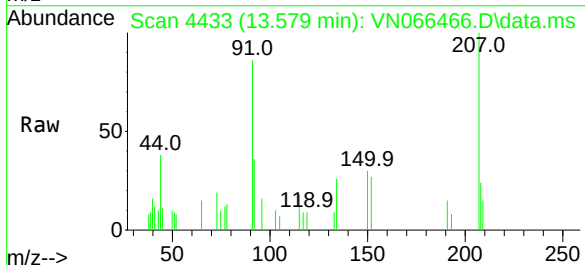


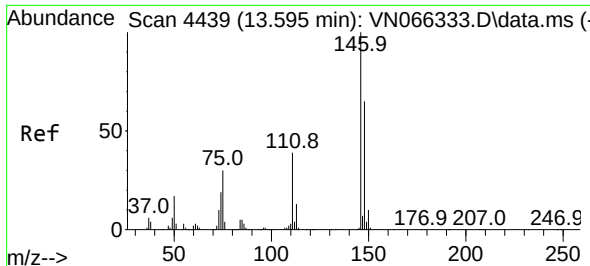

#91
1,2-Dichlorobenzene
Concen: 0.22 ug/l
RT: 13.600 min Scan# 4441
Delta R.T. 0.005 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37




Instrument :
MSVOA_N
ClientSampleId :
VN0402MBL01


Tgt Ion:146 Resp: 1807
Ion Ratio Lower Upper
146 100
111 28.0 19.7 59.1
148 33.0 32.3 96.8

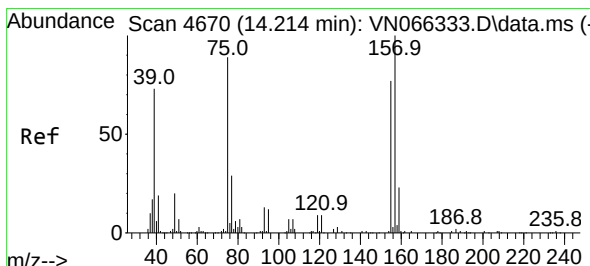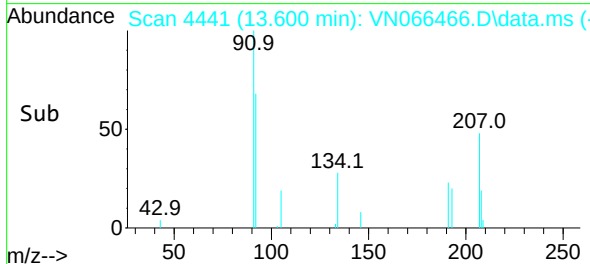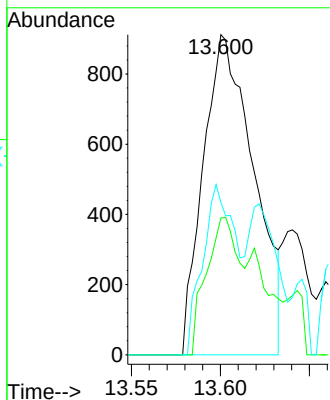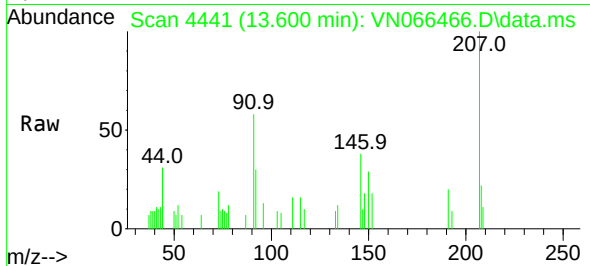

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.21 ug/l
RT: 14.220 min Scan# 4672
Delta R.T. -0.008 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37

Tgt Ion: 75 Resp: 253
Ion Ratio Lower Upper
75 100
155 0.0 43.8 131.3#
157 0.0 57.6 172.8#


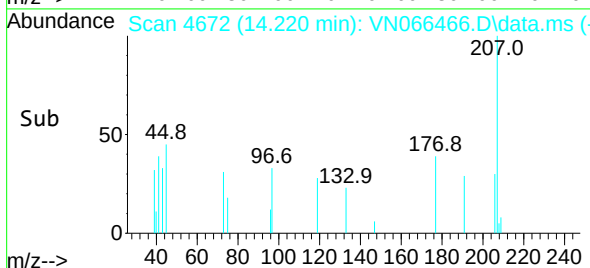
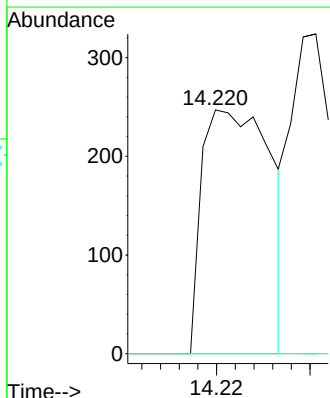
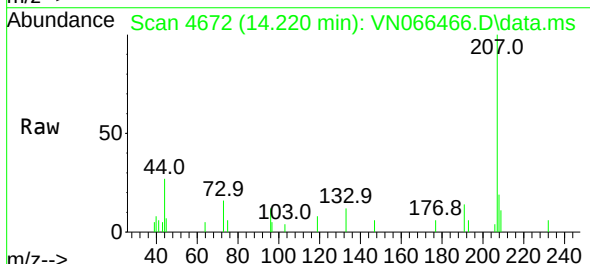


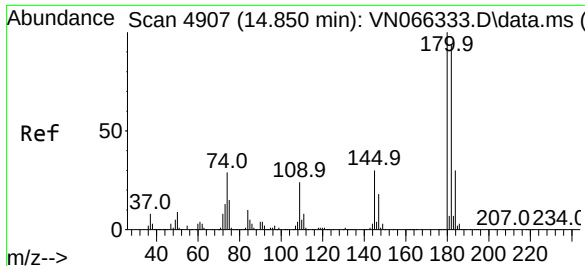

#93
1,2,4-Trichlorobenzene
Concen: 0.45 ug/l
RT: 14.984 min Scan# 4957
Delta R.T. 0.005 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37




Instrument :
MSVOA_N
ClientSampled :
VN0402MBL01


Tgt Ion:180 Resp: 2280
Ion Ratio Lower Upper
180 100
182 235.5 47.4 142.3#
145 69.6 14.2 42.8#

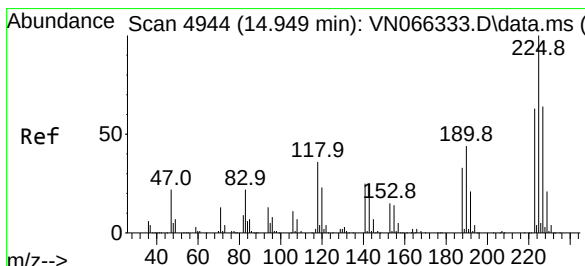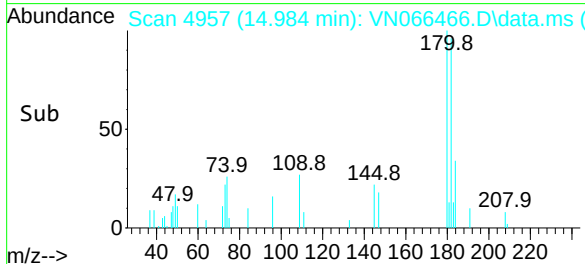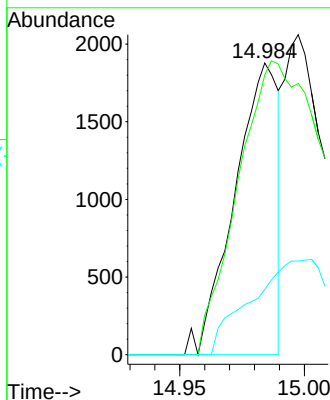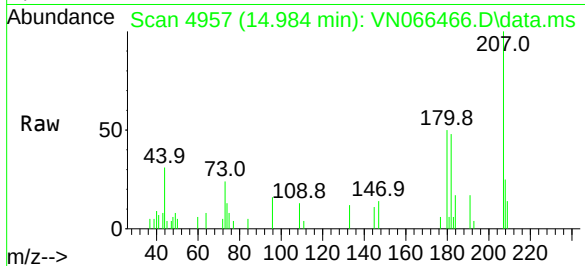

#94
Hexachlorobutadiene
Concen: 0.68 ug/l
RT: 15.102 min Scan# 5001
Delta R.T. -0.003 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37

Tgt Ion:225 Resp: 1878
Ion Ratio Lower Upper
225 100
223 67.0 31.1 93.5
227 58.8 32.1 96.3


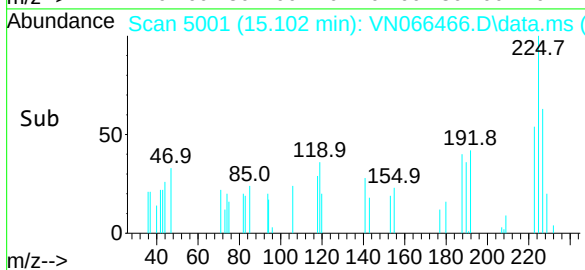
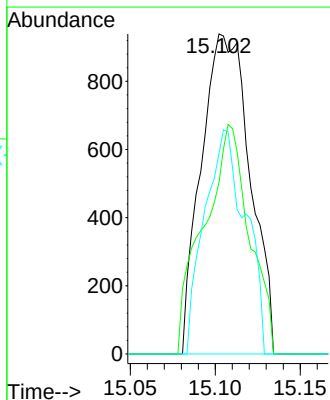
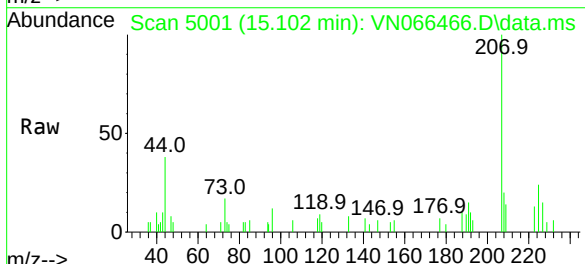




#95
Naphthalene
Concen: 3.55 ug/l
RT: 15.274 min Scan# 5065
Delta R.T. 0.013 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37

Instrument :
MSVOA_N
ClientSampleId :
VN0402MBL01

Tgt Ion:128 Resp: 37552
Ion Ratio Lower Upper
128 100
127 12.0 10.5 15.7
129 9.5 8.5 12.7



#96
1,2,3-Trichlorobenzene
Concen: 0.88 ug/l
RT: 15.504 min Scan# 5151
Delta R.T. 0.008 min
Lab File: VN066466.D
Acq: 2 Apr 2021 14:37

Tgt Ion:180 Resp: 4462
Ion Ratio Lower Upper
180 100
182 151.3 47.6 142.9#
145 50.1 15.4 46.1#

