

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN040222\
 Data File : VN071813.D
 Acq On : 02 Apr 2022 21:22
 Operator : JC\MD
 Sample : N2244-03
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-4-BD

Quant Time: Apr 04 01:10:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 31 01:57:54 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.081	168	663818	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.969	114	1132853	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	1162600	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.668	152	447019	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.433	65	381655	50.362	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 100.720%	
35) Dibromofluoromethane	8.022	113	320821	48.127	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 96.260%	
50) Toluene-d8	10.439	98	1436434	52.675	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 105.340%	
62) 4-Bromofluorobenzene	12.727	95	500429	56.741	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 113.480%	
Target Compounds						Qvalue
3) Chloromethane	2.269	50	34132	5.104	ug/l #	43
16) Acetone	4.293	43	6498	2.006	ug/l #	86
17) Carbon Disulfide	4.534	76	7858	0.625	ug/l	96
18) Methyl Acetate	4.863	43	1856	Below Cal	#	60
21) trans-1,2-Dichloroethene	5.604	96	2105	0.350	ug/l #	80
27) cis-1,2-Dichloroethene	7.328	96	84480	11.453	ug/l	88
31) Cyclohexane	8.081	56	13163	1.277	ug/l #	1
36) 1,1-Dichloropropene	8.081	75	45787	4.919	ug/l #	49
38) Carbon Tetrachloride	8.086	117	60716	6.655	ug/l #	16
40) Benzene	8.463	78	7148	0.243	ug/l	98
44) Trichloroethene	9.216	130	18985	2.506	ug/l	99
52) Toluene	10.504	92	18003	0.968	ug/l	97
60) Dibromochloromethane	10.969	129	17268	2.315	ug/l #	11
64) Tetrachloroethene	10.974	164	19538	2.545	ug/l	95
67) Ethyl Benzene	11.839	91	60643	1.539	ug/l	99
68) m/p-Xylenes	11.951	106	32832	2.168	ug/l	100
69) o-Xylene	12.274	106	71922	4.785	ug/l	98
73) Isopropylbenzene	12.580	105	11578	0.307	ug/l	98
76) 1,2,3-Trichloropropane	12.727	75	243799	23.543	ug/l #	1
78) n-propylbenzene	12.916	91	29900	0.755	ug/l	97
79) 2-Chlorotoluene	13.004	91	24260	0.955	ug/l	85
80) 1,3,5-Trimethylbenzene	13.057	105	17728	0.594	ug/l	96
81) trans-1,4-Dichloro-2-b...	12.727	75	243799	72.958	ug/l #	10
82) 4-Chlorotoluene	13.004	91	24260	1.030	ug/l	85
83) tert-Butylbenzene	13.368	119	8691	0.319	ug/l #	67
84) 1,2,4-Trimethylbenzene	13.363	105	62732	2.154	ug/l	97
89) n-Butylbenzene	13.939	91	4877	0.233	ug/l #	77
91) 1,2-Dichlorobenzene	13.986	146	3459	0.234	ug/l	98
93) 1,2,4-Trichlorobenzene	15.268	180	378	2.137	ug/l #	1
95) Naphthalene	15.509	128	26150	4.990	ug/l	98
96) 1,2,3-Trichlorobenzene	15.686	180	195	2.441	ug/l #	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Apr 04 01:10:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
Quant Title : SW846 8260
QLast Update : Thu Mar 31 01:57:54 2022
Response via : Initial Calibration









#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. -0.000 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22




Instrument :
MSVOA_N
ClientSampleId :
MW-4-BD


Tgt Ion:168 Resp: 663818
Ion Ratio Lower Upper
168 100
99 53.8 42.3 63.5

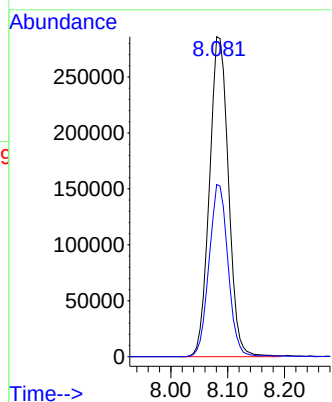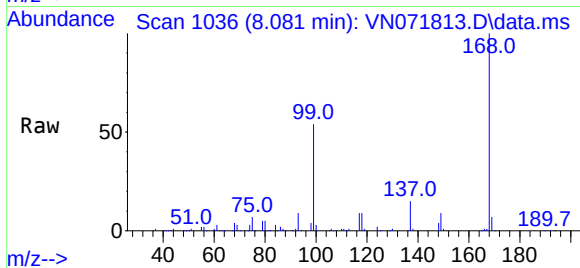

#3
Chloromethane
Concen: 5.104 ug/l
RT: 2.269 min Scan# 48
Delta R.T. -0.030 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22

Tgt Ion: 50 Resp: 34132
Ion Ratio Lower Upper
50 100
52 0.0 25.7 38.5#


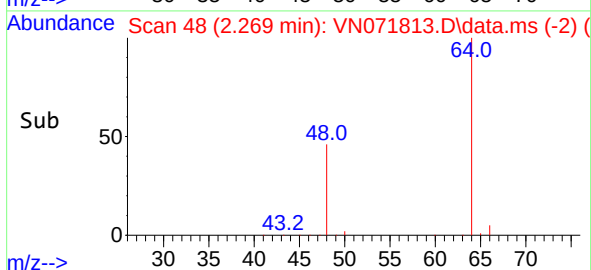

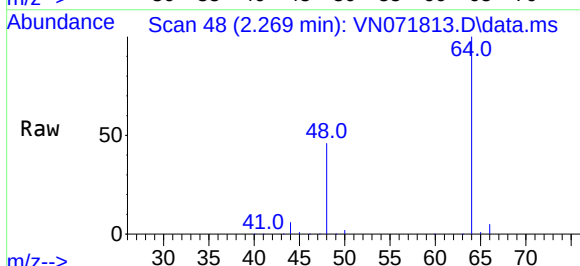




#16
Acetone
Concen: 2.006 ug/l
RT: 4.293 min Scan# 392
Delta R.T. 0.018 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22




Instrument :
MSVOA_N
ClientSampleId :
MW-4-BD


Tgt Ion: 43 Resp: 6498
Ion Ratio Lower Upper
43 100
58 40.6 26.0 39.0#

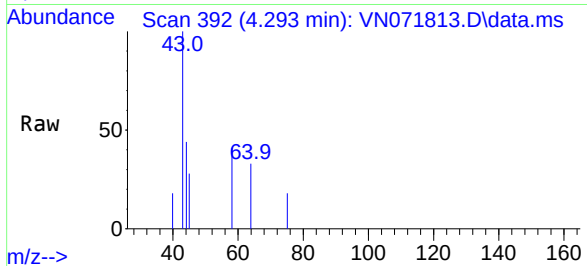

#17
Carbon Disulfide
Concen: 0.625 ug/l
RT: 4.534 min Scan# 433
Delta R.T. -0.000 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22

Tgt Ion: 76 Resp: 7858
Ion Ratio Lower Upper
76 100
78 10.4 7.2 10.8


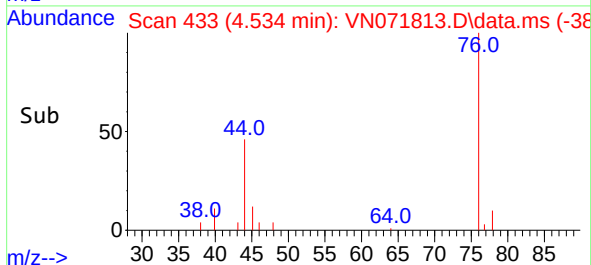

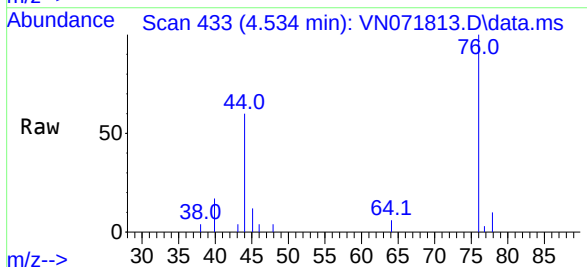




#18
Methyl Acetate
Concen: Below Cal
RT: 4.863 min Scan# 41
Delta R.T. 0.017 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22




Instrument :
MSVOA_N
ClientSampleId :
MW-4-BD


Tgt Ion: 43 Resp: 1856
Ion Ratio Lower Upper
43 100
74 6.3 21.6 32.4#



#21
trans-1,2-Dichloroethene
Concen: 0.350 ug/l
RT: 5.604 min Scan# 615
Delta R.T. 0.005 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22

Tgt Ion: 96 Resp: 2105
Ion Ratio Lower Upper
96 100
61 107.2 105.8 158.8
98 48.9 50.3 75.5#


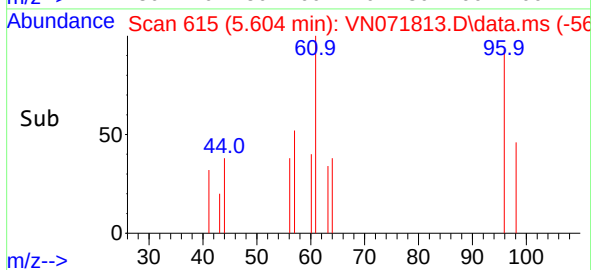






#27
cis-1,2-Dichloroethene
Concen: 11.453 ug/l
RT: 7.328 min Scan# 90
Delta R.T. 0.006 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22




Instrument :
MSVOA_N
ClientSampleId :
MW-4-BD


Tgt Ion: 96 Resp: 84480
Ion Ratio Lower Upper
96 100
61 118.3 0.0 280.6
98 64.2 0.0 128.4

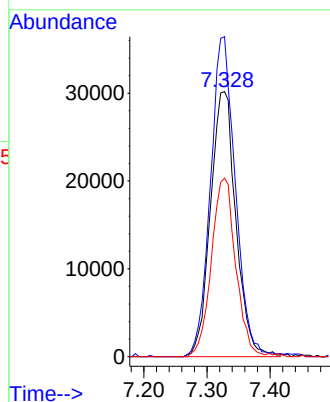

#31
Cyclohexane
Concen: 1.277 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. -0.011 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22

Tgt Ion: 56 Resp: 13163
Ion Ratio Lower Upper
56 100
69 163.2 27.8 41.8#
84 161.2 76.9 115.3#


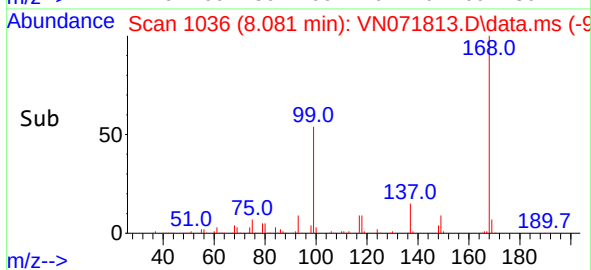




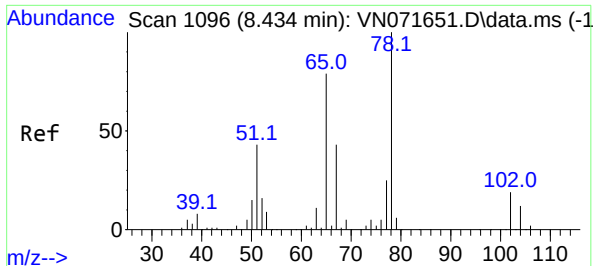

#33
1,2-Dichloroethane-d4
Concen: 50.362 ug/l
RT: 8.433 min Scan# 1096
Delta R.T. -0.001 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22




Instrument :
MSVOA_N
ClientSampleId :
MW-4-BD


Tgt Ion: 65 Resp: 381655
Ion Ratio Lower Upper
65 100
67 52.0 0.0 104.8

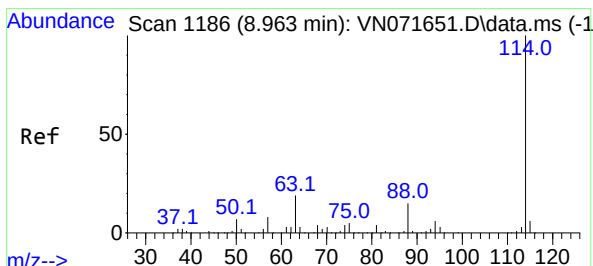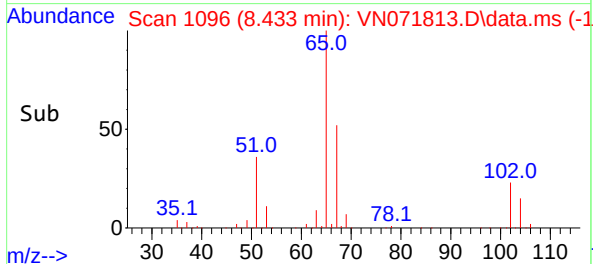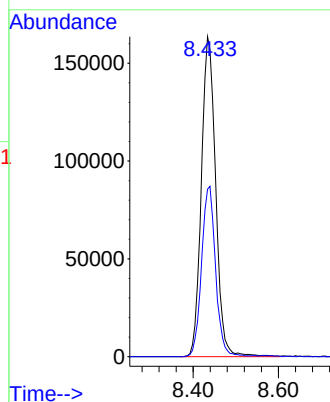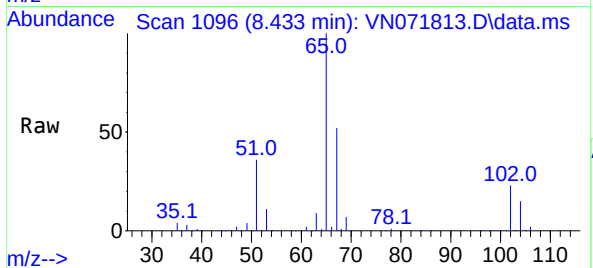

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.969 min Scan# 1187
Delta R.T. 0.006 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22

Tgt Ion:114 Resp: 1132853
Ion Ratio Lower Upper
114 100
63 19.0 0.0 40.0
88 16.3 0.0 32.6


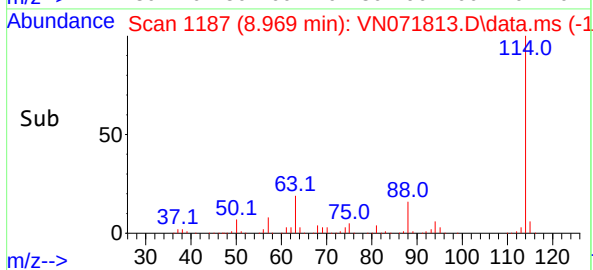
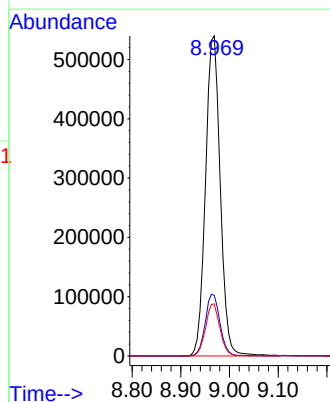
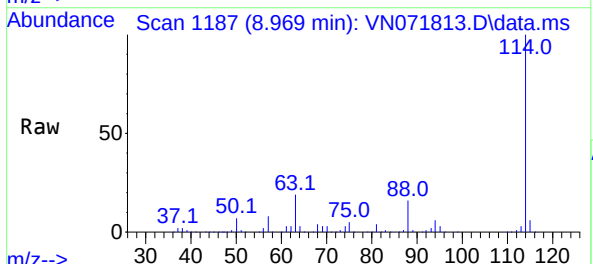


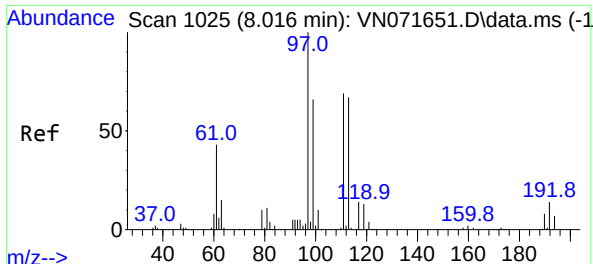

#35
Dibromofluoromethane
Concen: 48.127 ug/l
RT: 8.022 min Scan# 1026
Delta R.T. 0.006 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22




Instrument :
MSVOA_N
ClientSampleId :
MW-4-BD


Tgt Ion:113 Resp: 320821
Ion Ratio Lower Upper
113 100
111 103.4 81.4 122.0
192 22.0 17.0 25.6

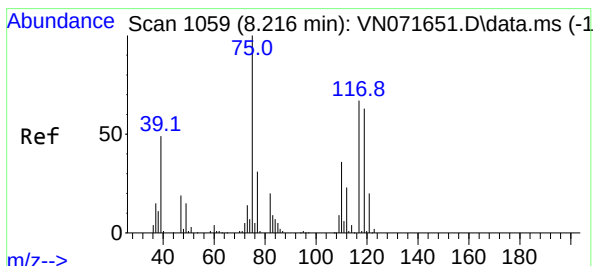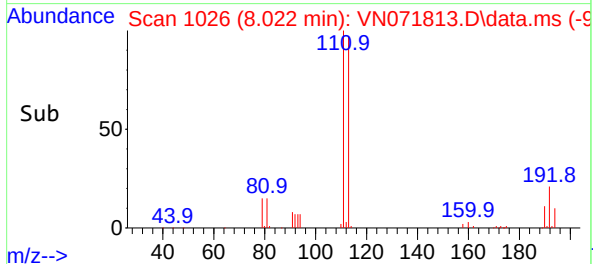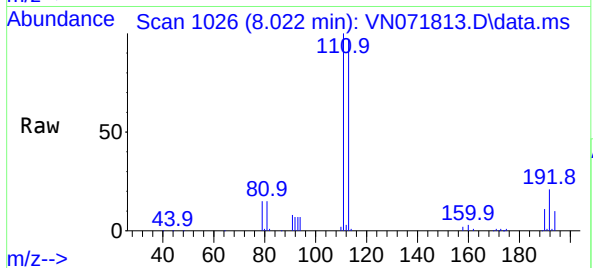

#36
1,1-Dichloropropene
Concen: 4.919 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. -0.135 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22

Tgt Ion: 75 Resp: 45787
Ion Ratio Lower Upper
75 100
110 9.0 18.3 54.8#
77 0.0 25.1 37.7#


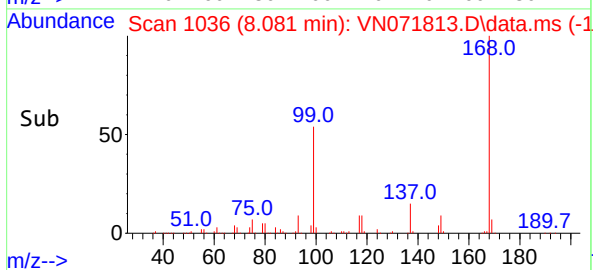

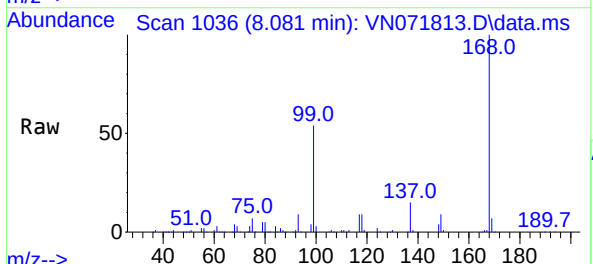


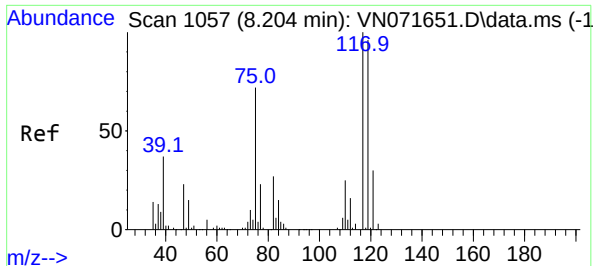

#38
Carbon Tetrachloride
Concen: 6.655 ug/l
RT: 8.086 min Scan# 1101
Delta R.T. -0.118 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22




Instrument :
MSVOA_N
ClientSampleId :
MW-4-BD


Tgt Ion:117 Resp: 60716
Ion Ratio Lower Upper
117 100
119 4.6 75.8 113.8#
121 0.0 24.6 37.0#

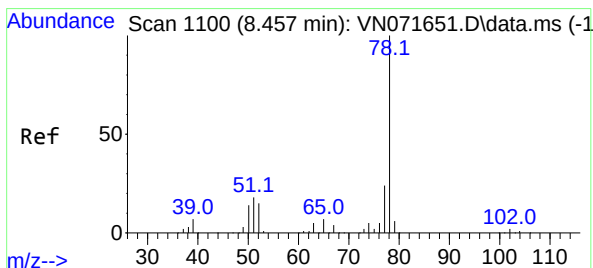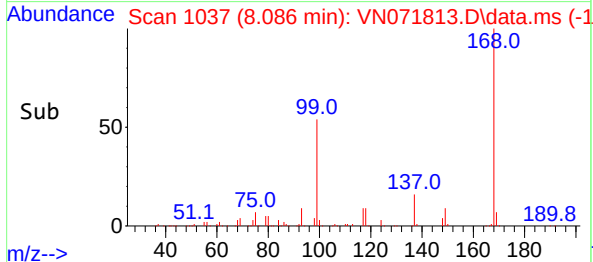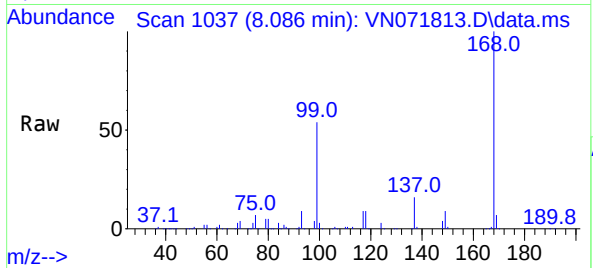

#40
Benzene
Concen: 0.243 ug/l
RT: 8.463 min Scan# 1101
Delta R.T. 0.006 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22

Tgt Ion: 78 Resp: 7148
Ion Ratio Lower Upper
78 100
77 25.2 19.4 29.0


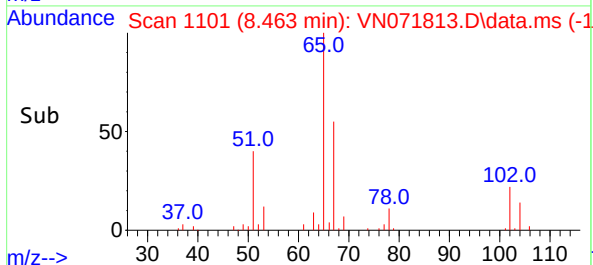
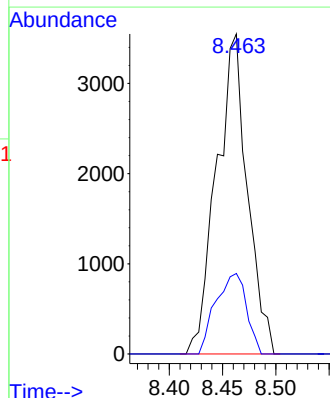
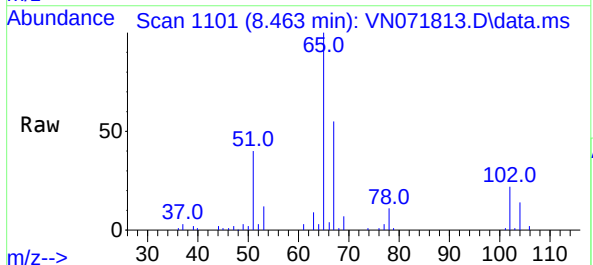


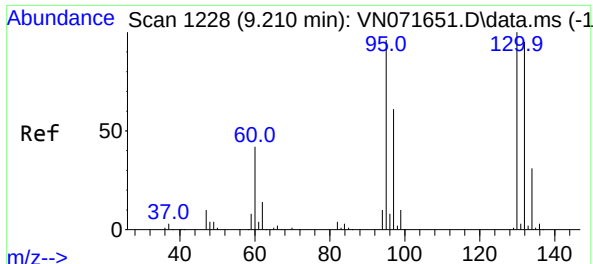

#44
Trichloroethene
Concen: 2.506 ug/l
RT: 9.216 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22




Instrument :
MSVOA_N
ClientSampleId :
MW-4-BD


Tgt Ion:130 Resp: 18985
Ion Ratio Lower Upper
130 100
95 94.3 0.0 186.8

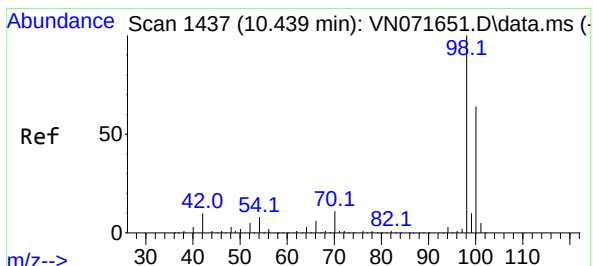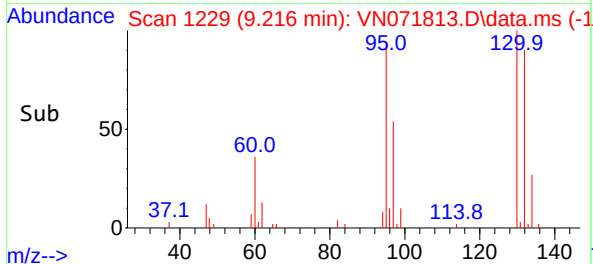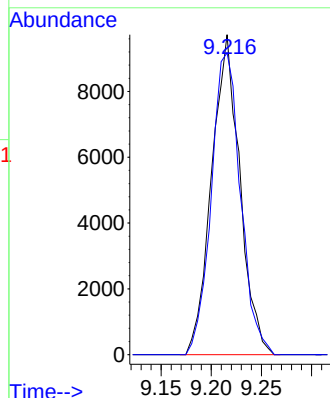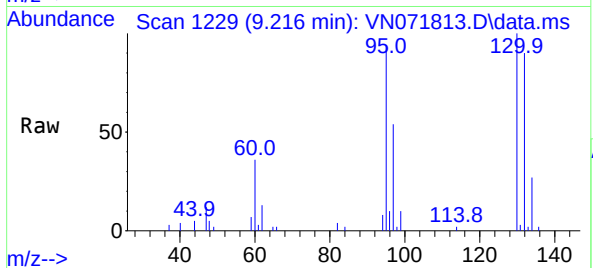

#50
Toluene-d8
Concen: 52.675 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. 0.000 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22

Tgt Ion: 98 Resp: 1436434
Ion Ratio Lower Upper
98 100
100 64.7 52.6 78.8


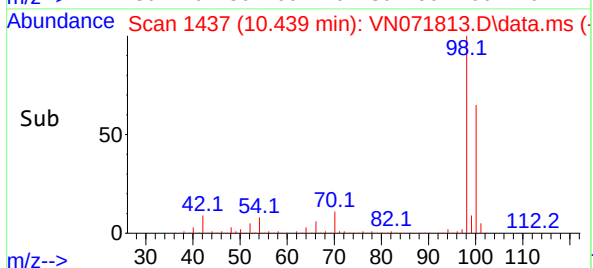

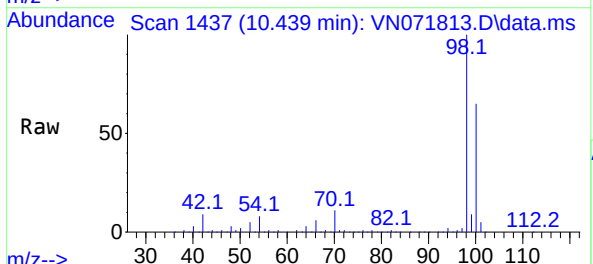




#52
Toluene
Concen: 0.968 ug/l
RT: 10.504 min Scan# 1447
Delta R.T. 0.006 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22




Instrument :
MSVOA_N
ClientSampleId :
MW-4-BD


Tgt Ion: 92 Resp: 18003
Ion Ratio Lower Upper
92 100
91 177.8 138.6 207.8

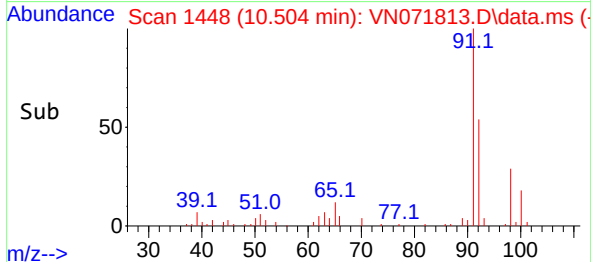

#60
Dibromochloromethane
Concen: 2.315 ug/l
RT: 10.969 min Scan# 1527
Delta R.T. -0.264 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22

Tgt Ion: 129 Resp: 17268
Ion Ratio Lower Upper
129 100
127 0.0 38.8 116.4#


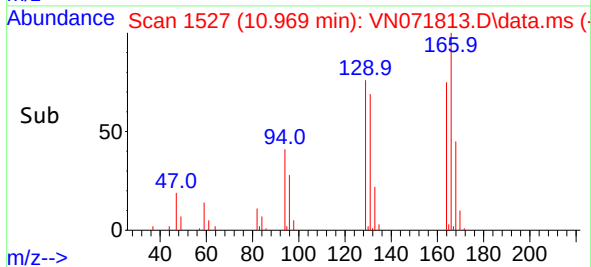

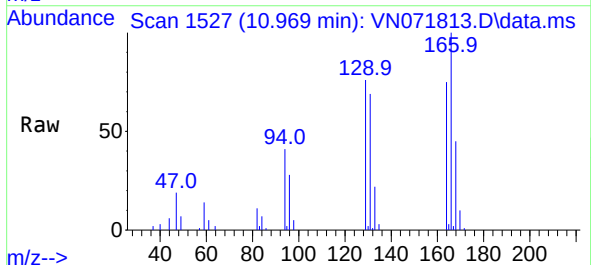


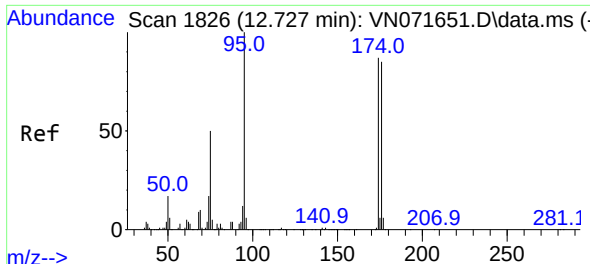

#62
4-Bromofluorobenzene
Concen: 56.741 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22




Instrument :
MSVOA_N
ClientSampleId :
MW-4-BD


Tgt Ion: 95 Resp: 500429
Ion Ratio Lower Upper
95 100
174 84.9 0.0 167.6
176 80.5 0.0 163.4

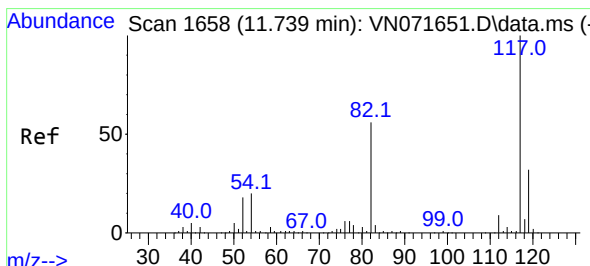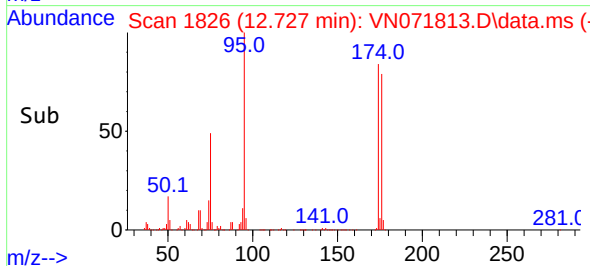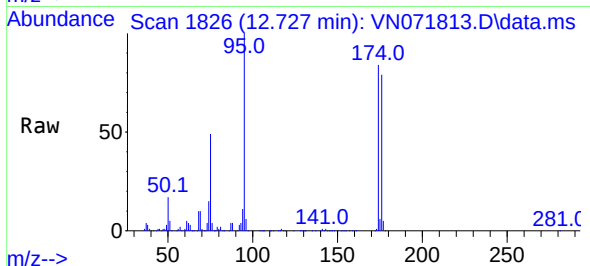

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 1658
Delta R.T. 0.000 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22

Tgt Ion: 117 Resp: 1162600
Ion Ratio Lower Upper
117 100
82 56.6 44.2 66.2
119 31.8 25.4 38.0


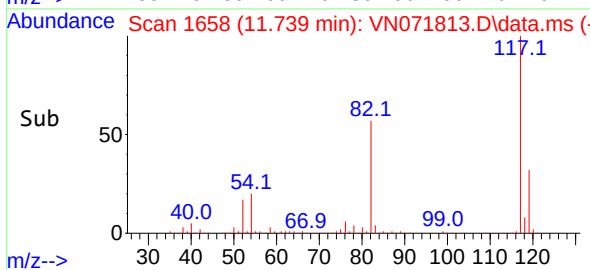

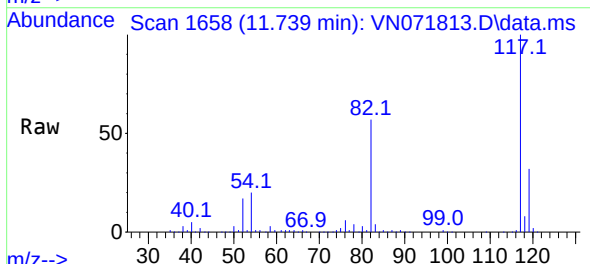




#64
Tetrachloroethene
Concen: 2.545 ug/l
RT: 10.974 min Scan# 11
Delta R.T. -0.001 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22




Instrument :
MSVOA_N
ClientSampleId :
MW-4-BD


Tgt Ion:164 Resp: 19538
Ion Ratio Lower Upper
164 100
166 125.5 104.2 156.2
129 90.2 73.9 110.9
131 96.0 69.4 104.2

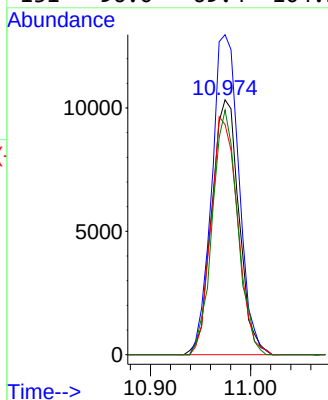

#67
Ethyl Benzene
Concen: 1.539 ug/l
RT: 11.839 min Scan# 1675
Delta R.T. 0.000 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22

Tgt Ion: 91 Resp: 60643
Ion Ratio Lower Upper
91 100
106 31.4 24.9 37.3


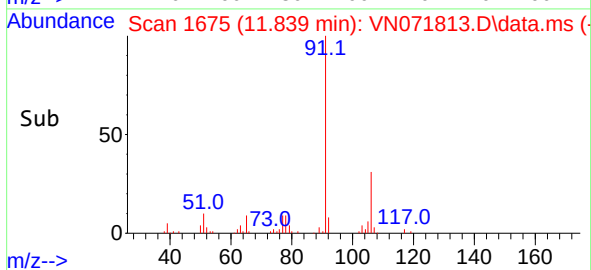
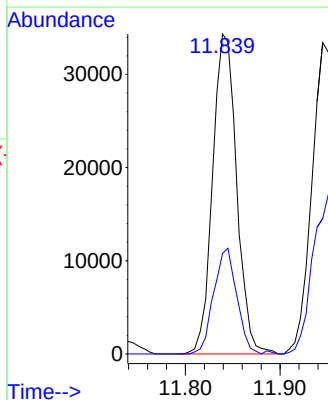





#68
m/p-Xylenes
Concen: 2.168 ug/l
RT: 11.951 min Scan# 1694
Delta R.T. -0.000 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22




Instrument :
MSVOA_N
ClientSampleId :
MW-4-BD


Tgt Ion:106 Resp: 32832
Ion Ratio Lower Upper
106 100
91 198.0 158.9 238.3



#69
o-Xylene
Concen: 4.785 ug/l
RT: 12.274 min Scan# 1749
Delta R.T. -0.001 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22

Tgt Ion:106 Resp: 71922
Ion Ratio Lower Upper
106 100
91 209.6 106.0 318.0



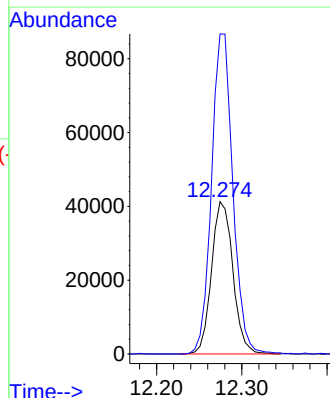





#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.668 min Scan# 1986
Delta R.T. -0.001 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22




Instrument :
MSVOA_N
ClientSampleId :
MW-4-BD


Tgt Ion:152 Resp: 447019
Ion Ratio Lower Upper
152 100
115 57.0 28.9 86.7
150 157.5 0.0 356.2

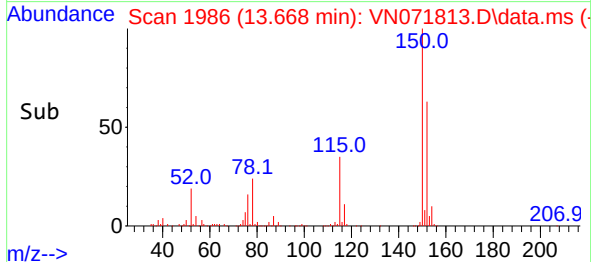

#73
Isopropylbenzene
Concen: 0.307 ug/l
RT: 12.580 min Scan# 1801
Delta R.T. 0.005 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22

Tgt Ion:105 Resp: 11578
Ion Ratio Lower Upper
105 100
120 28.1 13.5 40.4


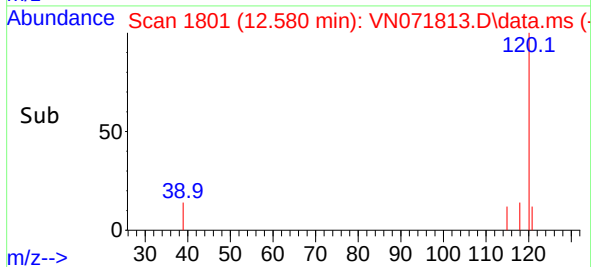

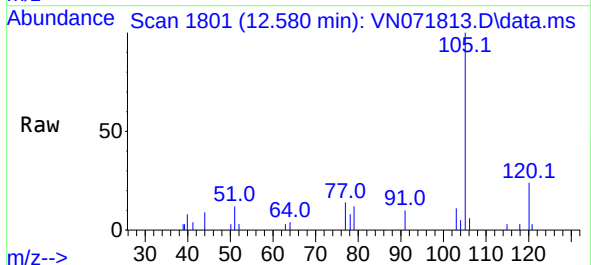




#76
1,2,3-Trichloropropane
Concen: 23.543 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. -0.147 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22




Instrument :
MSVOA_N
ClientSampleId :
MW-4-BD


Tgt Ion: 75 Resp: 243799
Ion Ratio Lower Upper
75 100
77 1.2 98.5 295.5#



#78
n-propylbenzene
Concen: 0.755 ug/l
RT: 12.916 min Scan# 1858
Delta R.T. -0.000 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22

Tgt Ion: 91 Resp: 29900
Ion Ratio Lower Upper
91 100
120 22.1 11.9 35.5









#79
2-Chlorotoluene
Concen: 0.955 ug/l
RT: 13.004 min Scan# 1873
Delta R.T. -0.000 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22




Instrument :
MSVOA_N
ClientSampleId :
MW-4-BD


Tgt Ion: 91 Resp: 24260
Ion Ratio Lower Upper
91 100
126 26.0 17.3 51.9



#80
1,3,5-Trimethylbenzene
Concen: 0.594 ug/l
RT: 13.057 min Scan# 1882
Delta R.T. 0.006 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22

Tgt Ion: 105 Resp: 17728
Ion Ratio Lower Upper
105 100
120 52.6 24.9 74.7



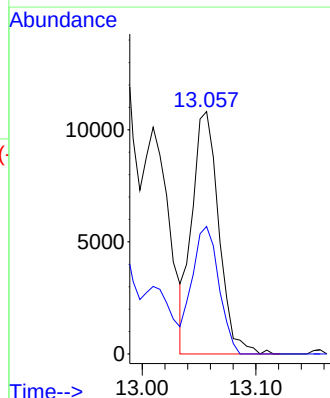





#81
trans-1,4-Dichloro-2-butene
Concen: 72.958 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.105 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22




Instrument :
MSVOA_N
ClientSampleId :
MW-4-BD


Tgt Ion: 75 Resp: 243799
Ion Ratio Lower Upper
75 100
53 0.0 78.0 117.0#
89 0.0 37.2 55.8#



#82
4-Chlorotoluene
Concen: 1.030 ug/l
RT: 13.004 min Scan# 1873
Delta R.T. -0.094 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22

Tgt Ion: 91 Resp: 24260
Ion Ratio Lower Upper
91 100
126 26.0 17.2 51.6









#83
tert-Butylbenzene
Concen: 0.319 ug/l
RT: 13.368 min Scan# 1926
Delta R.T. 0.052 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22




Instrument :
MSVOA_N
ClientSampleId :
MW-4-BD


Tgt Ion:119 Resp: 8691
Ion Ratio Lower Upper
119 100
91 82.3 31.6 94.8
134 0.0 13.7 41.1#

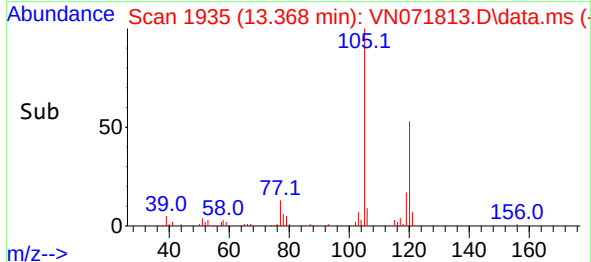

#84
1,2,4-Trimethylbenzene
Concen: 2.154 ug/l
RT: 13.363 min Scan# 1934
Delta R.T. -0.000 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22

Tgt Ion:105 Resp: 62732
Ion Ratio Lower Upper
105 100
120 44.8 23.3 69.8


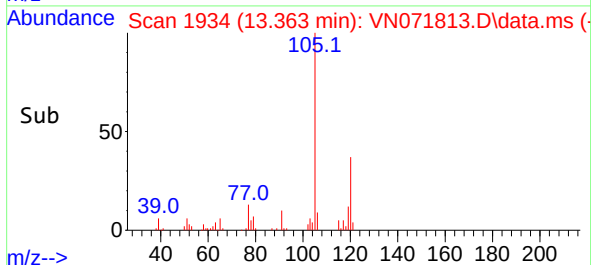

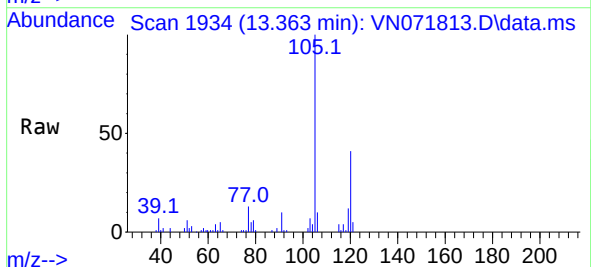




#89
n-Butylbenzene
Concen: 0.233 ug/l
RT: 13.939 min Scan# 2032
Delta R.T. -0.000 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22




Instrument :
MSVOA_N
ClientSampleId :
MW-4-BD


Tgt Ion: 91 Resp: 4877
Ion Ratio Lower Upper
91 100
92 48.2 26.9 80.7
134 0.0 13.6 40.8#



#91
1,2-Dichlorobenzene
Concen: 0.234 ug/l
RT: 13.986 min Scan# 2040
Delta R.T. 0.006 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22

Tgt Ion:146 Resp: 3459
Ion Ratio Lower Upper
146 100
111 44.8 20.9 62.8
148 63.5 32.1 96.3


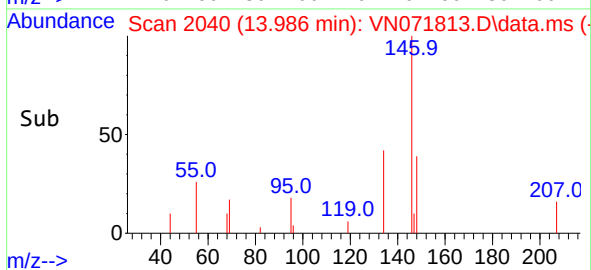






#93
1,2,4-Trichlorobenzene
Concen: 2.137 ug/l
RT: 15.268 min Scan# 21
Delta R.T. 0.011 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22




Instrument :
MSVOA_N
ClientSampleId :
MW-4-BD


Tgt Ion:180 Resp: 378
Ion Ratio Lower Upper
180 100
182 97.9 47.5 142.5
145 636.5 14.5 43.5#

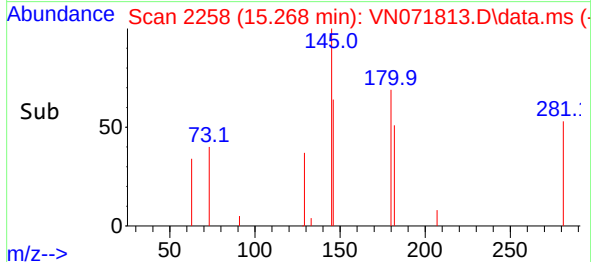

#95
Naphthalene
Concen: 4.990 ug/l
RT: 15.509 min Scan# 2299
Delta R.T. 0.011 min
Lab File: VN071813.D
Acq: 02 Apr 2022 21:22

Tgt Ion:128 Resp: 26150
Ion Ratio Lower Upper
128 100
127 11.8 10.3 15.5
129 10.3 8.6 13.0

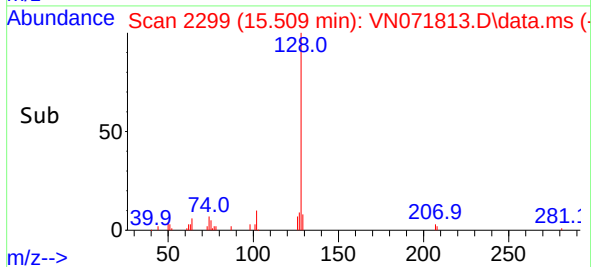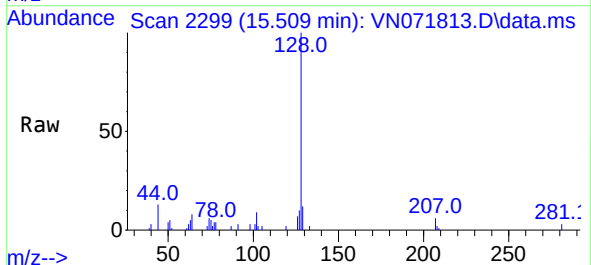



#96

1,2,3-Trichlorobenzene

Concen: 2.441 ug/l

RT: 15.686 min Scan# 21

Delta R.T. -0.006 min

Lab File: VN071813.D


Acq: 02 Apr 2022 21:22

Instrument :

MSVOA_N

ClientSampleId :

MW-4-BD



Tgt Ion:180 Resp: 195

Ion Ratio Lower Upper

180 100

182 57.9 47.8 143.3

145 337.4 15.5 46.5#

