


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN040222\
Data File : VN071796.D
Acq On : 02 Apr 2022 13:00
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
Title : SW846 8260
Last Update : Thu Mar 31 01:57:54 2022

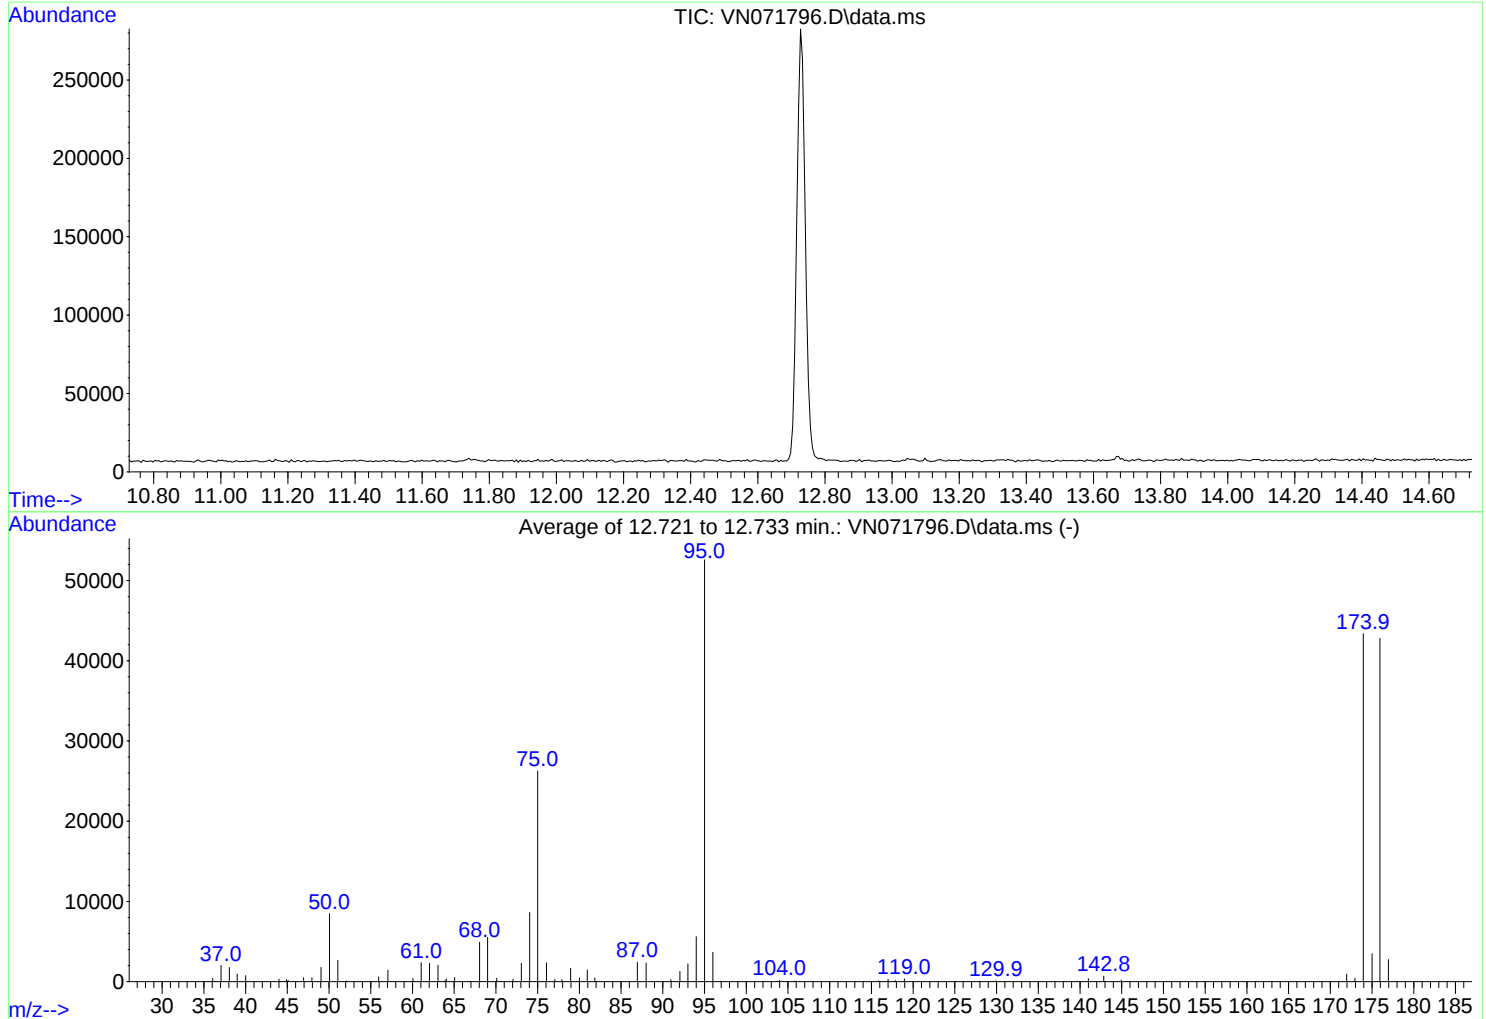

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1817

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	8477	PASS
75	95	30	60	50.0	26277	PASS
95	95	100	100	100.0	52581	PASS
96	95	5	9	6.9	3648	PASS
173	174	0.00	2	1.0	421	PASS
174	95	50	100	82.5	43363	PASS
175	174	5	9	8.0	3466	PASS
176	174	95	101	98.7	42811	PASS
177	176	5	9	6.4	2757	PASS