
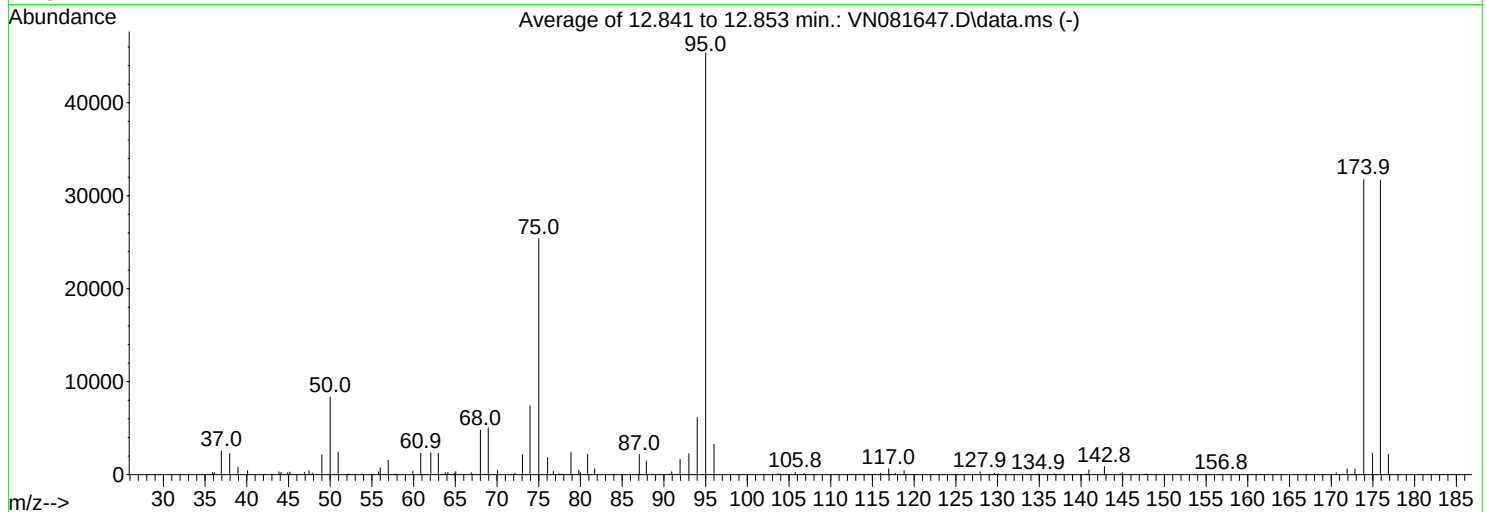


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN040224\
Data File : VN081647.D
Acq On : 02 Apr 2024 08:34
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031824W.M
Title : SW846 8260
Last Update : Tue Mar 19 06:00:00 2024

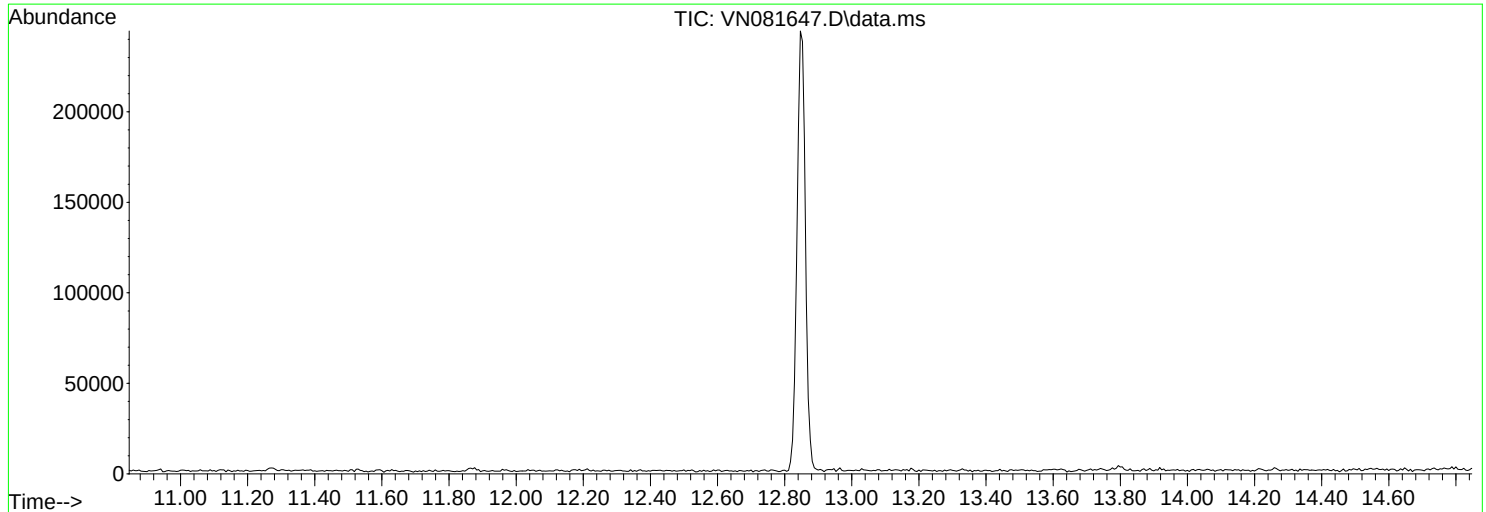

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.4	8360	PASS
75	95	30	60	56.0	25408	PASS
95	95	100	100	100.0	45368	PASS
96	95	5	9	7.2	3256	PASS
173	174	0.00	2	1.9	604	PASS
174	95	50	100	70.0	31757	PASS
175	174	5	9	7.2	2300	PASS
176	174	95	101	99.8	31683	PASS
177	176	5	9	6.9	2194	PASS

Average of 12.841 to 12.853 min.: VN081647.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	242	47.45	423	57.80	63	68.00	479
36.10	219	47.85	167	59.90	362	68.95	501
36.95	2541	49.00	2128	60.85	2301	70.05	45
37.95	2281	50.00	8360	62.05	2342	71.80	5
38.95	815	50.95	2422	62.95	2298	72.15	158
40.10	434	52.20	74	63.80	211	73.05	2155
43.85	315	53.00	64	64.10	241	73.95	7435
44.10	255	53.80	90	64.90	134	75.00	25408
44.90	220	55.80	310	65.05	332	76.05	1820
45.15	270	56.00	727	66.90	212	76.75	343
46.90	247	56.95	1533	67.10	72	77.40	101

Average of 12.841 to 12.853 min.: VN081647.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.70	80	90.95	316	116.95	640	144.70	90
78.85	2414	91.95	1639	117.75	147	144.95	224
79.80	479	93.00	2256	118.80	433	147.70	52
80.00	222	94.00	6147	127.90	311	147.90	89
80.85	2188	95.00	45368	129.65	158	154.90	54
81.70	645	96.00	3256	130.10	105	156.80	61
85.90	57	103.70	137	134.90	80	170.60	207
87.05	2166	104.00	92	136.80	108	171.90	623
87.90	1445	105.75	259	140.70	97	172.85	604
88.70	51	106.80	134	140.95	492	173.90	31757
90.70	70	115.95	162	142.80	860	174.95	2300

Average of 12.841 to 12.853 min.: VN081647.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
175.90	31683						
176.85	2194						

Instrument :

MSVOA_N

ClientSampleId :

BFB