
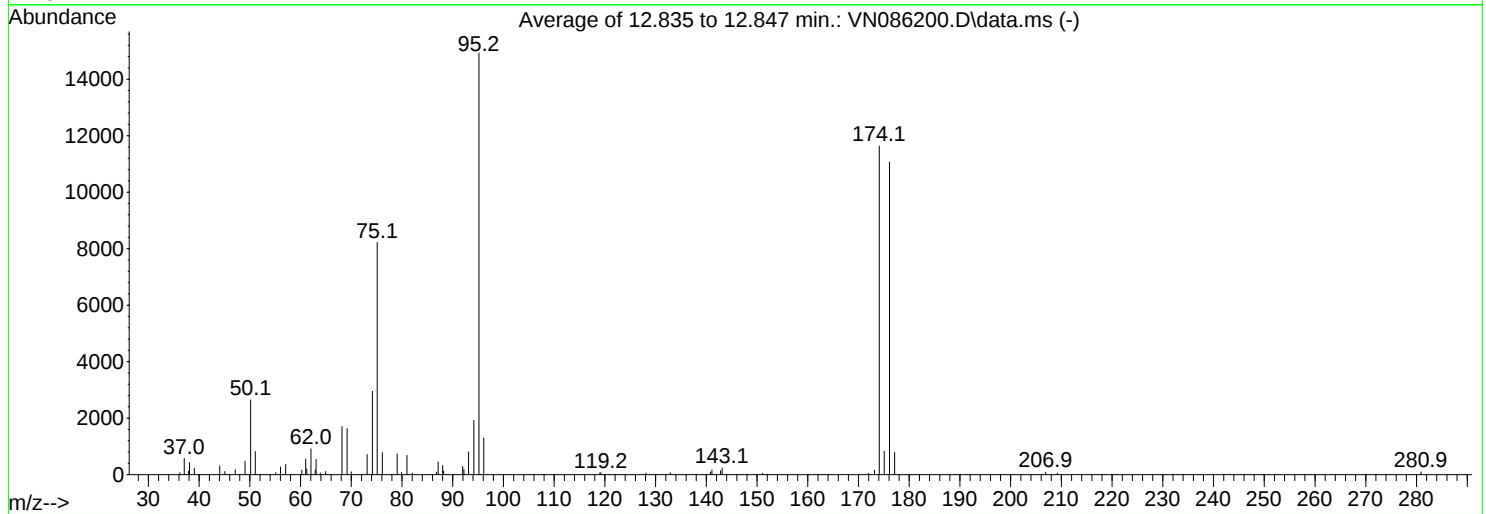


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN040225\
Data File : VN086200.D
Acq On : 02 Apr 2025 09:42
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031825W.M
Title : SW846 8260
Last Update : Wed Mar 19 03:20:56 2025

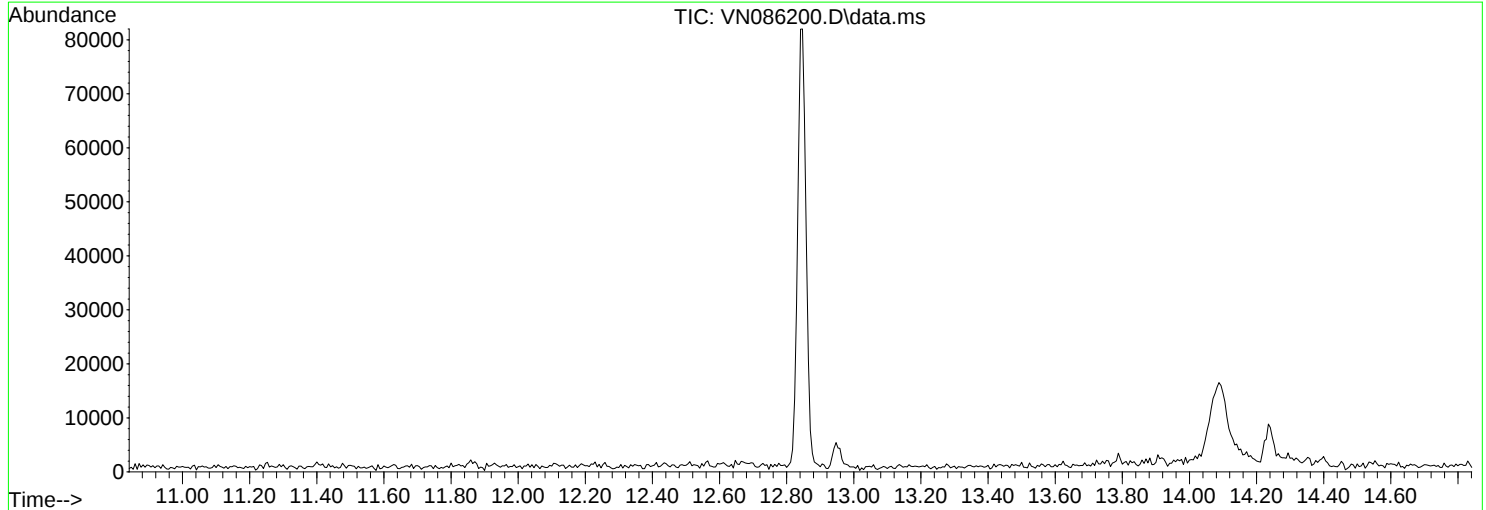

AutoFind: Scans 1850, 1851, 1852; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.7	2645	PASS
75	95	30	60	55.0	8217	PASS
95	95	100	100	100.0	14933	PASS
96	95	5	9	8.7	1300	PASS
173	174	0.00	2	1.3	157	PASS
174	95	50	100	77.9	11638	PASS
175	174	5	9	7.1	827	PASS
176	174	95	101	95.1	11066	PASS
177	176	5	9	7.1	784	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.20	70	55.10	73	68.15	1705	86.80	81
37.05	575	56.05	272	69.15	1629	87.10	45
37.90	127	57.05	361	70.00	103	88.00	32
38.10	425	60.25	167	73.10	713	88.20	13
39.05	229	61.00	551	74.15	2954	91.95	288
44.05	307	61.20	206	75.10	8217	92.20	194
45.05	115	62.05	912	76.10	784	93.10	807
47.10	178	62.90	164	79.05	731	94.15	1923
49.05	476	63.05	539	79.90	78	95.15	14933
50.15	2645	63.90	56	80.95	688	96.10	1300
51.05	817	64.95	111	82.00	57	119.00	66

Average of 12.835 to 12.847 min.: VN086200.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
119.20	70	175.05	827				
128.10	55	176.10	11066				
132.90	68	177.10	784				
140.80	88	206.90	86				
141.10	162	209.20	59				
142.80	142	280.90	97				
143.10	231						
151.10	52						
171.90	53						
173.15	157						
174.10	11638						

Instrument :

MSVOA_N

ClientSampleId :

BFB