


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN040324\
Data File : VN081657.D
Acq On : 03 Apr 2024 08:43
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031824W.M
Title : SW846 8260
Last Update : Tue Mar 19 06:00:00 2024

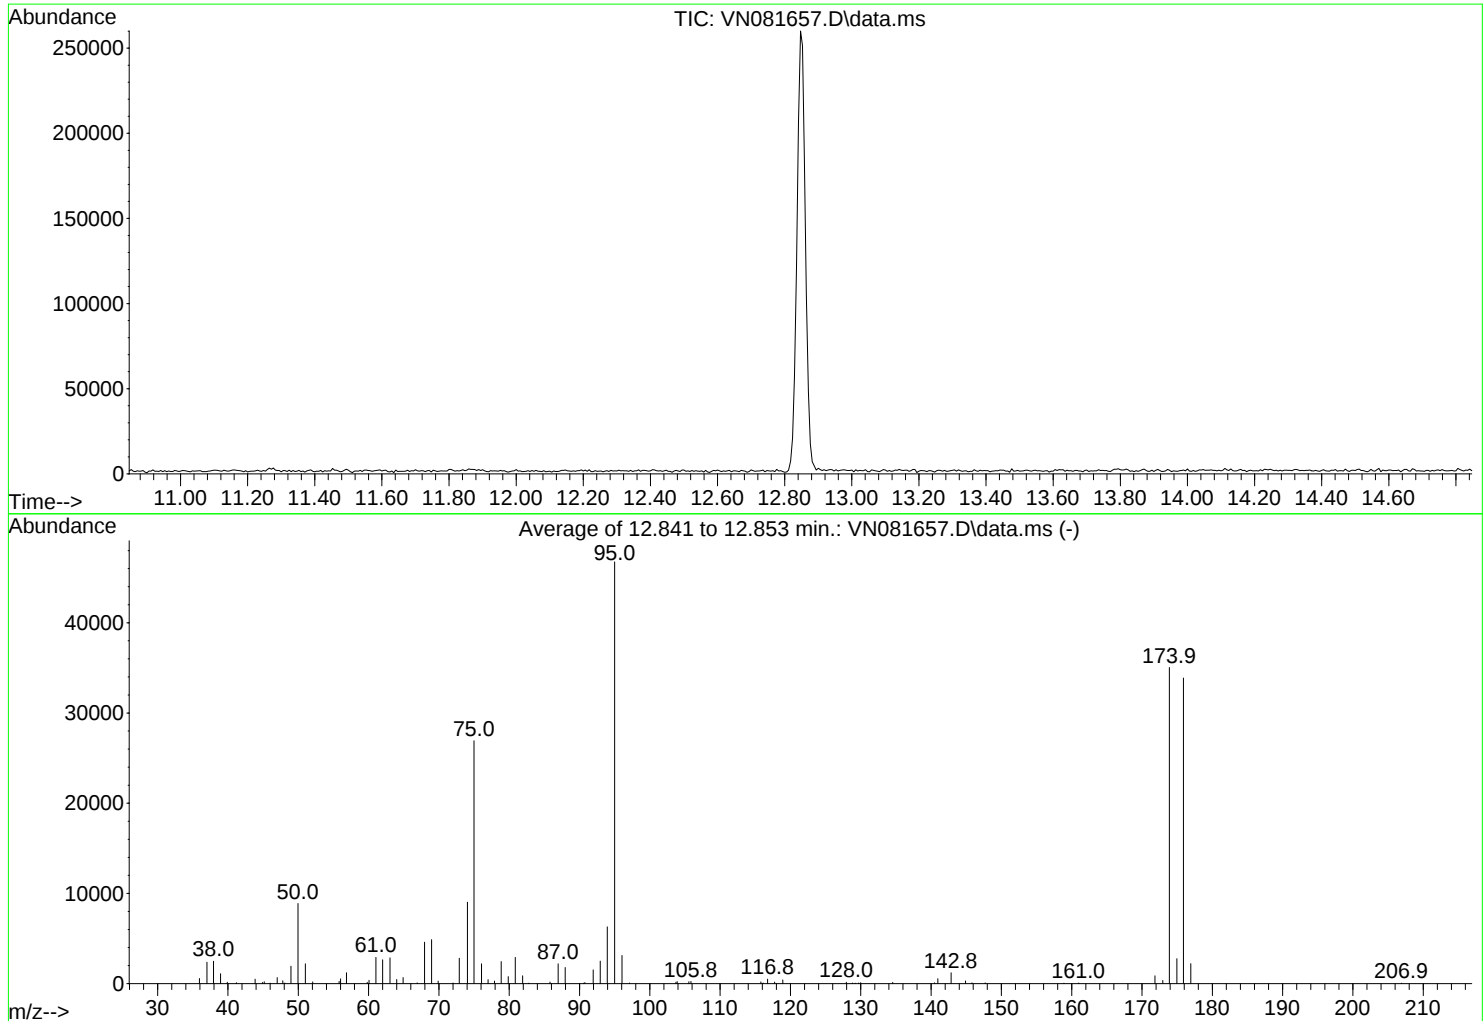

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.0	8882	PASS
75	95	30	60	57.6	26928	PASS
95	95	100	100	100.0	46755	PASS
96	95	5	9	6.7	3114	PASS
173	174	0.00	2	1.0	351	PASS
174	95	50	100	75.0	35045	PASS
175	174	5	9	7.9	2760	PASS
176	174	95	101	96.7	33880	PASS
177	176	5	9	6.6	2222	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	564	47.80	325	61.05	2913	74.05	902
37.00	2376	48.10	75	62.00	2650	75.00	2692
37.95	2485	48.95	1941	63.05	2848	76.05	220
38.95	1099	49.95	8882	64.00	460	77.00	44
39.90	163	51.00	2198	64.90	668	77.90	290
41.20	109	52.05	197	66.90	87	78.85	2448
43.85	505	55.80	252	67.95	4597	79.85	777
44.90	122	56.00	536	68.95	4880	80.85	2909
45.15	223	56.85	1203	69.90	284	81.90	877
46.00	55	59.80	135	72.00	71	82.80	52
47.00	672	60.05	381	72.90	2820	85.80	175

Average of 12.841 to 12.853 min.: VN081657.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
86.95	2209	103.90	224	129.70	73	171.85	879
87.95	1785	105.55	210	130.00	103	172.95	351
90.60	52	105.85	245	134.55	144	173.90	35045
90.75	116	115.80	197	140.50	98	174.95	2760
91.95	1518	116.10	65	140.95	559	175.90	33880
92.95	2509	116.75	502	142.85	1202	176.95	2222
93.95	6300	117.75	171	144.90	294	206.90	50
95.00	46755	118.90	413	145.80	84		
96.05	3114	127.95	152	147.70	97		
97.10	72	128.80	67	158.90	51		
103.70	156	129.20	54	161.00	74		

Instrument :

MSVOA_N

ClientSampleId :

BFB