


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN040419\
Data File : VN054935.D
Acq On : 4 Apr 2019 8:48
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N040419W.M
Title : SW846 8260
Last Update : Fri Apr 05 02:23:47 2019

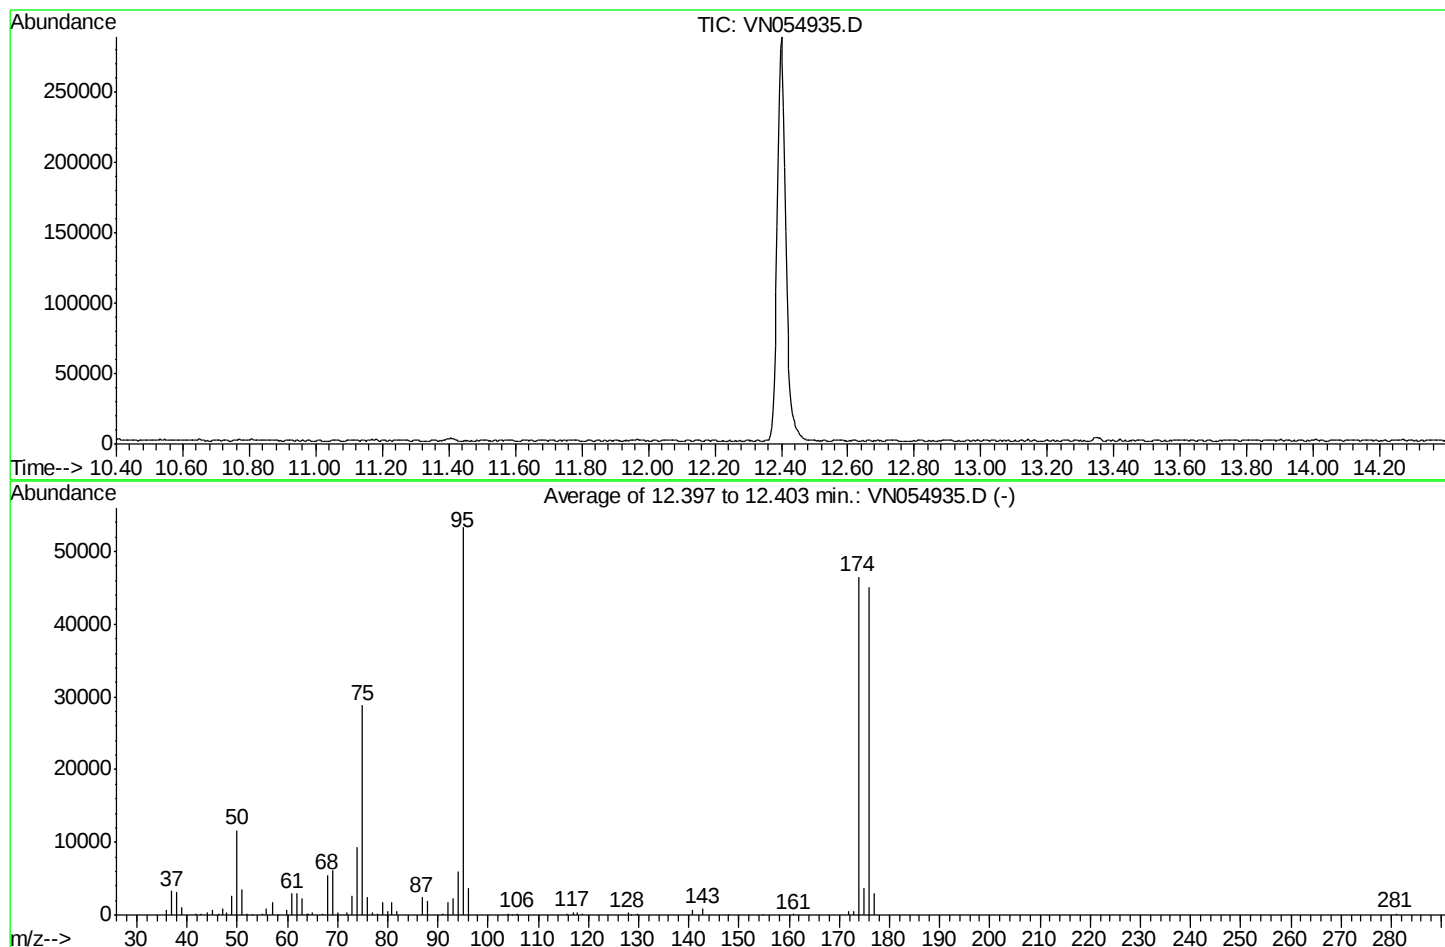

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	11694	PASS
75	95	30	60	54.0	28816	PASS
95	95	100	100	100.0	53320	PASS
96	95	5	9	7.1	3784	PASS
173	174	0.00	2	1.1	513	PASS
174	95	50	100	87.2	46514	PASS
175	174	5	9	7.9	3674	PASS
176	174	95	101	96.9	45072	PASS
177	176	5	9	6.6	2974	PASS