
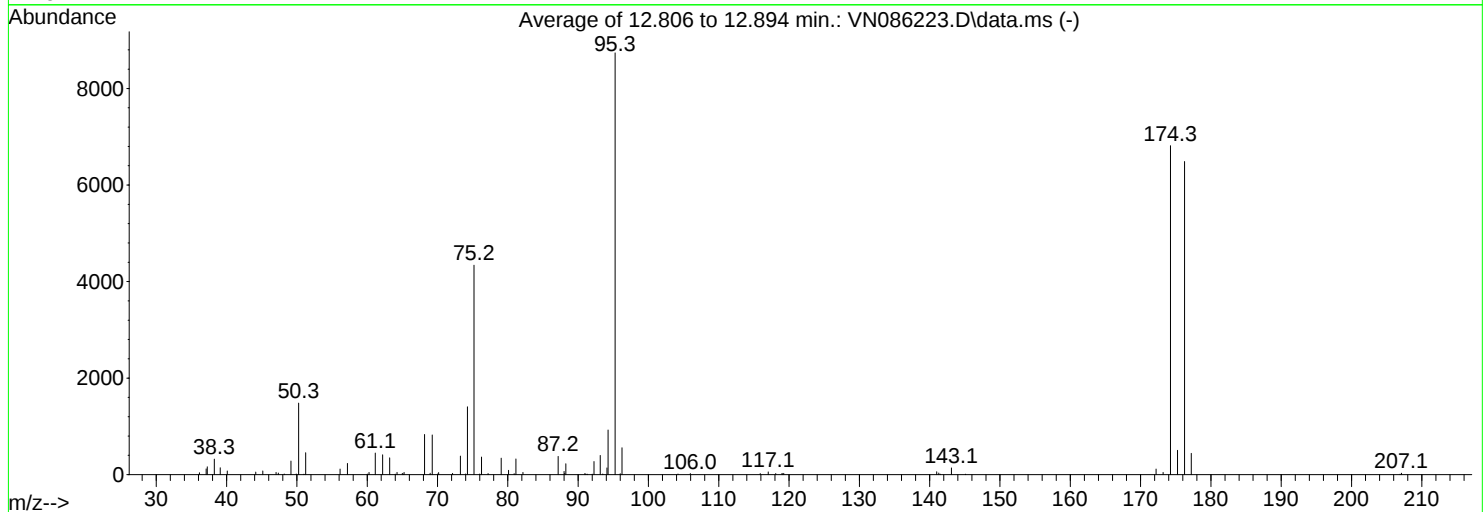


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN040425\
Data File : VN086223.D
Acq On : 04 Apr 2025 10:41
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N040425W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Sat Apr 05 00:04:36 2025

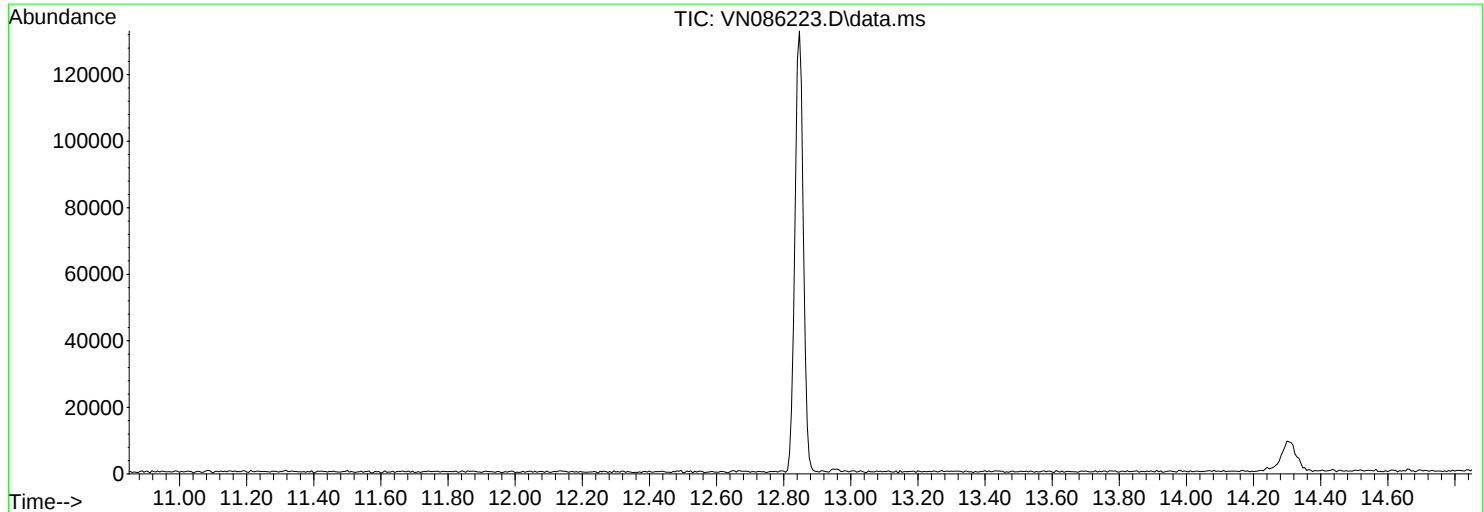

AutoFind: Averaged scan 1845 to 1860; Bkg corrected with scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.0	1482	PASS
75	95	30	60	49.7	4340	PASS
95	95	100	100	100.0	8738	PASS
96	95	5	9	6.4	558	PASS
173	174	0.00	2	0.7	48	PASS
174	95	50	100	78.0	6816	PASS
175	174	5	9	7.4	505	PASS
176	174	95	101	95.2	6488	PASS
177	176	5	9	6.8	440	PASS