

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN040519\
 Data File : VN054971.D
 Acq On : 5 Apr 2019 14:54
 Operator : JC/SP
 Sample : K2292-03
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-4

Quant Time: Apr 06 01:01:31 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N040419W.M
 Quant Title : SW846 8260
 QLast Update : Fri Apr 05 02:23:47 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	363007	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	653772	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	430222	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	91741	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	268727	56.15	ug/l	0.00
Spiked Amount	50.000		Recovery	=	112.30%	
35) Dibromofluoromethane	7.59	113	226477	53.22	ug/l	0.00
Spiked Amount	50.000		Recovery	=	106.44%	
50) Toluene-d8	10.09	98	610064	37.78	ug/l	0.00
Spiked Amount	50.000		Recovery	=	75.56%	
62) 4-Bromofluorobenzene	12.40	95	161019	29.88	ug/l	0.00
Spiked Amount	50.000		Recovery	=	59.76%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN040519\
Data File : VN054971.D
Acq On : 5 Apr 2019 14:54
Operator : JC/SP
Sample : K2292-03
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Quant Time: Apr 06 01:01:31 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N040419W.M
Quant Title : SW846 8260
QLast Update : Fri Apr 05 02:23:47 2019
Response via : Initial Calibration

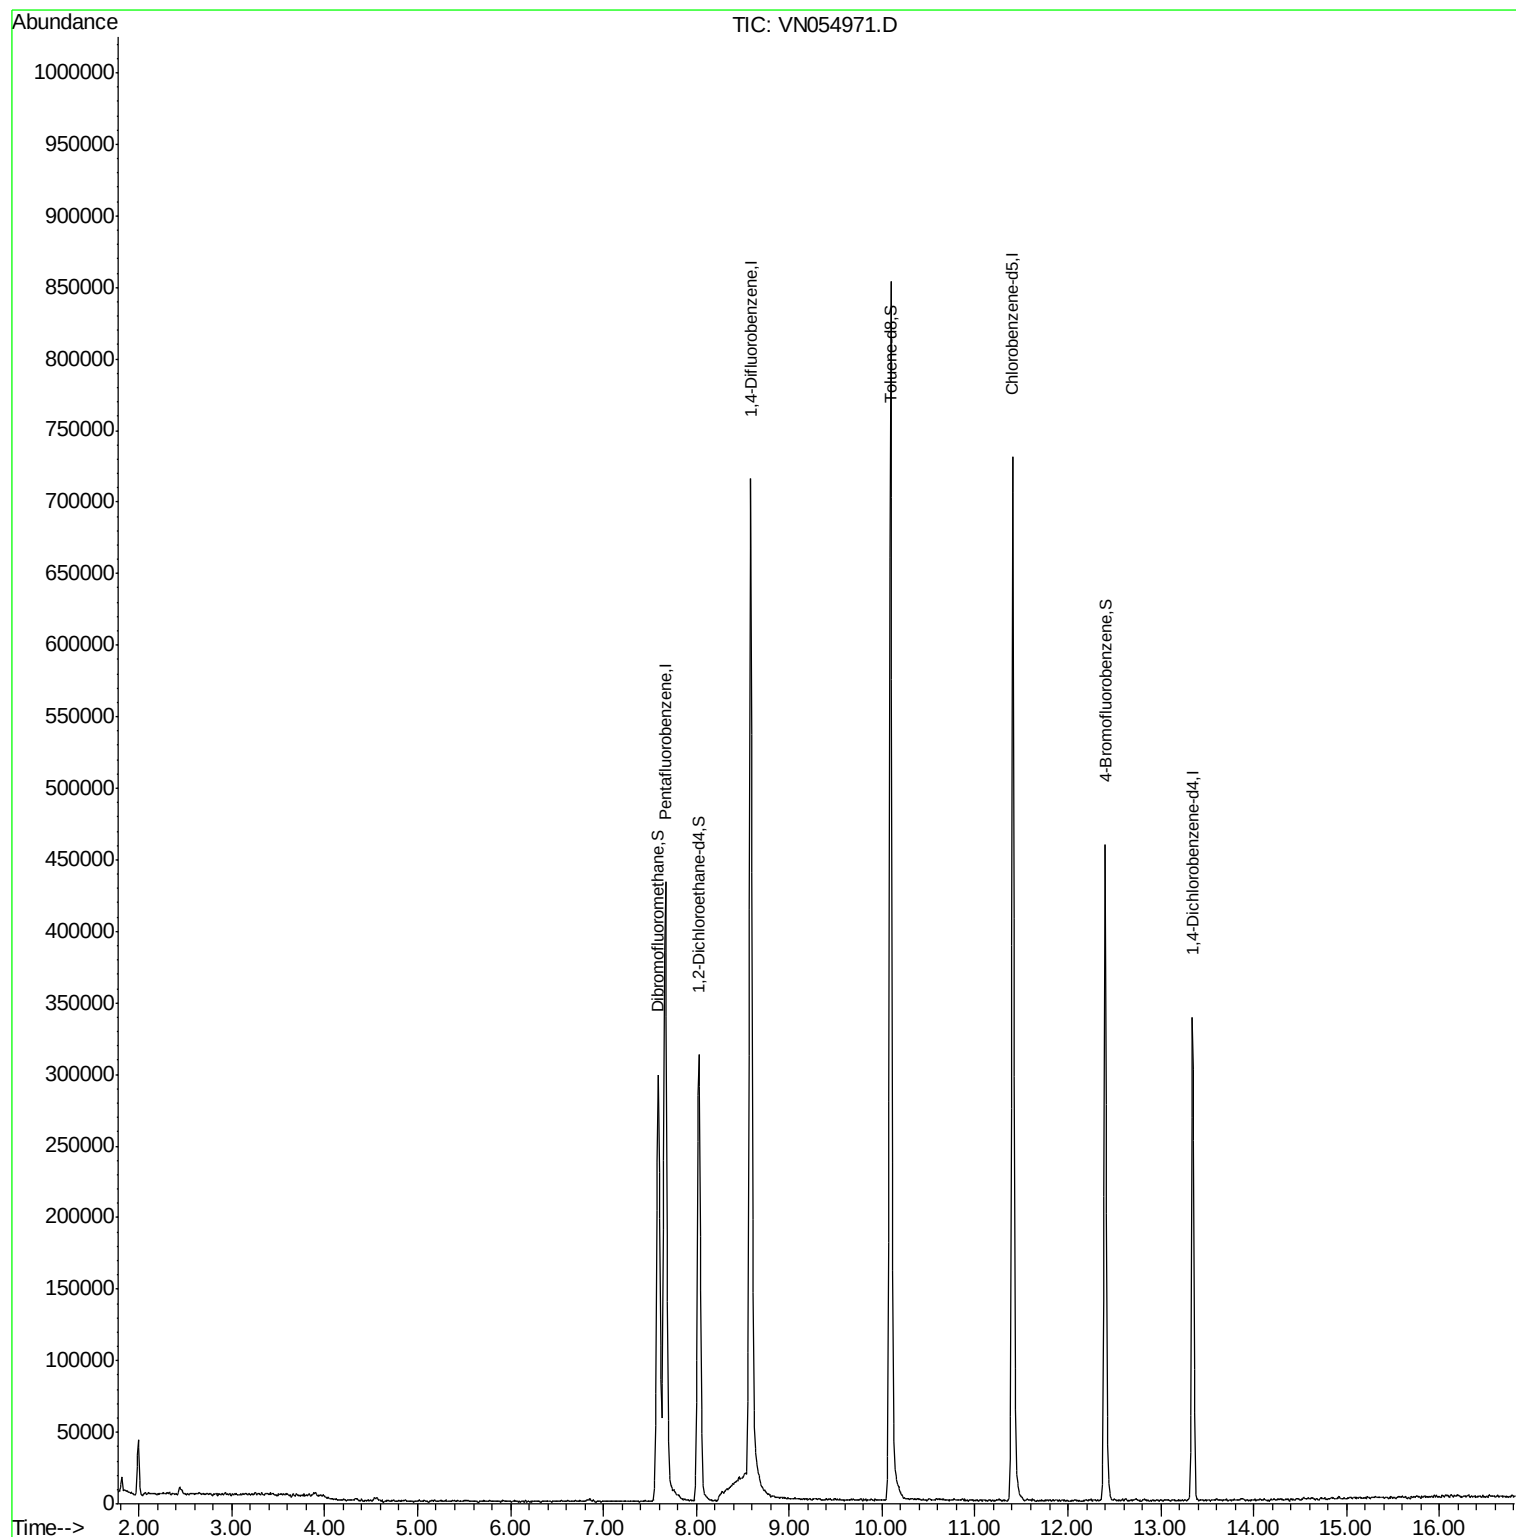

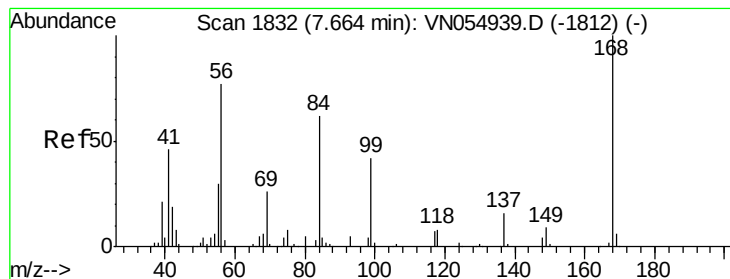

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. 0.00 min

Lab File: VN054971.D

Acq: 5 Apr 2019 14:54

Instrument :

MSVOA_N

ClientSampleId :


STORAGE-BLANK-WATER-REF-4

Tot Ion:168 Resp: 363007

Ion Ratio Lower Upper




168 100

99 56.6 44.1 66.1

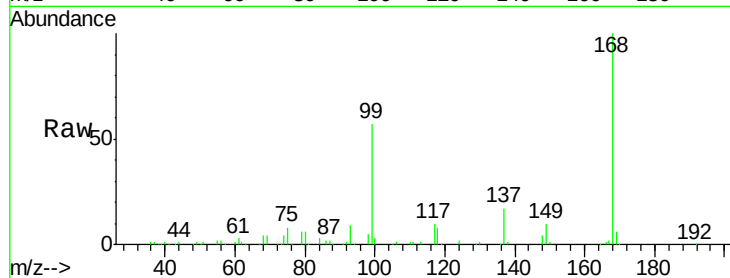

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

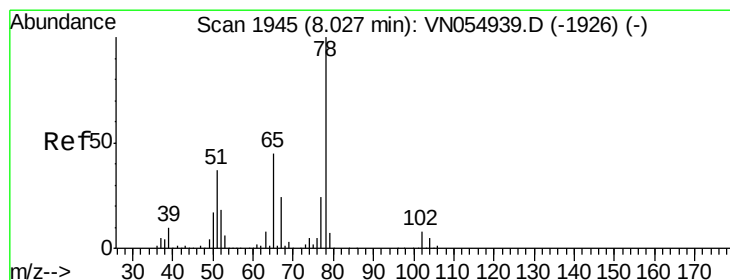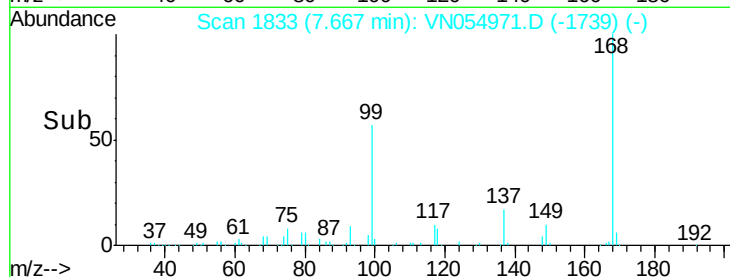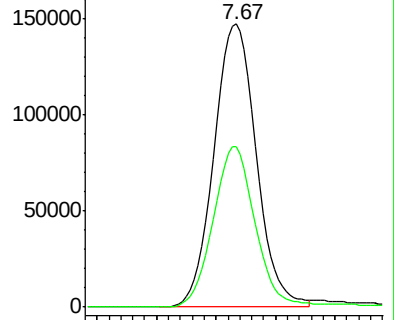

#33

1,2-Dichloroethane-d4

Concen: 56.147 ug/l

RT: 8.03 min Scan# 1945

Delta R.T. 0.00 min

Lab File: VN054971.D


Acq: 5 Apr 2019 14:54

Tgt Ion: 65 Resp: 268727

Ion Ratio Lower Upper



65 100


67 52.2 0.0 105.6

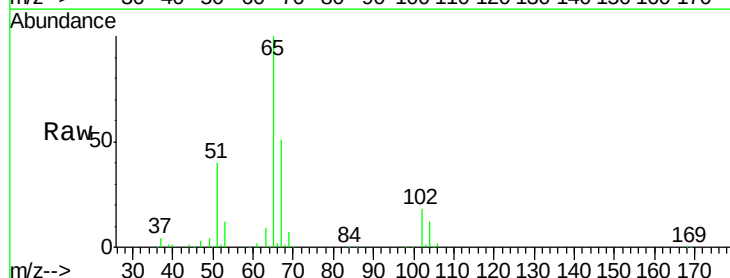

Abundance Ion 64.90 (64.60 to 65.60): VNO

Ion 66.90 (66.60 to 67.60): VNO

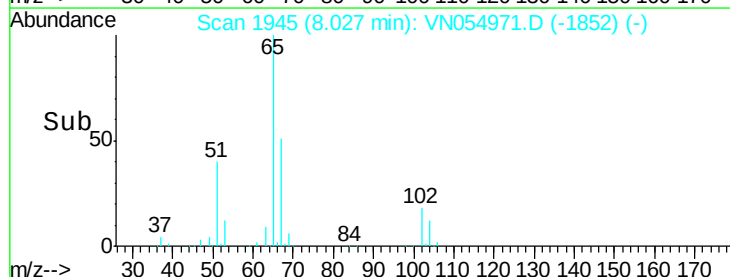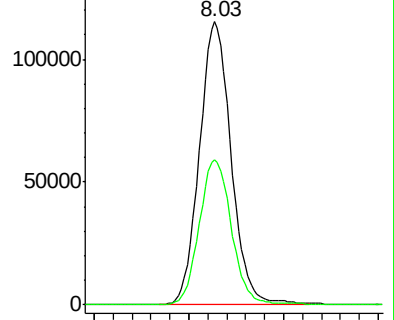


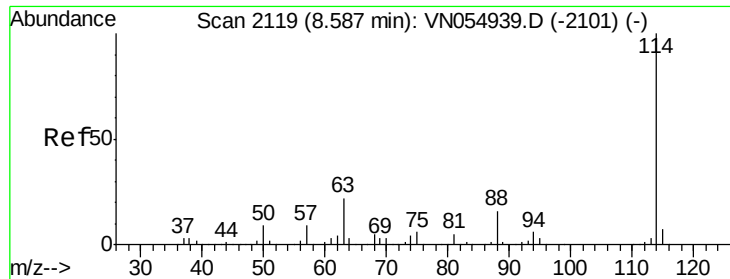




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.59 min Scan# 2119
 Delta R.T. 0.00 min
 Lab File: VN054971.D
 Acq: 5 Apr 2019 14:54

Instrument :
 MSVOA_N
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-4

Tot Ion:114 Resp: 653772
 Ion Ratio Lower Upper
 114 100
 63 22.4 0.0 44.6
 88 15.7 0.0 32.0

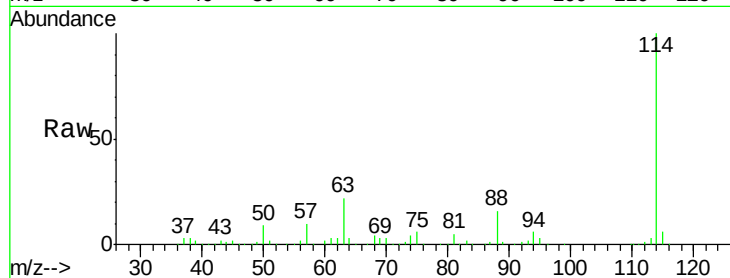


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): V
 Ion 87.90 (87.60 to 88.60): V

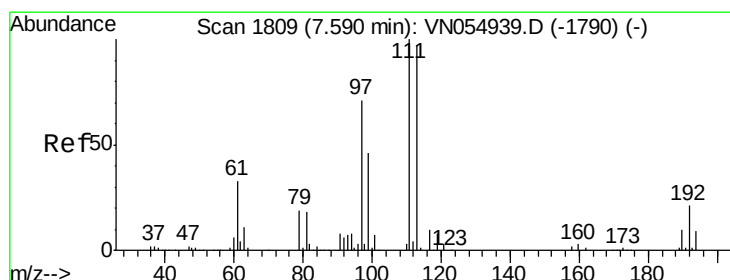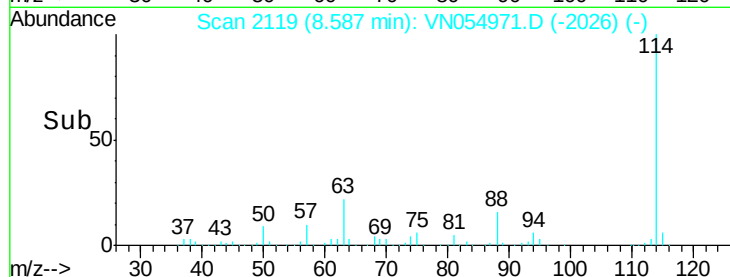
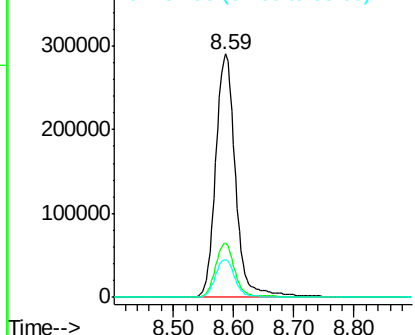



#35
 Dibromofluoromethane
 Concen: 53.216 ug/l
 RT: 7.59 min Scan# 1809
 Delta R.T. 0.00 min
 Lab File: VN054971.D
 Acq: 5 Apr 2019 14:54

Tgt Ion:113 Resp: 226477
 Ion Ratio Lower Upper
 113 100
 111 101.6 81.0 121.4
 192 20.8 16.5 24.7

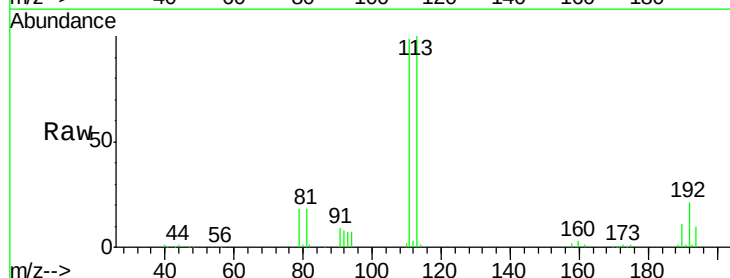

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

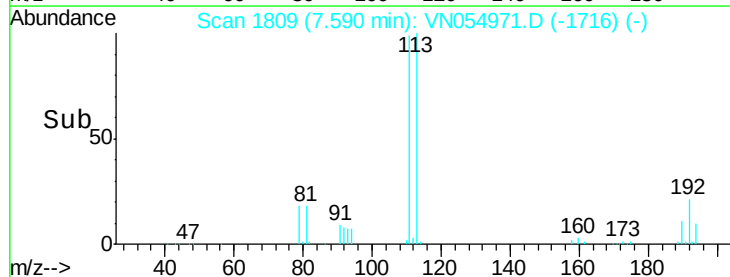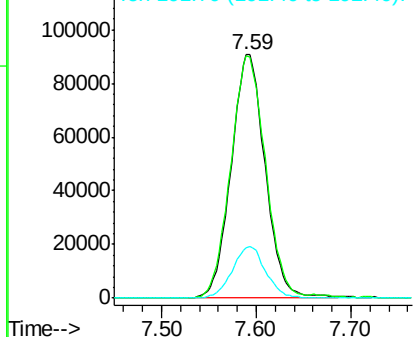

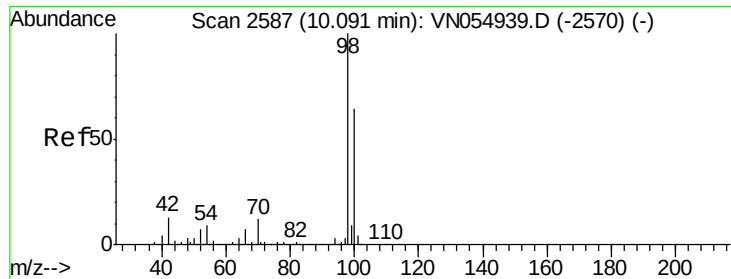

#50

Toluene-d8

Concen: 37.779 ug/l

RT: 10.09 min Scan# 2587

Delta R.T. 0.00 min

Lab File: VN054971.D

Acq: 5 Apr 2019 14:54

Instrument :

MSVOA_N

ClientSampleId :


STORAGE-BLANK-WATER-REF-4

Tot Ion: 98 Resp: 610064

Ion Ratio Lower Upper

98 100

100 64.7 51.5 77.3

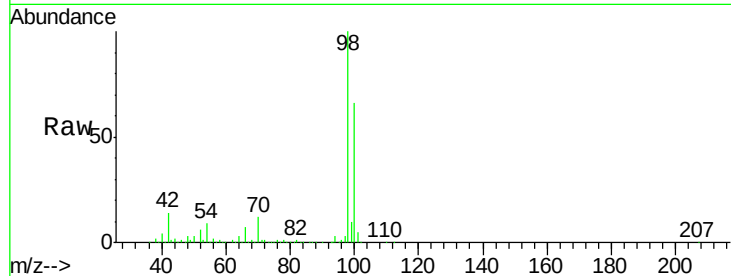

Abundance Ion 98.00 (97.70 to 98.70): VN054939.D (-2570) (-)

Ion 100.00 (99.70 to 100.70): VN054939.D (-2570) (-)

10.09



300000

200000

100000

0

Time-->

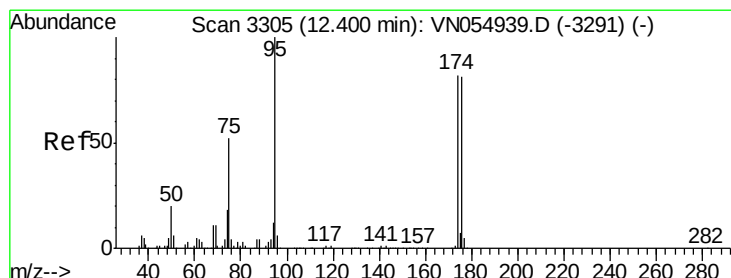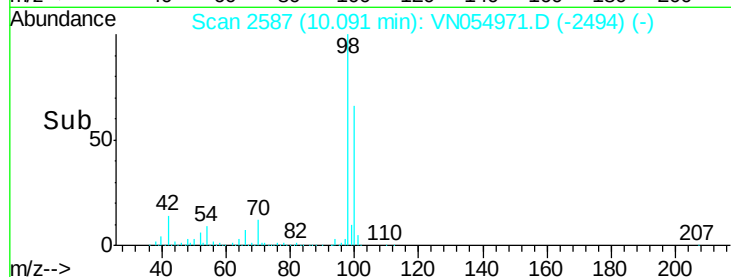

#62

4-Bromofluorobenzene

Concen: 29.879 ug/l

RT: 12.40 min Scan# 3305

Delta R.T. 0.00 min

Lab File: VN054971.D

Acq: 5 Apr 2019 14:54


Tgt Ion: 95 Resp: 161019

Ion Ratio Lower Upper

95 100

174 86.9 0.0 166.2

176 82.1 0.0 163.2

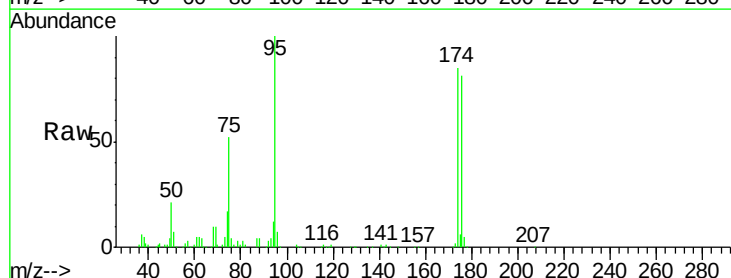

Abundance Ion 94.90 (94.60 to 95.60): VN054939.D (-3291) (-)

Ion 173.80 (173.50 to 174.50): VN054939.D (-3291) (-)

Ion 175.80 (175.50 to 176.50): VN054939.D (-3291) (-)

12.40

120000

100000

80000


60000


40000

20000

0

Time-->

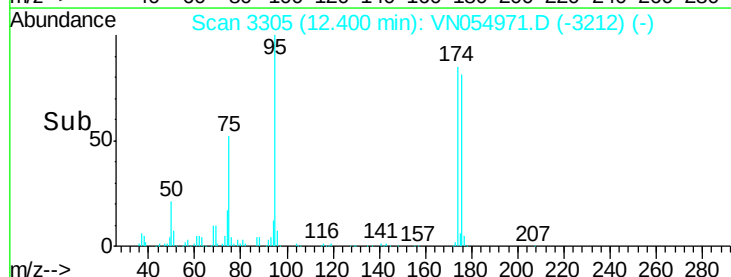


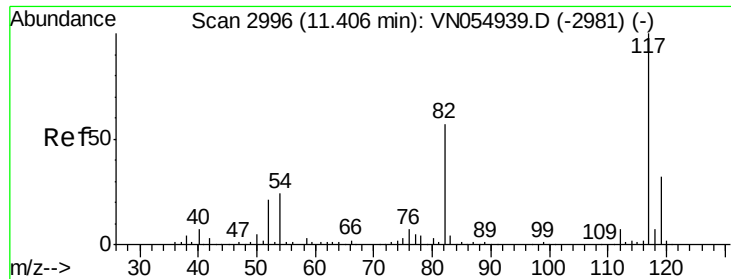




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.41 min Scan# 2996
Delta R.T. 0.00 min
Lab File: VN054971.D
Acq: 5 Apr 2019 14:54

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-WATER-REF-4

Tot Ion:117 Resp: 430222
Ion Ratio Lower Upper
117 100
82 55.4 45.3 67.9
119 32.6 25.8 38.6

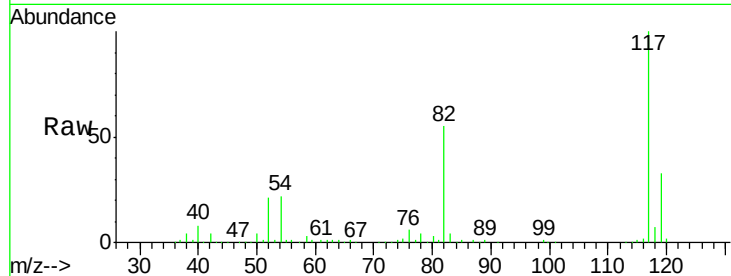


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

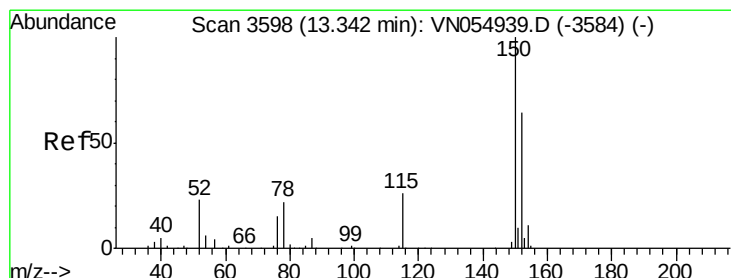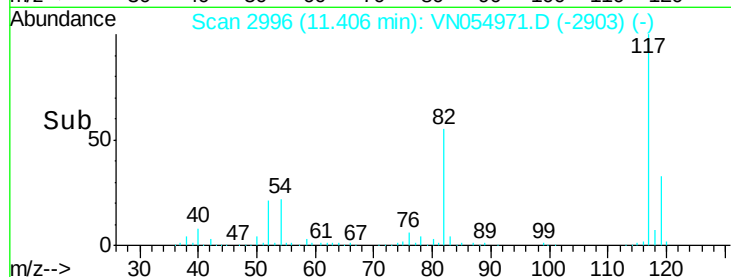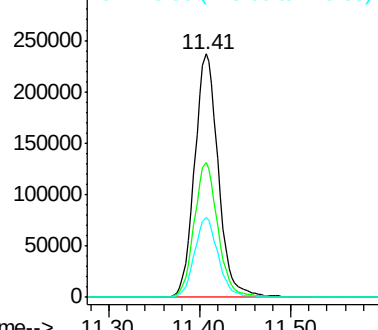

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.34 min Scan# 3598
Delta R.T. 0.00 min
Lab File: VN054971.D
Acq: 5 Apr 2019 14:54

Tgt Ion:152 Resp: 91741
Ion Ratio Lower Upper
152 100
115 57.9 28.9 86.8
150 155.6 0.0 345.4

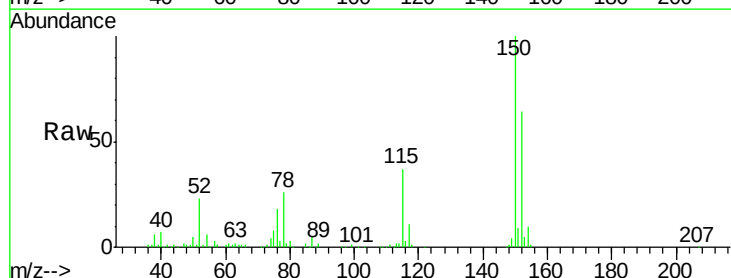

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

