

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN040522\
 Data File : VN071855.D
 Acq On : 05 Apr 2022 14:48
 Operator : JC\MD
 Sample : N2258-07
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 FB-040422

Quant Time: Apr 06 06:41:01 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 31 01:57:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.081	168	616795	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	1060444	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	1049934	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.668	152	372854	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.433	65	346500	49.209	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	98.420%
35) Dibromofluoromethane	8.022	113	299899	48.060	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	96.120%
50) Toluene-d8	10.439	98	1304997	51.123	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	102.240%
62) 4-Bromofluorobenzene	12.727	95	436622	52.887	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	105.780%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN040522\
Data File : VN071855.D
Acq On : 05 Apr 2022 14:48
Operator : JC\MD
Sample : N2258-07
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
FB-040422

Quant Time: Apr 06 06:41:01 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
Quant Title : SW846 8260
QLast Update : Thu Mar 31 01:57:54 2022
Response via : Initial Calibration

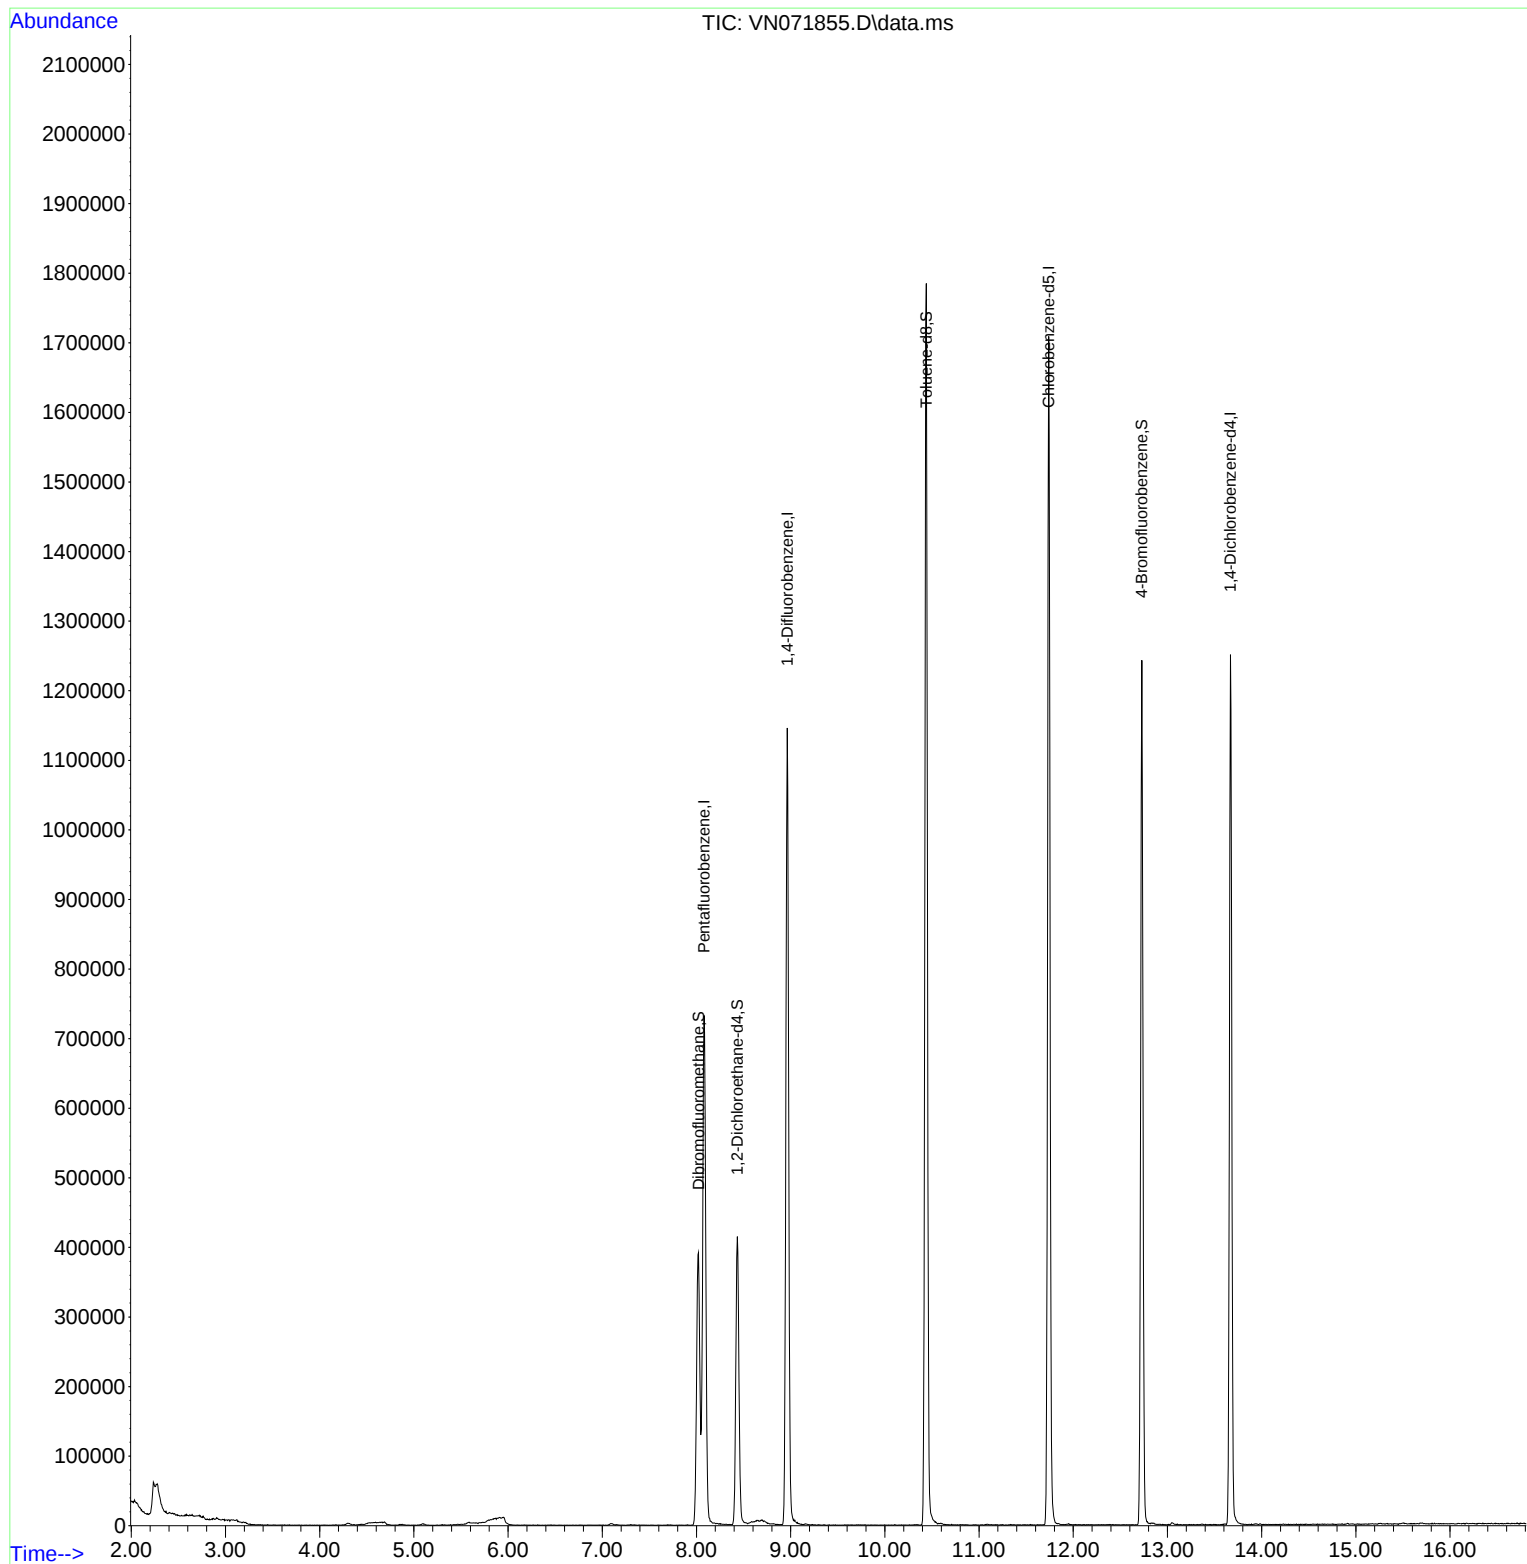

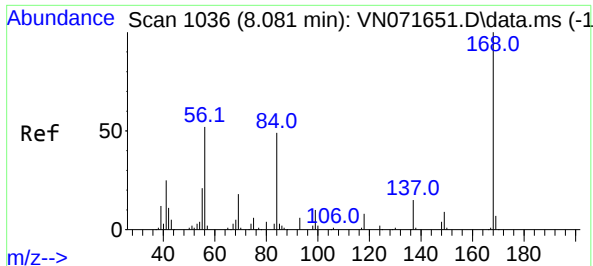

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.081 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN071855.D

Acq: 05 Apr 2022 14:48

Instrument :

MSVOA_N

ClientSampleId :





FB-040422

Tgt Ion:168 Resp: 616795

Ion Ratio Lower Upper

168 100

99 53.0 42.3 63.5

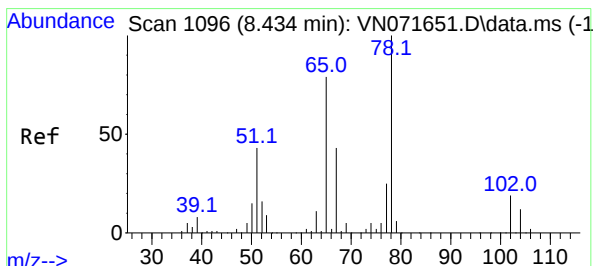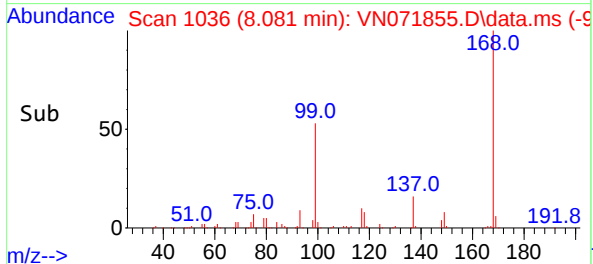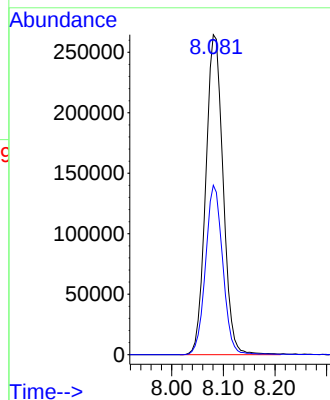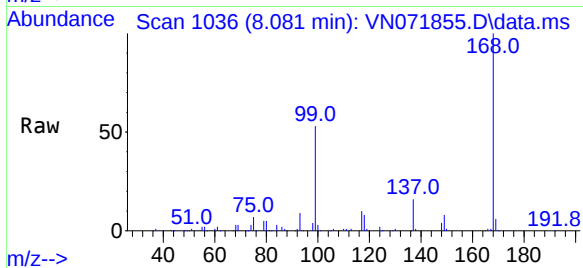

1,2-Dichloroethane-d4

Concen: 49.209 ug/l

RT: 8.433 min Scan# 1096

Delta R.T. -0.001 min

Lab File: VN071855.D




Acq: 05 Apr 2022 14:48


Tgt Ion: 65 Resp: 346500

Ion Ratio Lower Upper

65 100

67 52.1 0.0 104.8


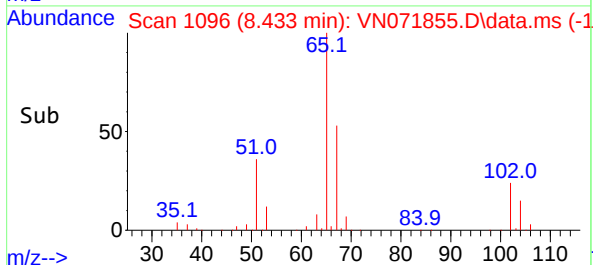
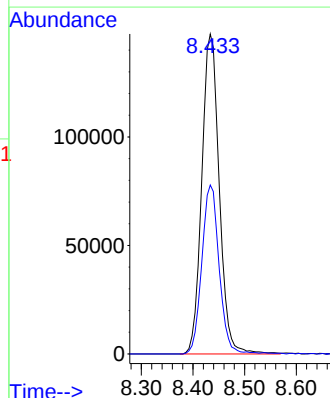
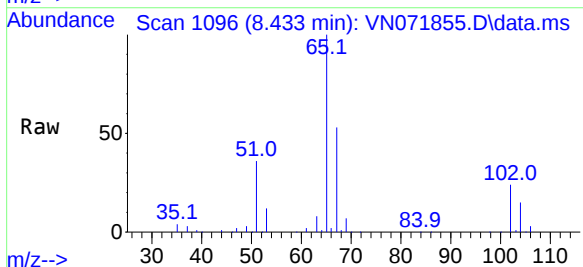


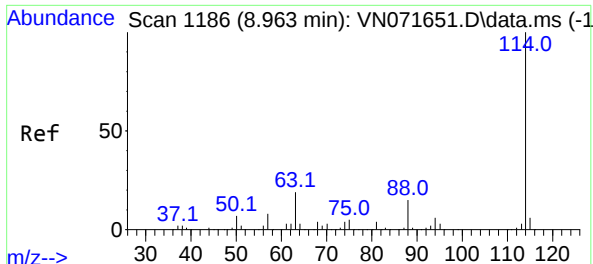

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.963 min Scan# 1186
Delta R.T. -0.000 min
Lab File: VN071855.D
Acq: 05 Apr 2022 14:48




Instrument :
MSVOA_N
ClientSampleId :
FB-040422


Tgt Ion:114 Resp: 1060444
Ion Ratio Lower Upper
114 100
63 18.7 0.0 40.0
88 15.2 0.0 32.6

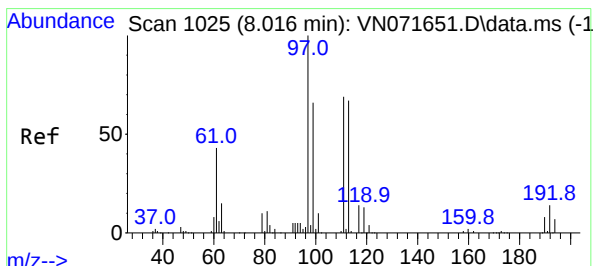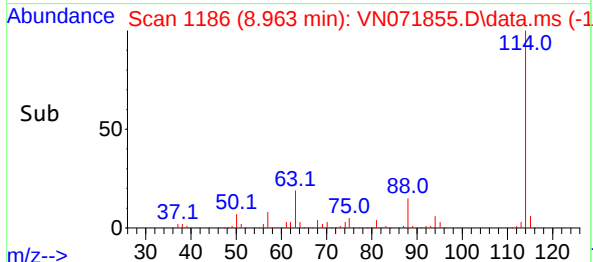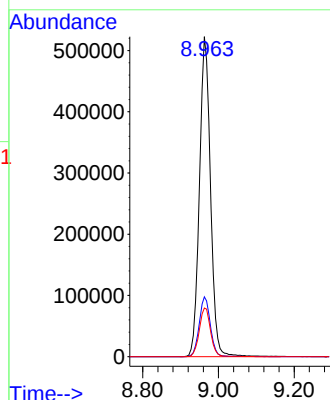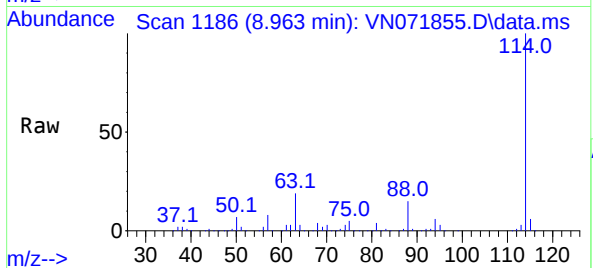

#35
Dibromofluoromethane
Concen: 48.060 ug/l
RT: 8.022 min Scan# 1026
Delta R.T. 0.006 min
Lab File: VN071855.D
Acq: 05 Apr 2022 14:48

Tgt Ion:113 Resp: 299899
Ion Ratio Lower Upper
113 100
111 102.5 81.4 122.0
192 22.1 17.0 25.6


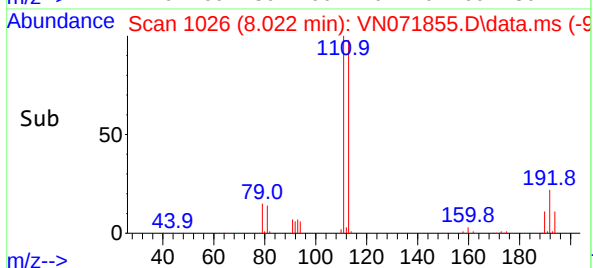
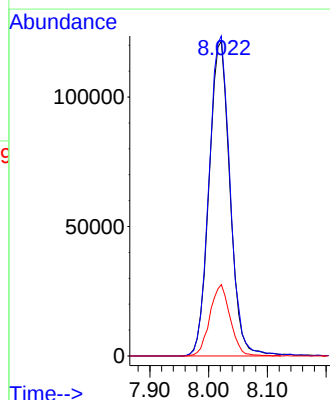
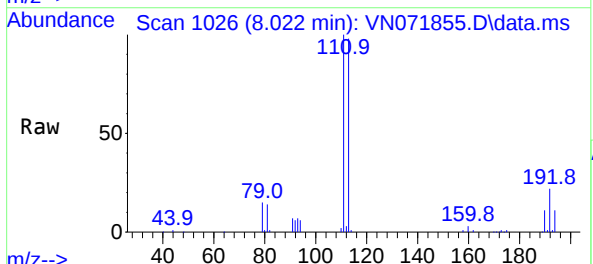


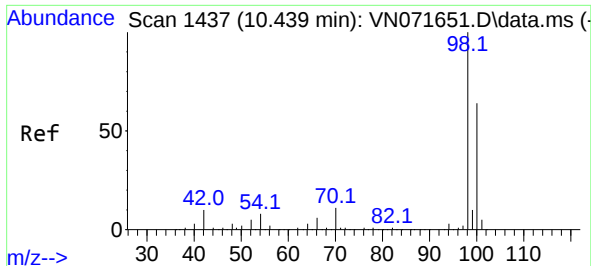

#50
Toluene-d8
Concen: 51.123 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. 0.000 min
Lab File: VN071855.D
Acq: 05 Apr 2022 14:48




Instrument :
MSVOA_N
ClientSampleId :
FB-040422


Tgt Ion: 98 Resp: 1304997
Ion Ratio Lower Upper
98 100
100 65.0 52.6 78.8

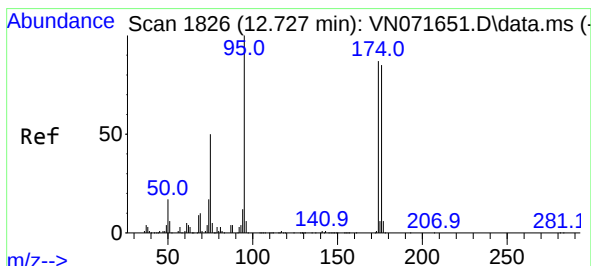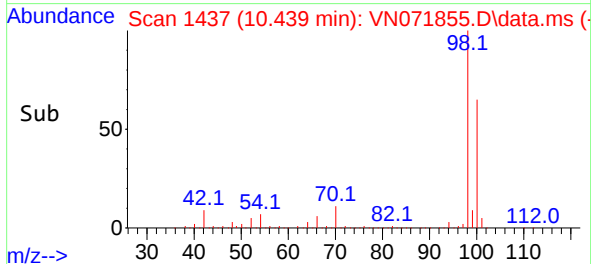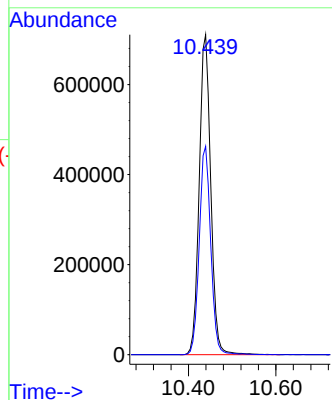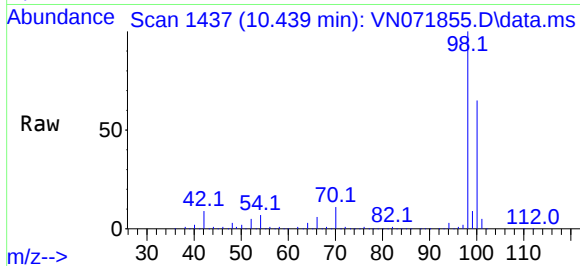

#62
4-Bromofluorobenzene
Concen: 52.887 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN071855.D
Acq: 05 Apr 2022 14:48

Tgt Ion: 95 Resp: 436622
Ion Ratio Lower Upper
95 100
174 85.6 0.0 167.6
176 82.9 0.0 163.4


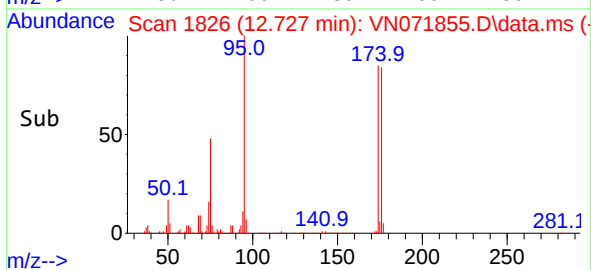
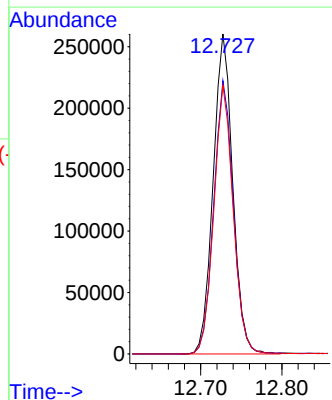
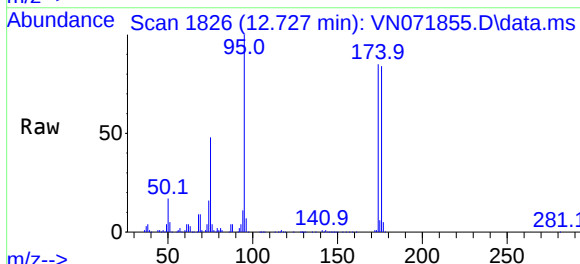


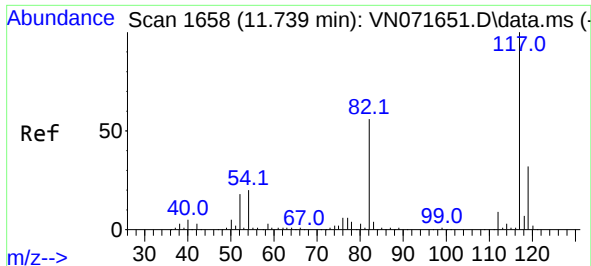

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN071855.D
Acq: 05 Apr 2022 14:48

Instrument :
MSVOA_N
ClientSampleId :
FB-040422

Tgt Ion:117 Resp: 1049934
Ion Ratio Lower Upper
117 100
82 56.2 44.2 66.2
119 32.6 25.4 38.0

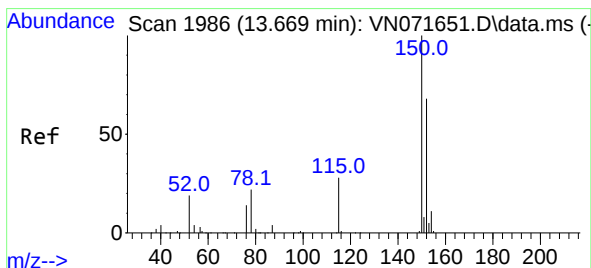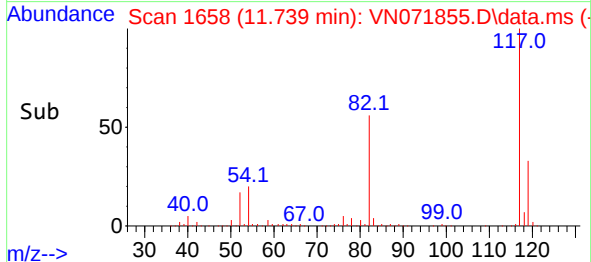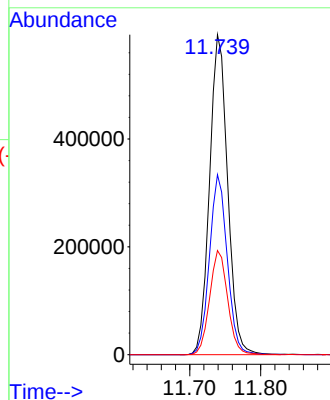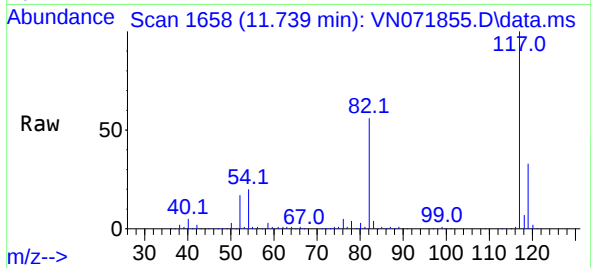

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.668 min Scan# 1986
Delta R.T. -0.001 min
Lab File: VN071855.D
Acq: 05 Apr 2022 14:48

Tgt Ion:152 Resp: 372854
Ion Ratio Lower Upper
152 100
115 57.5 28.9 86.7
150 158.8 0.0 356.2

