

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN040620\
 Data File : VN060856.D
 Acq On : 6 Apr 2020 17:05
 Operator : JC/MD
 Sample : L2132-08
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 T-2

Quant Time: Apr 07 08:30:05 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N031820W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 18 08:49:09 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.64	168	198012	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.57	114	331789	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.40	117	311236	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	141470	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.00	65	127956	47.07	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.14%	
35) Dibromofluoromethane	7.56	113	98765	49.23	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.46%	
50) Toluene-d8	10.08	98	405978	49.54	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.08%	
62) 4-Bromofluorobenzene	12.40	95	152833	50.89	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.78%	
Target Compounds						
16) Acetone	3.78	43	34697	36.035	ug/l	95
20) Methylene Chloride	4.52	84	6626	2.797	ug/l	94
25) 2-Butanone	6.80	43	12328	7.912	ug/l	94
43) Isopropyl Acetate	8.14	43	52075	9.096	ug/l #	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN040620\
Data File : VN060856.D
Acq On : 6 Apr 2020 17:05
Operator : JC/MD
Sample : L2132-08
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
T-2

Quant Time: Apr 07 08:30:05 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N031820W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 18 08:49:09 2020
Response via : Initial Calibration

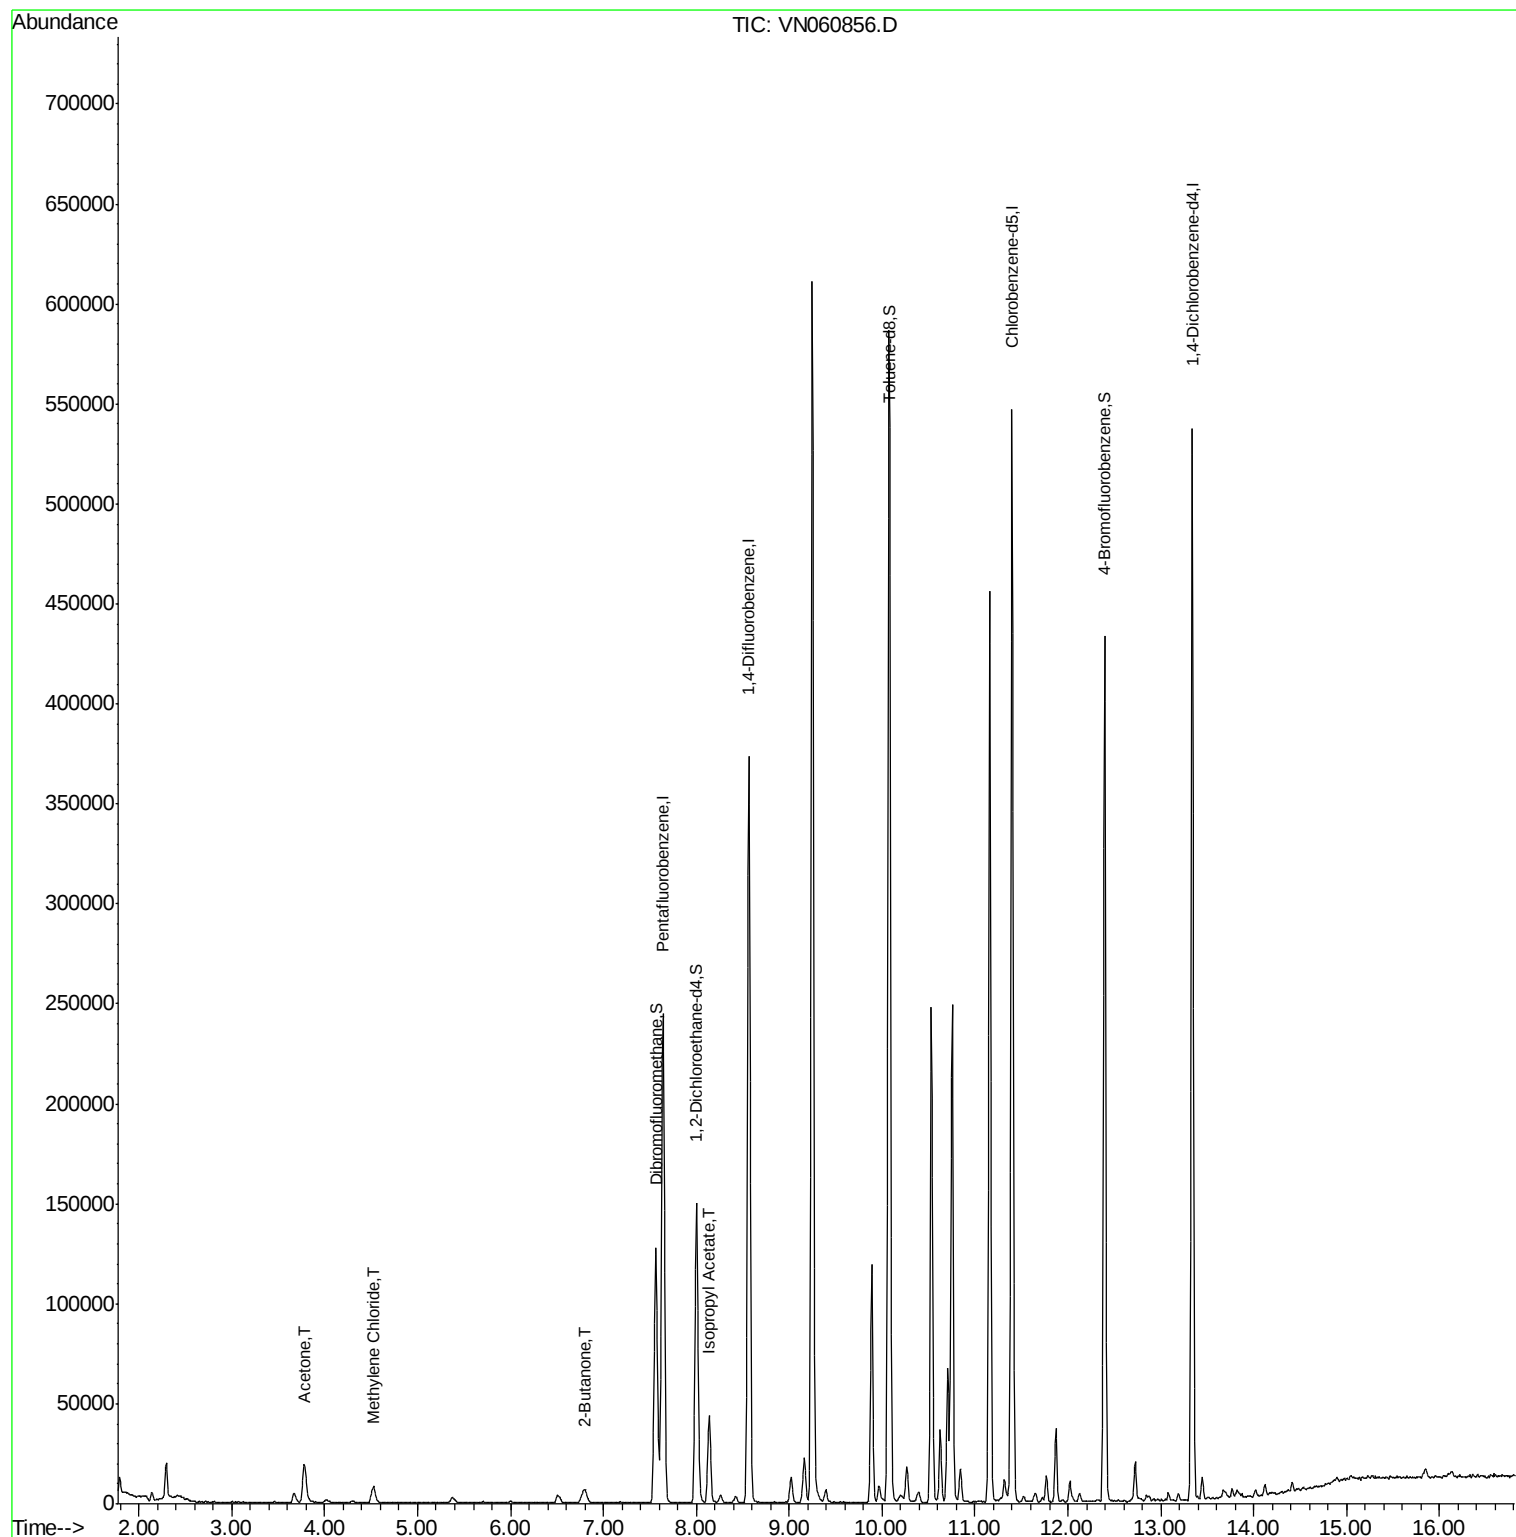



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.64 min Scan# 1825

Delta R.T. -0.00 min

Lab File: VN060856.D

Acq: 6 Apr 2020 17:05

Instrument :

MSVOA_N

ClientSampleId :


T-2

Tot Ion:168 Resp: 198012

Ion Ratio Lower Upper



168 100

99 57.7 44.0 66.0

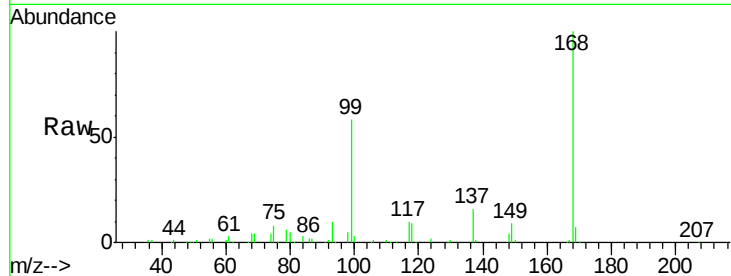

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN0

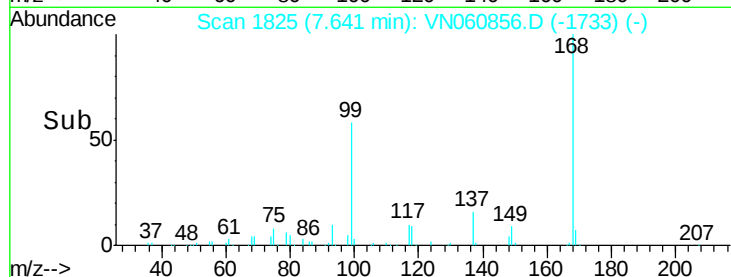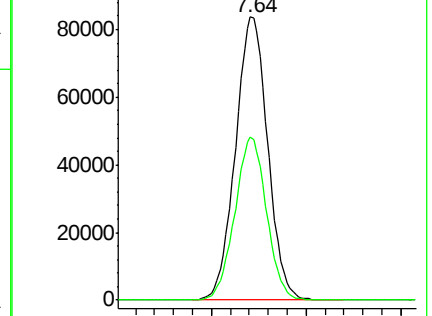

#16

Acetone

Concen: 36.035 ug/l

RT: 3.78 min Scan# 624

Delta R.T. 0.00 min

Lab File: VN060856.D


Acq: 6 Apr 2020 17:05

Tgt Ion: 43 Resp: 34697

Ion Ratio Lower Upper



43 100




58 34.1 25.1 37.7

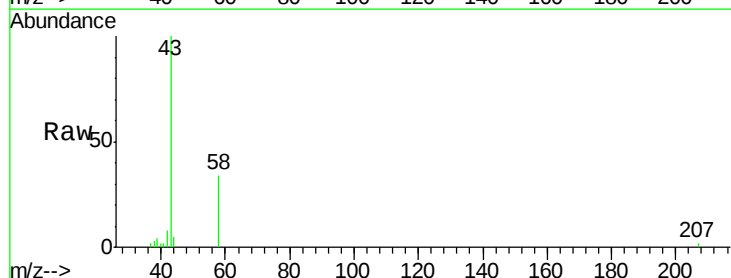

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0



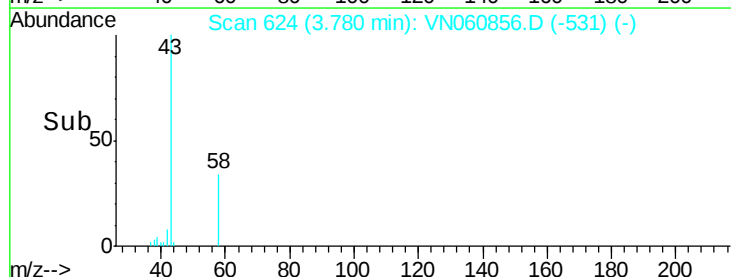
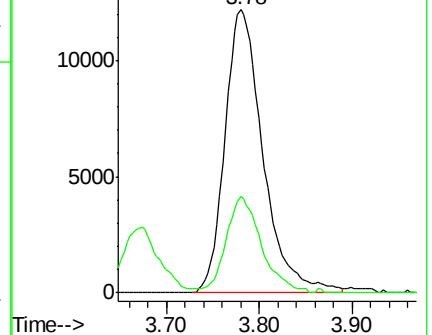


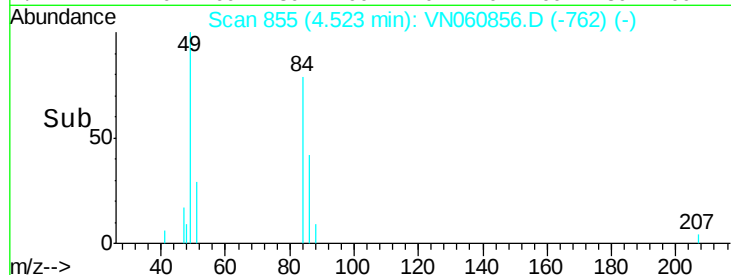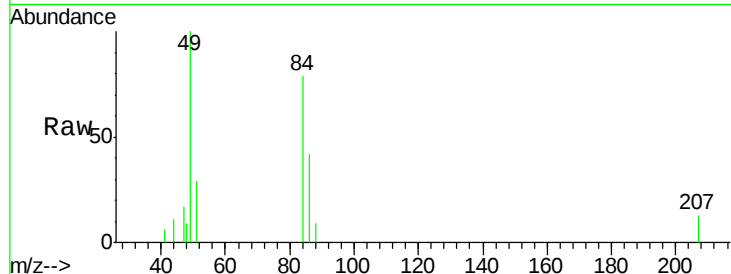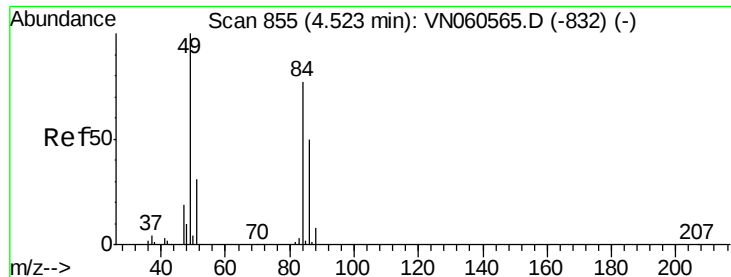

#20
Methylene Chloride
Concen: 2.797 ug/l
RT: 4.52 min Scan# 855
Delta R.T. 0.00 min
Lab File: VN060856.D
Acq: 6 Apr 2020 17:05


Instrument :
MSVOA_N
ClientSampled :
T-2

Tot Ion: 84	Resp: 6626
Ion Ratio	Lower Upper
84 100	
49 126.9	103.3 154.9
51 37.4	31.6 47.4
86 53.2	52.0 78.0

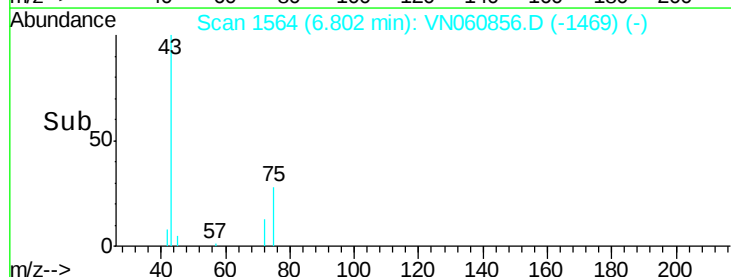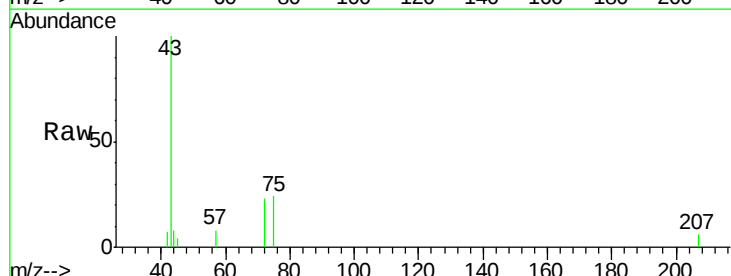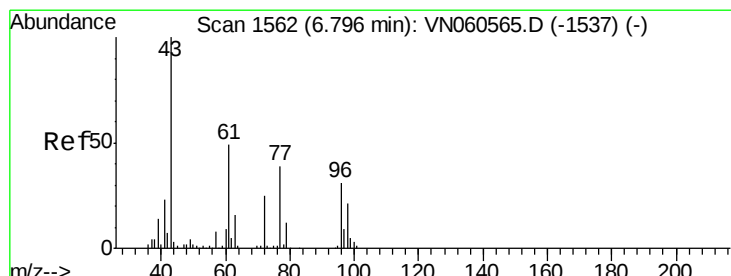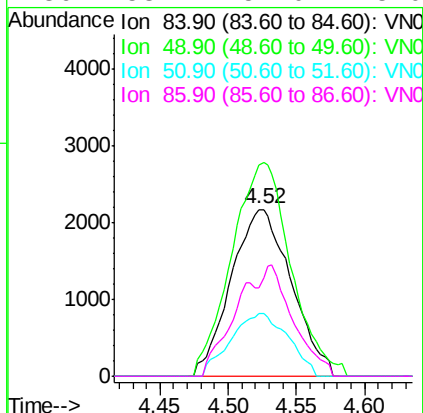

#25
2-Butanone
Concen: 7.912 ug/l
RT: 6.80 min Scan# 1564
Delta R.T. 0.01 min
Lab File: VN060856.D
Acq: 6 Apr 2020 17:05

Tgt Ion: 43	Resp: 12328
Ion Ratio	Lower Upper
43 100	
72 22.7	20.4 30.6




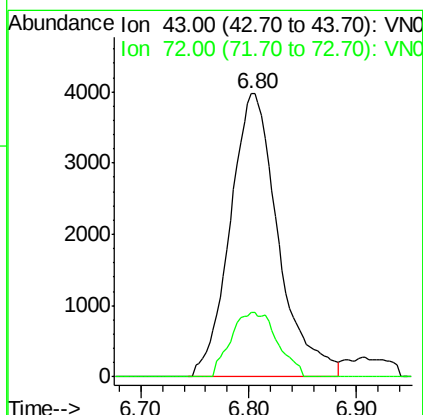




#33
 1,2-Dichloroethane-d4
 Concen: 47.073 ug/l
 RT: 8.00 min Scan# 1937
 Delta R.T. -0.00 min
 Lab File: VN060856.D
 Acq: 6 Apr 2020 17:05




Instrument :
 MSVOA_N
 ClientSampled :
 T-2


Tot Ion: 65 Resp: 127956
 Ion Ratio Lower Upper
 65 100
 67 54.2 0.0 107.6

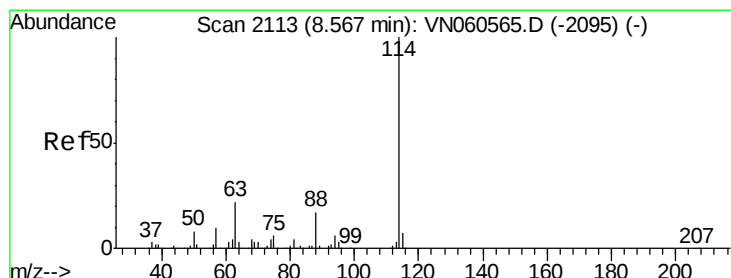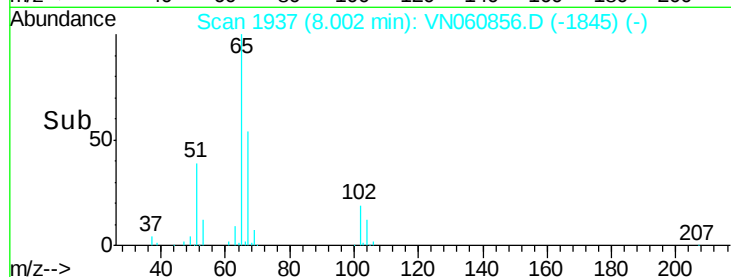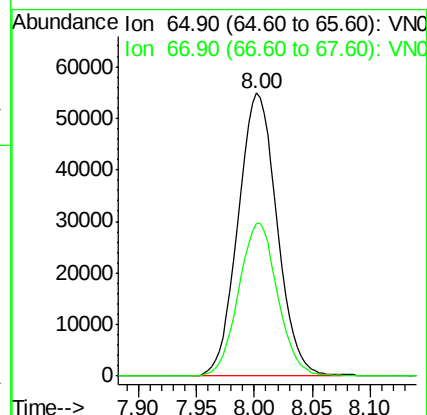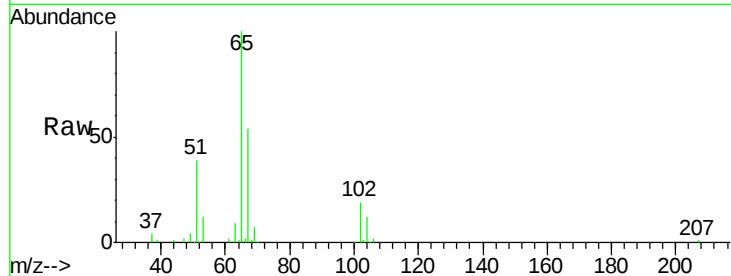

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.57 min Scan# 2113
 Delta R.T. 0.00 min
 Lab File: VN060856.D
 Acq: 6 Apr 2020 17:05

Tgt Ion: 114 Resp: 331789
 Ion Ratio Lower Upper
 114 100
 63 22.3 0.0 43.8
 88 16.4 0.0 33.0

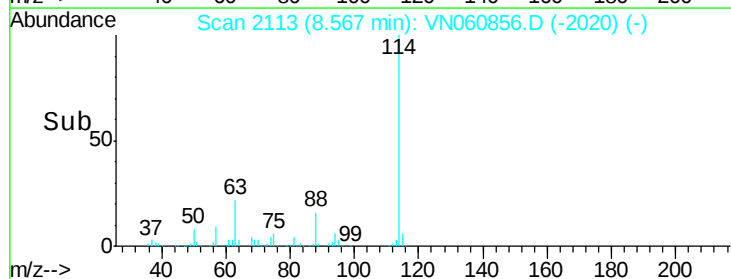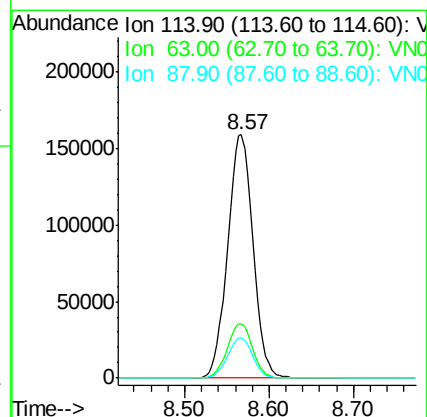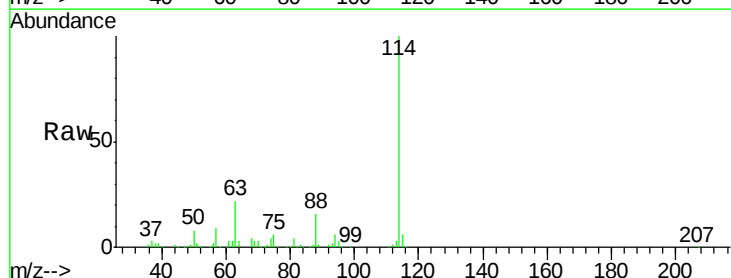

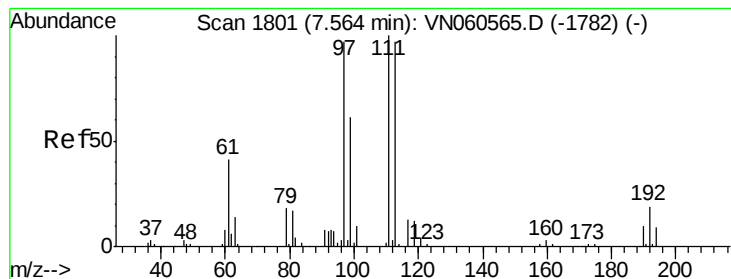

#35

Dibromofluoromethane

Concen: 49.229 ug/l

RT: 7.56 min Scan# 1801

Delta R.T. 0.00 min

Lab File: VN060856.D

Acq: 6 Apr 2020 17:05

Instrument :

MSVOA_N

ClientSampleId :

T-2


Tot Ion:113 Resp: 98765

Ion Ratio Lower Upper

113 100

111 101.8 82.9 124.3




192 19.6 15.8 23.8

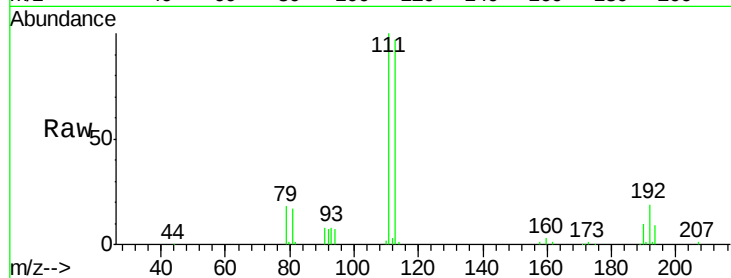

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

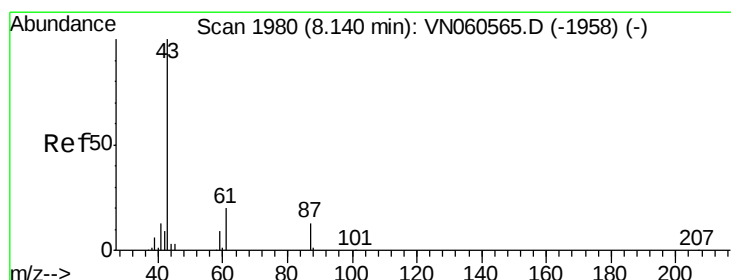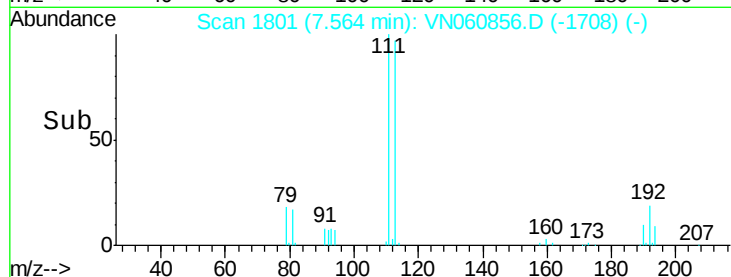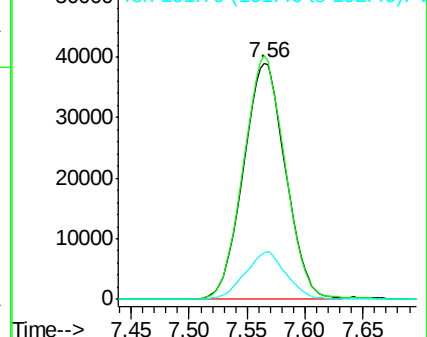

#43

Isopropyl Acetate

Concen: 9.096 ug/l

RT: 8.14 min Scan# 1979

Delta R.T. -0.00 min

Lab File: VN060856.D

Acq: 6 Apr 2020 17:05


Tgt Ion: 43 Resp: 52075

Ion Ratio Lower Upper

43 100

61 19.2 20.7 31.1#



87 12.2 9.8 14.8

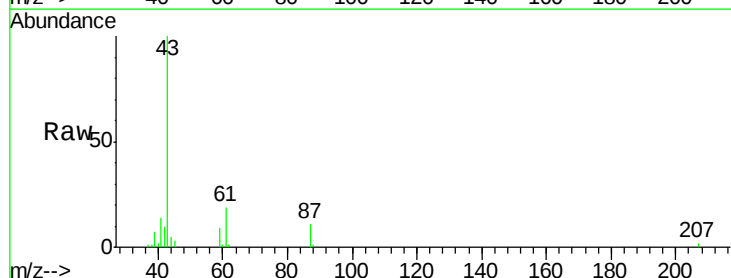


Abundance Ion 43.00 (42.70 to 43.70): V

Ion 61.00 (60.70 to 61.70): V

Ion 87.00 (86.70 to 87.70): V

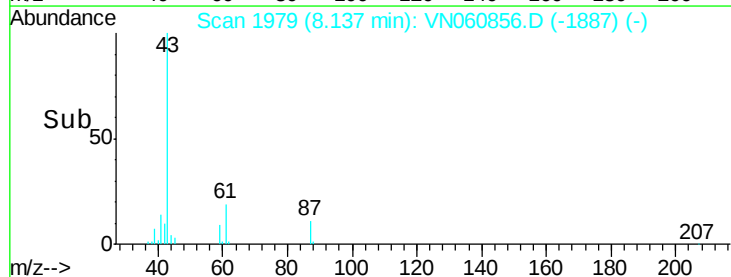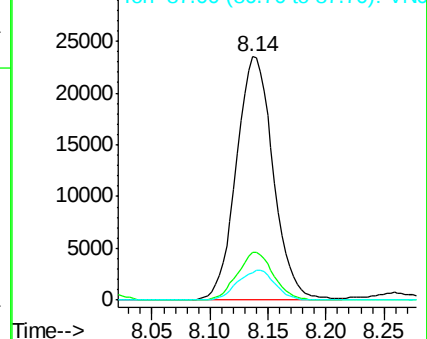

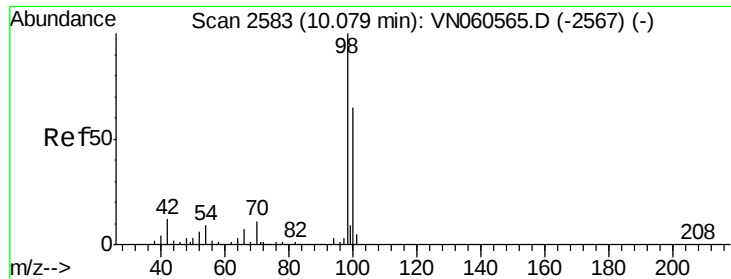

#50

Toluene-d8

Concen: 49.542 ug/l

RT: 10.08 min Scan# 2582

Delta R.T. -0.00 min

Lab File: VN060856.D

Acq: 6 Apr 2020 17:05

Instrument :

MSVOA_N

ClientSampleId :





T-2

Tot Ion: 98 Resp: 405978

Ion Ratio Lower Upper

98 100

100 65.2 51.8 77.8

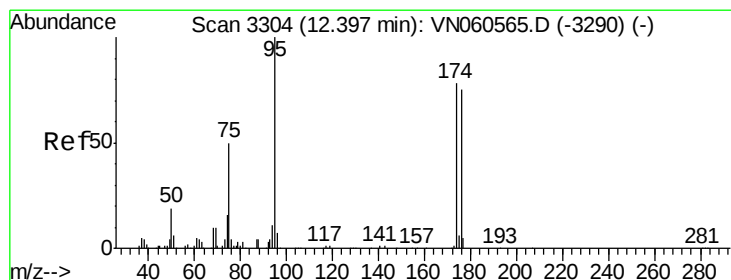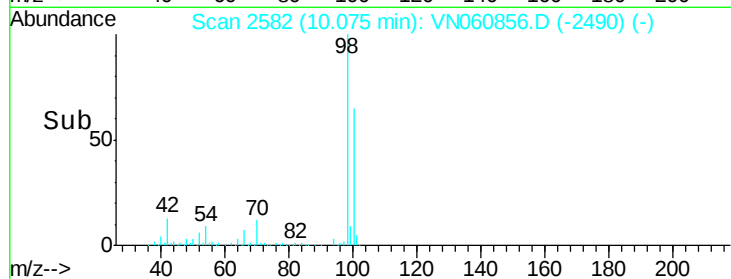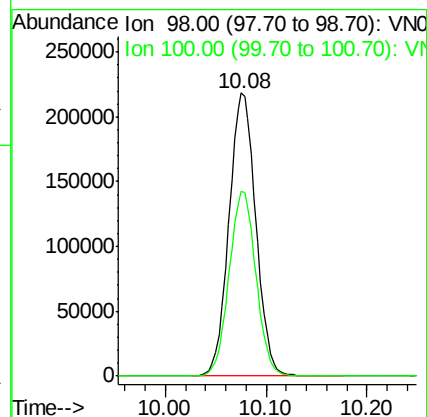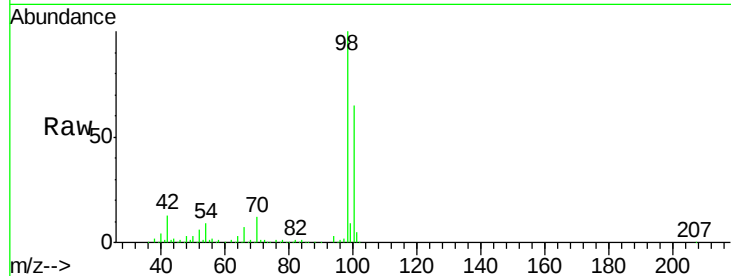

#62

4-Bromofluorobenzene

Concen: 50.890 ug/l

RT: 12.40 min Scan# 3304

Delta R.T. 0.00 min

Lab File: VN060856.D

Acq: 6 Apr 2020 17:05




Tgt Ion: 95 Resp: 152833


Ion Ratio Lower Upper

95 100

174 78.2 0.0 157.6

176 75.3 0.0 150.6

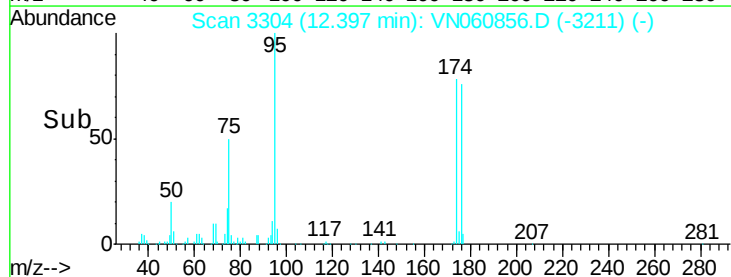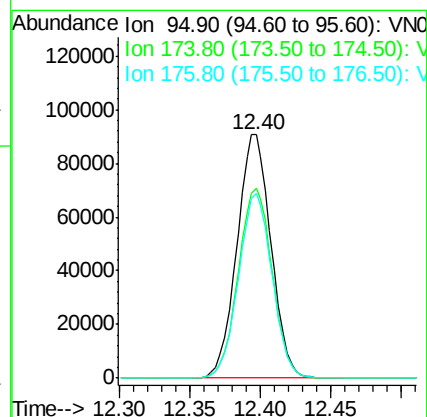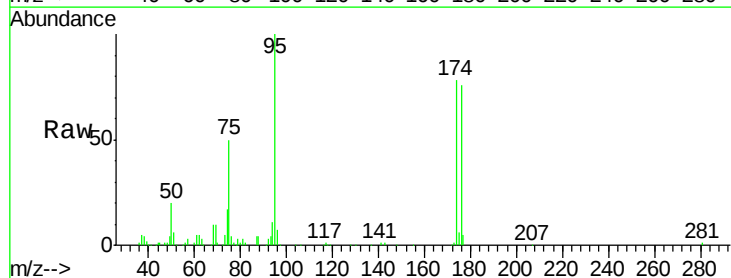


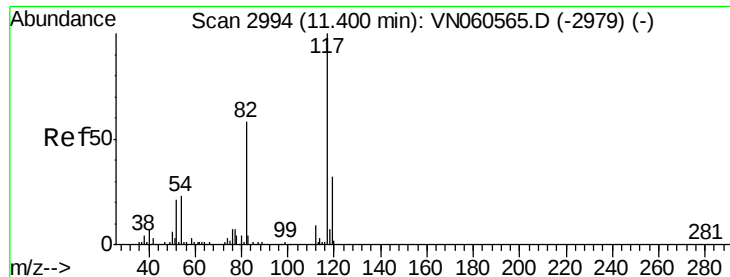




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.40 min Scan# 2994
Delta R.T. 0.00 min
Lab File: VN060856.D
Acq: 6 Apr 2020 17:05

Instrument :
MSVOA_N
ClientSampled :
T-2

Tot Ion:117 Resp: 311236
Ion Ratio Lower Upper
117 100
82 58.1 46.7 70.1
119 32.7 25.5 38.3

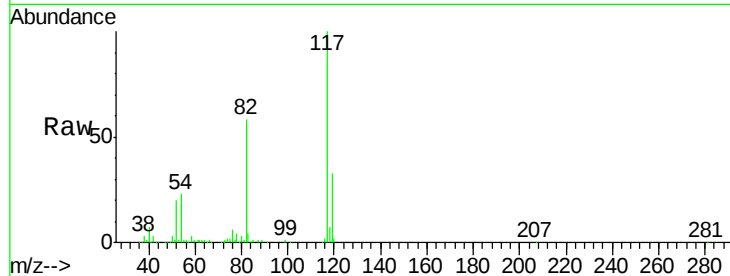


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

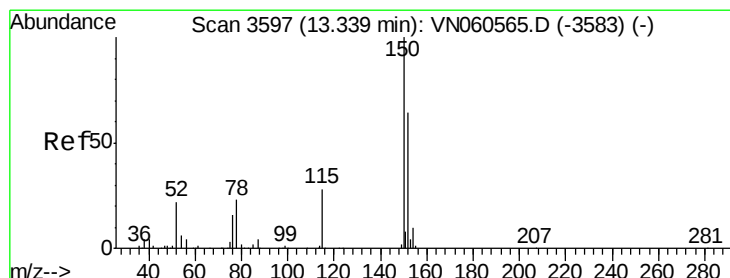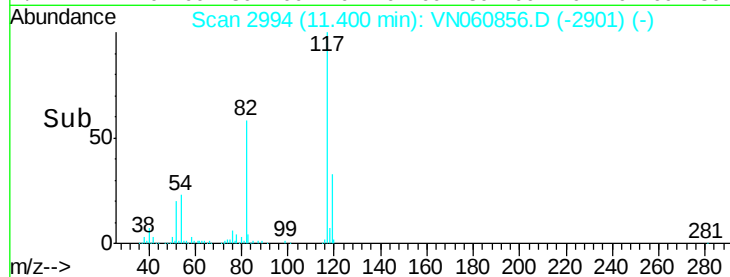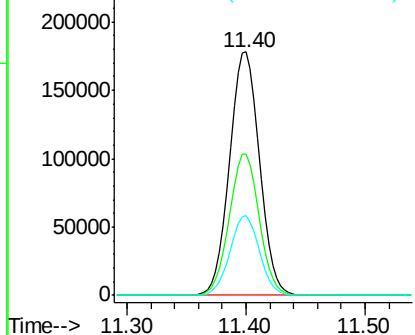

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.34 min Scan# 3597
Delta R.T. 0.00 min
Lab File: VN060856.D
Acq: 6 Apr 2020 17:05

Tgt Ion:152 Resp: 141470
Ion Ratio Lower Upper
152 100
115 60.1 30.2 90.6
150 158.4 0.0 350.2

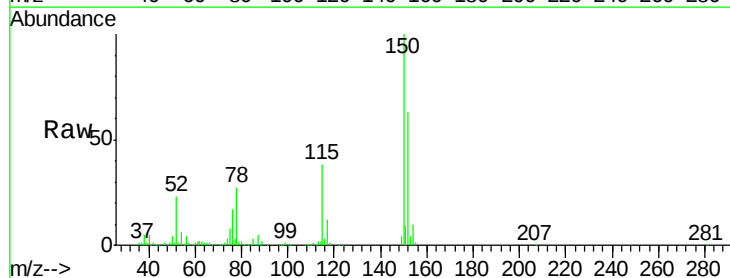

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

