


Acrolein


Response Ratio

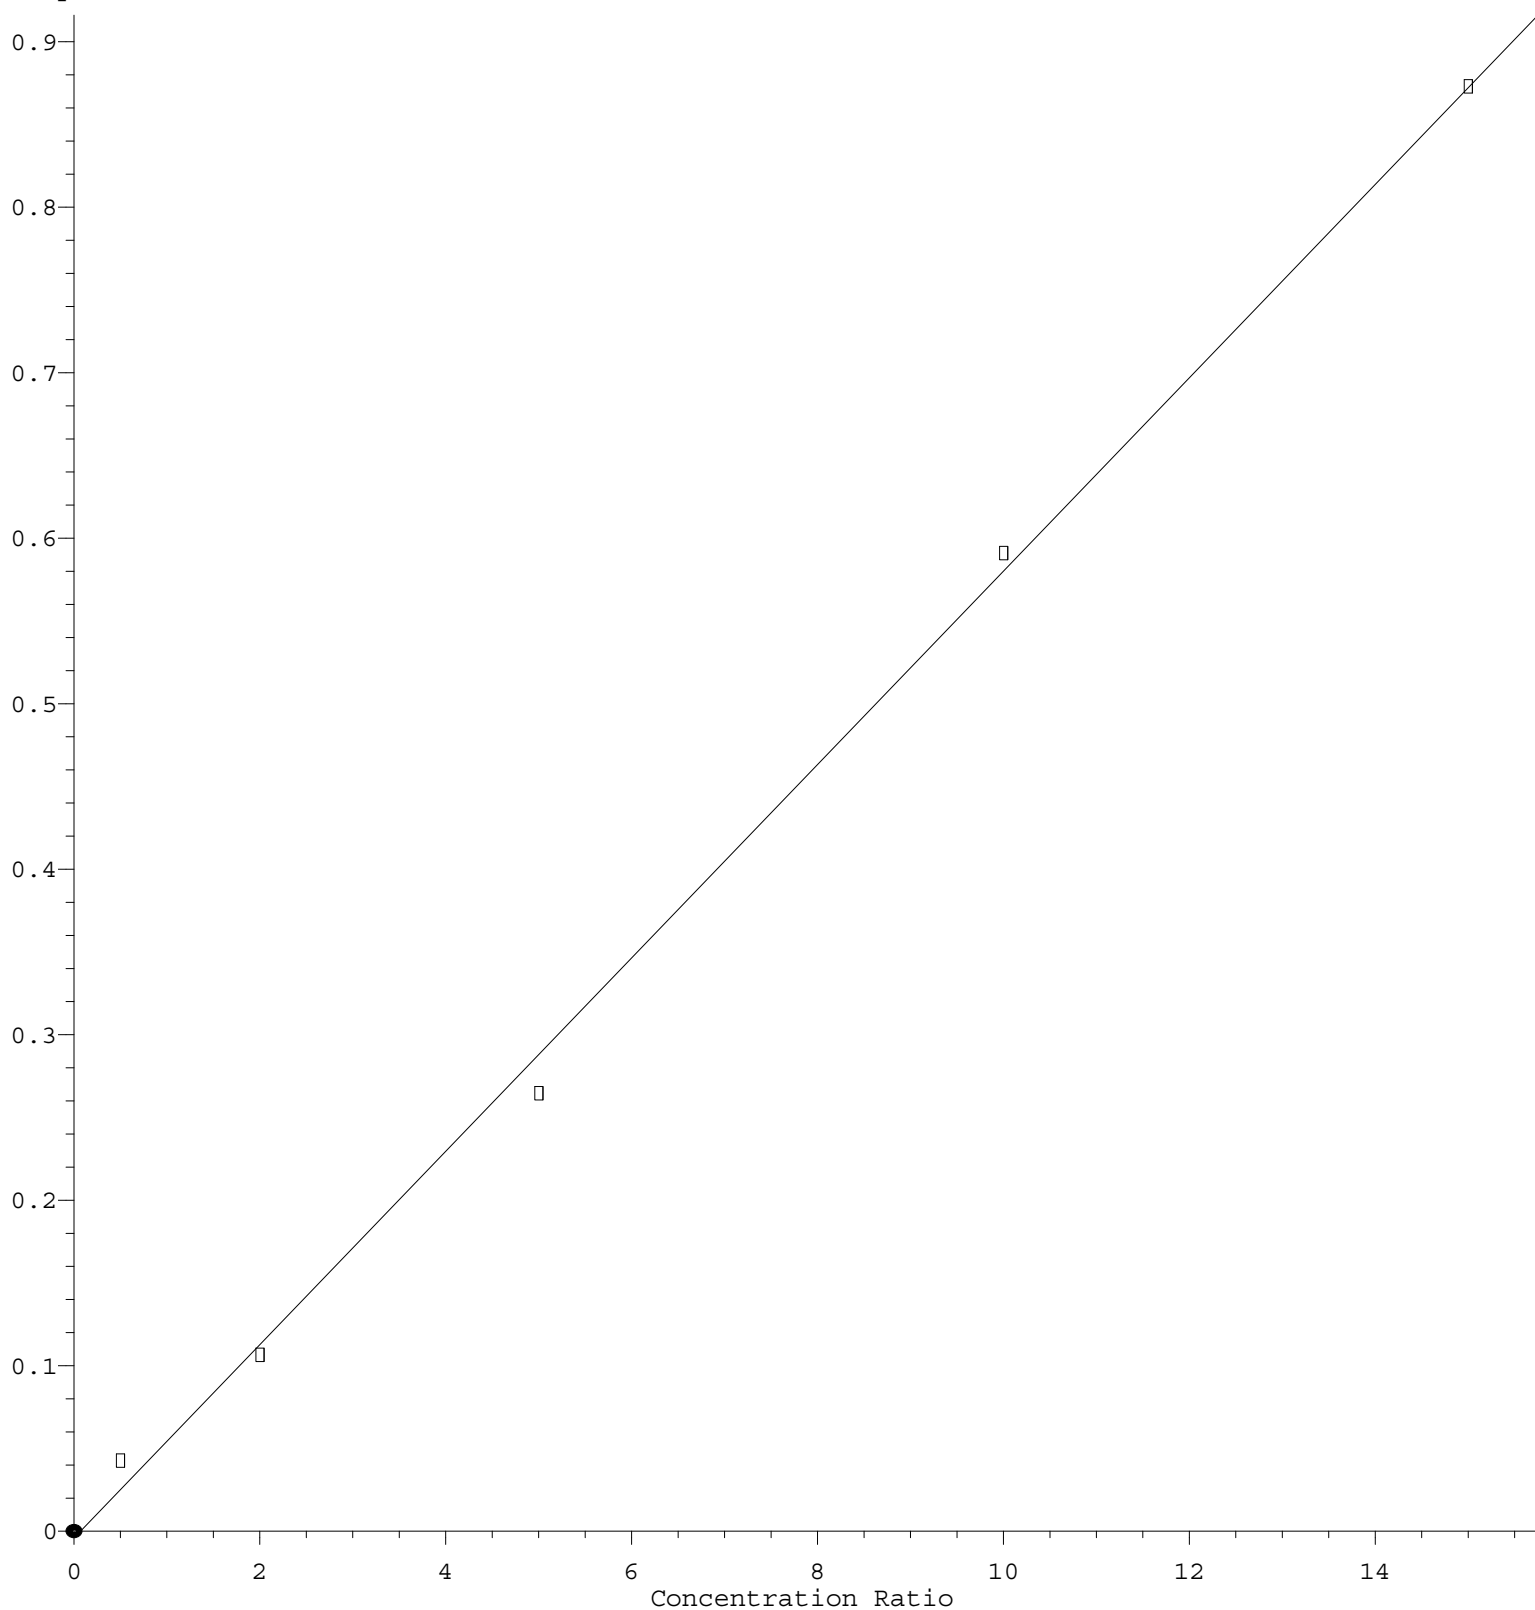

$\text{Response} = 5.843\text{e-}002 * \text{Amt} - 4.281\text{e-}003$
 Coef of Det (r^2) = 0.997931 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N040621W.M
 Calibration Table Last Updated: Tue Apr 06 15:38:34 2021

N-amyl acetate

Response Ratio

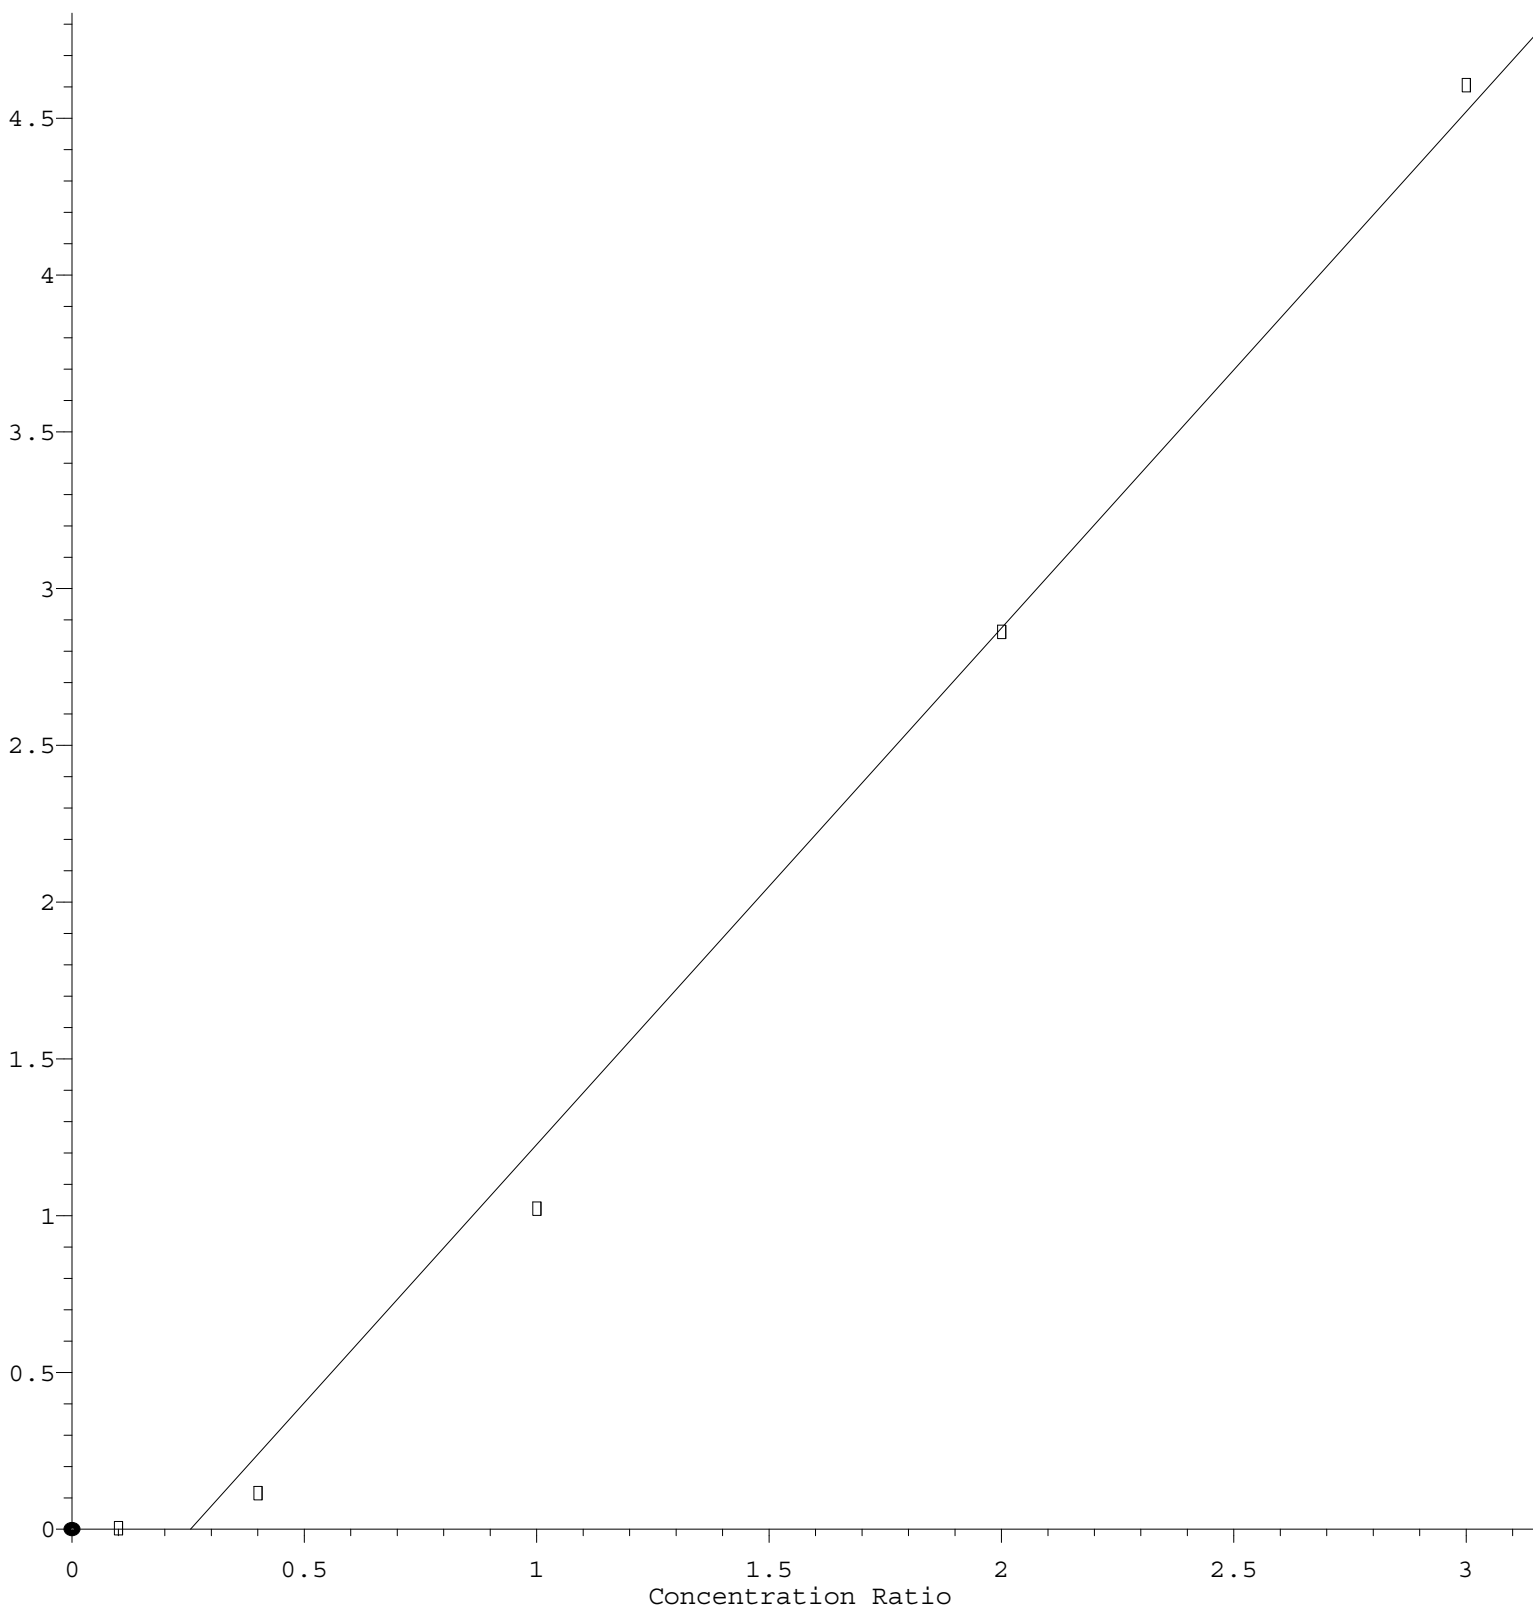

$$\text{Response} = 1.647\text{e}+000 * \text{Amt} - 4.192\text{e}-001$$


Coef of Det (r^2) = 0.991601 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N040621W.M

Calibration Table Last Updated: Tue Apr 06 15:38:34 2021

Styrene

Response Ratio

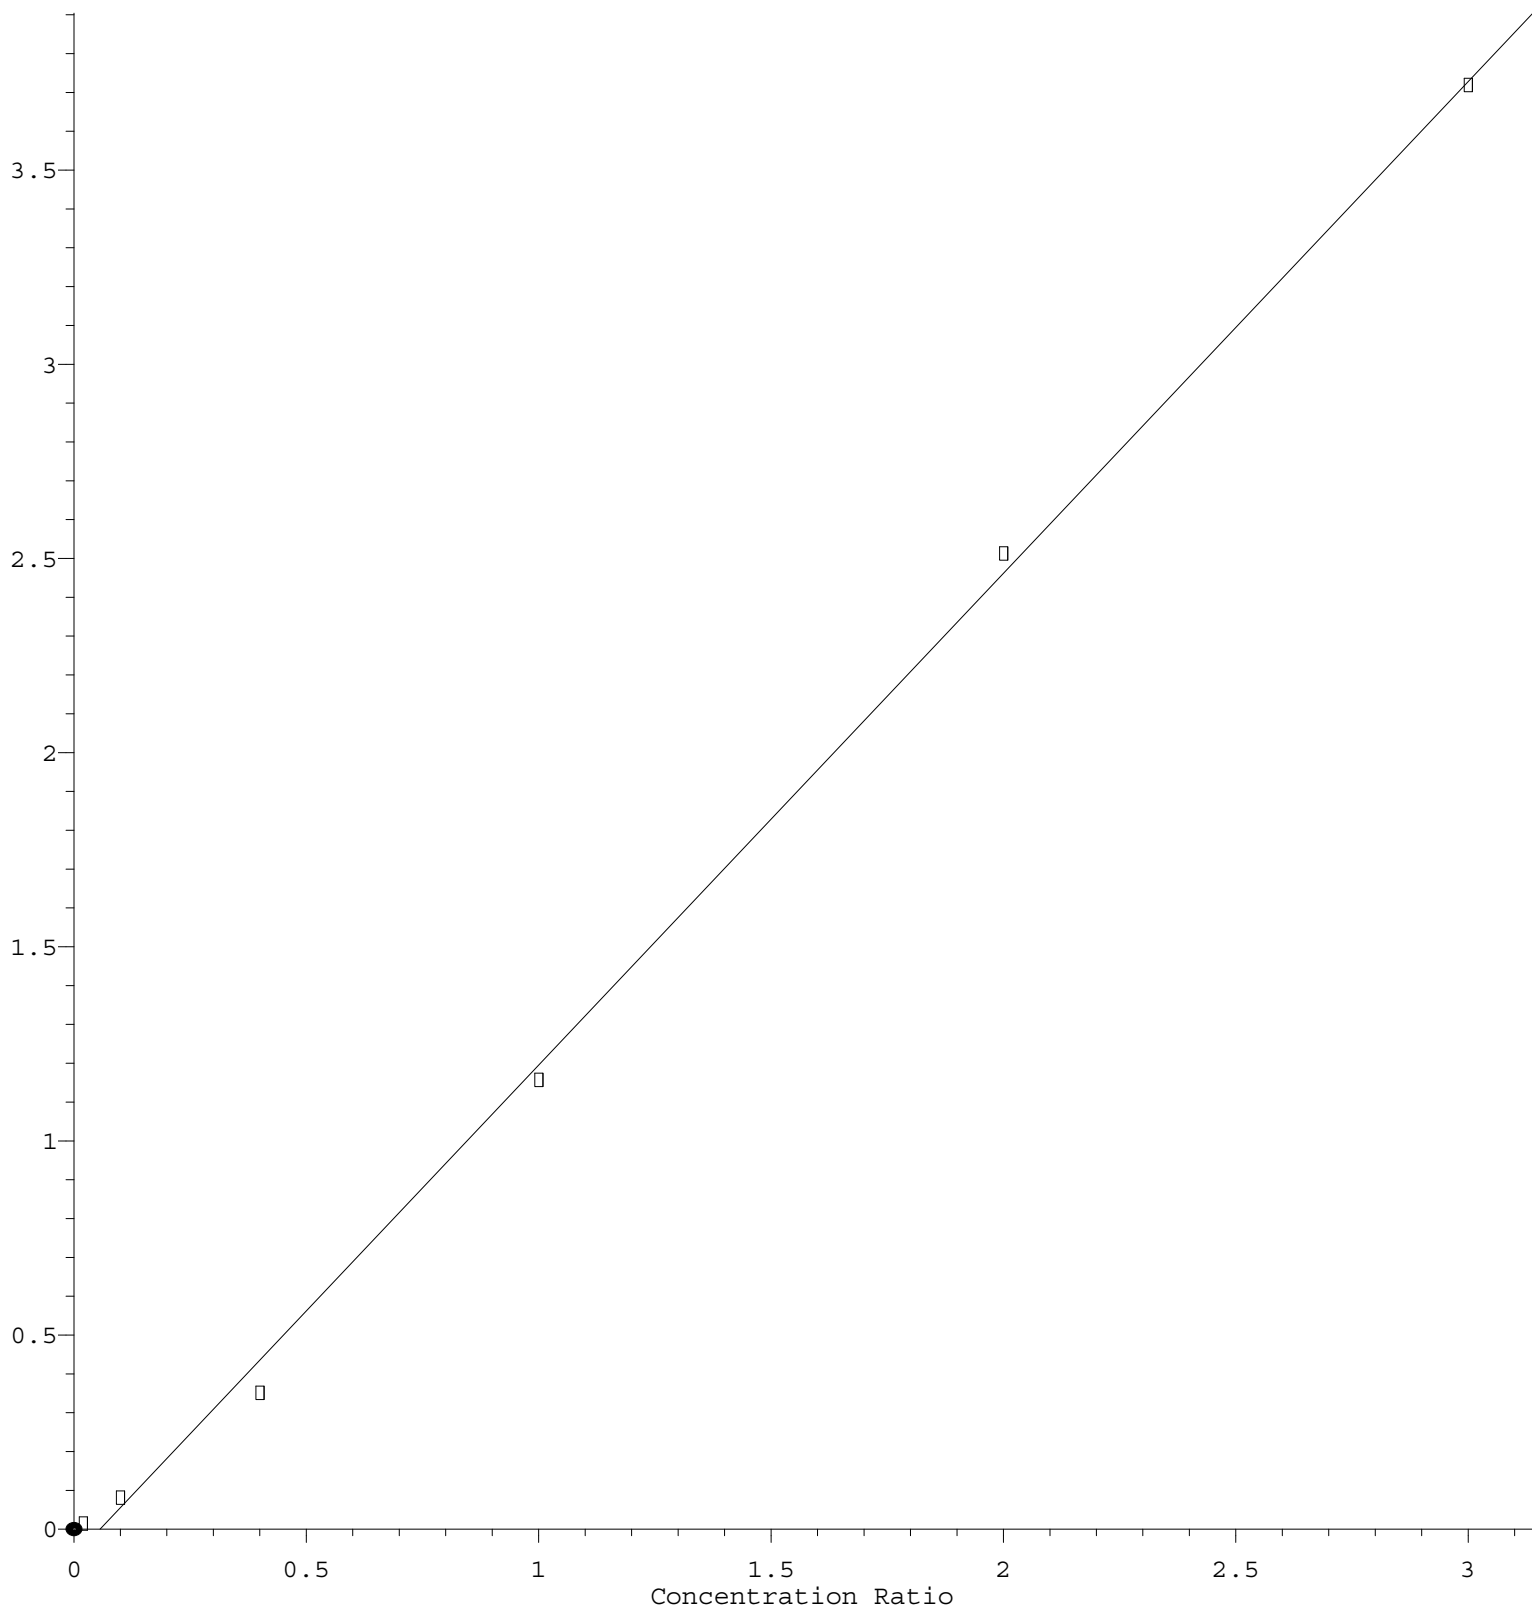

$$\text{Response} = 1.266\text{e}+000 * \text{Amt} - 7.039\text{e}-002$$


Coef of Det (r^2) = 0.998635 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N040621W.M

Calibration Table Last Updated: Tue Apr 06 15:38:34 2021

2-Hexanone


Response Ratio

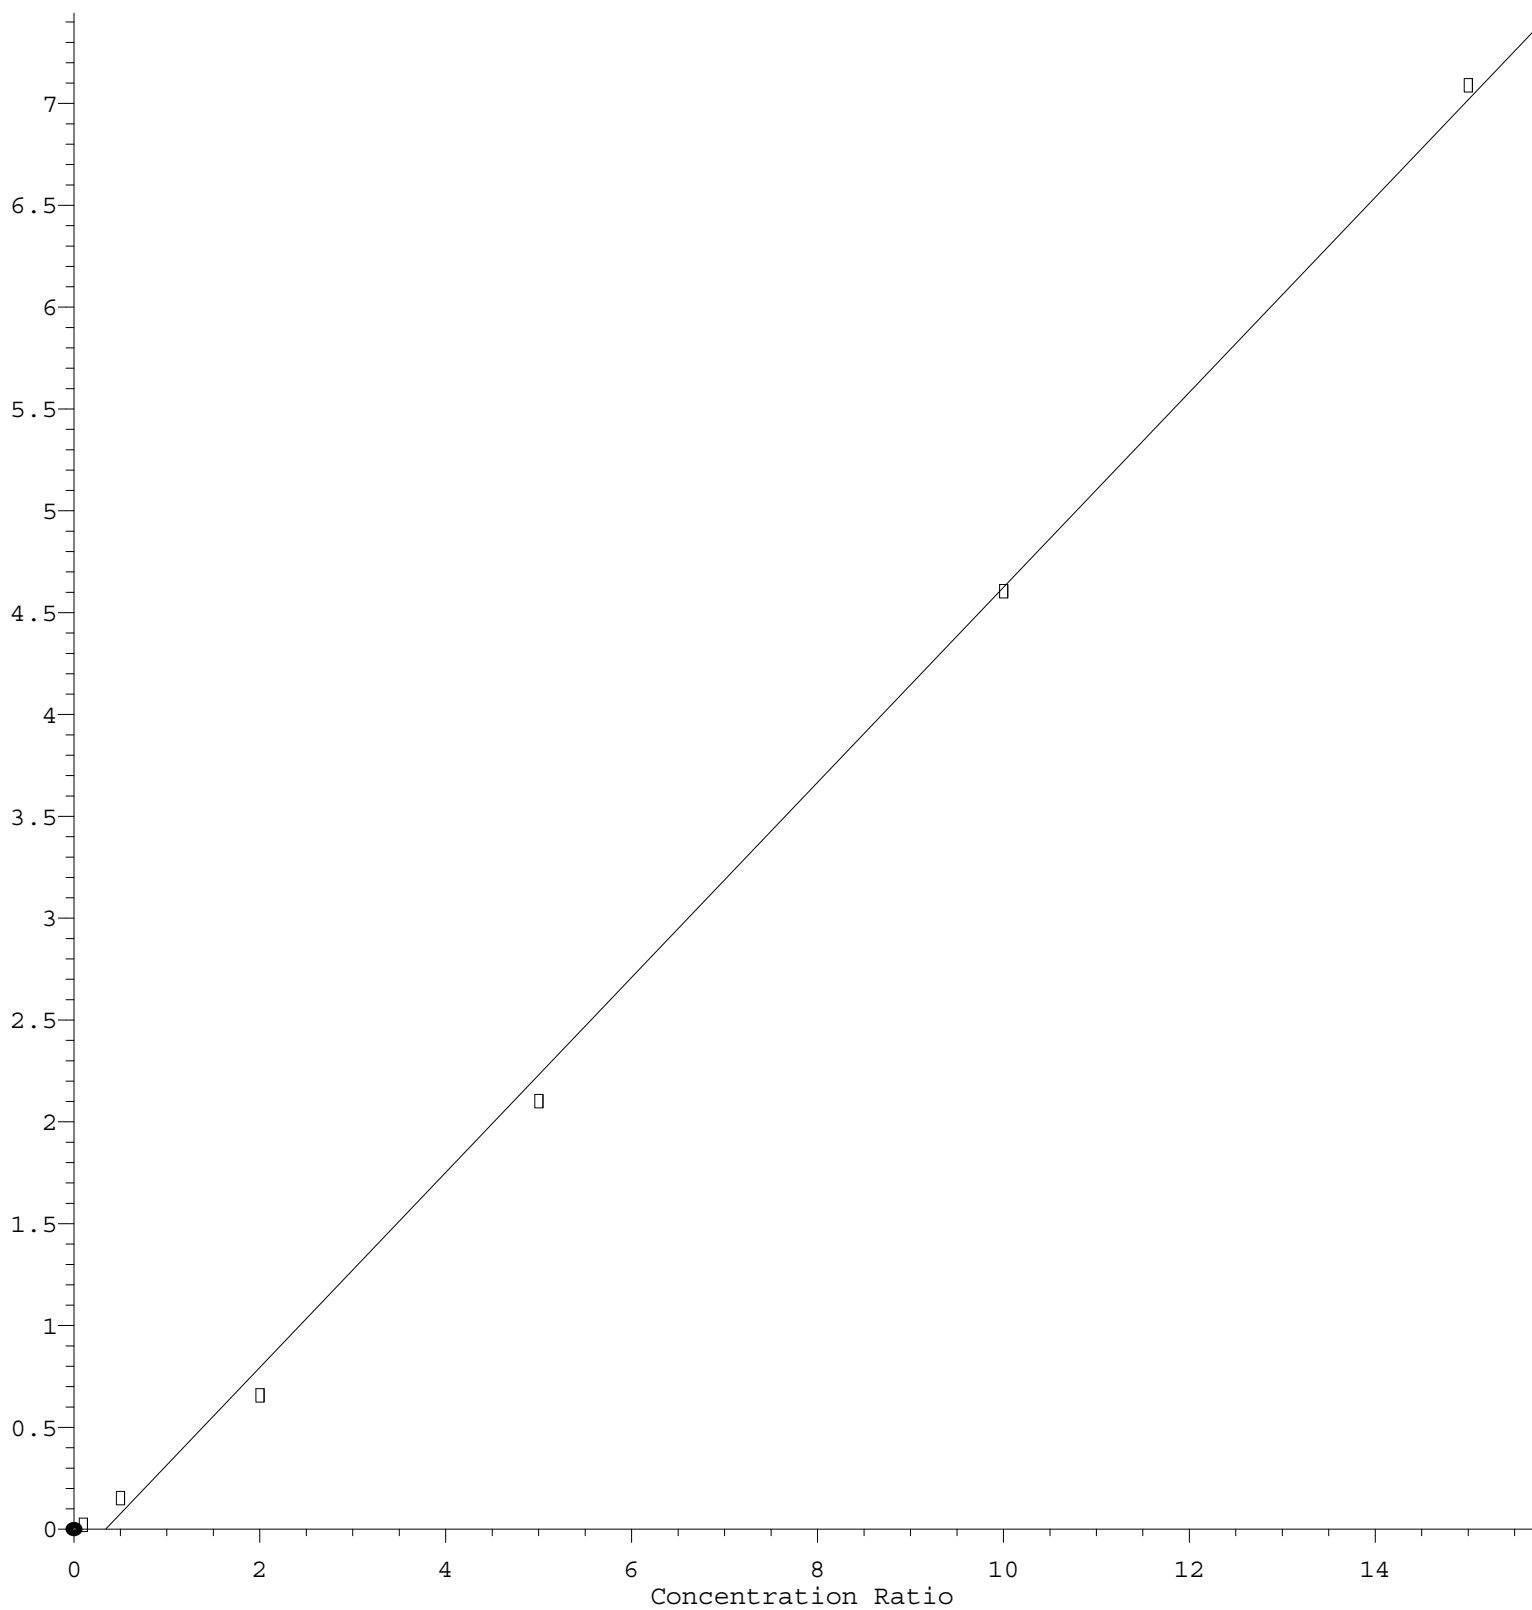

Response = 4.788e-001 * Amt - 1.639e-001
Coef of Det (r^2) = 0.998391 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N040621W.M
Calibration Table Last Updated: Tue Apr 06 15:38:34 2021

2-Chloroethyl Vinyl ether


Response Ratio

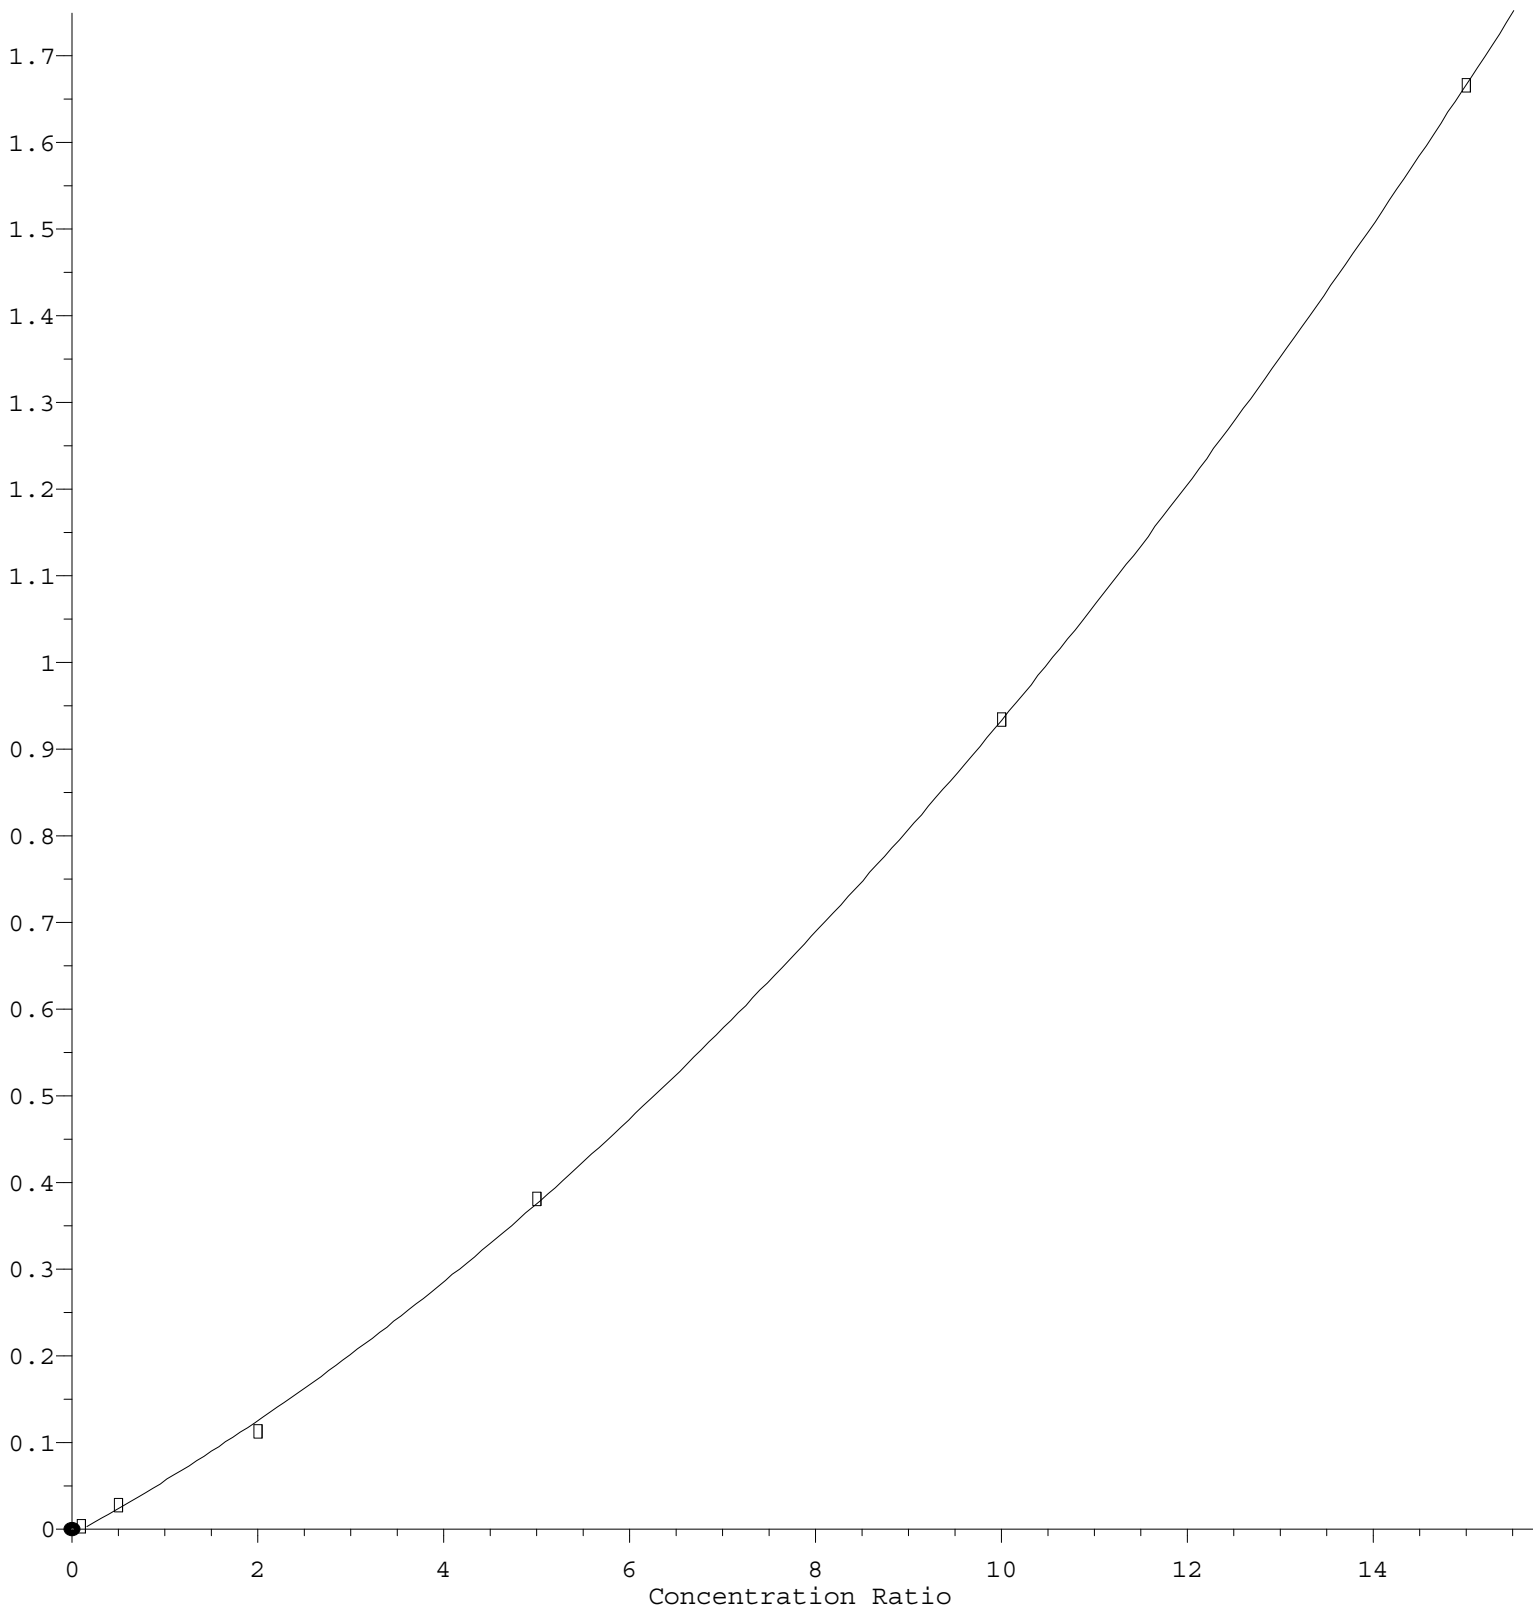

$R = 3.511e-003 A^2 + 5.885e-002 A - 6.295e-003$
 Coef of Det (r^2) = 0.999901 Curve Fit: Quadratic
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N040621W.M
 Calibration Table Last Updated: Tue Apr 06 15:38:34 2021

Ethyl methacrylate

Response Ratio

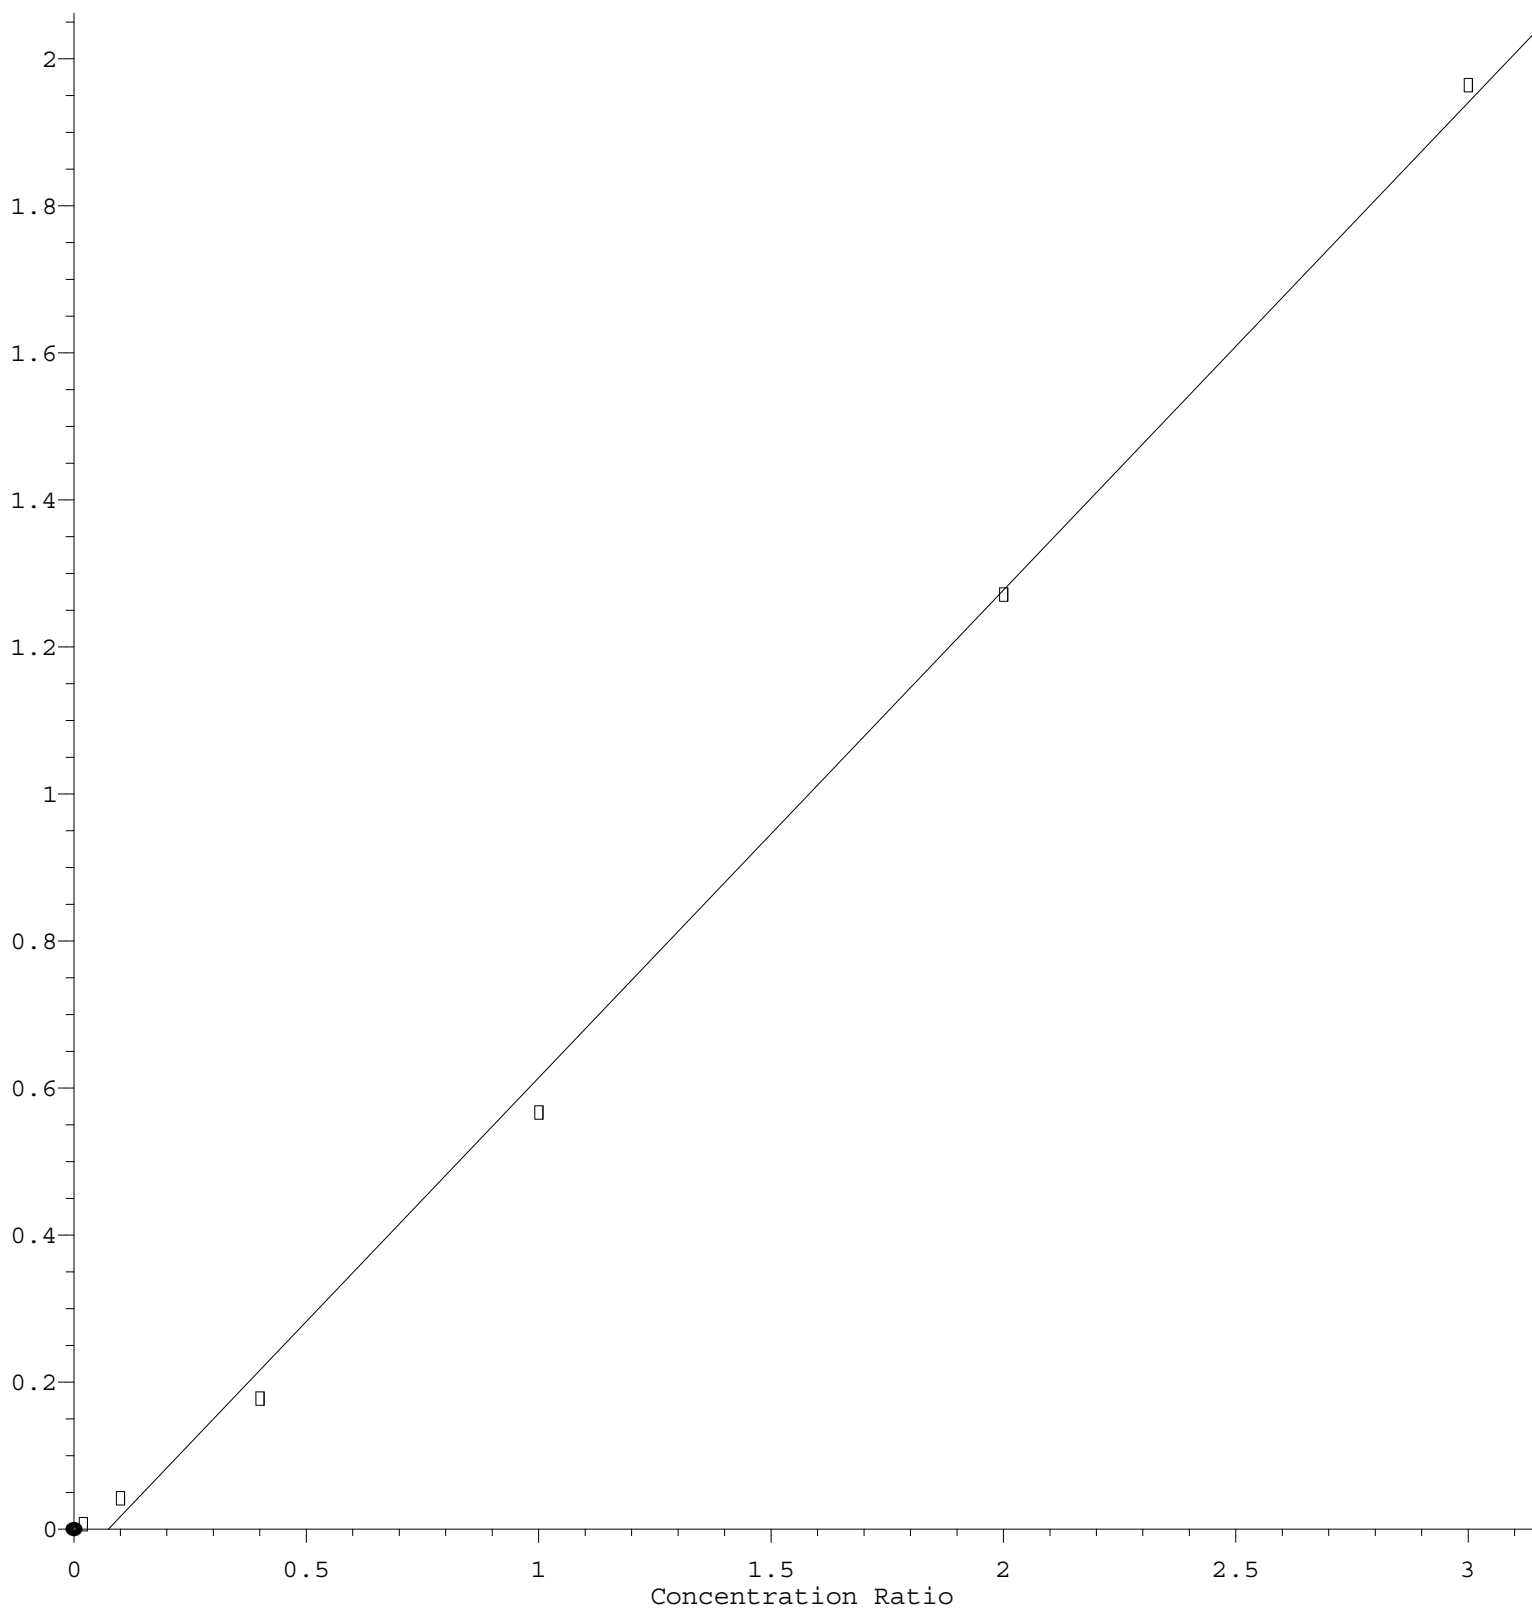

$$\text{Response} = 6.633\text{e-}001 * \text{Amt} - 4.934\text{e-}002$$


Coef of Det (r^2) = 0.997835 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N040621W.M

Calibration Table Last Updated: Tue Apr 06 15:38:34 2021

1,2,3-Trichlorobenzene

Response Ratio

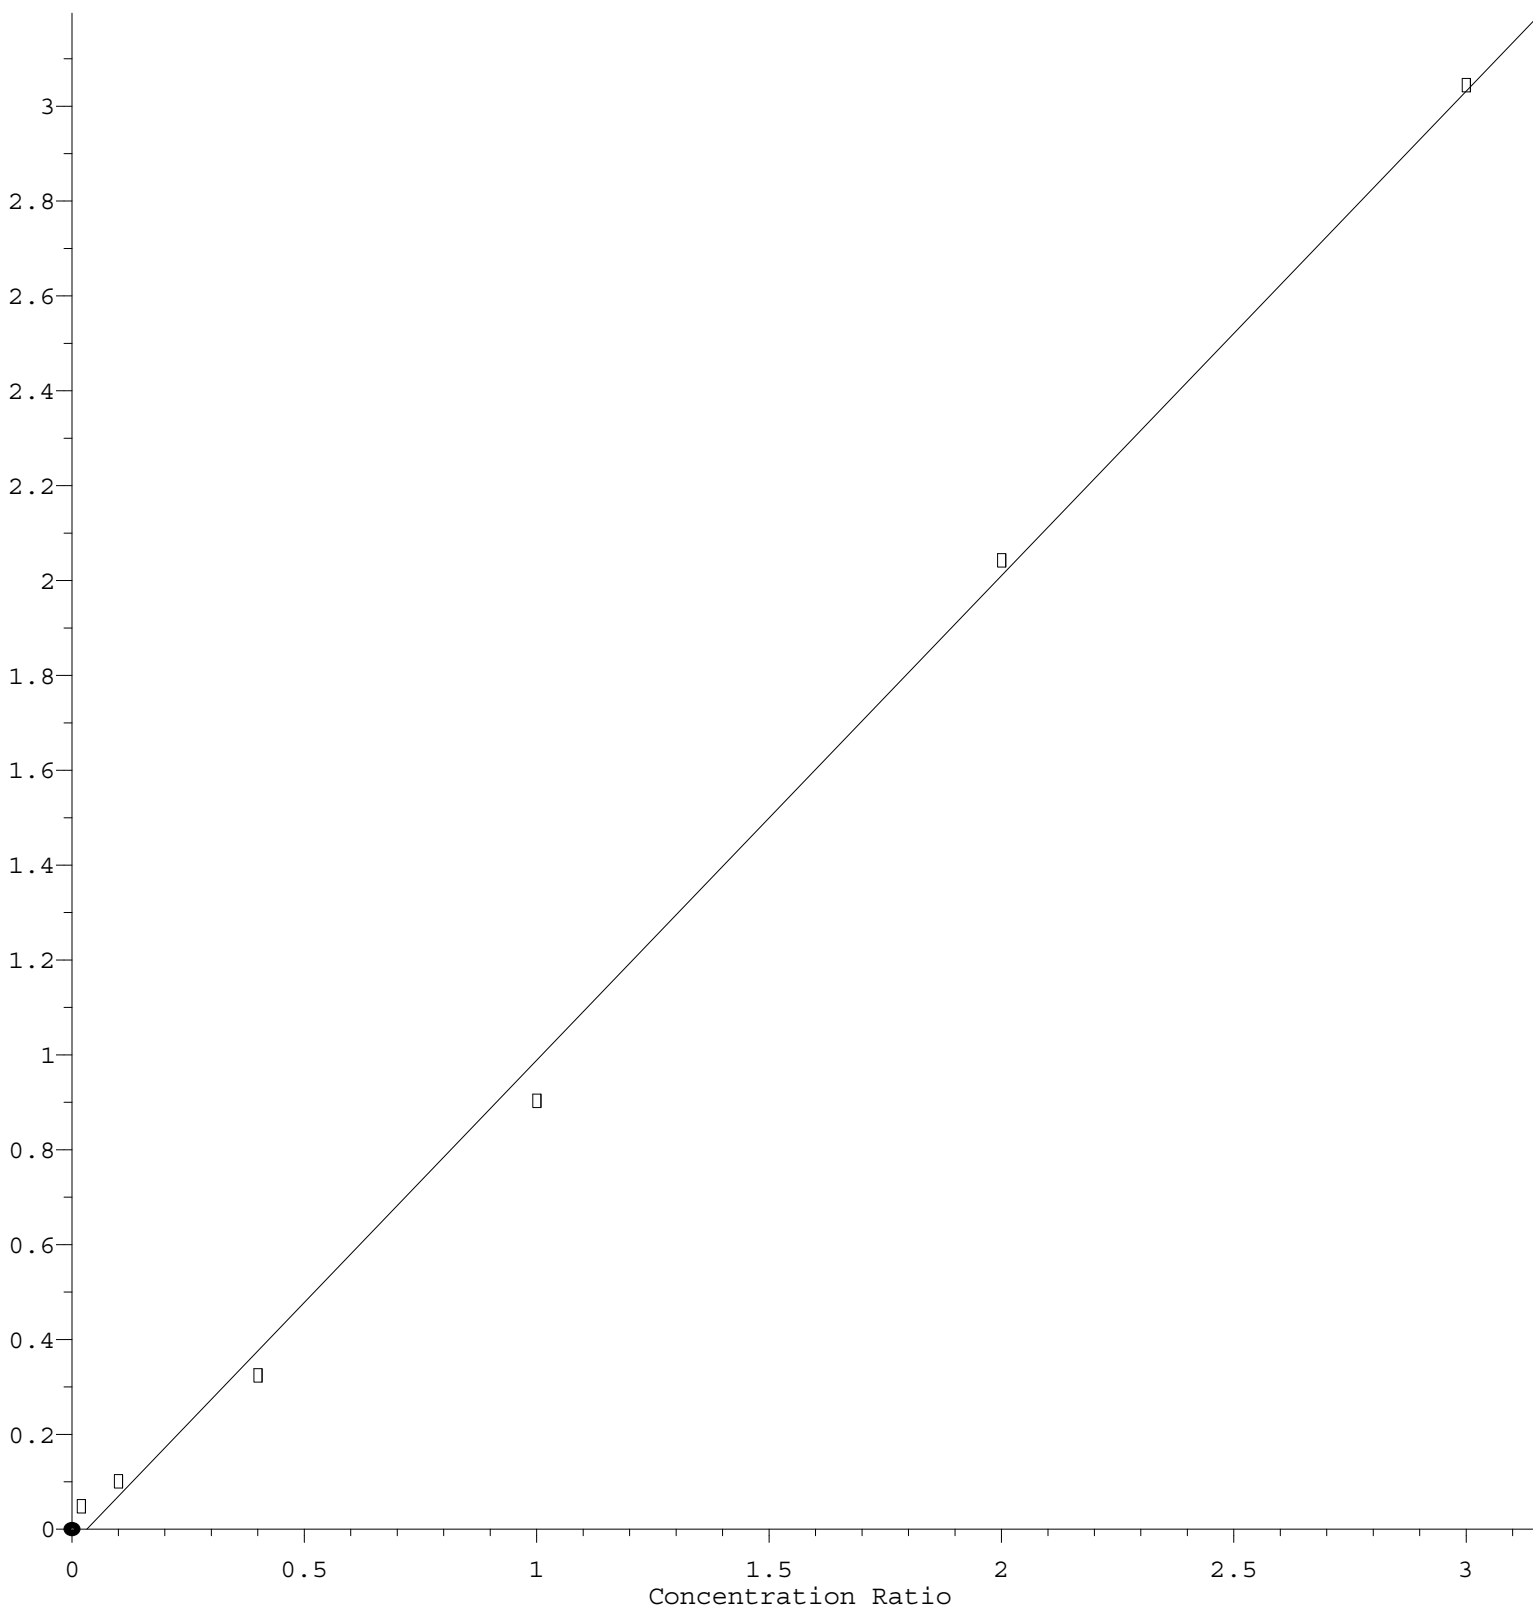

$$\text{Response} = 1.022\text{e}+000 * \text{Amt} - 3.298\text{e}-002$$


Coef of Det (r^2) = 0.997860 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N040621W.M

Calibration Table Last Updated: Tue Apr 06 15:38:34 2021

Naphthalene


Response Ratio

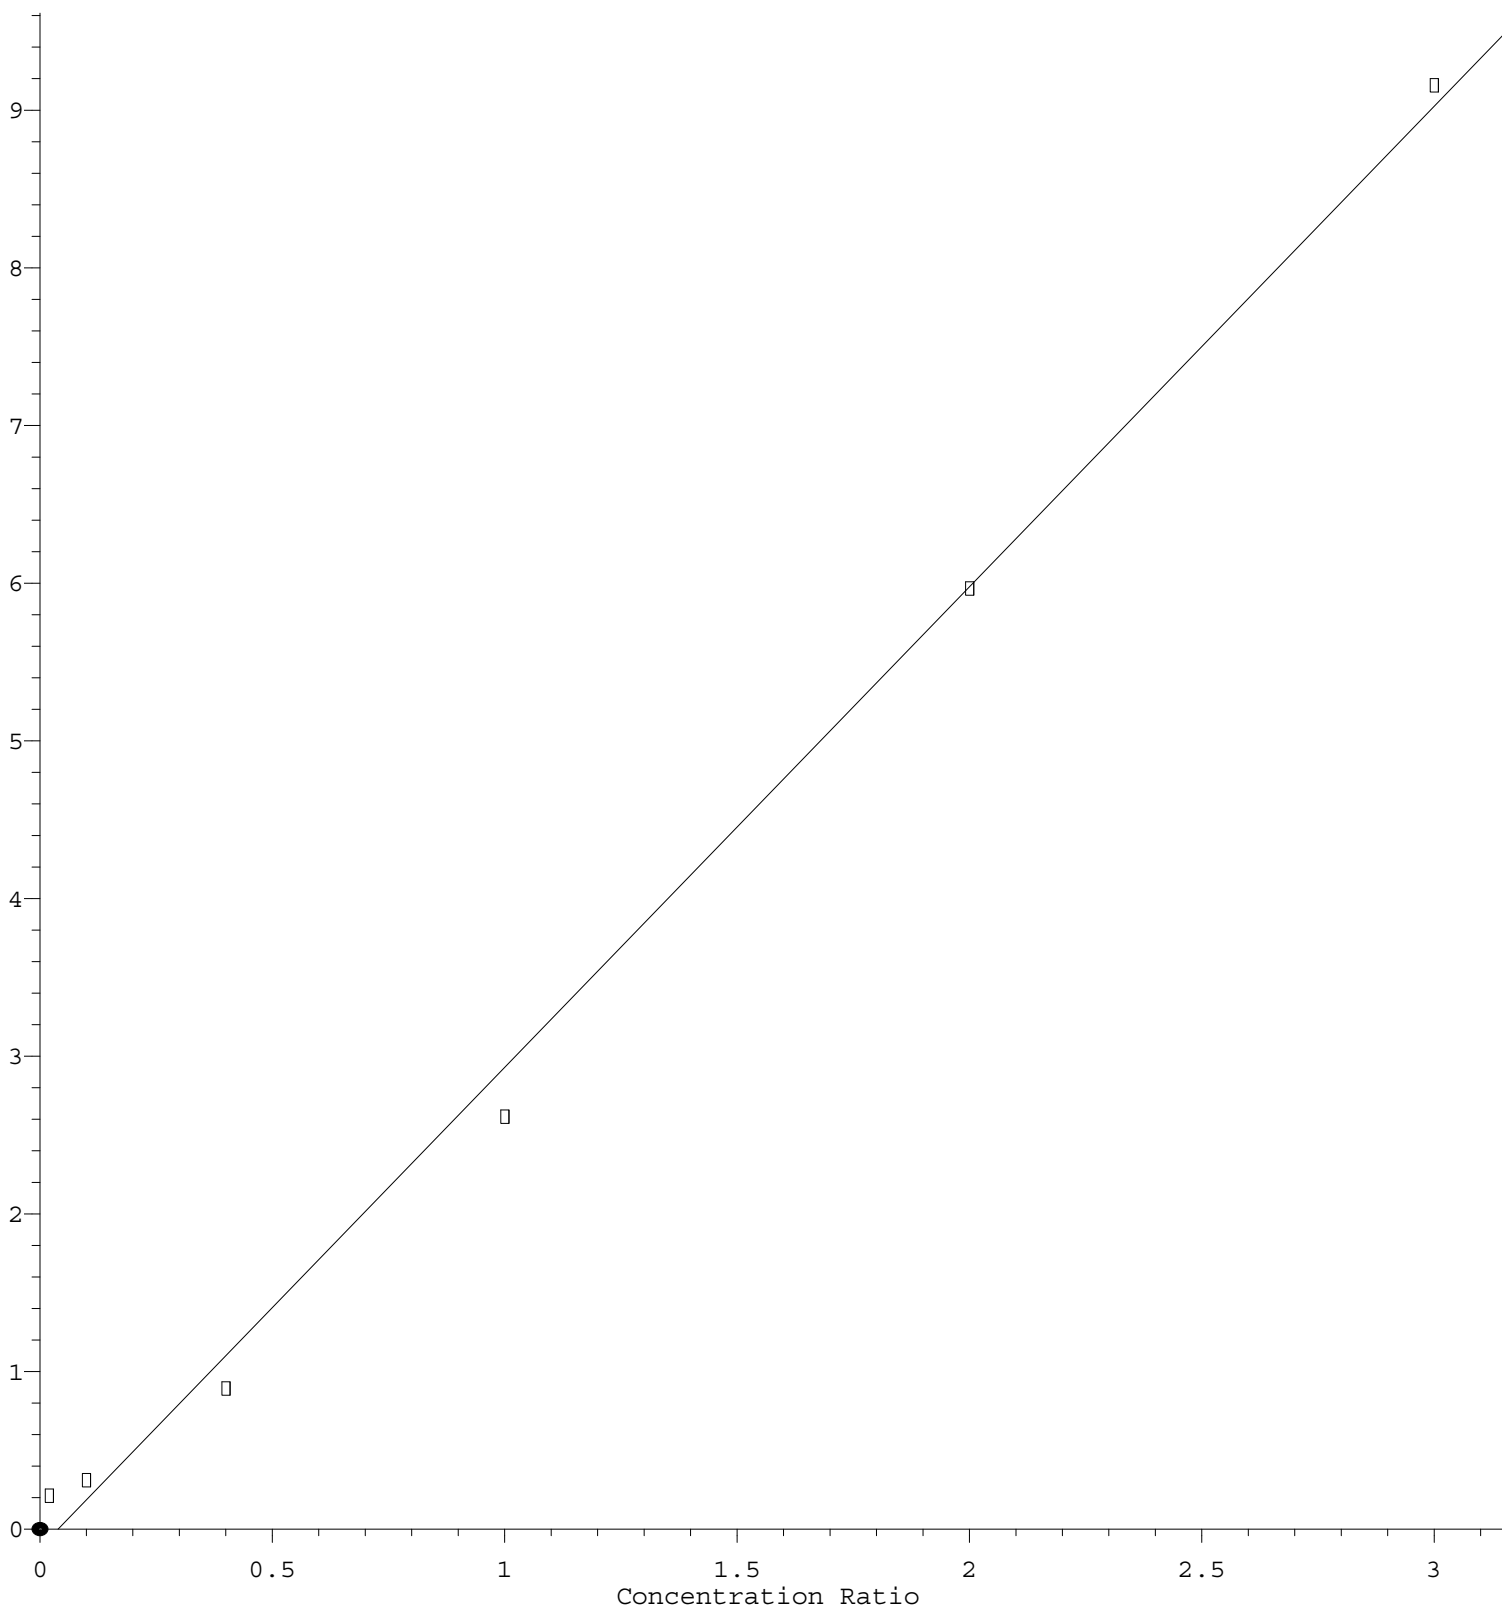

$\text{Response} = 3.048\text{e}+000 * \text{Amt} - 1.202\text{e}-001$
 Coef of Det (r^2) = 0.996255 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N040621W.M
 Calibration Table Last Updated: Tue Apr 06 15:38:34 2021

1,2,4-Trichlorobenzene

Response Ratio

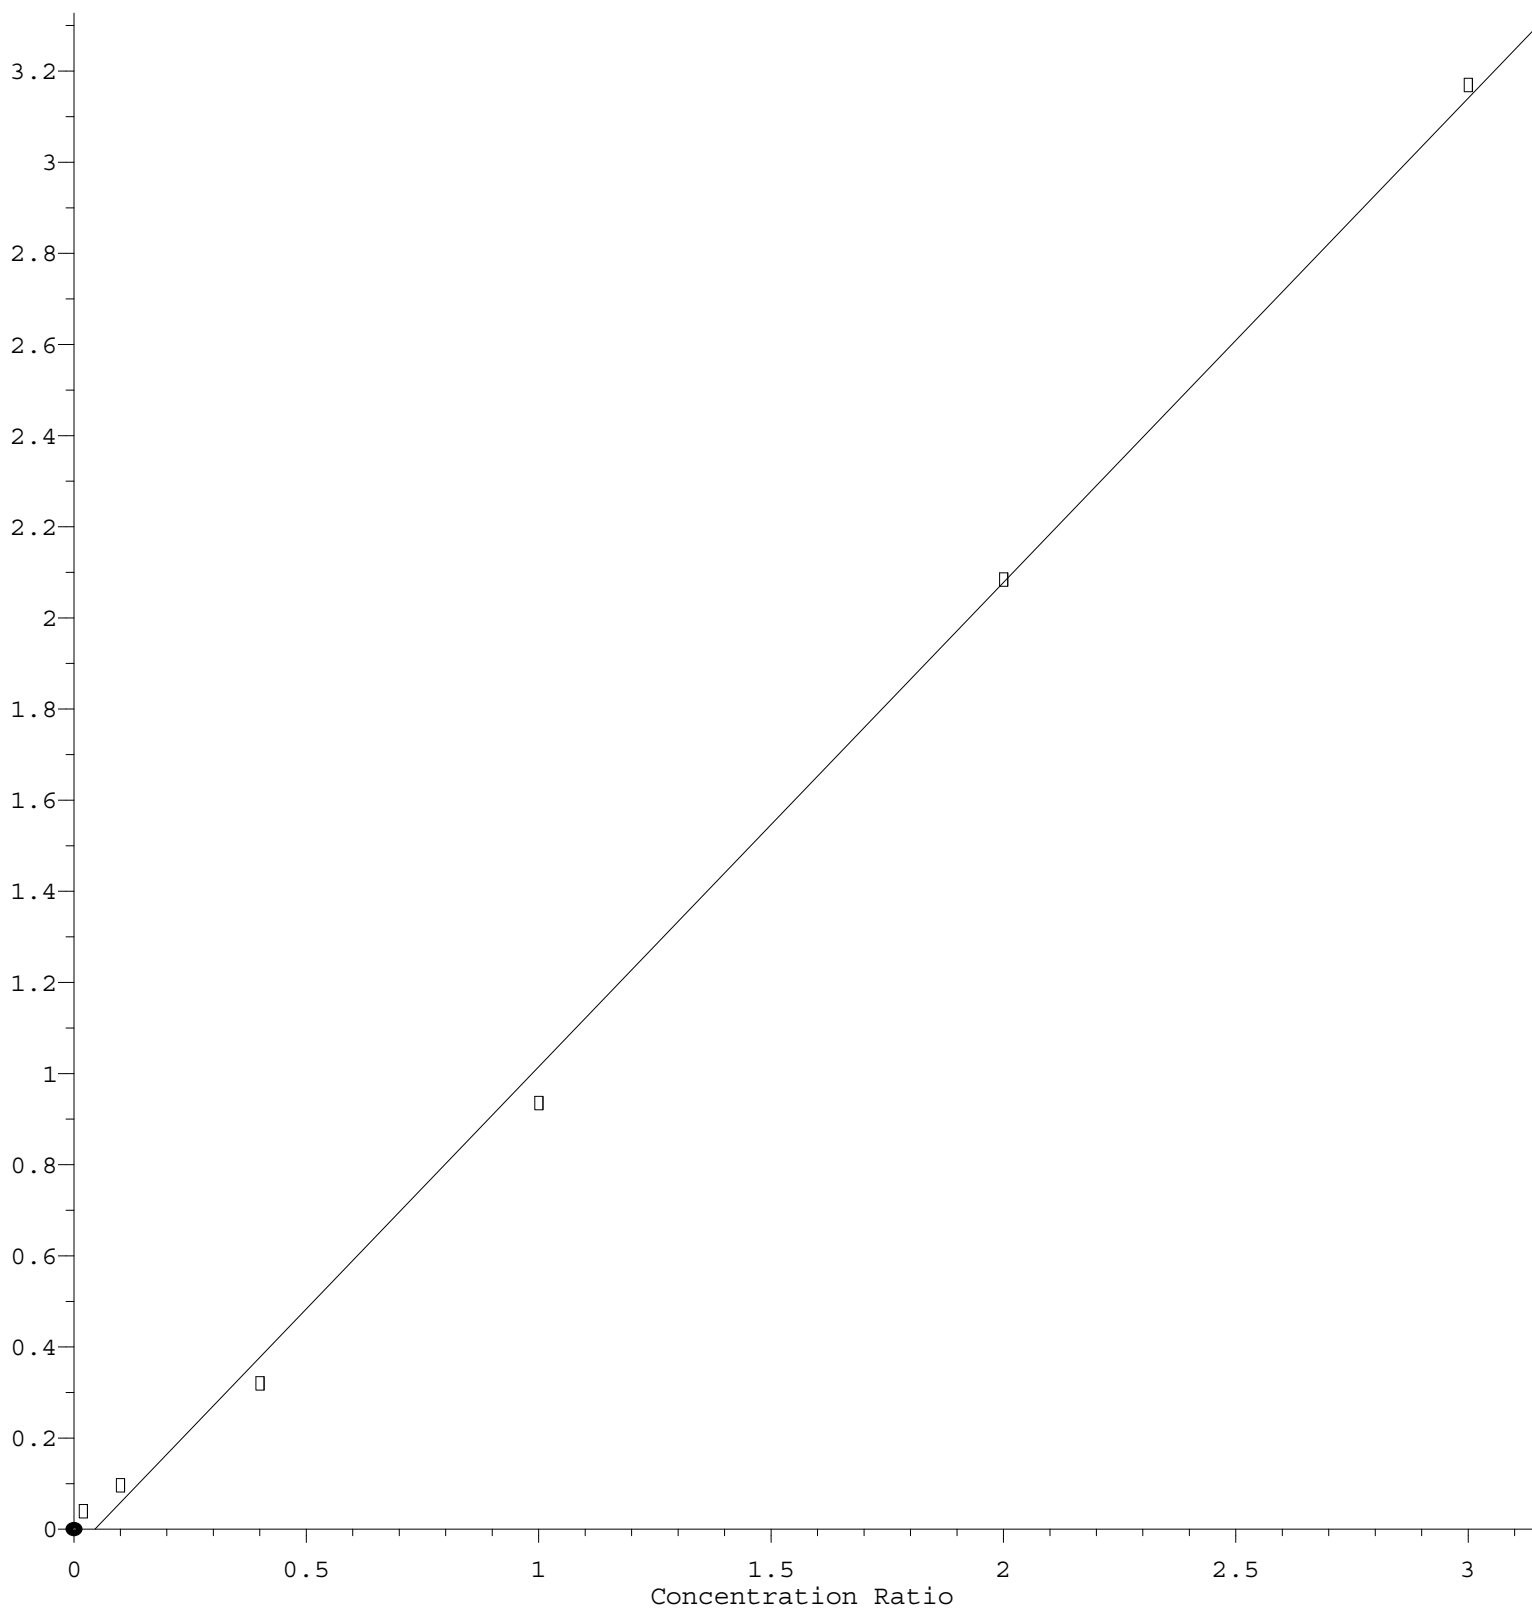

$$\text{Response} = 1.063\text{e}+000 * \text{Amt} - 4.757\text{e}-002$$


Coef of Det (r^2) = 0.997967 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N040621W.M

Calibration Table Last Updated: Tue Apr 06 15:38:34 2021

1,4-Dichlorobenzene

Response Ratio

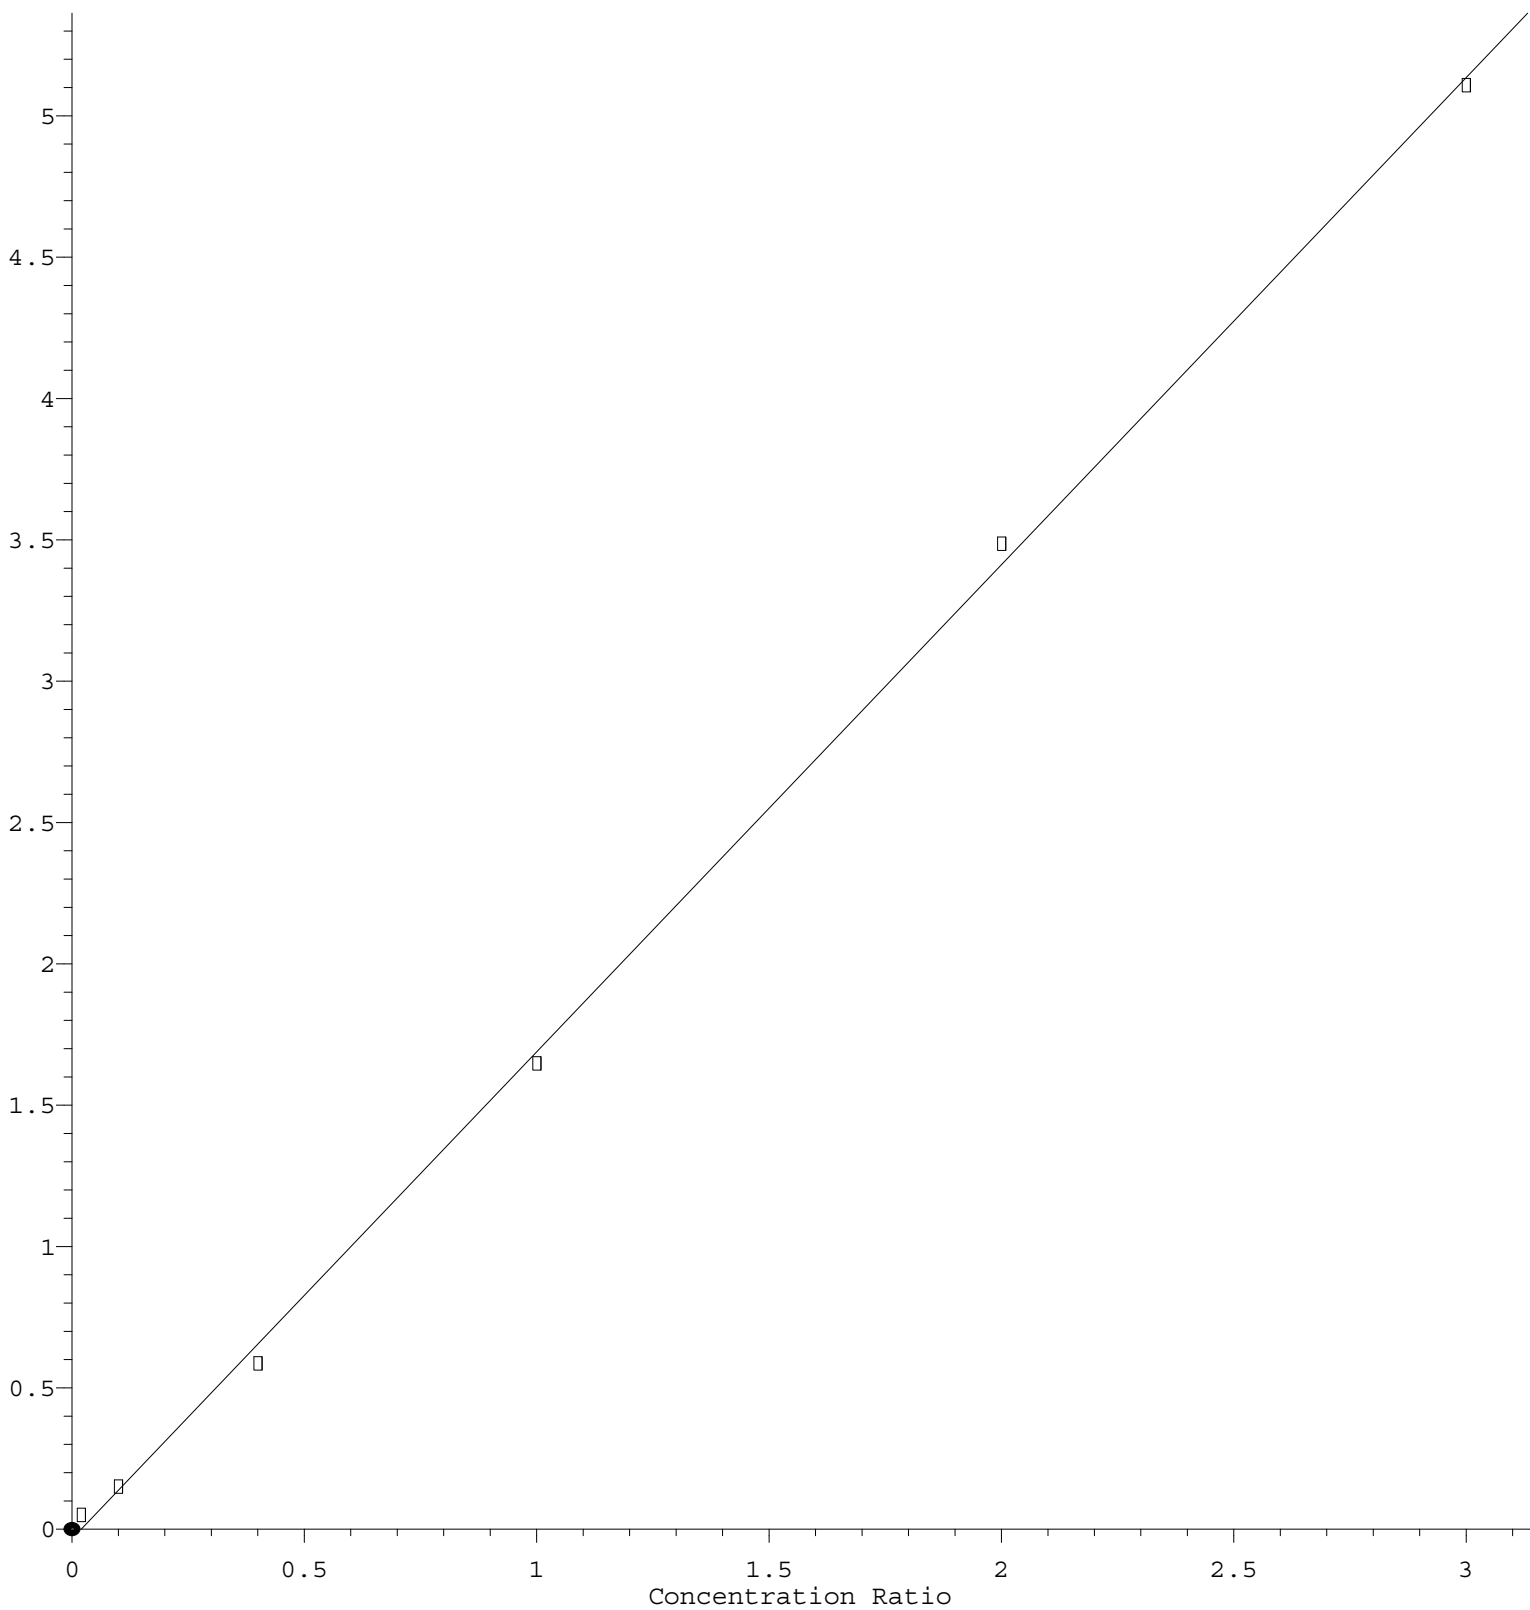

$$\text{Response} = 1.723\text{e}+000 * \text{Amt} - 3.447\text{e}-002$$


Coef of Det (r^2) = 0.999275 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N040621W.M

Calibration Table Last Updated: Tue Apr 06 15:38:34 2021

trans-1,4-Dichloro-2-butene

Response Ratio

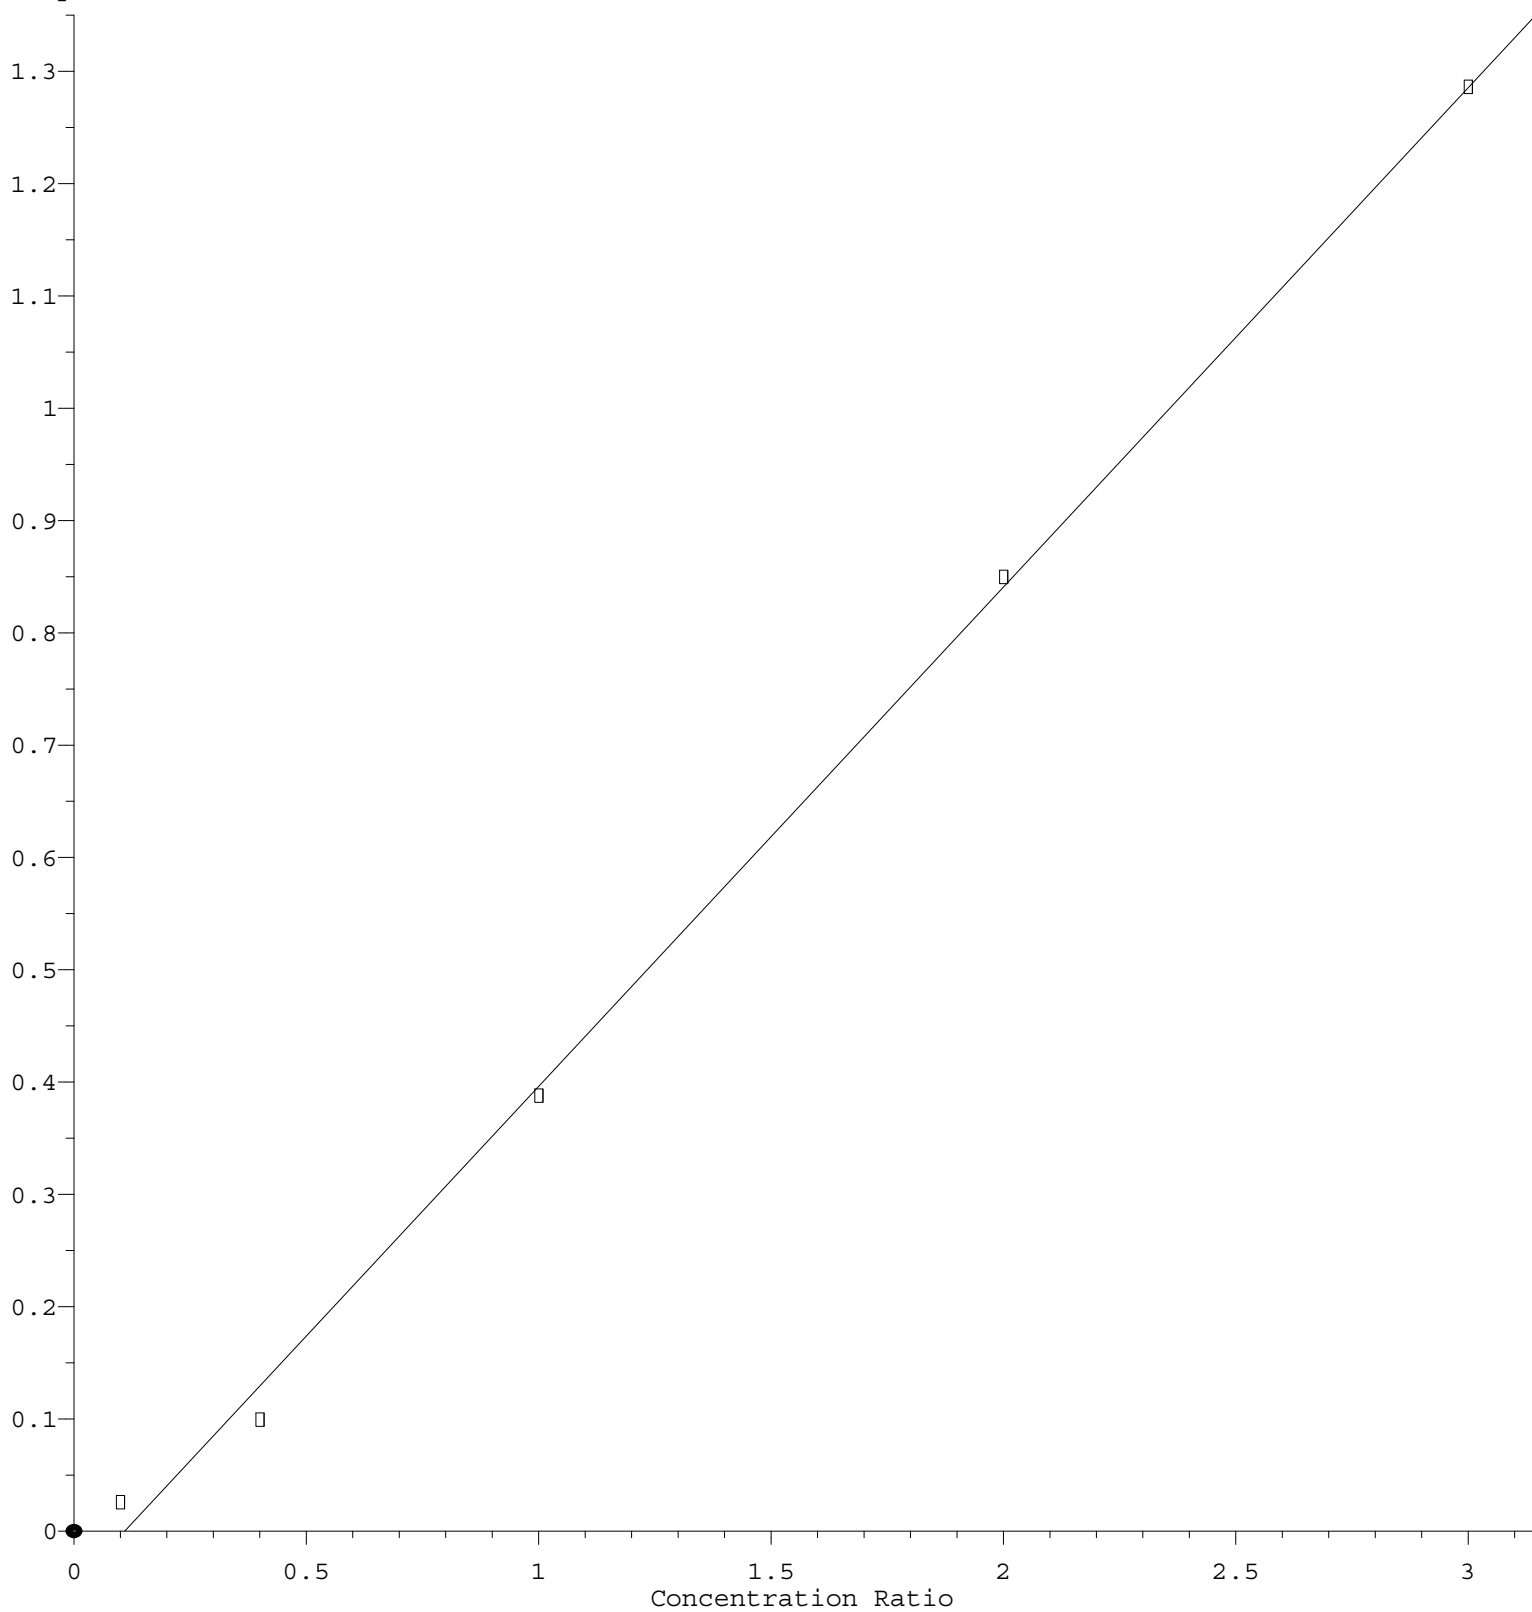

$$\text{Response} = 4.449\text{e-}001 * \text{Amt} - 4.855\text{e-}002$$

Coef of Det (r^2) = 0.998291 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N040621W.M

Calibration Table Last Updated: Tue Apr 06 15:38:34 2021