
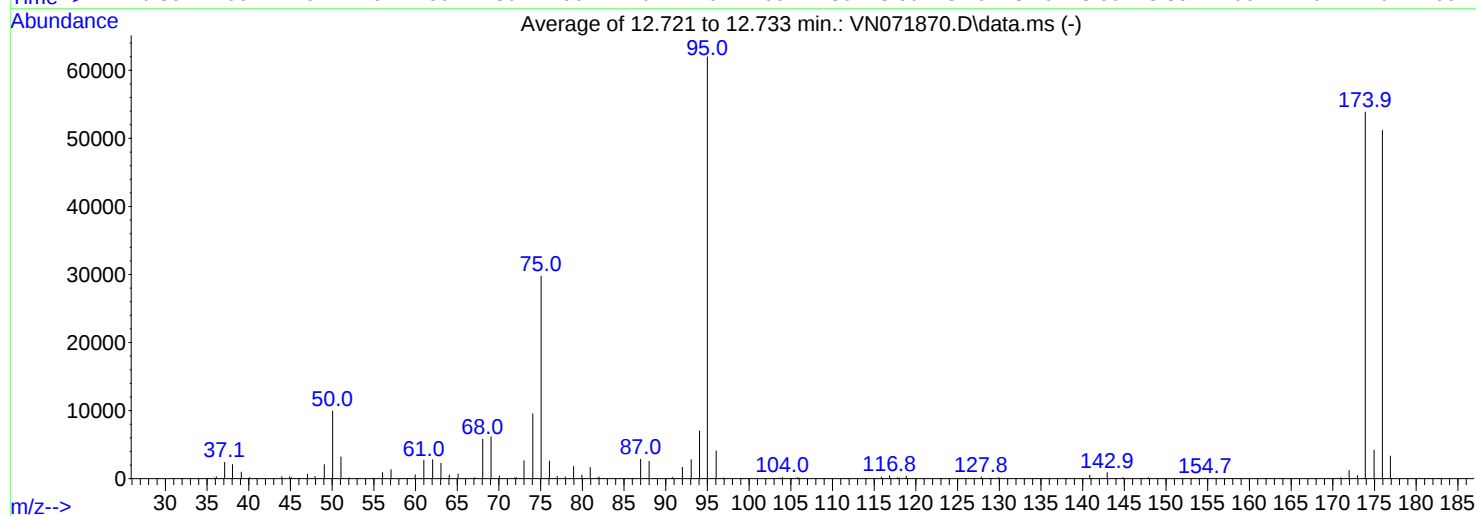


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN040622\
 Data File : VN071870.D
 Acq On : 06 Apr 2022 10:22
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
 Title : SW846 8260
 Last Update : Thu Mar 31 01:57:54 2022

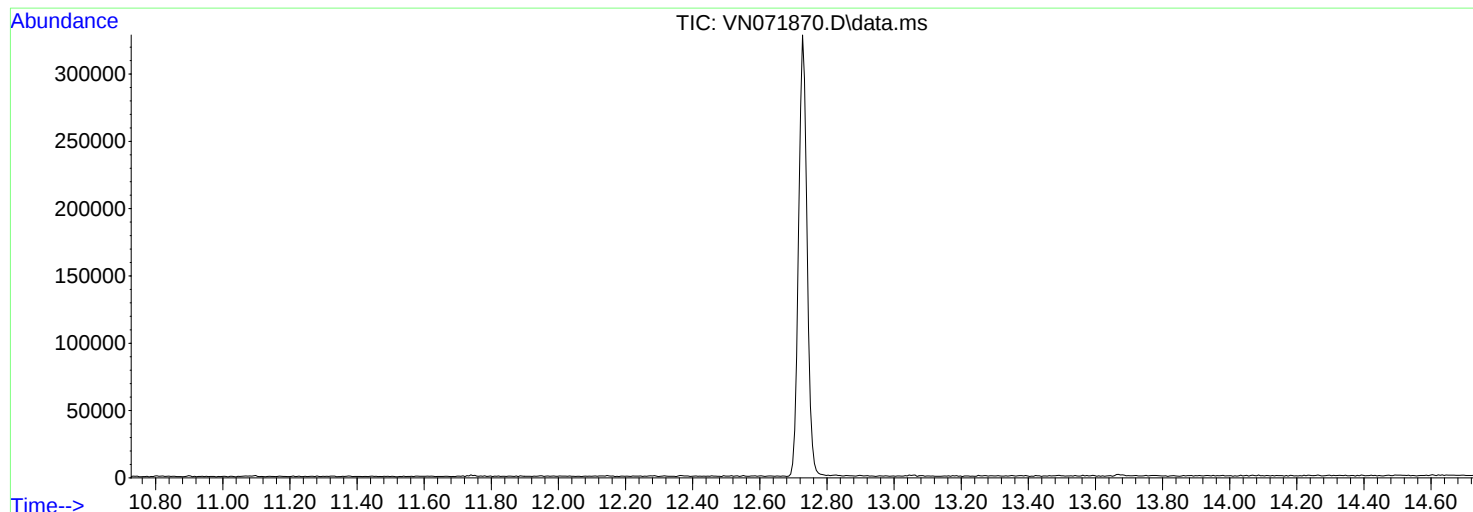

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1817

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	9951	PASS
75	95	30	60	48.0	29779	PASS
95	95	100	100	100.0	61984	PASS
96	95	5	9	6.6	4060	PASS
173	174	0.00	2	0.8	453	PASS
174	95	50	100	86.9	53877	PASS
175	174	5	9	7.8	4191	PASS
176	174	95	101	95.0	51197	PASS
177	176	5	9	6.5	3326	PASS