

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN040720\
 Data File : VN060876.D
 Acq On : 7 Apr 2020 14:56
 Operator : JC/MD
 Sample : L2167-01
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 STORAGE-BLANK-SOIL-REF-6

Quant Time: Apr 09 06:56:46 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N031820W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 18 08:49:09 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.64	168	206454	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.56	114	339677	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.40	117	311772	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	135623	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.00	65	129939	45.85	ug/l	0.00
Spiked Amount	50.000		Recovery	=	91.70%	
35) Dibromofluoromethane	7.56	113	99517	48.45	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.90%	
50) Toluene-d8	10.08	98	418081	49.83	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.66%	
62) 4-Bromofluorobenzene	12.40	95	151688	49.34	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.68%	


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN040720\
Data File : VN060876.D
Acq On : 7 Apr 2020 14:56
Operator : JC/MD
Sample : L2167-01
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Quant Time: Apr 09 06:56:46 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N031820W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 18 08:49:09 2020
Response via : Initial Calibration

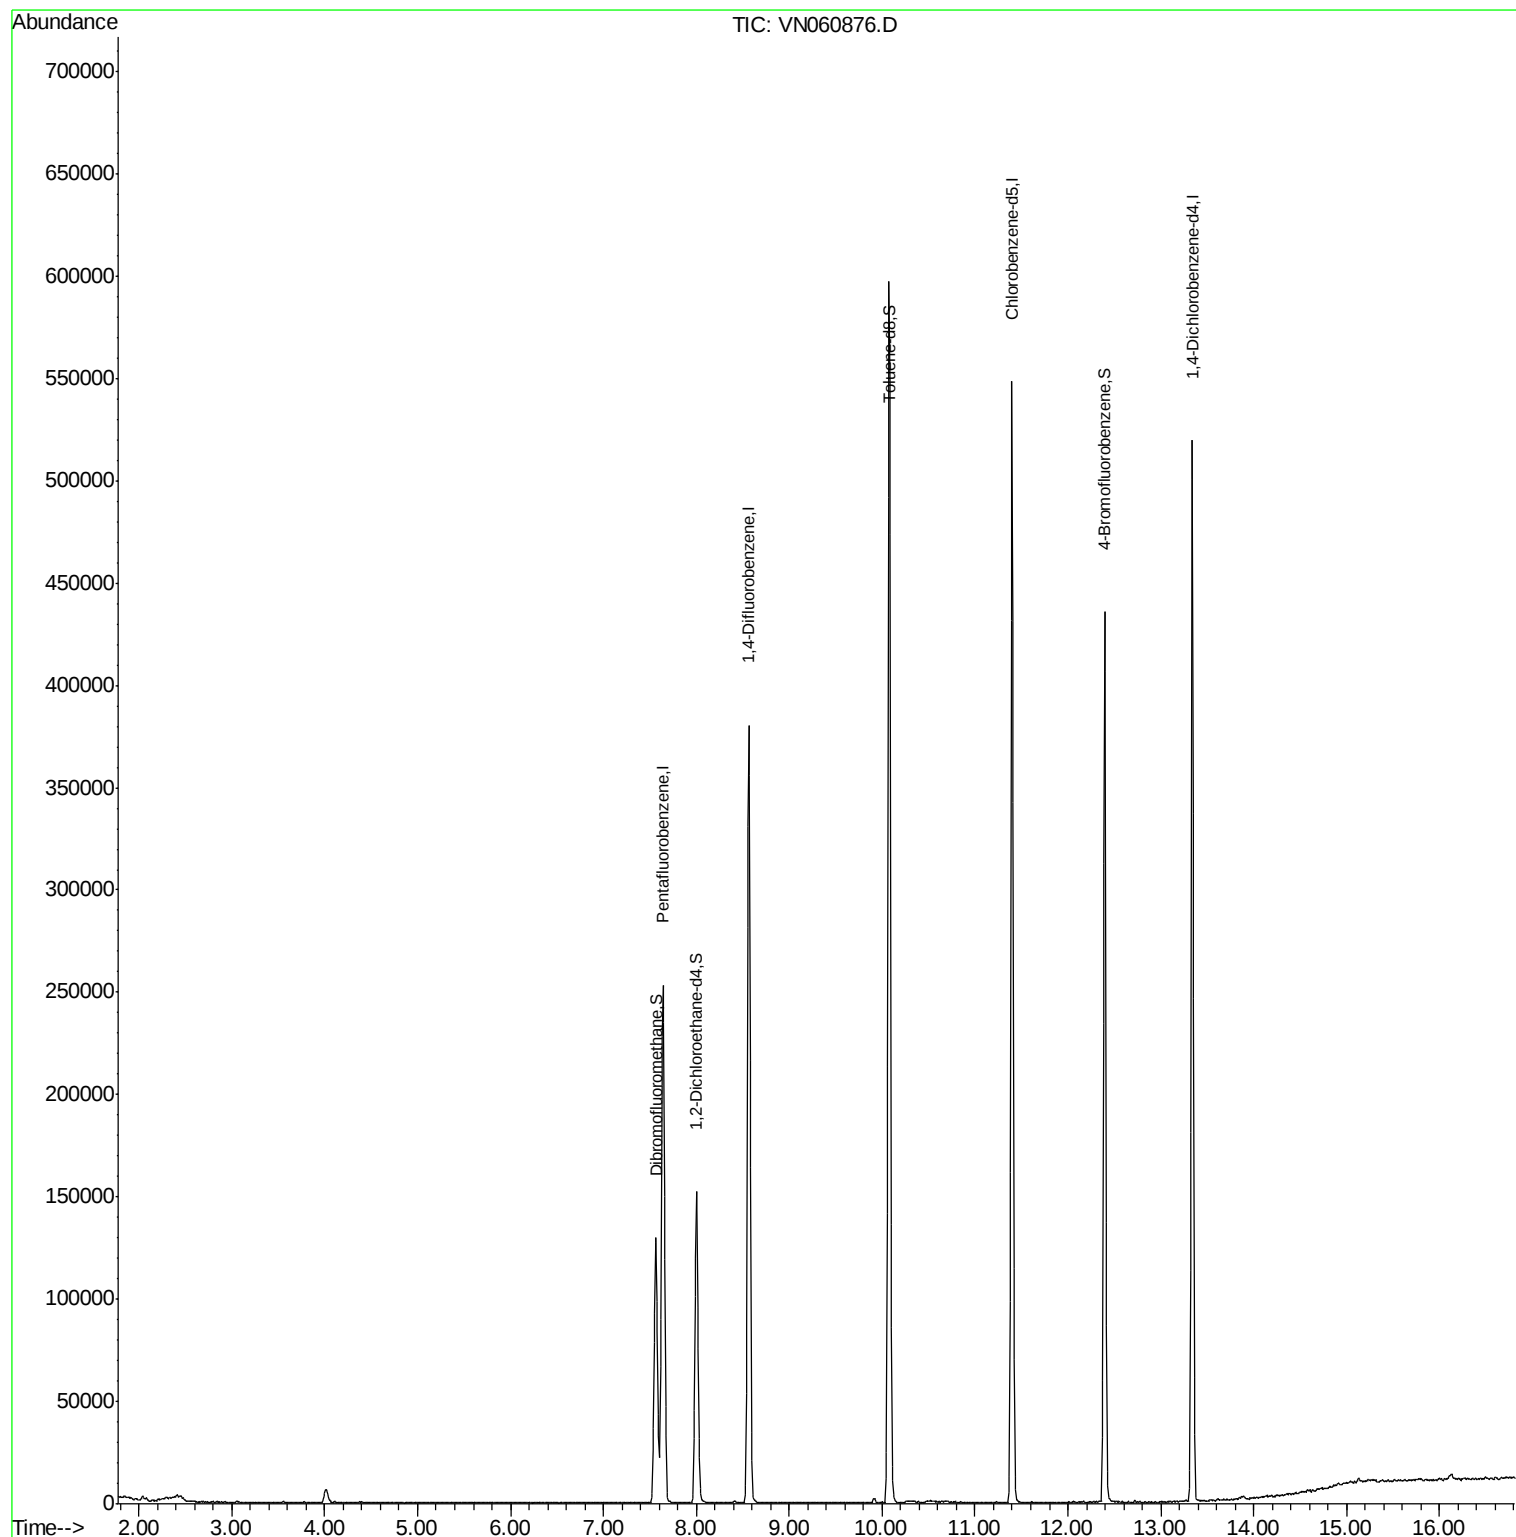



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.64 min Scan# 1825

Delta R.T. -0.00 min

Lab File: VN060876.D

Acq: 7 Apr 2020 14:56

Instrument :

MSVOA_N

ClientSampleId :


STORAGE-BLANK-SOIL-REF-6

Tot Ion:168 Resp: 206454

Ion Ratio Lower Upper




168 100

99 57.5 44.0 66.0

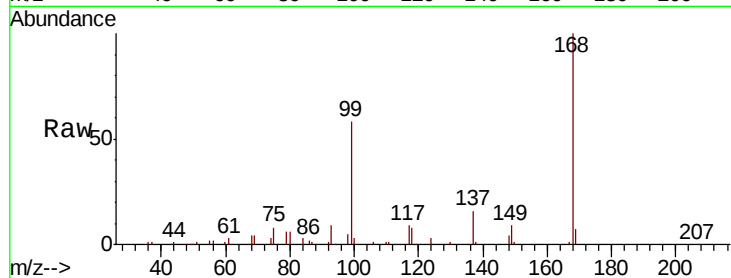

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

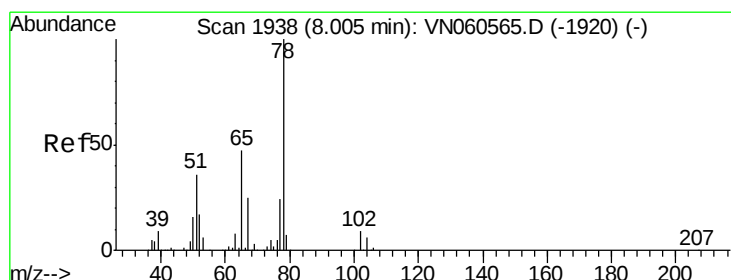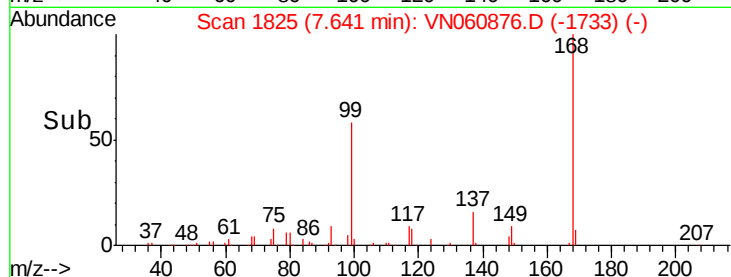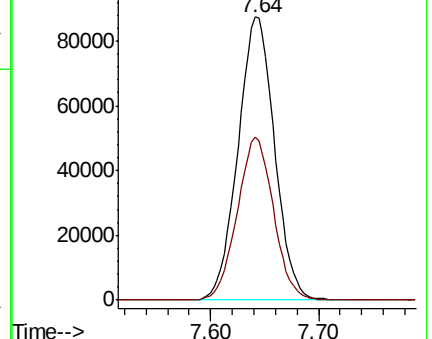

#33

1,2-Dichloroethane-d4

Concen: 45.848 ug/l

RT: 8.00 min Scan# 1937

Delta R.T. -0.00 min

Lab File: VN060876.D


Acq: 7 Apr 2020 14:56

Tgt Ion: 65 Resp: 129939

Ion Ratio Lower Upper



65 100


67 54.3 0.0 107.6

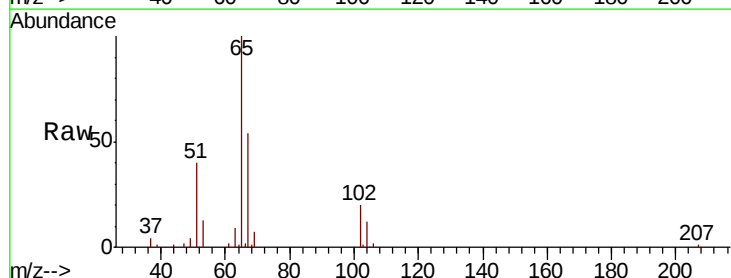

Abundance Ion 64.90 (64.60 to 65.60): VN

Ion 66.90 (66.60 to 67.60): VN

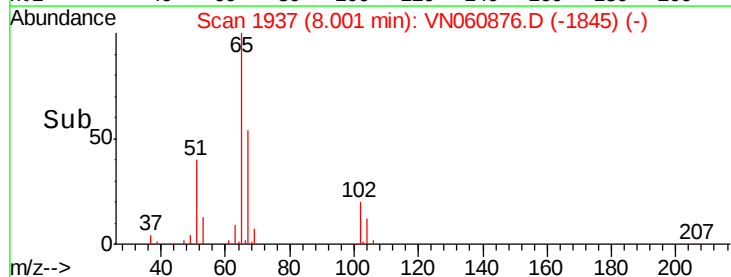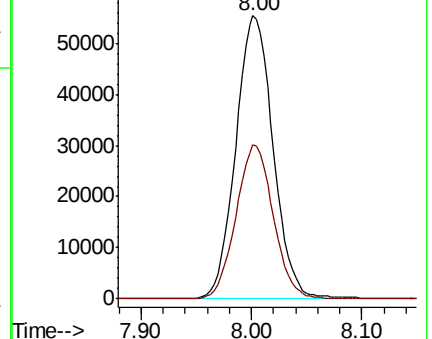

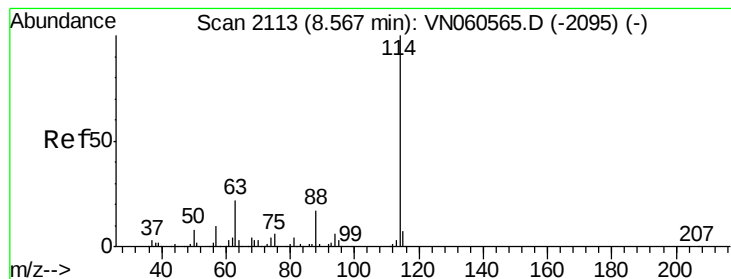

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.56 min Scan# 2112

Delta R.T. -0.00 min

Lab File: VN060876.D

Acq: 7 Apr 2020 14:56

Instrument :

MSVOA_N

ClientSampleId :

STORAGE-BLANK-SOIL-REF-6


Tot Ion:114 Resp: 339677

Ion Ratio Lower Upper

114 100

63 22.3 0.0 43.8




88 16.3 0.0 33.0

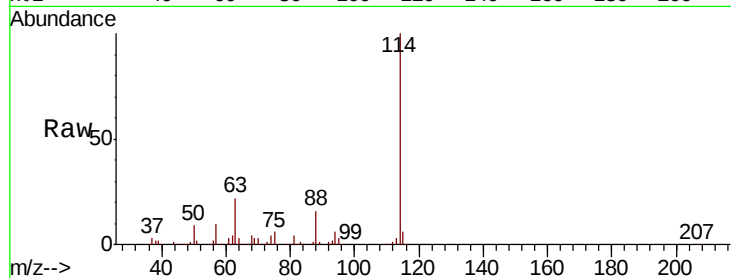

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VN

Ion 87.90 (87.60 to 88.60): VN

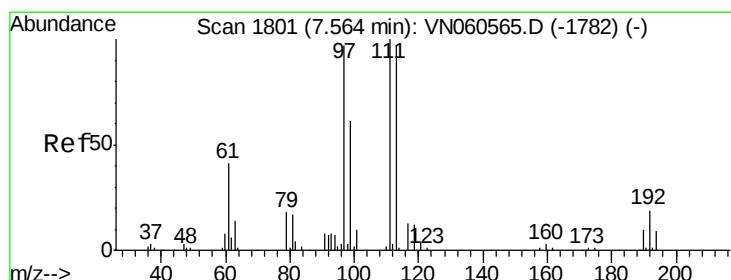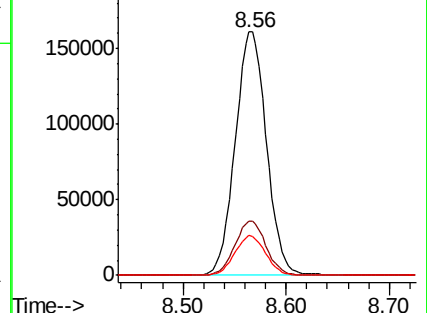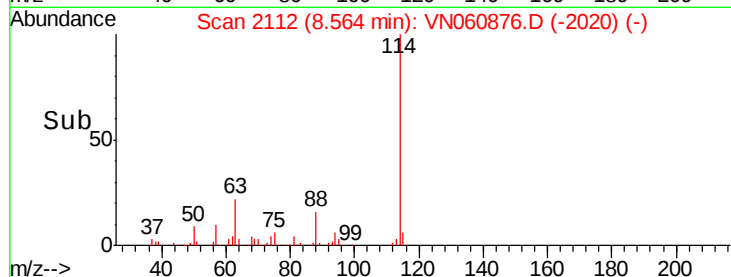

#35

Dibromofluoromethane

Concen: 48.452 ug/l

RT: 7.56 min Scan# 1801

Delta R.T. -0.00 min

Lab File: VN060876.D

Acq: 7 Apr 2020 14:56


Tgt Ion:113 Resp: 99517

Ion Ratio Lower Upper

113 100

111 103.6 82.9 124.3



192 21.0 15.8 23.8

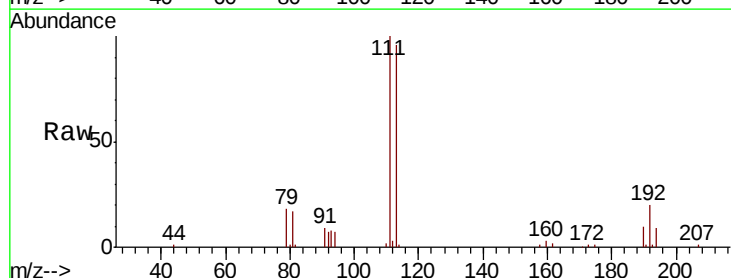


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

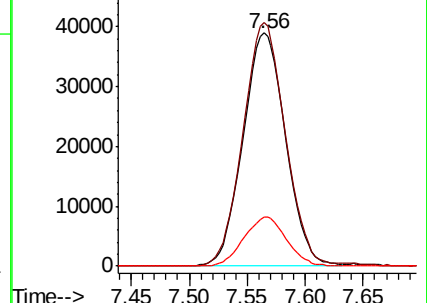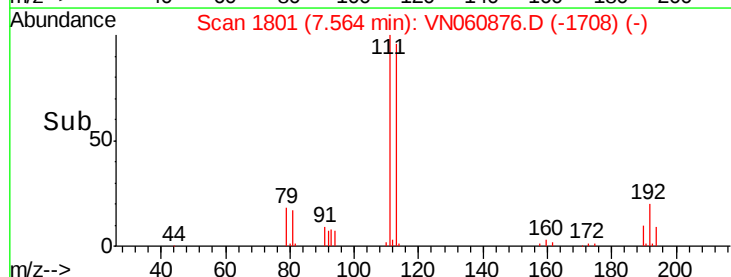

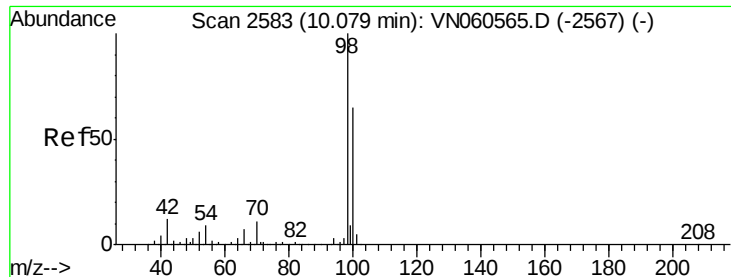

#50

Toluene-d8

Concen: 49.834 ug/l

RT: 10.08 min Scan# 2582

Delta R.T. -0.00 min

Lab File: VN060876.D

Acq: 7 Apr 2020 14:56

Instrument :

MSVOA_N

ClientSampleId :





STORAGE-BLANK-SOIL-REF-6

Tot Ion: 98 Resp: 418081

Ion Ratio Lower Upper

98 100

100 64.7 51.8 77.8

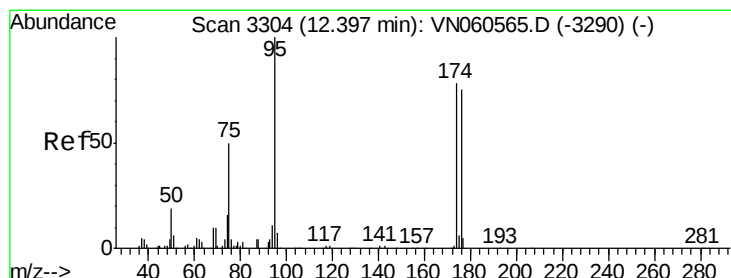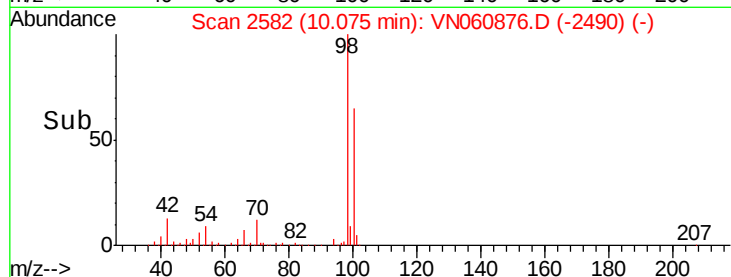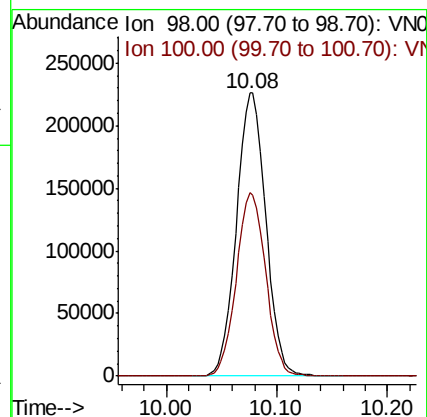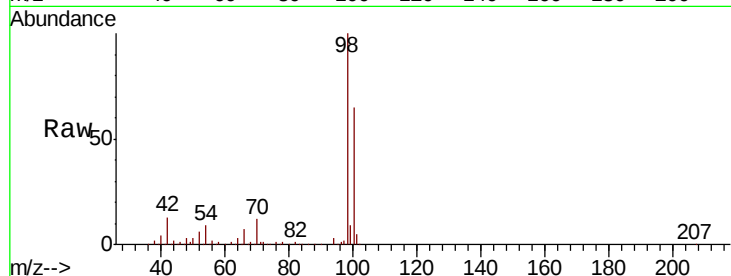

#62

4-Bromofluorobenzene

Concen: 49.336 ug/l

RT: 12.40 min Scan# 3304

Delta R.T. -0.00 min

Lab File: VN060876.D

Acq: 7 Apr 2020 14:56




Tgt Ion: 95 Resp: 151688


Ion Ratio Lower Upper

95 100

174 77.8 0.0 157.6

176 76.1 0.0 150.6


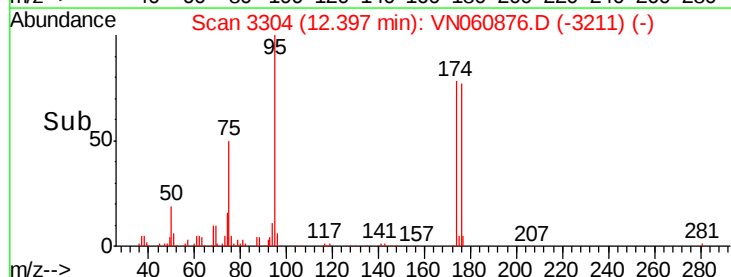
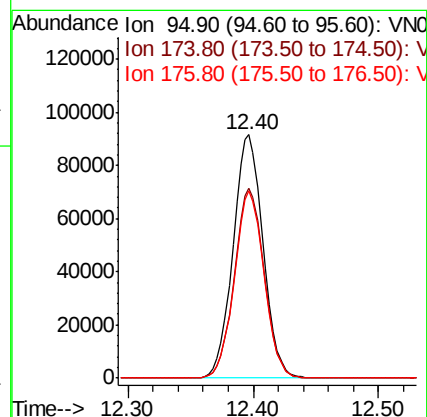
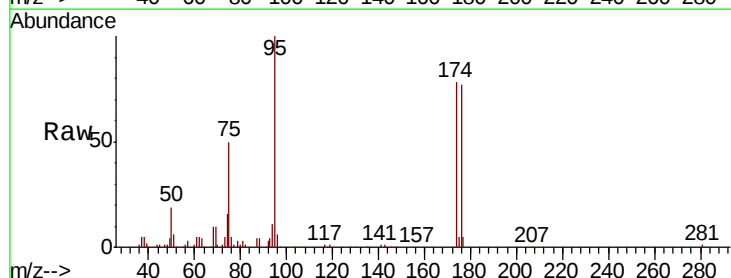


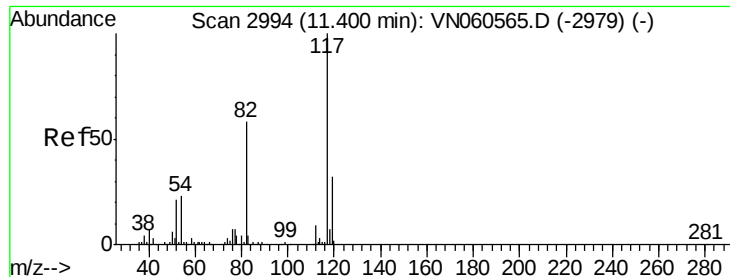

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.40 min Scan# 2994
Delta R.T. -0.00 min
Lab File: VN060876.D
Acq: 7 Apr 2020 14:56

Instrument :
MSVOA_N
ClientSampleId :
STORAGE-BLANK-SOIL-REF-6

Tot Ion:117 Resp: 311772
Ion Ratio Lower Upper
117 100
82 58.3 46.7 70.1
119 32.0 25.5 38.3

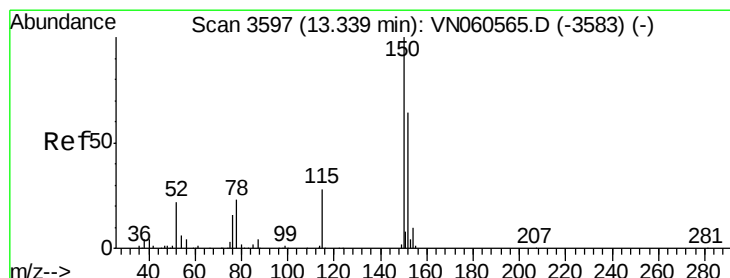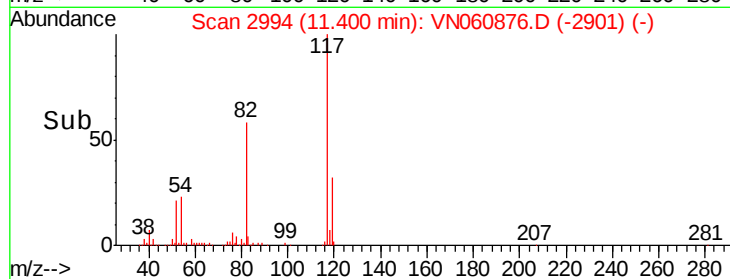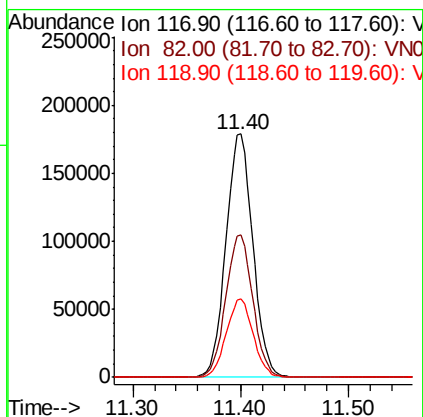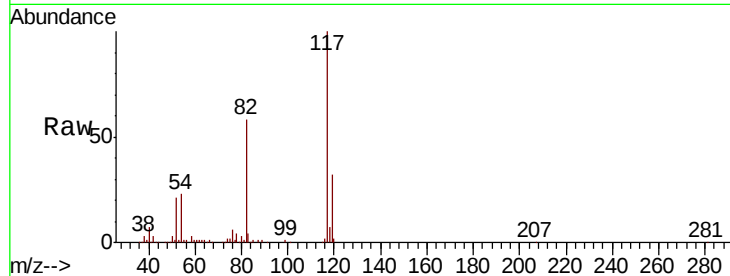

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.34 min Scan# 3597
Delta R.T. -0.00 min
Lab File: VN060876.D
Acq: 7 Apr 2020 14:56

Tgt Ion:152 Resp: 135623
Ion Ratio Lower Upper
152 100
115 59.2 30.2 90.6
150 157.1 0.0 350.2

