

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN040720\
 Data File : VN060880.D
 Acq On : 7 Apr 2020 16:26
 Operator : JC/MD
 Sample : L2166-06
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 TP-47-COMP

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N031820W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	7.564	1783	1801	1813	rBV2	128743	323003	20.44%	3.316%
2	7.641	1813	1825	1847	rVB	243673	577115	36.52%	5.924%
3	8.005	1921	1938	1961	rBV	151635	353097	22.35%	3.625%
4	8.140	1965	1980	1999	rVV	45726	97937	6.20%	1.005%
5	8.567	2096	2113	2140	rBV	378742	789523	49.96%	8.105%
6	9.165	2287	2299	2311	rBV2	18125	37549	2.38%	0.385%
7	9.249	2311	2325	2357	rVV	847281	1580156	100.00%	16.221%
8	9.889	2510	2524	2539	rBV	125280	215929	13.67%	2.217%
9	10.079	2568	2583	2606	rVB	609616	1119278	70.83%	11.490%
10	10.268	2631	2642	2659	rVB	37415	65983	4.18%	0.677%
11	10.532	2711	2724	2742	rBV	241285	403321	25.52%	4.140%
12	10.628	2742	2754	2765	rVV2	34079	57868	3.66%	0.594%
13	10.709	2765	2779	2784	rVV	60256	100247	6.34%	1.029%
14	10.754	2784	2793	2810	rVV	327471	540260	34.19%	5.546%
15	10.844	2812	2821	2836	rVB2	18803	32836	2.08%	0.337%
16	11.159	2904	2919	2937	rBV	490443	772704	48.90%	7.932%
17	11.400	2976	2994	3015	rVB	558496	977186	61.84%	10.031%
18	11.870	3128	3140	3153	rBV	50416	79746	5.05%	0.819%
19	12.397	3291	3304	3325	rBV	436726	733287	46.41%	7.528%
20	13.339	3584	3597	3614	rBV	537650	884358	55.97%	9.078%


Sum of corrected areas: 9741383

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN040720\
Data File : VN060880.D
Acq On : 7 Apr 2020 16:26
Operator : JC/MD
Sample : L2166-06
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TP-47-COMP

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N031820W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

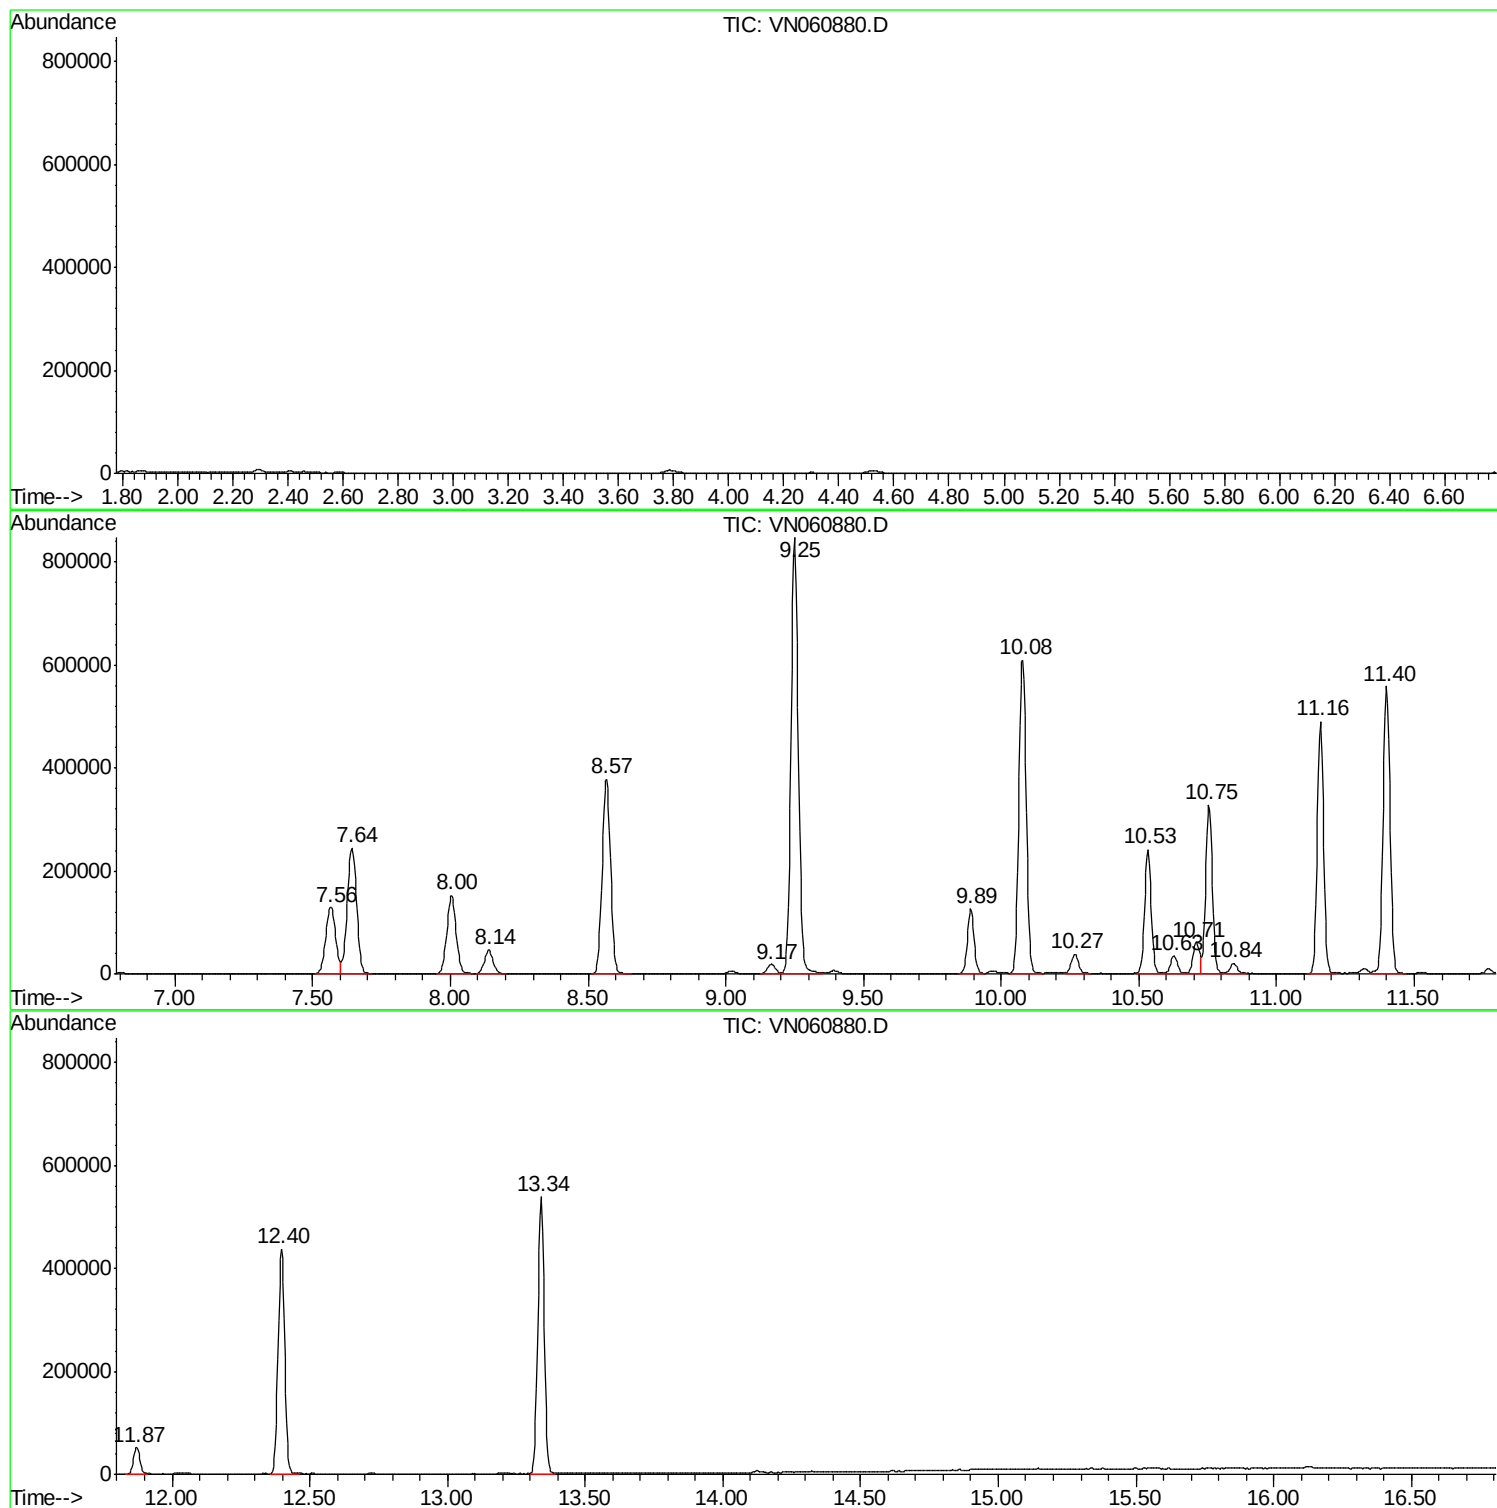

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN040720\
Data File : VN060880.D
Acq On : 7 Apr 2020 16:26
Operator : JC/MD
Sample : L2166-06
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TP-47-COMP

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N031820W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN040720\
Data File : VN060880.D
Acq On : 7 Apr 2020 16:26
Operator : JC/MD
Sample : L2166-06
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TP-47-COMP

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N031820W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc