

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN040720\
 Data File : VN060882.D
 Acq On : 7 Apr 2020 17:12
 Operator : JC/MD
 Sample : L2166-20
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 TP-45-COMP

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N031820W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	7.564	1783	1801	1813	rBV	125795	312873	18.30%	3.168%
2	7.641	1813	1825	1853	rVB	236548	554979	32.45%	5.620%
3	8.005	1921	1938	1960	rBV	146742	342155	20.01%	3.465%
4	8.140	1965	1980	1998	rVB	47528	101716	5.95%	1.030%
5	8.567	2093	2113	2136	rBV	362075	758190	44.34%	7.678%
6	9.165	2286	2299	2310	rBV	20113	39511	2.31%	0.400%
7	9.249	2310	2325	2360	rVV	911036	1709999	100.00%	17.317%
8	9.889	2509	2524	2540	rBV	130967	226734	13.26%	2.296%
9	10.075	2568	2582	2605	rBV	584021	1076768	62.97%	10.904%
10	10.268	2631	2642	2654	rVB	41036	70204	4.11%	0.711%
11	10.532	2707	2724	2739	rBV	246534	414910	24.26%	4.202%
12	10.625	2743	2753	2767	rVV2	37926	64825	3.79%	0.656%
13	10.709	2767	2779	2784	rVV	62518	105053	6.14%	1.064%
14	10.754	2784	2793	2811	rVV	372908	614269	35.92%	6.221%
15	10.844	2811	2821	2836	rVB2	21097	37572	2.20%	0.380%
16	11.159	2906	2919	2941	rBV	521972	827652	48.40%	8.381%
17	11.400	2979	2994	3010	rVB	534437	934172	54.63%	9.460%
18	11.770	3098	3109	3124	rBV	11418	17998	1.05%	0.182%
19	11.869	3127	3140	3153	rBV2	63020	100641	5.89%	1.019%
20	12.397	3291	3304	3323	rBV	423441	705695	41.27%	7.146%
21	13.339	3584	3597	3612	rBV	522951	858915	50.23%	8.698%


Sum of corrected areas: 9874831

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN040720\
Data File : VN060882.D
Acq On : 7 Apr 2020 17:12
Operator : JC/MD
Sample : L2166-20
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TP-45-COMP

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N031820W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

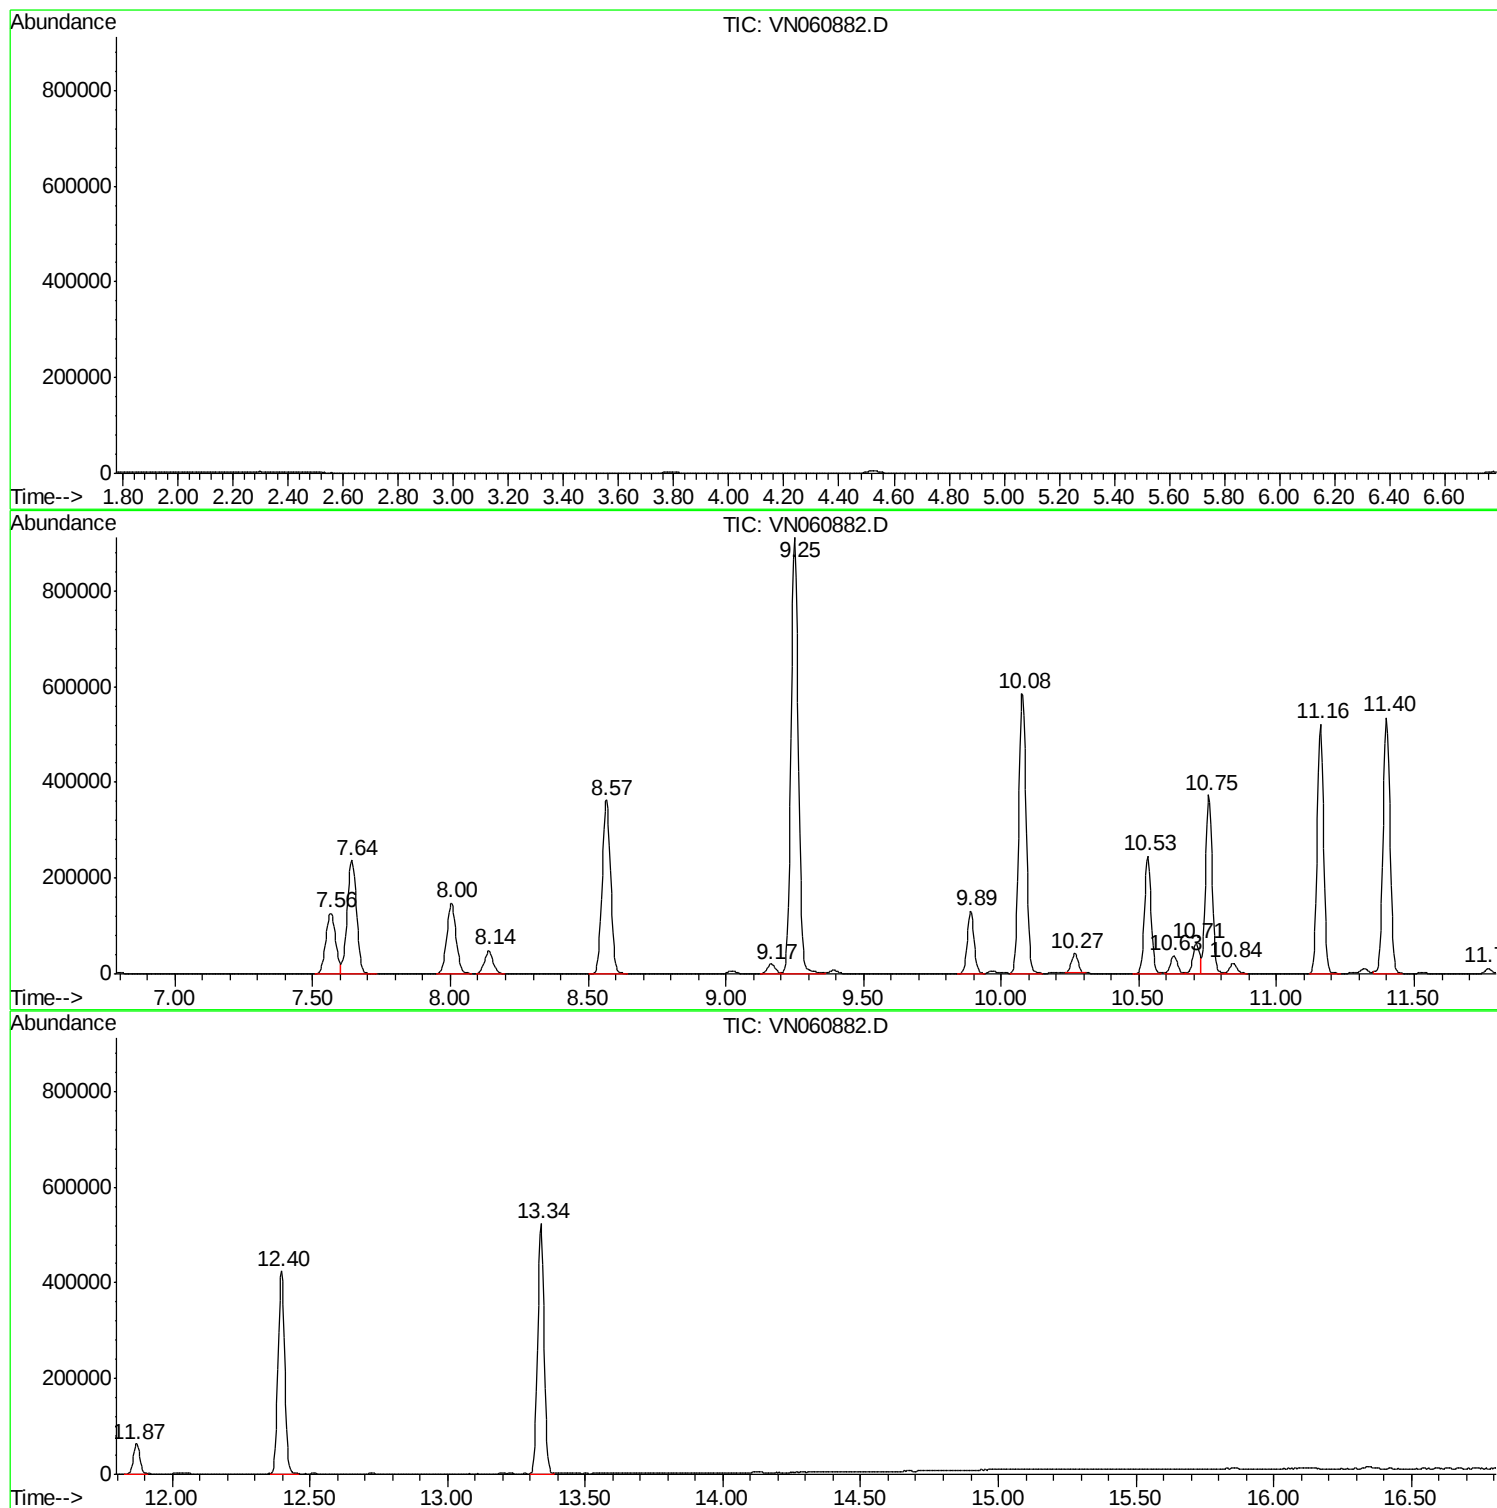

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN040720\
Data File : VN060882.D
Acq On : 7 Apr 2020 17:12
Operator : JC/MD
Sample : L2166-20
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TP-45-COMP

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N031820W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN040720\
Data File : VN060882.D
Acq On : 7 Apr 2020 17:12
Operator : JC/MD
Sample : L2166-20
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TP-45-COMP

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N031820W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc