


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN040721\
Data File : VN066506.D
Acq On : 7 Apr 2021 12:37
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N040621W.M
Title : SW846 8260
Last Update : Tue Apr 06 15:38:34 2021

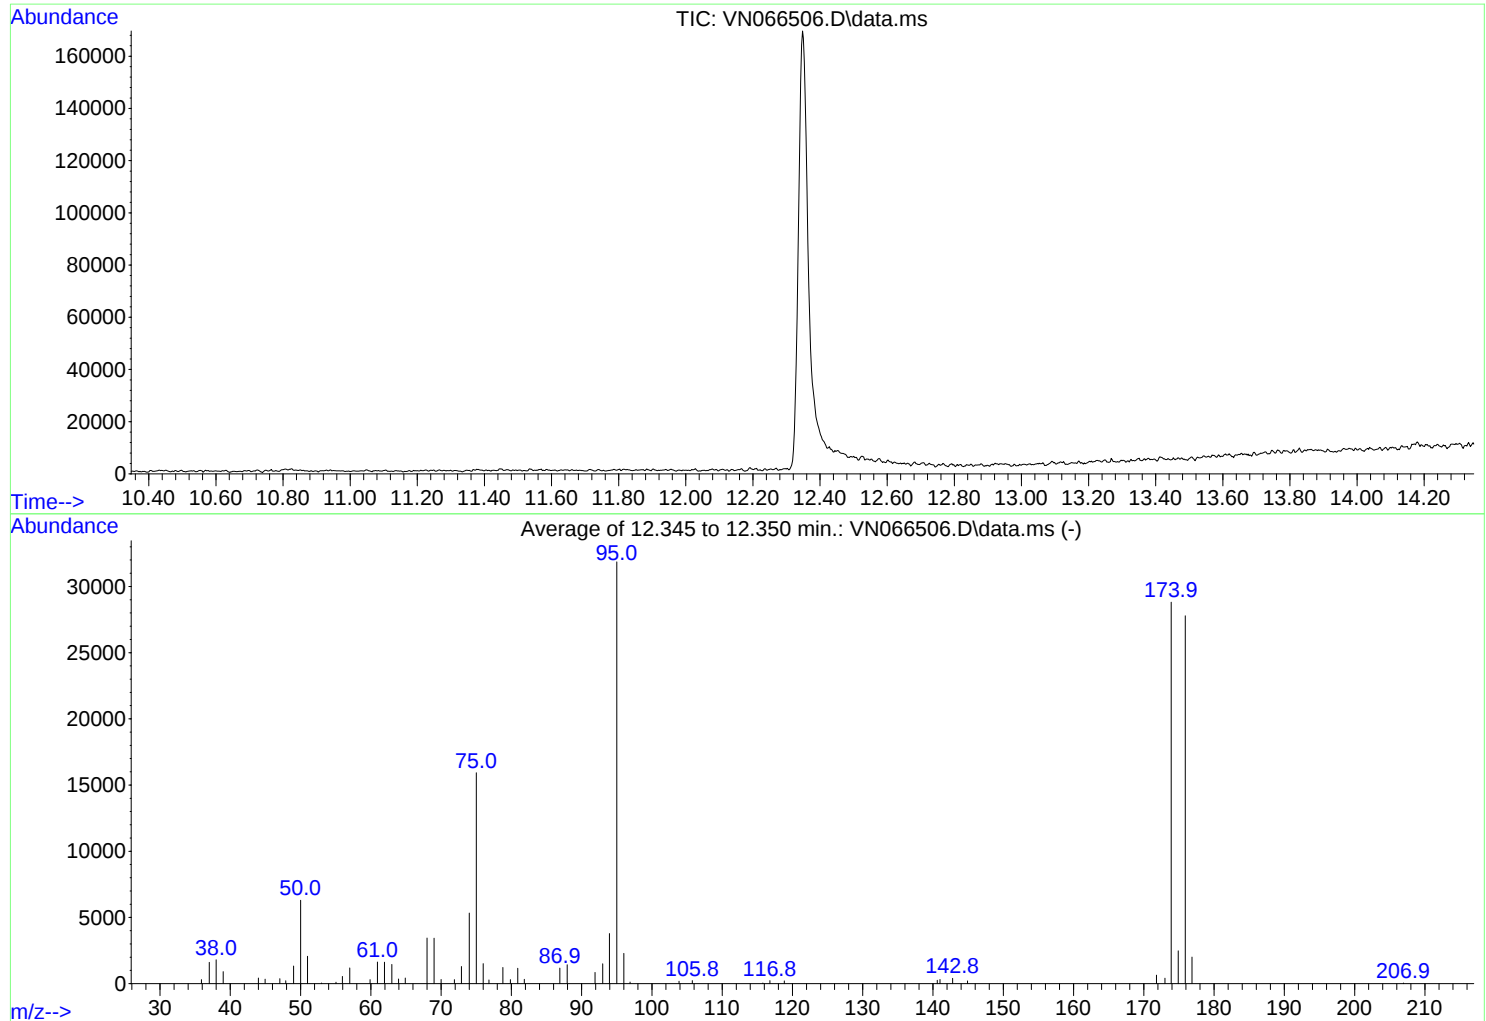

AutoFind: Scans 3973, 3974, 3975; Background Corrected with Scan 3958

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	6303	PASS
75	95	30	60	50.0	15934	PASS
95	95	100	100	100.0	31861	PASS
96	95	5	9	7.2	2282	PASS
173	174	0.00	2	1.4	414	PASS
174	95	50	100	90.4	28811	PASS
175	174	5	9	8.6	2482	PASS
176	174	95	101	96.4	27784	PASS
177	176	5	9	7.2	2013	PASS