

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN040722\  
 Data File : VN071896.D  
 Acq On : 07 Apr 2022 11:38  
 Operator : JC\MD  
 Sample : VN0407MBL01  
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA\_N/MEOH  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 VN0407MBL01

Quant Time: Apr 08 01:12:07 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N033022W.M  
 Quant Title : SW846 8260  
 QLast Update : Thu Mar 31 01:57:54 2022  
 Response via : Initial Calibration


| Compound                      | R.T.           | QIon | Response   | Conc      | Units  | Dev(Min) |
|-------------------------------|----------------|------|------------|-----------|--------|----------|
| -----                         |                |      |            |           |        |          |
| Internal Standards            |                |      |            |           |        |          |
| 1) Pentafluorobenzene         | 8.080          | 168  | 513164     | 50.000    | ug/l   | 0.00     |
| 34) 1,4-Difluorobenzene       | 8.963          | 114  | 876076     | 50.000    | ug/l   | 0.00     |
| 63) Chlorobenzene-d5          | 11.739         | 117  | 888208     | 50.000    | ug/l   | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 13.674         | 152  | 310362     | 50.000    | ug/l   | 0.00     |
|                               |                |      |            |           |        |          |
| System Monitoring Compounds   |                |      |            |           |        |          |
| 33) 1,2-Dichloroethane-d4     | 8.433          | 65   | 283552     | 48.401    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 61 - 141 |      | Recovery = | 96.800%   |        |          |
| 35) Dibromofluoromethane      | 8.022          | 113  | 254928     | 49.451    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 69 - 133 |      | Recovery = | 98.900%   |        |          |
| 50) Toluene-d8                | 10.439         | 98   | 1089478    | 51.662    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 65 - 126 |      | Recovery = | 103.320%  |        |          |
| 62) 4-Bromofluorobenzene      | 12.727         | 95   | 350093     | 51.330    | ug/l   | 0.00     |
| Spiked Amount 50.000          | Range 58 - 135 |      | Recovery = | 102.660%  |        |          |
|                               |                |      |            |           |        |          |
| Target Compounds              |                |      |            |           |        | Qvalue   |
| 3) Chloromethane              | 2.298          | 50   | 1551       | 0.300     | ug/l   | 92       |
| 5) Bromomethane               | 2.875          | 94   | 1790       | 0.485     | ug/l   | 85       |
| 10) Methyl Iodide             | 4.445          | 142  | 1742       | 0.280     | ug/l # | 71       |
| 15) Acrylonitrile             | 5.557          | 53   | 1125       | 0.407     | ug/l # | 75       |
| 16) Acetone                   | 4.292          | 43   | 2418       | 0.966     | ug/l   | 94       |
| 18) Methyl Acetate            | 4.857          | 43   | 5223       | Below Cal |        | 98       |
| 25) 2-Butanone                | 7.339          | 43   | 1381       | 0.383     | ug/l   | 94       |
| 29) Tetrahydrofuran           | 7.698          | 42   | 1031       | 0.441     | ug/l # | 56       |
| 31) Cyclohexane               | 8.080          | 56   | 8127       | 1.020     | ug/l # | 1        |
| 36) 1,1-Dichloropropene       | 8.080          | 75   | 34282      | 4.762     | ug/l # | 49       |
| 38) Carbon Tetrachloride      | 8.080          | 117  | 46421      | 6.579     | ug/l # | 18       |
| 43) Isopropyl Acetate         | 8.669          | 43   | 34326      | 2.619     | ug/l # | 53       |
| 49) 1,4-Dioxane               | 9.574          | 88   | 57         | Below Cal | #      | 1        |
| 51) 4-Methyl-2-Pentanone      | 10.333         | 43   | 3175       | 0.421     | ug/l # | 84       |
| 59) 2-Hexanone                | 11.086         | 43   | 6216       | 1.172     | ug/l   | 99       |
| 74) N-amyl acetate            | 12.386         | 43   | 3349       | 0.447     | ug/l   | 94       |
| 76) 1,2,3-Trichloropropane    | 12.727         | 75   | 167697     | 23.324    | ug/l # | 1        |
| 81) trans-1,4-Dichloro-2-b... | 12.727         | 75   | 167697     | 72.281    | ug/l # | 10       |
| 87) 1,3-Dichlorobenzene       | 13.615         | 146  | 2216       | 0.212     | ug/l   | 95       |
| 88) 1,4-Dichlorobenzene       | 13.615         | 146  | 2216       | 0.217     | ug/l   | 97       |
| 89) n-Butylbenzene            | 13.939         | 91   | 4371       | 0.301     | ug/l   | 96       |
| 91) 1,2-Dichlorobenzene       | 13.986         | 146  | 2598       | 0.253     | ug/l   | 99       |
| 92) 1,2-Dibromo-3-Chloropr... | 14.598         | 75   | 461        | 0.341     | ug/l   | 83       |
| 93) 1,2,4-Trichlorobenzene    | 15.262         | 180  | 3693       | 2.802     | ug/l   | 94       |
| 94) Hexachlorobutadiene       | 15.368         | 225  | 754        | 0.249     | ug/l   | 64       |
| 95) Naphthalene               | 15.504         | 128  | 12581      | 4.625     | ug/l   | 98       |
| 96) 1,2,3-Trichlorobenzene    | 15.698         | 180  | 4236       | 3.257     | ug/l   | 96       |
| -----                         |                |      |            |           |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN040722\  
Data File : VN071896.D  
Acq On : 07 Apr 2022 11:38  
Operator : JC\MD  
Sample : VN0407MBL01  
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA\_N/MEOH  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
VN0407MBL01

Quant Time: Apr 08 01:12:07 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N033022W.M  
Quant Title : SW846 8260  
QLast Update : Thu Mar 31 01:57:54 2022  
Response via : Initial Calibration



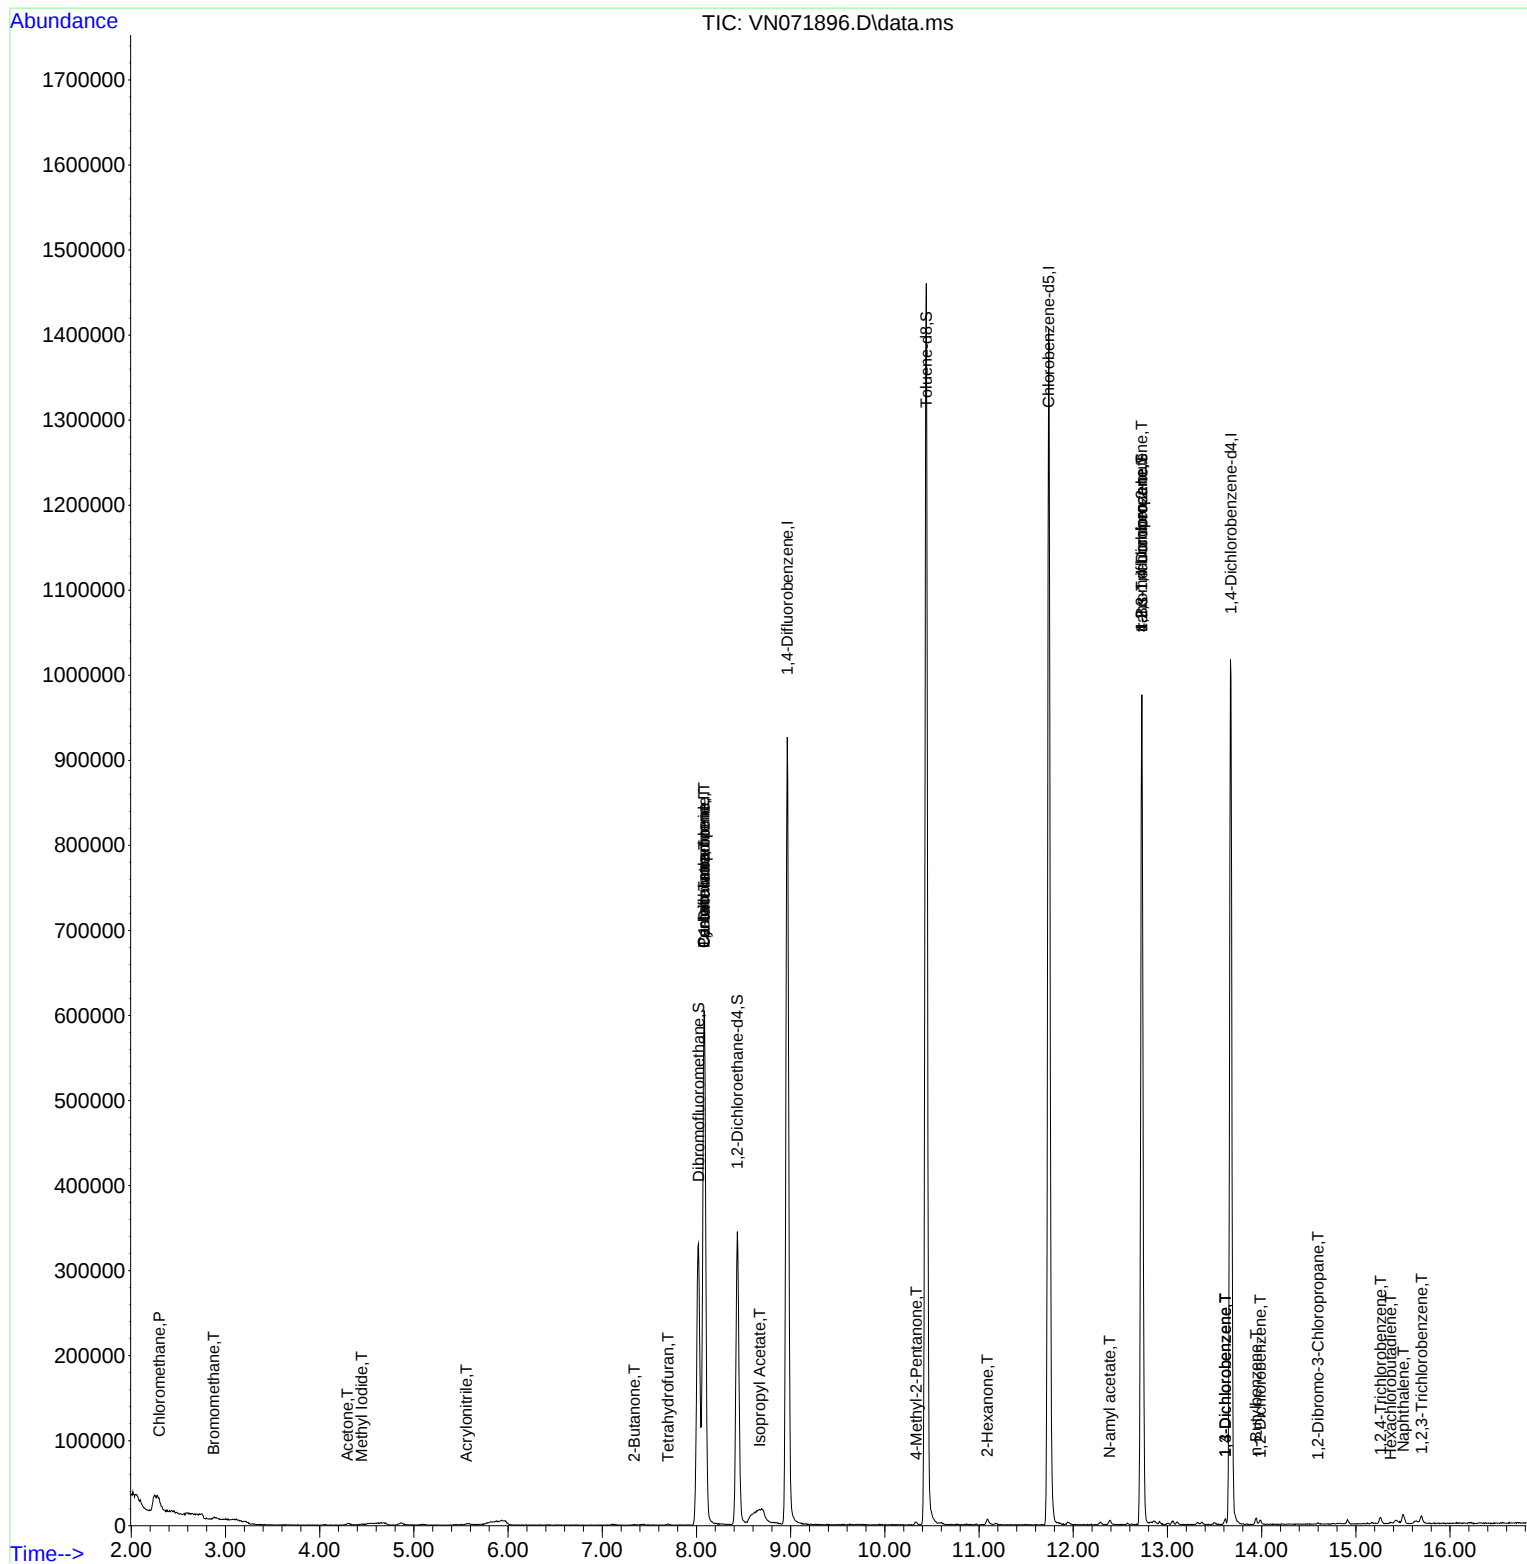




#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 8.080 min Scan# 1  
Delta R.T. -0.001 min  
Lab File: VN071896.D  
Acq: 07 Apr 2022 11:38




Instrument :  
MSVOA\_N  
ClientSampleId :  
VN0407MBL01


Tgt Ion:168 Resp: 513164  
Ion Ratio Lower Upper  
168 100  
99 53.3 42.3 63.5

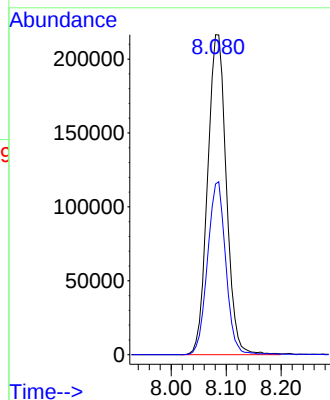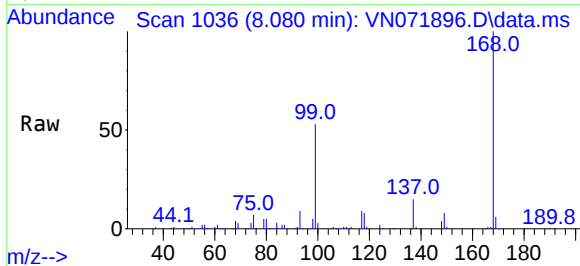

#3  
Chloromethane  
Concen: 0.300 ug/l  
RT: 2.298 min Scan# 53  
Delta R.T. -0.001 min  
Lab File: VN071896.D  
Acq: 07 Apr 2022 11:38

Tgt Ion: 50 Resp: 1551  
Ion Ratio Lower Upper  
50 100  
52 36.6 25.7 38.5


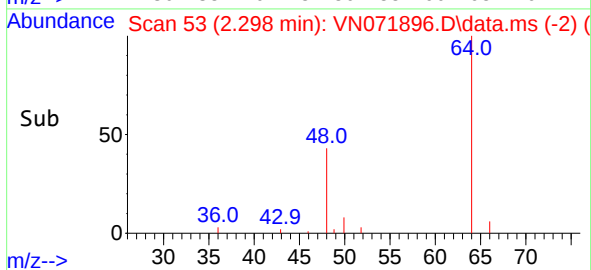
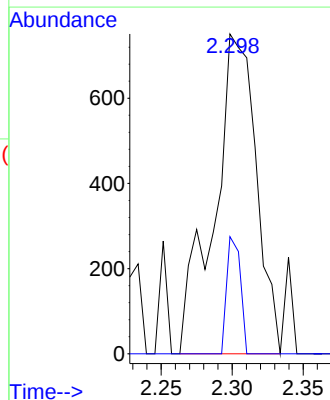
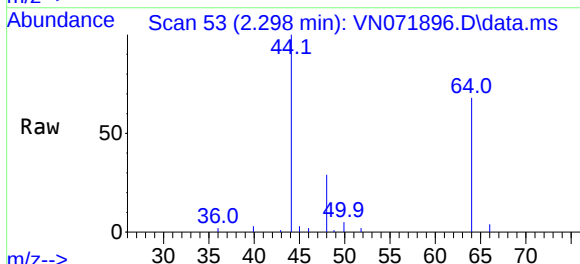




#5  
Bromomethane  
Concen: 0.485 ug/l  
RT: 2.875 min Scan# 11  
Delta R.T. 0.029 min  
Lab File: VN071896.D  
Acq: 07 Apr 2022 11:38




Instrument :  
MSVOA\_N  
ClientSampleId :  
VN0407MBL01


Tgt Ion: 94 Resp: 1790  
Ion Ratio Lower Upper  
94 100  
96 80.3 76.0 114.0

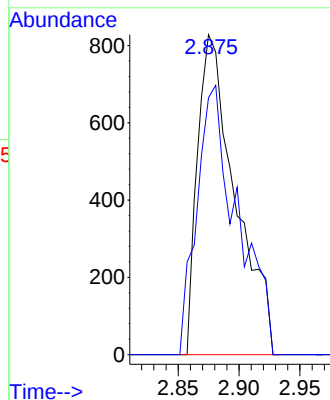

#10  
Methyl Iodide  
Concen: 0.280 ug/l  
RT: 4.445 min Scan# 418  
Delta R.T. 0.023 min  
Lab File: VN071896.D  
Acq: 07 Apr 2022 11:38

Tgt Ion: 142 Resp: 1742  
Ion Ratio Lower Upper  
142 100  
127 23.0 31.3 46.9#  
141 0.0 11.2 16.8#


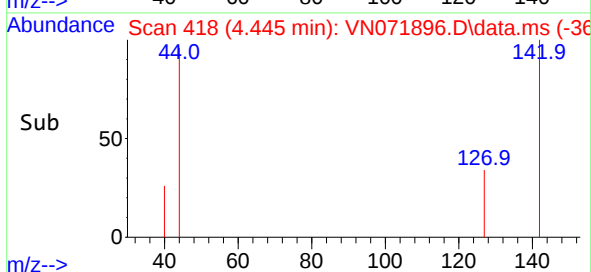
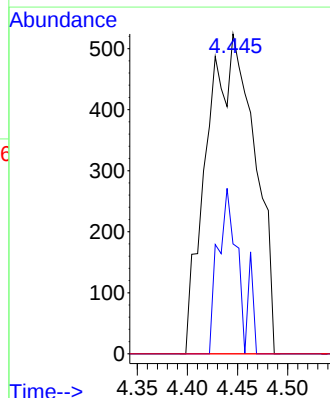





#15  
Acrylonitrile  
Concen: 0.407 ug/l  
RT: 5.557 min Scan# 605  
Delta R.T. 0.011 min  
Lab File: VN071896.D  
Acq: 07 Apr 2022 11:38




Instrument :  
MSVOA\_N  
ClientSampleId :  
VN0407MBL01


Tgt Ion: 53 Resp: 1125  
Ion Ratio Lower Upper  
53 100  
52 67.7 66.4 99.6  
51 10.1 28.5 42.7#



#16  
Acetone  
Concen: 0.966 ug/l  
RT: 4.292 min Scan# 392  
Delta R.T. 0.017 min  
Lab File: VN071896.D  
Acq: 07 Apr 2022 11:38

Tgt Ion: 43 Resp: 2418  
Ion Ratio Lower Upper  
43 100  
58 29.1 26.0 39.0


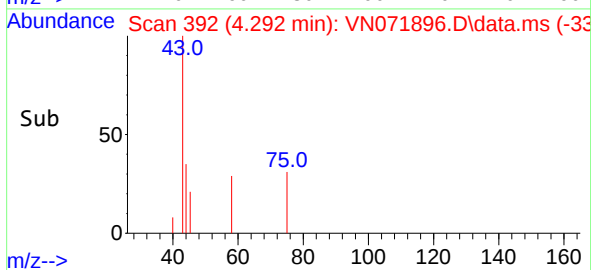






#18  
Methyl Acetate  
Concen: Below Cal  
RT: 4.857 min Scan# 41  
Delta R.T. 0.011 min  
Lab File: VN071896.D  
Acq: 07 Apr 2022 11:38




Instrument :  
MSVOA\_N  
ClientSampleId :  
VN0407MBL01


Tgt Ion: 43 Resp: 5223  
Ion Ratio Lower Upper  
43 100  
74 28.0 21.6 32.4



#25  
2-Butanone  
Concen: 0.383 ug/l  
RT: 7.339 min Scan# 910  
Delta R.T. 0.011 min  
Lab File: VN071896.D  
Acq: 07 Apr 2022 11:38

Tgt Ion: 43 Resp: 1381  
Ion Ratio Lower Upper  
43 100  
72 32.9 23.7 35.5

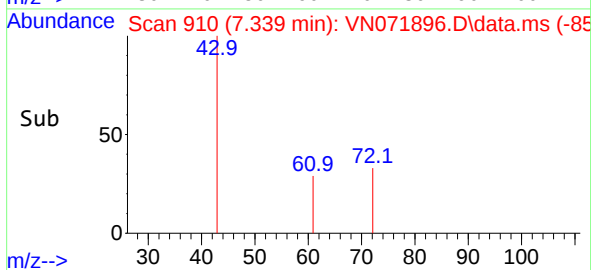



#29

Tetrahydrofuran

Concen: 0.441 ug/l

RT: 7.698 min Scan# 91

Delta R.T. 0.023 min

Lab File: VN071896.D

Acq: 07 Apr 2022 11:38

Instrument :

MSVOA\_N

ClientSampleId :

VN0407MBL01





Tgt Ion: 42 Resp: 1031

Ion Ratio Lower Upper

42 100

72 23.8 39.7 59.5#

71 12.6 36.6 55.0#

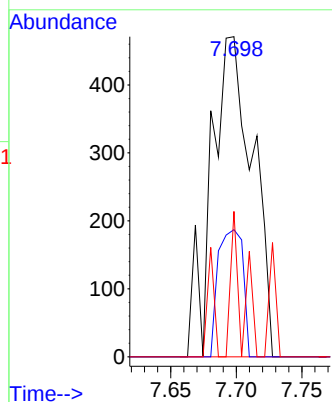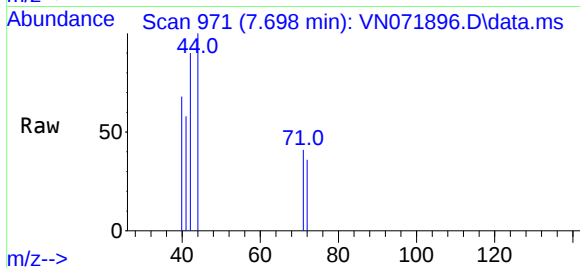

#31

Cyclohexane

Concen: 1.020 ug/l

RT: 8.080 min Scan# 1036

Delta R.T. -0.012 min

Lab File: VN071896.D

Acq: 07 Apr 2022 11:38




Tgt Ion: 56 Resp: 8127


Ion Ratio Lower Upper

56 100

69 185.8 27.8 41.8#

84 158.7 76.9 115.3#


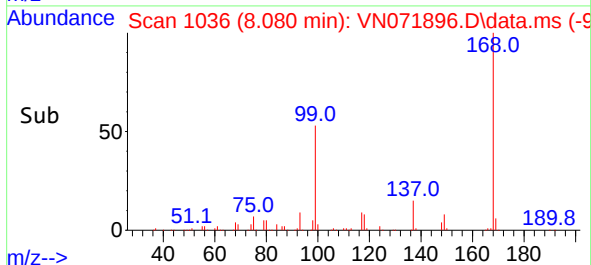

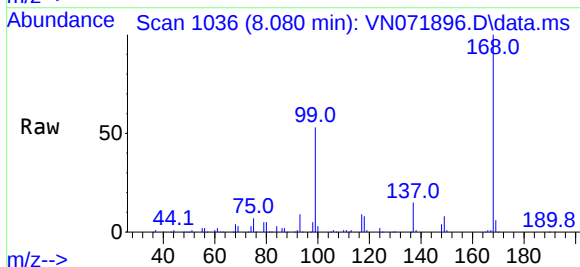


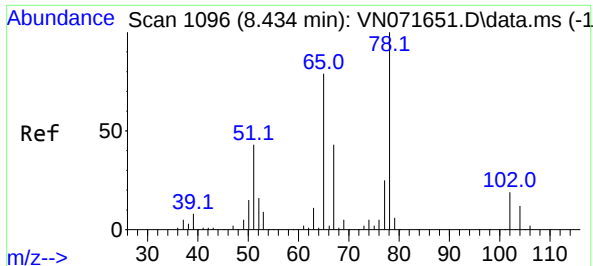

#33  
1,2-Dichloroethane-d4  
Concen: 48.401 ug/l  
RT: 8.433 min Scan# 1096  
Delta R.T. -0.001 min  
Lab File: VN071896.D  
Acq: 07 Apr 2022 11:38




Instrument :  
MSVOA\_N  
ClientSampleId :  
VN0407MBL01


Tgt Ion: 65 Resp: 283552  
Ion Ratio Lower Upper  
65 100  
67 53.1 0.0 104.8

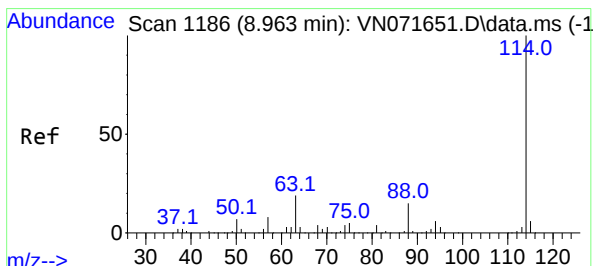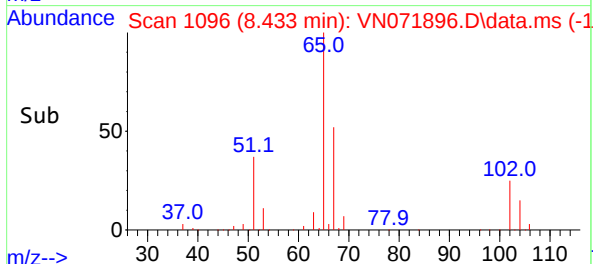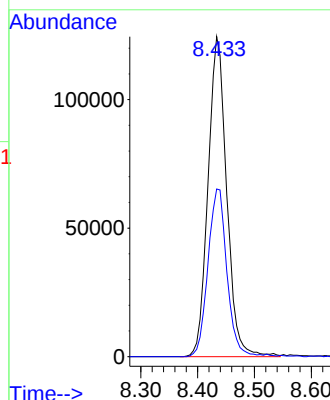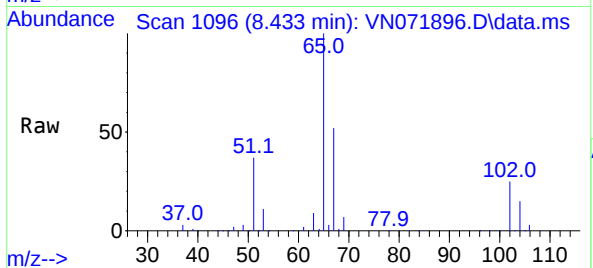

#34  
1,4-Difluorobenzene  
Concen: 50.000 ug/l  
RT: 8.963 min Scan# 1186  
Delta R.T. -0.000 min  
Lab File: VN071896.D  
Acq: 07 Apr 2022 11:38

Tgt Ion:114 Resp: 876076  
Ion Ratio Lower Upper  
114 100  
63 18.9 0.0 40.0  
88 15.9 0.0 32.6


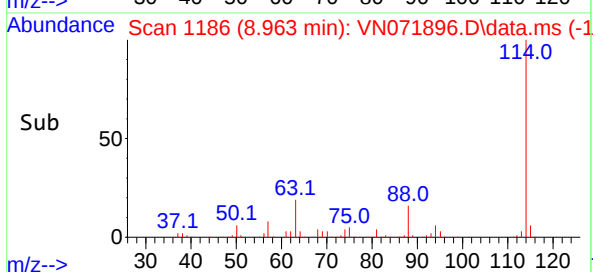
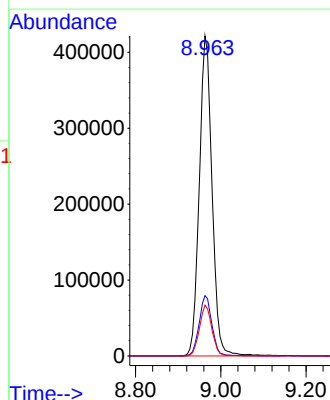
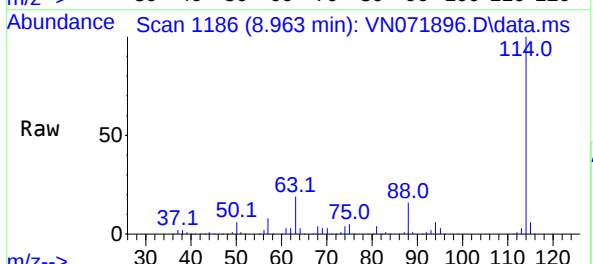


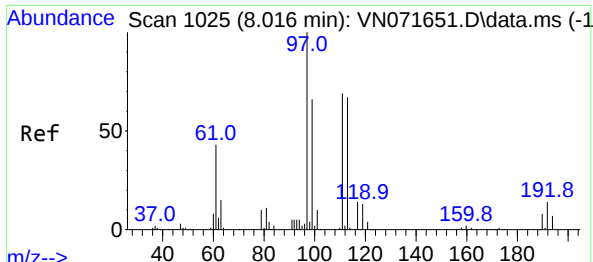

#35  
Dibromofluoromethane  
Concen: 49.451 ug/l  
RT: 8.022 min Scan# 1026  
Delta R.T. 0.006 min  
Lab File: VN071896.D  
Acq: 07 Apr 2022 11:38




Instrument :  
MSVOA\_N  
ClientSampleId :  
VN0407MBL01


Tgt Ion:113 Resp: 254928  
Ion Ratio Lower Upper  
113 100  
111 102.4 81.4 122.0  
192 21.9 17.0 25.6

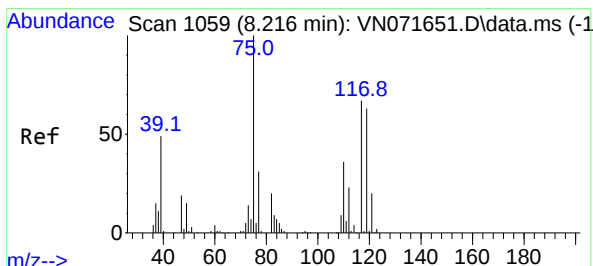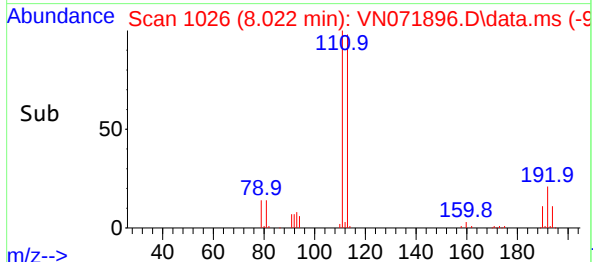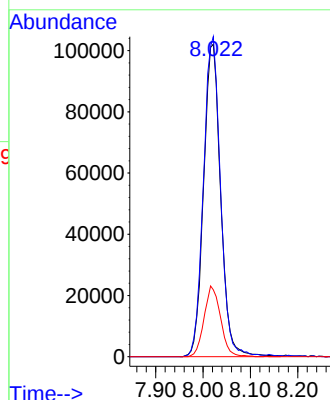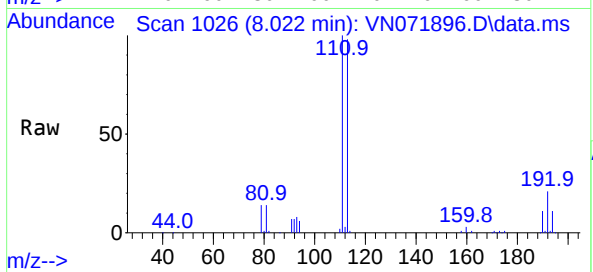

#36  
1,1-Dichloropropene  
Concen: 4.762 ug/l  
RT: 8.080 min Scan# 1036  
Delta R.T. -0.136 min  
Lab File: VN071896.D  
Acq: 07 Apr 2022 11:38

Tgt Ion: 75 Resp: 34282  
Ion Ratio Lower Upper  
75 100  
110 8.8 18.3 54.8#  
77 0.0 25.1 37.7#


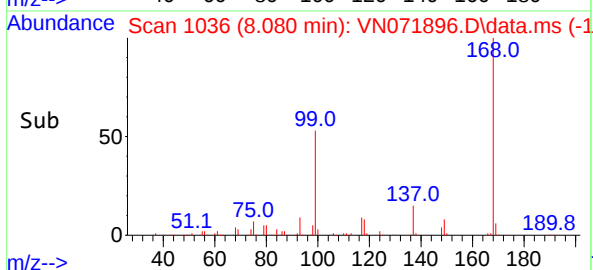
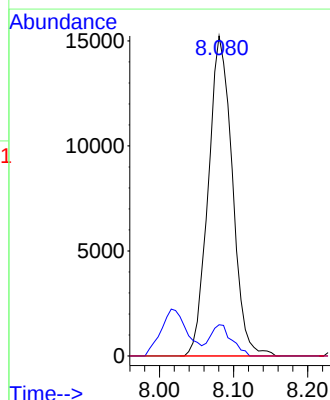
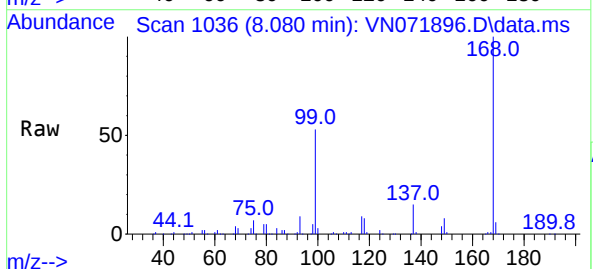


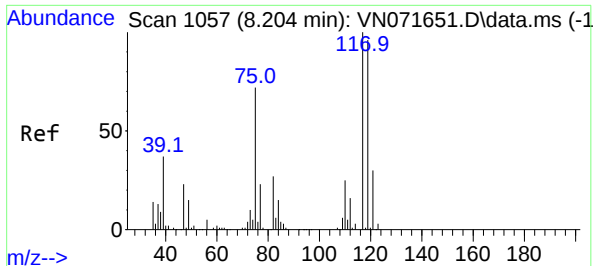

#38  
Carbon Tetrachloride  
Concen: 6.579 ug/l  
RT: 8.080 min Scan# 11036  
Delta R.T. -0.124 min  
Lab File: VN071896.D  
Acq: 07 Apr 2022 11:38




Instrument :  
MSVOA\_N  
ClientSampleId :  
VN0407MBL01


Tgt Ion:117 Resp: 46421  
Ion Ratio Lower Upper  
117 100  
119 7.0 75.8 113.8#  
121 0.0 24.6 37.0#

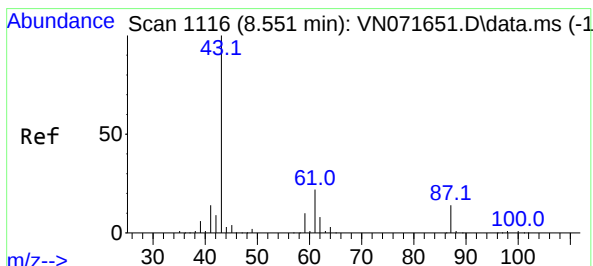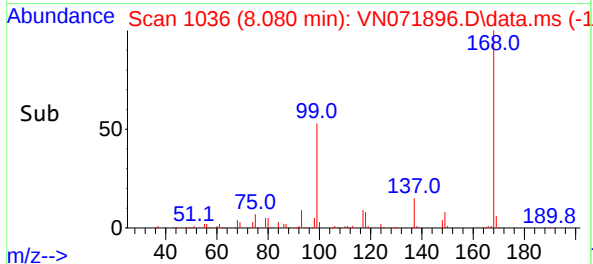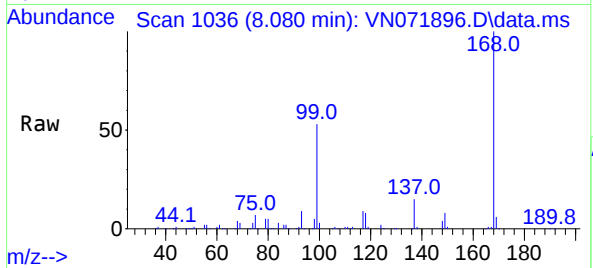

#43  
Isopropyl Acetate  
Concen: 2.619 ug/l  
RT: 8.669 min Scan# 1136  
Delta R.T. 0.118 min  
Lab File: VN071896.D  
Acq: 07 Apr 2022 11:38

Tgt Ion: 43 Resp: 34326  
Ion Ratio Lower Upper  
43 100  
61 0.0 21.9 32.9#  
87 0.0 12.0 18.0#


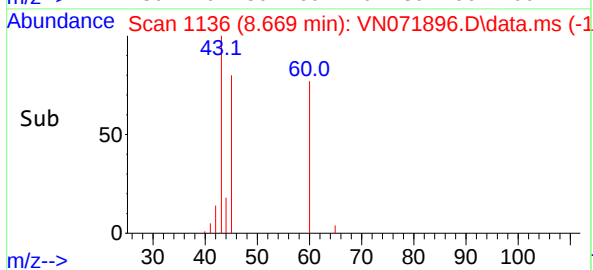

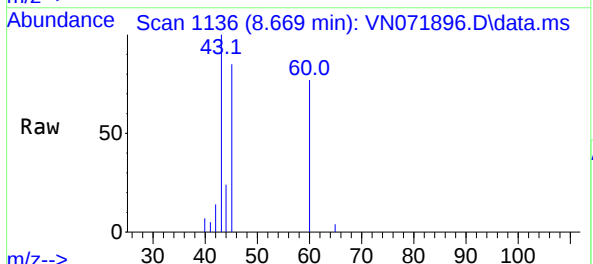


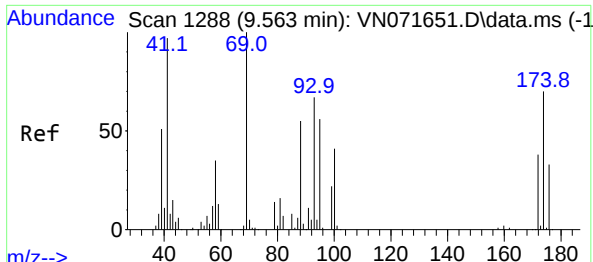

#49  
1,4-Dioxane  
Concen: Below Cal  
RT: 9.574 min Scan# 11  
Delta R.T. 0.011 min  
Lab File: VN071896.D  
Acq: 07 Apr 2022 11:38




Instrument :  
MSVOA\_N  
ClientSampleId :  
VN0407MBL01


Tgt Ion: 88 Resp: 57  
Ion Ratio Lower Upper  
88 100  
43 910.5 20.2 30.4#  
58 0.0 54.2 81.4#

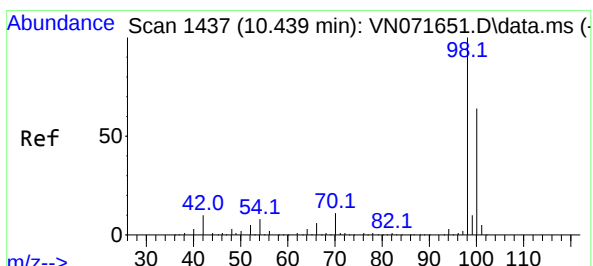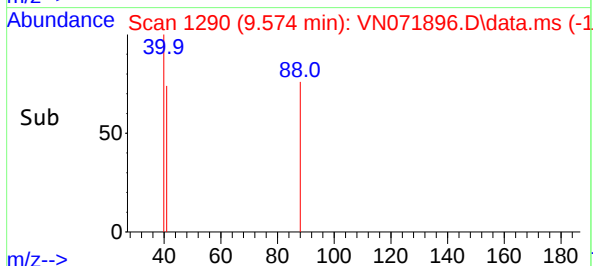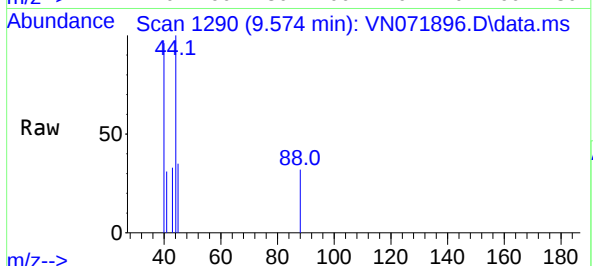

#50  
Toluene-d8  
Concen: 51.662 ug/l  
RT: 10.439 min Scan# 1437  
Delta R.T. 0.000 min  
Lab File: VN071896.D  
Acq: 07 Apr 2022 11:38

Tgt Ion: 98 Resp: 1089478  
Ion Ratio Lower Upper  
98 100  
100 64.7 52.6 78.8


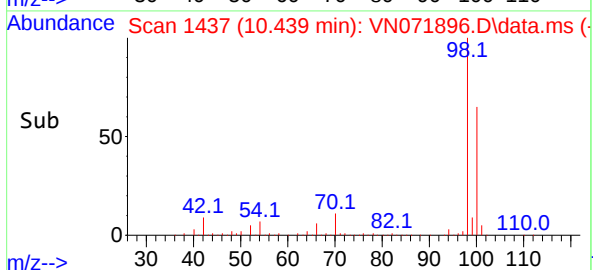

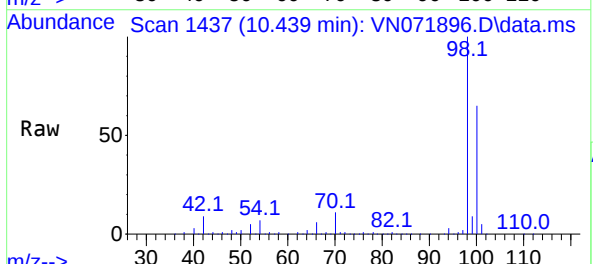




#51  
4-Methyl-2-Pentanone  
Concen: 0.421 ug/l  
RT: 10.333 min Scan# 1419  
Delta R.T. 0.011 min  
Lab File: VN071896.D  
Acq: 07 Apr 2022 11:38




Instrument :  
MSVOA\_N  
ClientSampleId :  
VN0407MBL01


Tgt Ion: 43 Resp: 3175  
Ion Ratio Lower Upper  
43 100  
58 32.7 34.1 51.1#

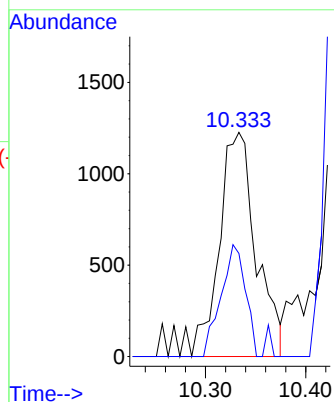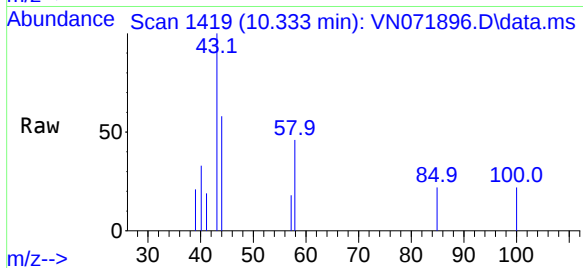

#59  
2-Hexanone  
Concen: 1.172 ug/l  
RT: 11.086 min Scan# 1547  
Delta R.T. 0.005 min  
Lab File: VN071896.D  
Acq: 07 Apr 2022 11:38

Tgt Ion: 43 Resp: 6216  
Ion Ratio Lower Upper  
43 100  
58 60.2 29.7 89.1


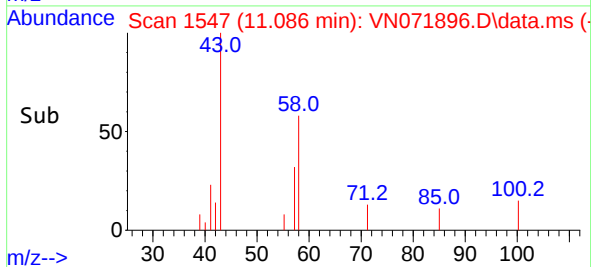
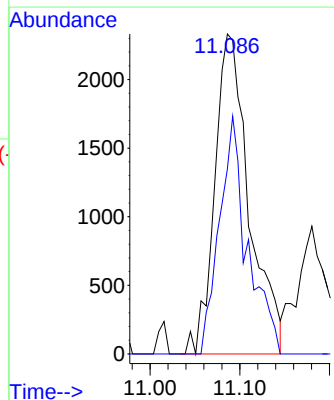
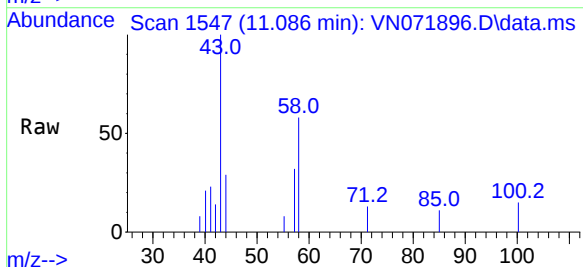




#62  
4-Bromofluorobenzene  
Concen: 51.330 ug/l  
RT: 12.727 min Scan# 11  
Delta R.T. 0.000 min  
Lab File: VN071896.D  
Acq: 07 Apr 2022 11:38




Instrument :  
MSVOA\_N  
ClientSampleId :  
VN0407MBL01


Tgt Ion: 95 Resp: 350093  
Ion Ratio Lower Upper  
95 100  
174 86.6 0.0 167.6  
176 84.6 0.0 163.4



#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 11.739 min Scan# 1658  
Delta R.T. 0.000 min  
Lab File: VN071896.D  
Acq: 07 Apr 2022 11:38

Tgt Ion: 117 Resp: 888208  
Ion Ratio Lower Upper  
117 100  
82 55.8 44.2 66.2  
119 33.4 25.4 38.0



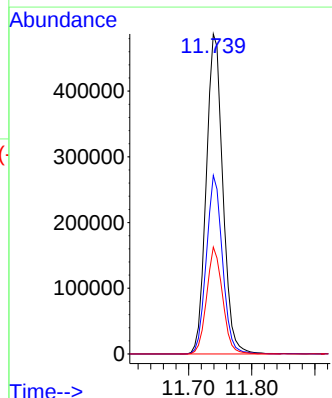





#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 13.674 min Scan# 1986  
Delta R.T. 0.005 min  
Lab File: VN071896.D  
Acq: 07 Apr 2022 11:38




Instrument :  
MSVOA\_N  
ClientSampleId :  
VN0407MBL01


Tgt Ion:152 Resp: 310362  
Ion Ratio Lower Upper  
152 100  
115 56.6 28.9 86.7  
150 158.1 0.0 356.2



#74  
N-ethyl acetate  
Concen: 0.447 ug/l  
RT: 12.386 min Scan# 1768  
Delta R.T. 0.006 min  
Lab File: VN071896.D  
Acq: 07 Apr 2022 11:38

Tgt Ion: 43 Resp: 3349  
Ion Ratio Lower Upper  
43 100  
70 43.0 39.0 58.4  
55 28.4 21.1 31.7  
61 24.0 21.1 31.7


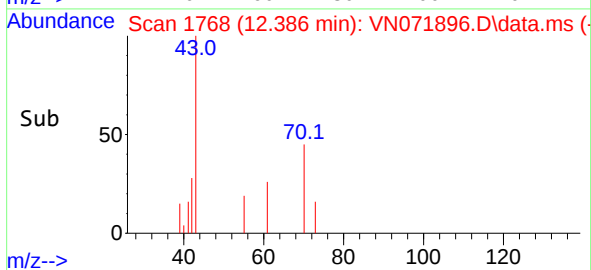






#76  
1,2,3-Trichloropropane  
Concen: 23.324 ug/l  
RT: 12.727 min Scan# 1826  
Delta R.T. -0.147 min  
Lab File: VN071896.D  
Acq: 07 Apr 2022 11:38




Instrument :  
MSVOA\_N  
ClientSampleId :  
VN0407MBL01


Tgt Ion: 75 Resp: 167697  
Ion Ratio Lower Upper  
75 100  
77 1.4 98.5 295.5#



#81  
trans-1,4-Dichloro-2-butene  
Concen: 72.281 ug/l  
RT: 12.727 min Scan# 1826  
Delta R.T. 0.105 min  
Lab File: VN071896.D  
Acq: 07 Apr 2022 11:38

Tgt Ion: 75 Resp: 167697  
Ion Ratio Lower Upper  
75 100  
53 0.0 78.0 117.0#  
89 0.0 37.2 55.8#

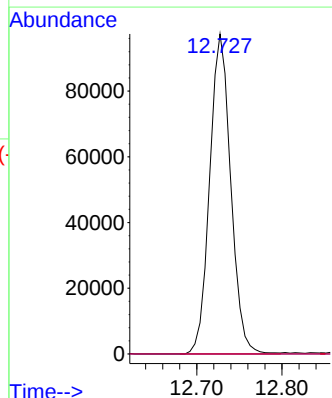



#87

1,3-Dichlorobenzene

Concen: 0.212 ug/l

RT: 13.615 min Scan# 1977

Delta R.T. 0.005 min

Lab File: VN071896.D

Acq: 07 Apr 2022 11:38

Instrument :

MSVOA\_N

ClientSampleId :

VN0407MBL01





Tgt Ion:146 Resp: 2216

Ion Ratio Lower Upper

146 100

111 33.3 20.0 60.0

148 63.0 32.0 96.0

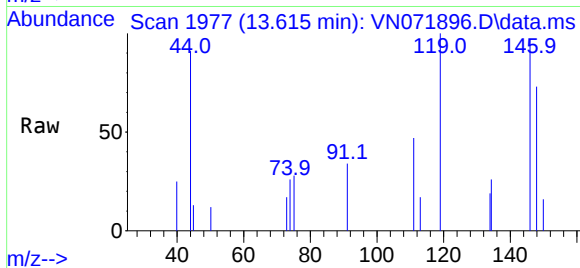

#88

1,4-Dichlorobenzene

Concen: 0.217 ug/l

RT: 13.615 min Scan# 1977

Delta R.T. -0.071 min

Lab File: VN071896.D

Acq: 07 Apr 2022 11:38




Tgt Ion:146 Resp: 2216


Ion Ratio Lower Upper

146 100

111 33.3 19.1 57.1

148 63.0 31.4 94.3



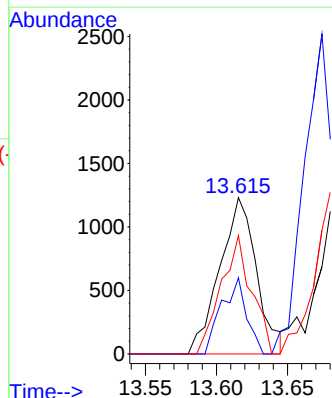
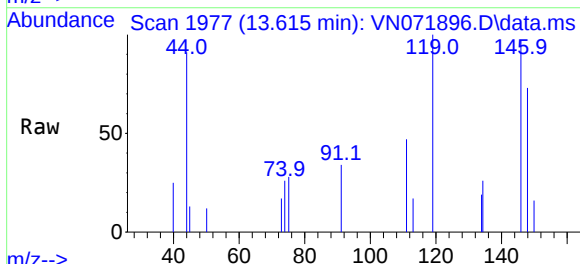




#89  
n-Butylbenzene  
Concen: 0.301 ug/l  
RT: 13.939 min Scan# 2032  
Delta R.T. -0.000 min  
Lab File: VN071896.D  
Acq: 07 Apr 2022 11:38




Instrument :  
MSVOA\_N  
ClientSampleId :  
VN0407MBL01


|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 91    | Resp: | 4371  |
| Ion      | Ratio | Lower | Upper |
| 91       | 100   |       |       |
| 92       | 50.4  | 26.9  | 80.7  |
| 134      | 26.4  | 13.6  | 40.8  |

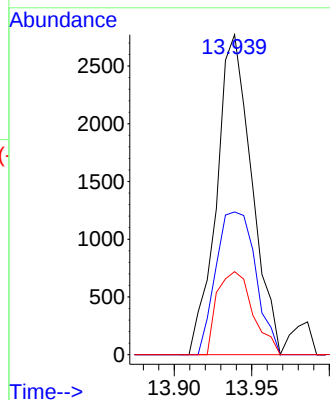

#91  
1,2-Dichlorobenzene  
Concen: 0.253 ug/l  
RT: 13.986 min Scan# 2040  
Delta R.T. 0.006 min  
Lab File: VN071896.D  
Acq: 07 Apr 2022 11:38

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 146   | Resp: | 2598  |
| Ion      | Ratio | Lower | Upper |
| 146      | 100   |       |       |
| 111      | 39.7  | 20.9  | 62.8  |
| 148      | 64.1  | 32.1  | 96.3  |



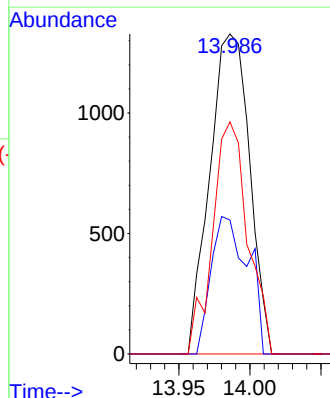





#92  
1,2-Dibromo-3-Chloropropane  
Concen: 0.341 ug/l  
RT: 14.598 min Scan# 2144  
Delta R.T. -0.000 min  
Lab File: VN071896.D  
Acq: 07 Apr 2022 11:38




Instrument :  
MSVOA\_N  
ClientSampleId :  
VN0407MBL01


Tgt Ion: 75 Resp: 461  
Ion Ratio Lower Upper  
75 100  
155 57.0 44.9 134.5  
157 113.2 59.0 176.8



#93  
1,2,4-Trichlorobenzene  
Concen: 2.802 ug/l  
RT: 15.262 min Scan# 2257  
Delta R.T. 0.005 min  
Lab File: VN071896.D  
Acq: 07 Apr 2022 11:38

Tgt Ion: 180 Resp: 3693  
Ion Ratio Lower Upper  
180 100  
182 92.2 47.5 142.5  
145 21.0 14.5 43.5


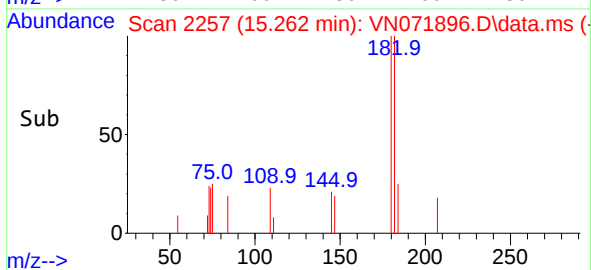






#94  
Hexachlorobutadiene  
Concen: 0.249 ug/l  
RT: 15.368 min Scan# 21  
Delta R.T. 0.005 min  
Lab File: VN071896.D  
Acq: 07 Apr 2022 11:38




Instrument :  
MSVOA\_N  
ClientSampleId :  
VN0407MBL01


|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 225   | Resp: | 754   |
| Ion      | Ratio | Lower | Upper |
| 225      | 100   |       |       |
| 223      | 33.8  | 32.4  | 97.2  |
| 227      | 38.5  | 31.8  | 95.4  |



#95  
Naphthalene  
Concen: 4.625 ug/l  
RT: 15.504 min Scan# 2298  
Delta R.T. 0.006 min  
Lab File: VN071896.D  
Acq: 07 Apr 2022 11:38


|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 128   | Resp: | 12581 |
| Ion      | Ratio | Lower | Upper |
| 128      | 100   |       |       |
| 127      | 13.4  | 10.3  | 15.5  |
| 129      | 12.2  | 8.6   | 13.0  |

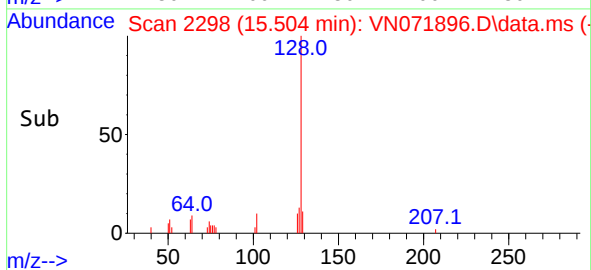



#96  
 1,2,3-Trichlorobenzene  
 Concen: 3.257 ug/l  
 RT: 15.698 min Scan# 21  
 Delta R.T. 0.006 min  
 Lab File: VN071896.D  
 Acq: 07 Apr 2022 11:38

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 VN0407MBL01



|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 180   | Resp: | 4236  |
| Ion      | Ratio | Lower | Upper |
| 180      | 100   |       |       |
| 182      | 99.2  | 47.8  | 143.3 |
| 145      | 33.3  | 15.5  | 46.5  |

