
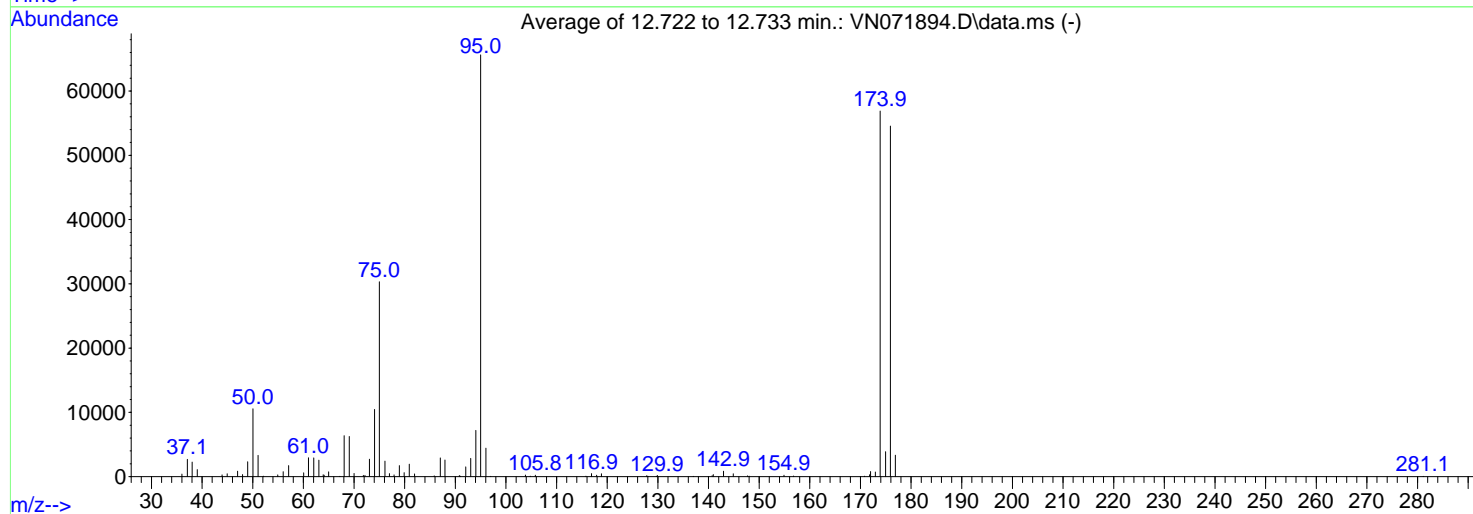


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN040722\  
 Data File : VN071894.D  
 Acq On : 07 Apr 2022 09:47  
 Operator : JC\MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA\_N/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N033022W.M  
 Title : SW846 8260  
 Last Update : Thu Mar 31 01:57:54 2022

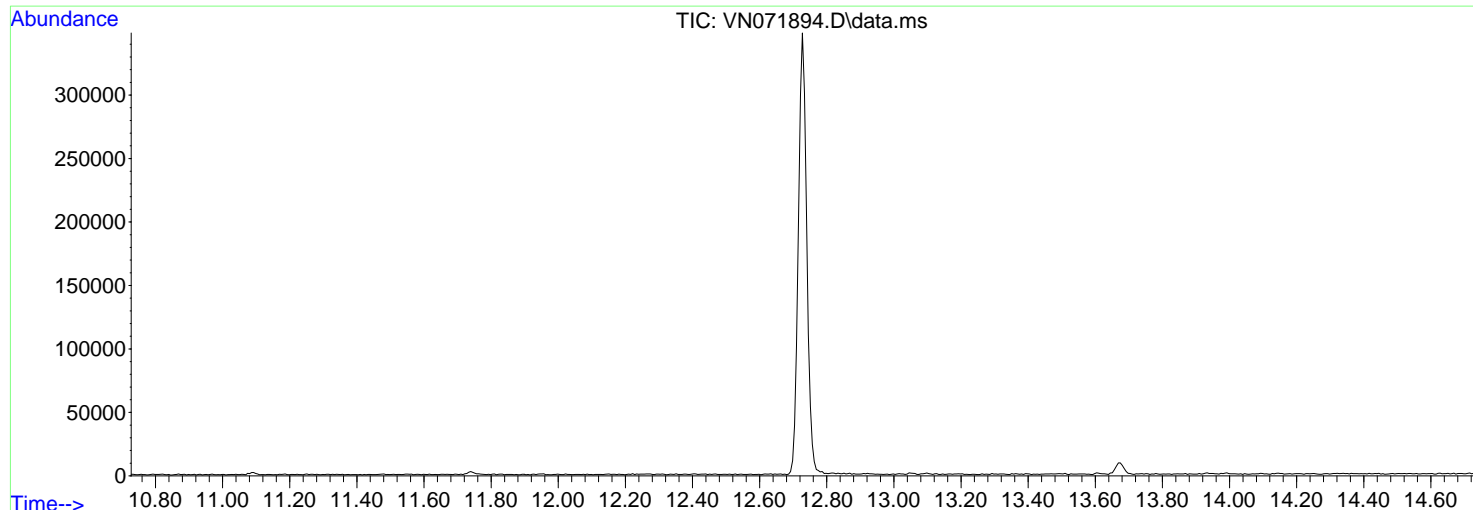

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1817

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	10570	PASS
75	95	30	60	46.2	30328	PASS
95	95	100	100	100.0	65635	PASS
96	95	5	9	6.8	4435	PASS
173	174	0.00	2	1.3	732	PASS
174	95	50	100	86.7	56891	PASS
175	174	5	9	6.8	3889	PASS
176	174	95	101	95.9	54549	PASS
177	176	5	9	6.1	3348	PASS