
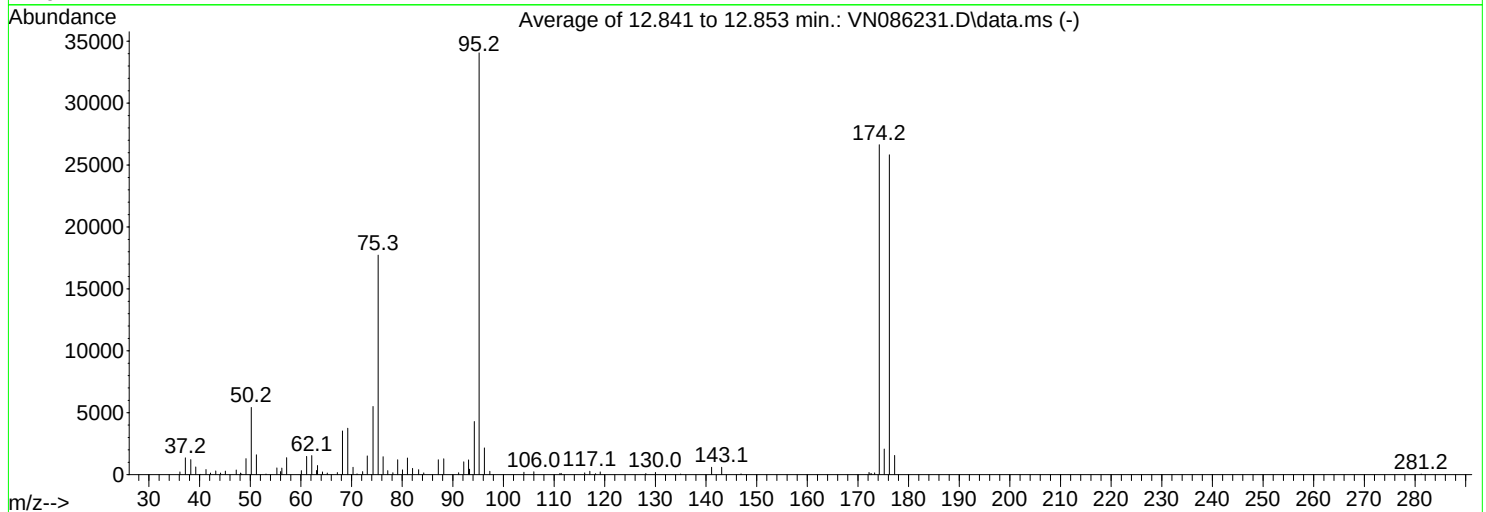


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN040725\
Data File : VN086231.D
Acq On : 07 Apr 2025 09:22
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N040725W.M
Title : SW846 8260
Last Update : Tue Apr 08 04:20:42 2025

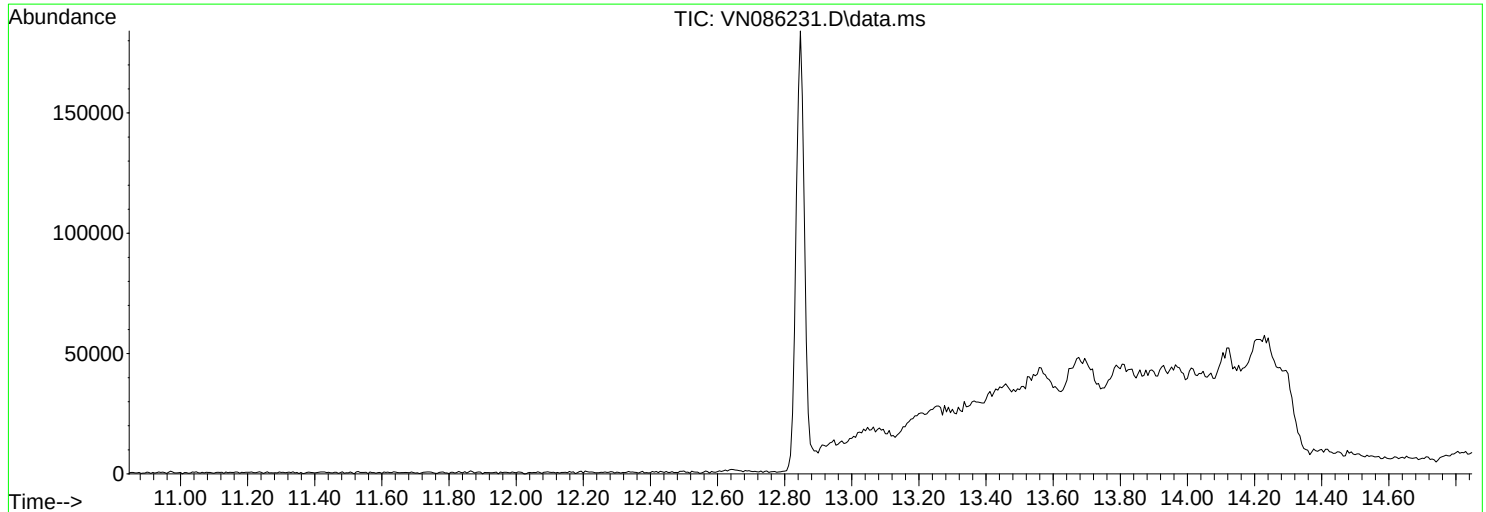

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	5430	PASS
75	95	30	60	52.0	17728	PASS
95	95	100	100	100.0	34064	PASS
96	95	5	9	6.3	2155	PASS
173	174	0.00	2	0.6	149	PASS
174	95	50	100	78.2	26648	PASS
175	174	5	9	7.8	2072	PASS
176	174	95	101	96.9	25827	PASS
177	176	5	9	6.0	1546	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.10	221	48.10	125	61.15	1473	72.20	251
37.20	1361	48.30	54	62.15	1540	73.10	151
38.25	1221	49.15	1296	63.10	343	74.25	550
39.25	618	50.20	5430	63.30	736	75.25	1772
40.10	21	51.20	1602	64.25	221	76.25	1454
41.25	408	53.10	57	65.20	136	77.15	325
42.15	129	55.25	545	67.20	165	78.15	152
43.20	301	56.00	245	68.20	3524	79.10	1205
44.15	126	56.25	526	69.25	3745	80.05	382
45.10	282	57.20	1373	70.30	595	81.05	1344
47.25	377	60.10	327	71.10	68	82.05	507

Average of 12.841 to 12.853 min.: VN086231.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
83.25	396	97.30	279	135.00	52	177.25	1546
84.25	147	104.05	201	141.10	591	281.20	51
87.15	1196	106.00	233	143.10	596		
88.20	1284	111.15	106	146.90	68		
91.15	153	111.40	99	172.20	181		
92.15	1039	116.05	142	172.40	79		
93.10	1185	117.05	279	172.70	81		
93.30	442	118.20	75	173.30	149		
94.25	4284	119.10	221	174.20	26648		
95.20	34064	128.10	89	175.20	2072		
96.25	2155	130.00	184	176.20	25827		

Instrument :

MSVOA_N

ClientSampleId :

BFB