

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN040822\
 Data File : VN071920.D
 Acq On : 08 Apr 2022 17:32
 Operator : JC\MD
 Sample : N2308-01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 EFF0422

Quant Time: Apr 09 05:06:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 31 01:57:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.086	168	707475	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	1196744	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	1232317	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.668	152	444374	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.433	65	383449	47.476	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	94.960%
35) Dibromofluoromethane	8.022	113	338924	48.128	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	96.260%
50) Toluene-d8	10.439	98	1494820	51.889	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	103.780%
62) 4-Bromofluorobenzene	12.727	95	487406	52.314	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	104.620%
Target Compounds						
					Qvalue	
11) Tert butyl alcohol	5.369	59	28808	21.979	ug/l	100
16) Acetone	4.304	43	6691	1.938	ug/l #	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN040822\
Data File : VN071920.D
Acq On : 08 Apr 2022 17:32
Operator : JC\MD
Sample : N2308-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
EFF0422

Quant Time: Apr 09 05:06:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
Quant Title : SW846 8260
QLast Update : Thu Mar 31 01:57:54 2022
Response via : Initial Calibration




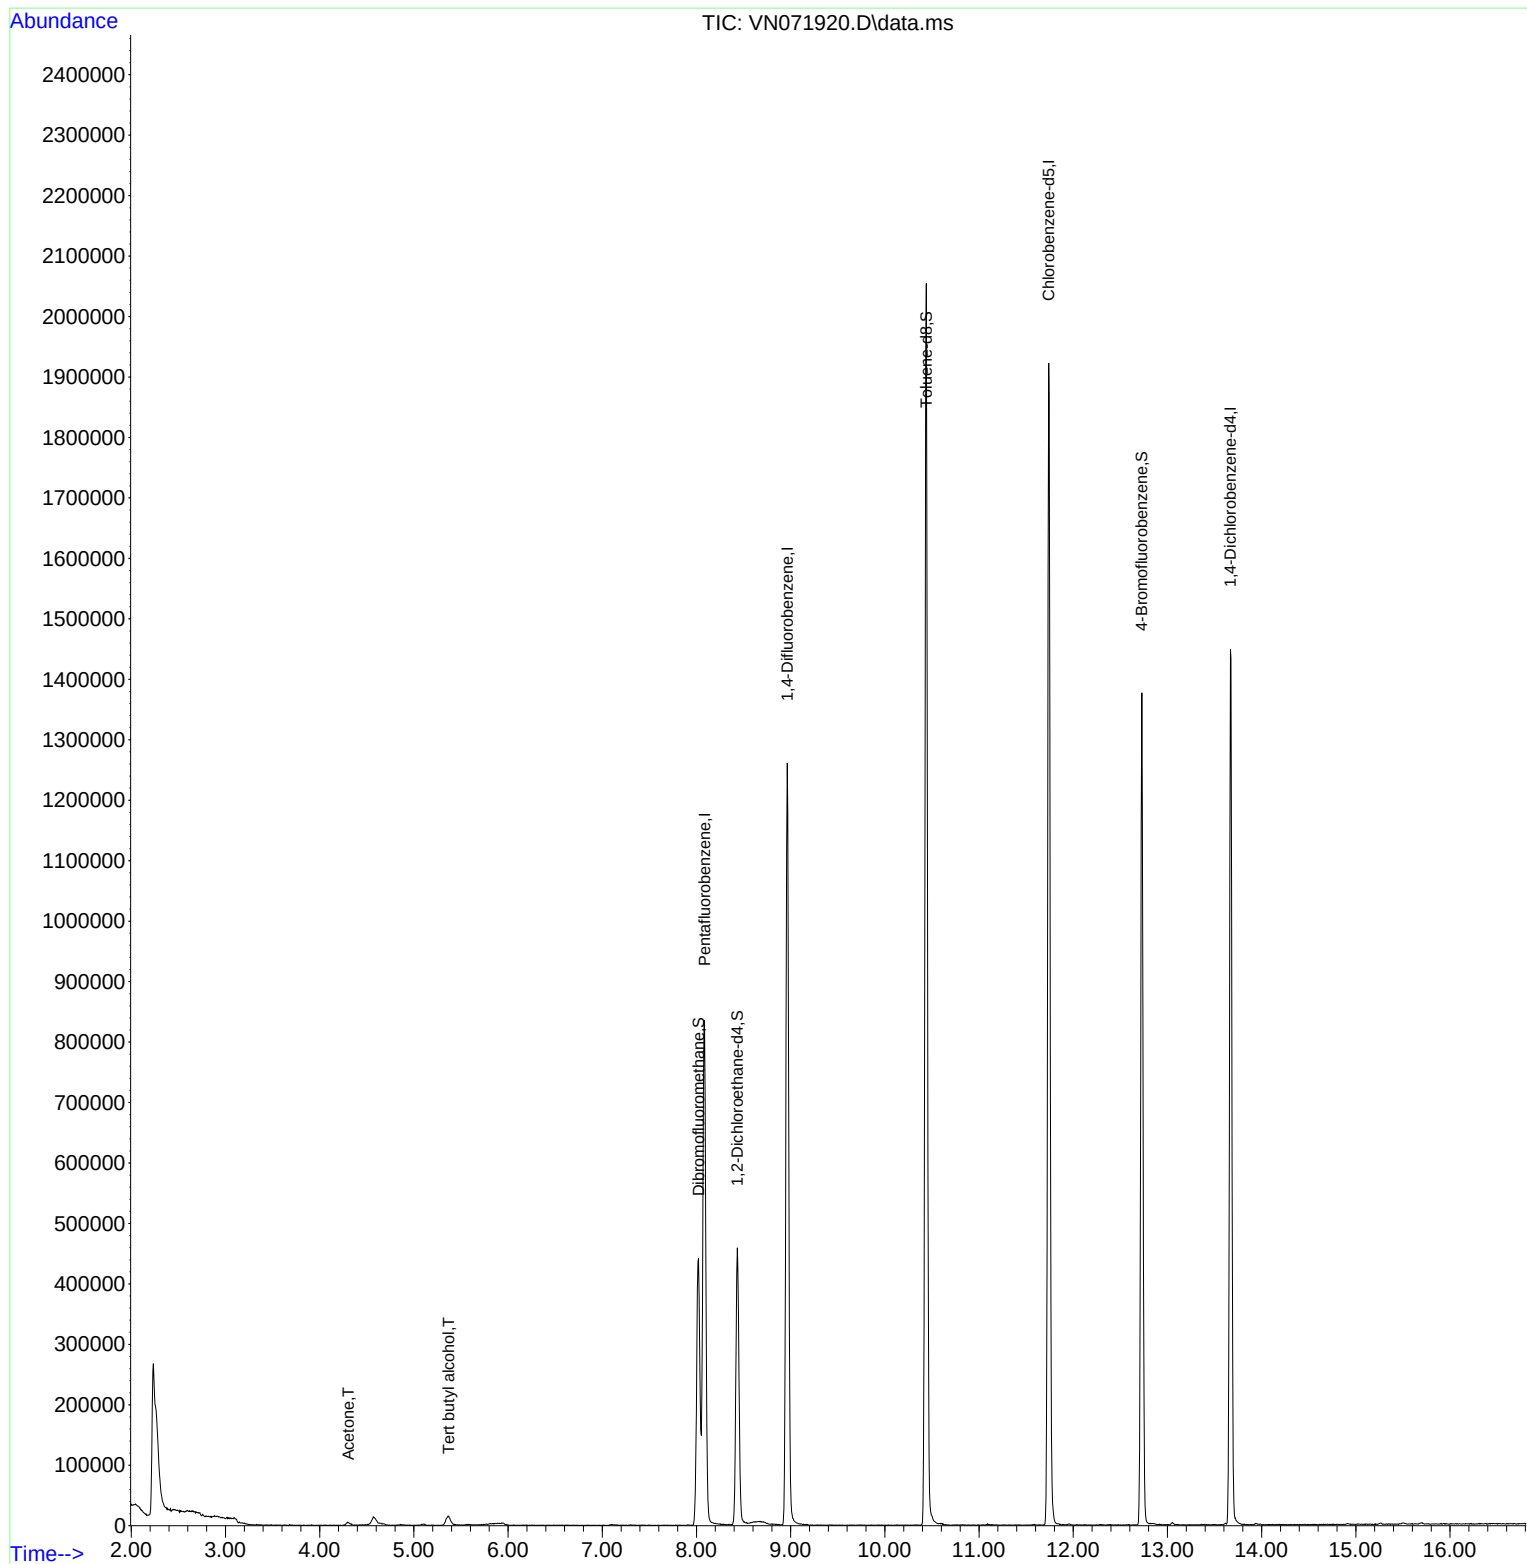


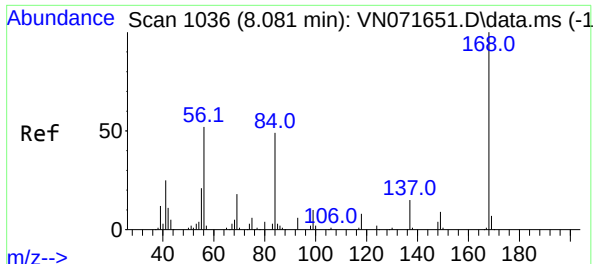

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.086 min Scan# 10
Delta R.T. 0.005 min
Lab File: VN071920.D
Acq: 08 Apr 2022 17:32




Instrument :
MSVOA_N
ClientSampleId :
EFF0422


Tgt Ion:168 Resp: 707475
Ion Ratio Lower Upper
168 100
99 49.4 42.3 63.5

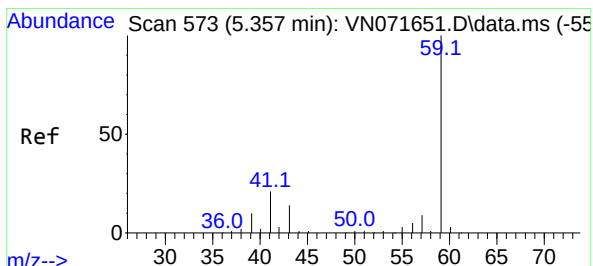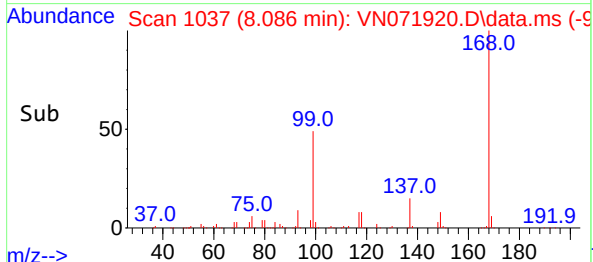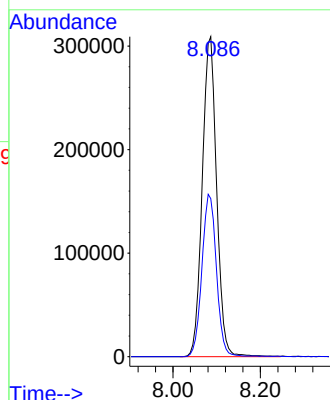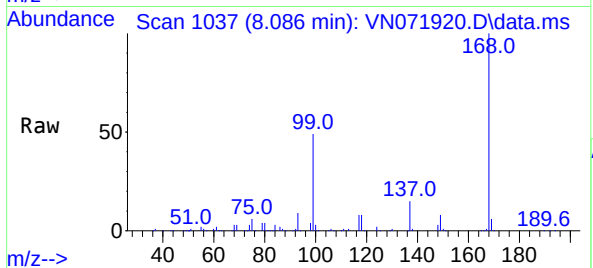

#11
Tert butyl alcohol
Concen: 21.979 ug/l
RT: 5.369 min Scan# 575
Delta R.T. 0.012 min
Lab File: VN071920.D
Acq: 08 Apr 2022 17:32

Tgt Ion: 59 Resp: 28808
Ion Ratio Lower Upper
59 100
57 10.3 8.3 12.5


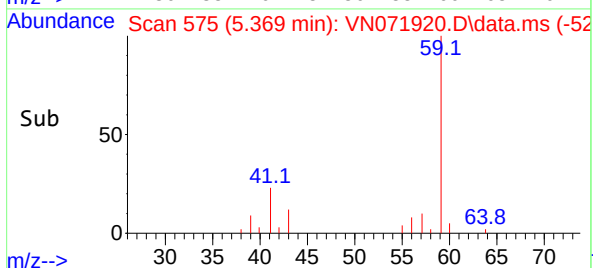
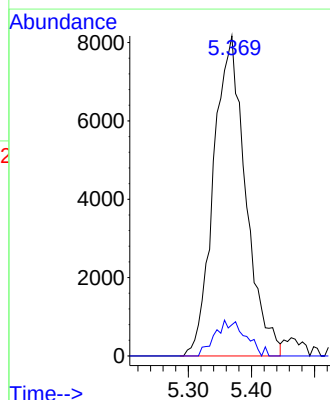
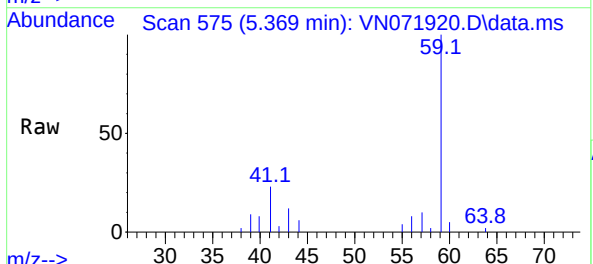


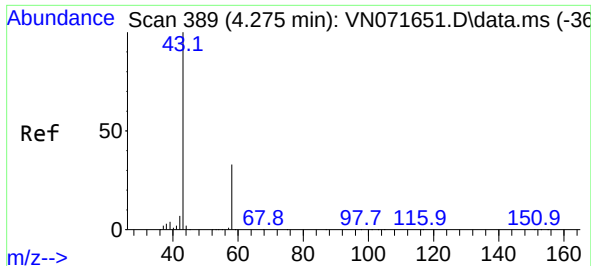

#16
Acetone
Concen: 1.938 ug/l
RT: 4.304 min Scan# 394
Delta R.T. 0.029 min
Lab File: VN071920.D
Acq: 08 Apr 2022 17:32




Instrument :
MSVOA_N
ClientSampleId :
EFF0422


Tgt Ion: 43 Resp: 6691
Ion Ratio Lower Upper
43 100
58 18.9 26.0 39.0#

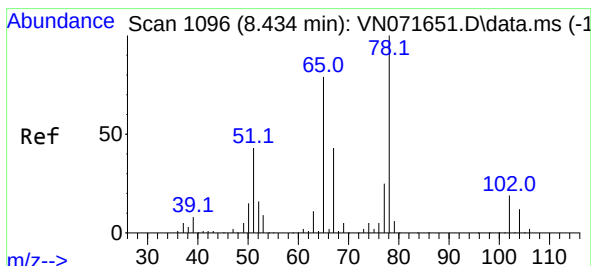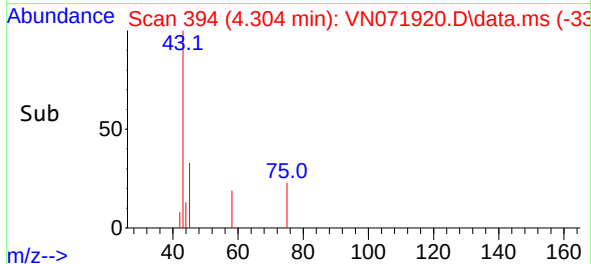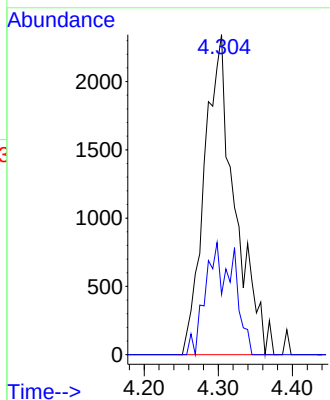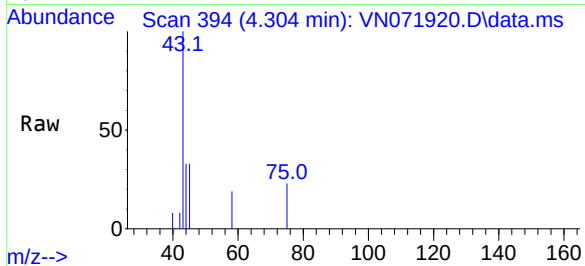

#33
1,2-Dichloroethane-d4
Concen: 47.476 ug/l
RT: 8.433 min Scan# 1096
Delta R.T. -0.001 min
Lab File: VN071920.D
Acq: 08 Apr 2022 17:32

Tgt Ion: 65 Resp: 383449
Ion Ratio Lower Upper
65 100
67 52.9 0.0 104.8


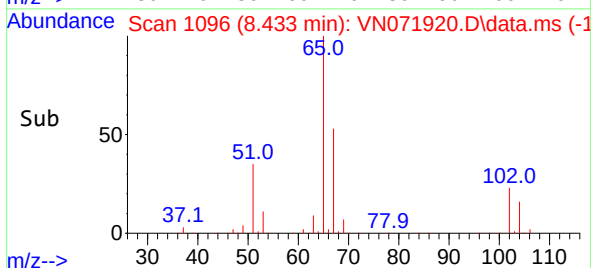
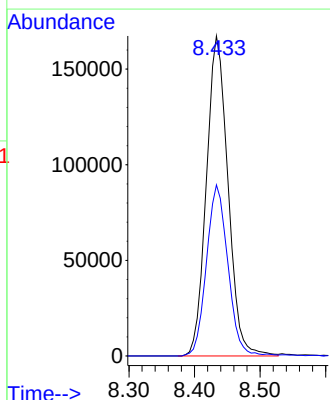
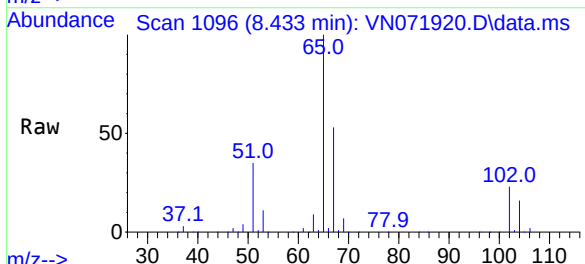


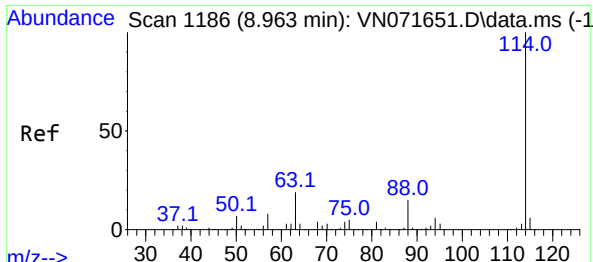

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.963 min Scan# 1186
Delta R.T. -0.000 min
Lab File: VN071920.D
Acq: 08 Apr 2022 17:32




Instrument :
MSVOA_N
ClientSampleId :
EFF0422


Tgt Ion:114 Resp: 1196744
Ion Ratio Lower Upper
114 100
63 19.4 0.0 40.0
88 14.9 0.0 32.6

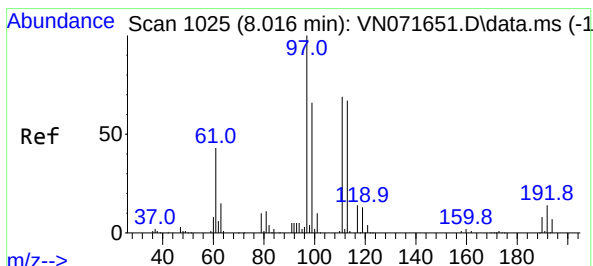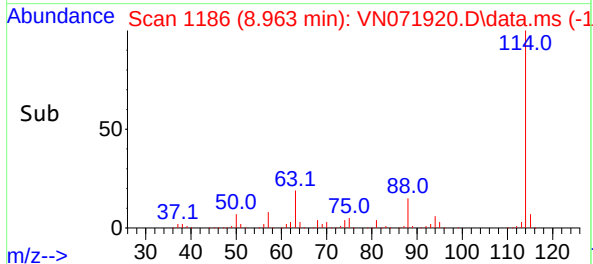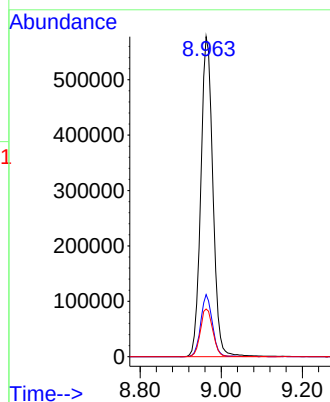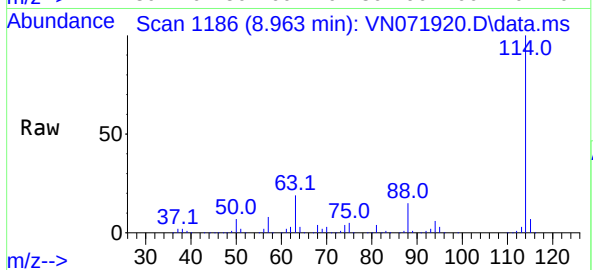

#35
Dibromofluoromethane
Concen: 48.128 ug/l
RT: 8.022 min Scan# 1026
Delta R.T. 0.006 min
Lab File: VN071920.D
Acq: 08 Apr 2022 17:32

Tgt Ion:113 Resp: 338924
Ion Ratio Lower Upper
113 100
111 102.7 81.4 122.0
192 21.8 17.0 25.6


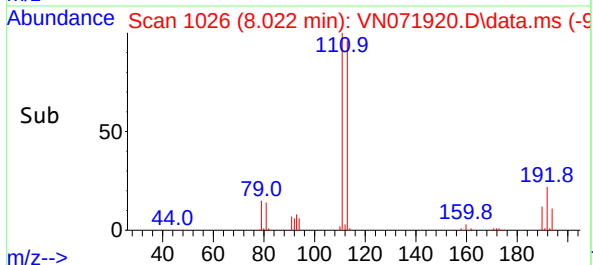
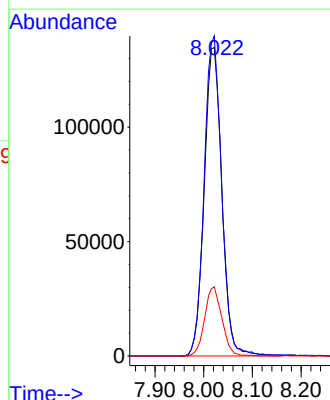
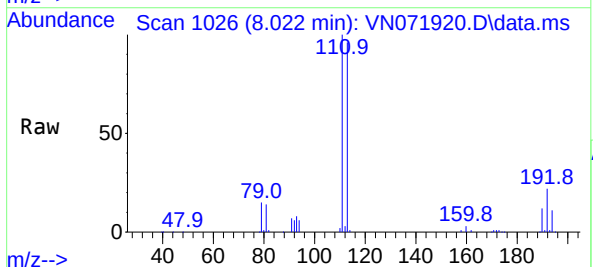


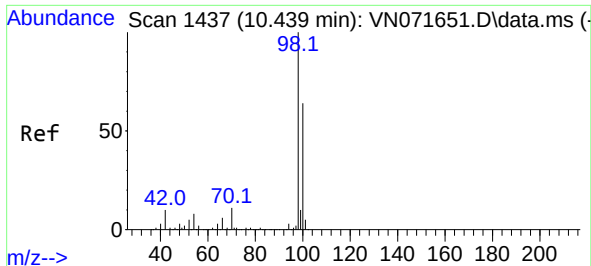

#50
Toluene-d8
Concen: 51.889 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. 0.000 min
Lab File: VN071920.D
Acq: 08 Apr 2022 17:32




Instrument :
MSVOA_N
ClientSampleId :
EFF0422


Tgt Ion: 98 Resp: 1494820
Ion Ratio Lower Upper
98 100
100 65.2 52.6 78.8

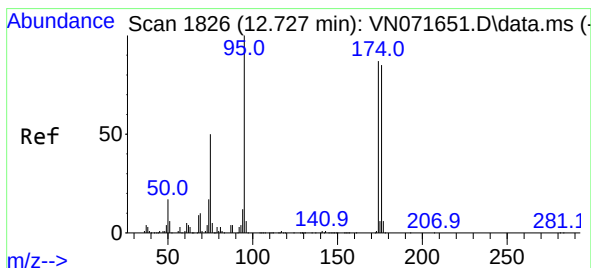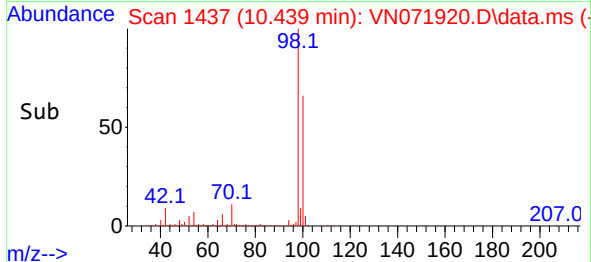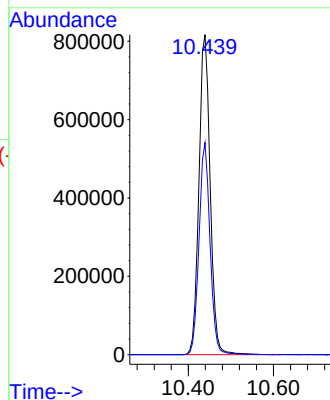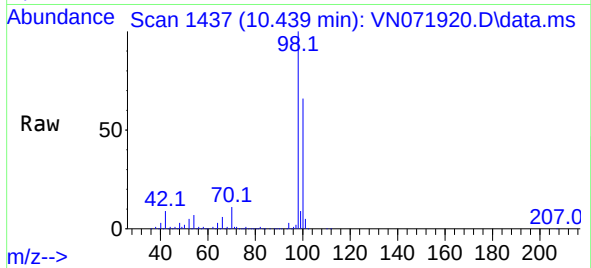

#62
4-Bromofluorobenzene
Concen: 52.314 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN071920.D
Acq: 08 Apr 2022 17:32

Tgt Ion: 95 Resp: 487406
Ion Ratio Lower Upper
95 100
174 86.1 0.0 167.6
176 84.1 0.0 163.4


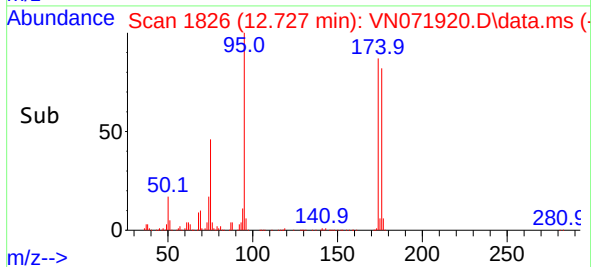
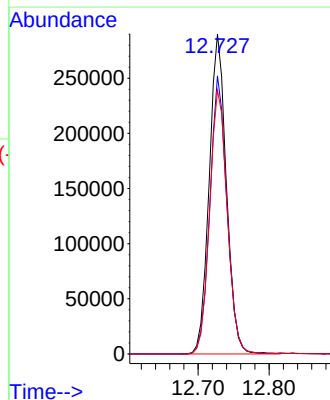
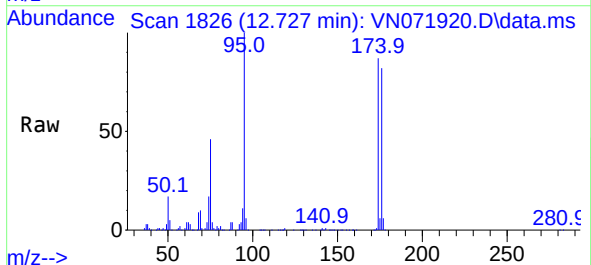


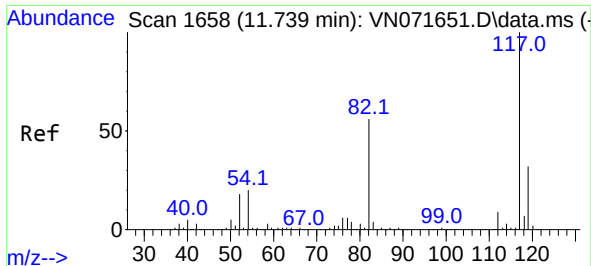

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 1
Delta R.T. 0.000 min
Lab File: VN071920.D
Acq: 08 Apr 2022 17:32

Instrument :
MSVOA_N
ClientSampleId :
EFF0422

Tgt Ion:117 Resp: 1232317
Ion Ratio Lower Upper
117 100
82 55.5 44.2 66.2
119 32.9 25.4 38.0

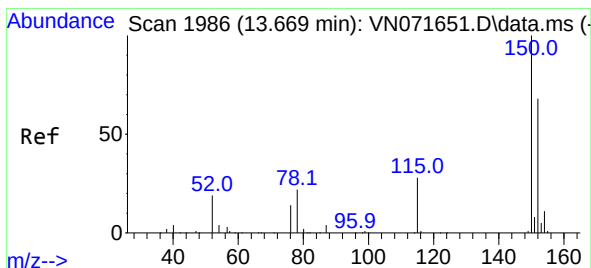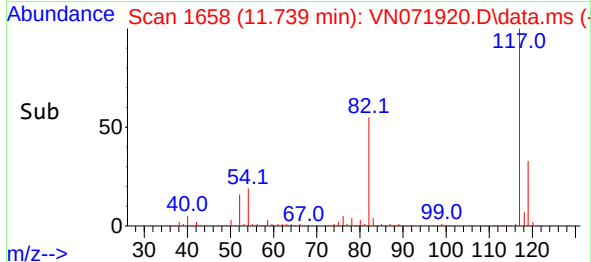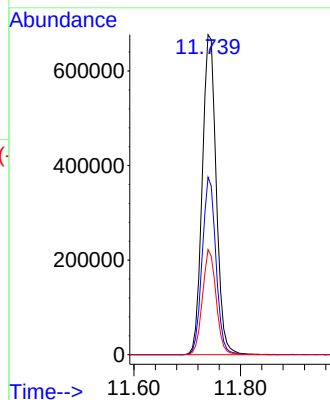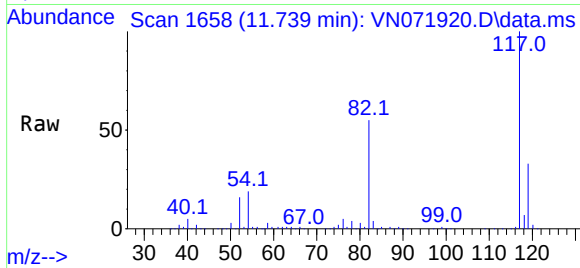

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.668 min Scan# 1986
Delta R.T. -0.001 min
Lab File: VN071920.D
Acq: 08 Apr 2022 17:32

Tgt Ion:152 Resp: 444374
Ion Ratio Lower Upper
152 100
115 56.4 28.9 86.7
150 156.7 0.0 356.2

