
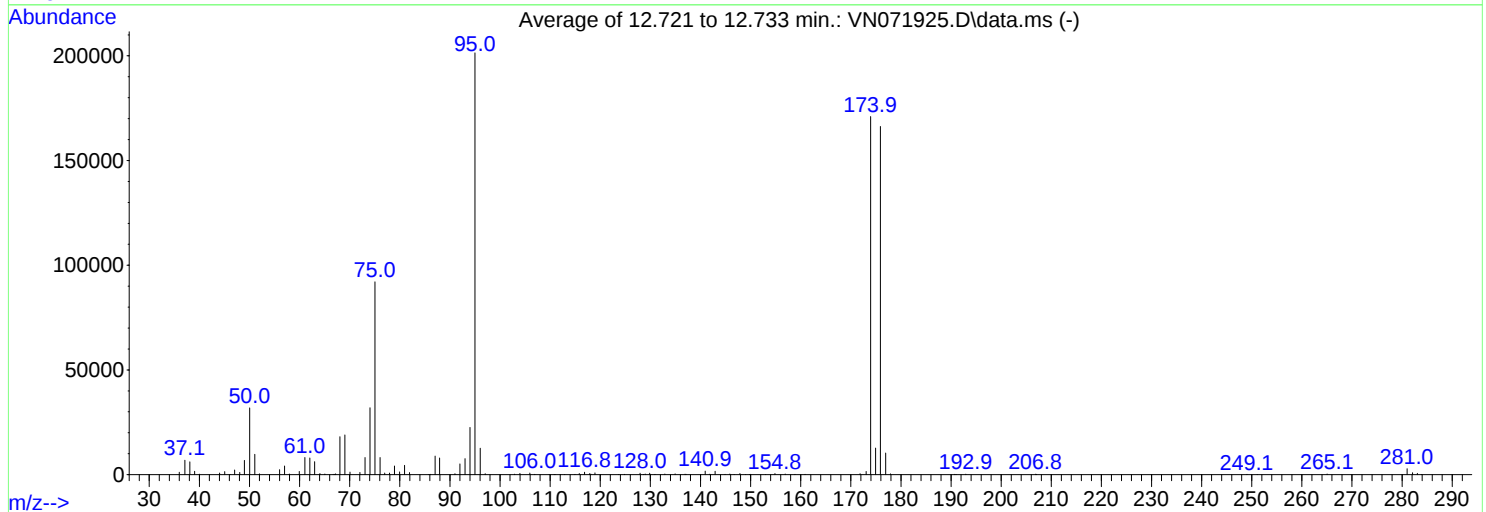


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN040822\
 Data File : VN071925.D
 Acq On : 08 Apr 2022 19:33
 Operator : JC\MD
 Sample : VSTDCCC050
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_N
 LabSampleId :
 VSTDCCC050

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
 Title : SW846 8260
 Last Update : Thu Mar 31 01:57:54 2022

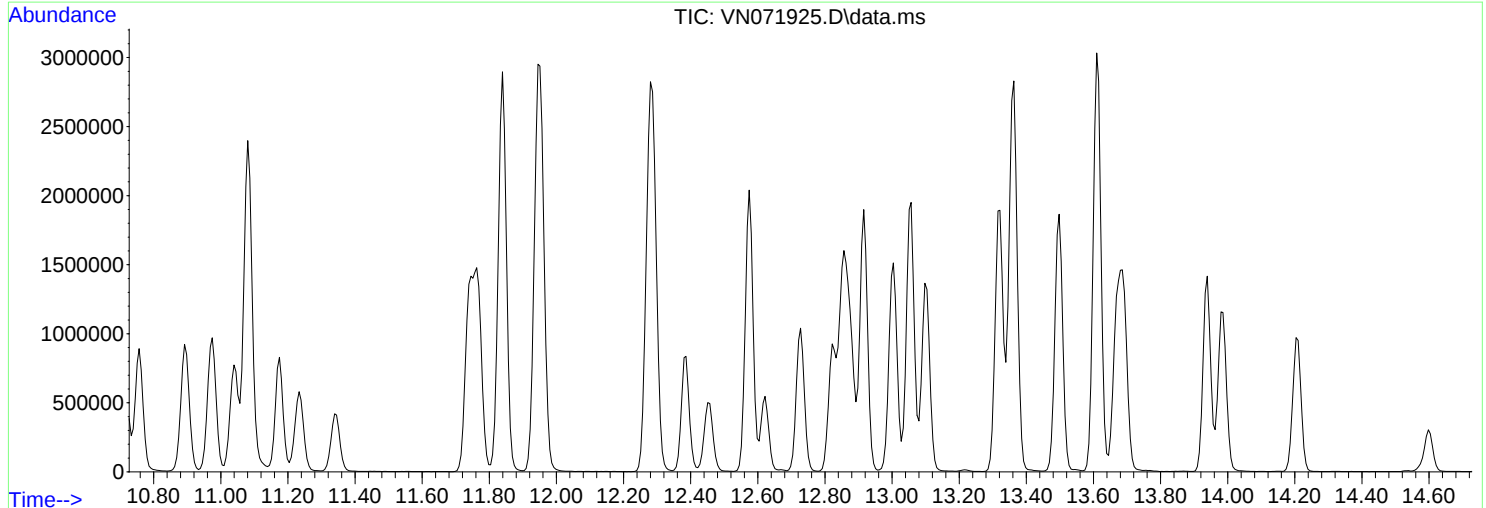

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1816

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	31840	PASS
75	95	30	60	45.7	92095	PASS
95	95	100	100	100.0	201429	PASS
96	95	5	9	6.3	12610	PASS
173	174	0.00	2	0.9	1552	PASS
174	95	50	100	84.9	170987	PASS
175	174	5	9	7.4	12719	PASS
176	174	95	101	97.3	166293	PASS
177	176	5	9	6.2	10301	PASS