
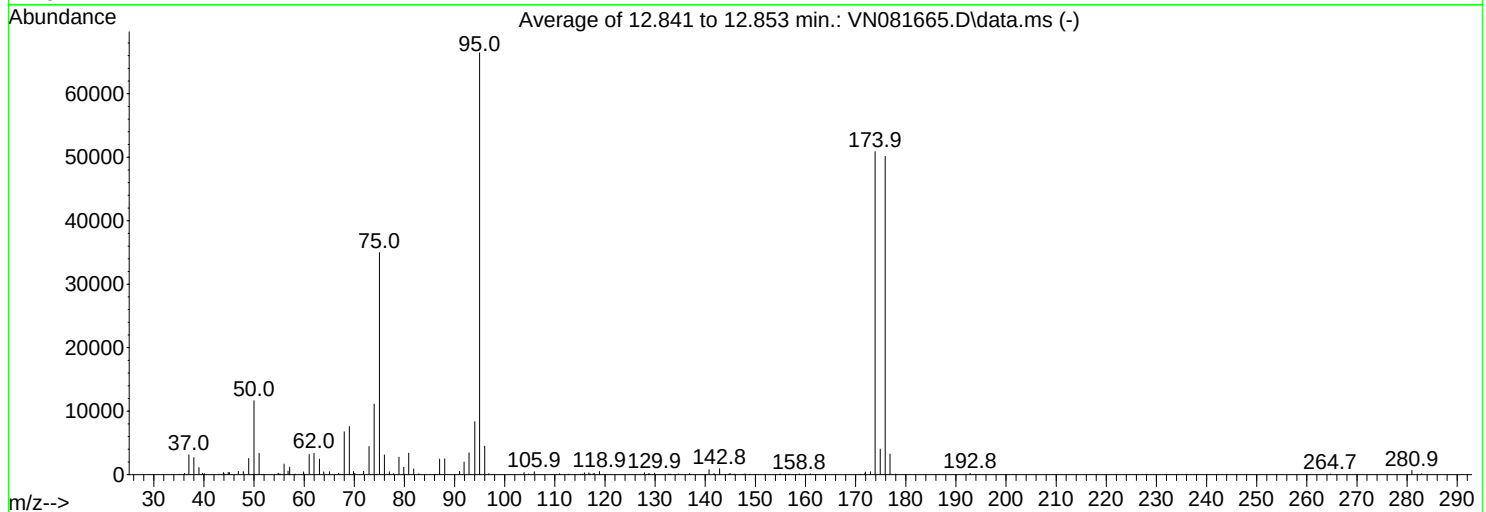


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN040824\
Data File : VN081665.D
Acq On : 08 Apr 2024 08:37
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N031824W.M
Title : SW846 8260
Last Update : Tue Mar 19 06:00:00 2024

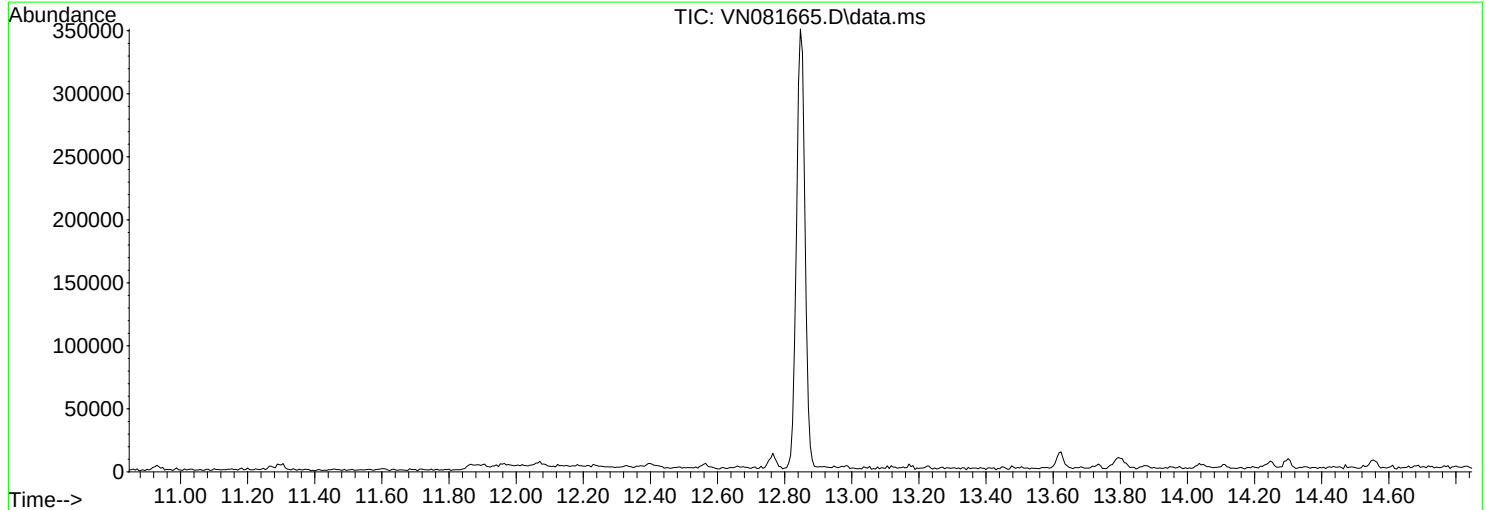

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.5	11656	PASS
75	95	30	60	52.6	34973	PASS
95	95	100	100	100.0	66443	PASS
96	95	5	9	6.7	4482	PASS
173	174	0.00	2	0.9	464	PASS
174	95	50	100	76.6	50880	PASS
175	174	5	9	7.9	4024	PASS
176	174	95	101	98.5	50131	PASS
177	176	5	9	6.5	3251	PASS

Average of 12.841 to 12.853 min.: VN081665.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.10	55	44.85	355	56.00	1677	66.85	231
35.90	55	45.10	332	56.80	544	67.10	91
36.10	199	46.85	512	57.10	1194	68.00	675
37.00	3137	47.85	489	58.20	96	69.00	759
38.00	2690	48.95	2558	59.90	435	69.85	470
39.00	1100	50.00	11656	60.10	76	70.10	193
39.75	239	51.00	3356	61.00	3178	71.85	534
40.10	177	51.80	52	61.95	3358	72.95	4437
43.00	85	54.80	216	63.05	2440	73.95	11116
43.90	341	55.00	130	63.90	430	75.00	34973
44.05	139	55.30	82	65.05	455	76.00	3111

Average of 12.841 to 12.853 min.: VN081665.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.00	465	91.90	1982	115.10	61	129.90	251
77.80	150	92.90	3465	115.50	78	132.70	97
78.90	2754	94.05	8348	115.90	288	133.10	93
79.85	1159	95.00	66443	116.80	289	134.70	126
80.85	3379	96.00	4482	117.00	136	136.85	159
81.85	921	96.85	152	117.60	112	140.75	786
82.85	131	103.85	324	117.85	219	141.75	168
86.10	63	104.80	99	118.90	475	142.85	927
87.00	2457	105.90	466	127.85	312	144.70	83
88.05	2497	110.95	157	128.70	134	144.95	223
91.00	512	112.70	64	128.85	132	145.90	111

Average of 12.841 to 12.853 min.: VN081665.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
147.70	63	172.95	464				
147.95	138	173.90	50880				
148.90	60	174.90	4024				
154.80	63	175.90	50131				
155.00	95	176.85	3251				
156.70	66	178.00	92				
158.75	126	192.85	205				
161.00	121	264.70	108				
171.00	54	280.95	670				
171.80	150	282.10	80				
171.95	416	282.90	137				