
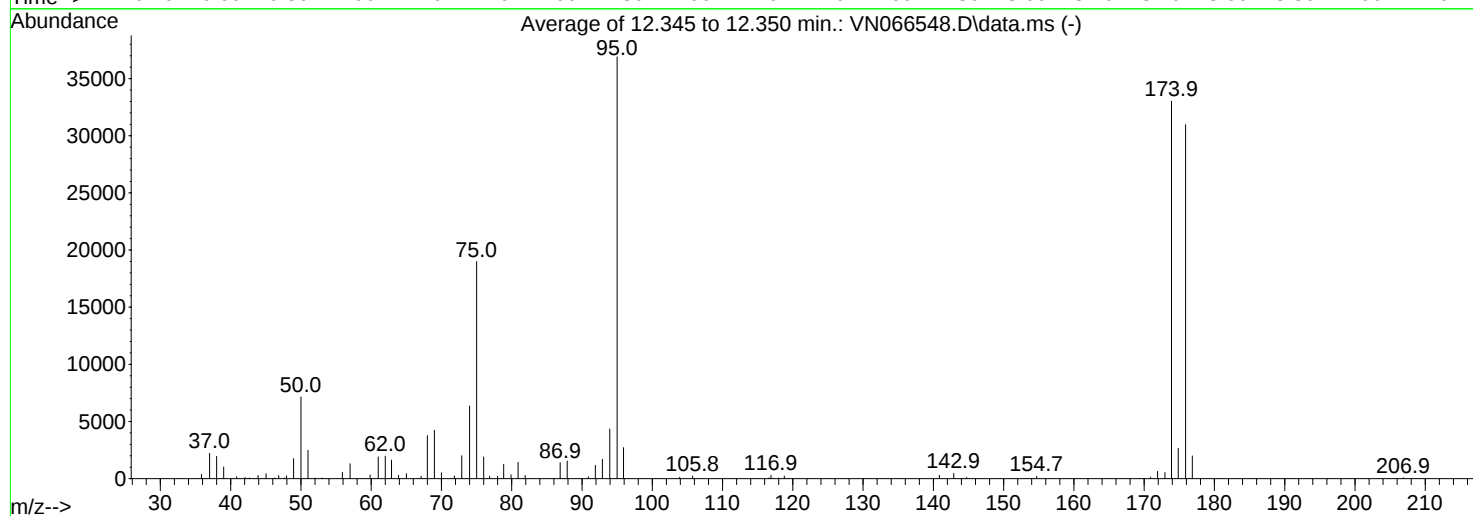


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN040921\
 Data File : VN066548.D
 Acq On : 9 Apr 2021 2:26
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N032421W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Mon Apr 12 02:23:50 2021

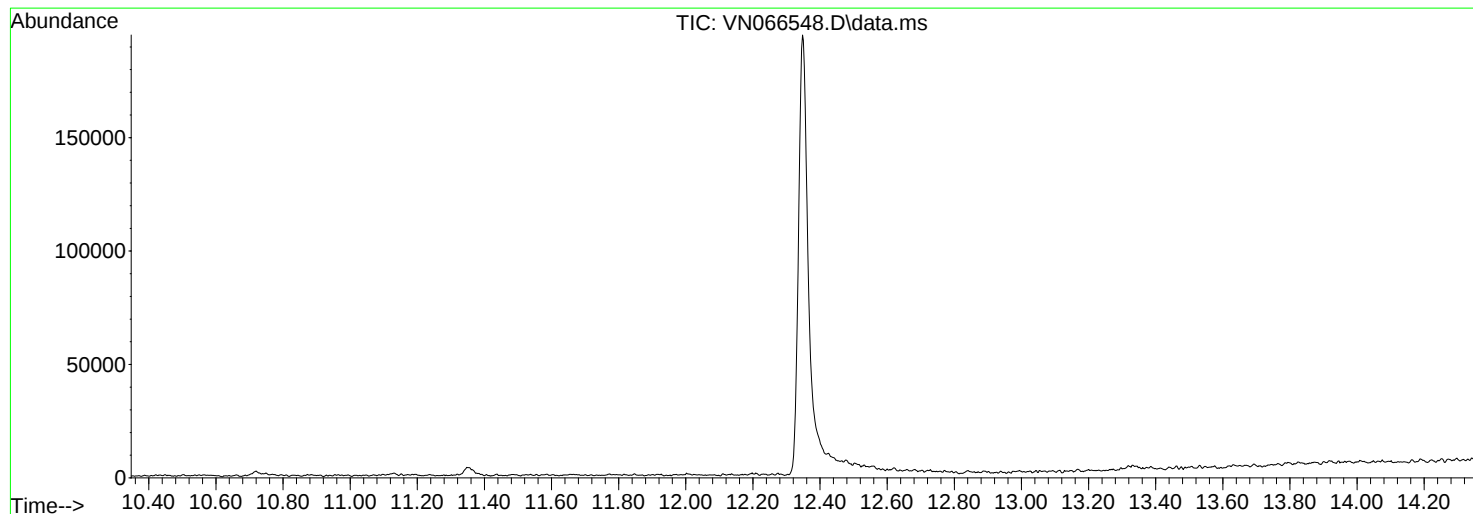

AutoFind: Scans 3973, 3974, 3975; Background Corrected with Scan 3959

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	7154	PASS
75	95	30	60	51.5	19000	PASS
95	95	100	100	100.0	36904	PASS
96	95	5	9	7.4	2722	PASS
173	174	0.00	2	1.6	533	PASS
174	95	50	100	89.5	33027	PASS
175	174	5	9	8.0	2656	PASS
176	174	95	101	93.8	30963	FAIL*
177	176	5	9	6.4	1985	PASS