


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041021\
Data File : VN066561.D
Acq On : 9 Apr 2021 16:30
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N041021W.M
Title : SW846 8260
Last Update : Mon Apr 12 13:08:33 2021

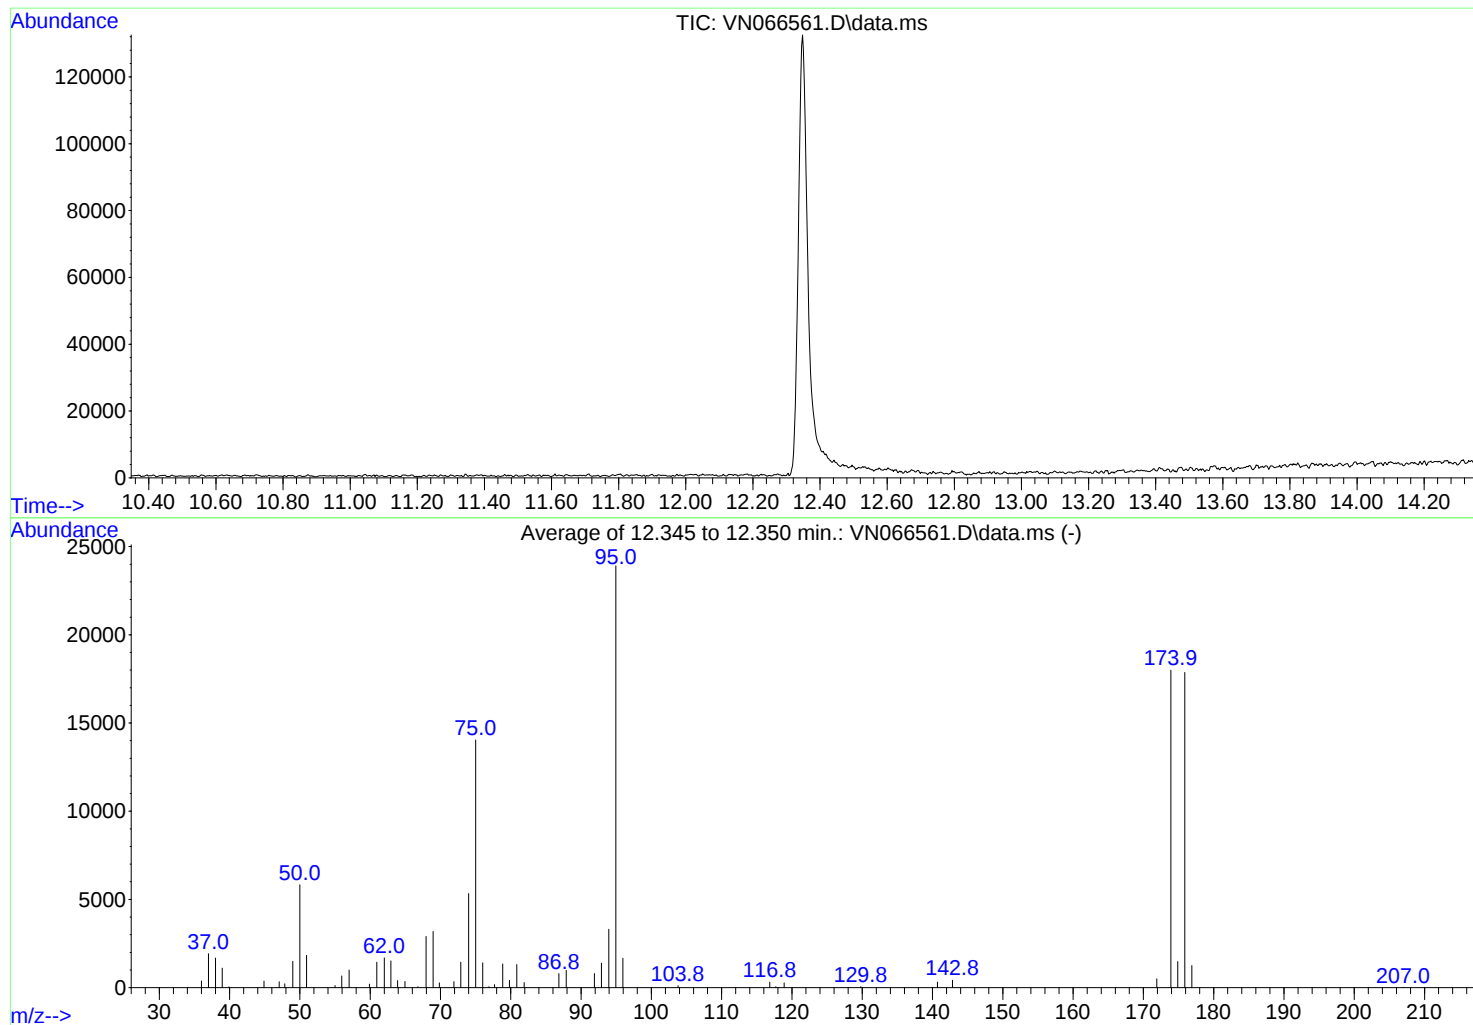

AutoFind: Scans 3973, 3974, 3975; Background Corrected with Scan 3958

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.4	5836	PASS
75	95	30	60	58.7	14040	PASS
95	95	100	100	100.0	23909	PASS
96	95	5	9	7.0	1672	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	75.3	17997	PASS
175	174	5	9	8.2	1480	PASS
176	174	95	101	99.3	17867	PASS
177	176	5	9	7.0	1249	PASS