
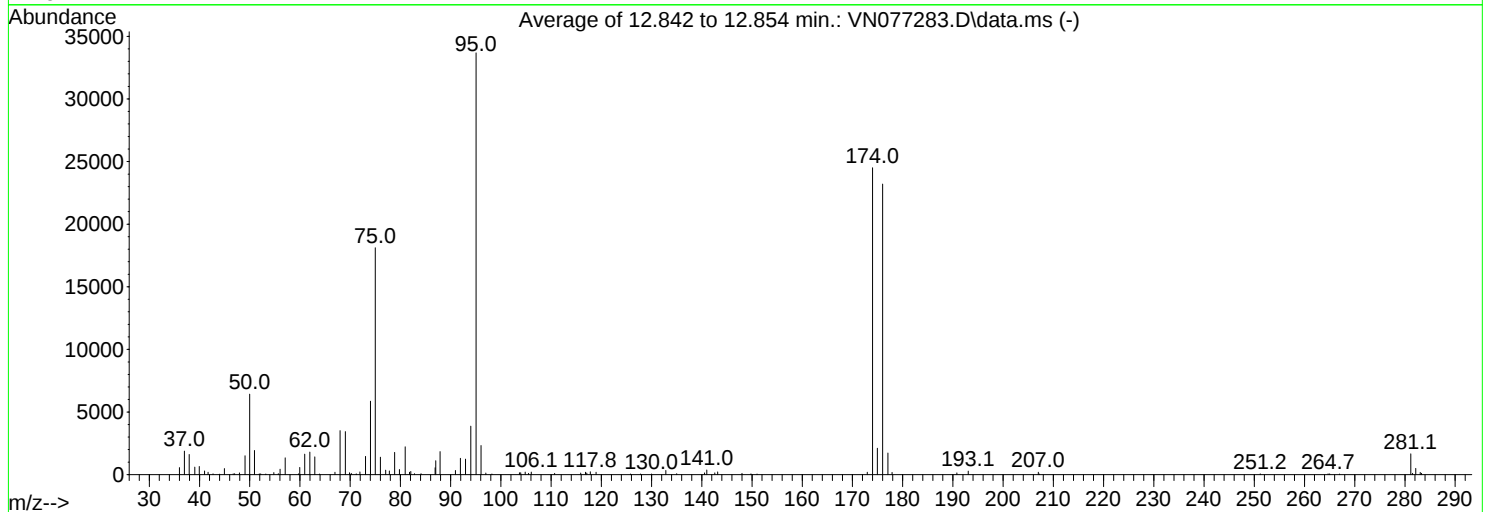


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041023\
 Data File : VN077283.D
 Acq On : 10 Apr 2023 08:51
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N040723W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Apr 07 13:04:49 2023

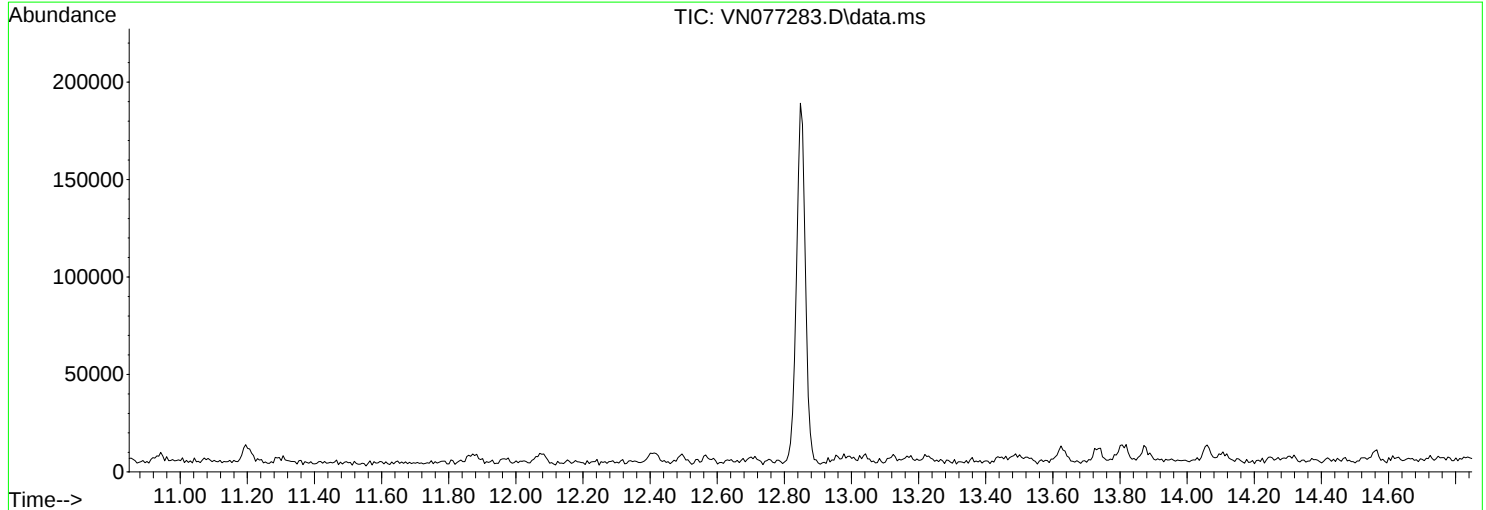

AutoFind: Scans 1854, 1855, 1856; Background Corrected with Scan 1847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	6423	PASS
75	95	30	60	53.8	18120	PASS
95	95	100	100	100.0	33680	PASS
96	95	5	9	6.9	2321	PASS
173	174	0.00	2	0.8	189	PASS
174	95	50	100	72.8	24509	PASS
175	174	5	9	8.6	2114	PASS
176	174	95	101	94.7	23200	FAIL*
177	176	5	9	7.5	1730	PASS