
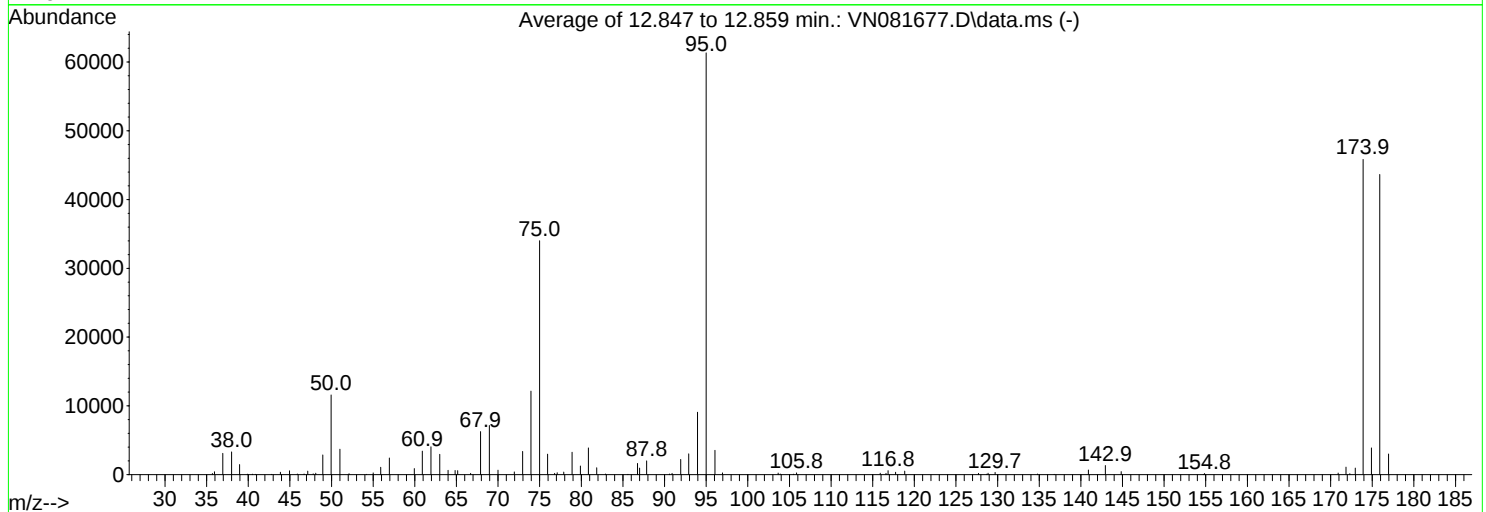


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041024\
Data File : VN081677.D
Acq On : 10 Apr 2024 12:37
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N041024W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu Apr 11 09:25:01 2024

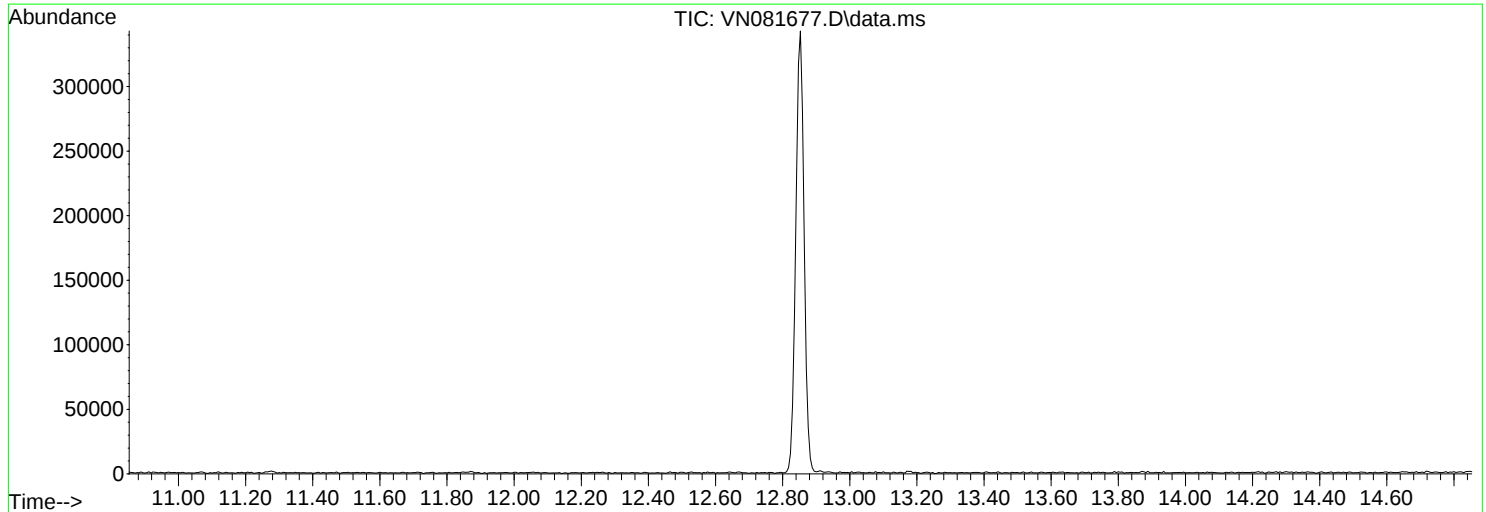

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.9	11578	PASS
75	95	30	60	55.4	34005	PASS
95	95	100	100	100.0	61331	PASS
96	95	5	9	5.8	3533	PASS
173	174	0.00	2	2.1	946	FAIL*
174	95	50	100	74.7	45843	PASS
175	174	5	9	8.5	3888	PASS
176	174	95	101	95.2	43653	PASS
177	176	5	9	6.9	3011	PASS