


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN041119\
 Data File : VN054975.D
 Acq On : 11 Apr 2019 13:43
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N041119W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Apr 12 07:55:25 2019

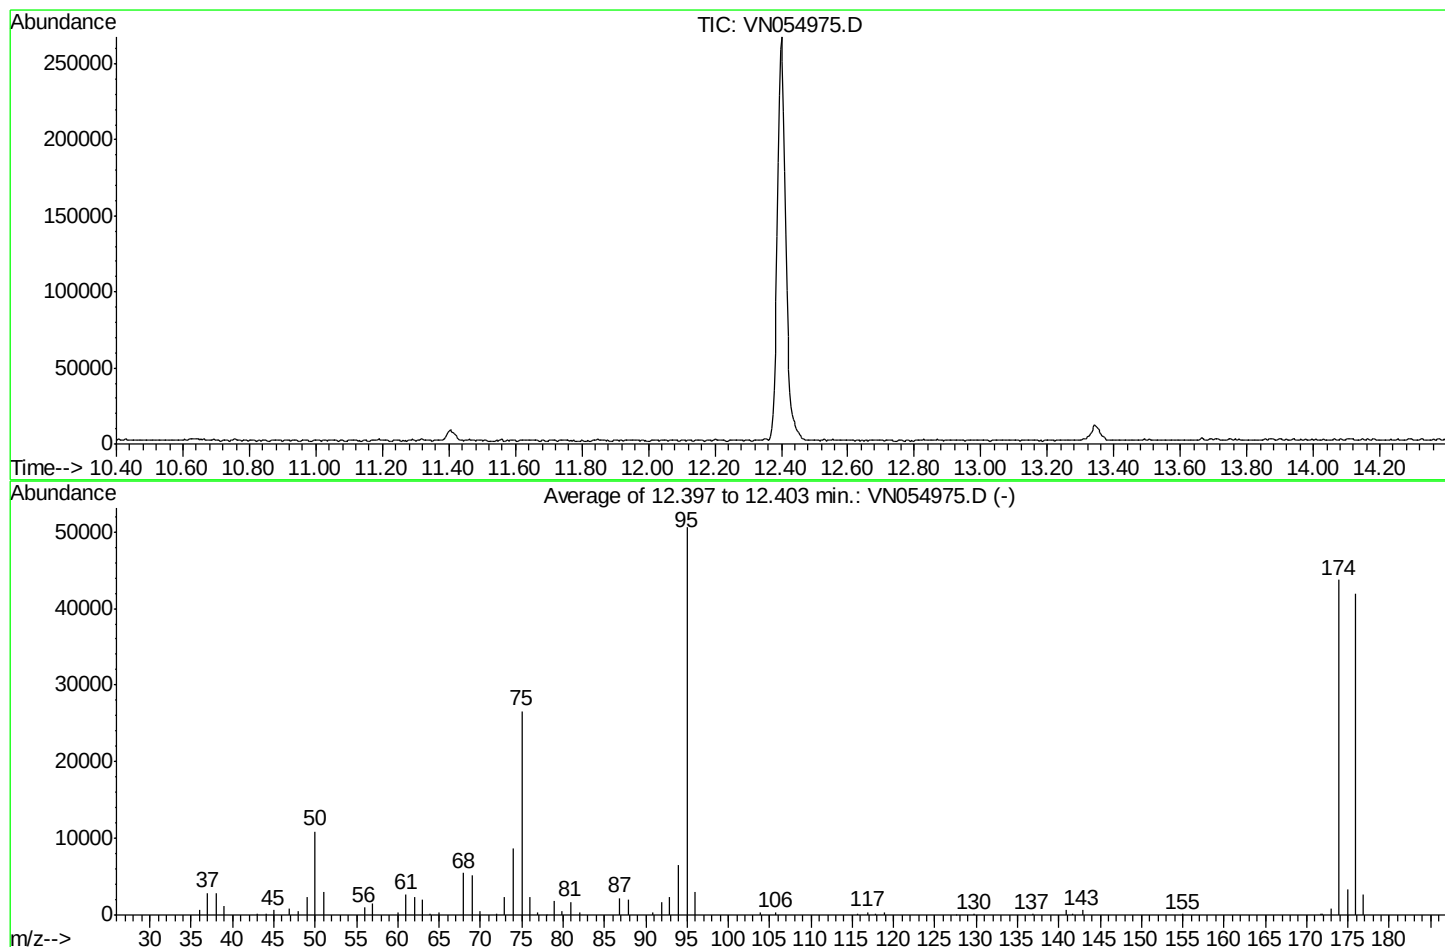

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	10866	PASS
75	95	30	60	52.6	26621	PASS
95	95	100	100	100.0	50586	PASS
96	95	5	9	6.0	3022	PASS
173	174	0.00	2	1.7	758	PASS
174	95	50	100	86.4	43728	PASS
175	174	5	9	7.7	3364	PASS
176	174	95	101	95.9	41917	PASS
177	176	5	9	6.4	2672	PASS