

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041122\
 Data File : VN071928.D
 Acq On : 11 Apr 2022 12:04
 Operator : JC\MD
 Sample : VN0411MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0411MBL01

Quant Time: Apr 11 12:28:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 31 01:57:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.081	168	531100	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	888848	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	909367	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.668	152	324325	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.433	65	286374	47.232	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	94.460%
35) Dibromofluoromethane	8.016	113	255128	48.778	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	97.560%
50) Toluene-d8	10.439	98	1109028	51.833	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	103.660%
62) 4-Bromofluorobenzene	12.727	95	365535	52.824	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	105.640%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041122\
Data File : VN071928.D
Acq On : 11 Apr 2022 12:04
Operator : JC\MD
Sample : VN0411MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0411MBL01

Quant Time: Apr 11 12:28:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
Quant Title : SW846 8260
QLast Update : Thu Mar 31 01:57:54 2022
Response via : Initial Calibration




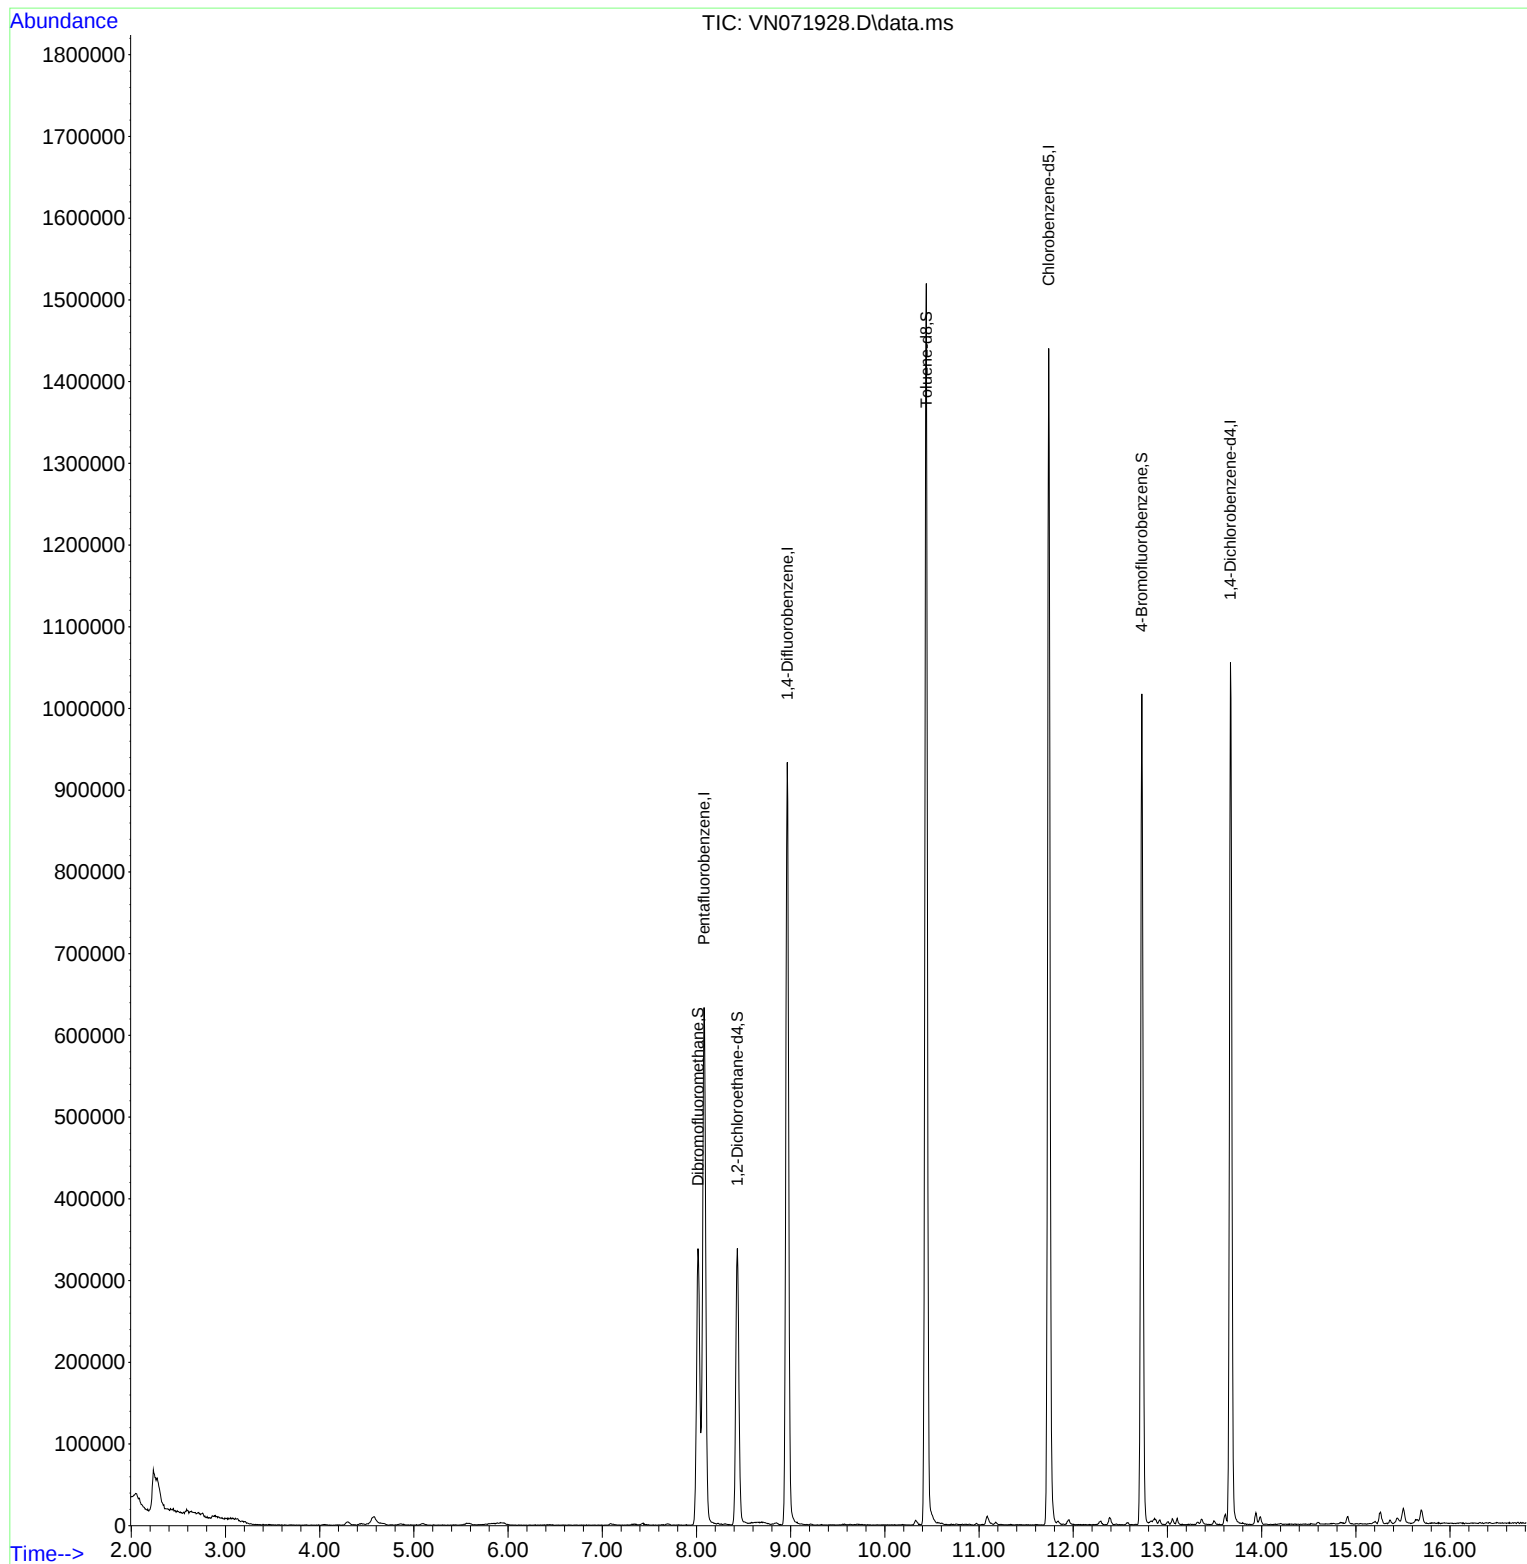


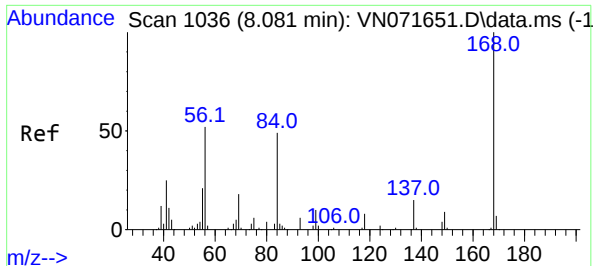

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. -0.000 min
Lab File: VN071928.D
Acq: 11 Apr 2022 12:04




Instrument :
MSVOA_N
ClientSampleId :
VN0411MBL01


Tgt Ion:168 Resp: 531100
Ion Ratio Lower Upper
168 100
99 52.6 42.3 63.5

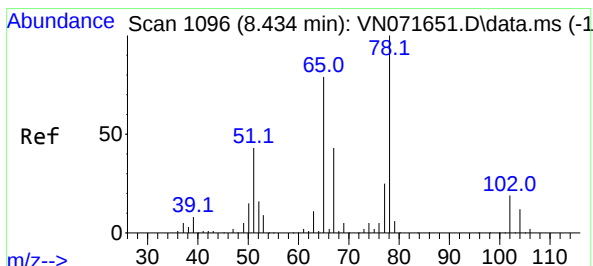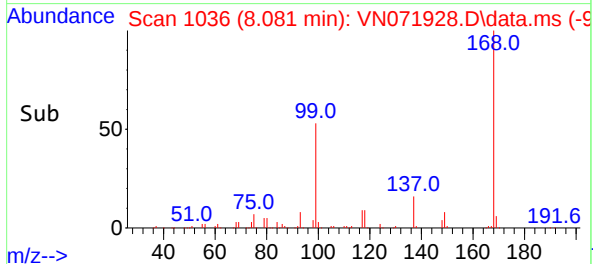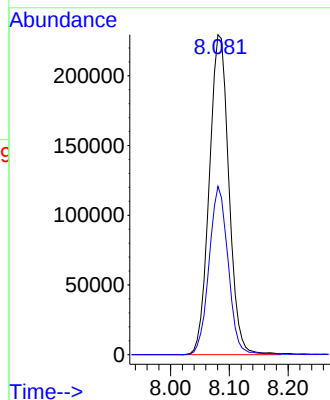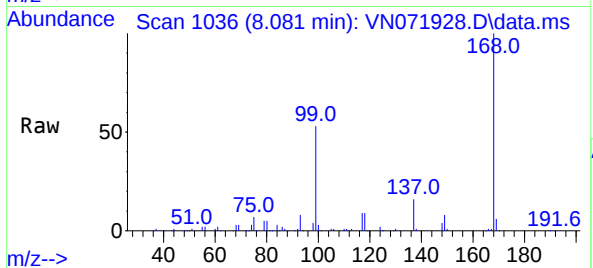

#33
1,2-Dichloroethane-d4
Concen: 47.232 ug/l
RT: 8.433 min Scan# 1096
Delta R.T. -0.001 min
Lab File: VN071928.D
Acq: 11 Apr 2022 12:04

Tgt Ion: 65 Resp: 286374
Ion Ratio Lower Upper
65 100
67 52.7 0.0 104.8

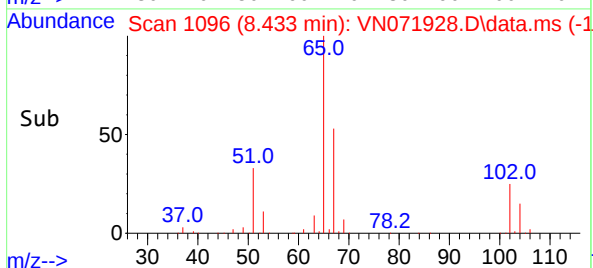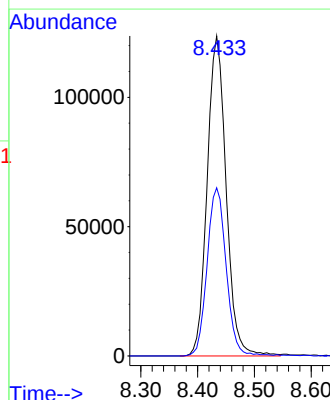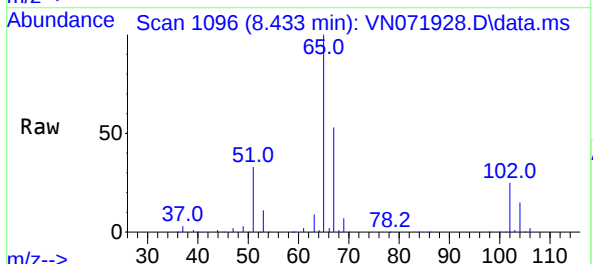




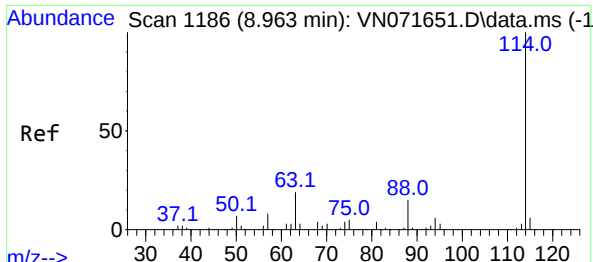


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.963 min Scan# 1186
Delta R.T. -0.000 min
Lab File: VN071928.D
Acq: 11 Apr 2022 12:04

Instrument :
MSVOA_N
ClientSampleId :
VN0411MBL01

Tgt Ion:114 Resp: 888848




Ion	Ratio	Lower	Upper
114	100		
63	19.6	0.0	40.0
88	15.5	0.0	32.6

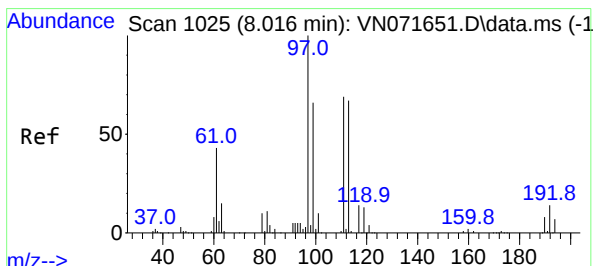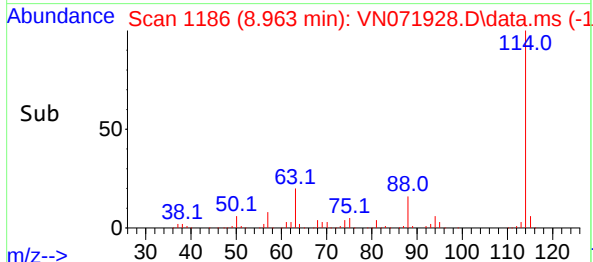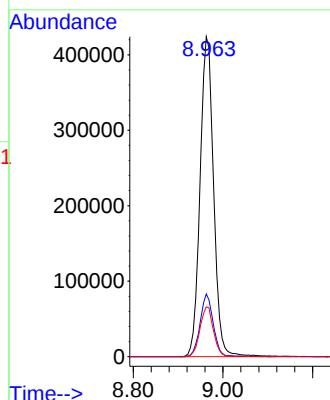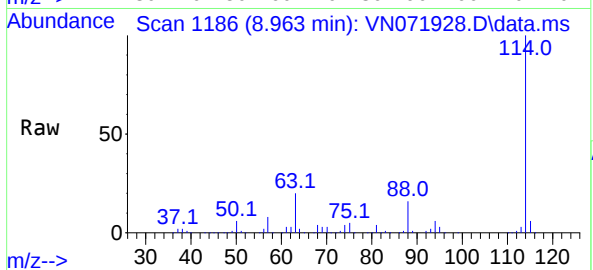


#35
Dibromofluoromethane
Concen: 48.778 ug/l
RT: 8.016 min Scan# 1025
Delta R.T. -0.000 min
Lab File: VN071928.D
Acq: 11 Apr 2022 12:04

Tgt Ion:113 Resp: 255128

Ion	Ratio	Lower	Upper
113	100		
111	102.4	81.4	122.0
192	22.8	17.0	25.6


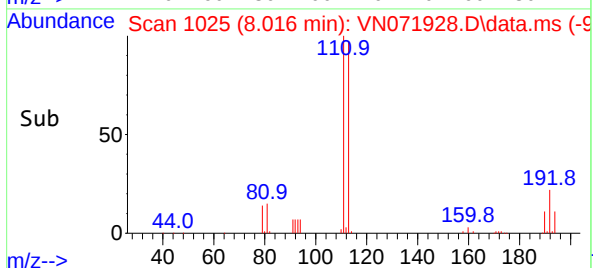
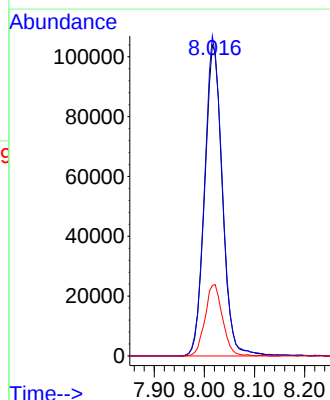
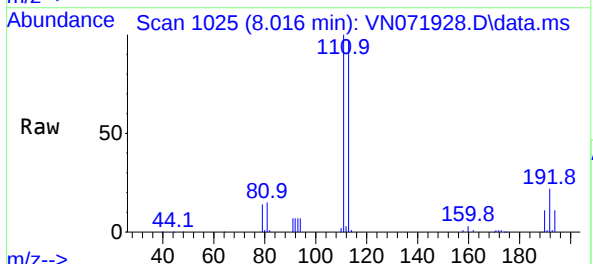


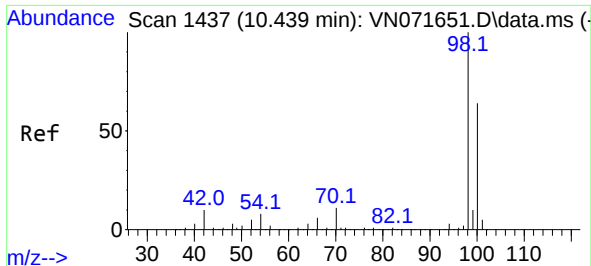

#50
Toluene-d8
Concen: 51.833 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. 0.000 min
Lab File: VN071928.D
Acq: 11 Apr 2022 12:04




Instrument :
MSVOA_N
ClientSampleId :
VN0411MBL01


Tgt Ion: 98 Resp: 1109028
Ion Ratio Lower Upper
98 100
100 64.9 52.6 78.8

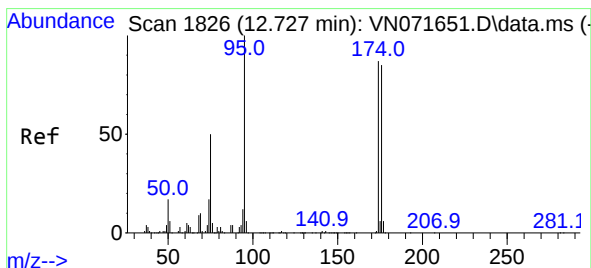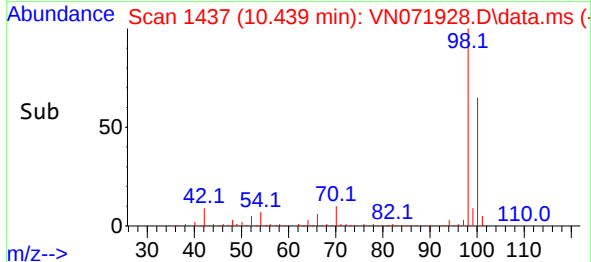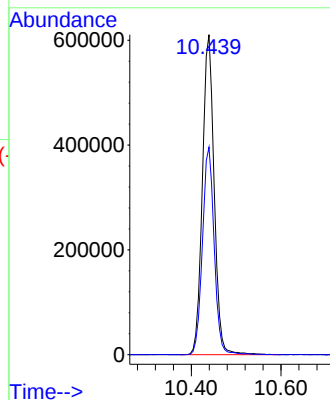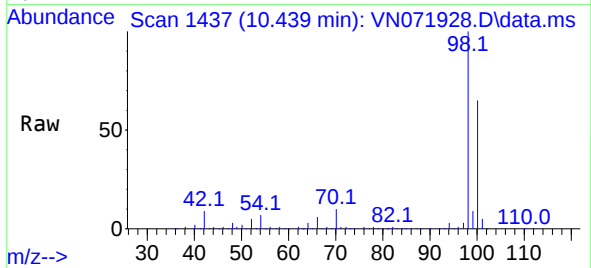

#62
4-Bromofluorobenzene
Concen: 52.824 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN071928.D
Acq: 11 Apr 2022 12:04

Tgt Ion: 95 Resp: 365535
Ion Ratio Lower Upper
95 100
174 86.5 0.0 167.6
176 83.1 0.0 163.4


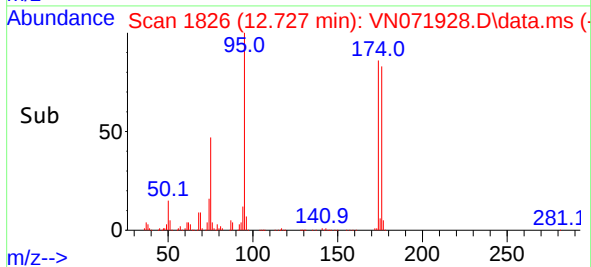
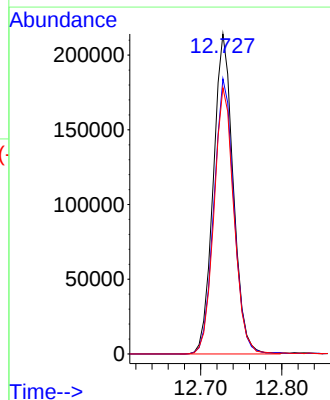
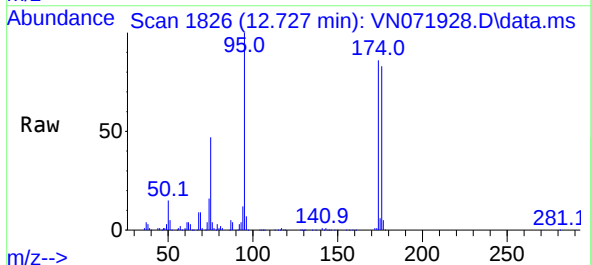


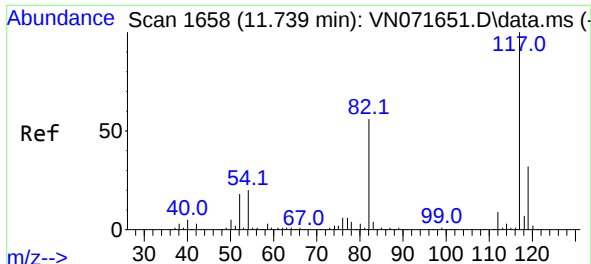

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN071928.D
Acq: 11 Apr 2022 12:04

Instrument :
MSVOA_N
ClientSampleId :
VN0411MBL01

Tgt Ion:117 Resp: 909367
Ion Ratio Lower Upper
117 100
82 54.4 44.2 66.2
119 32.9 25.4 38.0

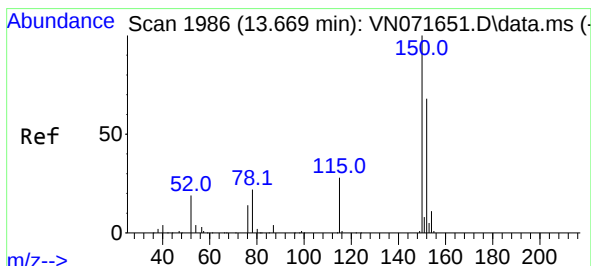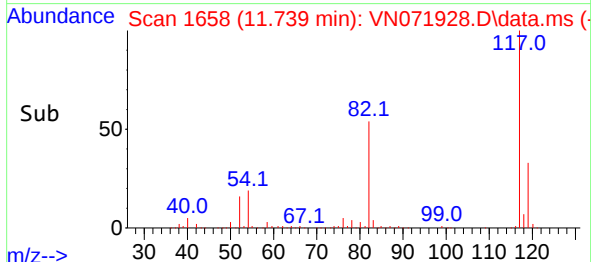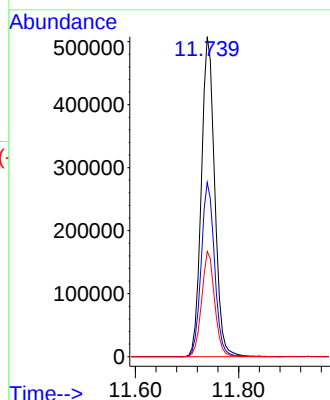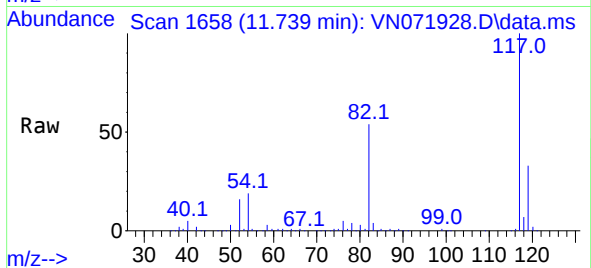

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.668 min Scan# 1986
Delta R.T. -0.001 min
Lab File: VN071928.D
Acq: 11 Apr 2022 12:04

Tgt Ion:152 Resp: 324325
Ion Ratio Lower Upper
152 100
115 56.3 28.9 86.7
150 156.5 0.0 356.2

