

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041122\
 Data File : VN071929.D
 Acq On : 11 Apr 2022 12:28
 Operator : JC\MD
 Sample : VN0411WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0411WBL01

Quant Time: Apr 11 13:03:00 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
 Quant Title : SW846 8260
 QLast Update : Thu Mar 31 01:57:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.080	168	645589	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	1102283	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	1157299	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.668	152	434328	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.433	65	351274	47.662	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	95.320%
35) Dibromofluoromethane	8.016	113	316243	48.755	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	97.520%
50) Toluene-d8	10.439	98	1385185	52.204	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	104.400%
62) 4-Bromofluorobenzene	12.727	95	484933	56.509	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	113.020%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041122\
Data File : VN071929.D
Acq On : 11 Apr 2022 12:28
Operator : JC\MD
Sample : VN0411WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0411WBL01

Quant Time: Apr 11 13:03:00 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N033022W.M
Quant Title : SW846 8260
QLast Update : Thu Mar 31 01:57:54 2022
Response via : Initial Calibration

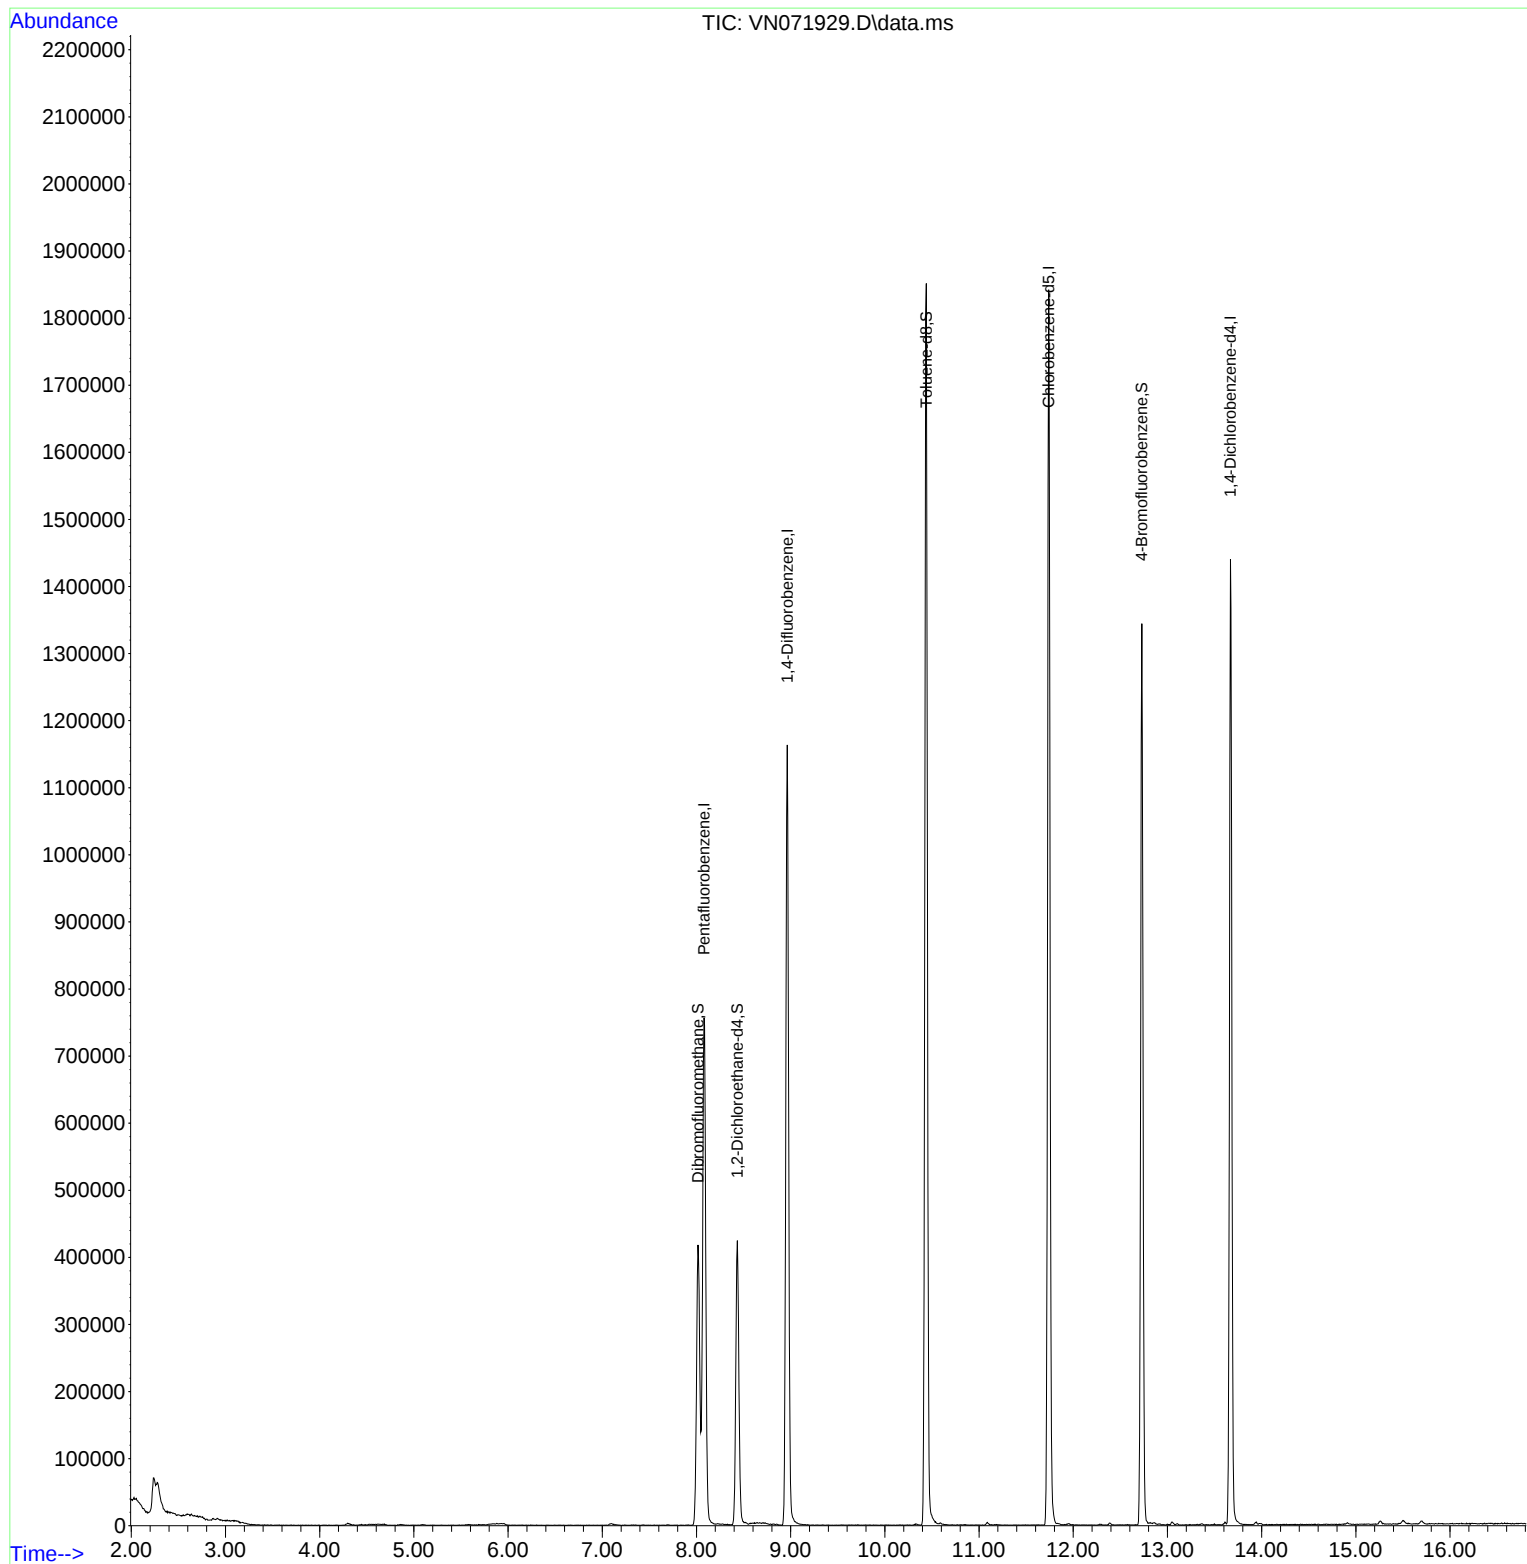

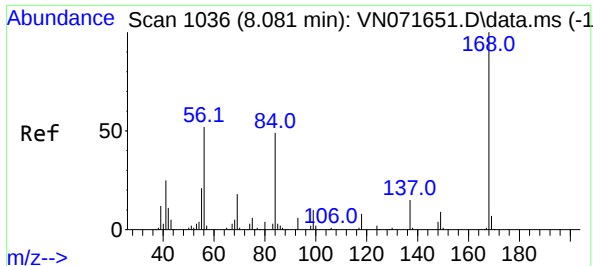

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.080 min Scan# 1036

Delta R.T. -0.001 min

Lab File: VN071929.D

Acq: 11 Apr 2022 12:28

Instrument :

MSVOA_N

ClientSampleId :





VN0411WBL01

Tgt Ion:168 Resp: 645589

Ion Ratio Lower Upper

168 100

99 50.1 42.3 63.5

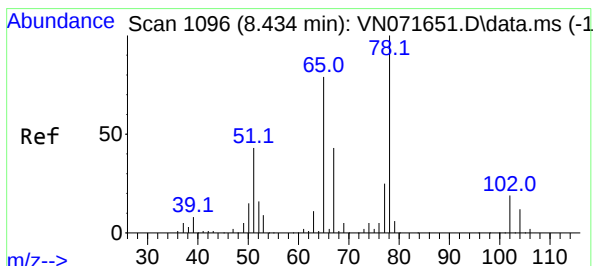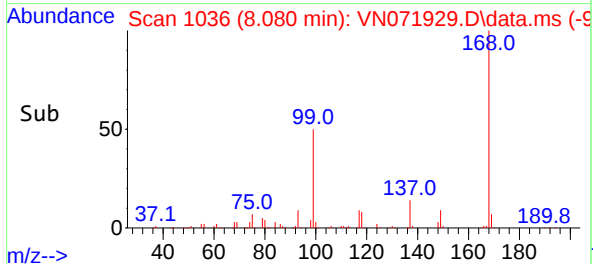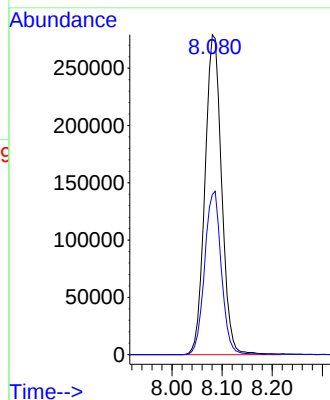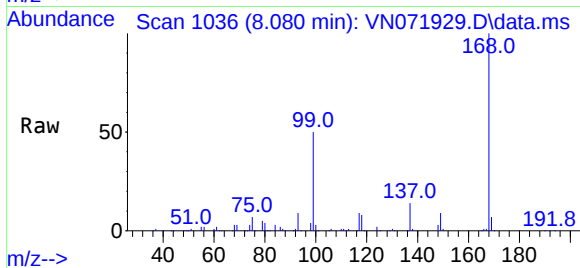

1,2-Dichloroethane-d4

Concen: 47.662 ug/l

RT: 8.433 min Scan# 1096

Delta R.T. -0.001 min

Lab File: VN071929.D




Acq: 11 Apr 2022 12:28


Tgt Ion: 65 Resp: 351274

Ion Ratio Lower Upper

65 100

67 53.1 0.0 104.8


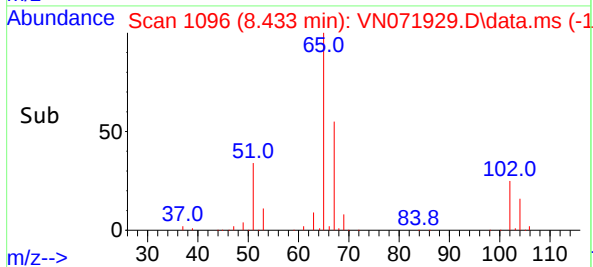
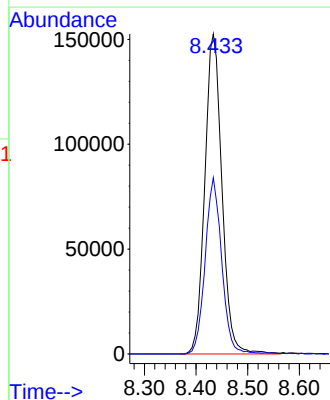
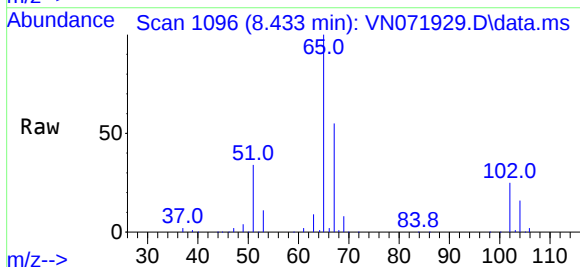


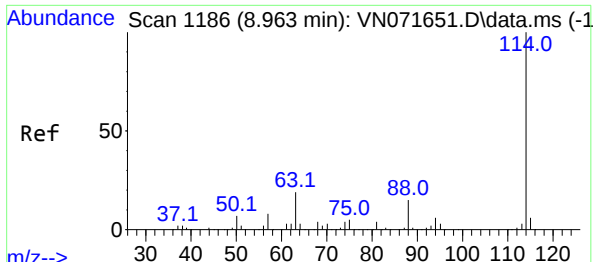

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.963 min Scan# 1186
Delta R.T. -0.000 min
Lab File: VN071929.D
Acq: 11 Apr 2022 12:28




Instrument :
MSVOA_N
ClientSampleId :
VN0411WBL01


Tgt Ion:114 Resp: 1102283
Ion Ratio Lower Upper
114 100
63 19.4 0.0 40.0
88 15.8 0.0 32.6

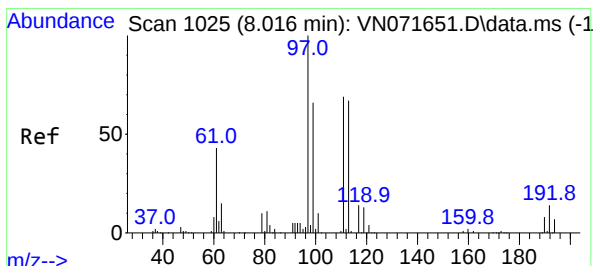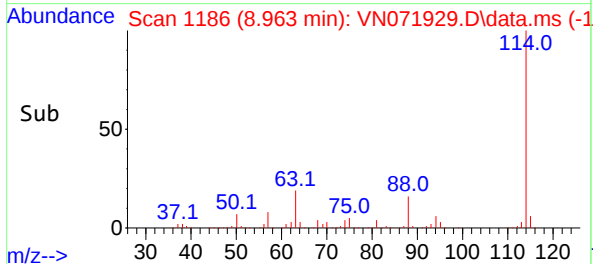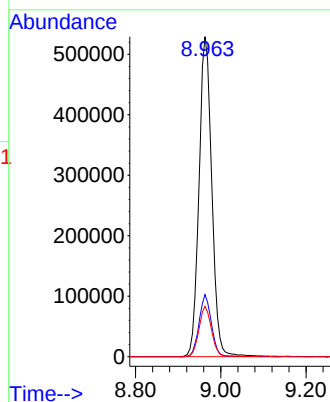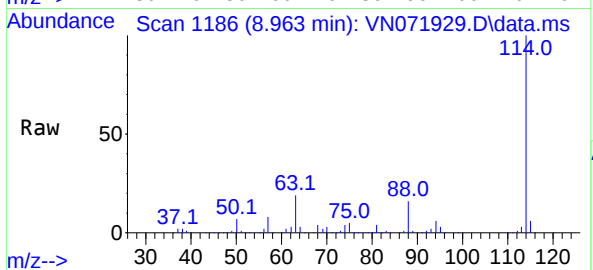

#35
Dibromofluoromethane
Concen: 48.755 ug/l
RT: 8.016 min Scan# 1025
Delta R.T. -0.000 min
Lab File: VN071929.D
Acq: 11 Apr 2022 12:28

Tgt Ion:113 Resp: 316243
Ion Ratio Lower Upper
113 100
111 102.0 81.4 122.0
192 22.5 17.0 25.6


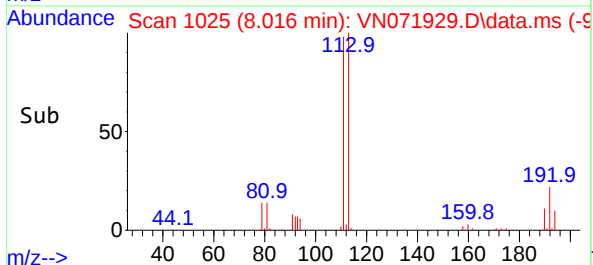
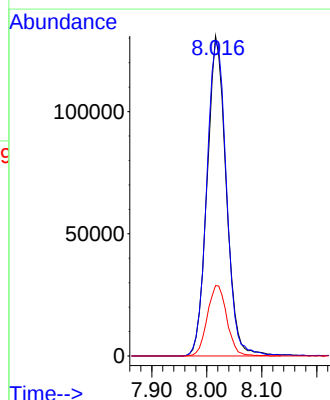
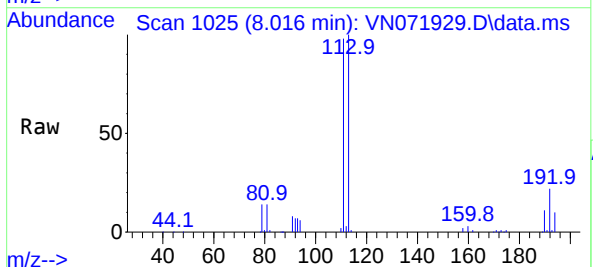


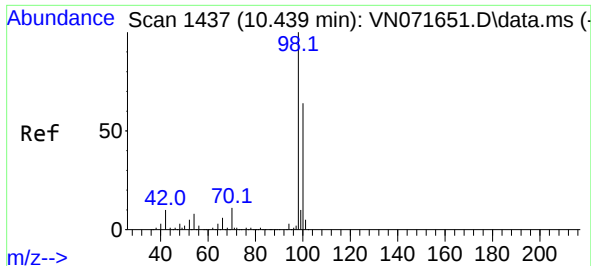

#50
Toluene-d8
Concen: 52.204 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. 0.000 min
Lab File: VN071929.D
Acq: 11 Apr 2022 12:28




Instrument :
MSVOA_N
ClientSampleId :
VN0411WBL01


Tgt Ion: 98 Resp: 1385185
Ion Ratio Lower Upper
98 100
100 64.2 52.6 78.8

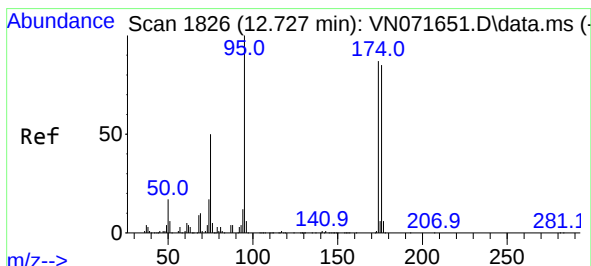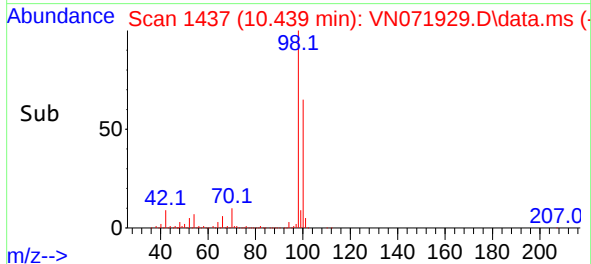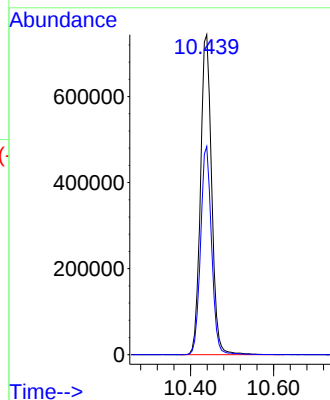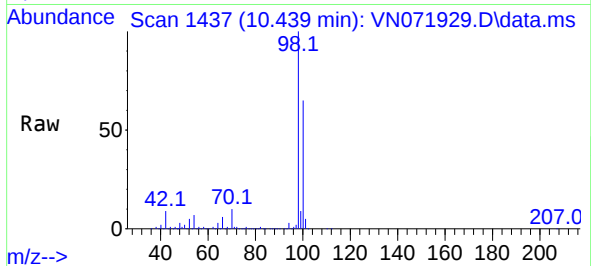

#62
4-Bromofluorobenzene
Concen: 56.509 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN071929.D
Acq: 11 Apr 2022 12:28

Tgt Ion: 95 Resp: 484933
Ion Ratio Lower Upper
95 100
174 86.0 0.0 167.6
176 82.8 0.0 163.4


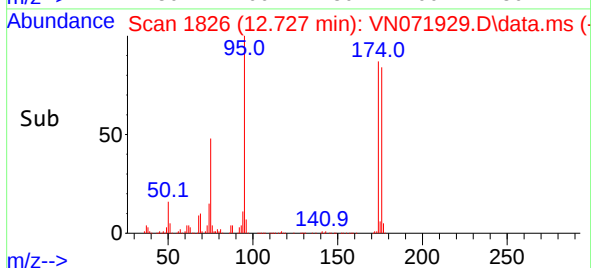
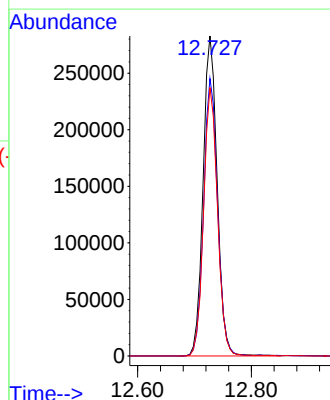
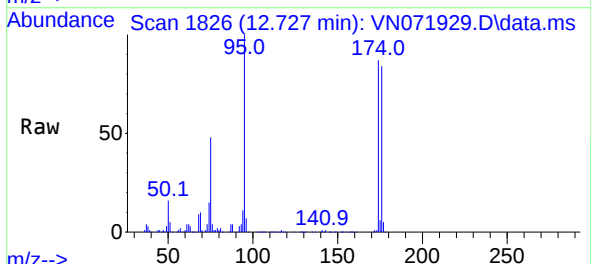


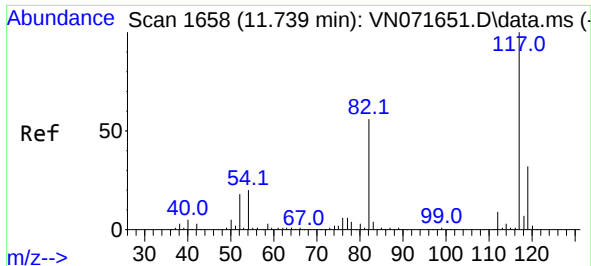

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN071929.D
Acq: 11 Apr 2022 12:28

Instrument :
MSVOA_N
ClientSampleId :
VN0411WBL01

Tgt Ion:117 Resp: 1157299
Ion Ratio Lower Upper
117 100
82 55.2 44.2 66.2
119 32.8 25.4 38.0

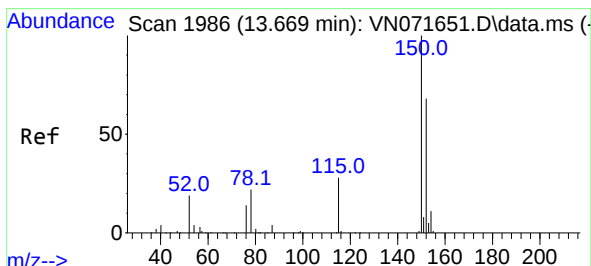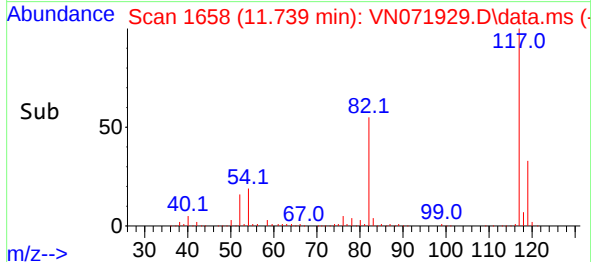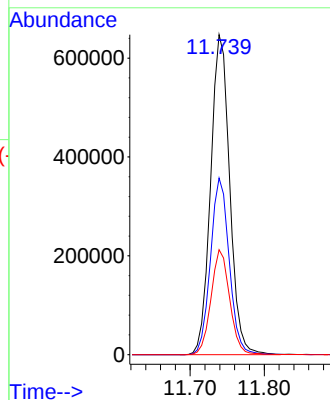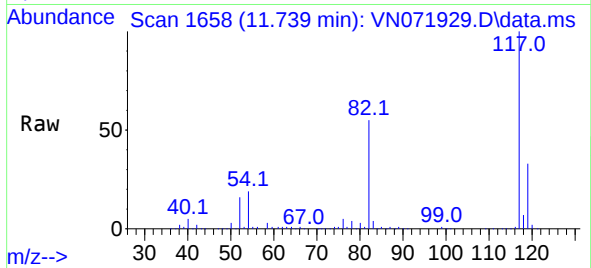

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.668 min Scan# 1986
Delta R.T. -0.001 min
Lab File: VN071929.D
Acq: 11 Apr 2022 12:28

Tgt Ion:152 Resp: 434328
Ion Ratio Lower Upper
152 100
115 56.9 28.9 86.7
150 159.0 0.0 356.2

