
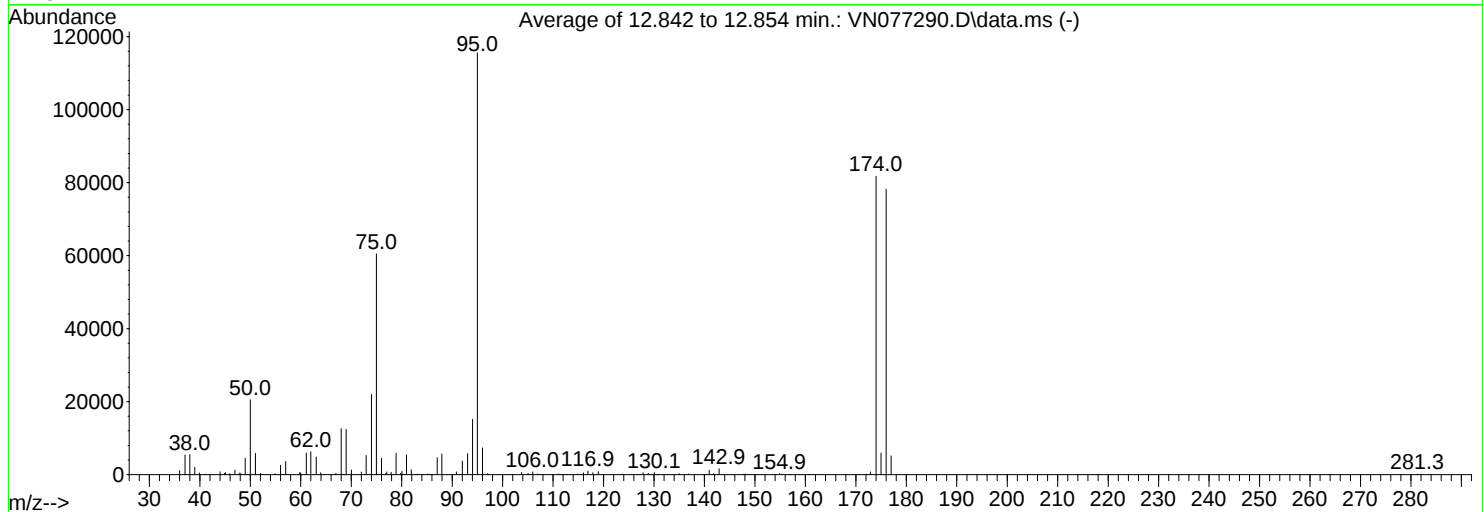


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041123\
Data File : VN077290.D
Acq On : 11 Apr 2023 08:27
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N040523W.M
Title : SW846 8260
Last Update : Thu Apr 06 08:27:03 2023

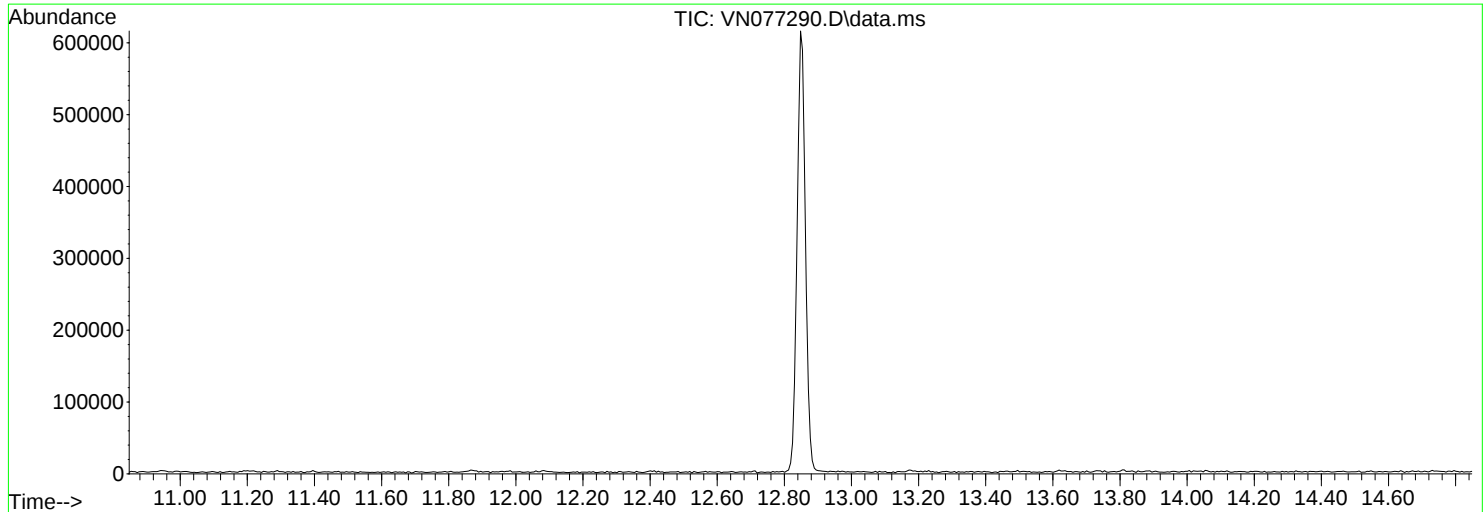

AutoFind: Scans 1854, 1855, 1856; Background Corrected with Scan 1846

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	20500	PASS
75	95	30	60	52.3	60480	PASS
95	95	100	100	100.0	115563	PASS
96	95	5	9	6.4	7342	PASS
173	174	0.00	2	0.9	728	PASS
174	95	50	100	70.7	81752	PASS
175	174	5	9	7.2	5923	PASS
176	174	95	101	95.7	78221	PASS
177	176	5	9	6.6	5149	PASS

Average of 12.842 to 12.854 min.: VN077290.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	1117	46.95	1273	57.00	3577	72.00	721
37.05	5401	47.60	158	59.80	588	72.95	527
38.00	5506	47.95	547	60.00	506	74.00	2196
39.00	2016	48.20	174	61.10	5901	75.00	6048
39.90	465	49.00	4476	62.00	6266	76.00	4461
41.10	79	50.00	20500	63.05	4809	76.80	269
43.00	25	51.00	5822	63.95	513	77.05	747
44.00	791	52.05	351	66.95	351	77.90	659
44.90	321	53.80	60	68.00	12643	78.90	5882
45.05	570	54.90	250	69.00	12394	79.80	384
45.95	272	56.00	2591	70.05	1295	80.05	866

Average of 12.842 to 12.854 min.: VN077290.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.95	5417	93.05	5764	111.10	193	127.85	524
81.90	1327	94.05	15157	111.60	96	128.10	111
82.80	54	95.00	115563	112.10	54	128.85	362
83.05	136	96.00	7342	112.80	96	130.05	560
85.20	164	97.05	290	114.80	167	130.70	82
85.70	108	101.90	63	116.00	467	130.90	61
86.00	63	103.75	555	116.90	975	132.70	64
87.05	4630	105.05	358	117.90	509	135.00	266
87.95	5644	105.95	766	118.95	773	136.85	208
90.85	746	106.90	184	123.80	154	140.95	1175
92.00	3737	110.10	61	126.90	56	141.80	250

Average of 12.842 to 12.854 min.: VN077290.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
142.90	1611	160.90	61				
145.80	95	171.40	58				
147.80	112	172.10	137				
148.10	165	172.30	58				
149.80	62	172.90	728				
154.90	315	174.00	81752				
155.20	55	175.00	5923				
156.90	90	176.00	78221				
157.10	111	177.00	5149				
158.90	75	281.30	133				
160.70	63	282.05	119				

Instrument :

MSVOA_N

ClientSampleId :

BFB