
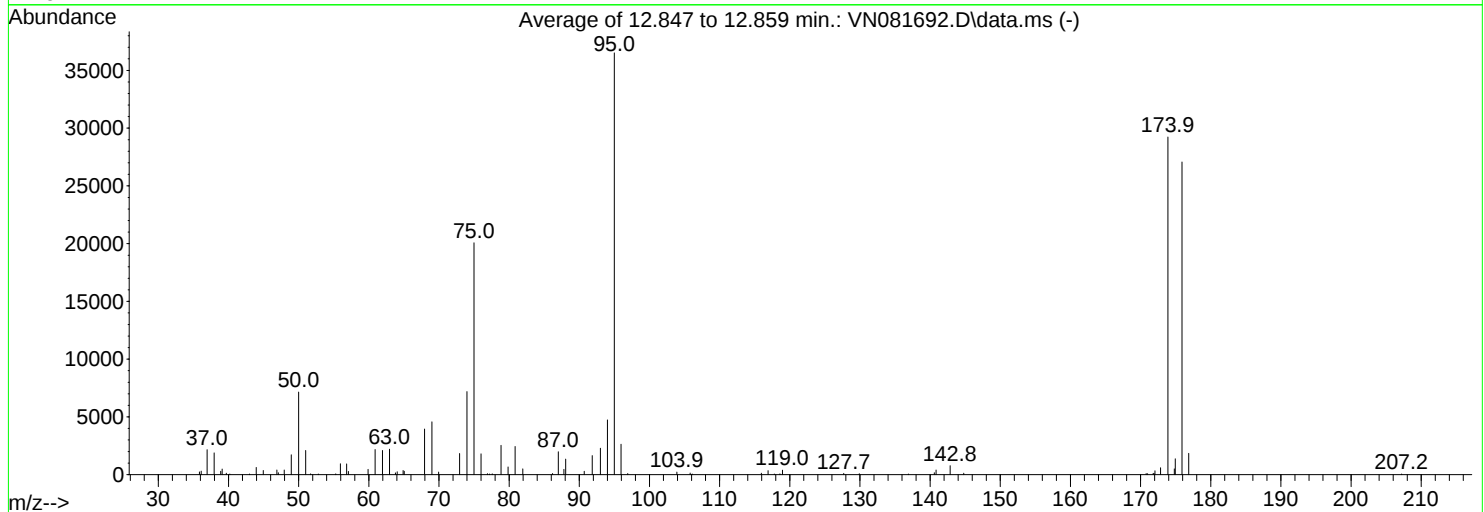


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN041124\
Data File : VN081692.D
Acq On : 11 Apr 2024 11:31
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N041024W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu Apr 11 09:25:01 2024

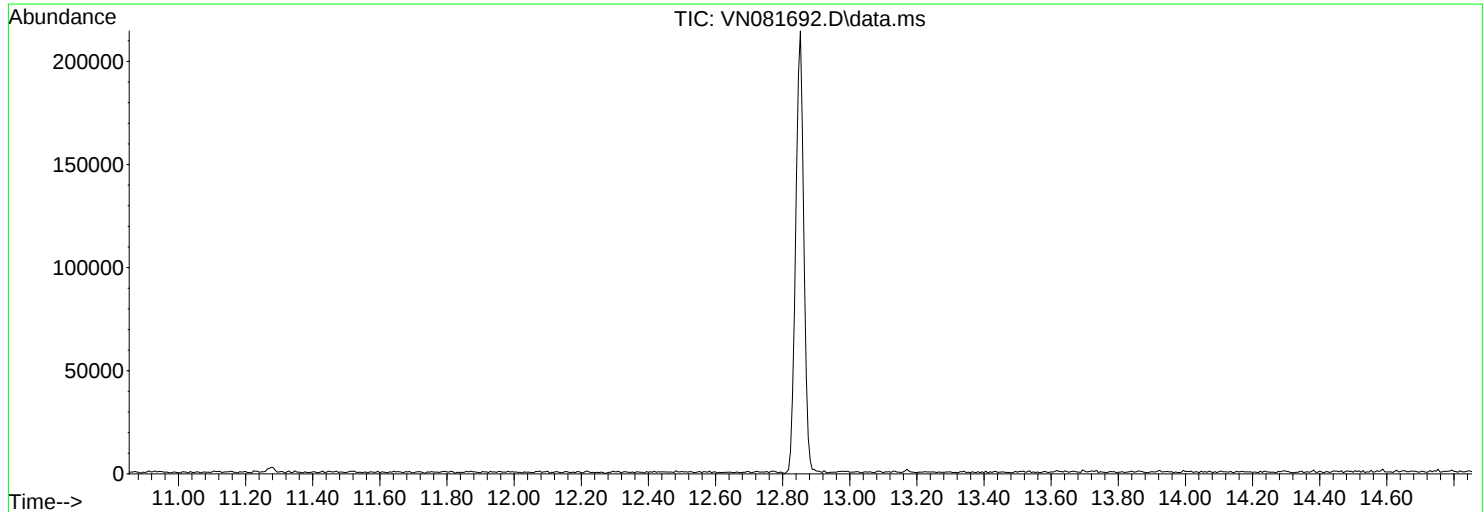

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1846

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.6	7147	PASS
75	95	30	60	55.0	20075	PASS
95	95	100	100	100.0	36520	PASS
96	95	5	9	7.2	2639	PASS
173	174	0.00	2	2.0	594	FAIL*
174	95	50	100	80.0	29229	PASS
175	174	5	9	4.7	1377	FAIL*
176	174	95	101	92.6	27067	FAIL*
177	176	5	9	6.8	1847	PASS