


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN041219\
Data File : VN054990.D
Acq On : 12 Apr 2019 8:45
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N041119W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Apr 12 07:55:25 2019

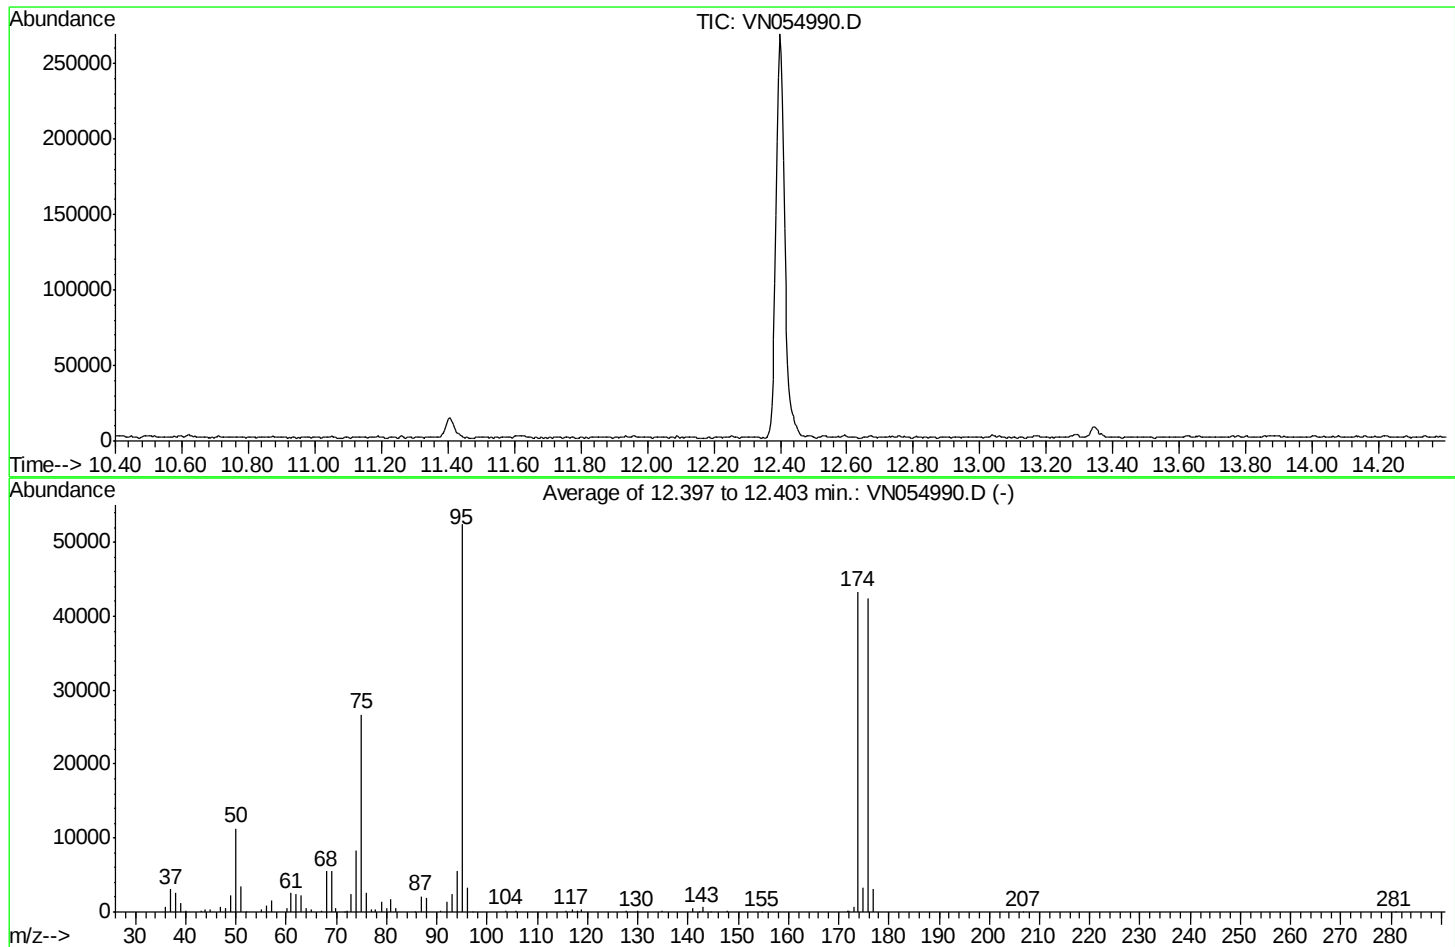

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	11285	PASS
75	95	30	60	50.9	26674	PASS
95	95	100	100	100.0	52429	PASS
96	95	5	9	6.4	3369	PASS
173	174	0.00	2	1.5	650	PASS
174	95	50	100	82.7	43357	PASS
175	174	5	9	7.7	3347	PASS
176	174	95	101	97.7	42352	PASS
177	176	5	9	7.3	3077	PASS